

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071719\
 Data File : PS005533.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2019 08:20
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 12:11:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	4.933	0.000	1049.6E6	0	522.255	N.D. #
3) T	4-Nitroph...	5.388	0.000	13199234	0	18.224	N.D. #
5) T	DICAMBA	0.000	5.432	0	714.1E6	N.D.	190.759
8) T	DICHLORPROP	0.000	5.972	0	14661175	N.D.	15.184
9) T	2,4-D	6.607	0.000	951.2E6	0	611.890	N.D. #
10) T	Pentachlo...	6.857	0.000	14911778	0	<MDL	N.D. #
12) T	2,4,5-T	7.675	7.384	40418128	193.2E6	5.022	37.880 #
14) T	DINOSEB	9.295	0.000	31974506	0	5.003	N.D. #
15) T	Picloram	9.132	9.089	1037.3E6	505.8E6	90.272	67.026 #
16) T	DCPA	9.567	9.043	18640082	19576641	1.869	2.876 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071719\
Data File : PS005533.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2019 08:20
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 12:11:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

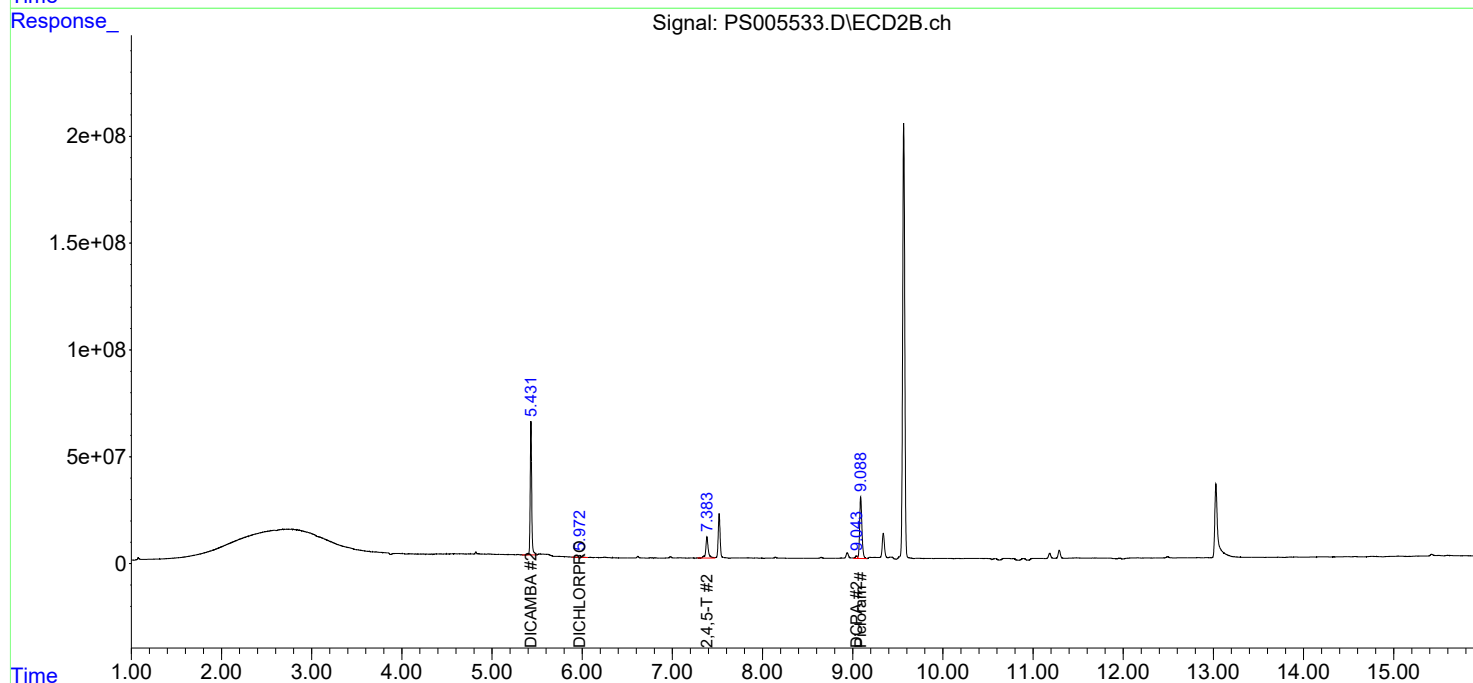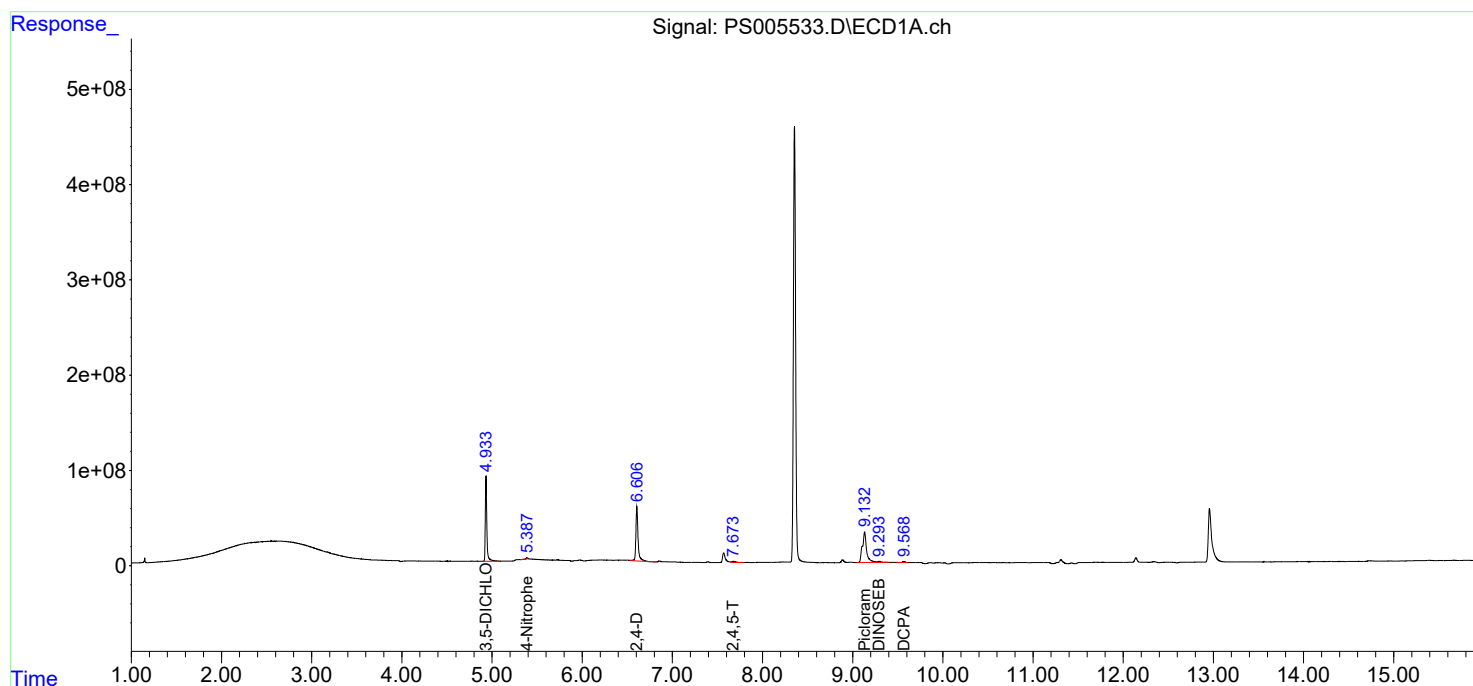


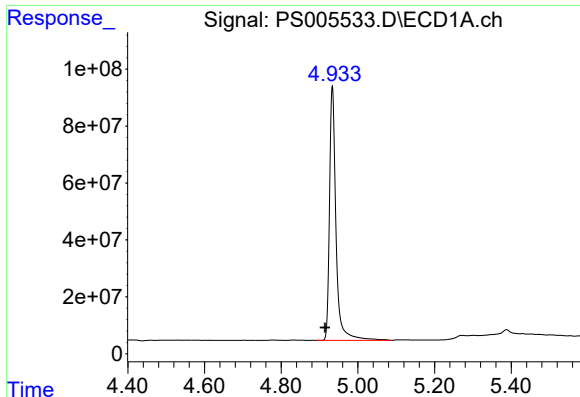

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.933 min
Delta R.T.: 0.019 min
Response: 1049586091
Conc: 522.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

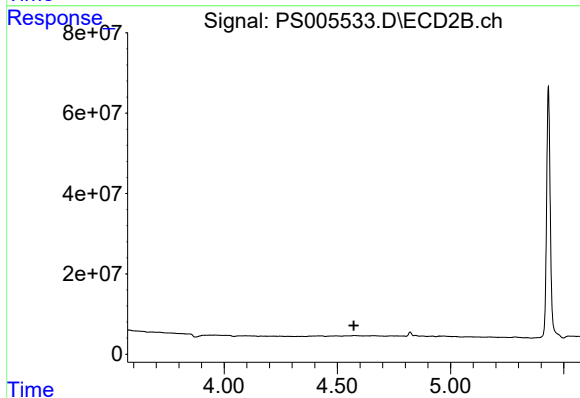


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.573 min
Response: 0
Conc: N.D.

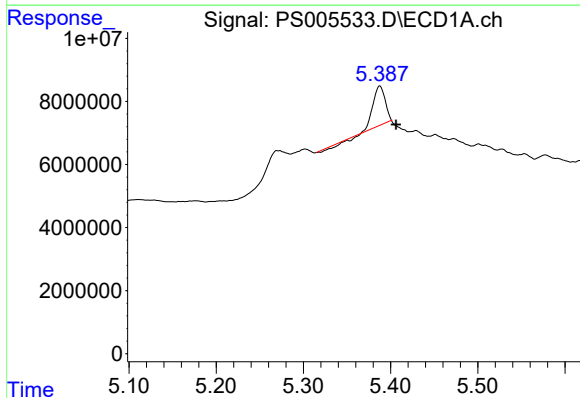


#3 4-Nitrophenol

R.T.: 5.388 min
Delta R.T.: -0.019 min
Response: 13199234
Conc: 18.22 ng/ml

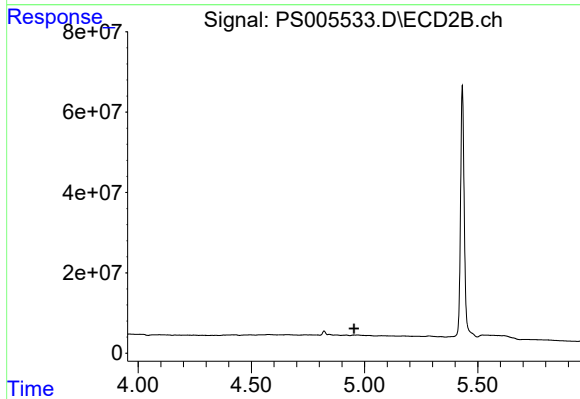

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

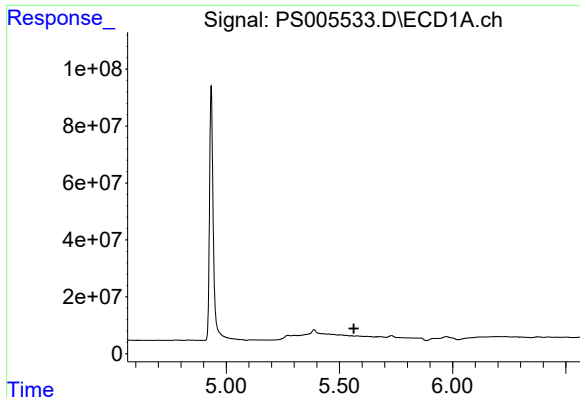

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 5.564 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

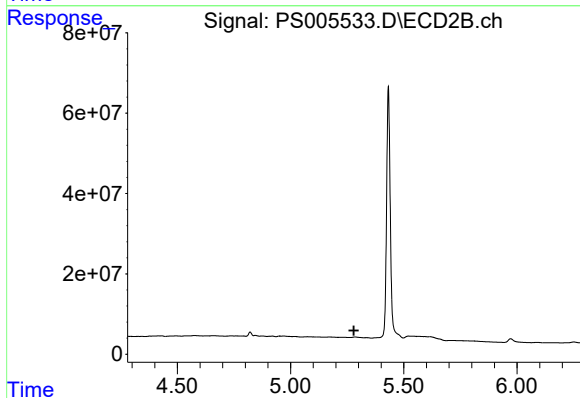


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 5.280 min
Response: 0
Conc: N.D.

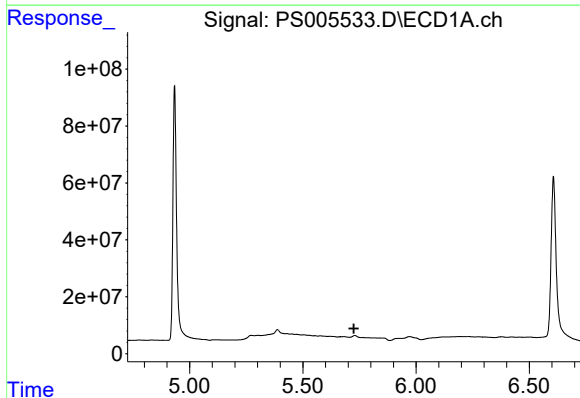


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.725 min
Response: 0
Conc: N.D.

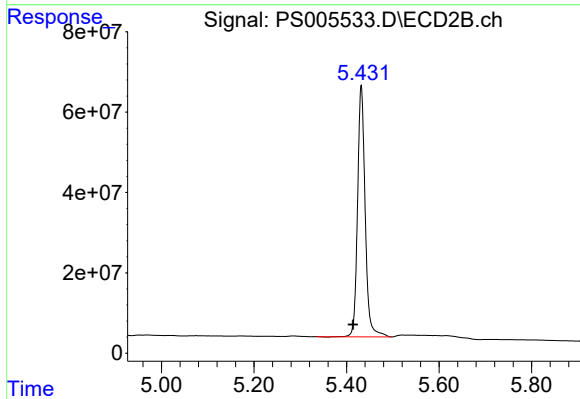

#5 DICAMBA


R.T.: 5.432 min
Delta R.T.: 0.018 min
Response: 714072164
Conc: 190.76 ng/ml

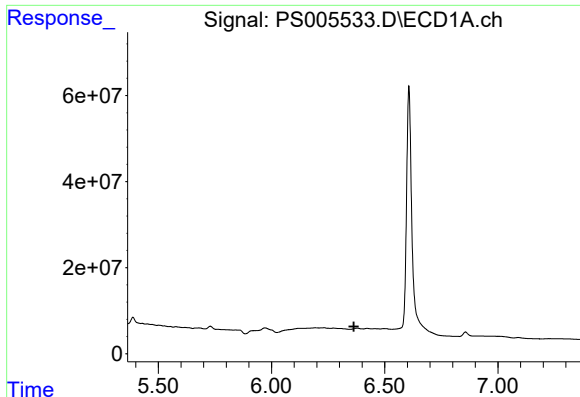

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.363 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

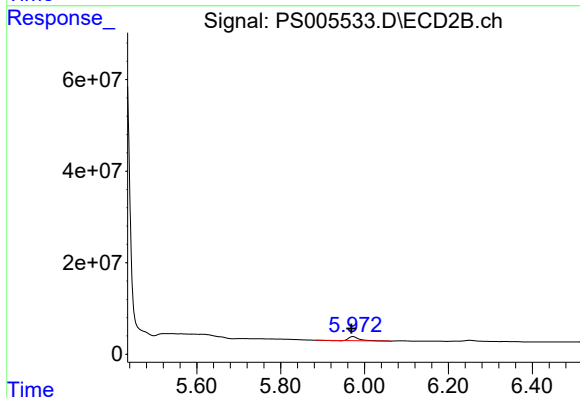


#8 DICHLORPROP

R.T.: 5.972 min
Delta R.T.: 0.003 min
Response: 14661175
Conc: 15.18 ng/ml

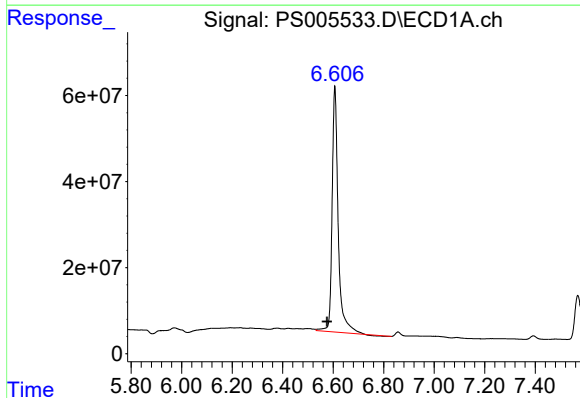


#9 2,4-D

R.T.: 6.607 min
Delta R.T.: 0.030 min
Response: 951243998
Conc: 611.89 ng/ml

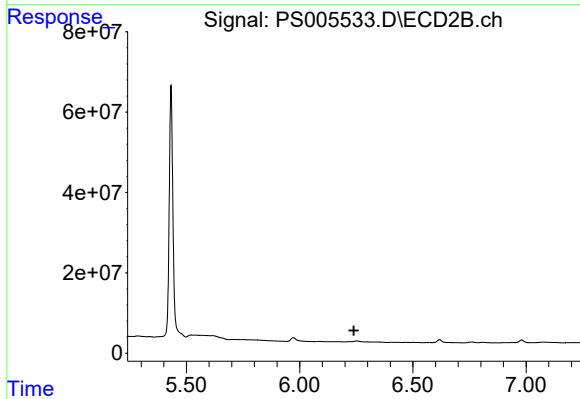

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.240 min
Response: 0
Conc: N.D.

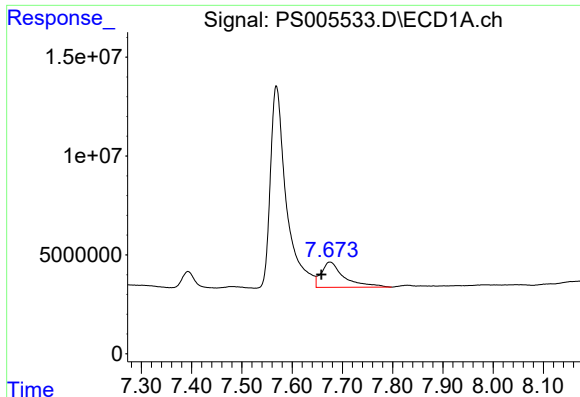

#12 2,4,5-T


R.T.: 7.675 min
Delta R.T.: 0.017 min
Response: 40418128
Conc: 5.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

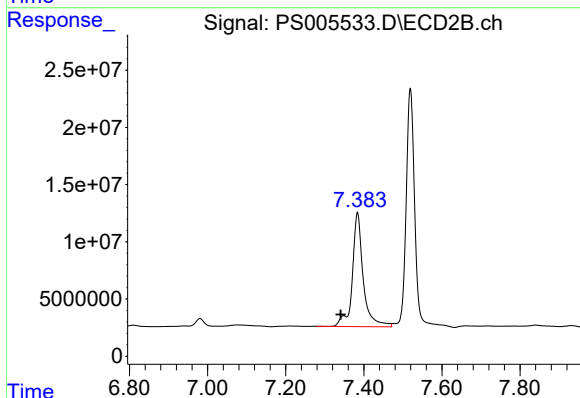


#12 2,4,5-T

R.T.: 7.384 min
Delta R.T.: 0.043 min
Response: 193218888
Conc: 37.88 ng/ml

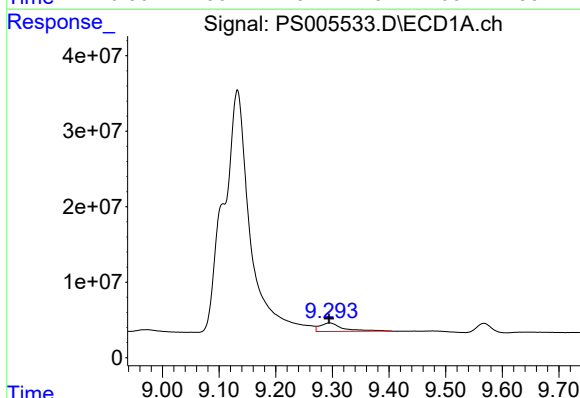


#14 DINOSEB

R.T.: 9.295 min
Delta R.T.: 0.000 min
Response: 31974506
Conc: 5.00 ng/ml

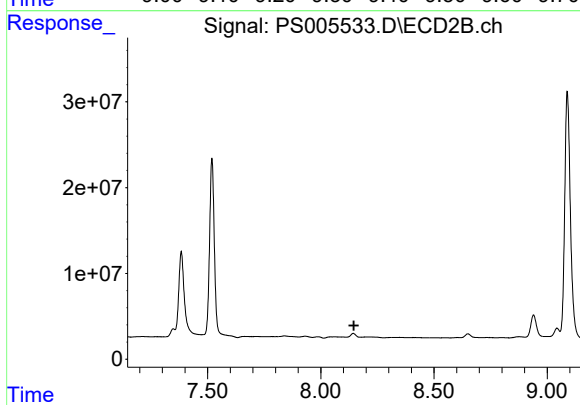

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 8.146 min
Response: 0
Conc: N.D.

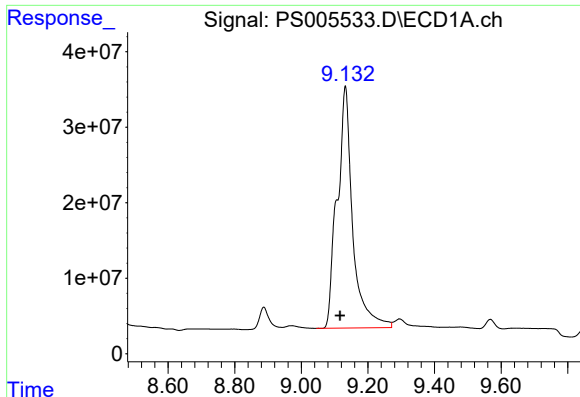

#15 Picloram


R.T.: 9.132 min
Delta R.T.: 0.016 min
Response: 1037322665
Conc: 90.27 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

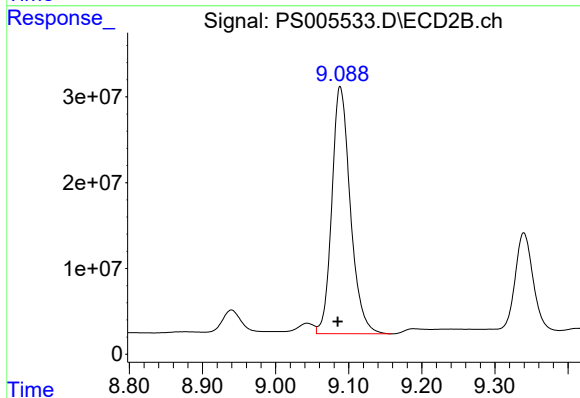


#15 Picloram

R.T.: 9.089 min
Delta R.T.: 0.004 min
Response: 505808582
Conc: 67.03 ng/ml

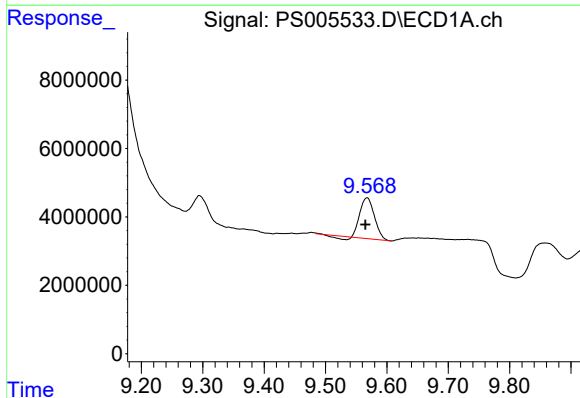

#16 DCPA

R.T.: 9.567 min
Delta R.T.: 0.002 min
Response: 18640082
Conc: 1.87 ng/ml

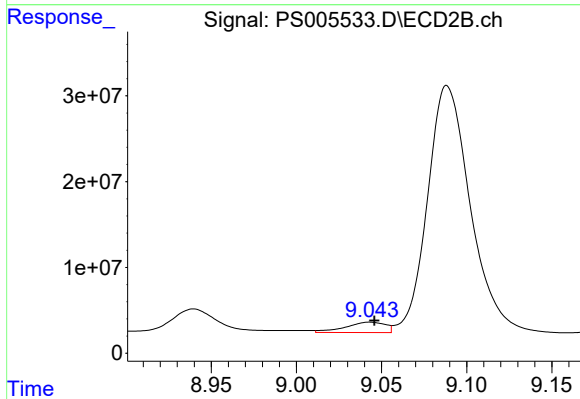

#16 DCPA

R.T.: 9.043 min
Delta R.T.: -0.002 min
Response: 19576641
Conc: 2.88 ng/ml