

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071719\
 Data File : PS005534.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2019 08:42
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 12:12:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.571	5.286	689.3E6	488.7E6	469.559	487.585
Target Compounds							
2) T	3,5-DICHL...	4.943	0.000	14060951	0	6.996	N.D. #
12) T	2,4,5-T	0.000	7.397	0	89025928	N.D.	17.453
15) T	Picloram	9.145	9.100	472.4E6	350.6E6	41.108	46.458
16) T	DCPA	0.000	9.100	0	350.6E6	N.D.	51.501



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071719\
Data File : PS005534.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2019 08:42
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 12:12:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

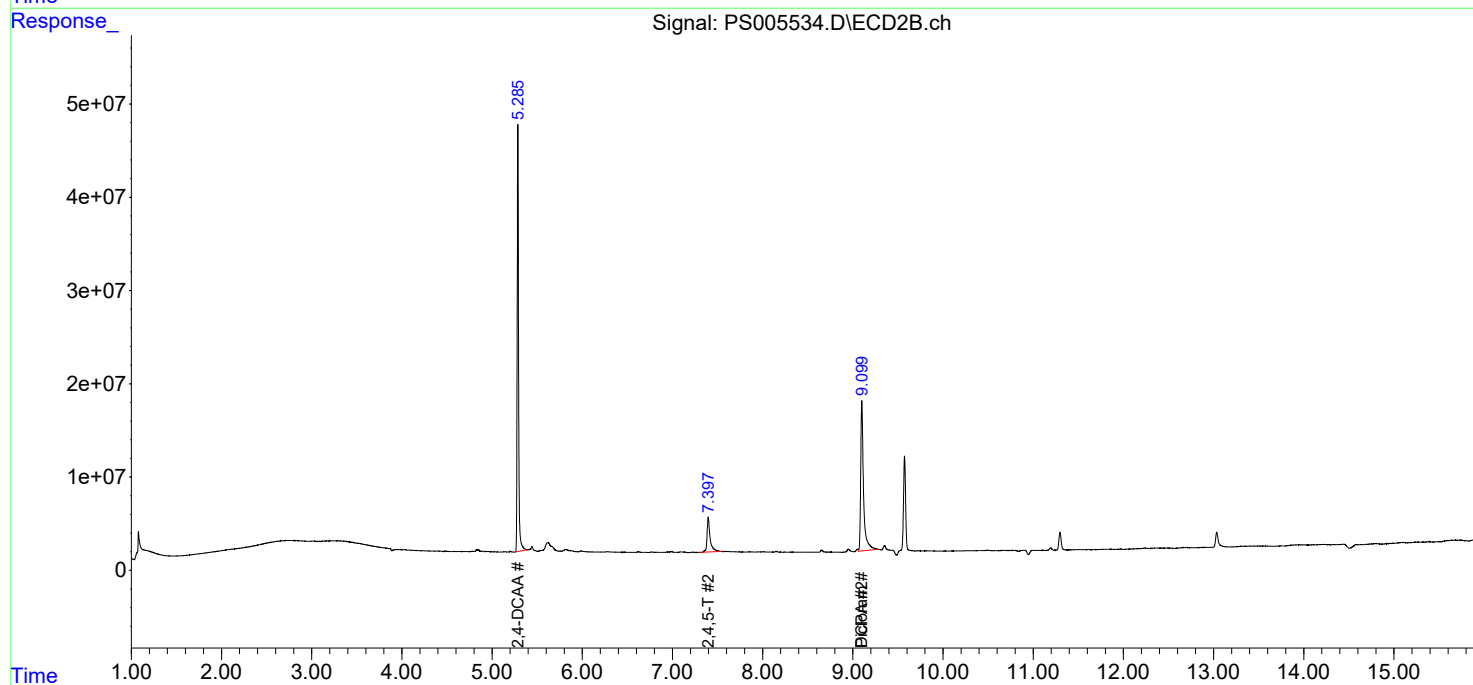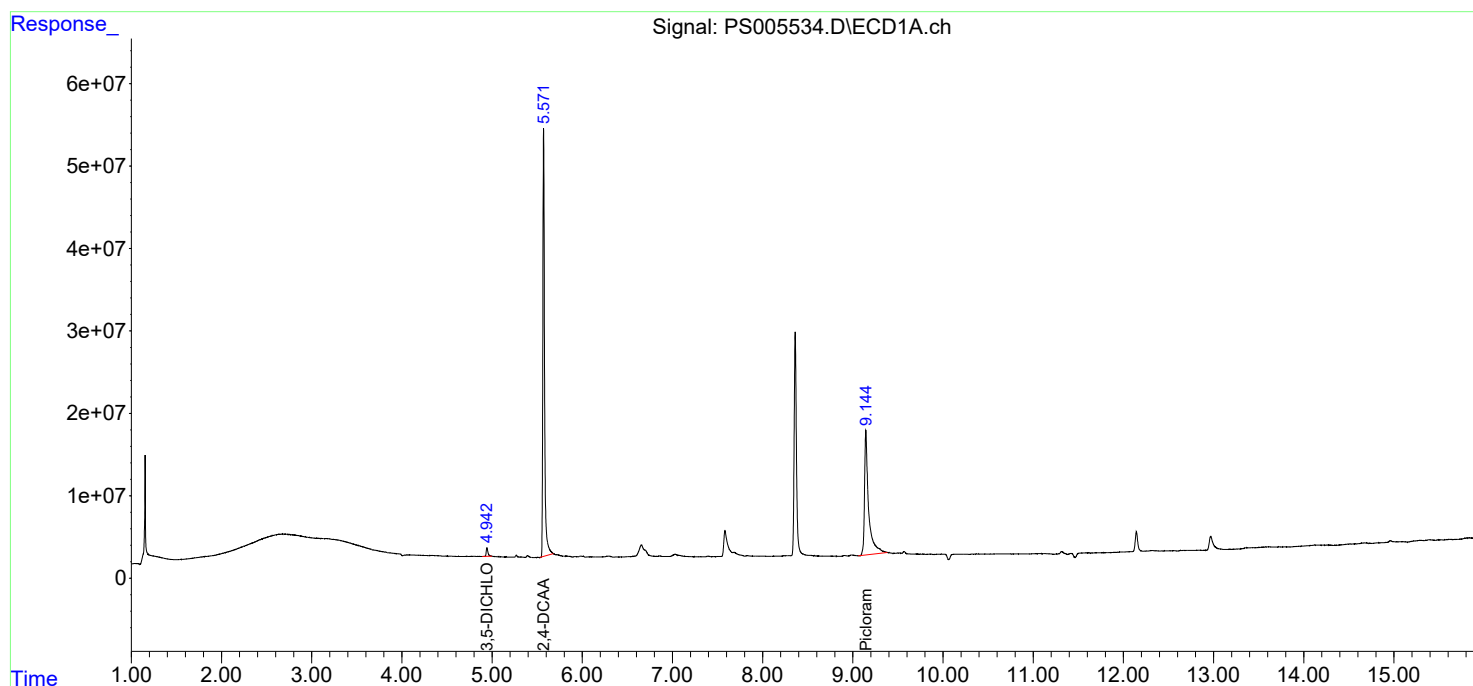


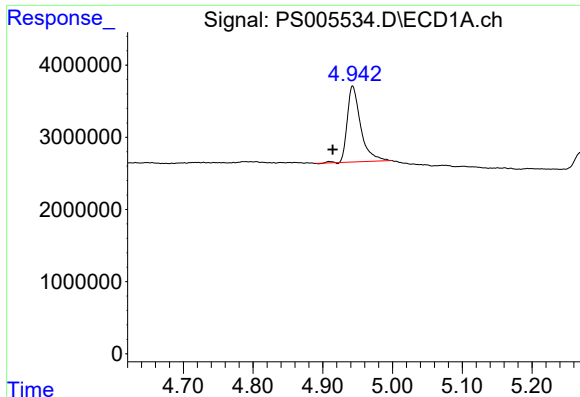

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.943 min
Delta R.T.: 0.029 min
Response: 14060951
Conc: 7.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

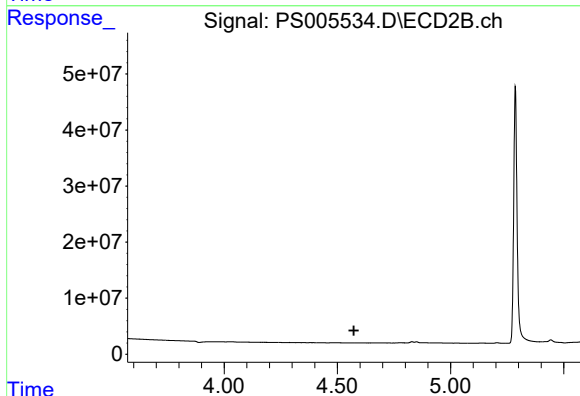


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.573 min
Response: 0
Conc: N.D.

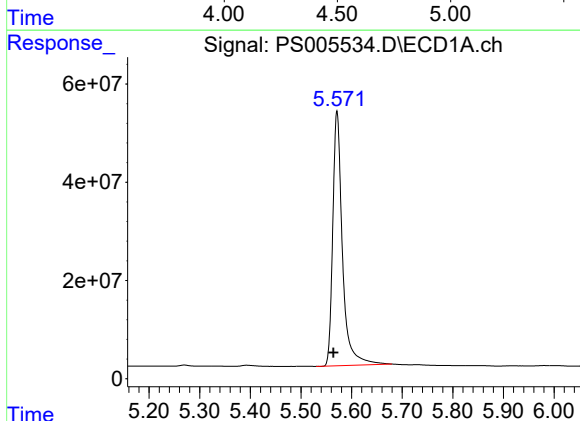


#4 2,4-DCAA

R.T.: 5.571 min
Delta R.T.: 0.008 min
Response: 689261855
Conc: 469.56 ng/ml

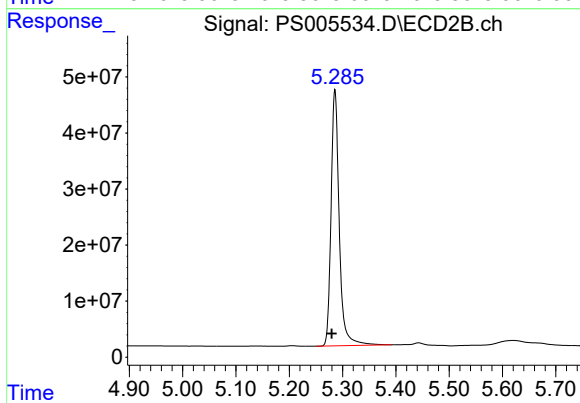

#4 2,4-DCAA


R.T.: 5.286 min
Delta R.T.: 0.006 min
Response: 488739778
Conc: 487.58 ng/ml

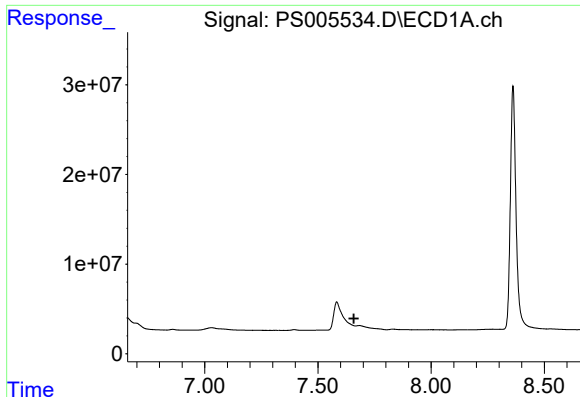

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.659 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

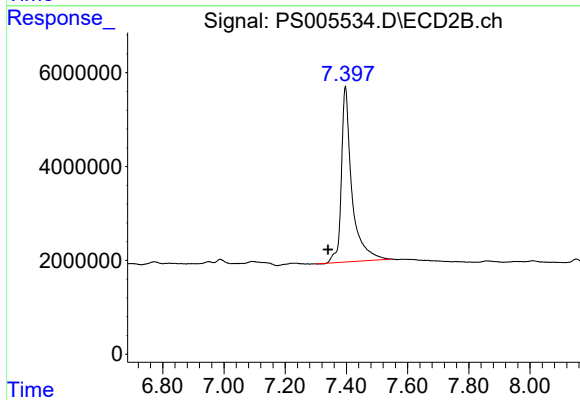


#12 2,4,5-T

R.T.: 7.397 min
Delta R.T.: 0.056 min
Response: 89025928
Conc: 17.45 ng/ml

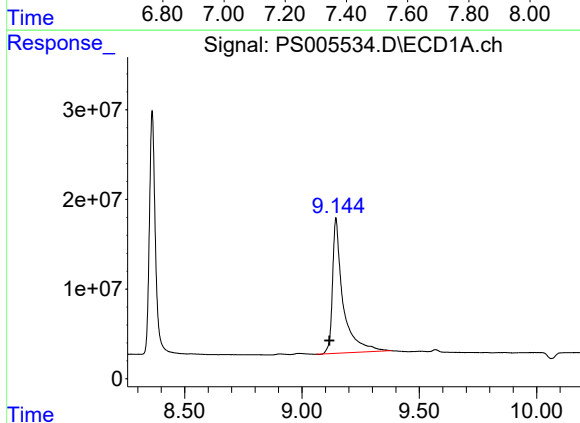


#15 Picloram

R.T.: 9.145 min
Delta R.T.: 0.028 min
Response: 472381619
Conc: 41.11 ng/ml

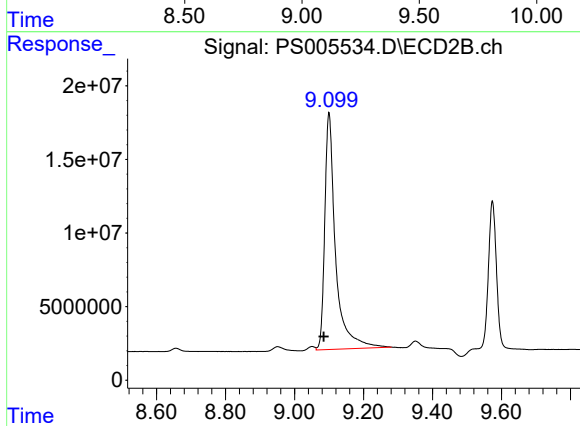

#15 Picloram


R.T.: 9.100 min
Delta R.T.: 0.015 min
Response: 350592721
Conc: 46.46 ng/ml

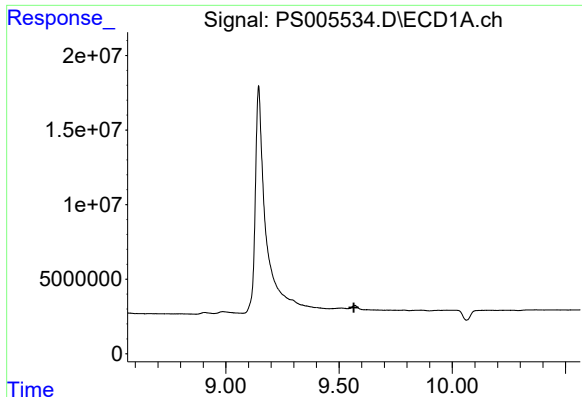

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.565 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

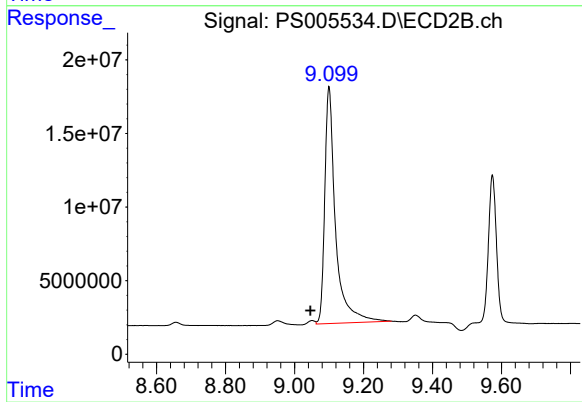

#16 DCPA

R.T.: 9.100 min
Delta R.T.: 0.054 min
Response: 350592721
Conc: 51.50 ng/ml