

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071819\
 Data File : PS005554.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2019 23:03
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 09:14:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 19 08:54:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.594	5.310	562.7E6	361.8E6	357.092	350.324
Target Compounds							
2) T	3,5-DICHL...	4.956	0.000	1456831	0	<MDL	N.D. #
5) T	DICAMBA	5.755	0.000	3963318	0	<MDL	N.D. #
7) T	MCPA	5.999	5.643	1652086	86670294	<MDL	19.670 #
8) T	DICHLORPROP	6.398	0.000	1216094	0	<MDL	N.D. #
10) T	Pentachlo...	6.880	0.000	21283687	0	<MDL	N.D. #
11) T	2,4,5-TP ...	7.418	0.000	6926728	0	<MDL	N.D. #
12) T	2,4,5-T	7.708	0.000	10687105	0	1.262	N.D. #
13) T	2,4-DB	8.248	0.000	7498695	0	5.986	N.D. #
14) T	DINOSEB	9.320	0.000	8603190	0	1.233	N.D. #
15) T	Picloram	9.184	9.131	35150089	21450848	2.821	2.739
16) T	DCPA	9.591	0.000	6895315	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071819\
Data File : PS005554.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2019 23:03
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 09:14:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
Quant Title : 8080.M
QLast Update : Fri Jul 19 08:54:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

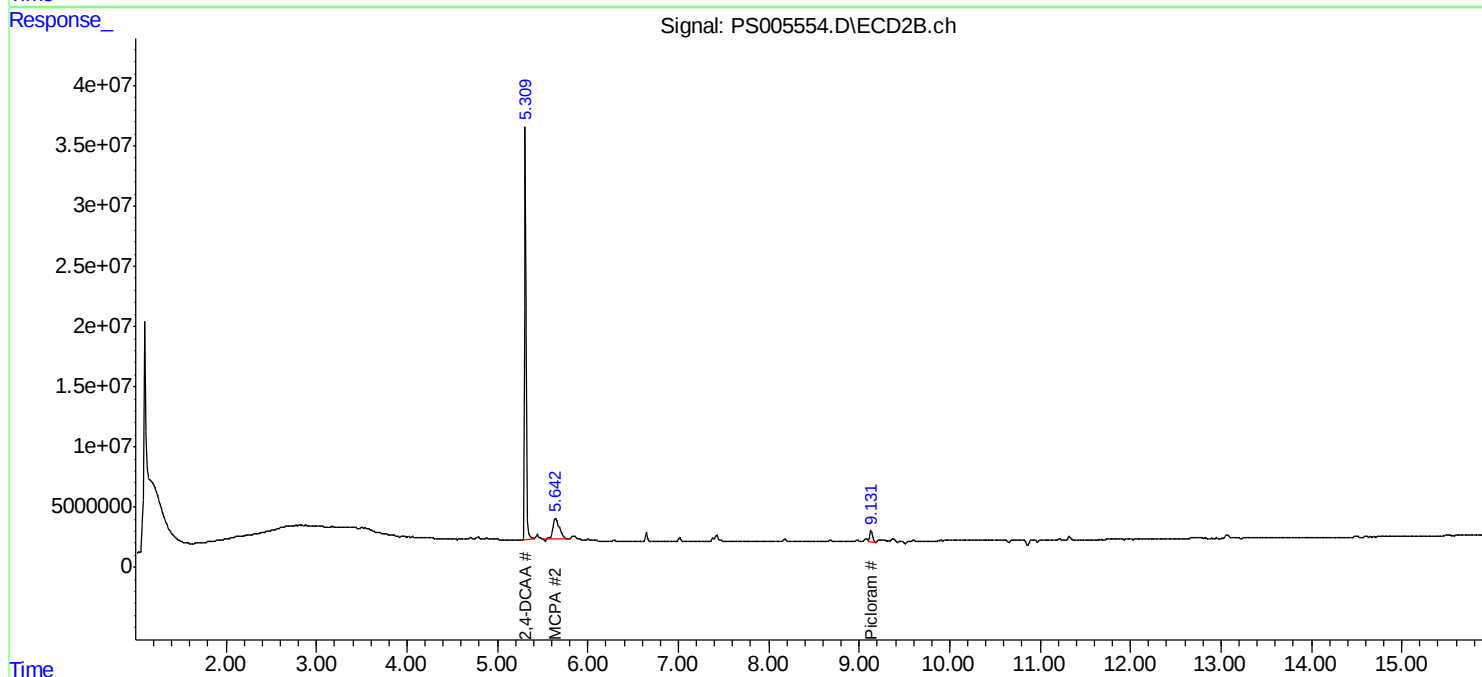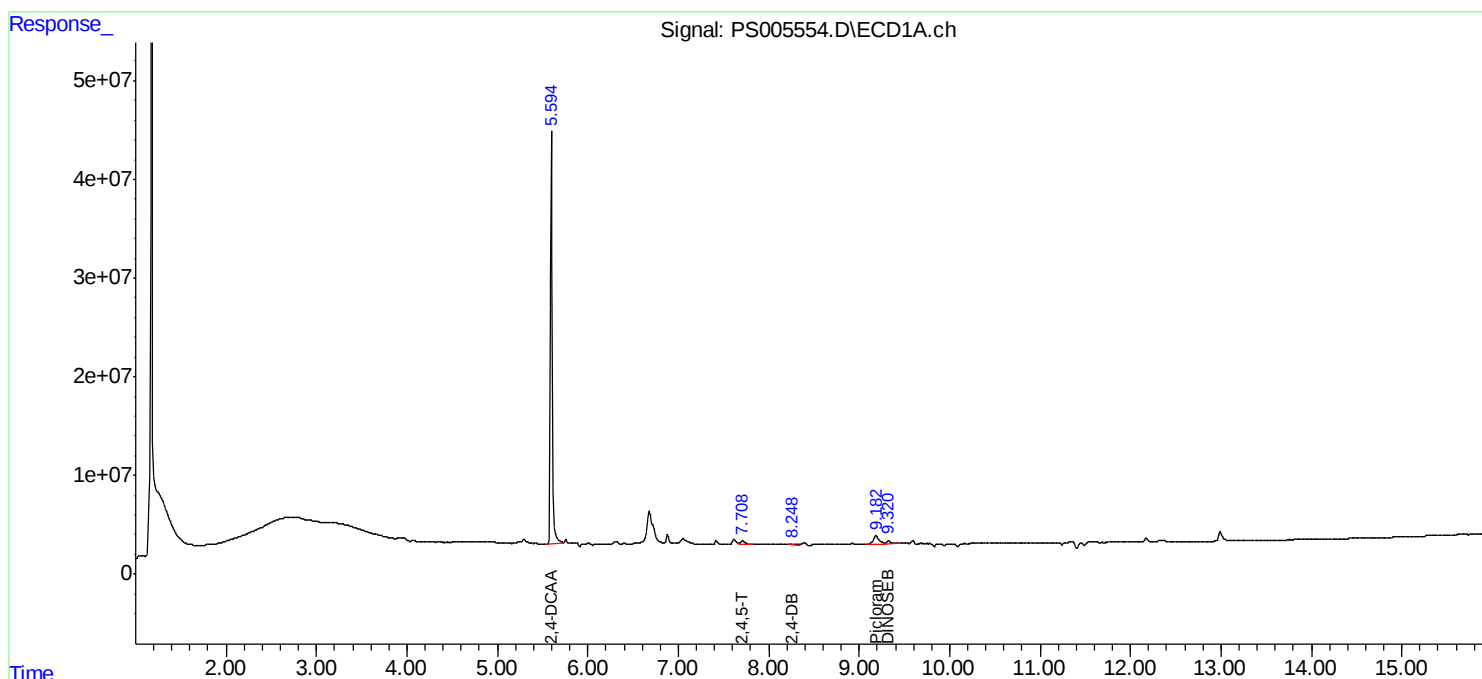


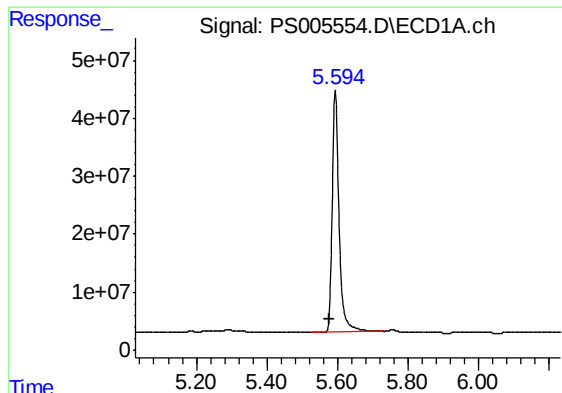

#4 2,4-DCAA


R.T.: 5.594 min
Delta R.T.: 0.018 min
Response: 562688625
Conc: 357.09 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

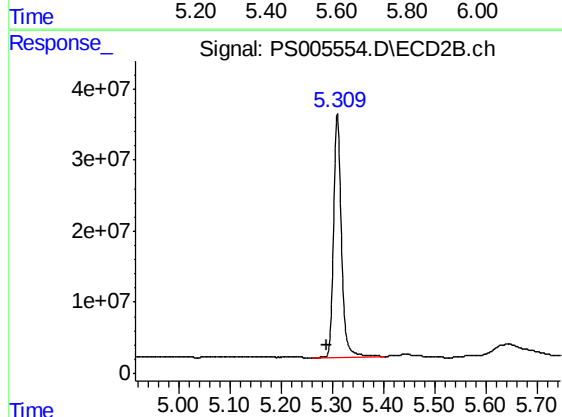


#4 2,4-DCAA

R.T.: 5.310 min
Delta R.T.: 0.022 min
Response: 361849562
Conc: 350.32 ng/ml

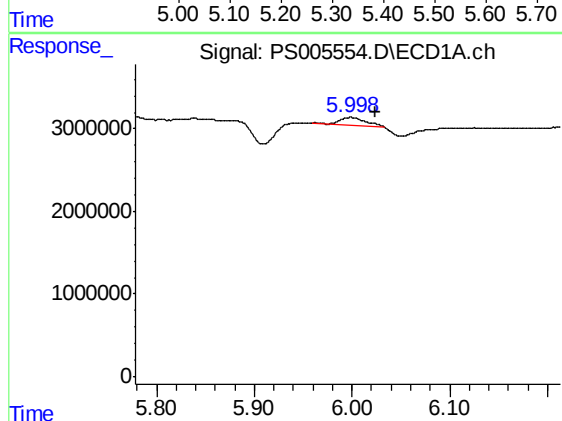


#7 MCPA

R.T.: 5.999 min
Delta R.T.: -0.026 min
Response: 1652086
Conc: N.D.

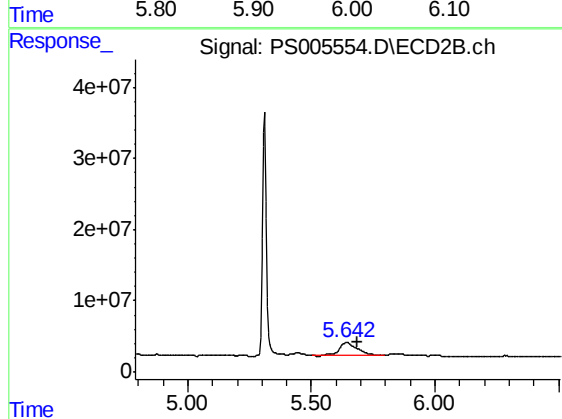

#7 MCPA


R.T.: 5.643 min
Delta R.T.: -0.044 min
Response: 86670294
Conc: 19.67 ug/ml

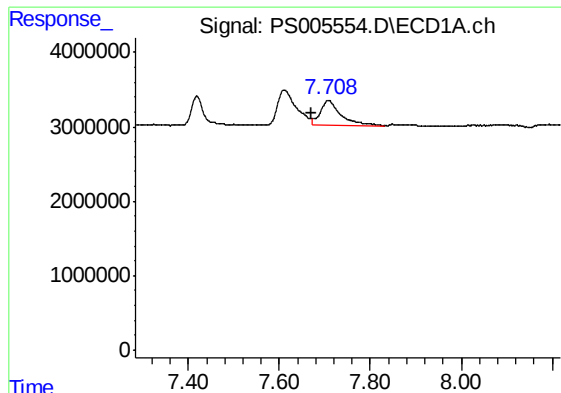

#12 2,4,5-T


R.T.: 7.708 min
Delta R.T.: 0.036 min
Response: 10687105
Conc: 1.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

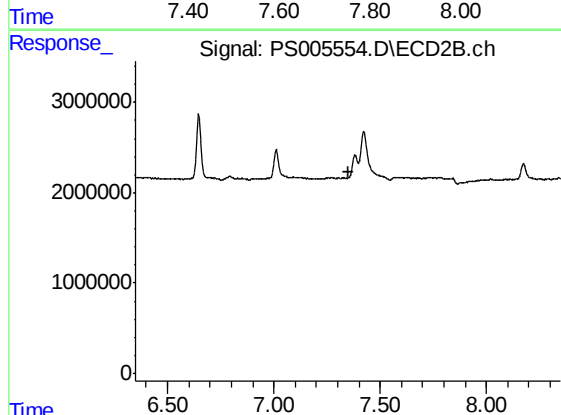


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.349 min
Response: 0
Conc: N.D.

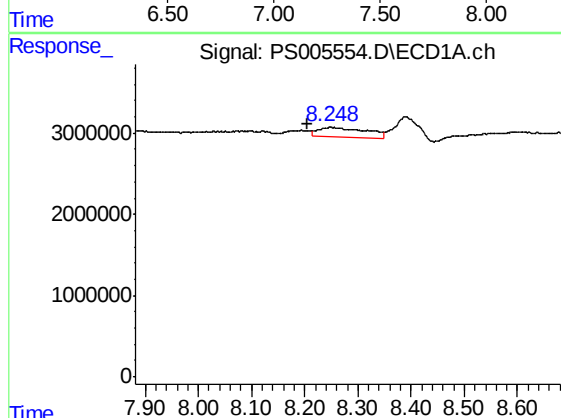


#13 2,4-DB

R.T.: 8.248 min
Delta R.T.: 0.043 min
Response: 7498695
Conc: 5.99 ng/ml

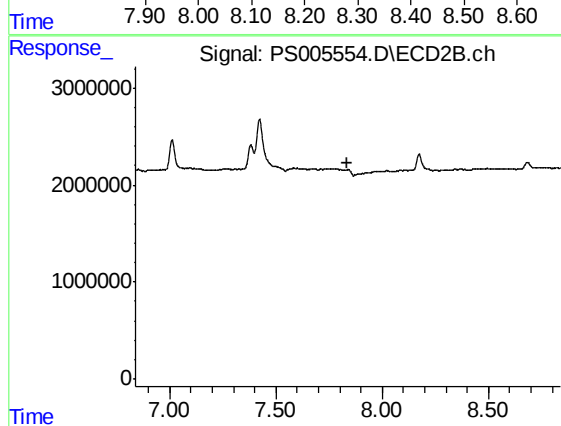

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.

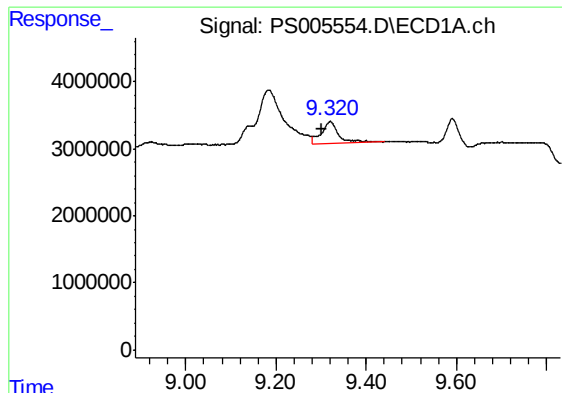

#14 DINOSEB


R.T.: 9.320 min
Delta R.T.: 0.020 min
Response: 8603190
Conc: 1.23 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

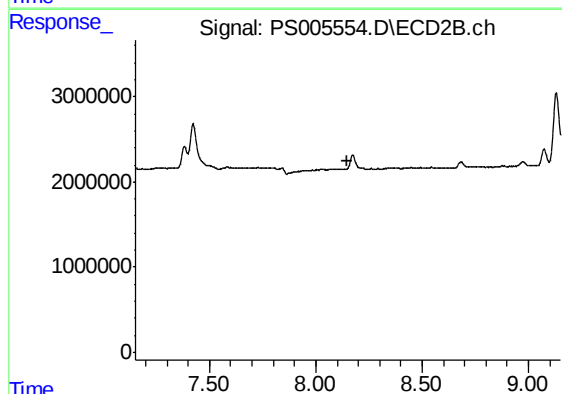


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 8.151 min
Response: 0
Conc: N.D.

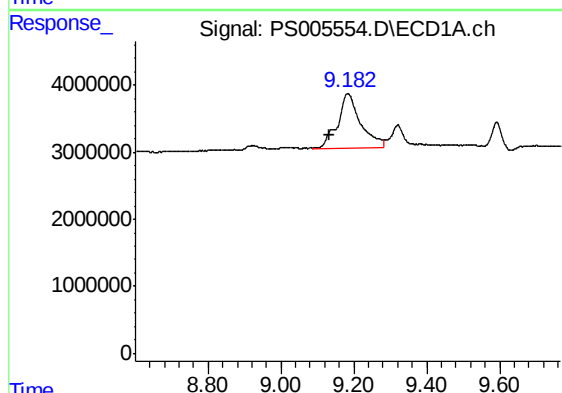

#15 Picloram

R.T.: 9.184 min
Delta R.T.: 0.050 min
Response: 35150089
Conc: 2.82 ng/ml

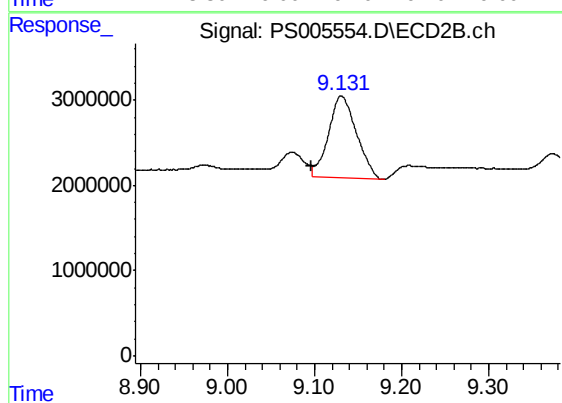

#15 Picloram

R.T.: 9.131 min
Delta R.T.: 0.035 min
Response: 21450848
Conc: 2.74 ng/ml