

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071919\
 Data File : PS005557.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2019 08:53
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 17:02:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 19 08:54:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.570	5.285	592.0E6	378.0E6	375.699	366.004
Target Compounds							
3) T	4-Nitroph...	5.390	0.000	2926774	0	4.094	N.D. #
7) T	MCPA	0.000	5.617	0	49698017	N.D.	11.279
9) T	2,4-D	6.655	0.000	96236927	0	54.877	N.D. #
10) T	Pentachlo...	6.856	0.000	2940314	0	<MDL	N.D. #
11) T	2,4,5-TP ...	7.392	0.000	1141207	0	<MDL	N.D. #
12) T	2,4,5-T	7.680	7.394	10933985	44420114	1.292	8.656 #
15) T	Picloram	9.141	9.097	361.6E6	211.0E6	29.022	26.942
16) T	DCPA	9.566	9.097	4200602	211.0E6	<MDL	29.855 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071919\
Data File : PS005557.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2019 08:53
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 17:02:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
Quant Title : 8080.M
QLast Update : Fri Jul 19 08:54:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

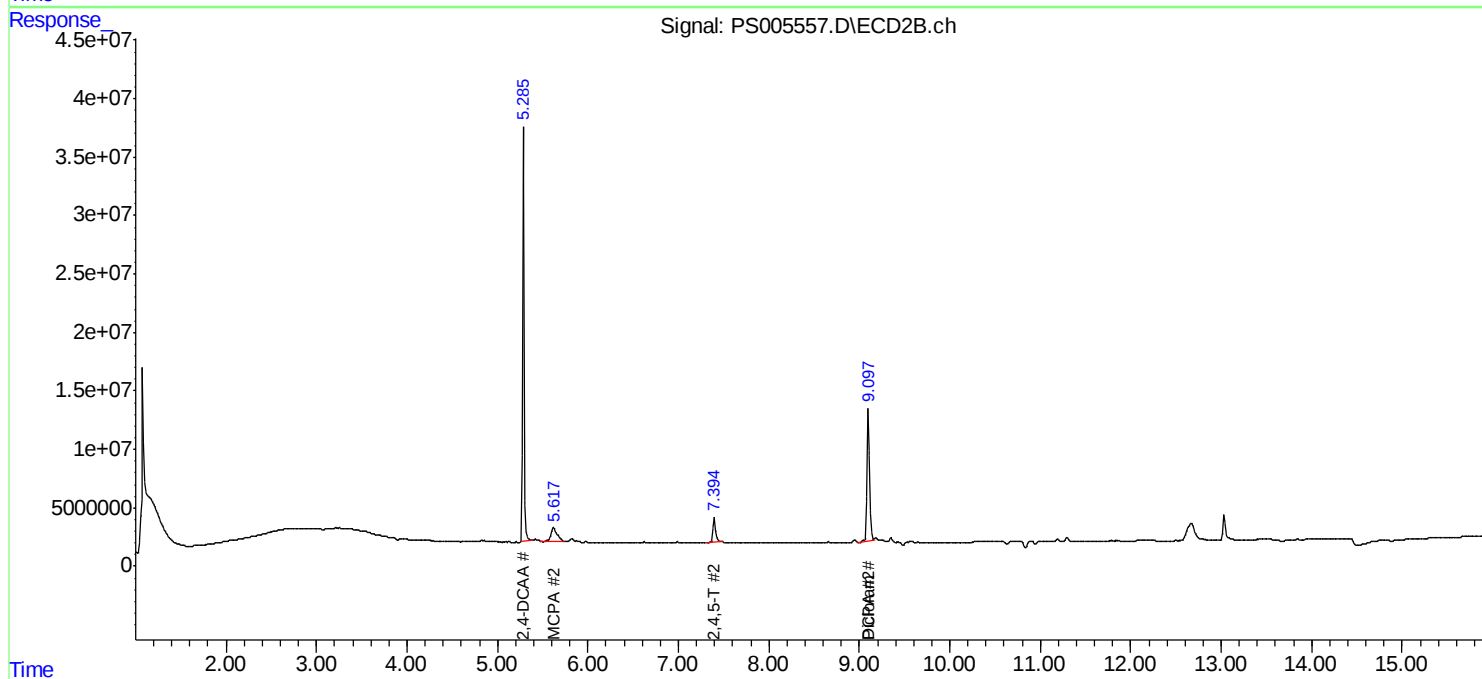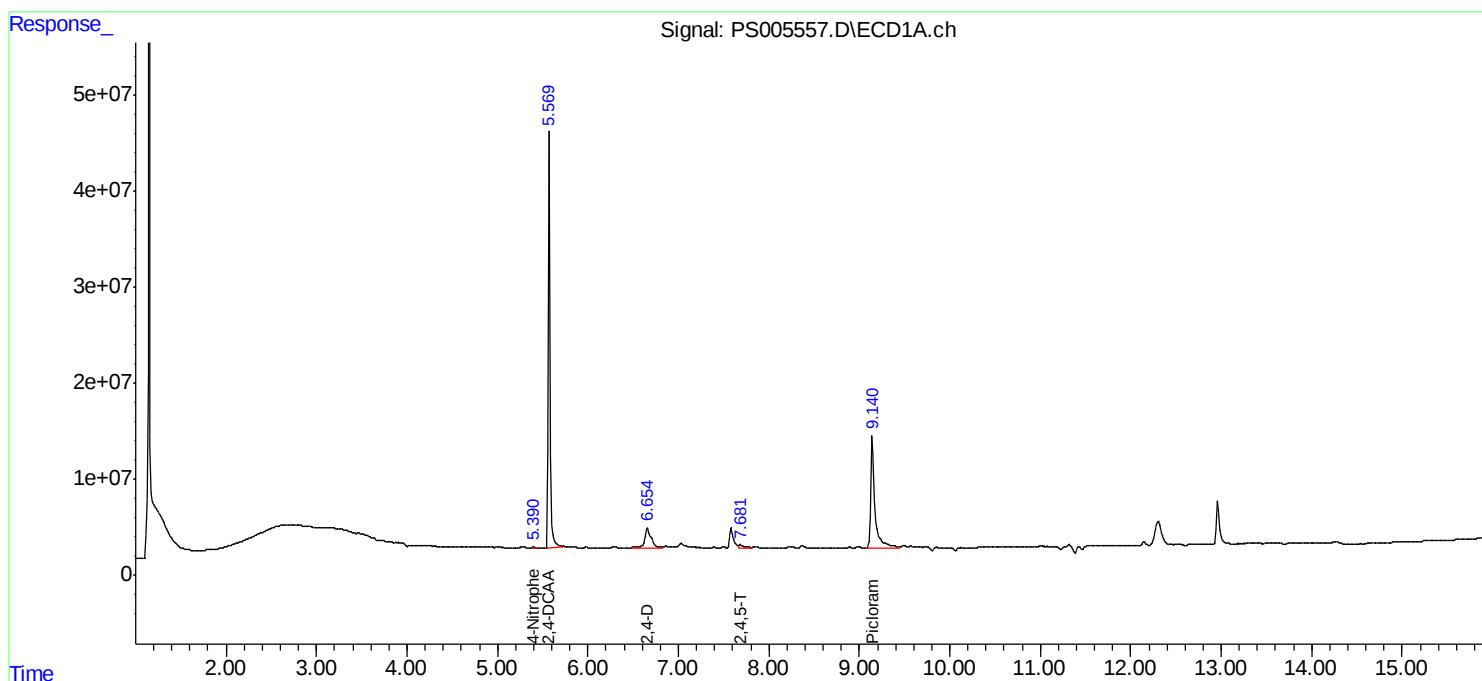


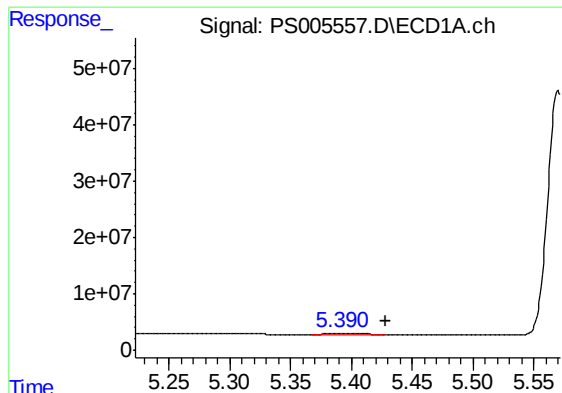

#3 4-Nitrophenol


R.T.: 5.390 min
Delta R.T.: -0.038 min
Response: 2926774
Conc: 4.09 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

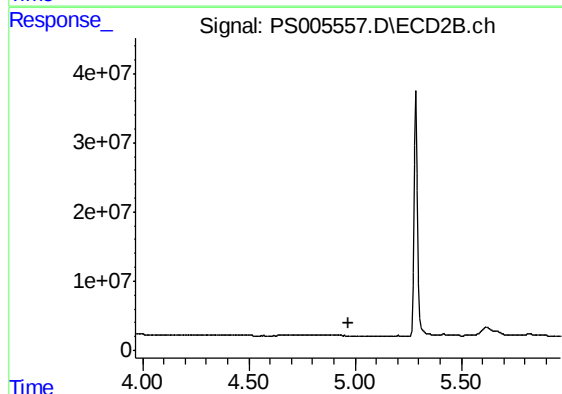


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.966 min
Response: 0
Conc: N.D.

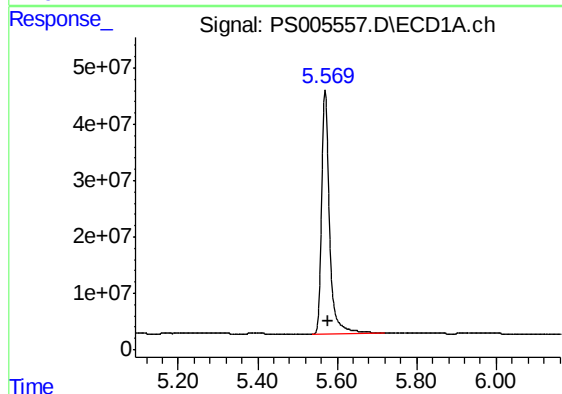


#4 2,4-DCAA

R.T.: 5.570 min
Delta R.T.: -0.006 min
Response: 592008772
Conc: 375.70 ng/ml

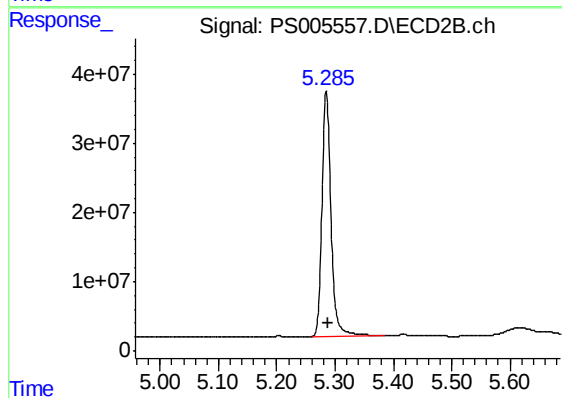

#4 2,4-DCAA


R.T.: 5.285 min
Delta R.T.: -0.003 min
Response: 378045256
Conc: 366.00 ng/ml

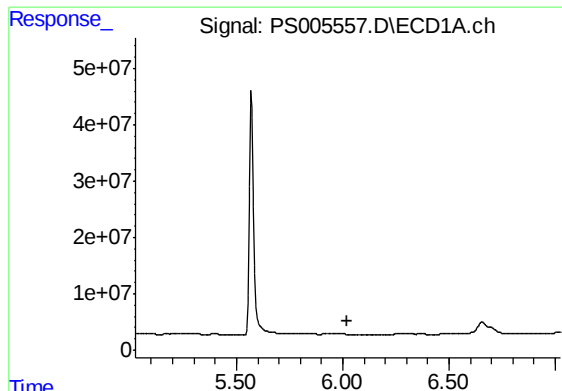

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 6.024 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

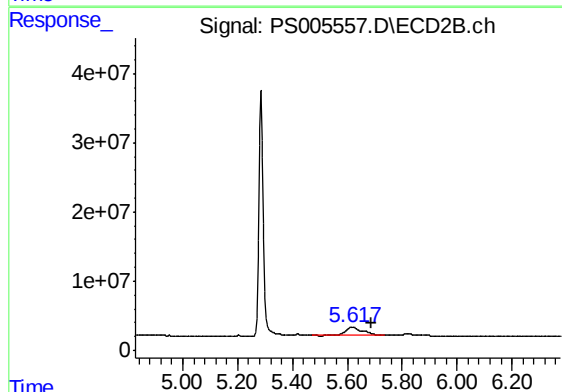


#7 MCPA

R.T.: 5.617 min
Delta R.T.: -0.070 min
Response: 49698017
Conc: 11.28 ug/ml

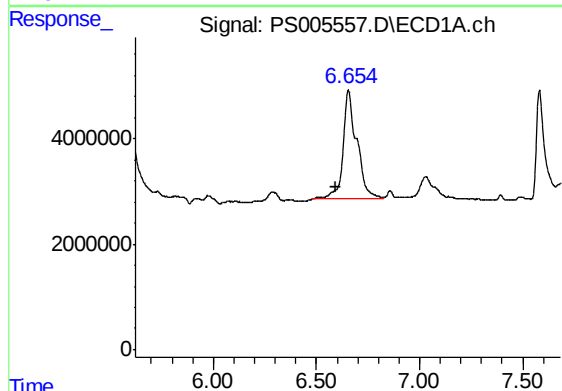


#9 2,4-D

R.T.: 6.655 min
Delta R.T.: 0.062 min
Response: 96236927
Conc: 54.88 ng/ml

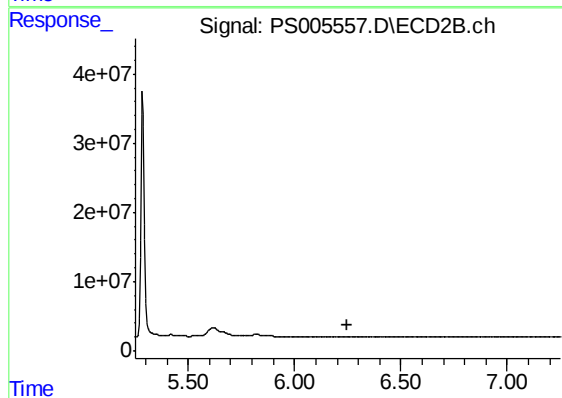

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 6.251 min
Response: 0
Conc: N.D.

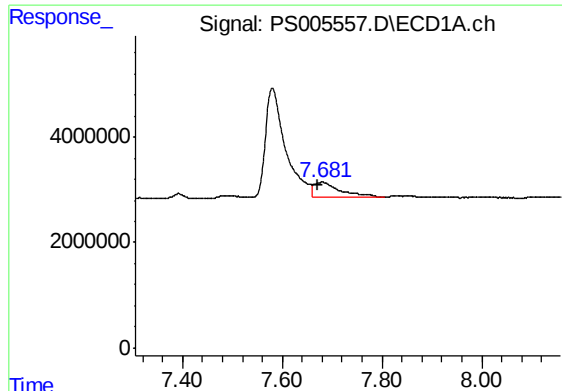

#12 2,4,5-T


R.T.: 7.680 min
Delta R.T.: 0.008 min
Response: 10933985
Conc: 1.29 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

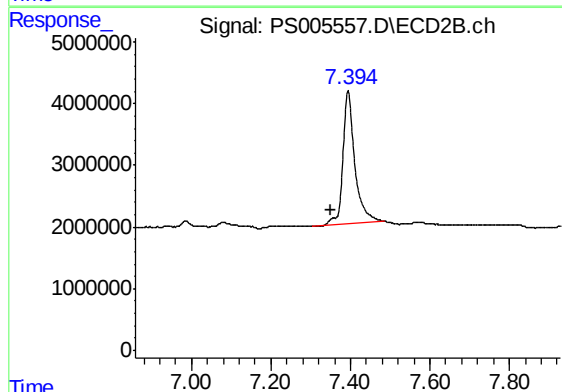


#12 2,4,5-T

R.T.: 7.394 min
Delta R.T.: 0.045 min
Response: 44420114
Conc: 8.66 ng/ml

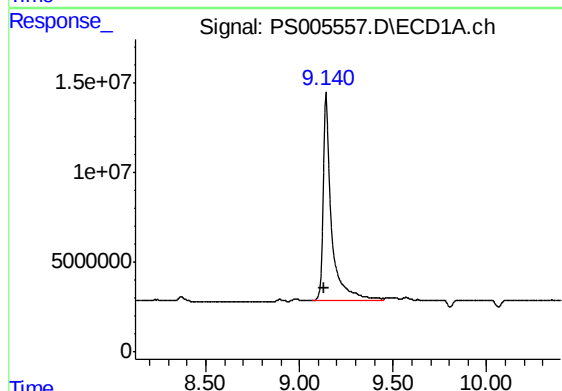


#15 Picloram

R.T.: 9.141 min
Delta R.T.: 0.008 min
Response: 361573266
Conc: 29.02 ng/ml

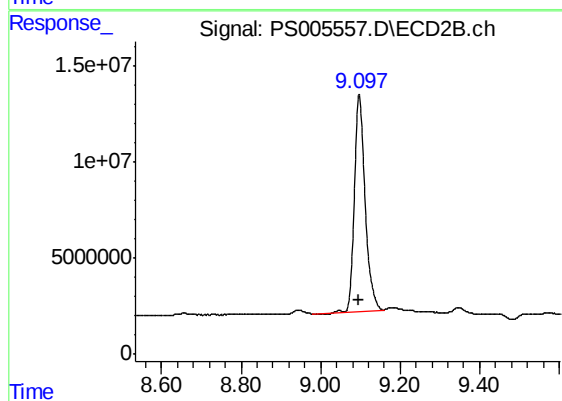

#15 Picloram


R.T.: 9.097 min
Delta R.T.: 0.001 min
Response: 211031546
Conc: 26.94 ng/ml

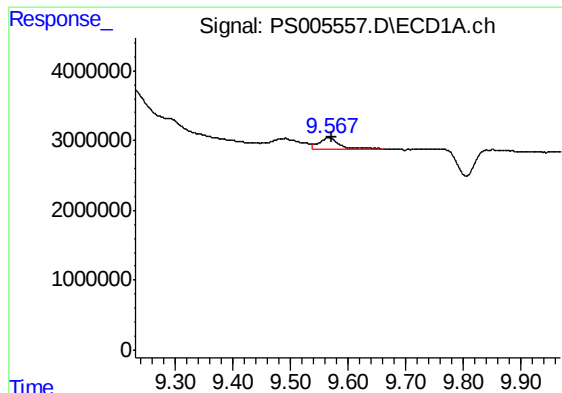

#16 DCPA

R.T.: 9.566 min
Delta R.T.: -0.006 min
Response: 4200602
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

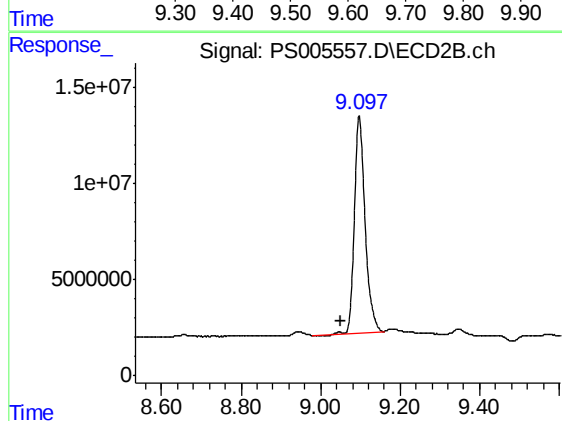

#16 DCPA

R.T.: 9.097 min
Delta R.T.: 0.046 min
Response: 211031546
Conc: 29.86 ng/ml