

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071919\
 Data File : PS005568.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2019 15:32
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 17:05:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 19 08:54:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.569	5.286	610.2E6	394.8E6	387.256	382.204
Target Compounds							
2) T	3,5-DICHL...	4.855	0.000	5555106	0	2.611	N.D. #
3) T	4-Nitroph...	5.391	0.000	3517711	0	4.921	N.D. #
7) T	MCPA	5.981	5.619	2968036	90194853	<MDL	20.470 #
9) T	2,4-D	6.654	0.000	166.2E6	0	94.800	N.D. #
10) T	Pentachlo...	6.855	0.000	3882929	0	<MDL	N.D. #
11) T	2,4,5-TP ...	7.392	0.000	594223	0	<MDL	N.D. #
12) T	2,4,5-T	7.686	0.000	1879511	0	<MDL	N.D. #
14) T	DINOSEB	9.295	0.000	1804260	0	<MDL	N.D. #
15) T	Picloram	9.116	0.000	10232106	0	<MDL	N.D. #
16) T	DCPA	9.566	0.000	17211540	0	1.581	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071919\
Data File : PS005568.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2019 15:32
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 17:05:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
Quant Title : 8080.M
QLast Update : Fri Jul 19 08:54:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

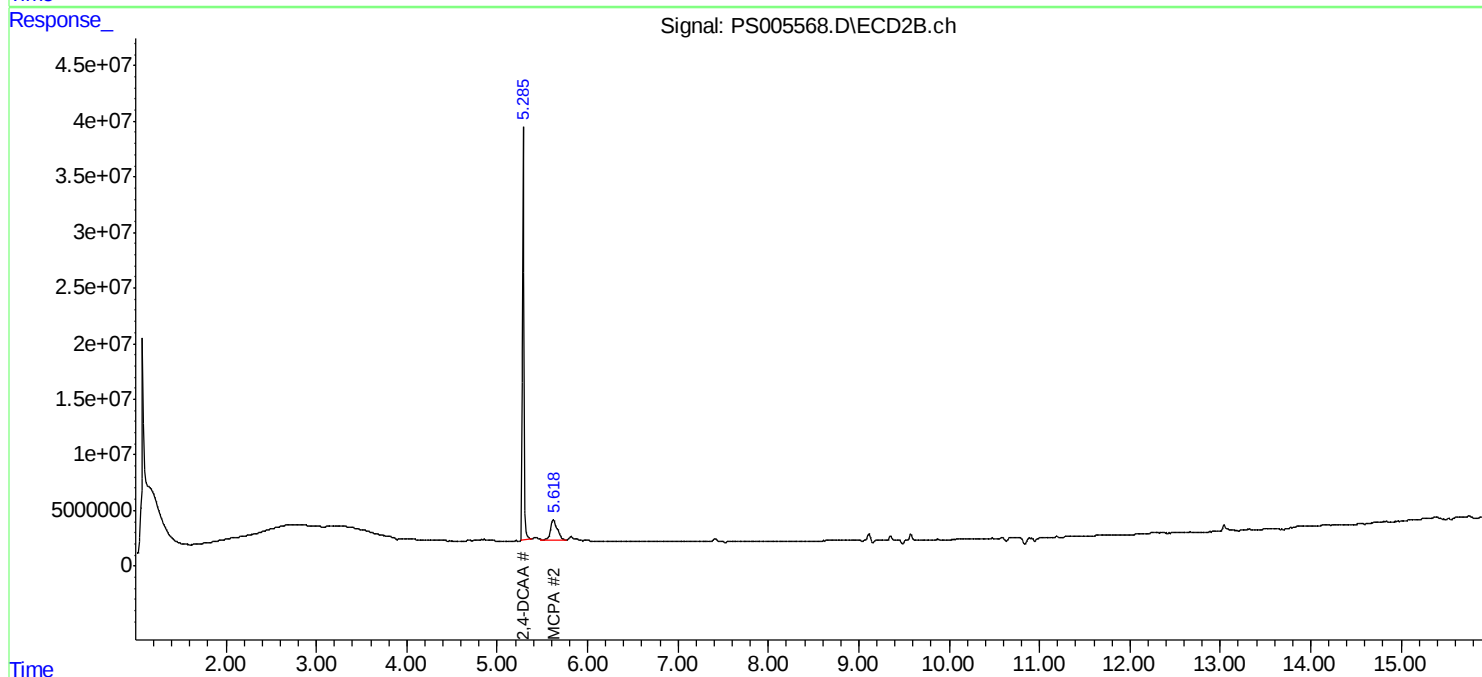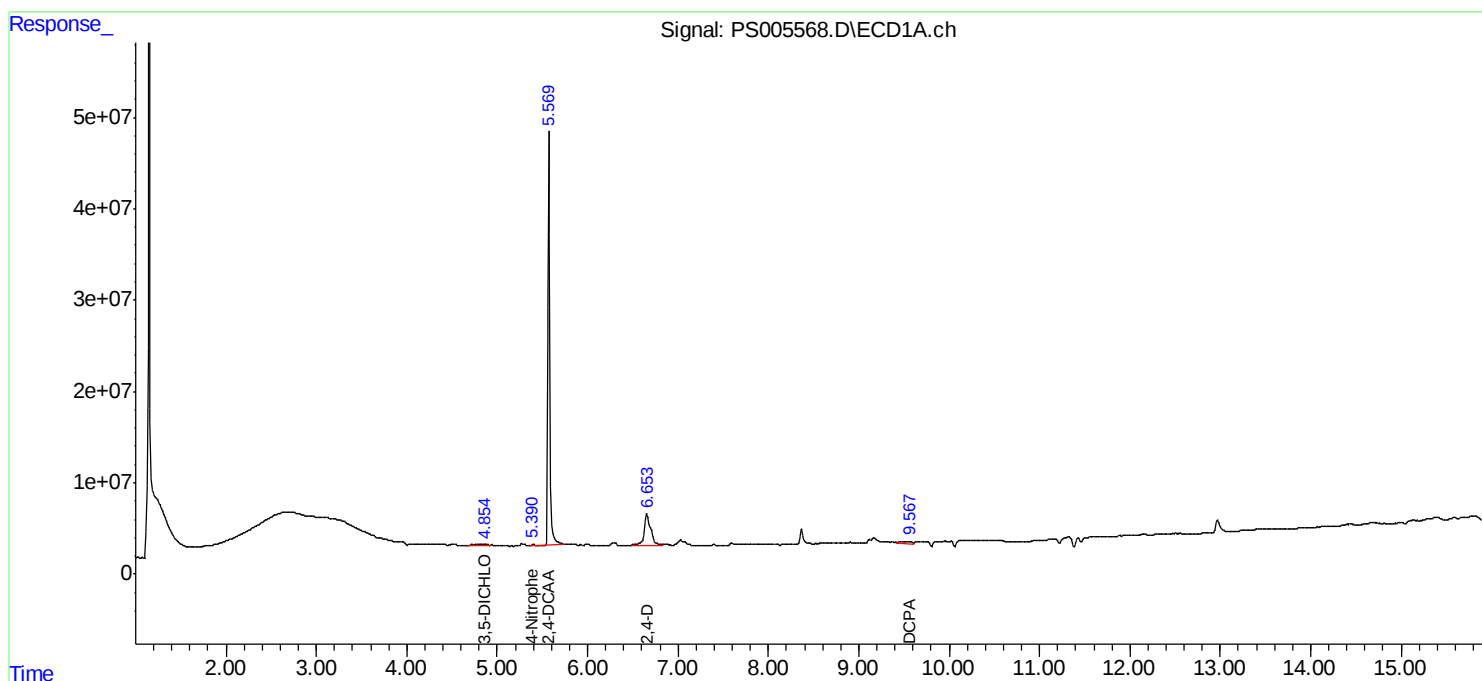


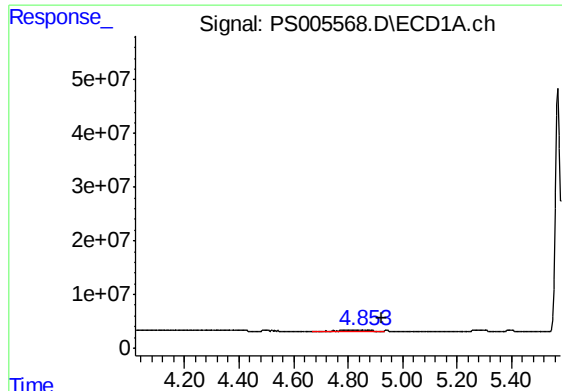

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.855 min
Delta R.T.: -0.070 min
Response: 5555106
Conc: 2.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

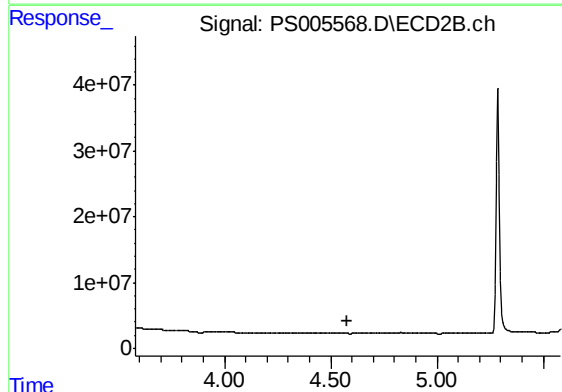


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.581 min
Response: 0
Conc: N.D.

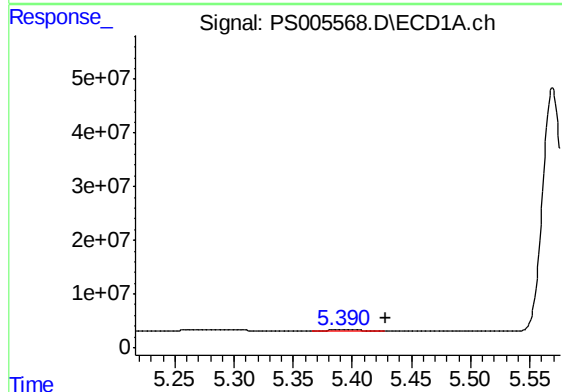


#3 4-Nitrophenol

R.T.: 5.391 min
Delta R.T.: -0.037 min
Response: 3517711
Conc: 4.92 ng/ml

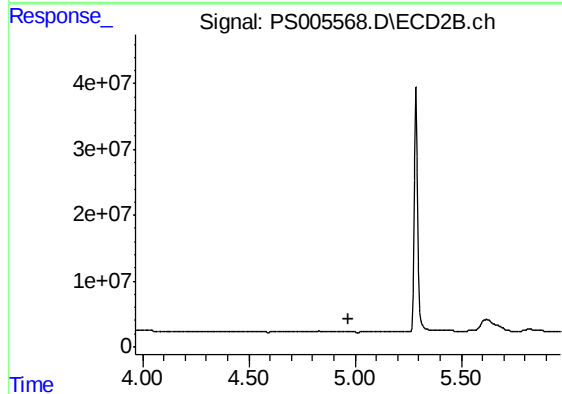

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 4.966 min
Response: 0
Conc: N.D.

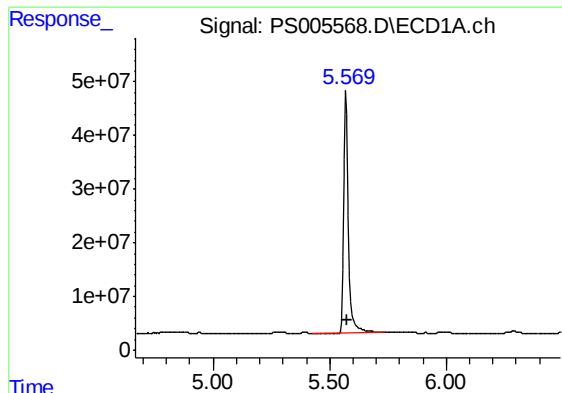

#4 2,4-DCAA


R.T.: 5.569 min
Delta R.T.: -0.007 min
Response: 610220544
Conc: 387.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

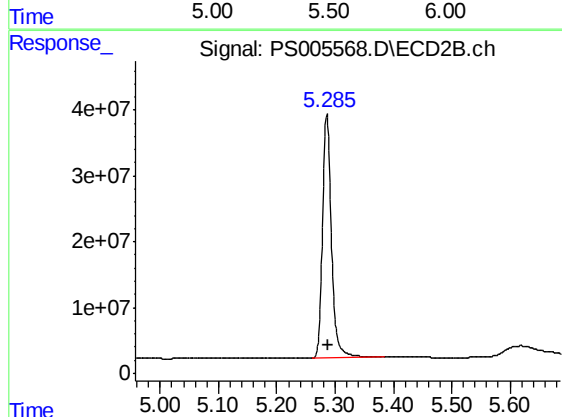


#4 2,4-DCAA

R.T.: 5.286 min
Delta R.T.: -0.002 min
Response: 394778344
Conc: 382.20 ng/ml

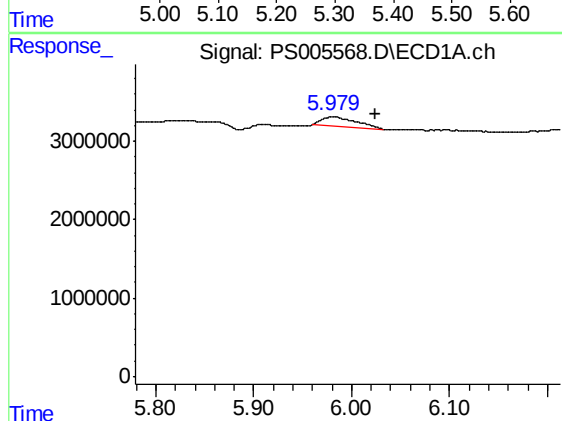


#7 MCPA

R.T.: 5.981 min
Delta R.T.: -0.044 min
Response: 2968036
Conc: N.D.

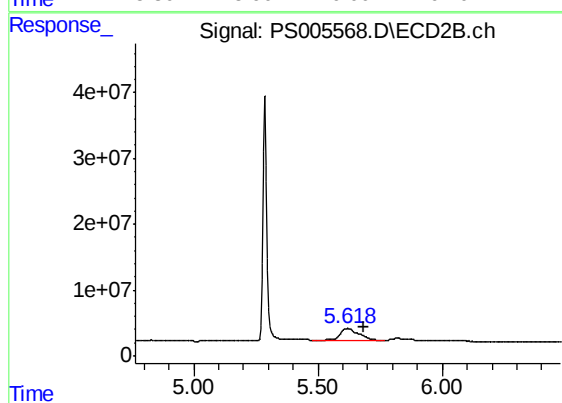

#7 MCPA


R.T.: 5.619 min
Delta R.T.: -0.068 min
Response: 90194853
Conc: 20.47 ug/ml

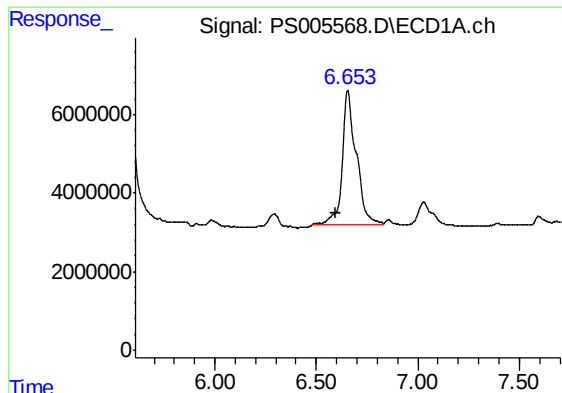

#9 2,4-D


R.T.: 6.654 min
Delta R.T.: 0.061 min
Response: 166248609
Conc: 94.80 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

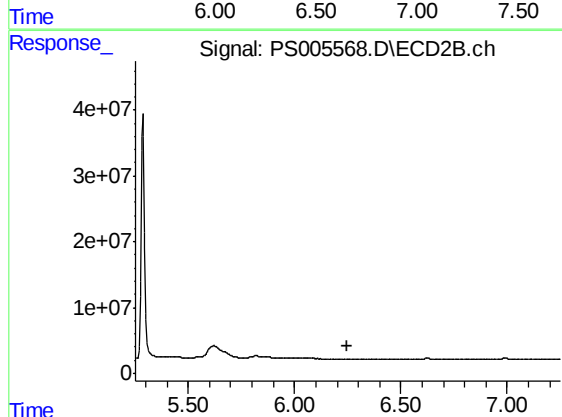


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.251 min
Response: 0
Conc: N.D.

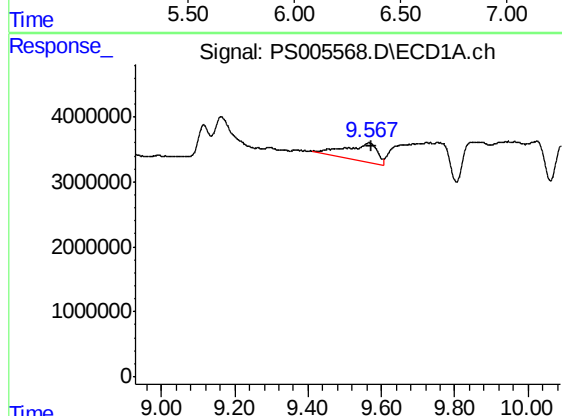

#16 DCPA

R.T.: 9.566 min
Delta R.T.: -0.006 min
Response: 17211540
Conc: 1.58 ng/ml

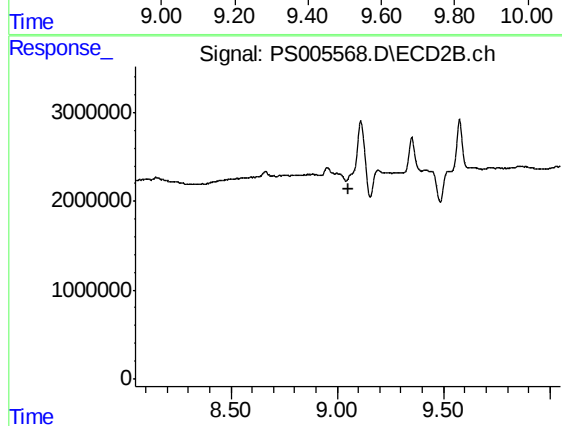

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.051 min
Response: 0
Conc: N.D.