

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071919\
 Data File : PS005579.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2019 19:35
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 00:24:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 19 08:54:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.561	5.277	647.2E6	372.6E6	410.753	360.754
Target Compounds							
3) T	4-Nitroph...	5.382	0.000	3982265	0	5.571	N.D. #
9) T	2,4-D	6.647	0.000	188.5E6	0	107.484	N.D. #
10) T	Pentachlo...	6.846	0.000	5211213	0	<MDL	N.D. #
11) T	2,4,5-TP ...	7.381	0.000	1416948	0	<MDL	N.D. #
12) T	2,4,5-T	7.675	0.000	3051842	0	<MDL	N.D. #
13) T	2,4-DB	8.216	0.000	7924975	0	6.326	N.D. #
15) T	Picloram	9.149	0.000	19614712	0	1.574	N.D. #
16) T	DCPA	9.558	0.000	10170961	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071919\
Data File : PS005579.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2019 19:35
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 00:24:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
Quant Title : 8080.M
QLast Update : Fri Jul 19 08:54:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

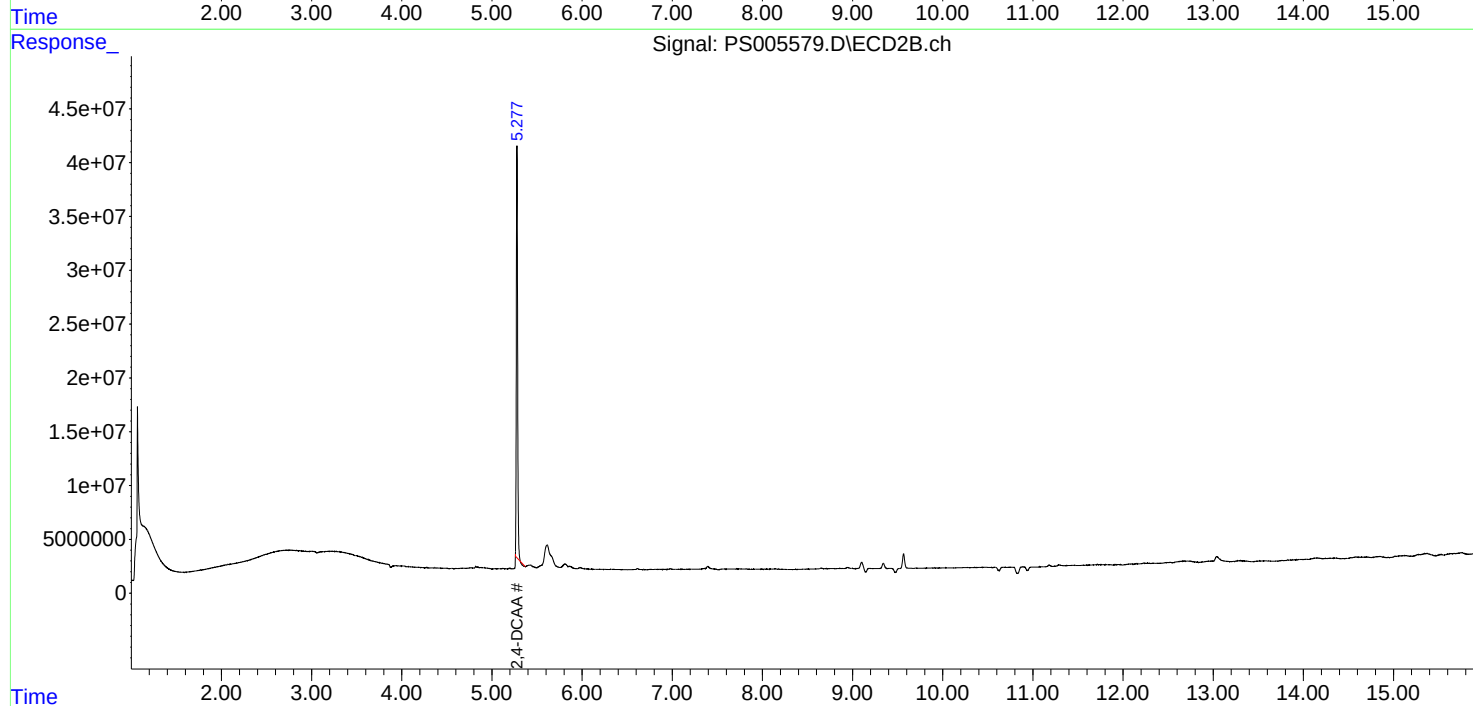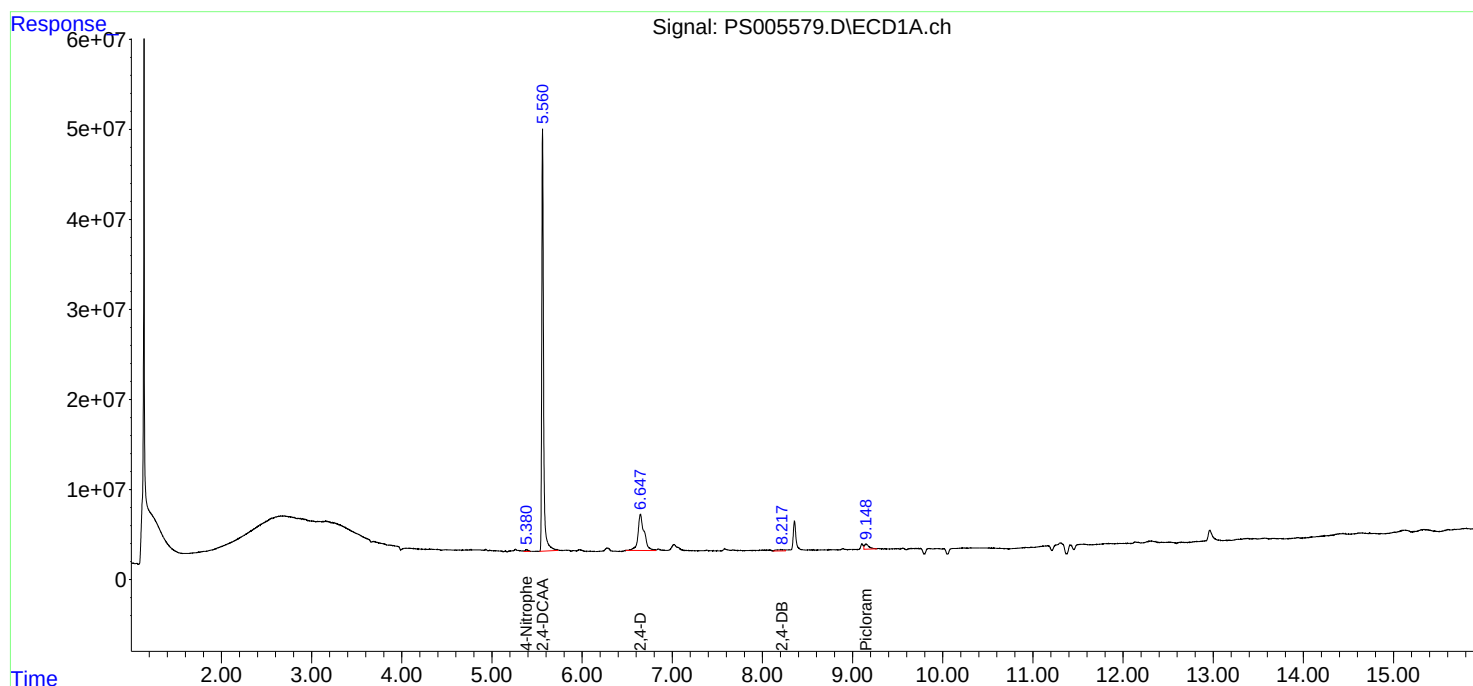


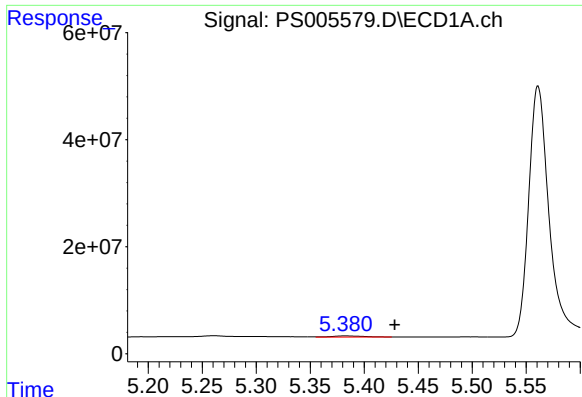

#3 4-Nitrophenol


R.T.: 5.382 min
Delta R.T.: -0.046 min
Response: 3982265
Conc: 5.57 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

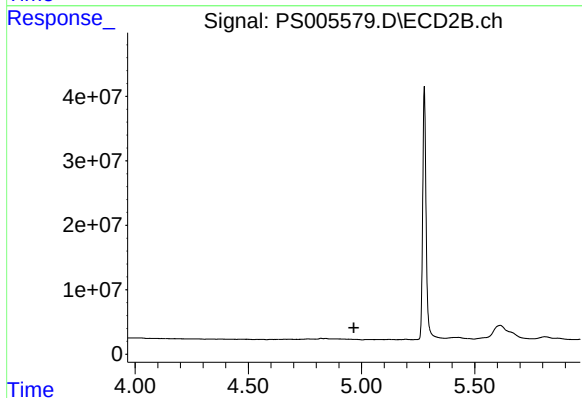


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 4.966 min
Response: 0
Conc: N.D.

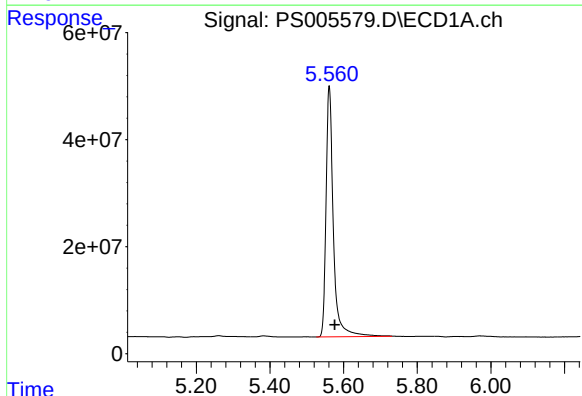


#4 2,4-DCAA

R.T.: 5.561 min
Delta R.T.: -0.015 min
Response: 647245287
Conc: 410.75 ng/ml

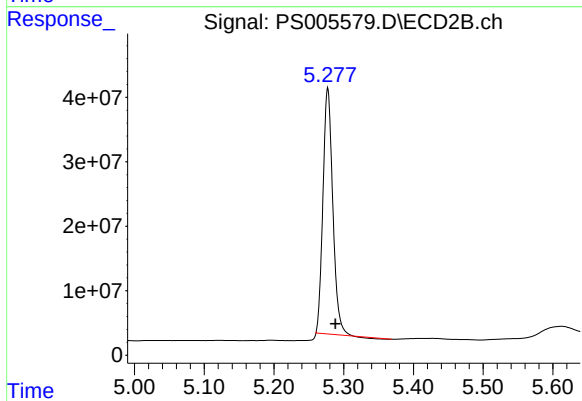

#4 2,4-DCAA


R.T.: 5.277 min
Delta R.T.: -0.011 min
Response: 372623401
Conc: 360.75 ng/ml

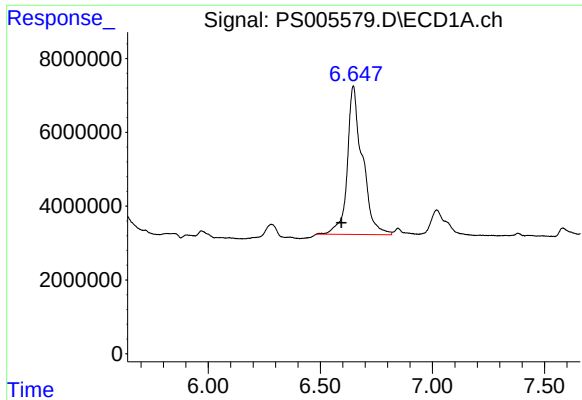

#9 2,4-D


R.T.: 6.647 min
Delta R.T.: 0.054 min
Response: 188493586
Conc: 107.48 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

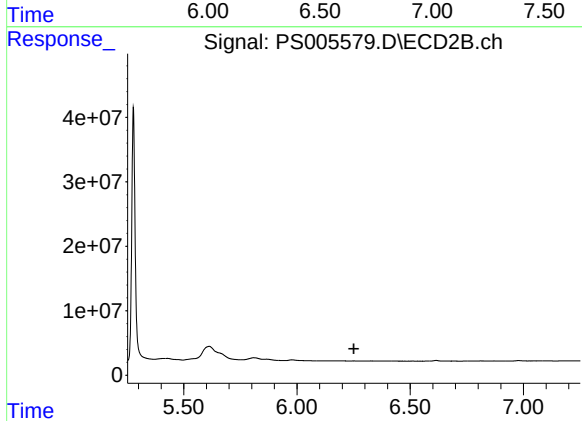


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.251 min
Response: 0
Conc: N.D.

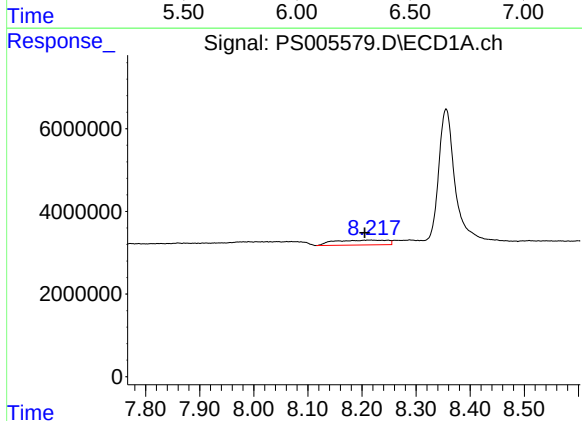


#13 2,4-DB

R.T.: 8.216 min
Delta R.T.: 0.011 min
Response: 7924975
Conc: 6.33 ng/ml

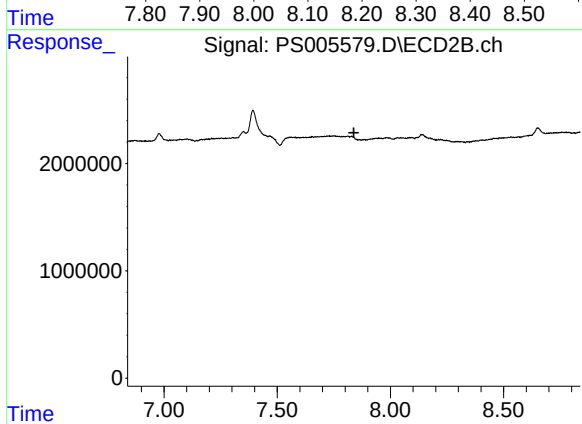

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.

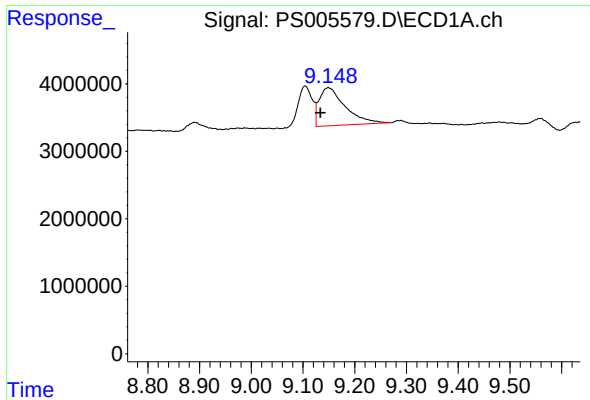

#15 Picloram

R.T.: 9.149 min
Delta R.T.: 0.015 min
Response: 19614712
Conc: 1.57 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

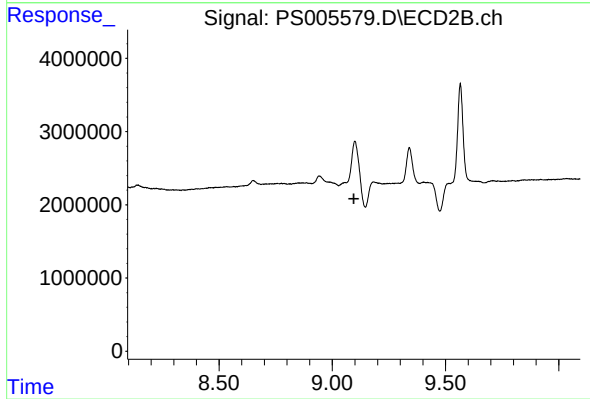

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.096 min
Response: 0
Conc: N.D.