

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071919\
 Data File : PS005591.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2019 00:01
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 00:30:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 19 08:54:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.582	5.298	675.0E6	429.2E6	428.377	415.486
Target Compounds							
2) T	3,5-DICHL...	4.953	0.000	2051991	0	<MDL	N.D. #
3) T	4-Nitroph...	5.403	0.000	2737904	0	3.830	N.D. #
7) T	MCPA	5.993	5.631	2635616	83763066	<MDL	19.011 #
10) T	Pentachlo...	6.868	0.000	4875325	0	<MDL	N.D. #
11) T	2,4,5-TP ...	7.404	0.000	811232	0	<MDL	N.D. #
12) T	2,4,5-T	7.700	0.000	2761985	0	<MDL	N.D. #
13) T	2,4-DB	8.271	0.000	9964788	0	7.955	N.D. #
14) T	DINOSEB	9.306	0.000	11084298	0	1.589	N.D. #
15) T	Picloram	9.127	0.000	17686045	0	1.420	N.D. #
16) T	DCPA	9.578	0.000	17254474	0	1.585	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071919\
Data File : PS005591.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2019 00:01
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 00:30:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
Quant Title : 8080.M
QLast Update : Fri Jul 19 08:54:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

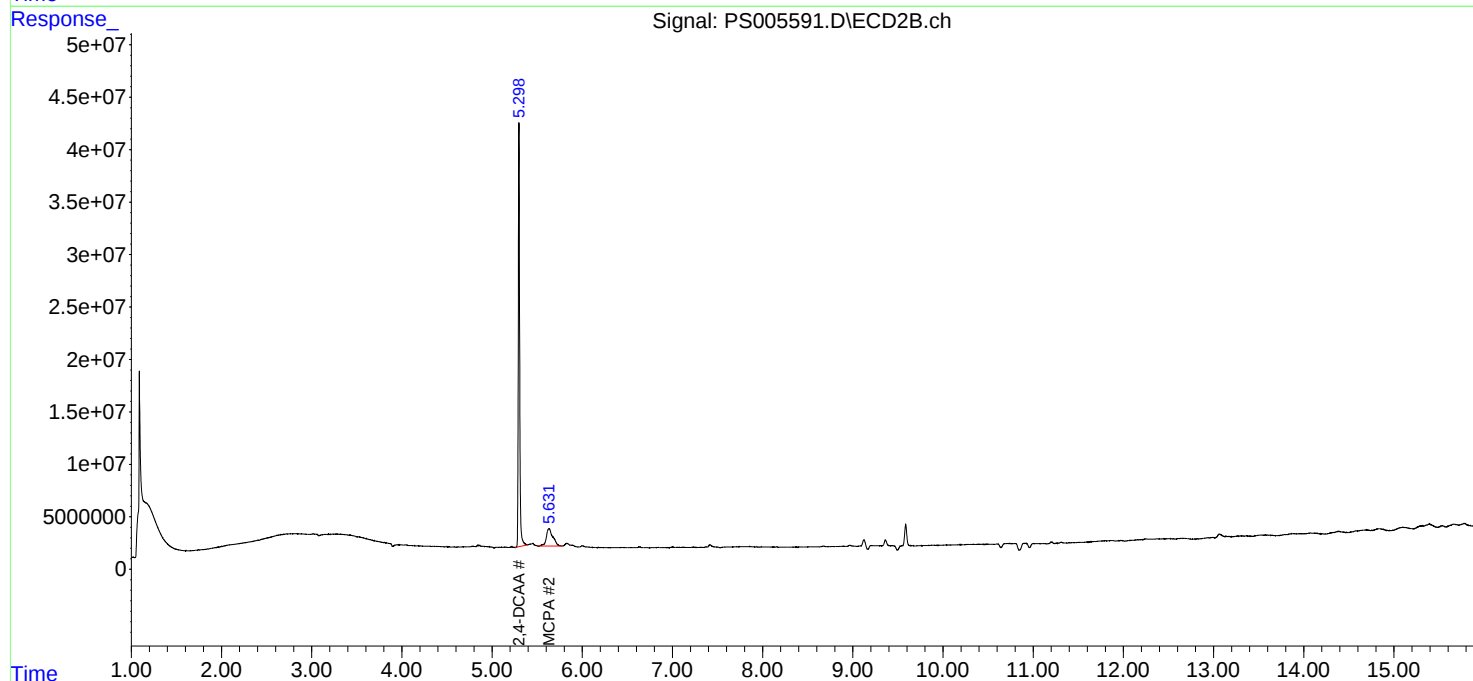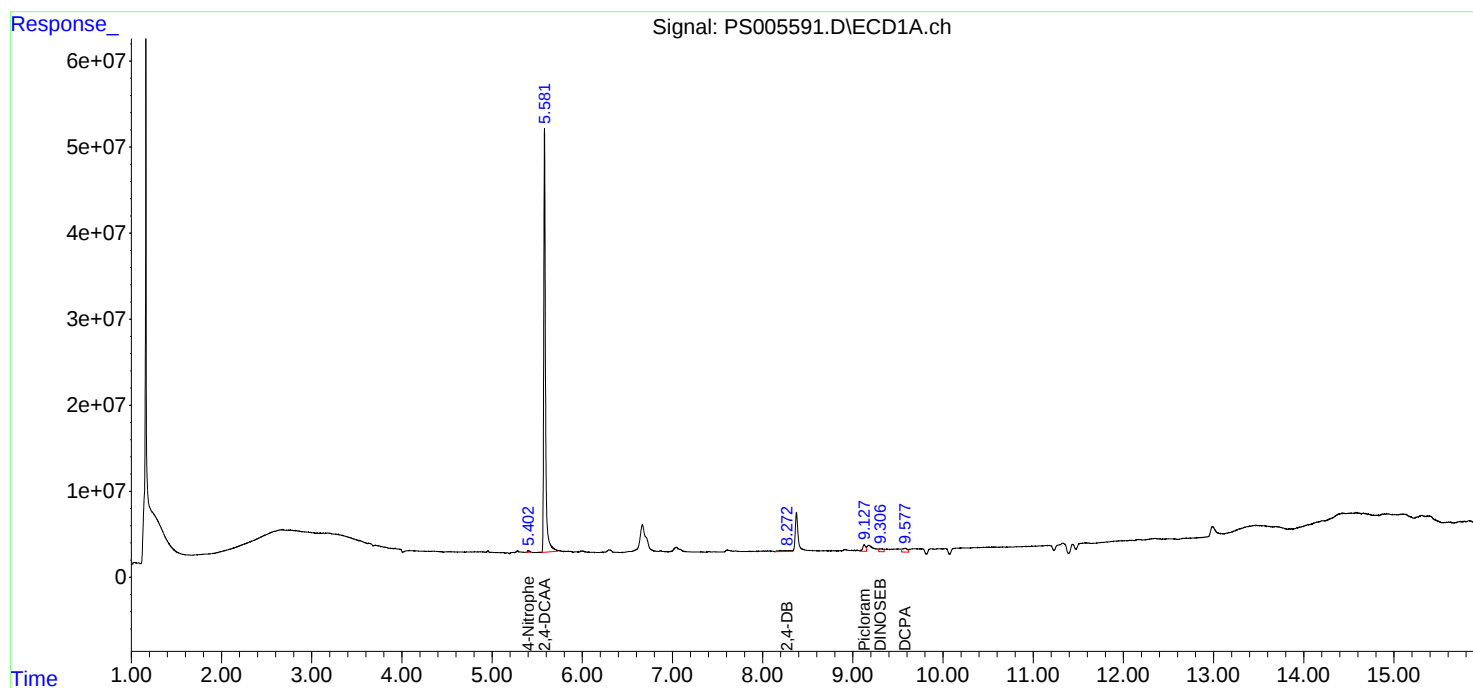


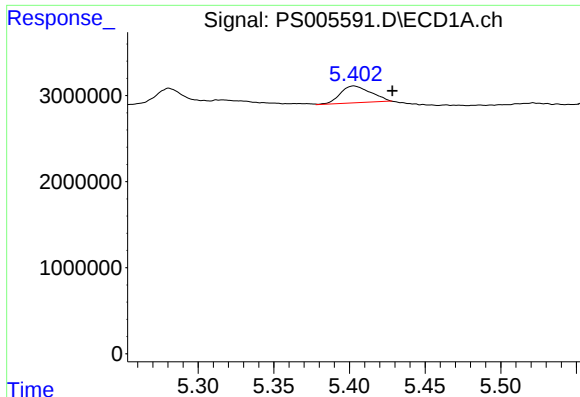

#3 4-Nitrophenol


R.T.: 5.403 min
Delta R.T.: -0.025 min
Response: 2737904
Conc: 3.83 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

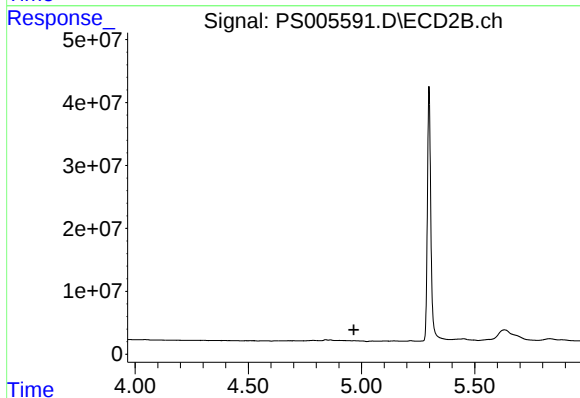


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.966 min
Response: 0
Conc: N.D.

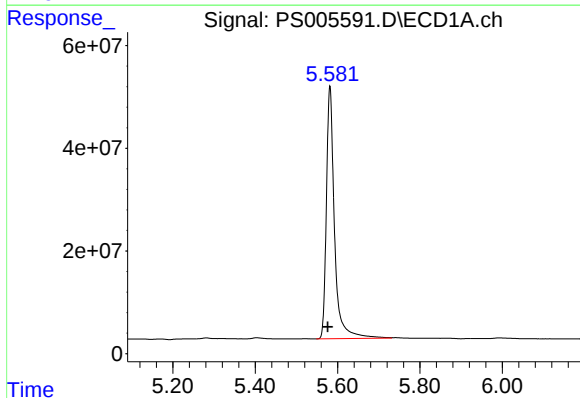


#4 2,4-DCAA

R.T.: 5.582 min
Delta R.T.: 0.006 min
Response: 675016375
Conc: 428.38 ng/ml

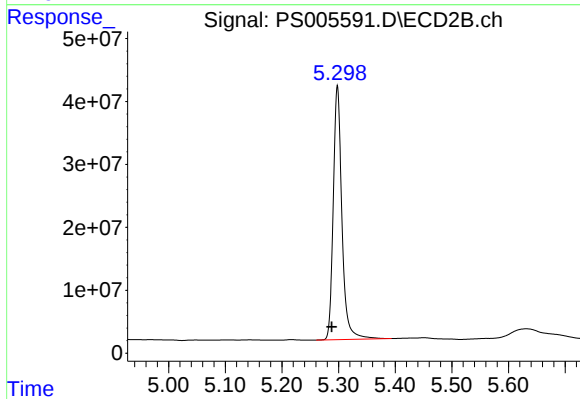

#4 2,4-DCAA


R.T.: 5.298 min
Delta R.T.: 0.010 min
Response: 429155780
Conc: 415.49 ng/ml

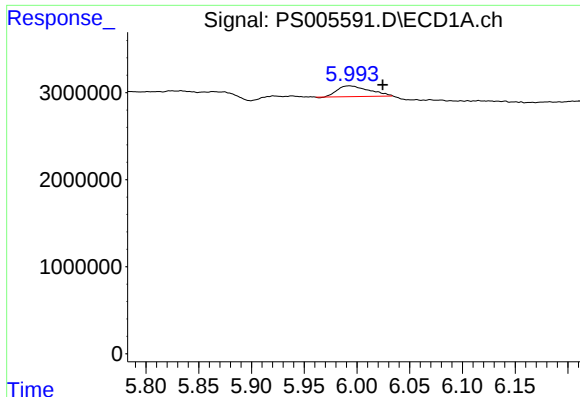

#7 MCPA


R.T.: 5.993 min
Delta R.T.: -0.032 min
Response: 2635616
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

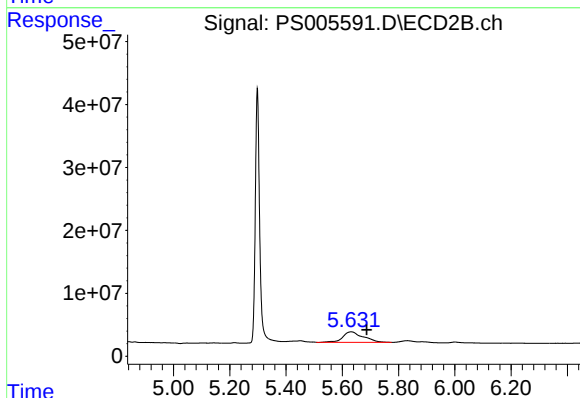


#7 MCPA

R.T.: 5.631 min
Delta R.T.: -0.055 min
Response: 83763066
Conc: 19.01 ug/ml

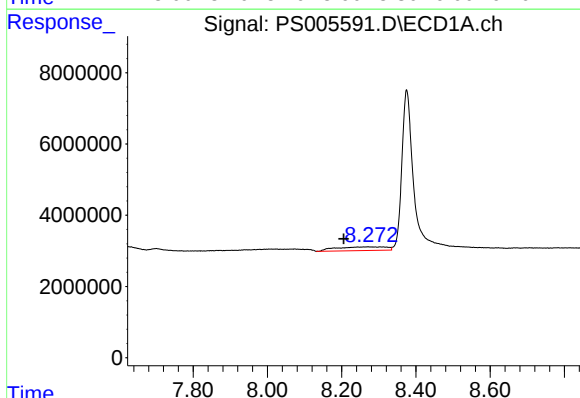


#13 2,4-DB

R.T.: 8.271 min
Delta R.T.: 0.066 min
Response: 9964788
Conc: 7.95 ng/ml

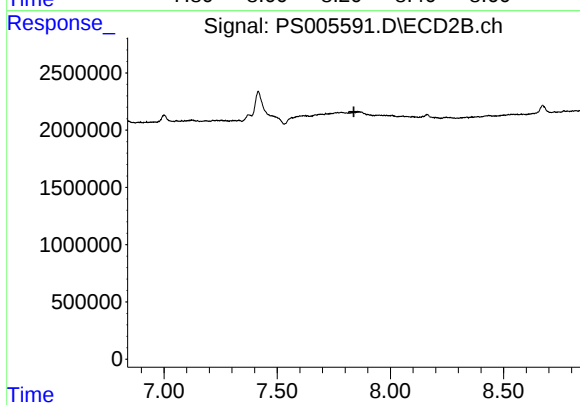

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 7.838 min
Response: 0
Conc: N.D.

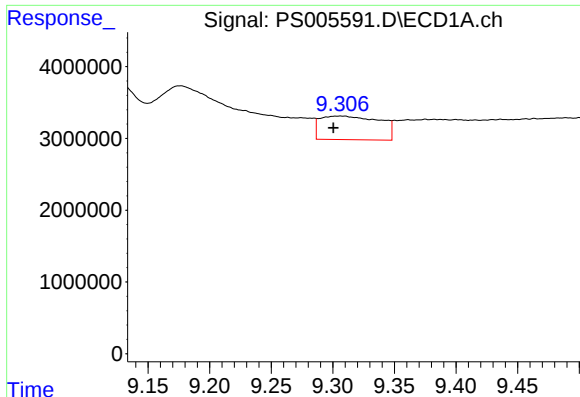

#14 DINoseb


R.T.: 9.306 min
Delta R.T.: 0.005 min
Response: 11084298
Conc: 1.59 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

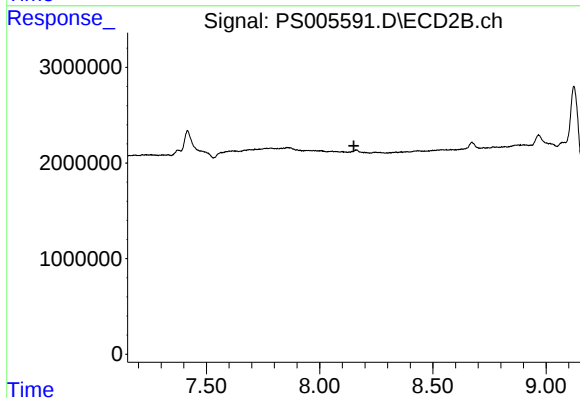


#14 DINoseb

R.T.: 0.000 min
Exp R.T. : 8.151 min
Response: 0
Conc: N.D.

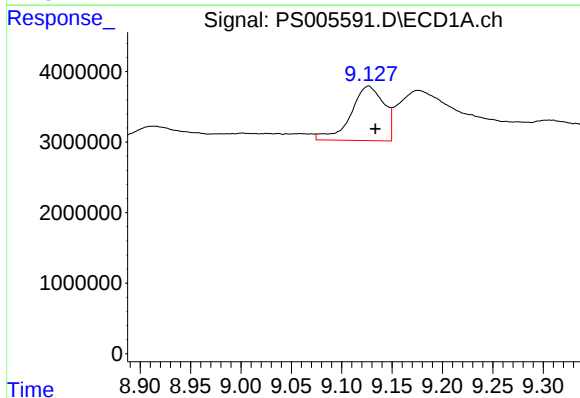


#15 Picloram

R.T.: 9.127 min
Delta R.T.: -0.007 min
Response: 17686045
Conc: 1.42 ng/ml

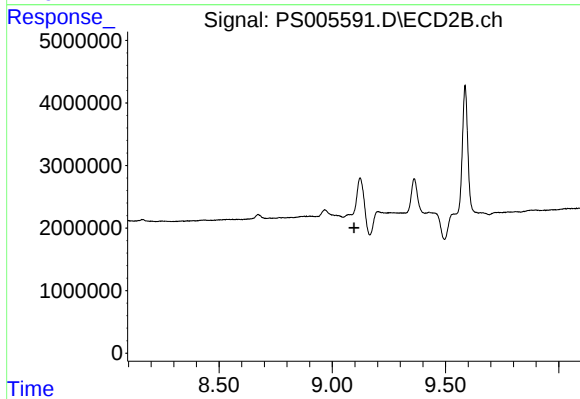

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 9.096 min
Response: 0
Conc: N.D.

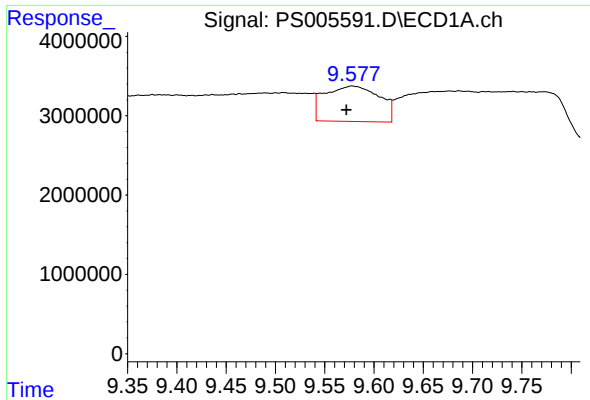

#16 DCPA

R.T.: 9.578 min
Delta R.T.: 0.006 min
Response: 17254474
Conc: 1.58 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

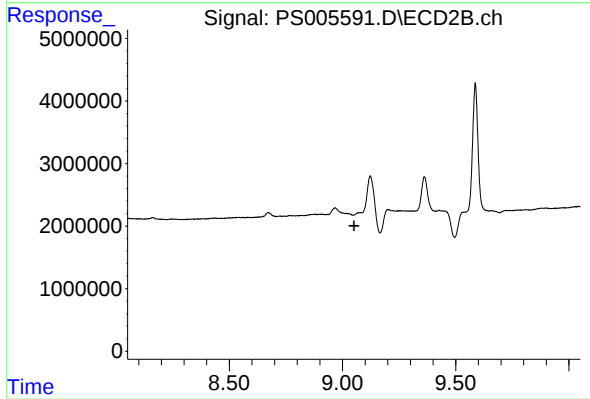

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.051 min
Response: 0
Conc: N.D.