

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071919\
 Data File : PS005603.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2019 04:27
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 05:18:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 19 08:54:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.579	5.280	708.8E6	438.9E6	449.821	424.904
Target Compounds							
2) T	3,5-DICHL...	4.950	0.000	3493660	0	1.642	N.D. #
3) T	4-Nitroph...	5.401	0.000	3453225	0	4.831	N.D. #
6) T	MCP	5.923	0.000	917513	0	<MDL	N.D. #
7) T	MCPA	5.987	0.000	4958637	0	<MDL	N.D. #
10) T	Pentachlo...	6.866	0.000	6449360	0	<MDL	N.D. #
11) T	2,4,5-TP ...	7.401	0.000	1409188	0	<MDL	N.D. #
12) T	2,4,5-T	7.690	0.000	3596691	0	<MDL	N.D. #
13) T	2,4-DB	8.182	0.000	2197669	0	1.754	N.D. #
14) T	DINOSEB	9.305	0.000	9610295	0	1.378	N.D. #
15) T	Picloram	9.120	0.000	21083344	0	1.692	N.D. #
16) T	DCPA	9.577	0.000	19729564	0	1.812	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071919\
Data File : PS005603.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2019 04:27
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 05:18:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
Quant Title : 8080.M
QLast Update : Fri Jul 19 08:54:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

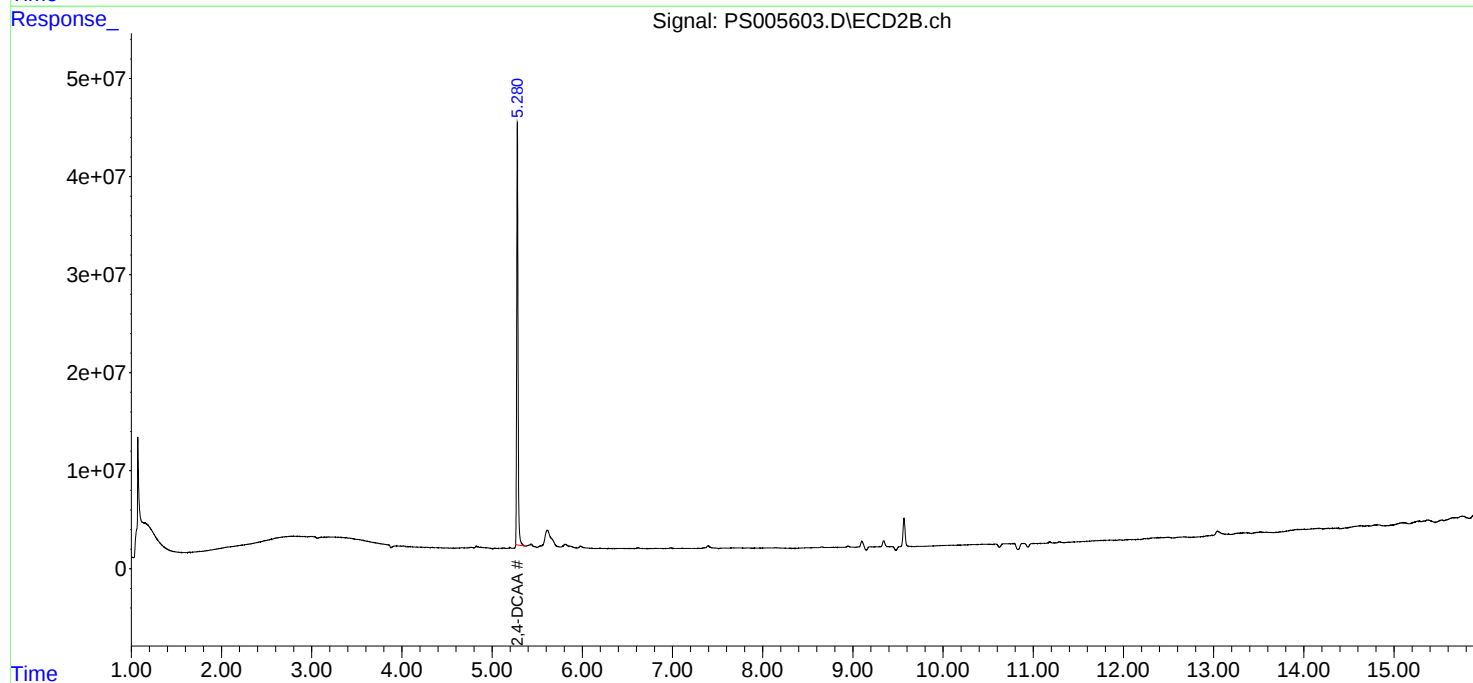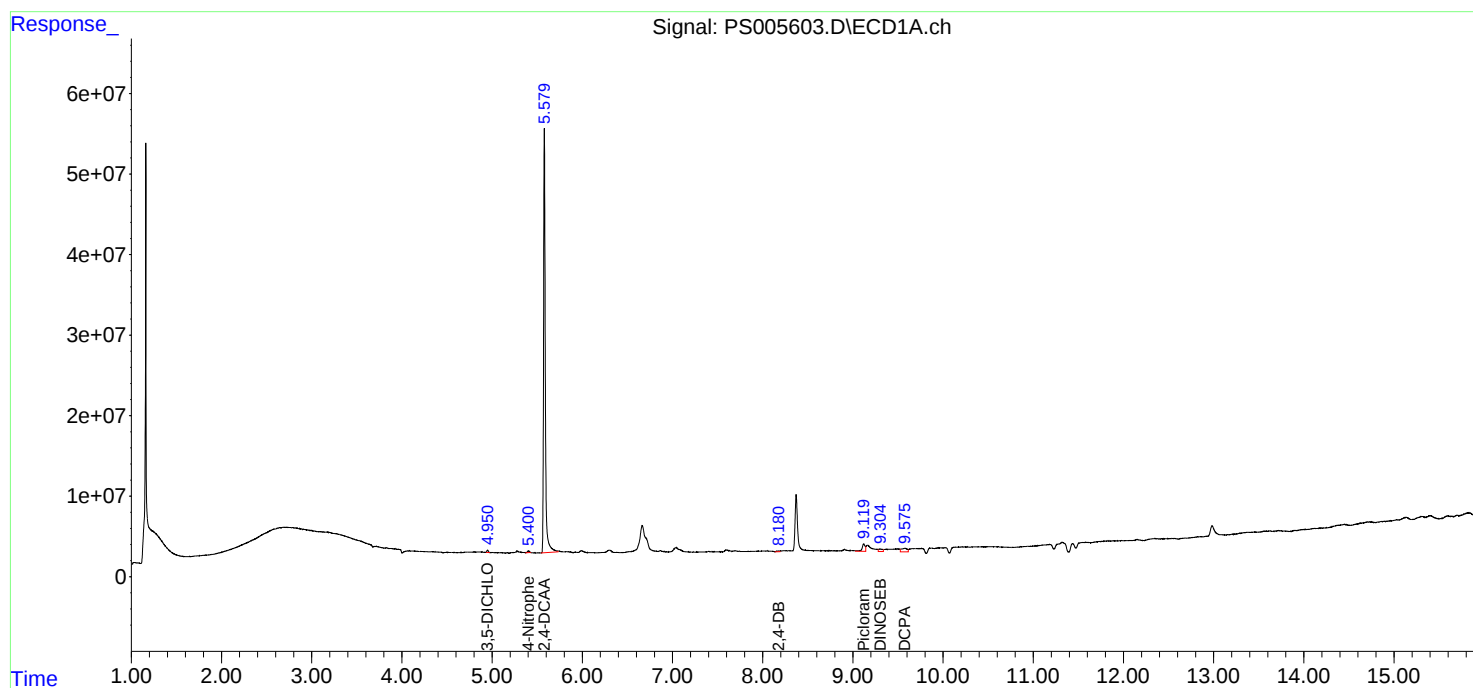


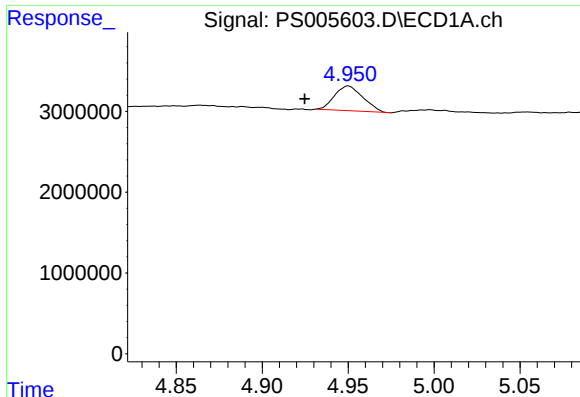

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.950 min
Delta R.T.: 0.025 min
Response: 3493660
Conc: 1.64 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

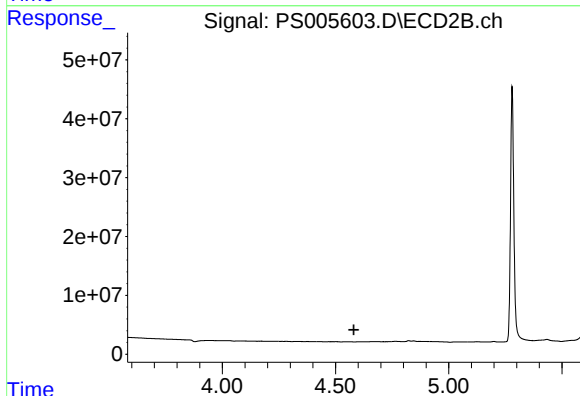


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.581 min
Response: 0
Conc: N.D.

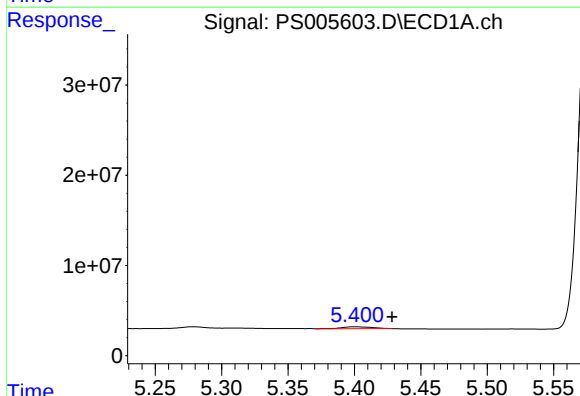


#3 4-Nitrophenol

R.T.: 5.401 min
Delta R.T.: -0.027 min
Response: 3453225
Conc: 4.83 ng/ml

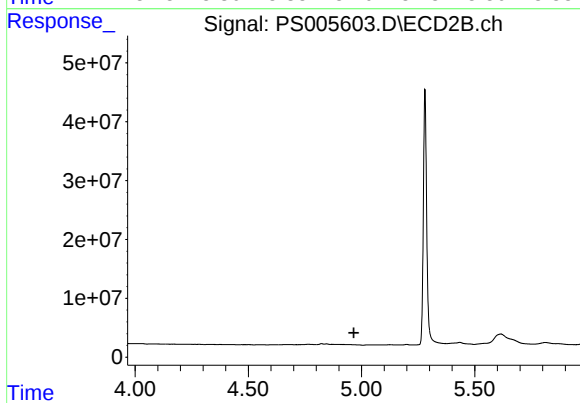

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 4.966 min
Response: 0
Conc: N.D.

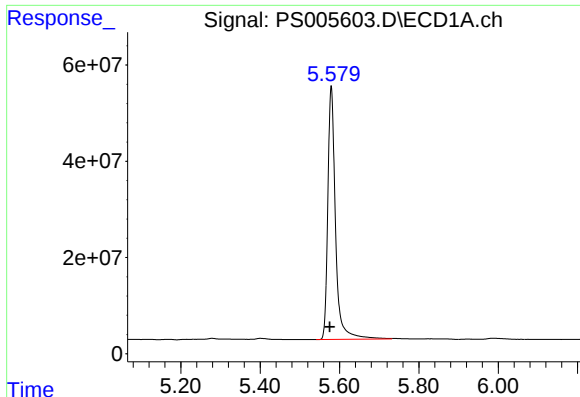

#4 2,4-DCAA


R.T.: 5.579 min
Delta R.T.: 0.003 min
Response: 708806597
Conc: 449.82 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

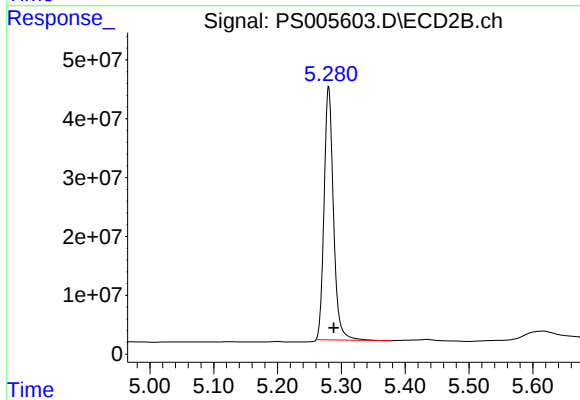


#4 2,4-DCAA

R.T.: 5.280 min
Delta R.T.: -0.008 min
Response: 438883147
Conc: 424.90 ng/ml

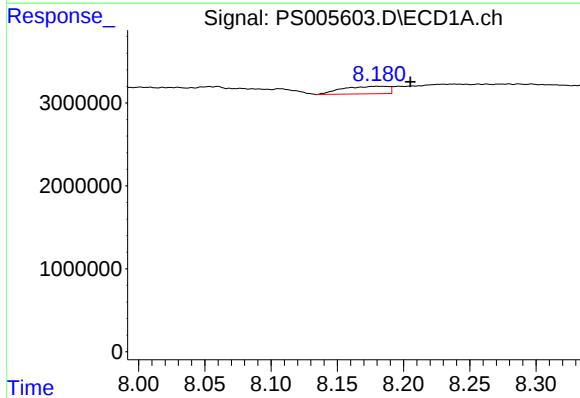


#13 2,4-DB

R.T.: 8.182 min
Delta R.T.: -0.023 min
Response: 2197669
Conc: 1.75 ng/ml

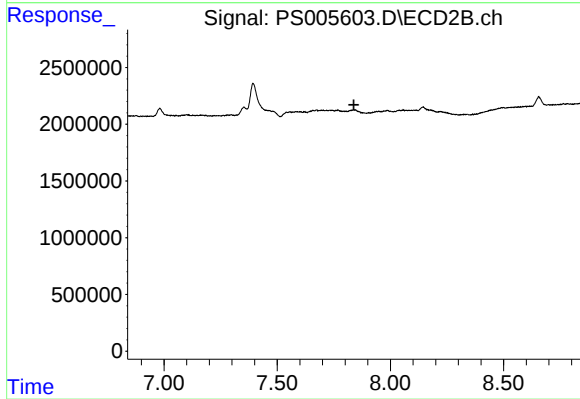

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 7.838 min
Response: 0
Conc: N.D.

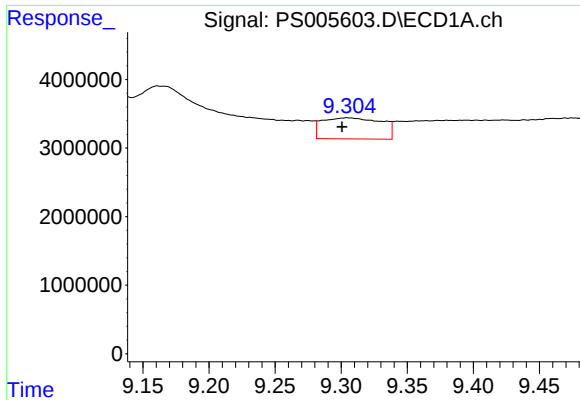

#14 DINOSEB


R.T.: 9.305 min
Delta R.T.: 0.004 min
Response: 9610295
Conc: 1.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

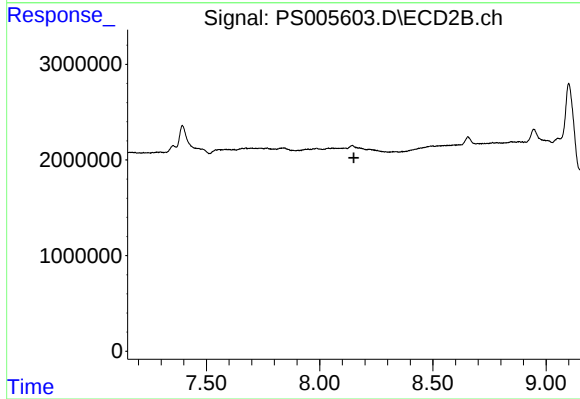


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 8.151 min
Response: 0
Conc: N.D.

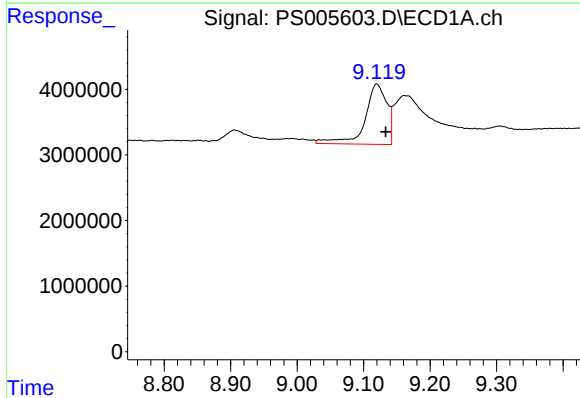


#15 Picloram

R.T.: 9.120 min
Delta R.T.: -0.013 min
Response: 21083344
Conc: 1.69 ng/ml

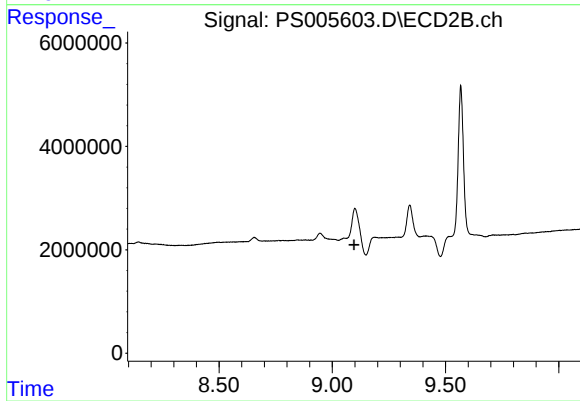

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 9.096 min
Response: 0
Conc: N.D.

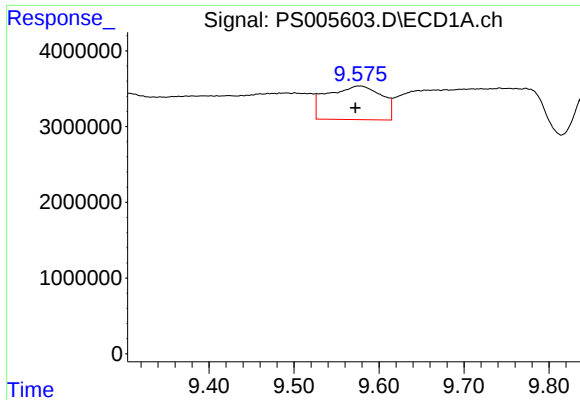

#16 DCPA

R.T.: 9.577 min
Delta R.T.: 0.005 min
Response: 19729564
Conc: 1.81 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

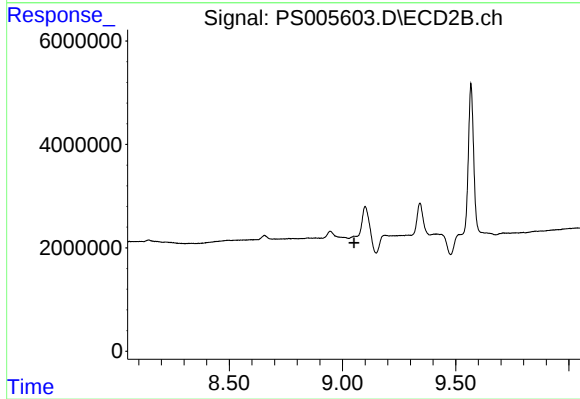

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.051 min
Response: 0
Conc: N.D.