

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071919\
 Data File : PS005602.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2019 04:05
 Operator : SM\AJ
 Sample : K3835-32
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SB-7(13-15)

Manual Integrations
 APPROVED

Ankita
 7/21/2019 12:00:21 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 05:18:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 19 08:54:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	5.598	5.315	331.4E6	169.4E6	210.330m	164.041m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071919\
Data File : PS005602.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2019 04:05
Operator : SM\AJ
Sample : K3835-32
Misc :
ALS Vial : 41 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
SB-7(13-15)


Manual Integrations
APPROVED

Ankita
7/21/2019 12:00:21 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 05:18:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
Quant Title : 8080.M
QLast Update : Fri Jul 19 08:54:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

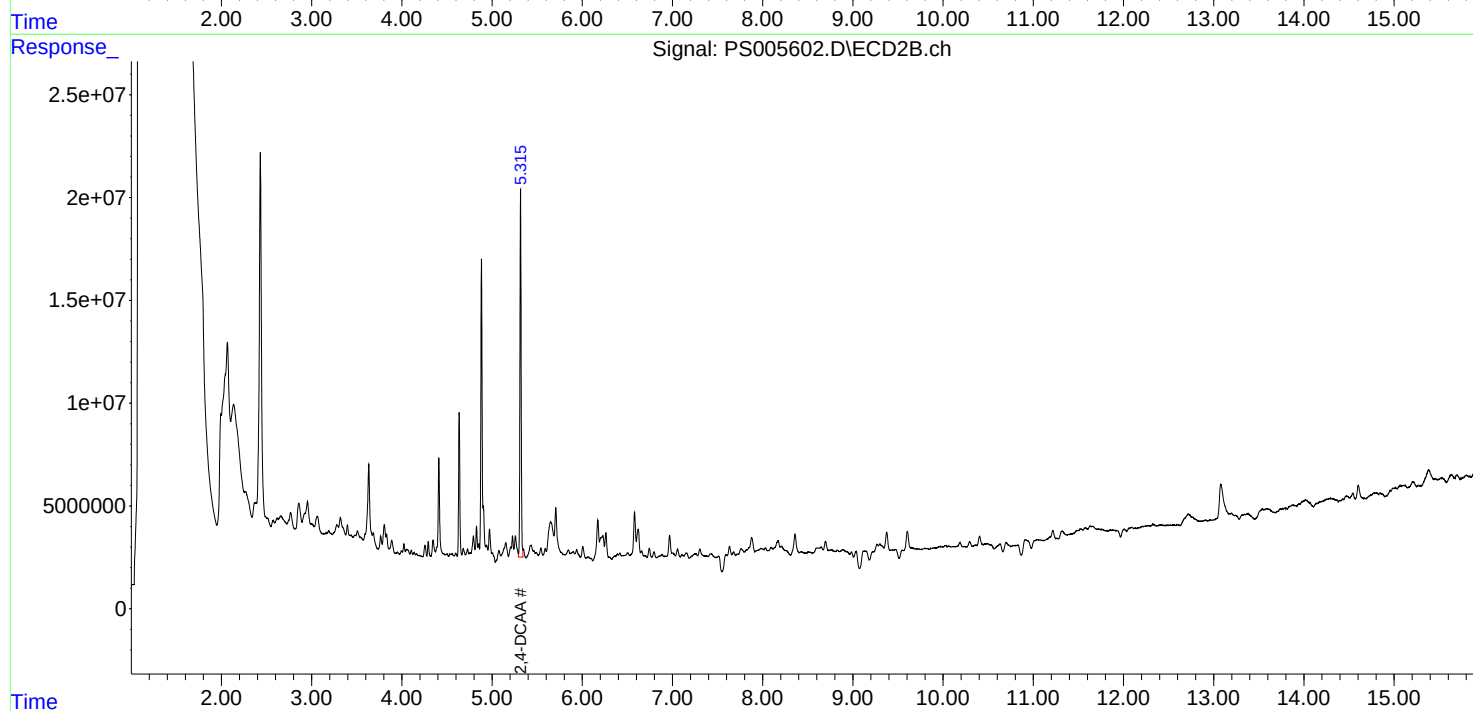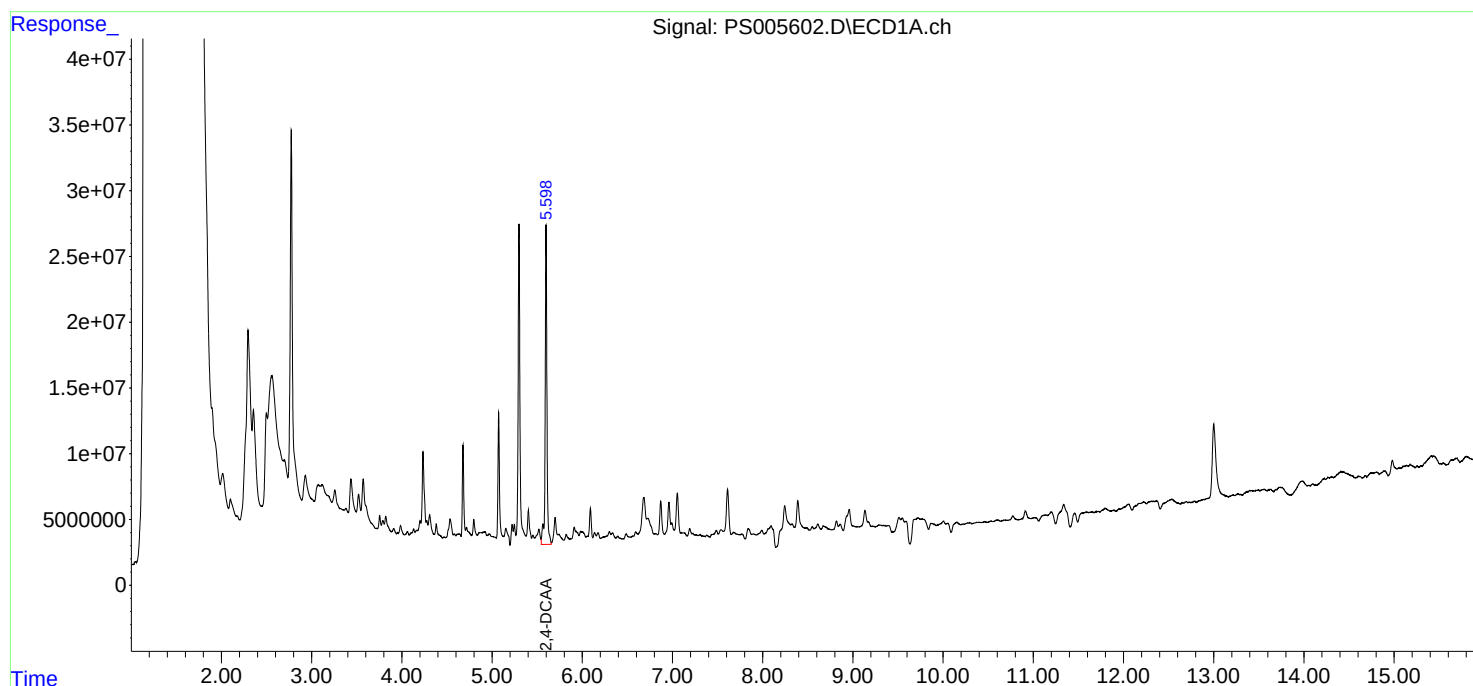

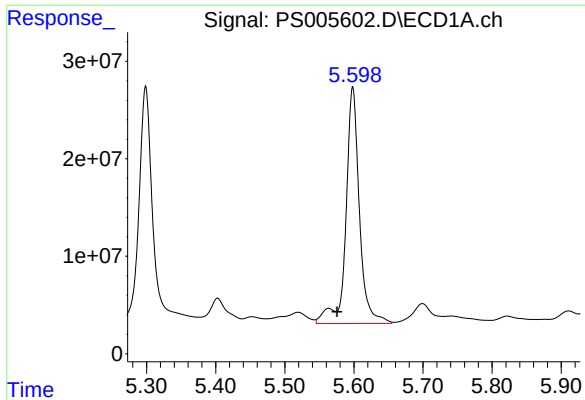


#4 2,4-DCAA

R.T.: 5.598 min
Delta R.T.: 0.022 min
Response: 331428476
Conc: 210.33 ng/ml m

Instrument :
ECD_S
ClientSampleId :
SB-7(13-15)

Manual Integrations
APPROVED

Ankita
7/21/2019 12:00:21 PM

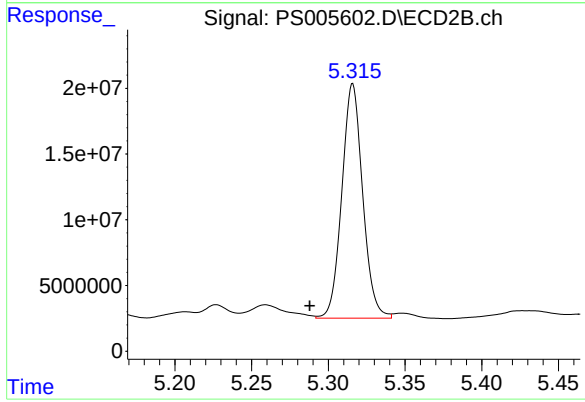

#4 2,4-DCAA

R.T.: 5.315 min
Delta R.T.: 0.027 min
Response: 169437907
Conc: 164.04 ng/ml m