

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072019\
 Data File : PS005617.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2019 14:30
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 00:49:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 19 08:54:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.593	5.309	798.3E6	508.4E6	506.638	492.222
Target Compounds							
2) T	3,5-DICHL...	4.964	0.000	7186493	0	3.378	N.D. #
3) T	4-Nitroph...	5.414	0.000	2164220	0	3.027	N.D. #
6) T	MCP	5.937	0.000	138088	0	<MDL	N.D. #
7) T	MCPA	6.001	5.642	3880755	71725428	<MDL	16.279 #
8) T	DICHLORPROP	6.313	0.000	9311628	0	6.126	N.D. #
9) T	2,4-D	6.532	0.000	1992851	0	1.136	N.D. #
10) T	Pentachlo...	6.879	0.000	8188926	0	<MDL	N.D. #
11) T	2,4,5-TP ...	7.416	0.000	2754989	0	<MDL	N.D. #
12) T	2,4,5-T	7.705	0.000	6722700	0	<MDL	N.D. #
13) T	2,4-DB	8.248	0.000	6199599	0	4.949	N.D. #
14) T	DINOSEB	9.318	0.000	23296639	0	3.340	N.D. #
15) T	Picloram	9.132	9.127	40206708	43650677	3.227	5.573 #
16) T	DCPA	9.590	0.000	13746540	0	1.262	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072019\
Data File : PS005617.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2019 14:30
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 00:49:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
Quant Title : 8080.M
QLast Update : Fri Jul 19 08:54:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

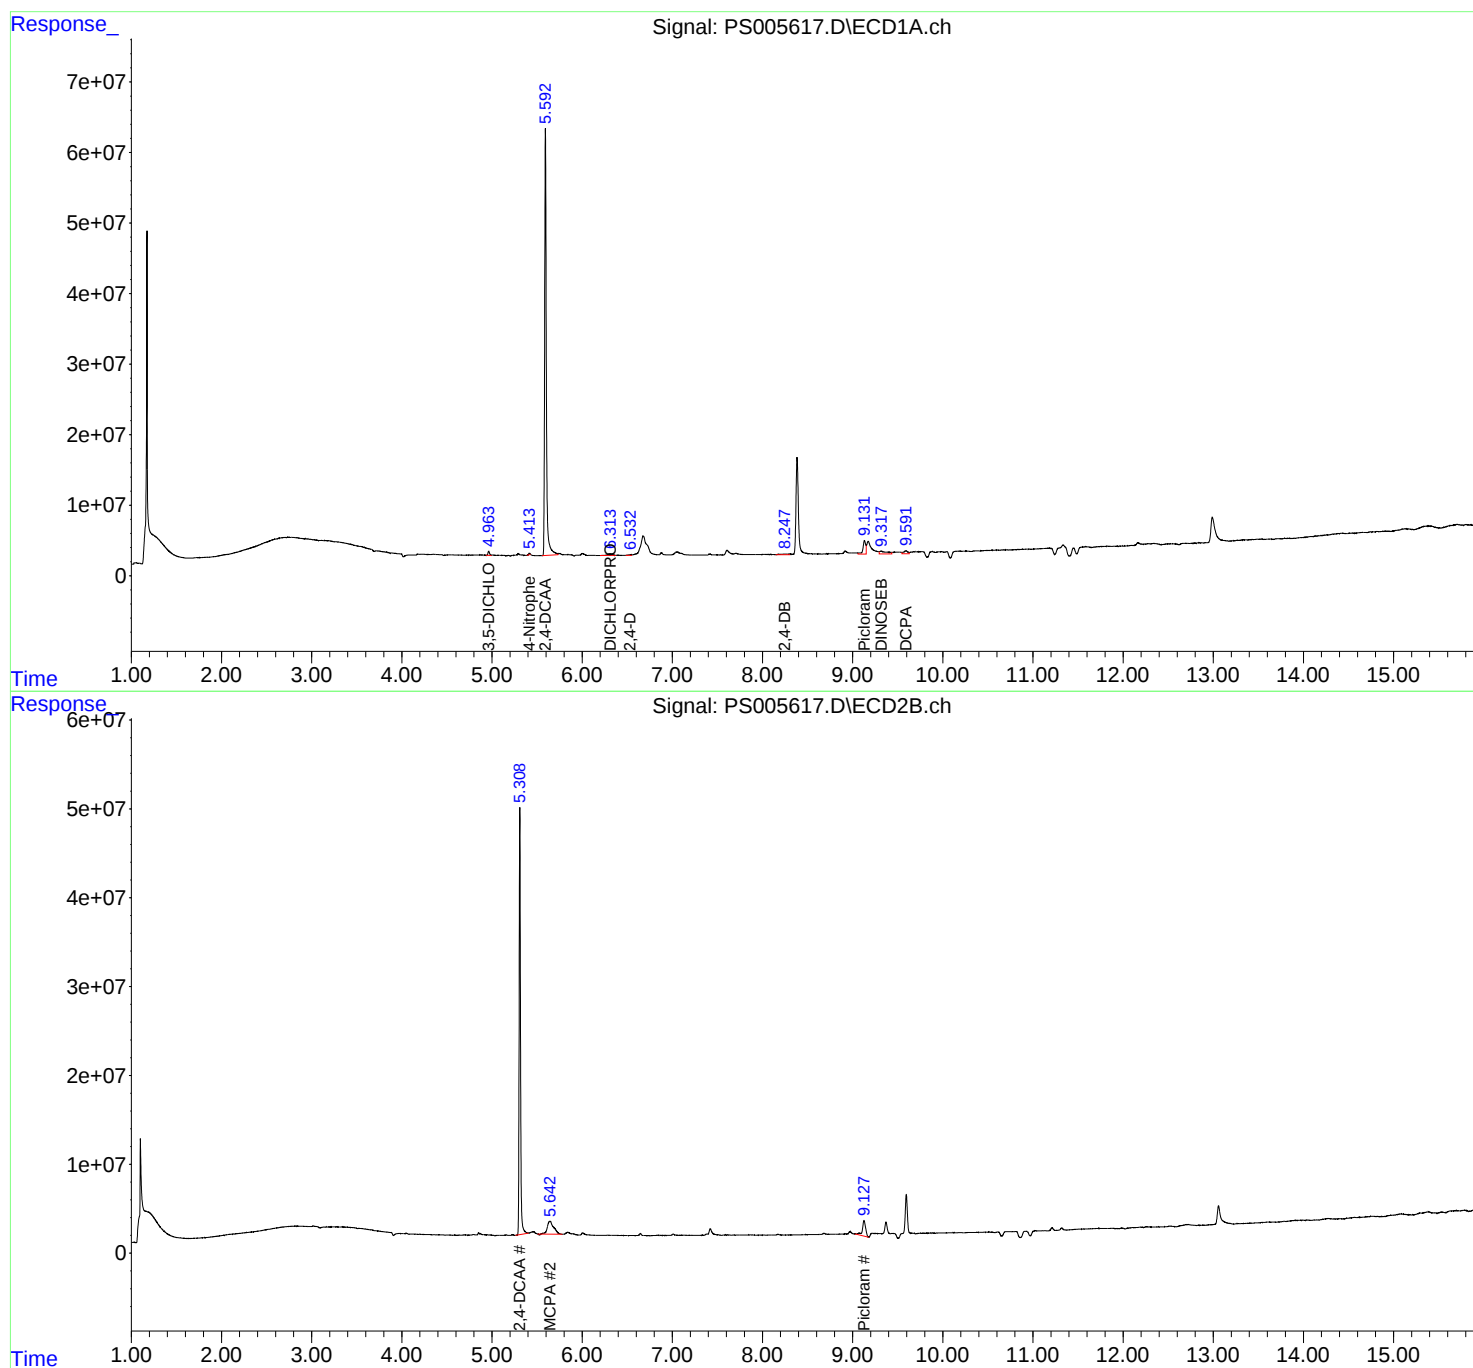


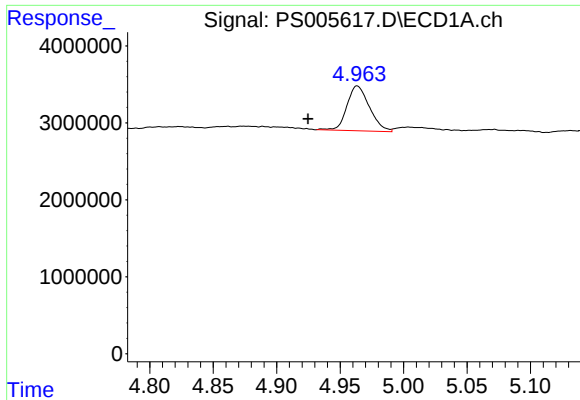

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.964 min
Delta R.T.: 0.039 min
Response: 7186493
Conc: 3.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

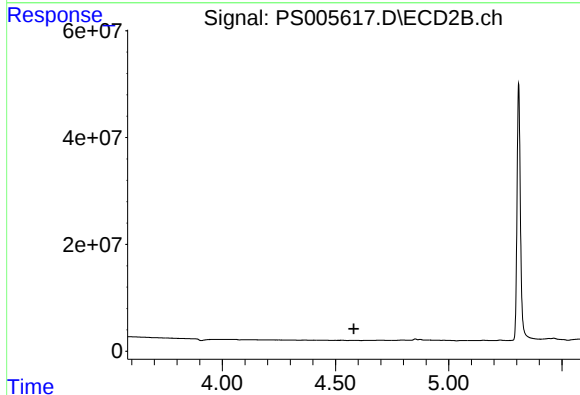


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.581 min
Response: 0
Conc: N.D.

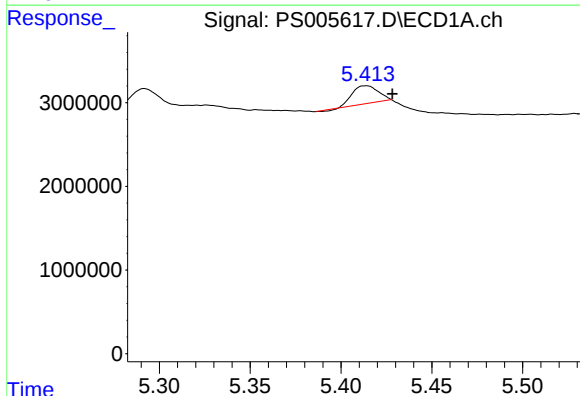


#3 4-Nitrophenol

R.T.: 5.414 min
Delta R.T.: -0.014 min
Response: 2164220
Conc: 3.03 ng/ml

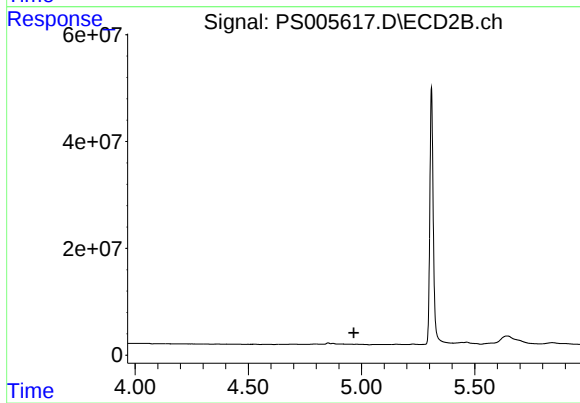

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 4.966 min
Response: 0
Conc: N.D.

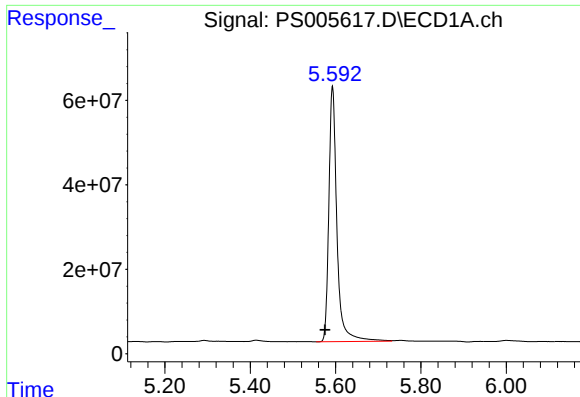

#4 2,4-DCAA


R.T.: 5.593 min
Delta R.T.: 0.017 min
Response: 798337256
Conc: 506.64 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

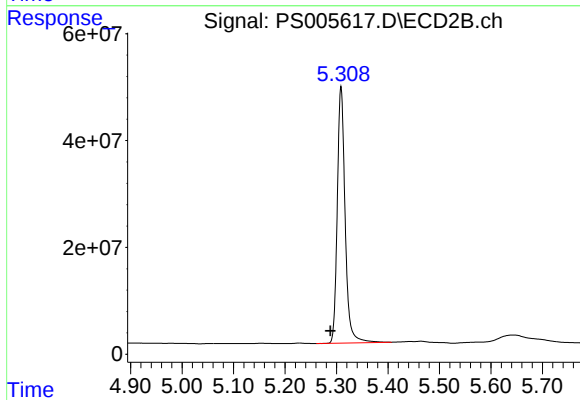


#4 2,4-DCAA

R.T.: 5.309 min
Delta R.T.: 0.021 min
Response: 508416330
Conc: 492.22 ng/ml

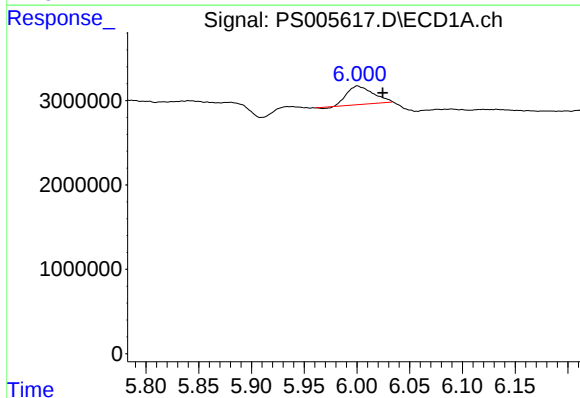


#7 MCPA

R.T.: 6.001 min
Delta R.T.: -0.023 min
Response: 3880755
Conc: N.D.

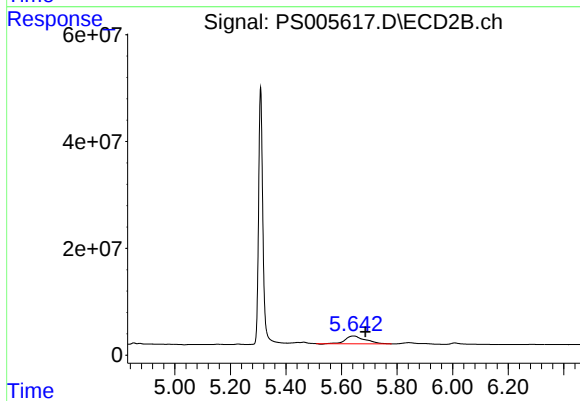

#7 MCPA


R.T.: 5.642 min
Delta R.T.: -0.045 min
Response: 71725428
Conc: 16.28 ug/ml

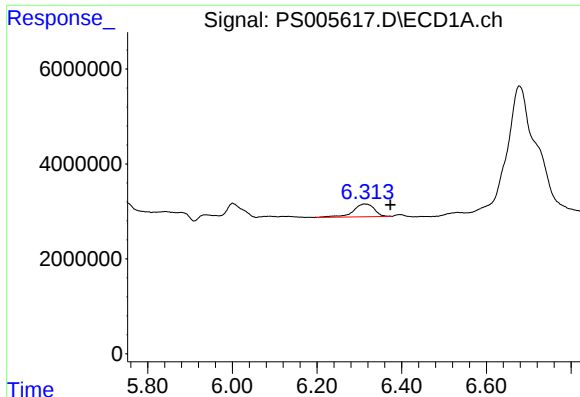

#8 DICHLORPROP


R.T.: 6.313 min
Delta R.T.: -0.061 min
Response: 9311628
Conc: 6.13 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

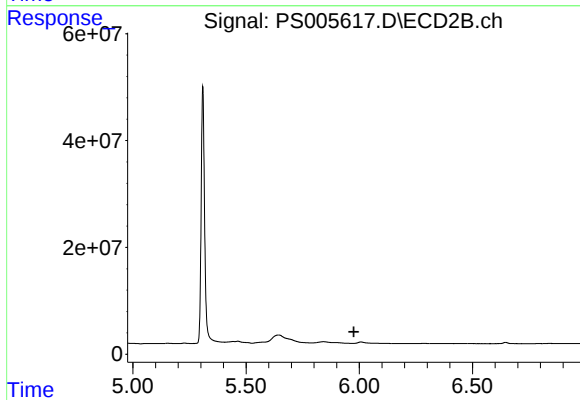


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 5.976 min
Response: 0
Conc: N.D.

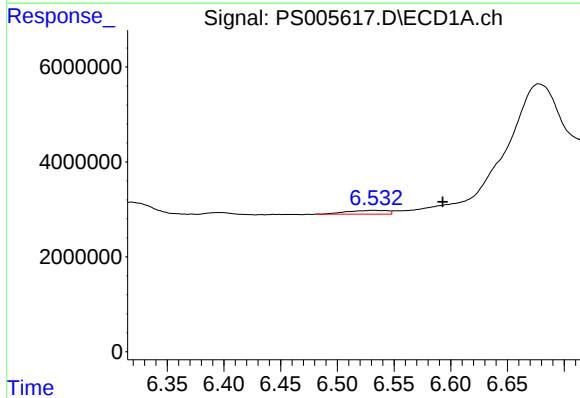


#9 2,4-D

R.T.: 6.532 min
Delta R.T.: -0.061 min
Response: 1992851
Conc: 1.14 ng/ml

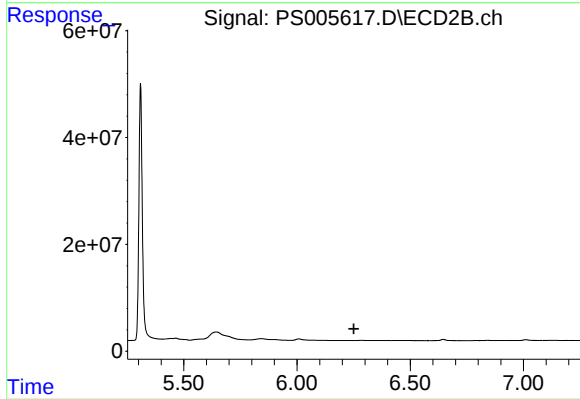

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 6.251 min
Response: 0
Conc: N.D.

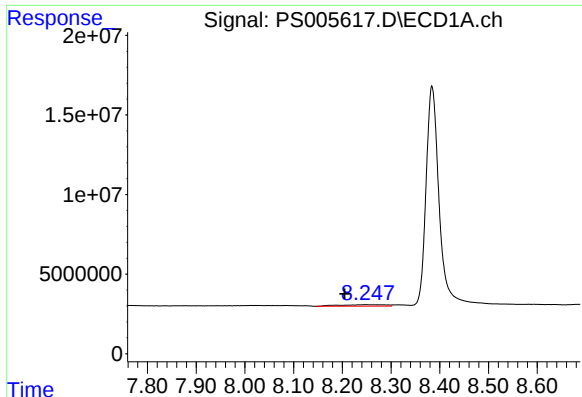

#13 2,4-DB


R.T.: 8.248 min
Delta R.T.: 0.043 min
Response: 6199599
Conc: 4.95 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

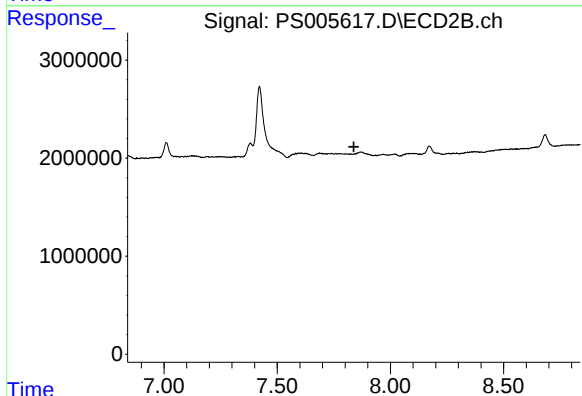


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.

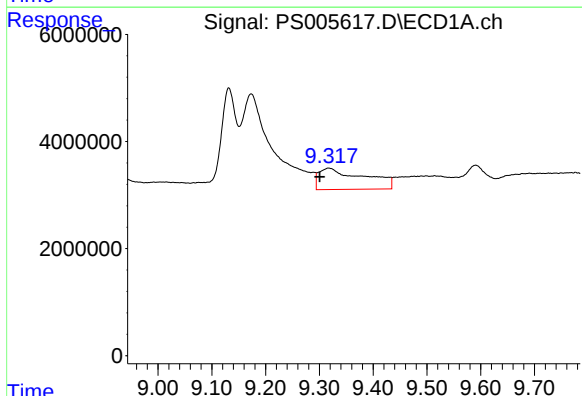


#14 DINOSEB

R.T.: 9.318 min
Delta R.T.: 0.017 min
Response: 23296639
Conc: 3.34 ng/ml

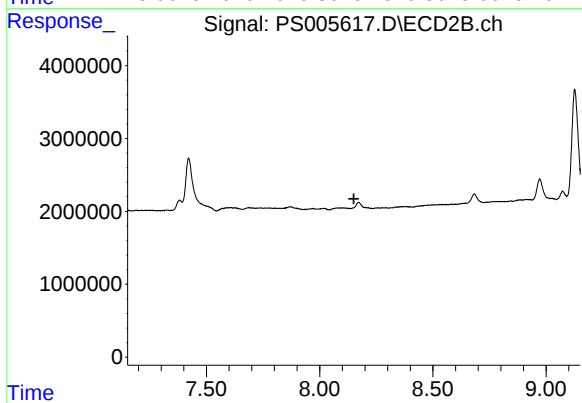

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 8.151 min
Response: 0
Conc: N.D.

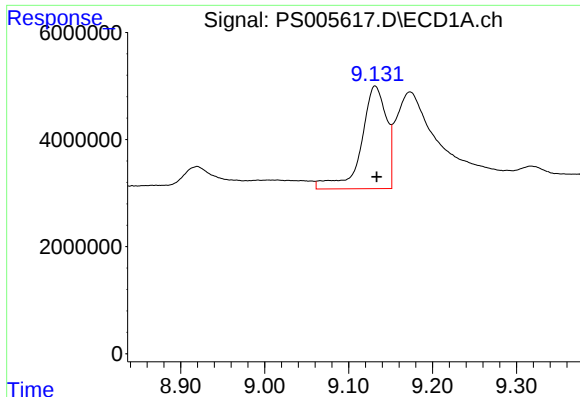

#15 Picloram


R.T.: 9.132 min
Delta R.T.: -0.002 min
Response: 40206708
Conc: 3.23 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

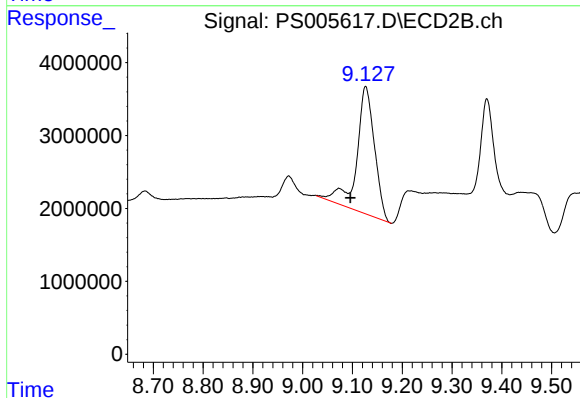


#15 Picloram

R.T.: 9.127 min
Delta R.T.: 0.031 min
Response: 43650677
Conc: 5.57 ng/ml

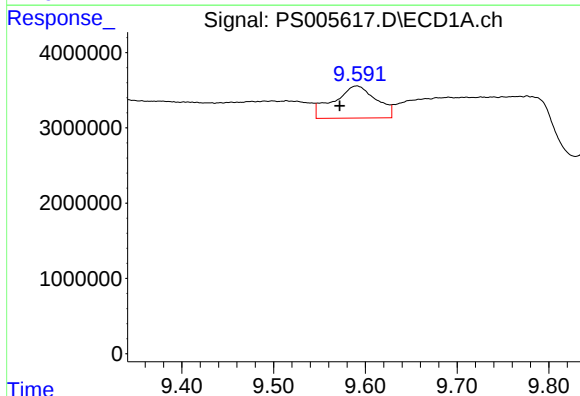

#16 DCPA

R.T.: 9.590 min
Delta R.T.: 0.018 min
Response: 13746540
Conc: 1.26 ng/ml

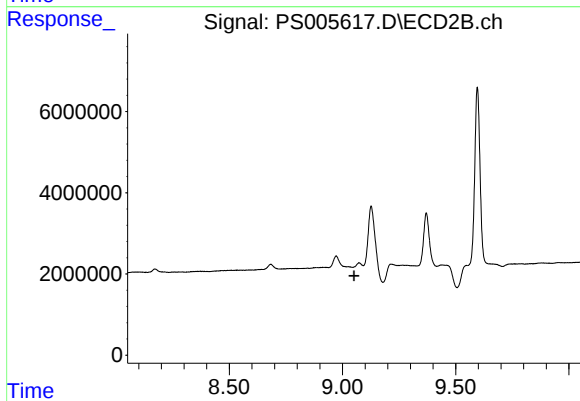

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.051 min
Response: 0
Conc: N.D.