

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072019\
 Data File : PS005627.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2019 18:11
 Operator : SM\AJ
 Sample : K3618-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HD-01-071719

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 00:53:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 19 08:54:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.566	5.283	389.2E6	271.4E6	246.984	262.758
Target Compounds							
2) T	3,5-DICHL...	4.888	4.601	4867641	218.4E6	2.288	161.104 #
3) T	4-Nitroph...	5.417	0.000	2339580	0	3.273	N.D. #
5) T	DICAMBA	5.756	5.388	7981737	19107691	1.290	4.829 #
6) T	MCP	5.872	0.000	7707662	0	1.587	N.D. #
8) T	DICHLORPROP	6.344	5.971	5773212	43006186	3.798	42.160 #
9) T	2,4-D	6.651	0.000	107.5E6	0	61.295	N.D. #
10) T	Pentachlo...	6.927	0.000	16598689	0	<MDL	N.D. #
11) T	2,4,5-TP ...	7.387	6.934	1540835	62661485	<MDL	11.243 #
12) T	2,4,5-T	7.668	0.000	5843978	0	<MDL	N.D. #
13) T	2,4-DB	8.209	0.000	6288849	0	5.020	N.D. #
14) T	DINOSEB	9.303	0.000	2347447	0	<MDL	N.D. #
15) T	Picloram	9.109	0.000	25889791	0	2.078	N.D. #
16) T	DCPA	9.535	0.000	13994578	0	1.285	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072019\
Data File : PS005627.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2019 18:11
Operator : SM\AJ
Sample : K3618-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HD-01-071719

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 00:53:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
Quant Title : 8080.M
QLast Update : Fri Jul 19 08:54:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

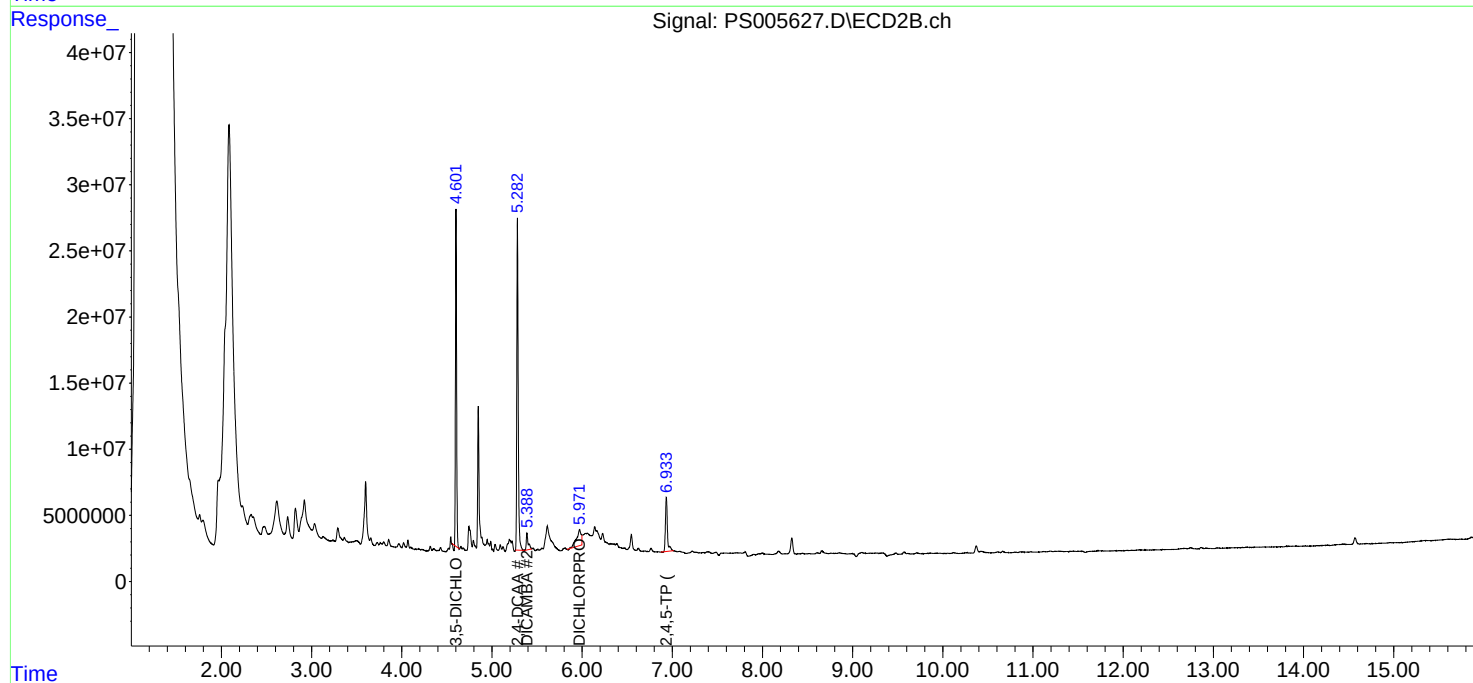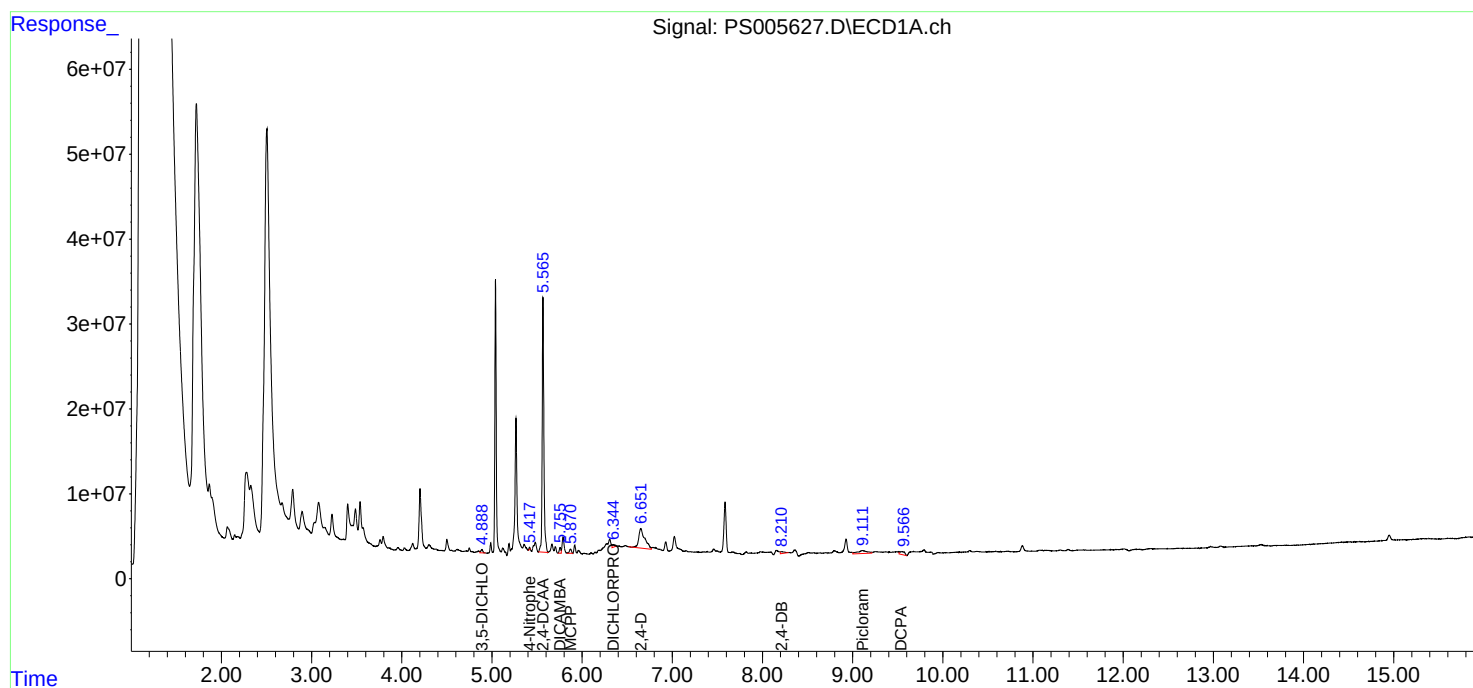


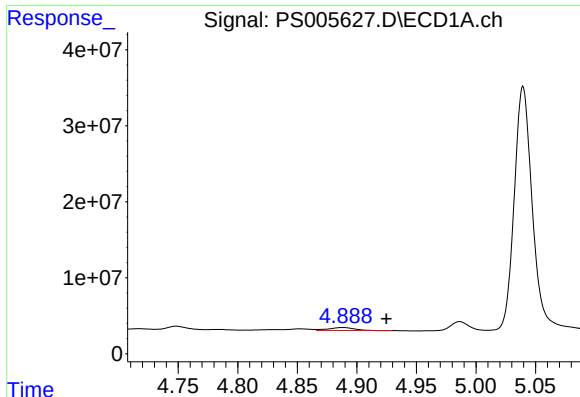

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.888 min
Delta R.T.: -0.037 min
Response: 4867641
Conc: 2.29 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-01-071719

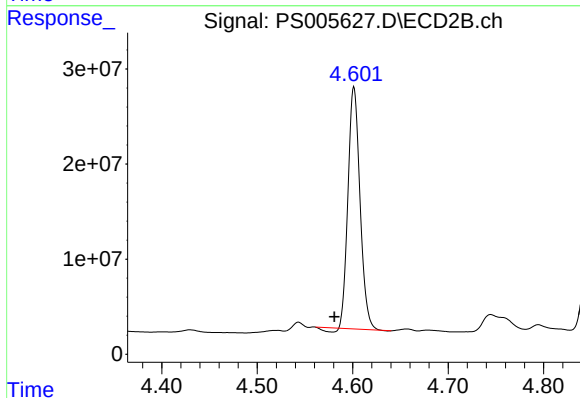


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.601 min
Delta R.T.: 0.020 min
Response: 218371199
Conc: 161.10 ng/ml

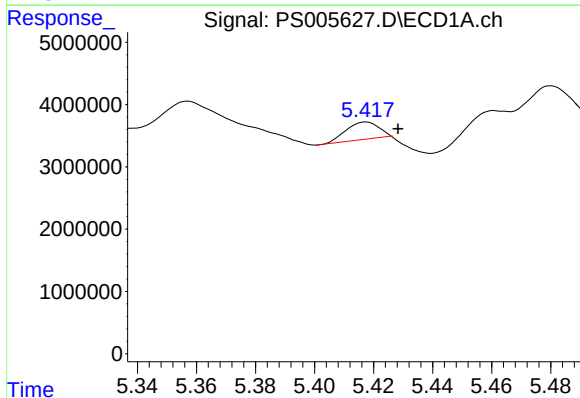


#3 4-Nitrophenol

R.T.: 5.417 min
Delta R.T.: -0.011 min
Response: 2339580
Conc: 3.27 ng/ml

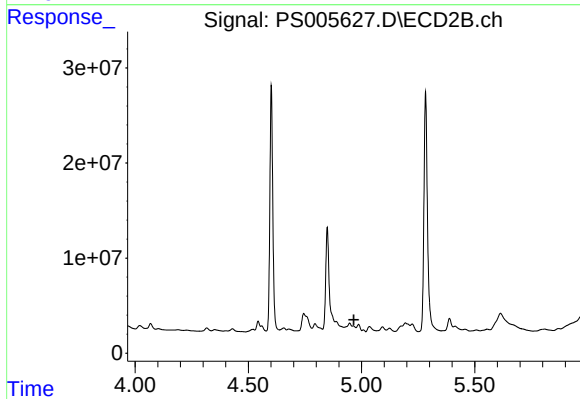

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 4.966 min
Response: 0
Conc: N.D.

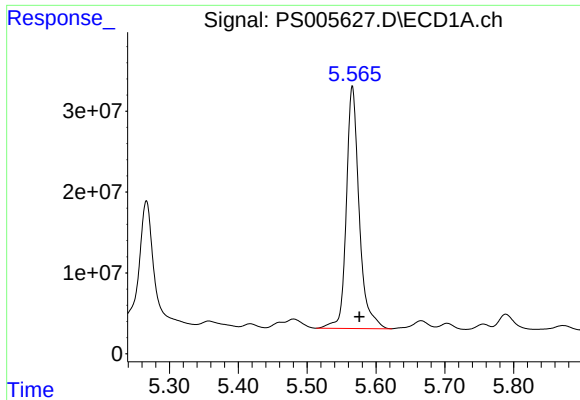

#4 2,4-DCAA


R.T.: 5.566 min
Delta R.T.: -0.010 min
Response: 389186429
Conc: 246.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-01-071719

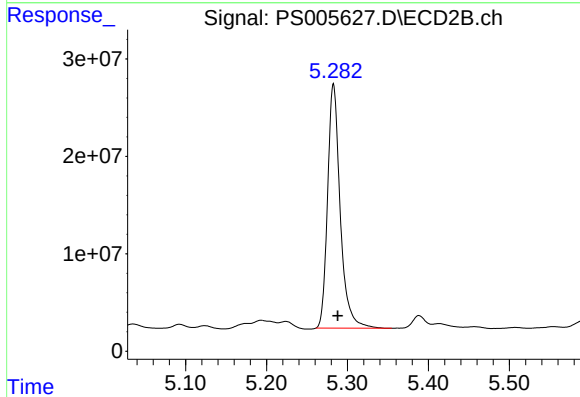


#4 2,4-DCAA

R.T.: 5.283 min
Delta R.T.: -0.005 min
Response: 271402934
Conc: 262.76 ng/ml

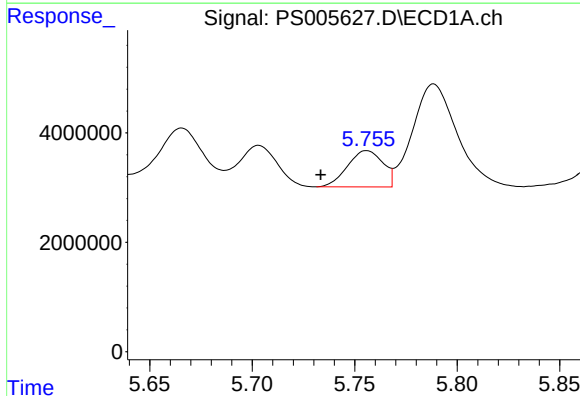


#5 DICAMBA

R.T.: 5.756 min
Delta R.T.: 0.023 min
Response: 7981737
Conc: 1.29 ng/ml

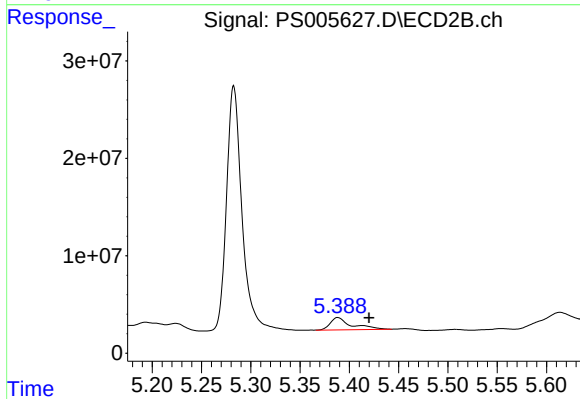

#5 DICAMBA


R.T.: 5.388 min
Delta R.T.: -0.032 min
Response: 19107691
Conc: 4.83 ng/ml

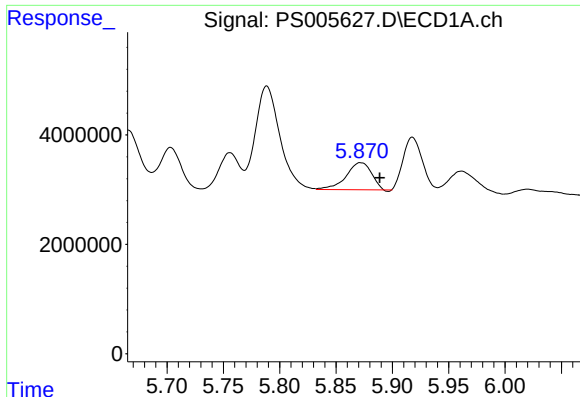

#6 MCP


R.T.: 5.872 min
Delta R.T.: -0.017 min
Response: 7707662
Conc: 1.59 ug/ml

Instrument :
ECD_S
ClientSampleId :
HD-01-071719

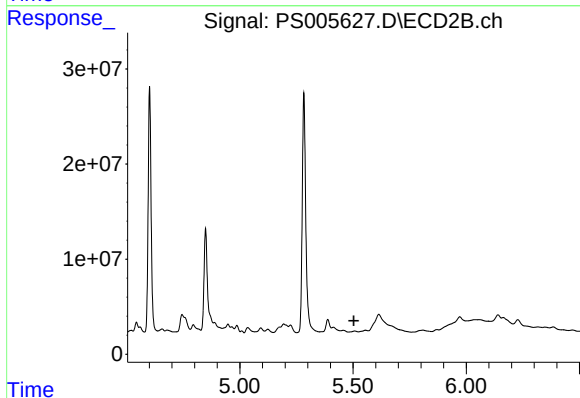


#6 MCP

R.T.: 0.000 min
Exp R.T.: 5.504 min
Response: 0
Conc: N.D.

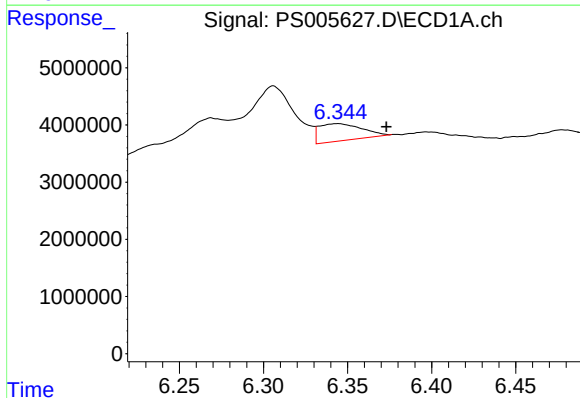


#8 DICHLORPROP

R.T.: 6.344 min
Delta R.T.: -0.030 min
Response: 5773212
Conc: 3.80 ng/ml

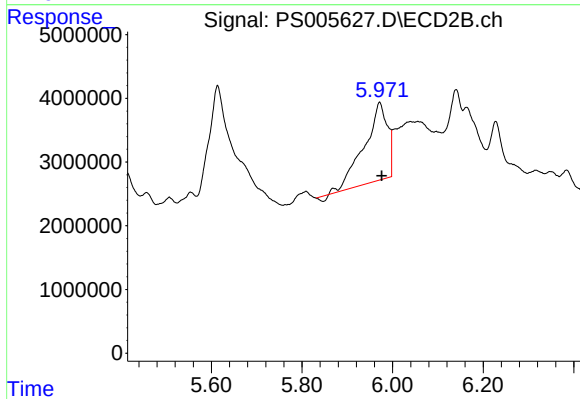

#8 DICHLORPROP


R.T.: 5.971 min
Delta R.T.: -0.005 min
Response: 43006186
Conc: 42.16 ng/ml

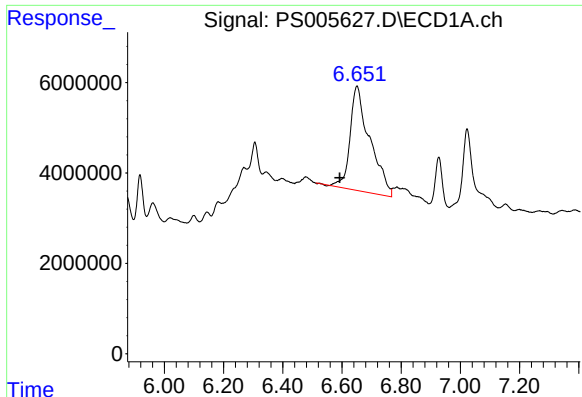

#9 2,4-D


R.T.: 6.651 min
Delta R.T.: 0.058 min
Response: 107491364
Conc: 61.29 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-01-071719

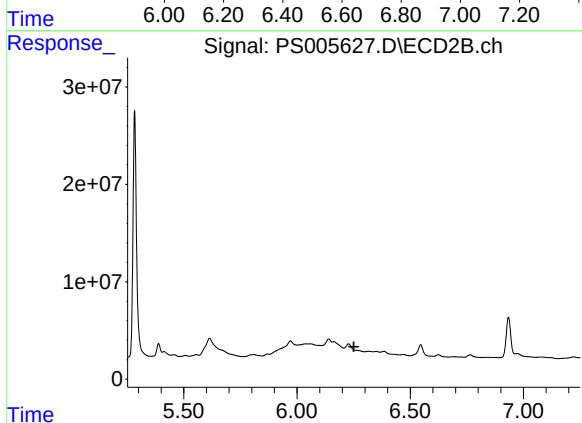


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.251 min
Response: 0
Conc: N.D.

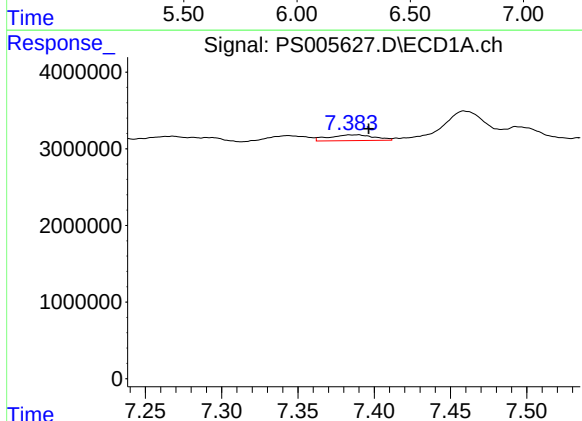


#11 2,4,5-TP (SILVEX)

R.T.: 7.387 min
Delta R.T.: -0.010 min
Response: 1540835
Conc: N.D.

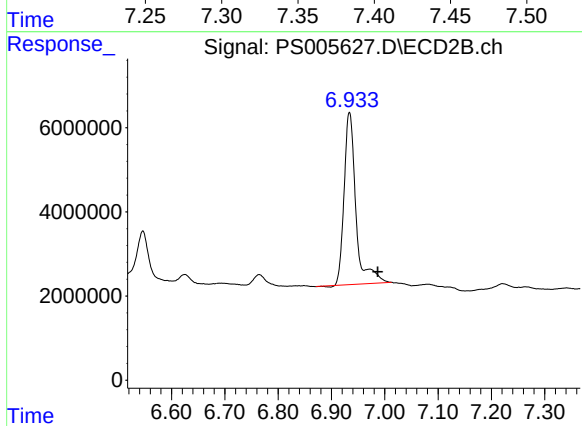

#11 2,4,5-TP (SILVEX)


R.T.: 6.934 min
Delta R.T.: -0.053 min
Response: 62661485
Conc: 11.24 ng/ml

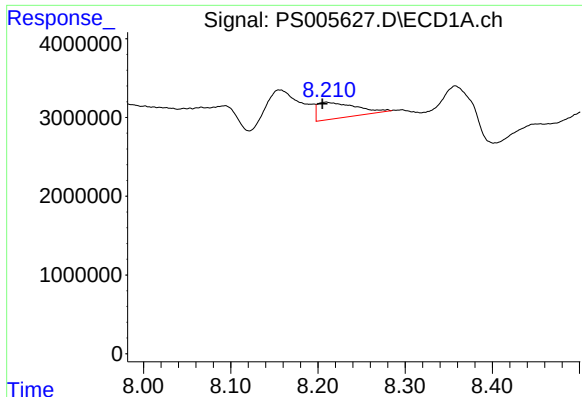

#13 2,4-DB


R.T.: 8.209 min
Delta R.T.: 0.004 min
Response: 6288849
Conc: 5.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-01-071719

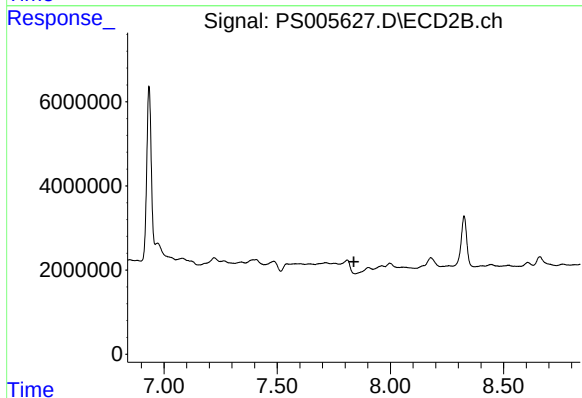


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.

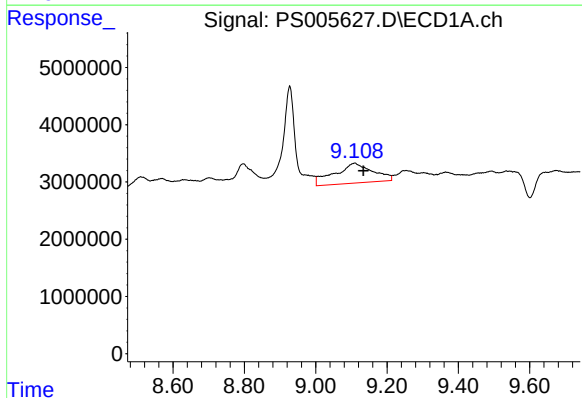


#15 Picloram

R.T.: 9.109 min
Delta R.T.: -0.024 min
Response: 25889791
Conc: 2.08 ng/ml

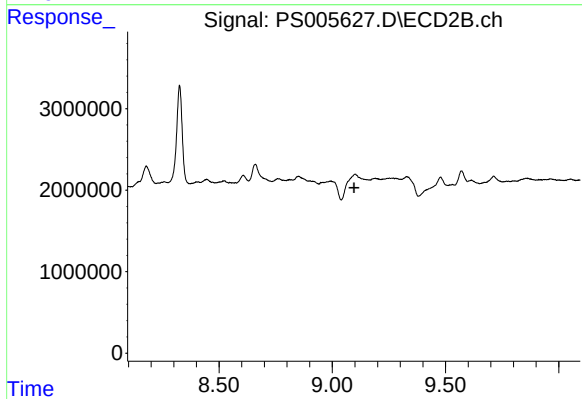

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 9.096 min
Response: 0
Conc: N.D.

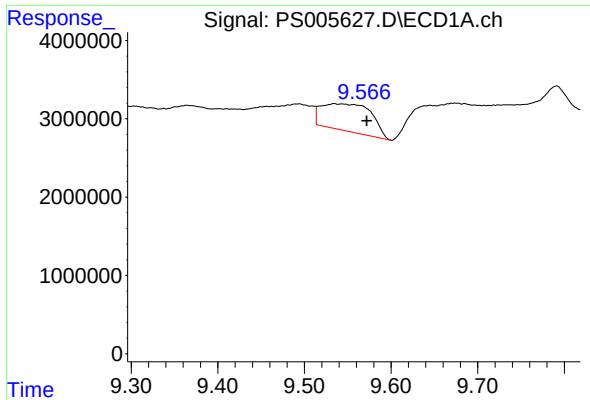

#16 DCPA

R.T.: 9.535 min
Delta R.T.: -0.037 min
Response: 13994578
Conc: 1.29 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-01-071719

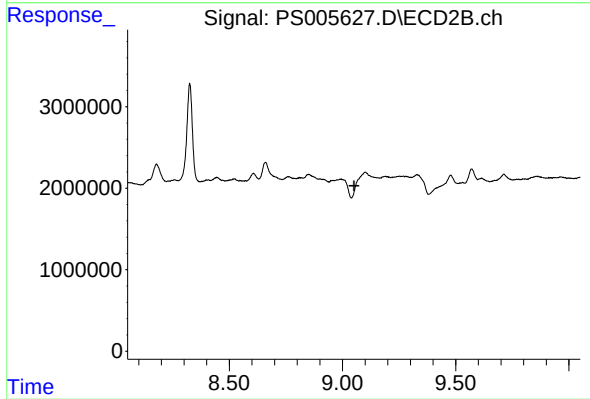

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.051 min
Response: 0
Conc: N.D.