

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072019\
 Data File : PS005628.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2019 18:33
 Operator : SM\AJ
 Sample : K3868-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 00:54:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 19 08:54:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.571	5.286	306.4E6	217.1E6	194.420	210.190
Target Compounds							
2) T	3,5-DICHL...	4.893	4.604	5682586	205.2E6	2.671	151.350 #
3) T	4-Nitroph...	5.484	4.989	24284237	14303069	33.970	28.864
5) T	DICAMBA	5.708	5.391	3135998	8170600	<MDL	2.065 #
6) T	MCP	5.876	0.000	7421602	0	1.528	N.D. #
8) T	DICHLORPROP	6.347	5.974	4157845	10214726	2.735	10.014 #
9) T	2,4-D	6.594	0.000	9112529	0	5.196	N.D. #
11) T	2,4,5-TP ...	7.388	6.936	1015444	53663173	<MDL	9.628 #
12) T	2,4,5-T	7.674	0.000	5120752	0	<MDL	N.D. #
13) T	2,4-DB	8.216	0.000	19366763	0	15.460	N.D. #
14) T	DINOSEB	9.317	0.000	33177858	0	4.756	N.D. #
15) T	Picloram	9.114	0.000	34515052	0	2.770	N.D. #
16) T	DCPA	9.570	0.000	13944206	0	1.281	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072019\
Data File : PS005628.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2019 18:33
Operator : SM\AJ
Sample : K3868-06
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
TP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 00:54:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
Quant Title : 8080.M
QLast Update : Fri Jul 19 08:54:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

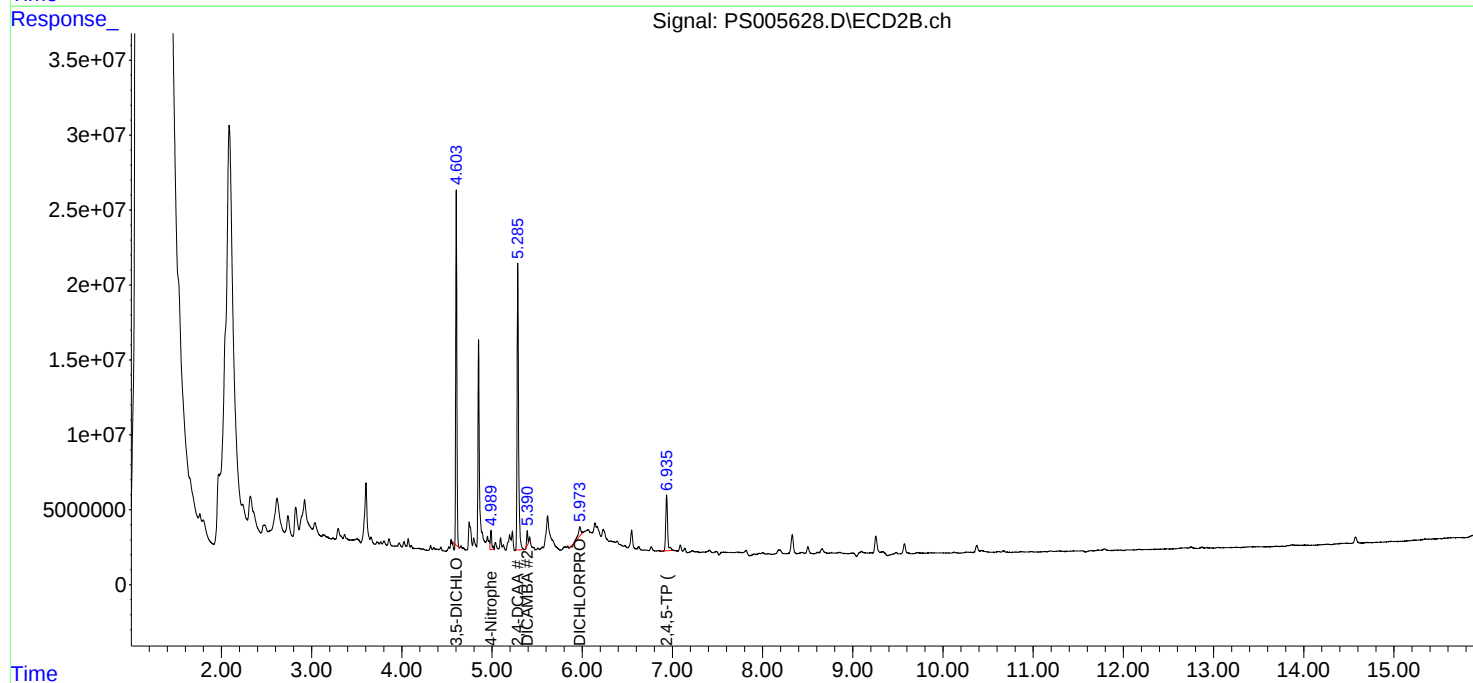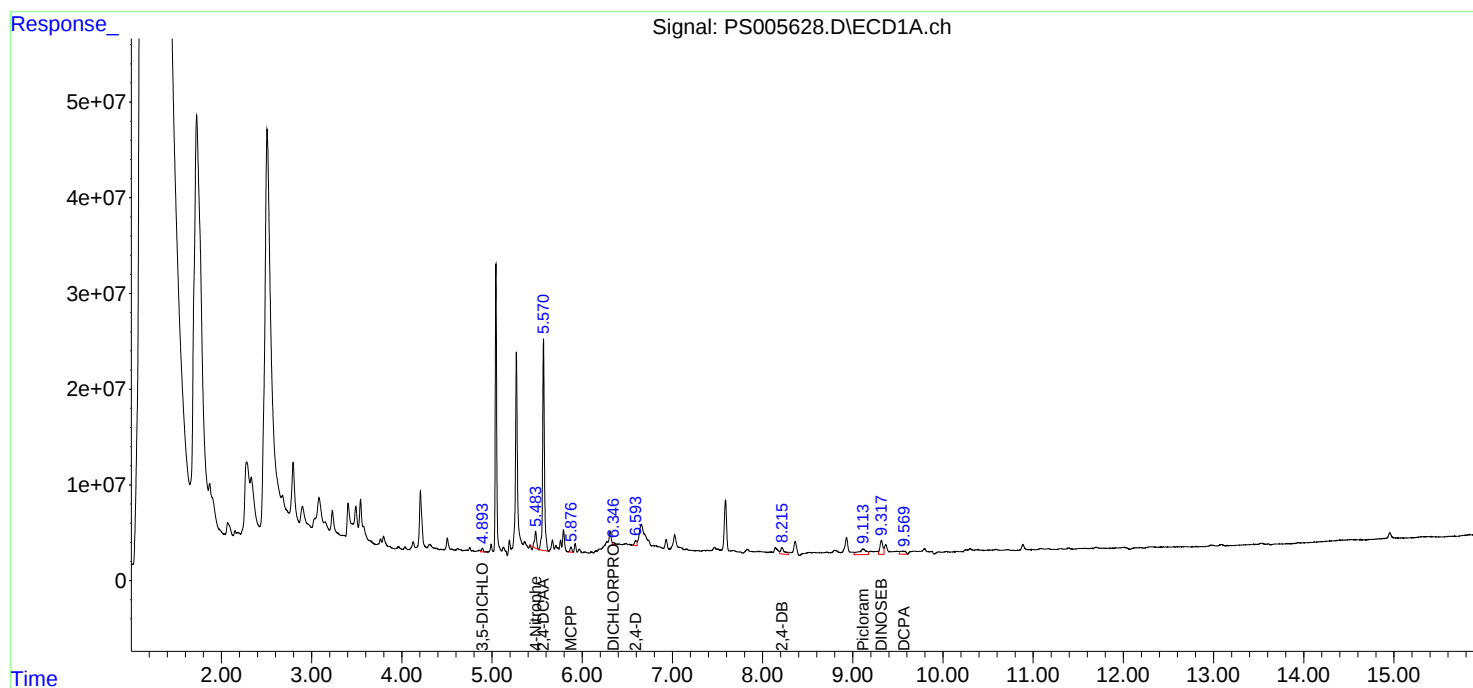


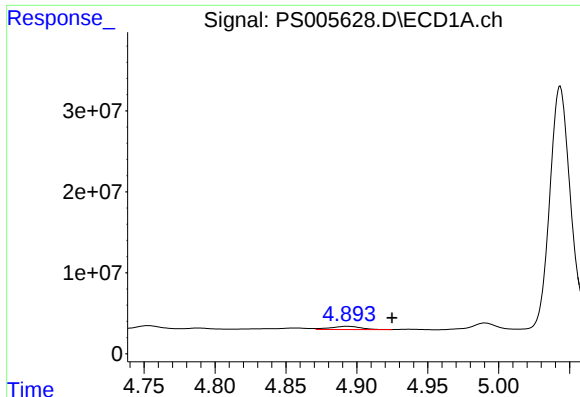

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.893 min
Delta R.T.: -0.031 min
Response: 5682586
Conc: 2.67 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-1

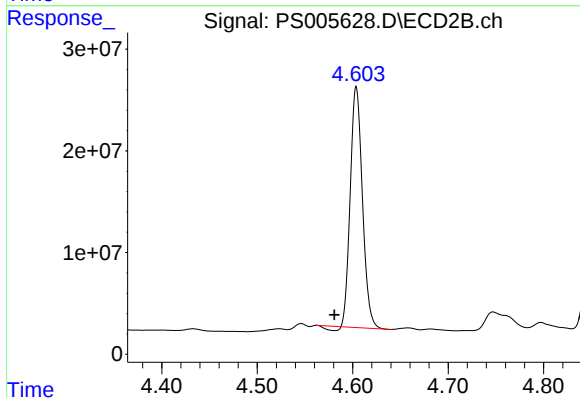


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.604 min
Delta R.T.: 0.023 min
Response: 205150071
Conc: 151.35 ng/ml

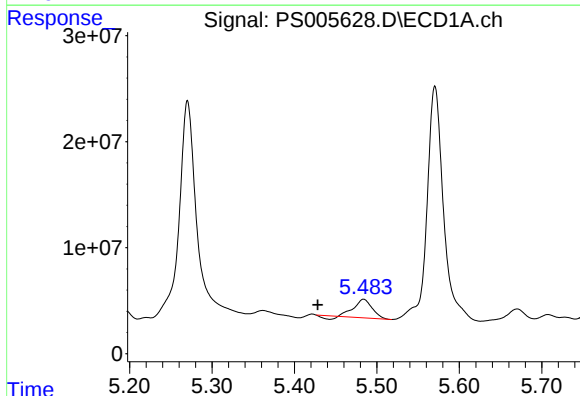


#3 4-Nitrophenol

R.T.: 5.484 min
Delta R.T.: 0.056 min
Response: 24284237
Conc: 33.97 ng/ml

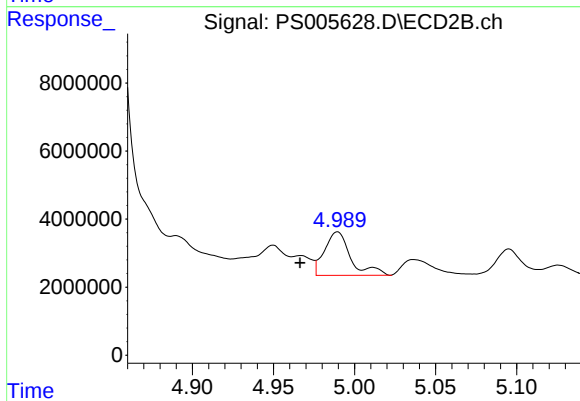

#3 4-Nitrophenol


R.T.: 4.989 min
Delta R.T.: 0.023 min
Response: 14303069
Conc: 28.86 ng/ml

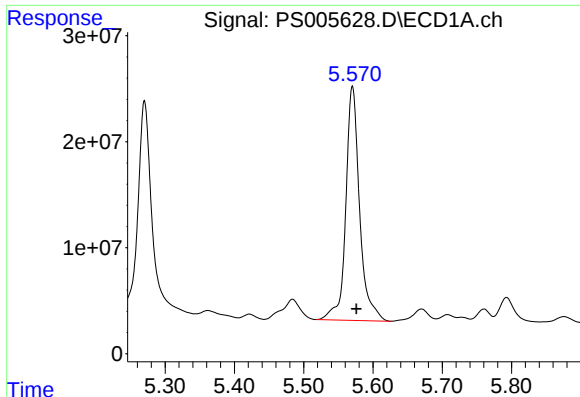

#4 2,4-DCAA


R.T.: 5.571 min
Delta R.T.: -0.005 min
Response: 306358562
Conc: 194.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-1

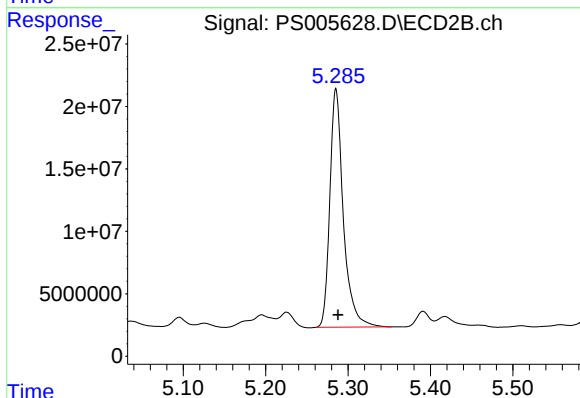


#4 2,4-DCAA

R.T.: 5.286 min
Delta R.T.: -0.002 min
Response: 217105130
Conc: 210.19 ng/ml

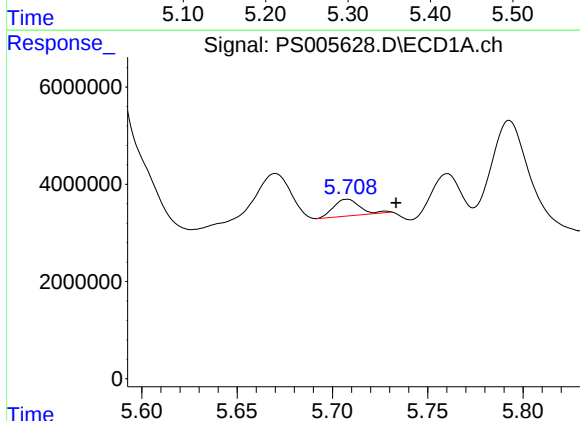


#5 DICAMBA

R.T.: 5.708 min
Delta R.T.: -0.026 min
Response: 3135998
Conc: N.D.

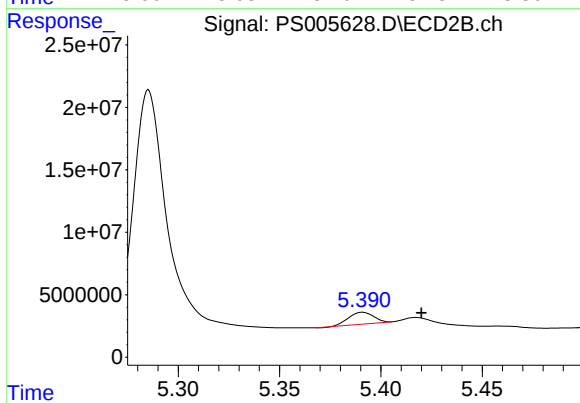

#5 DICAMBA


R.T.: 5.391 min
Delta R.T.: -0.029 min
Response: 8170600
Conc: 2.06 ng/ml

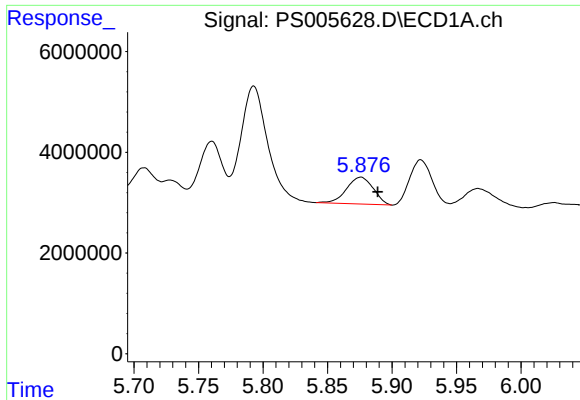

#6 MCP


R.T.: 5.876 min
Delta R.T.: -0.013 min
Response: 7421602
Conc: 1.53 ug/ml

Instrument :
ECD_S
ClientSampleId :
TP-1

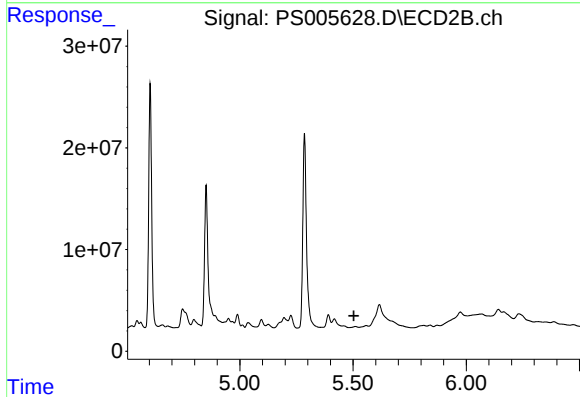


#6 MCP

R.T.: 0.000 min
Exp R.T.: 5.504 min
Response: 0
Conc: N.D.

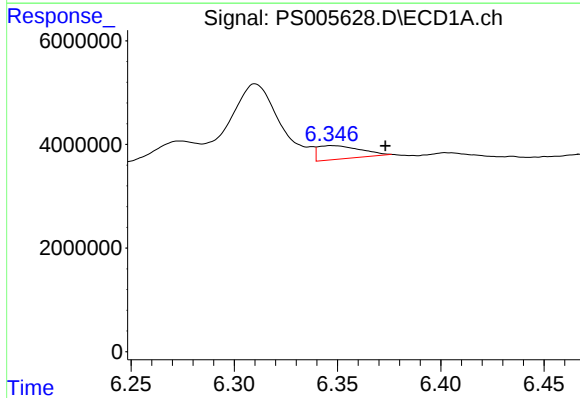


#8 DICHLORPROP

R.T.: 6.347 min
Delta R.T.: -0.026 min
Response: 4157845
Conc: 2.74 ng/ml

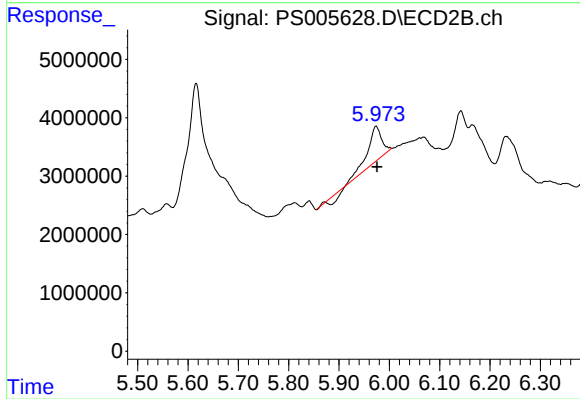

#8 DICHLORPROP


R.T.: 5.974 min
Delta R.T.: -0.002 min
Response: 10214726
Conc: 10.01 ng/ml

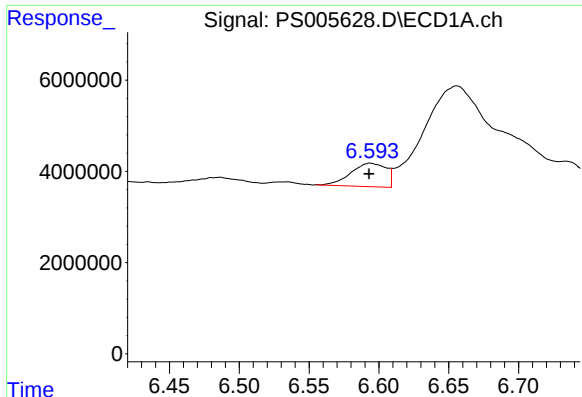

#9 2,4-D


R.T.: 6.594 min
Delta R.T.: 0.001 min
Response: 9112529
Conc: 5.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-1

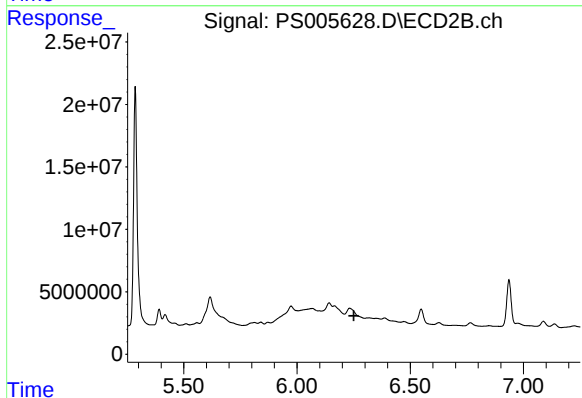


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.251 min
Response: 0
Conc: N.D.

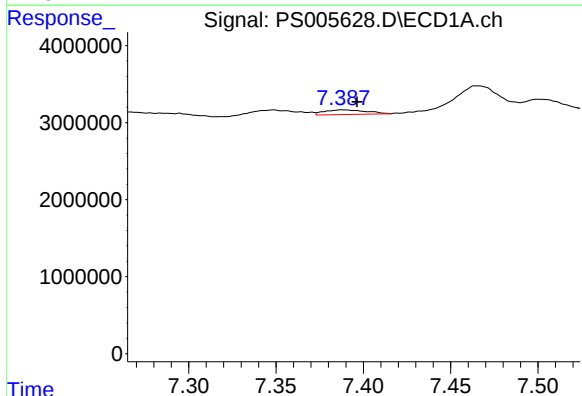


#11 2,4,5-TP (SILVEX)

R.T.: 7.388 min
Delta R.T.: -0.008 min
Response: 1015444
Conc: N.D.

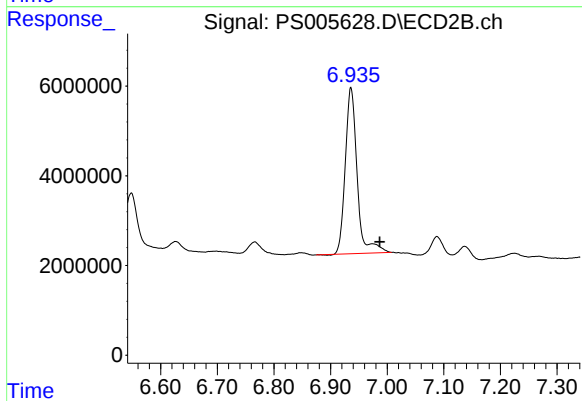

#11 2,4,5-TP (SILVEX)


R.T.: 6.936 min
Delta R.T.: -0.051 min
Response: 53663173
Conc: 9.63 ng/ml

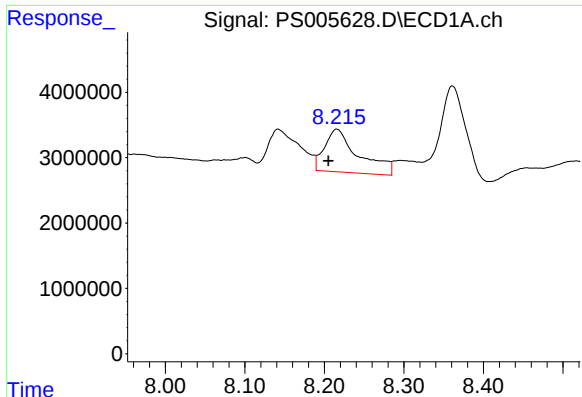

#13 2,4-DB


R.T.: 8.216 min
Delta R.T.: 0.011 min
Response: 19366763
Conc: 15.46 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-1

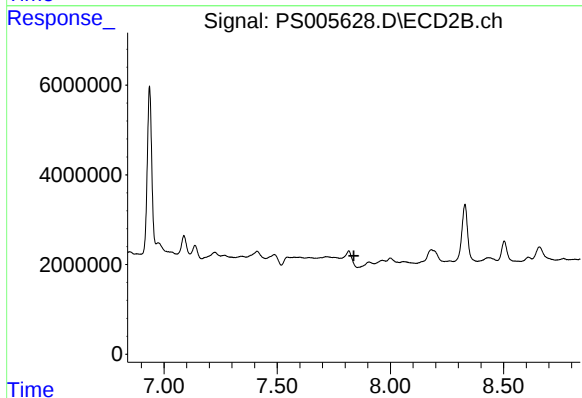


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.

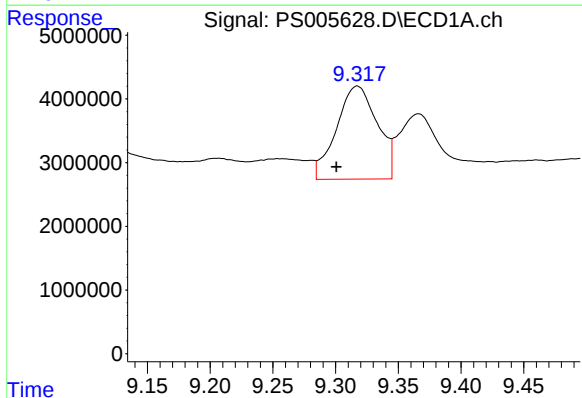


#14 DINOSEB

R.T.: 9.317 min
Delta R.T.: 0.017 min
Response: 33177858
Conc: 4.76 ng/ml

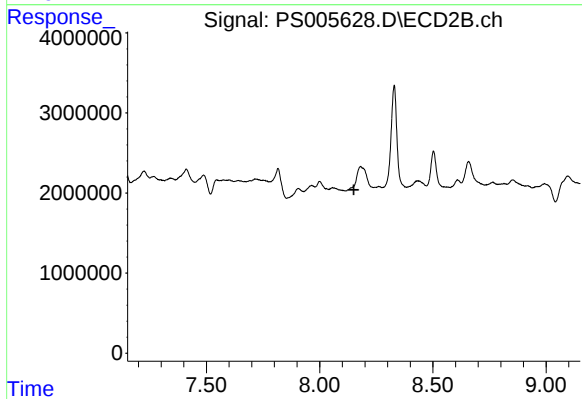

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 8.151 min
Response: 0
Conc: N.D.

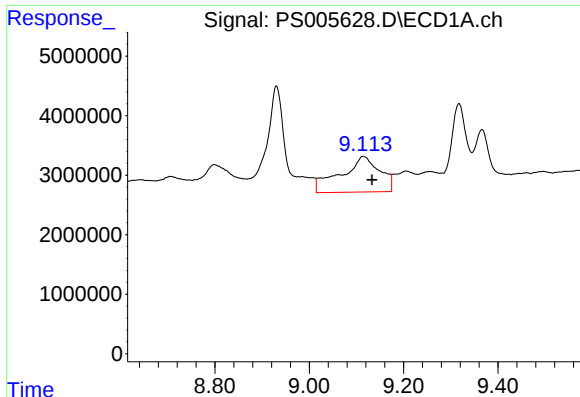

#15 Picloram


R.T.: 9.114 min
Delta R.T.: -0.019 min
Response: 34515052
Conc: 2.77 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-1

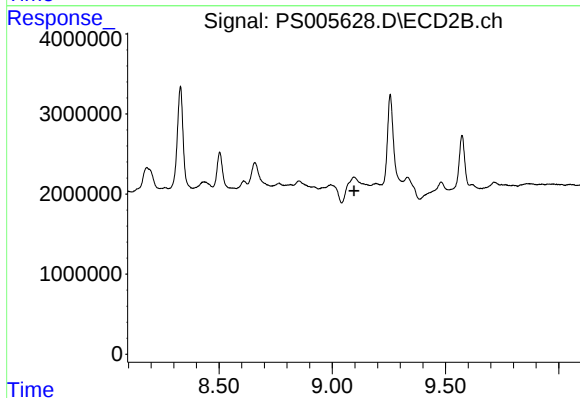


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.096 min
Response: 0
Conc: N.D.

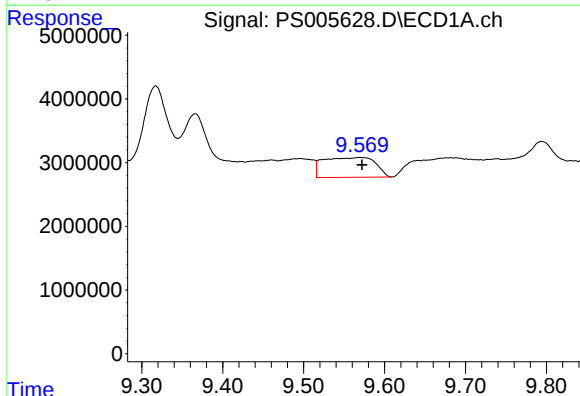

#16 DCPA

R.T.: 9.570 min
Delta R.T.: -0.002 min
Response: 13944206
Conc: 1.28 ng/ml

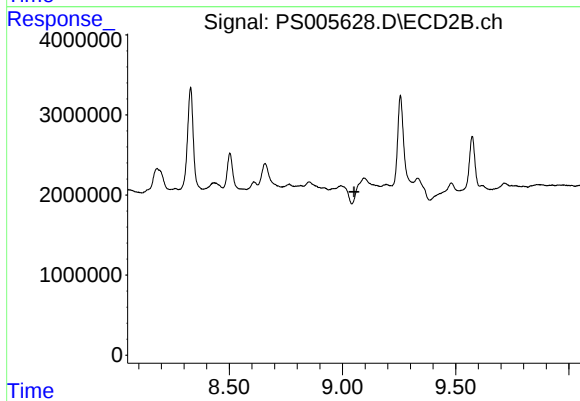

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.051 min
Response: 0
Conc: N.D.