

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072019\
 Data File : PS005629.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2019 18:55
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 00:54:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 19 08:54:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.561	5.277	786.3E6	490.8E6	498.986	475.186
Target Compounds							
3) T	4-Nitroph...	5.382	0.000	5192531	0	7.264	N.D. #
5) T	DICAMBA	5.720	0.000	1144210	0	<MDL	N.D. #
9) T	2,4-D	6.645	0.000	108.4E6	0	61.800	N.D. #
10) T	Pentachlo...	6.847	0.000	6063266	0	<MDL	N.D. #
11) T	2,4,5-TP ...	7.385	0.000	2679760	0	<MDL	N.D. #
12) T	2,4,5-T	7.681	0.000	7105494	0	<MDL	N.D. #
14) T	DINOSEB	9.283	0.000	13875557	0	1.989	N.D. #
15) T	Picloram	9.150	9.099	59477248	41674964	4.774	5.321
16) T	DCPA	9.558	9.099	4771278	41674964	<MDL	5.896 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072019\
Data File : PS005629.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2019 18:55
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 00:54:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
Quant Title : 8080.M
QLast Update : Fri Jul 19 08:54:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

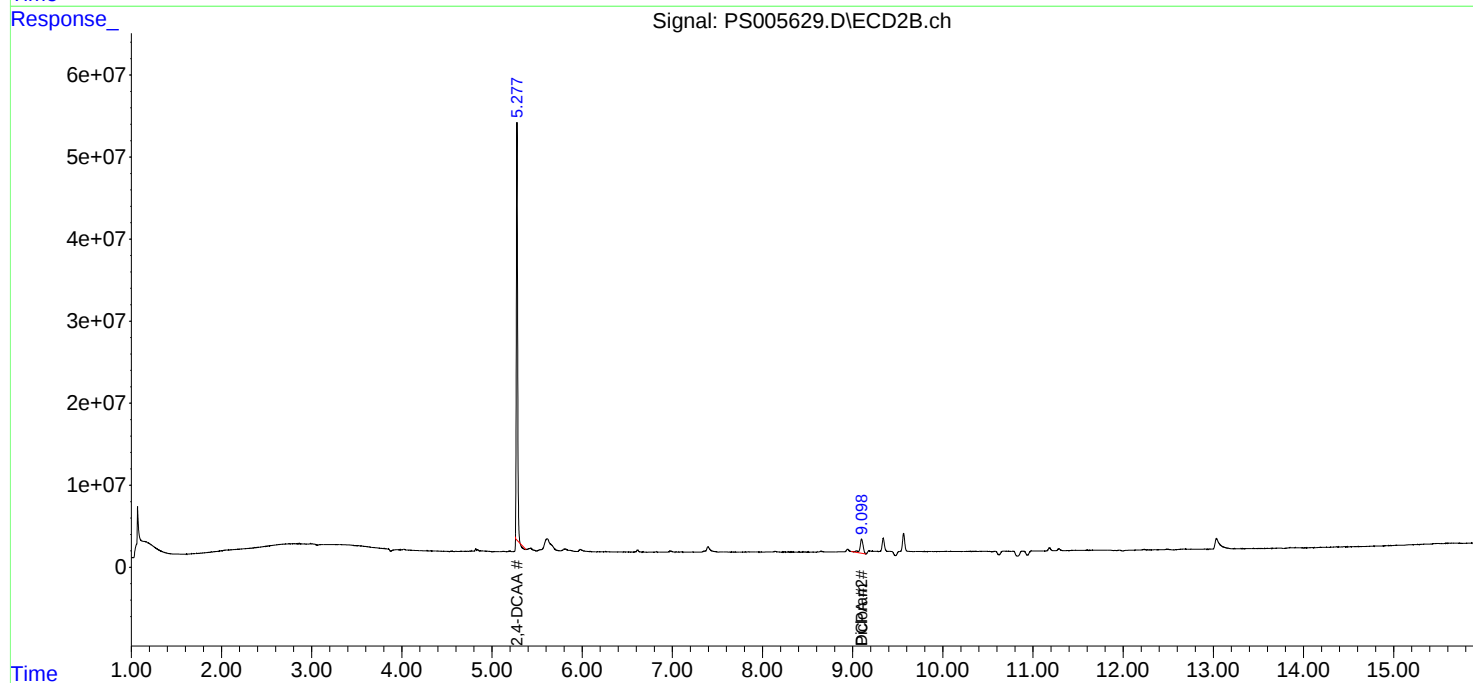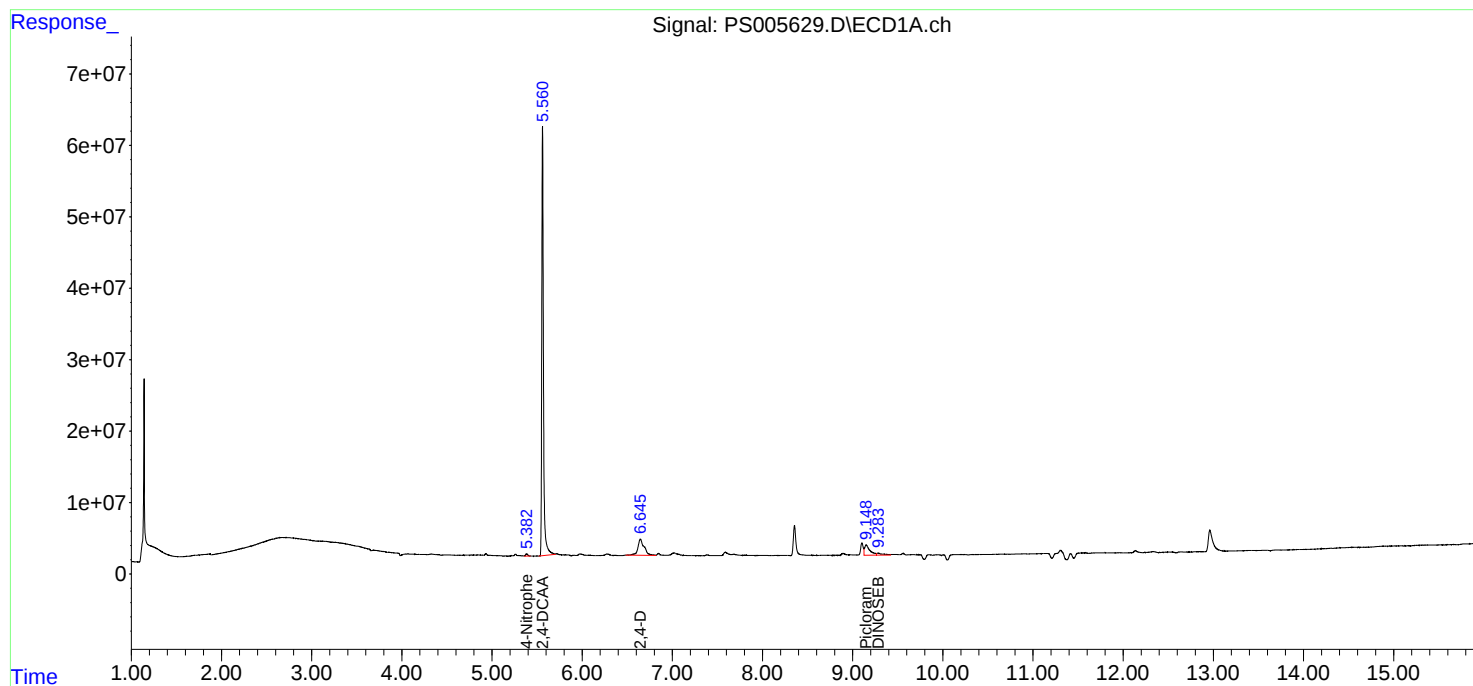


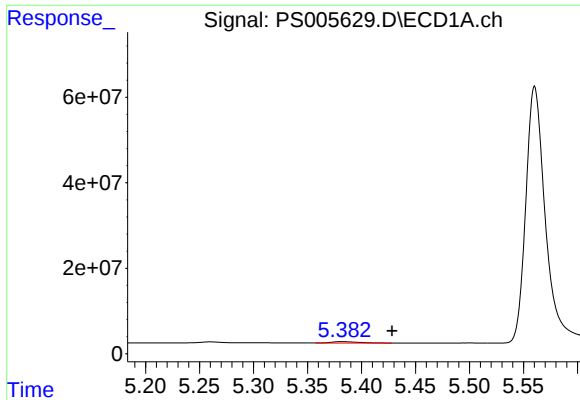

#3 4-Nitrophenol


R.T.: 5.382 min
Delta R.T.: -0.046 min
Response: 5192531
Conc: 7.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

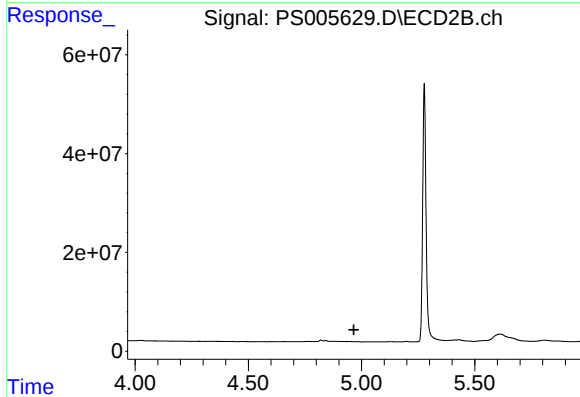


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.966 min
Response: 0
Conc: N.D.

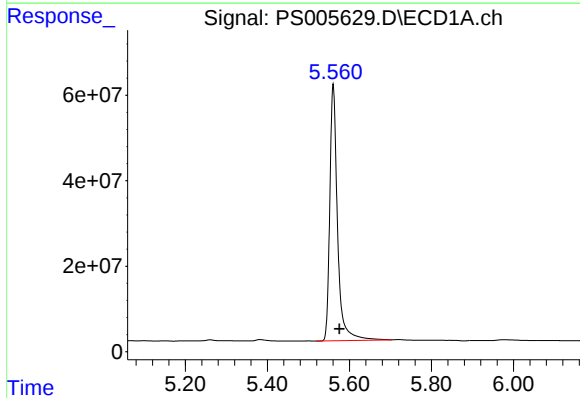


#4 2,4-DCAA

R.T.: 5.561 min
Delta R.T.: -0.015 min
Response: 786278941
Conc: 498.99 ng/ml

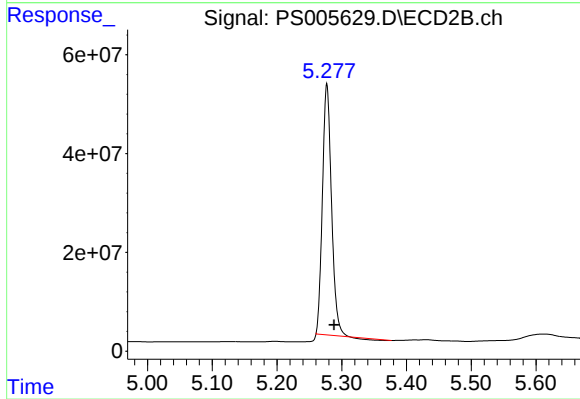

#4 2,4-DCAA


R.T.: 5.277 min
Delta R.T.: -0.011 min
Response: 490819646
Conc: 475.19 ng/ml

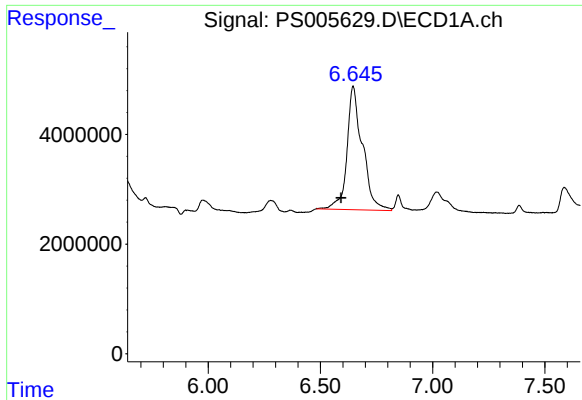

#9 2,4-D


R.T.: 6.645 min
Delta R.T.: 0.052 min
Response: 108378122
Conc: 61.80 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

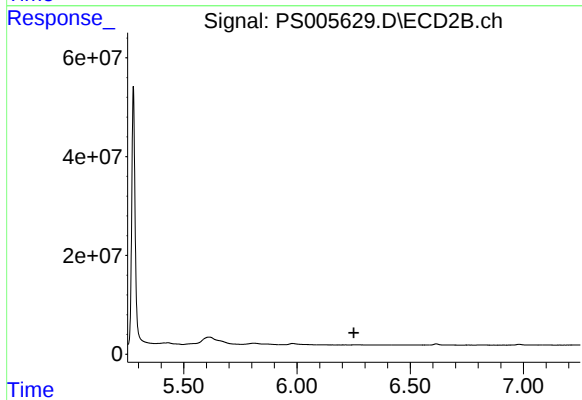


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.251 min
Response: 0
Conc: N.D.

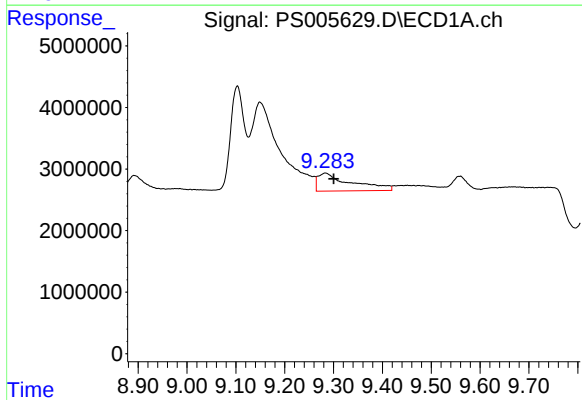


#14 DINOSEB

R.T.: 9.283 min
Delta R.T.: -0.017 min
Response: 13875557
Conc: 1.99 ng/ml

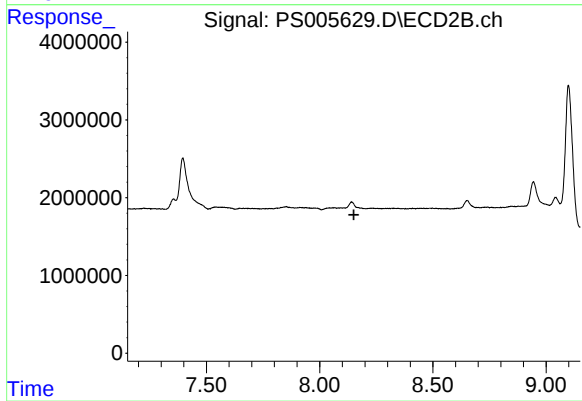

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 8.151 min
Response: 0
Conc: N.D.

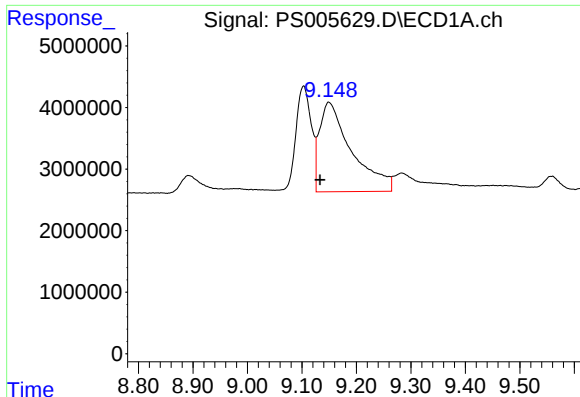

#15 Picloram


R.T.: 9.150 min
Delta R.T.: 0.016 min
Response: 59477248
Conc: 4.77 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

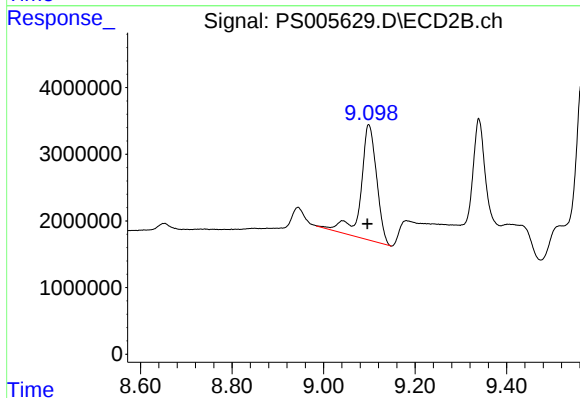


#15 Picloram

R.T.: 9.099 min
Delta R.T.: 0.003 min
Response: 41674964
Conc: 5.32 ng/ml

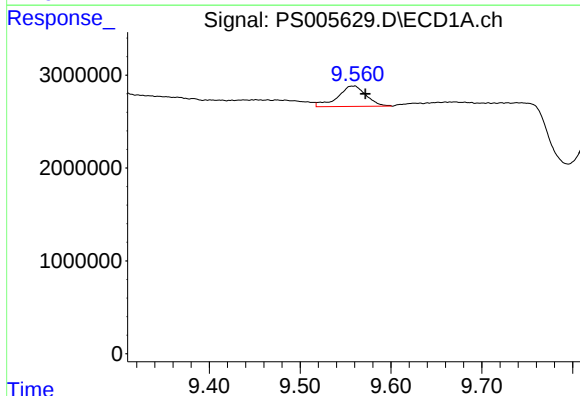

#16 DCPA

R.T.: 9.558 min
Delta R.T.: -0.014 min
Response: 4771278
Conc: N.D.

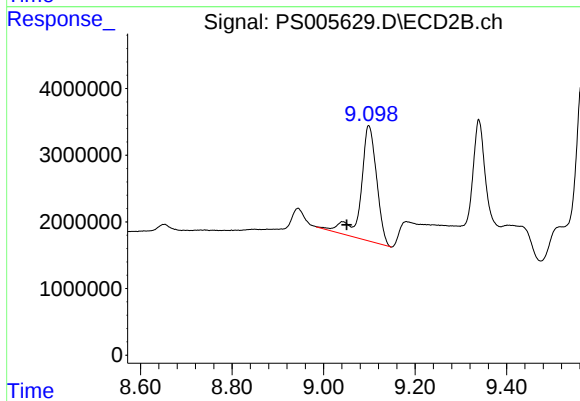

#16 DCPA

R.T.: 9.099 min
Delta R.T.: 0.048 min
Response: 41674964
Conc: 5.90 ng/ml