

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072019\
 Data File : PS005634.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2019 20:45
 Operator : SM\AJ
 Sample : K3887-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 AOC-7(1)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 00:56:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 19 08:54:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.564	5.281	410.7E6	275.7E6	260.629	266.884
Target Compounds							
2) T	3,5-DICHL...	4.881	4.600	5574552	89139447	2.620	65.763 #
3) T	4-Nitroph...	5.416	0.000	4258760	0	5.957	N.D. #
5) T	DICAMBA	5.747	0.000	1320193	0	<MDL	N.D. #
6) T	MCP	5.872	0.000	7028871	0	1.447	N.D. #
8) T	DICHLORPROP	6.347	0.000	1935333	0	1.273	N.D. #
9) T	2,4-D	6.649	0.000	123.7E6	0	70.542	N.D. #
10) T	Pentachlo...	6.925	0.000	20128747	0	<MDL	N.D. #
11) T	2,4,5-TP ...	7.350	0.000	2574571	0	<MDL	N.D. #
13) T	2,4-DB	8.207	0.000	16470671	0	13.148	N.D. #
14) T	DINOSEB	9.301	0.000	13186081	0	1.890	N.D. #
15) T	Picloram	9.104	0.000	38588967	0	3.097	N.D. #
16) T	DCPA	9.545	0.000	18065579	0	1.659	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072019\
Data File : PS005634.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2019 20:45
Operator : SM\AJ
Sample : K3887-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
AOC-7(1)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 00:56:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
Quant Title : 8080.M
QLast Update : Fri Jul 19 08:54:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

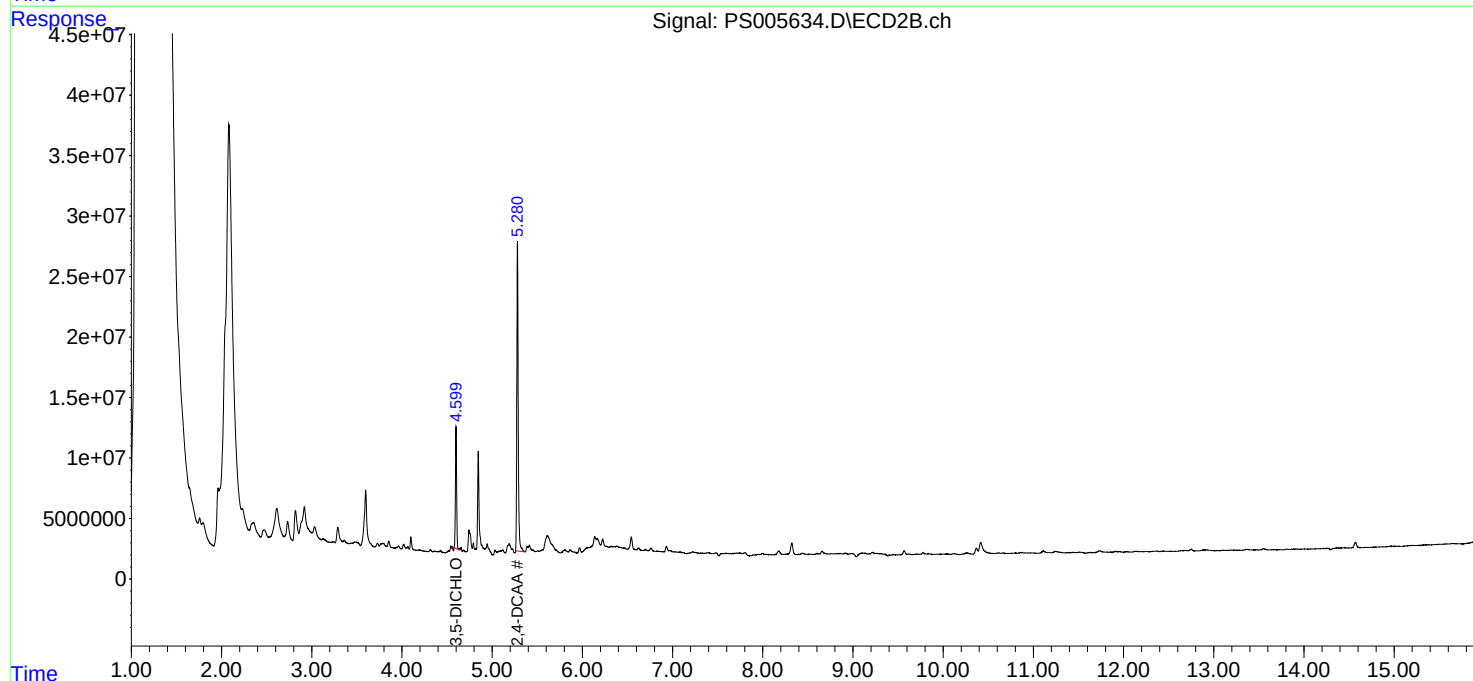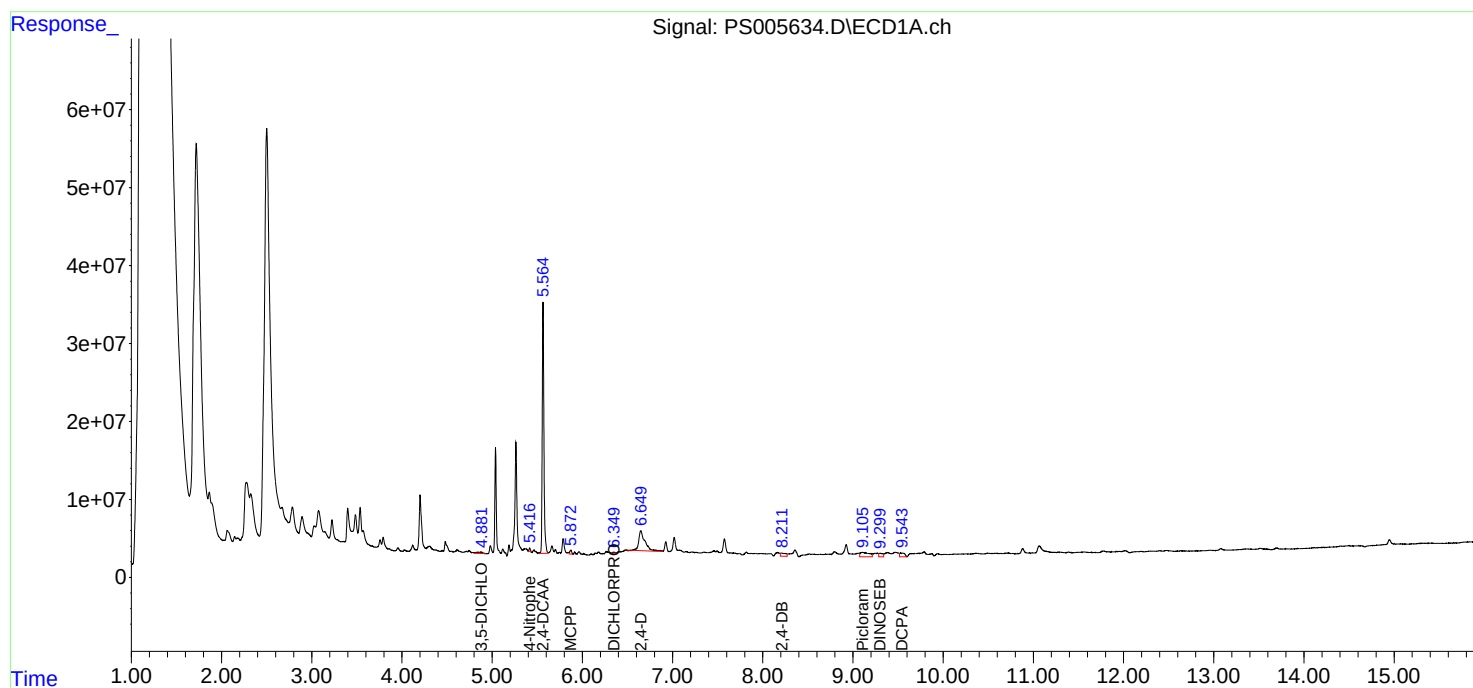


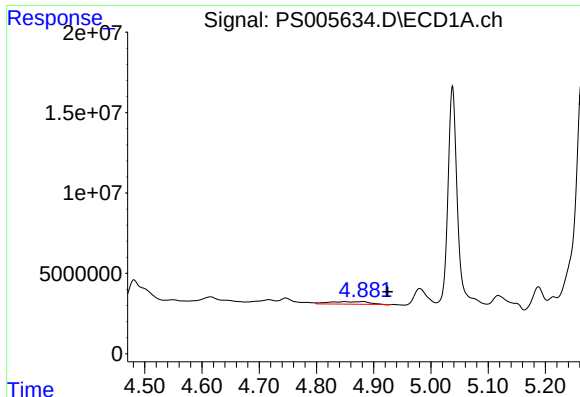

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.881 min
Delta R.T.: -0.044 min
Response: 5574552
Conc: 2.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
AOC-7(1)

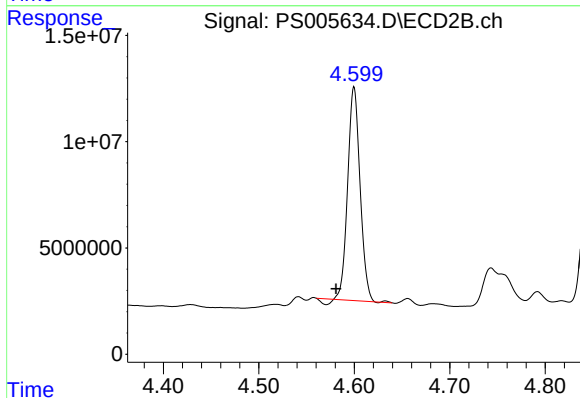


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.600 min
Delta R.T.: 0.019 min
Response: 89139447
Conc: 65.76 ng/ml

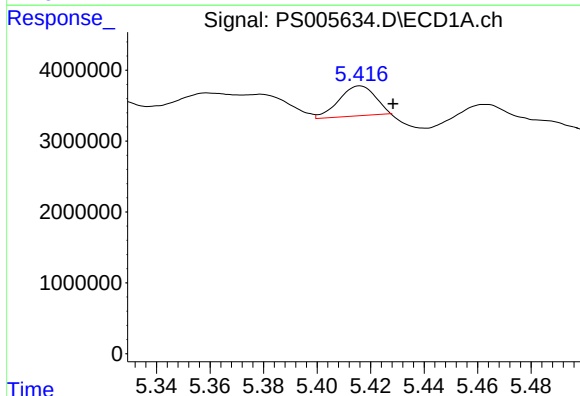


#3 4-Nitrophenol

R.T.: 5.416 min
Delta R.T.: -0.012 min
Response: 4258760
Conc: 5.96 ng/ml

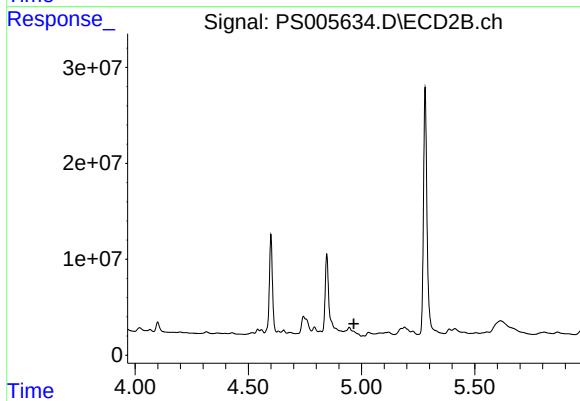

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 4.966 min
Response: 0
Conc: N.D.

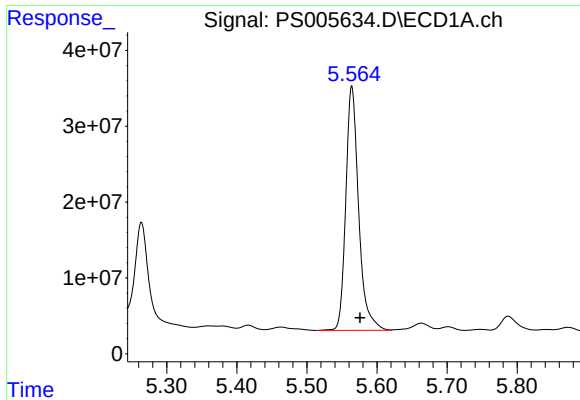

#4 2,4-DCAA


R.T.: 5.564 min
Delta R.T.: -0.012 min
Response: 410686449
Conc: 260.63 ng/ml

Instrument :
ECD_S
ClientSampleId :
AOC-7(1)

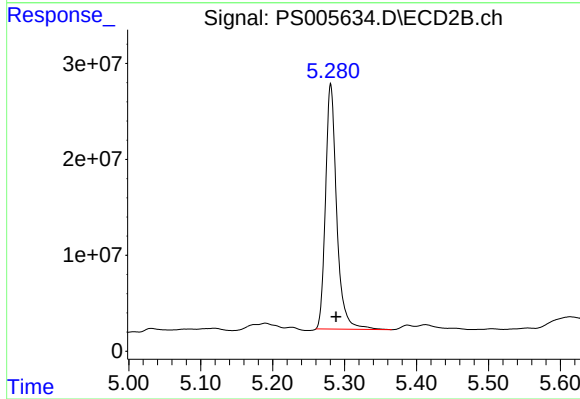


#4 2,4-DCAA

R.T.: 5.281 min
Delta R.T.: -0.007 min
Response: 275664400
Conc: 266.88 ng/ml

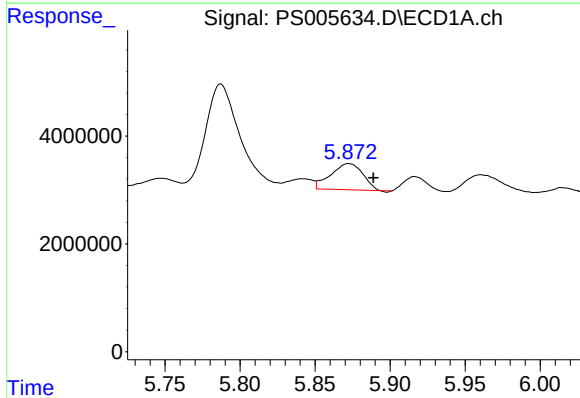


#6 MCPP

R.T.: 5.872 min
Delta R.T.: -0.016 min
Response: 7028871
Conc: 1.45 ug/ml

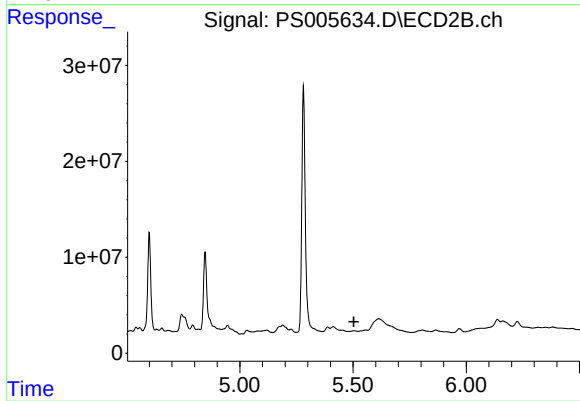

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 5.504 min
Response: 0
Conc: N.D.

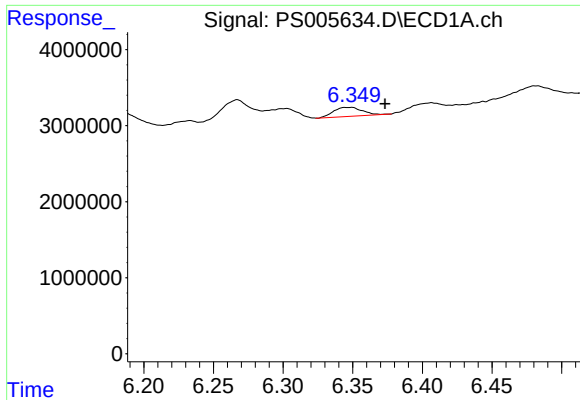

#8 DICHLORPROP


R.T.: 6.347 min
Delta R.T.: -0.026 min
Response: 1935333
Conc: 1.27 ng/ml

Instrument :
ECD_S
ClientSampleId :
AOC-7(1)

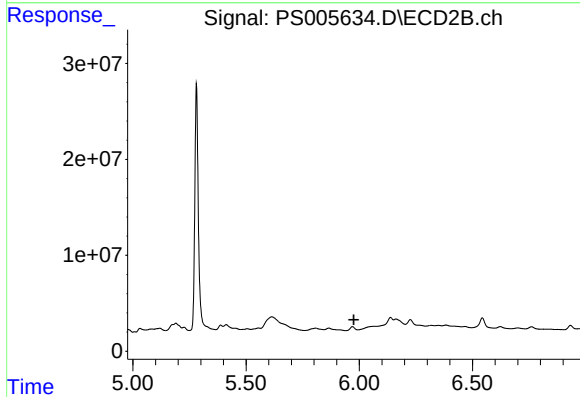


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 5.976 min
Response: 0
Conc: N.D.

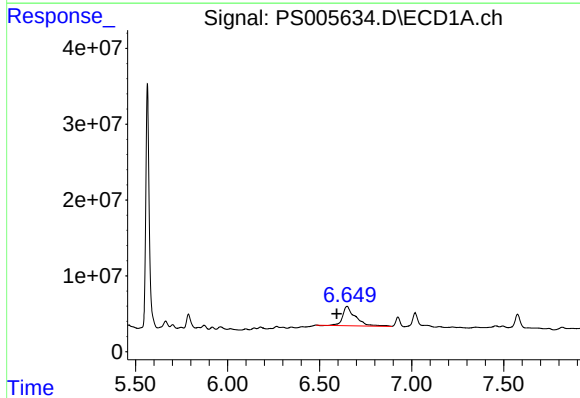


#9 2,4-D

R.T.: 6.649 min
Delta R.T.: 0.056 min
Response: 123707937
Conc: 70.54 ng/ml

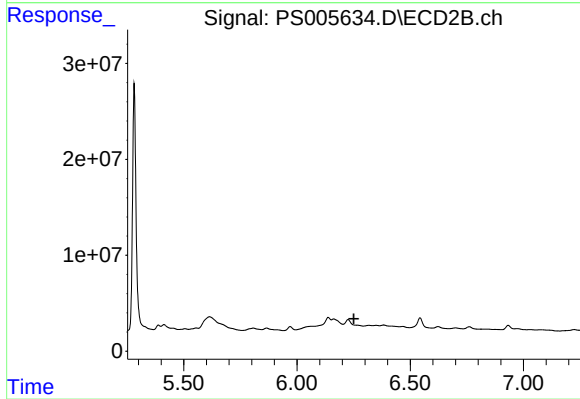

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 6.251 min
Response: 0
Conc: N.D.

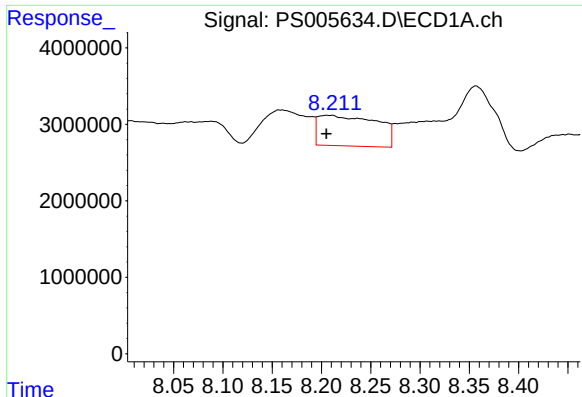

#13 2,4-DB


R.T.: 8.207 min
Delta R.T.: 0.002 min
Response: 16470671
Conc: 13.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
AOC-7(1)

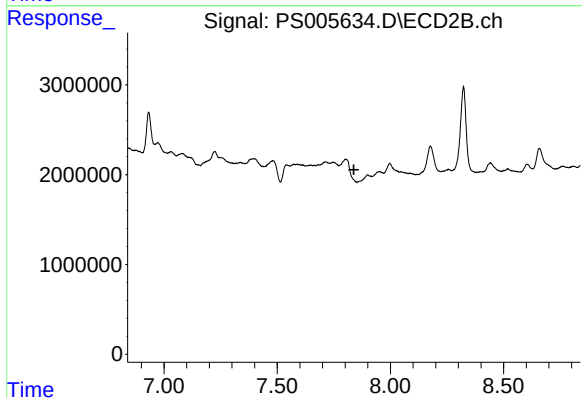


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.

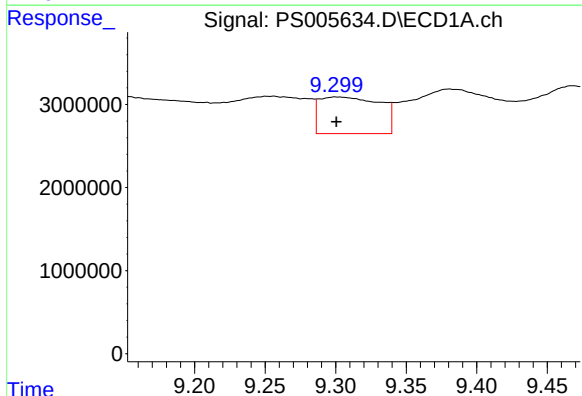


#14 DINOSEB

R.T.: 9.301 min
Delta R.T.: 0.000 min
Response: 13186081
Conc: 1.89 ng/ml

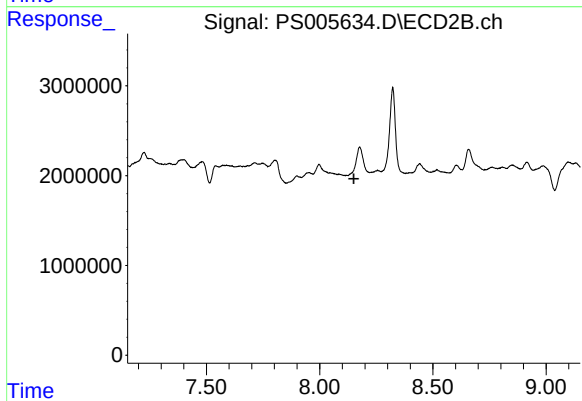

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 8.151 min
Response: 0
Conc: N.D.

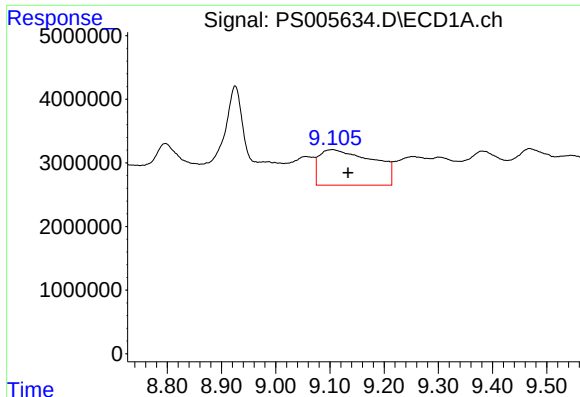

#15 Picloram


R.T.: 9.104 min
Delta R.T.: -0.029 min
Response: 38588967
Conc: 3.10 ng/ml

Instrument :
ECD_S
ClientSampleId :
AOC-7(1)

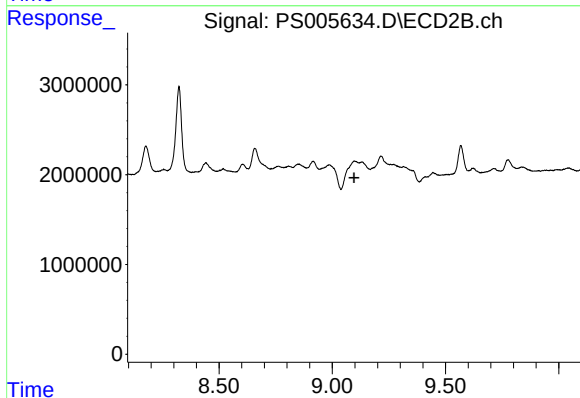


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.096 min
Response: 0
Conc: N.D.

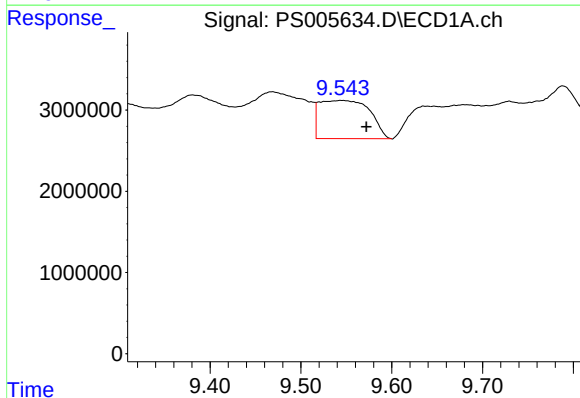

#16 DCPA

R.T.: 9.545 min
Delta R.T.: -0.027 min
Response: 18065579
Conc: 1.66 ng/ml

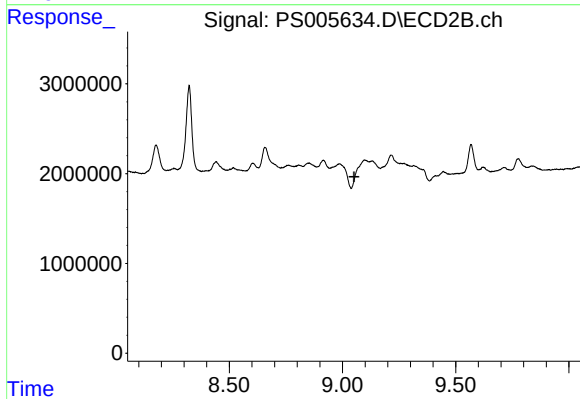

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.051 min
Response: 0
Conc: N.D.