

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072019\
 Data File : PS005636.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2019 21:30
 Operator : SM\AJ
 Sample : K3887-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 AOC-7(3)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 00:57:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 19 08:54:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.561	5.278	353.7E6	214.1E6	224.480	207.315
Target Compounds							
2) T	3,5-DICHL...	4.979	4.596	3441881	64548133	1.618	47.621 #
3) T	4-Nitroph...	5.412	0.000	4177374	0	5.844	N.D. #
5) T	DICAMBA	5.750	0.000	3254373	0	<MDL	N.D. #
6) T	MCP	5.868	0.000	8100293	0	1.668	N.D. #
8) T	DICHLORPROP	6.344	0.000	1524860	0	1.003	N.D. #
9) T	2,4-D	6.646	6.222	117.2E6	12394737	66.832	10.615 #
10) T	Pentachlo...	6.800	0.000	3517735	0	<MDL	N.D. #
11) T	2,4,5-TP ...	7.384	0.000	3612006	0	<MDL	N.D. #
13) T	2,4-DB	8.207	0.000	13497547	0	10.775	N.D. #
14) T	DINOSEB	9.298	0.000	9699486	0	1.391	N.D. #
15) T	Picloram	9.102	0.000	41095200	0	3.299	N.D. #
16) T	DCPA	9.533	0.000	13691272	0	1.257	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072019\
Data File : PS005636.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2019 21:30
Operator : SM\AJ
Sample : K3887-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
AOC-7(3)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 00:57:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
Quant Title : 8080.M
QLast Update : Fri Jul 19 08:54:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

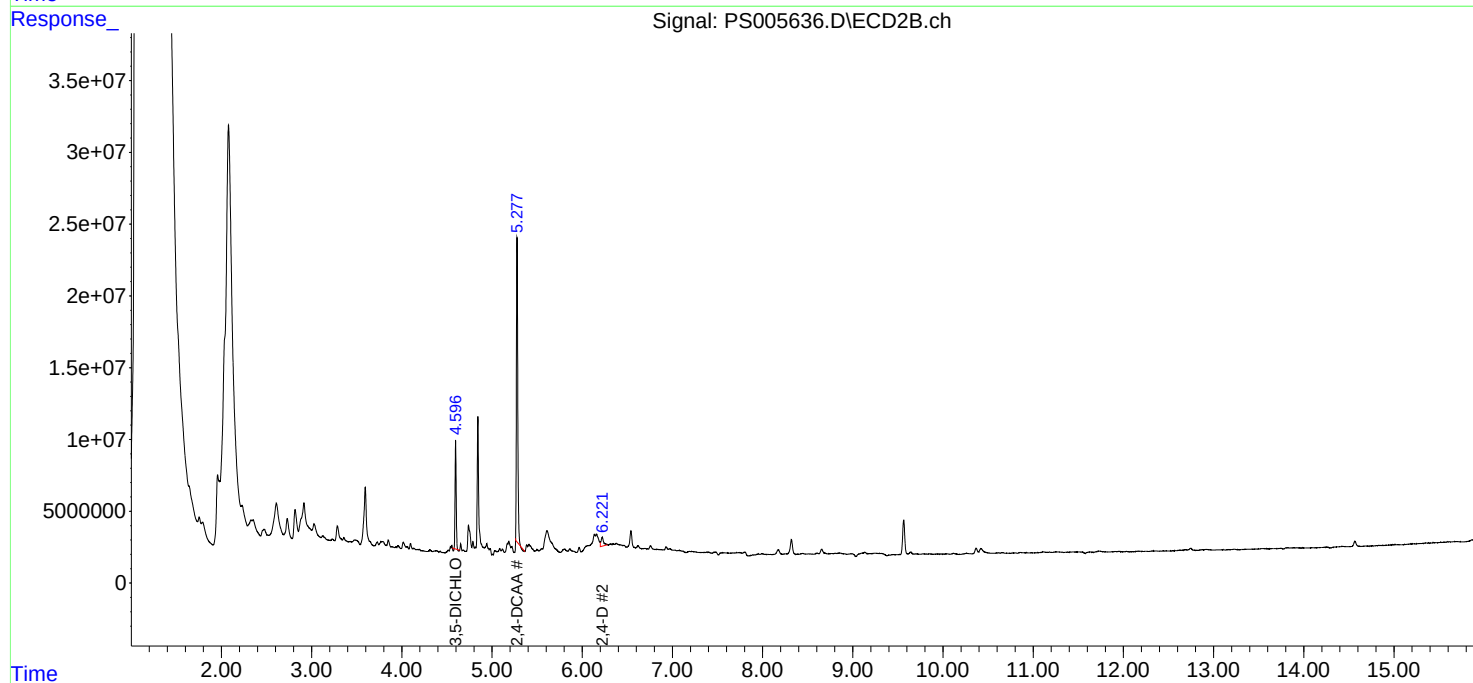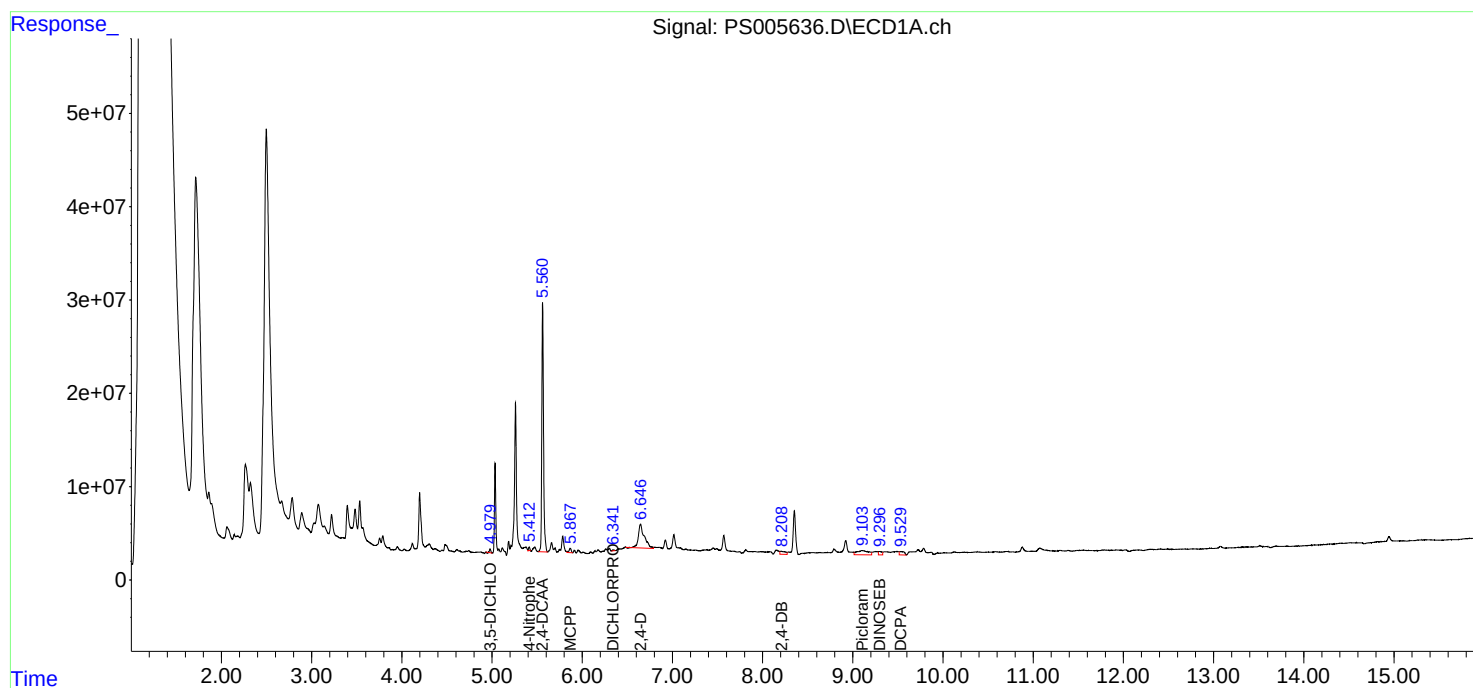


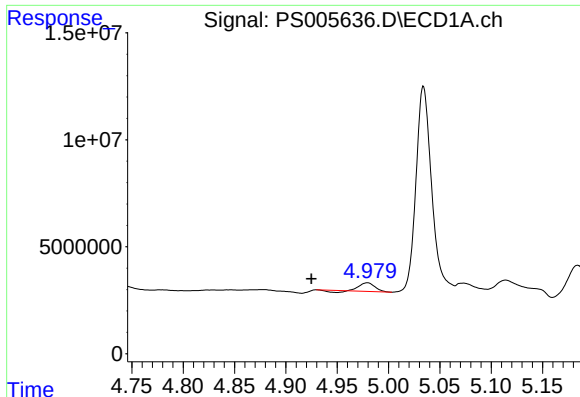

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.979 min
Delta R.T.: 0.054 min
Response: 3441881
Conc: 1.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
AOC-7(3)

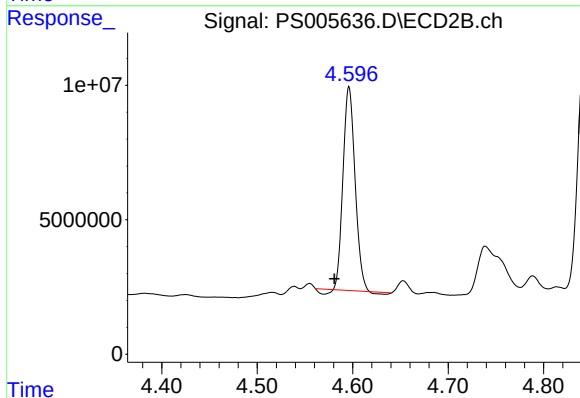


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.596 min
Delta R.T.: 0.015 min
Response: 64548133
Conc: 47.62 ng/ml

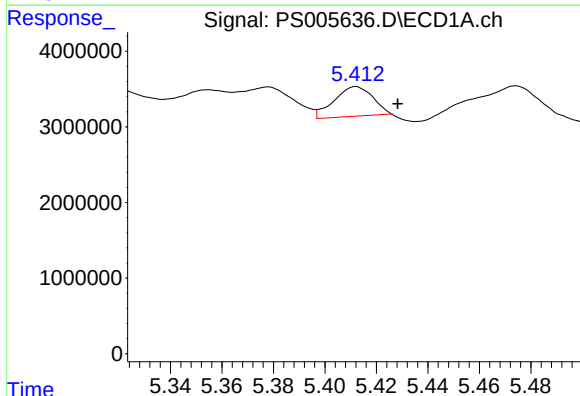


#3 4-Nitrophenol

R.T.: 5.412 min
Delta R.T.: -0.016 min
Response: 4177374
Conc: 5.84 ng/ml

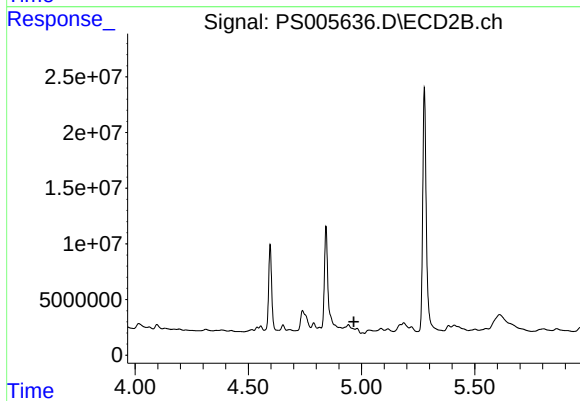

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 4.966 min
Response: 0
Conc: N.D.

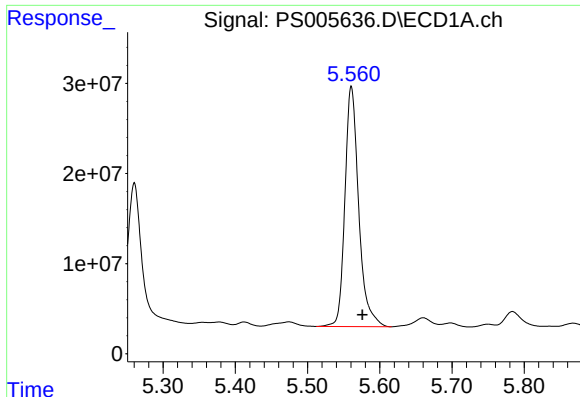

#4 2,4-DCAA


R.T.: 5.561 min
Delta R.T.: -0.015 min
Response: 353725706
Conc: 224.48 ng/ml

Instrument :
ECD_S
ClientSampleId :
AOC-7(3)

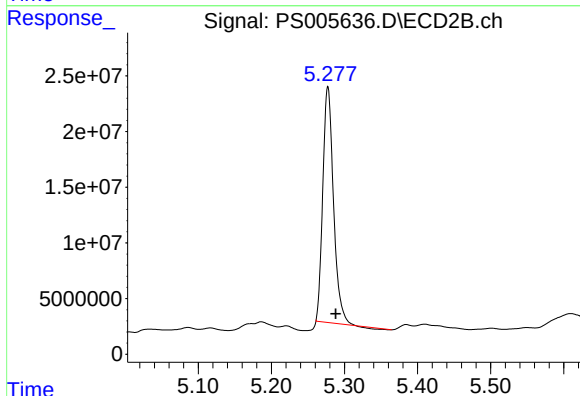


#4 2,4-DCAA

R.T.: 5.278 min
Delta R.T.: -0.010 min
Response: 214135974
Conc: 207.32 ng/ml

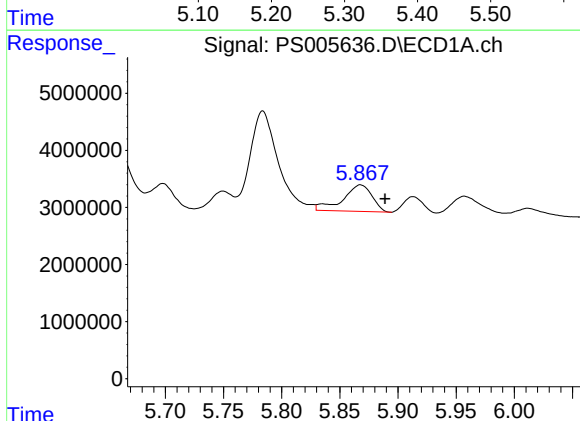


#6 MCP

R.T.: 5.868 min
Delta R.T.: -0.021 min
Response: 8100293
Conc: 1.67 ug/ml

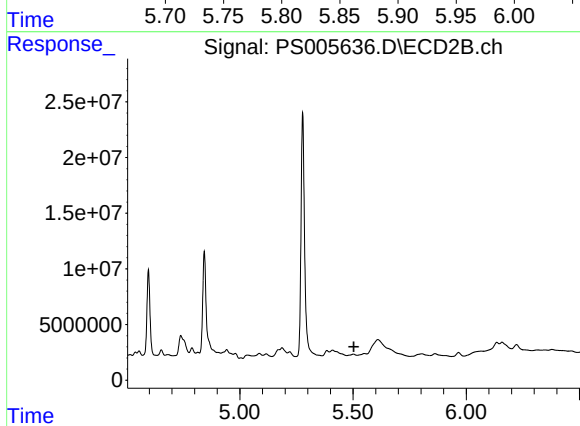

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.504 min
Response: 0
Conc: N.D.

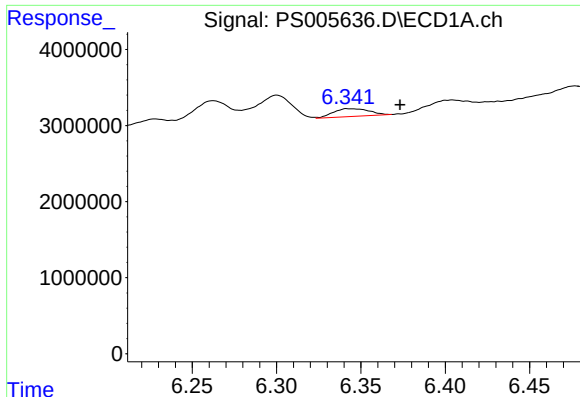

#8 DICHLORPROP


R.T.: 6.344 min
Delta R.T.: -0.029 min
Response: 1524860
Conc: 1.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
AOC-7(3)

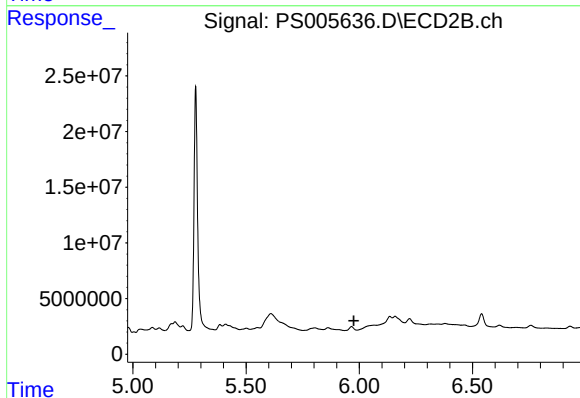


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 5.976 min
Response: 0
Conc: N.D.

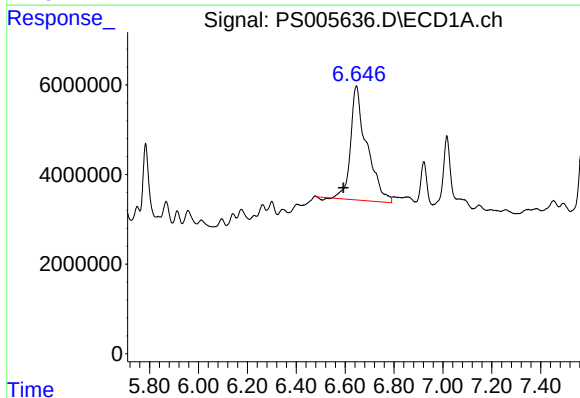


#9 2,4-D

R.T.: 6.646 min
Delta R.T.: 0.053 min
Response: 117201854
Conc: 66.83 ng/ml

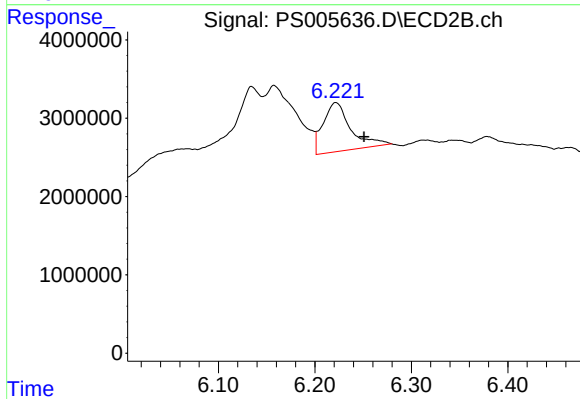

#9 2,4-D


R.T.: 6.222 min
Delta R.T.: -0.029 min
Response: 12394737
Conc: 10.61 ng/ml

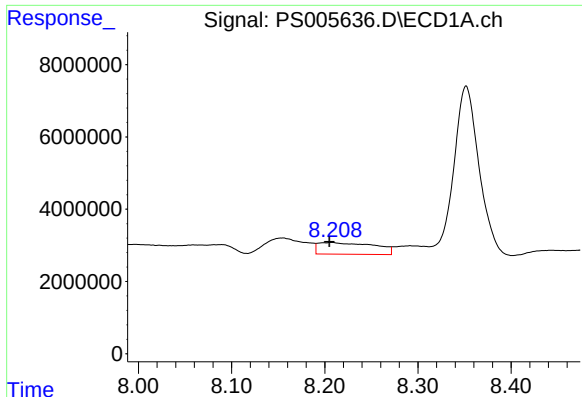

#13 2,4-DB


R.T.: 8.207 min
Delta R.T.: 0.002 min
Response: 13497547
Conc: 10.77 ng/ml

Instrument :
ECD_S
ClientSampleId :
AOC-7(3)

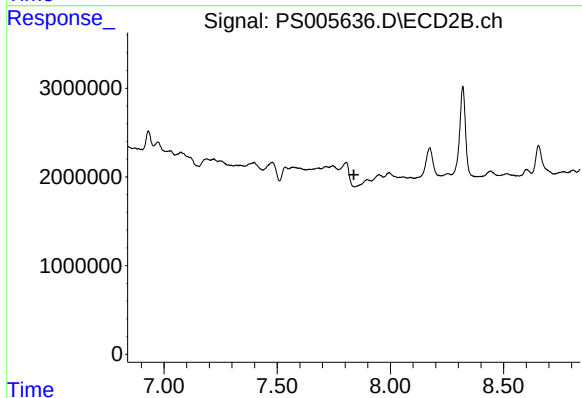


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.

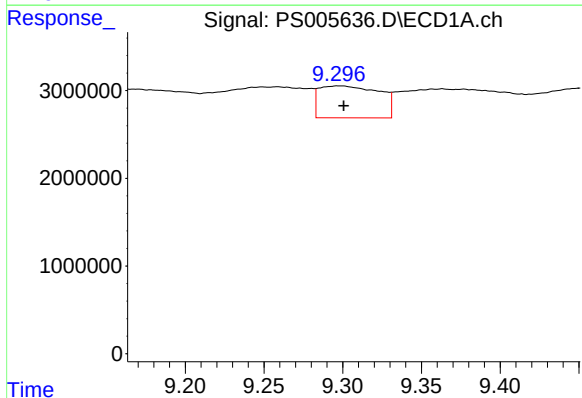


#14 DINOSEB

R.T.: 9.298 min
Delta R.T.: -0.003 min
Response: 9699486
Conc: 1.39 ng/ml

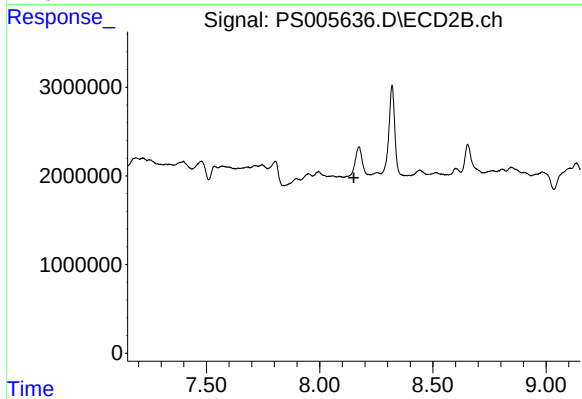

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 8.151 min
Response: 0
Conc: N.D.

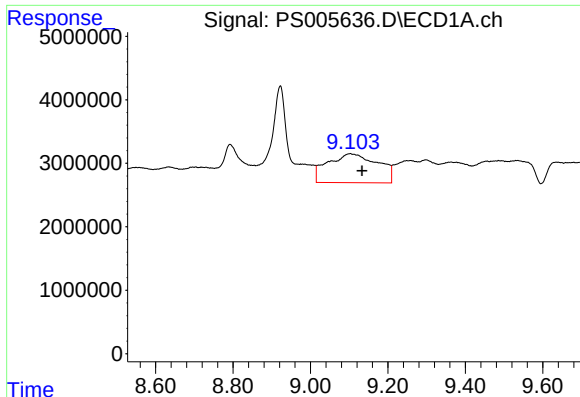

#15 Picloram


R.T.: 9.102 min
Delta R.T.: -0.031 min
Response: 41095200
Conc: 3.30 ng/ml

Instrument :
ECD_S
ClientSampleId :
AOC-7(3)

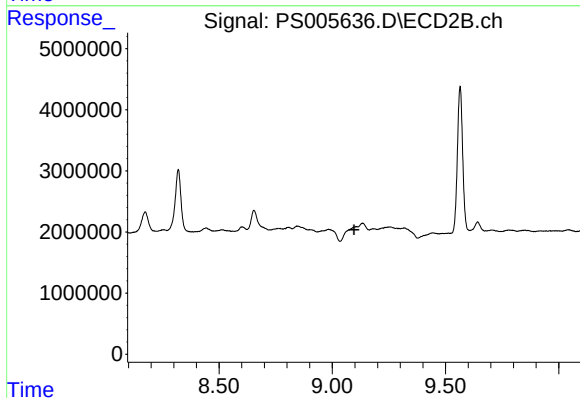


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.096 min
Response: 0
Conc: N.D.

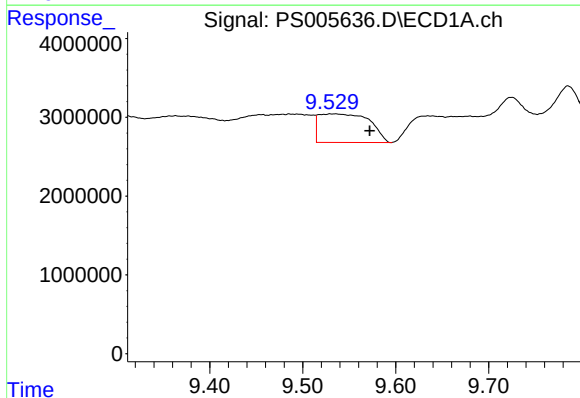

#16 DCPA

R.T.: 9.533 min
Delta R.T.: -0.039 min
Response: 13691272
Conc: 1.26 ng/ml

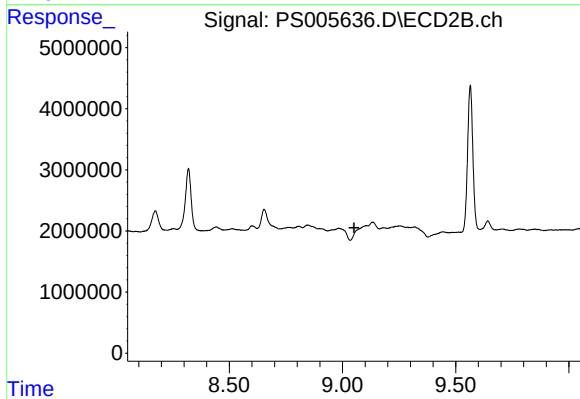

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.051 min
Response: 0
Conc: N.D.