

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072019\
 Data File : PS005640.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2019 22:58
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 00:58:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 19 08:54:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.564	5.281	856.4E6	583.2E6	543.463	564.664
Target Compounds							
3) T	4-Nitroph...	5.385	0.000	5664813	0	7.924	N.D. #
7) T	MCPA	0.000	5.617	0	68675139	N.D.	15.586
9) T	2,4-D	6.649	0.000	107.5E6	0	61.298	N.D. #
10) T	Pentachlo...	6.851	0.000	6596307	0	<MDL	N.D. #
11) T	2,4,5-TP ...	7.390	0.000	2783495	0	<MDL	N.D. #
12) T	2,4,5-T	7.686	0.000	7619779	0	<MDL	N.D. #
14) T	DINOSEB	9.287	0.000	12801986	0	1.835	N.D. #
15) T	Picloram	9.107	9.104	35231095	32791350	2.828	4.186 #
16) T	DCPA	9.562	9.104	4096548	32791350	<MDL	4.639 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072019\
Data File : PS005640.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2019 22:58
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 00:58:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
Quant Title : 8080.M
QLast Update : Fri Jul 19 08:54:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

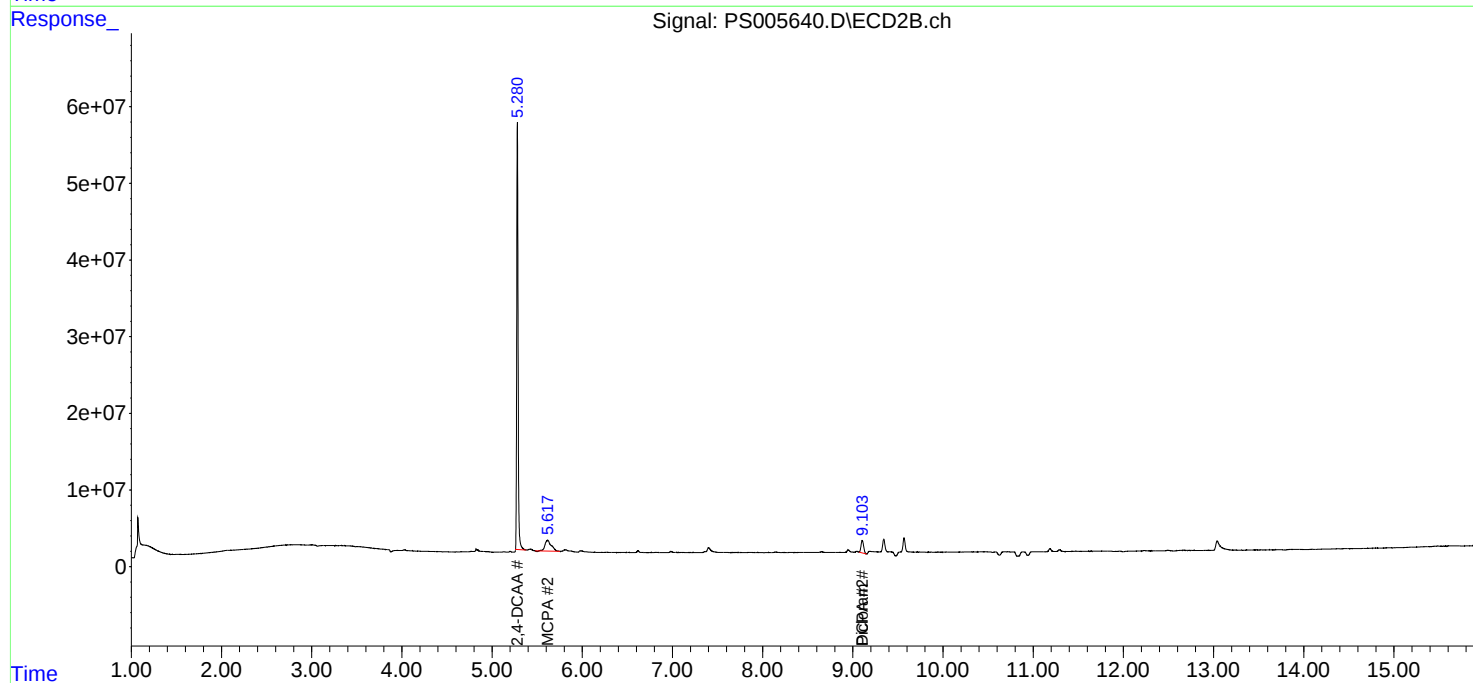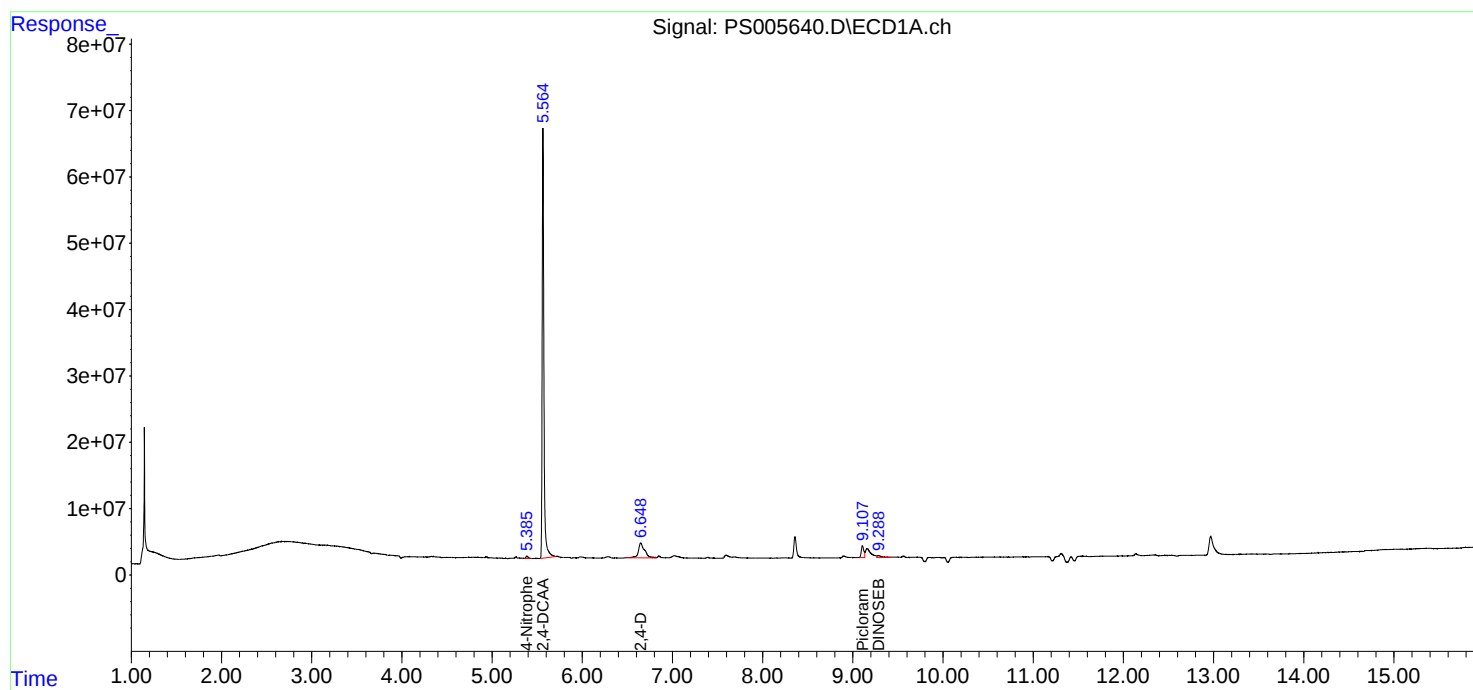


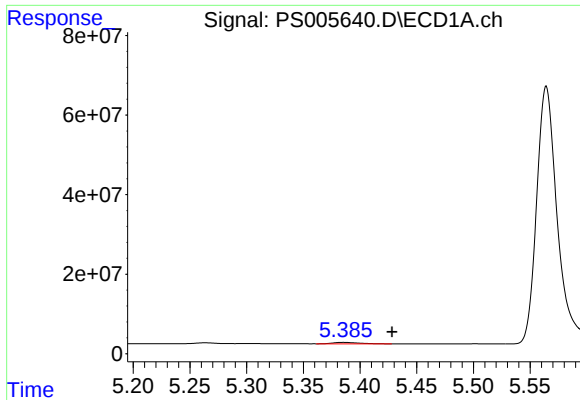

#3 4-Nitrophenol


R.T.: 5.385 min
Delta R.T.: -0.043 min
Response: 5664813
Conc: 7.92 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

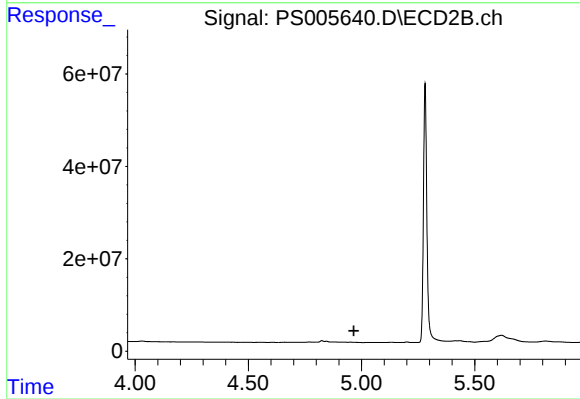


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.966 min
Response: 0
Conc: N.D.

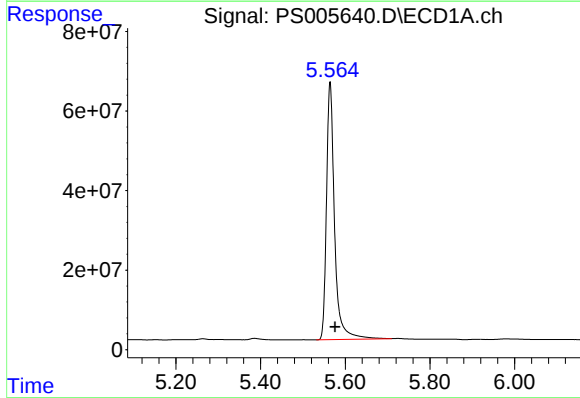


#4 2,4-DCAA

R.T.: 5.564 min
Delta R.T.: -0.012 min
Response: 856364518
Conc: 543.46 ng/ml

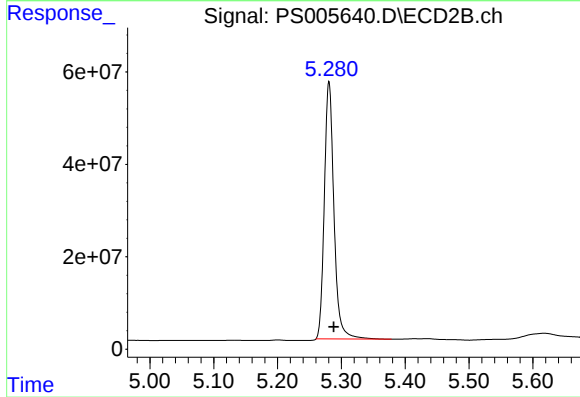

#4 2,4-DCAA


R.T.: 5.281 min
Delta R.T.: -0.007 min
Response: 583241843
Conc: 564.66 ng/ml

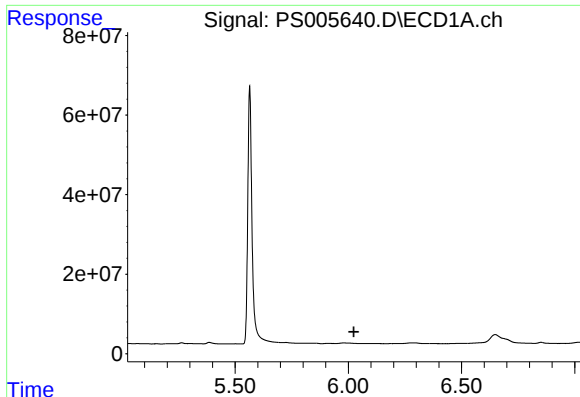

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.024 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

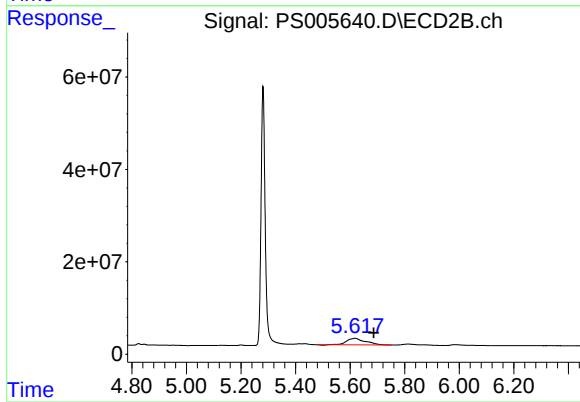


#7 MCPA

R.T.: 5.617 min
Delta R.T.: -0.069 min
Response: 68675139
Conc: 15.59 ug/ml

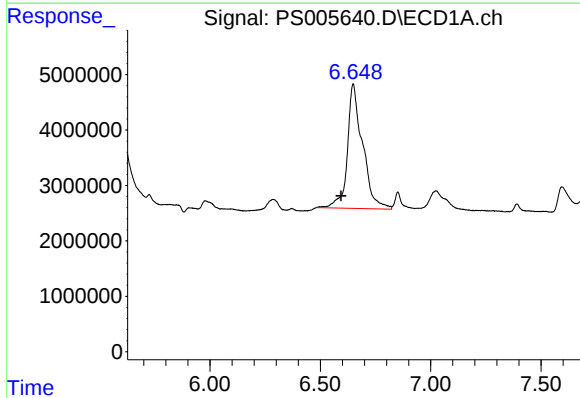


#9 2,4-D

R.T.: 6.649 min
Delta R.T.: 0.056 min
Response: 107497846
Conc: 61.30 ng/ml

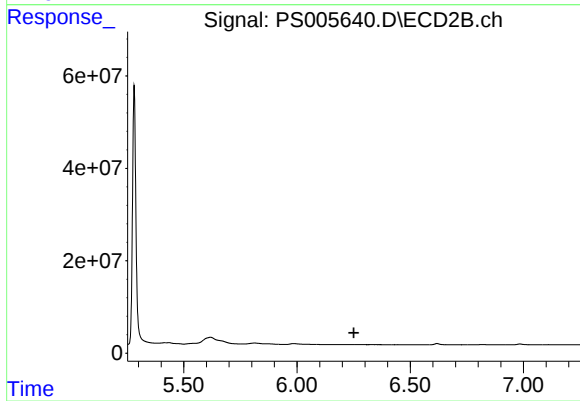

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.251 min
Response: 0
Conc: N.D.

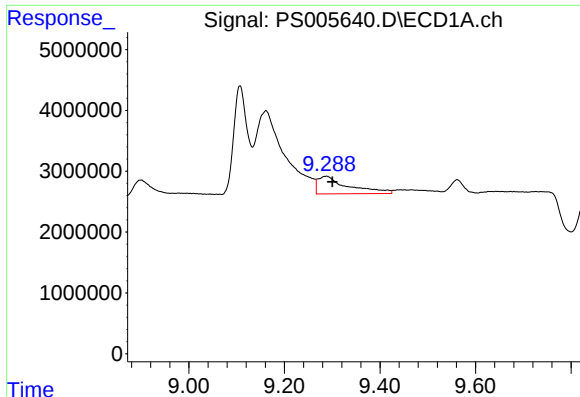

#14 DINOSEB


R.T.: 9.287 min
Delta R.T.: -0.013 min
Response: 12801986
Conc: 1.84 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

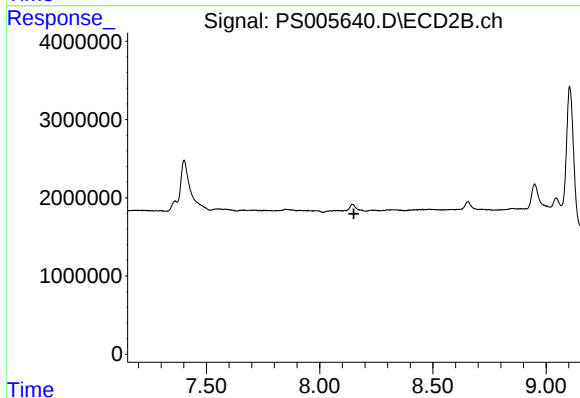


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 8.151 min
Response: 0
Conc: N.D.

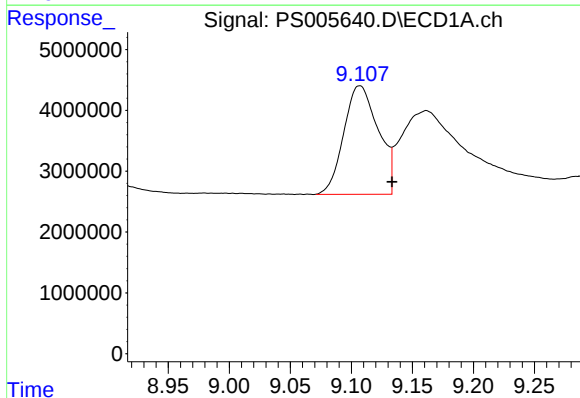


#15 Picloram

R.T.: 9.107 min
Delta R.T.: -0.026 min
Response: 35231095
Conc: 2.83 ng/ml

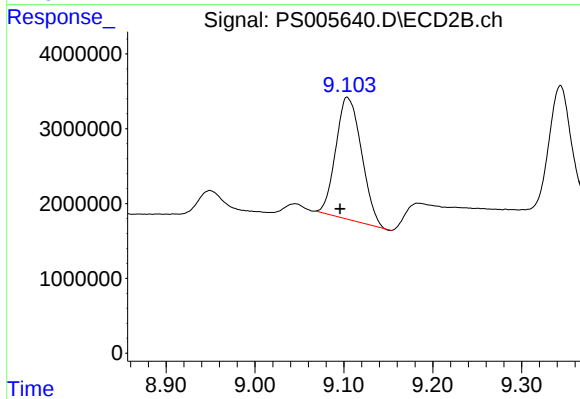

#15 Picloram


R.T.: 9.104 min
Delta R.T.: 0.008 min
Response: 32791350
Conc: 4.19 ng/ml

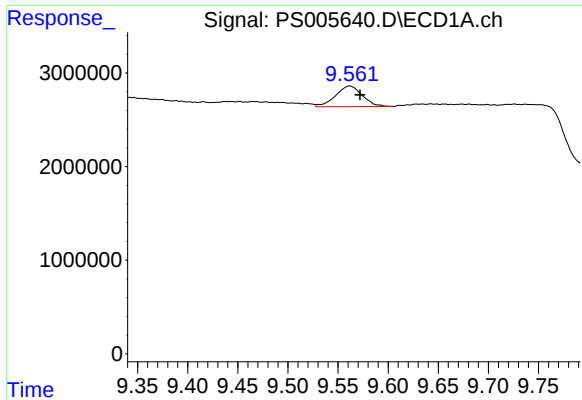

#16 DCPA

R.T.: 9.562 min
Delta R.T.: -0.011 min
Response: 4096548
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

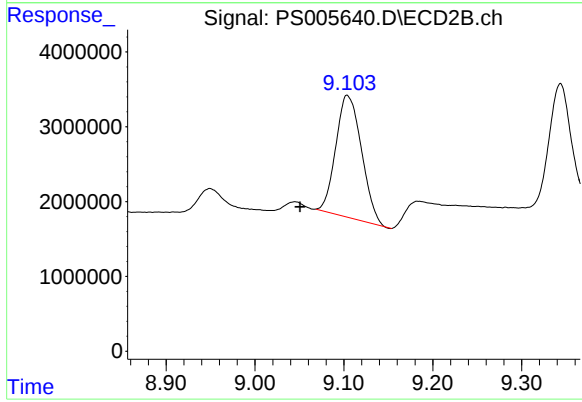

#16 DCPA

R.T.: 9.104 min
Delta R.T.: 0.053 min
Response: 32791350
Conc: 4.64 ng/ml