

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072319\
 Data File : PS005655.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2019 17:46
 Operator : SM\AJ
 Sample : K3868-08
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 00:50:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 19 08:54:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.561	5.278	297.3E6	197.8E6	188.649	191.524
Target Compounds							
2) T	3,5-DICHL...	4.876	4.596	-488498	97609680	N.D.	72.012
3) T	4-Nitroph...	5.412	0.000	4245134	0	5.938	N.D. #
5) T	DICAMBA	5.782	0.000	29918984	0	4.837	N.D. #
6) T	MCP	5.865	0.000	7139737	0	1.470	N.D. #
7) T	MCPA	6.093	0.000	1049840	0	<MDL	N.D. #
8) T	DICHLORPROP	6.345	0.000	1527049	0	1.005	N.D. #
9) T	2,4-D	6.644	0.000	144.5E6	0	82.409	N.D. #
10) T	Pentachlo...	6.842	0.000	11268480	0	<MDL	N.D. #
11) T	2,4,5-TP ...	7.453	0.000	6187052	0	<MDL	N.D. #
13) T	2,4-DB	8.203	0.000	31170635	0	24.883	N.D. #
14) T	DINOSEB	9.356	0.000	22879006	0	3.280	N.D. #
15) T	Picloram	9.136	0.000	65547930	0	5.261	N.D. #
16) T	DCPA	9.536	0.000	15131626	0	1.390	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072319\
Data File : PS005655.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2019 17:46
Operator : SM\AJ
Sample : K3868-08
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
TP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 00:50:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
Quant Title : 8080.M
QLast Update : Fri Jul 19 08:54:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

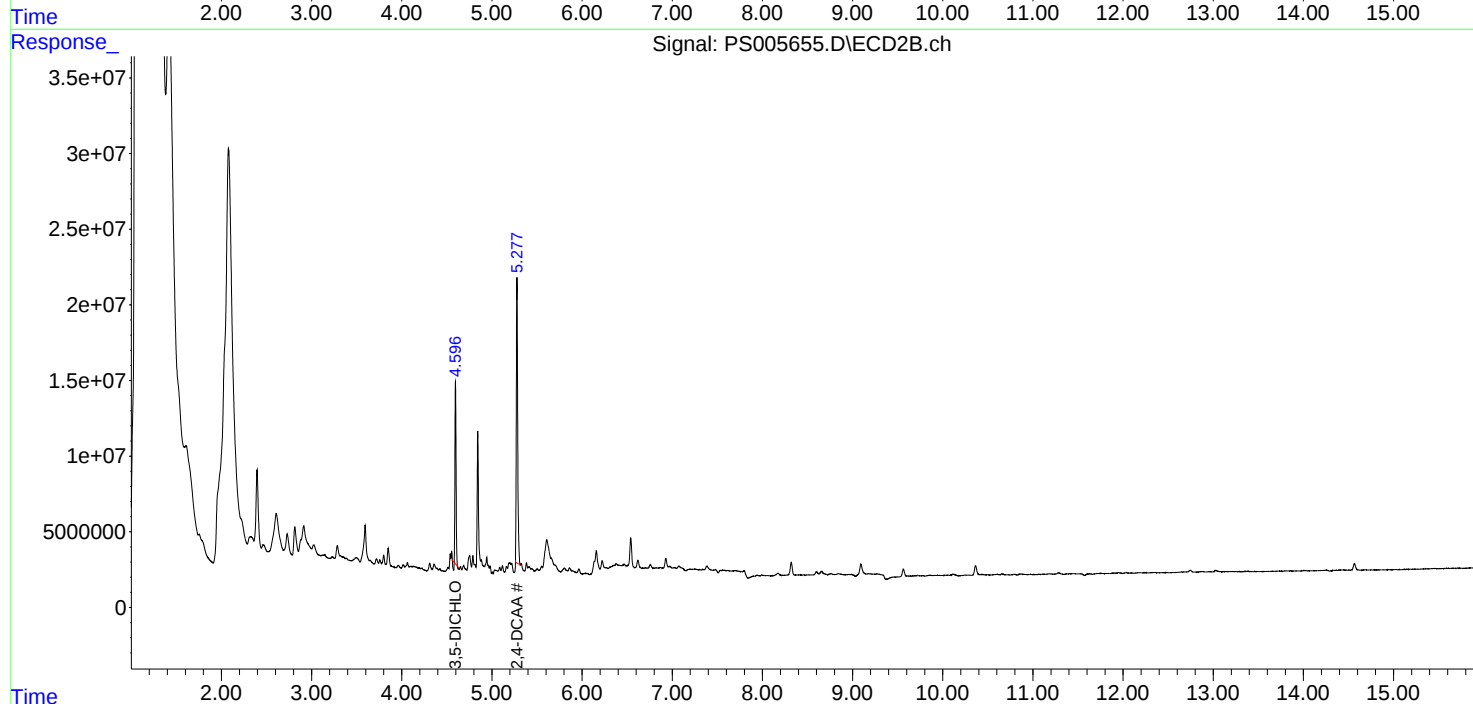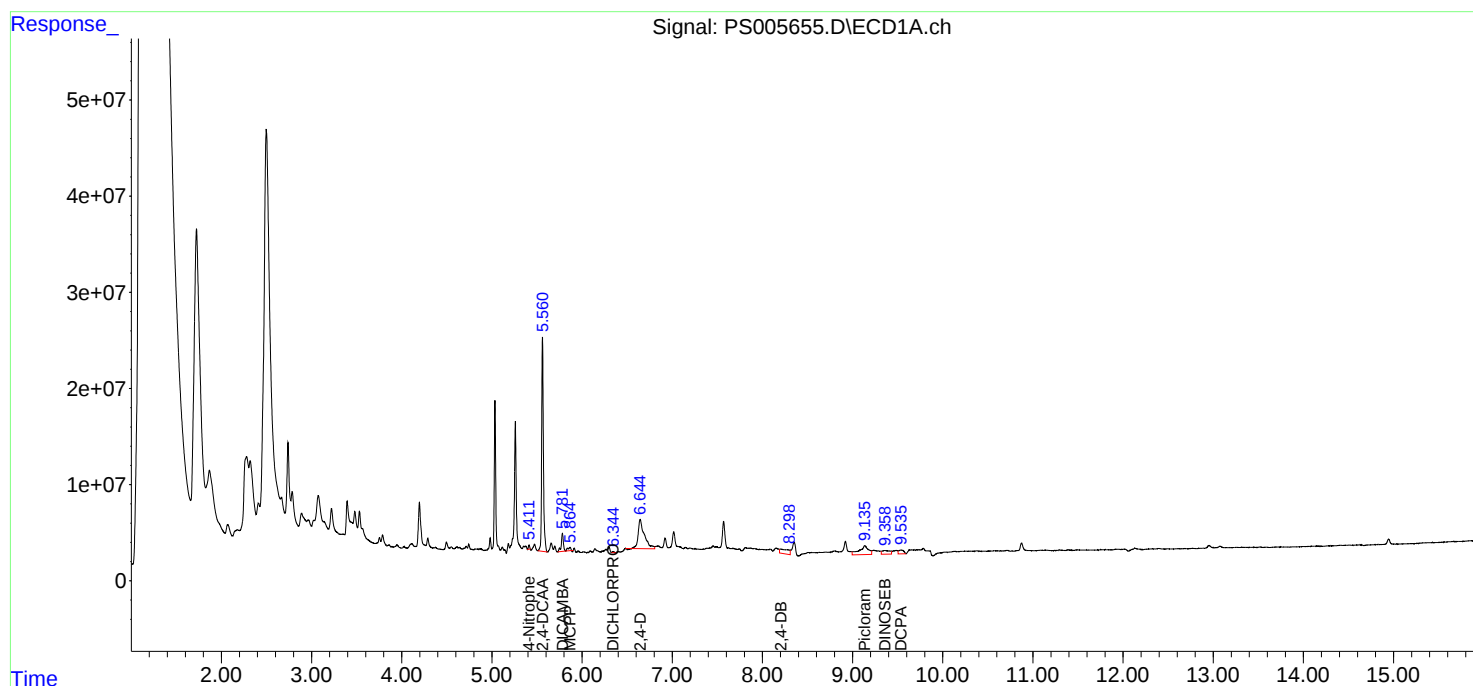


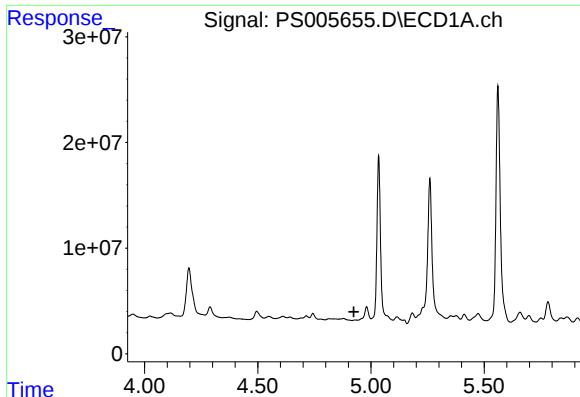

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.876 min
Delta R.T.: -0.048 min
Response: -488498
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-2

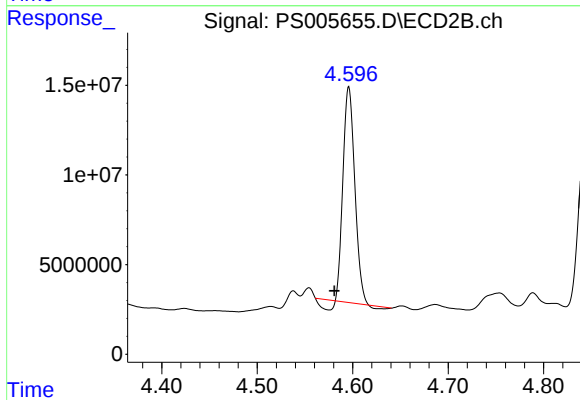


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.596 min
Delta R.T.: 0.015 min
Response: 97609680
Conc: 72.01 ng/ml

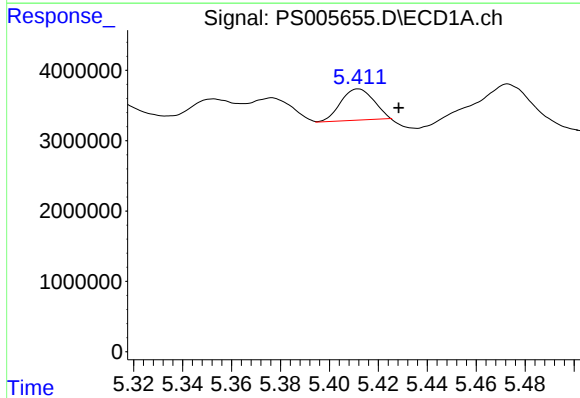


#3 4-Nitrophenol

R.T.: 5.412 min
Delta R.T.: -0.016 min
Response: 4245134
Conc: 5.94 ng/ml

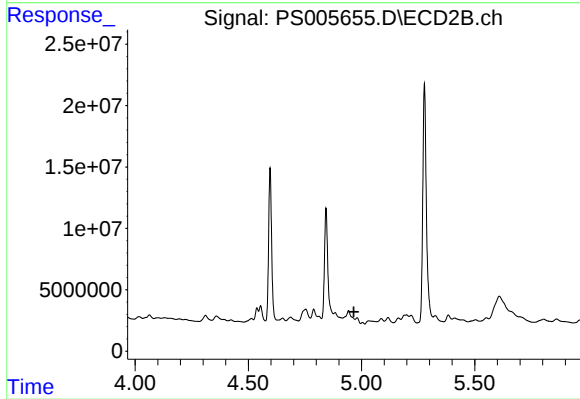

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 4.966 min
Response: 0
Conc: N.D.

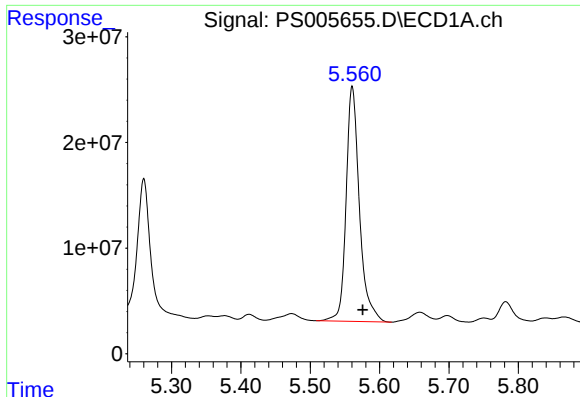

#4 2,4-DCAA


R.T.: 5.561 min
Delta R.T.: -0.015 min
Response: 297264724
Conc: 188.65 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-2

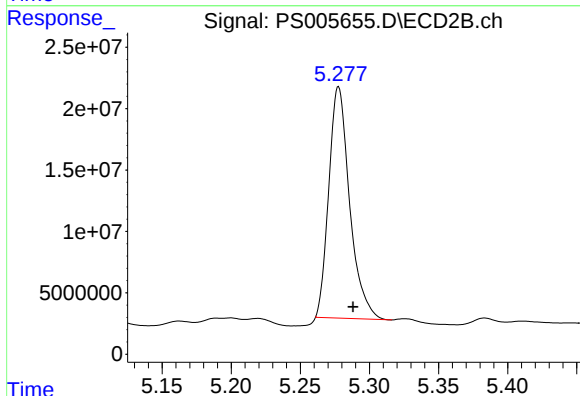


#4 2,4-DCAA

R.T.: 5.278 min
Delta R.T.: -0.010 min
Response: 197824760
Conc: 191.52 ng/ml

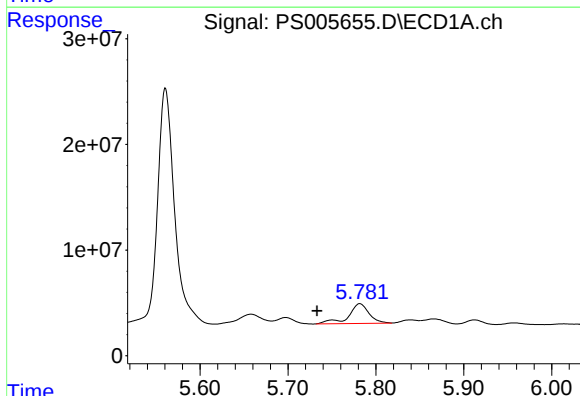


#5 DICAMBA

R.T.: 5.782 min
Delta R.T.: 0.049 min
Response: 29918984
Conc: 4.84 ng/ml

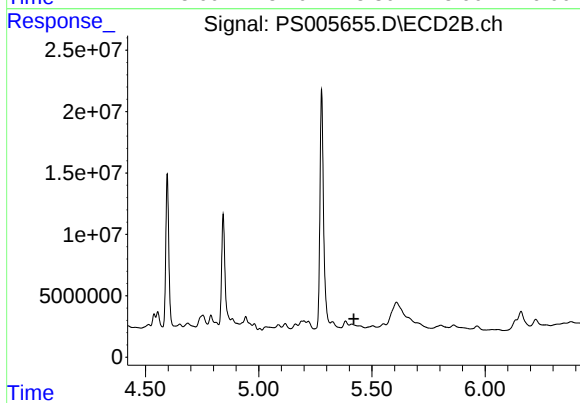

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.420 min
Response: 0
Conc: N.D.

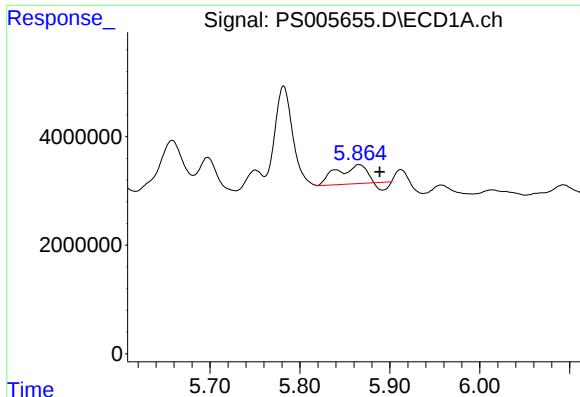

#6 MCP


R.T.: 5.865 min
Delta R.T.: -0.024 min
Response: 7139737
Conc: 1.47 ug/ml

Instrument :
ECD_S
ClientSampleId :
TP-2

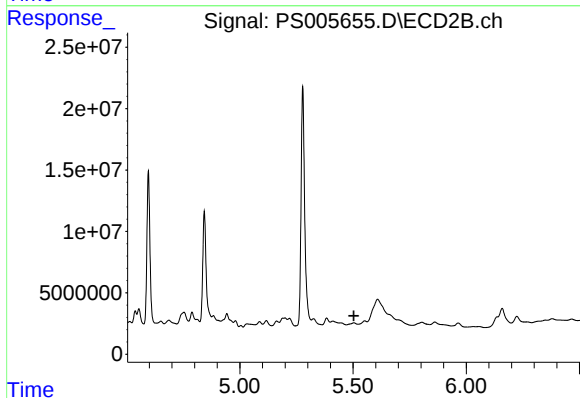


#6 MCP

R.T.: 0.000 min
Exp R.T. : 5.504 min
Response: 0
Conc: N.D.

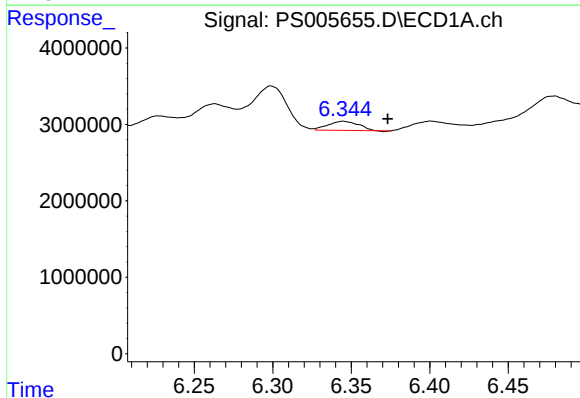


#8 DICHLORPROP

R.T.: 6.345 min
Delta R.T.: -0.028 min
Response: 1527049
Conc: 1.00 ng/ml

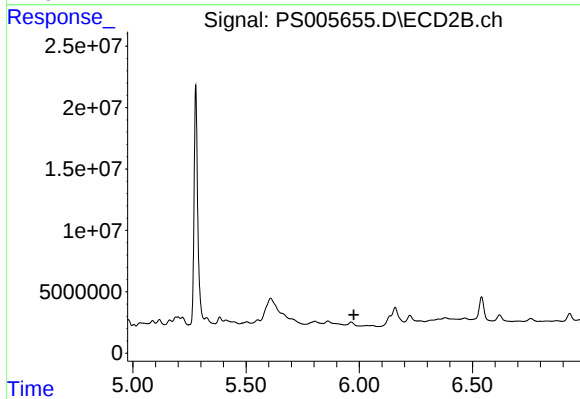

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 5.976 min
Response: 0
Conc: N.D.

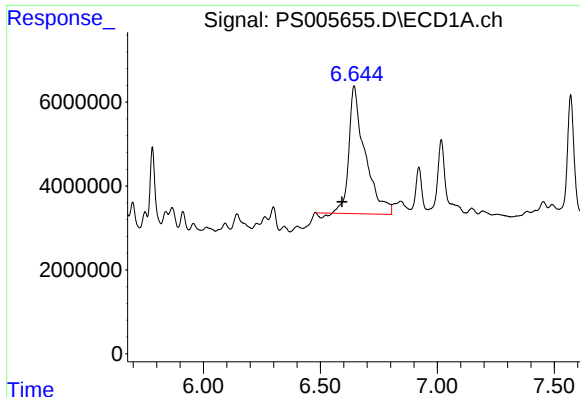

#9 2,4-D


R.T.: 6.644 min
Delta R.T.: 0.051 min
Response: 144519117
Conc: 82.41 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-2

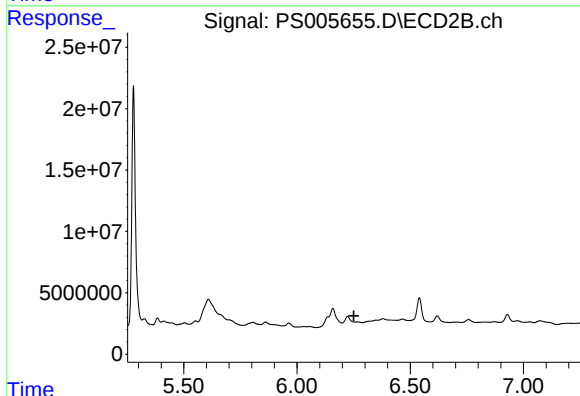


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.251 min
Response: 0
Conc: N.D.

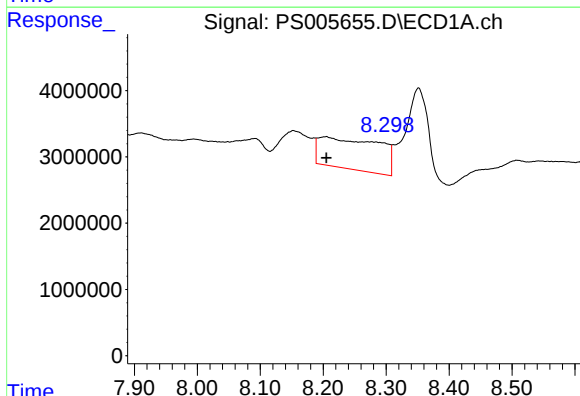


#13 2,4-DB

R.T.: 8.203 min
Delta R.T.: -0.002 min
Response: 31170635
Conc: 24.88 ng/ml

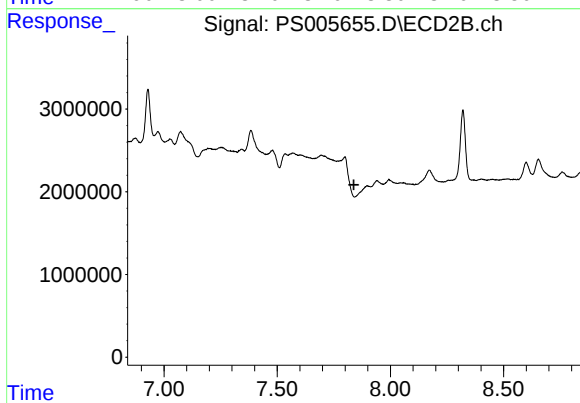

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.

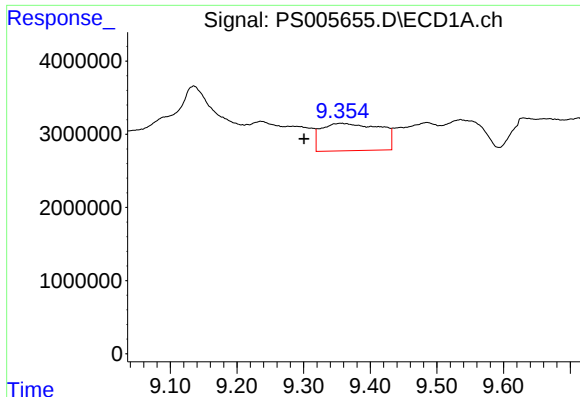

#14 DINOSEB


R.T.: 9.356 min
Delta R.T.: 0.056 min
Response: 22879006
Conc: 3.28 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-2

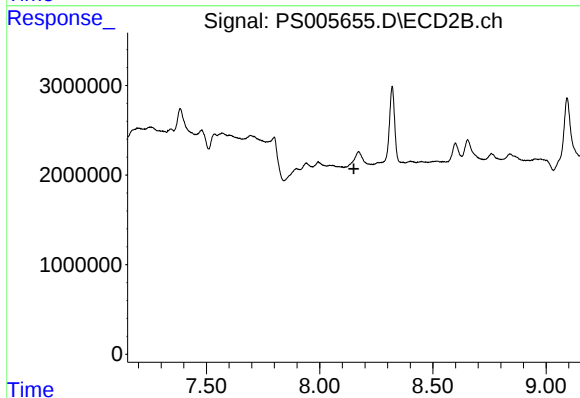


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 8.151 min
Response: 0
Conc: N.D.

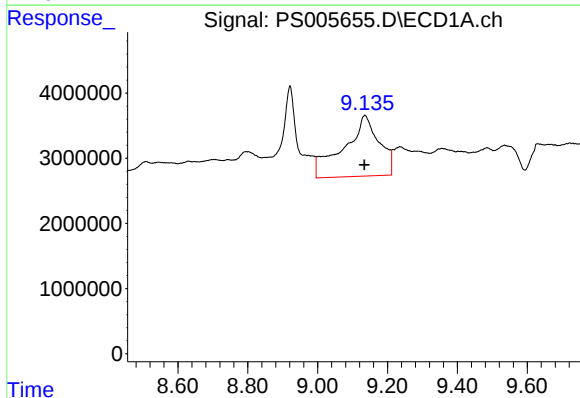


#15 Picloram

R.T.: 9.136 min
Delta R.T.: 0.002 min
Response: 65547930
Conc: 5.26 ng/ml

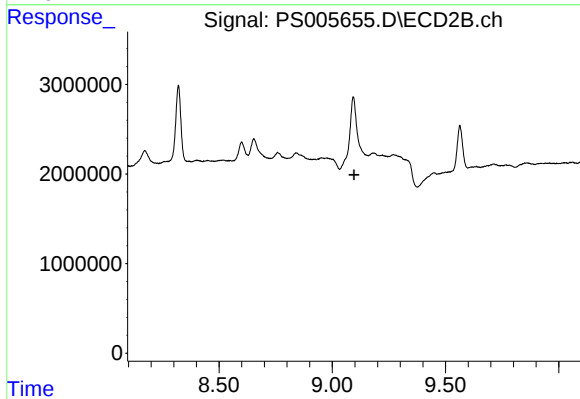

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 9.096 min
Response: 0
Conc: N.D.

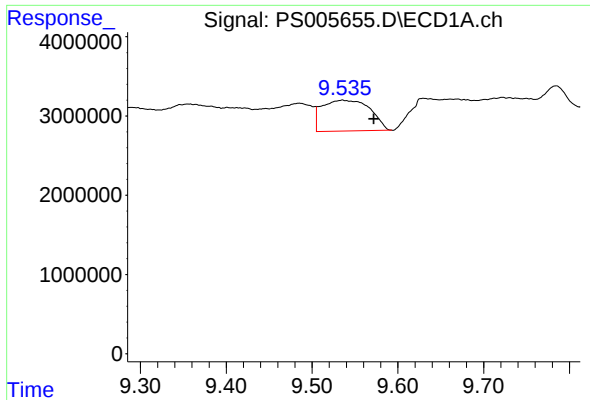

#16 DCPA

R.T.: 9.536 min
Delta R.T.: -0.036 min
Response: 15131626
Conc: 1.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-2

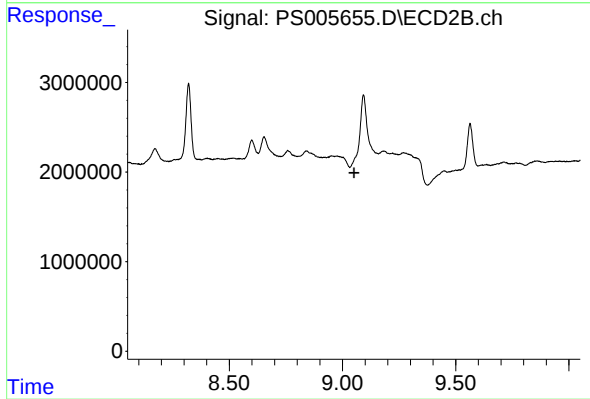

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.051 min
Response: 0
Conc: N.D.