

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072319\
 Data File : PS005656.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2019 18:08
 Operator : SM\AJ
 Sample : K3868-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 00:50:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 19 08:54:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.566	5.283	276.2E6	186.9E6	175.255	180.930
Target Compounds							
2) T	3,5-DICHL...	4.881	4.600	2807014	63640120	1.319	46.951 #
3) T	4-Nitroph...	5.417	0.000	2419890	0	3.385	N.D. #
5) T	DICAMBA	5.755	0.000	6214215	0	1.005	N.D. #
6) T	MCP	5.871	0.000	8264954	0	1.702	N.D. #
8) T	DICHLORPROP	6.351	0.000	1297826	0	<MDL	N.D. #
9) T	2,4-D	6.649	0.000	189.1E6	0	107.816	N.D. #
10) T	Pentachlo...	6.844	0.000	12299068	0	<MDL	N.D. #
11) T	2,4,5-TP ...	7.458	0.000	5802343	0	<MDL	N.D. #
13) T	2,4-DB	8.206	0.000	2440888	0	1.949	N.D. #
14) T	DINOSEB	9.245	0.000	26496973	0	3.799	N.D. #
15) T	Picloram	9.142	0.000	60114548	0	4.825	N.D. #
16) T	DCPA	9.536	0.000	15902410	0	1.460	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072319\
Data File : PS005656.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2019 18:08
Operator : SM\AJ
Sample : K3868-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
TP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 00:50:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
Quant Title : 8080.M
QLast Update : Fri Jul 19 08:54:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

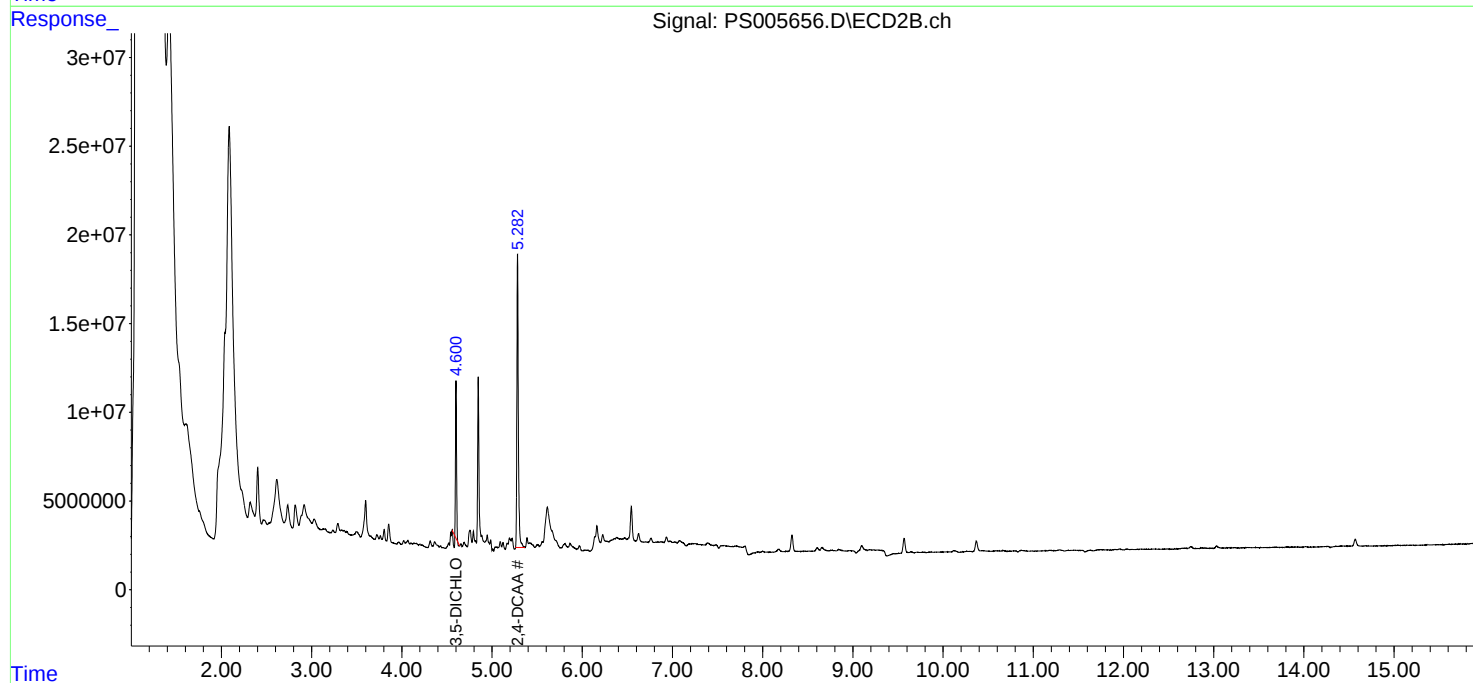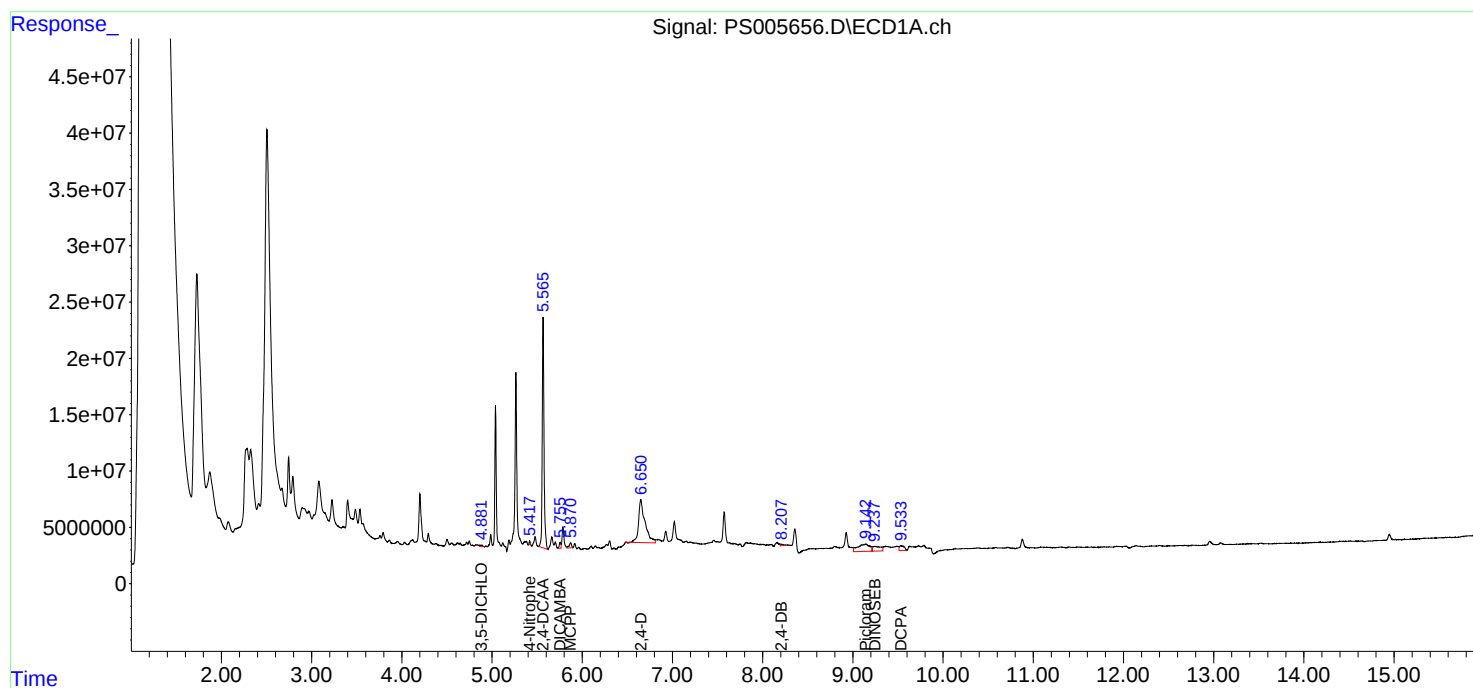


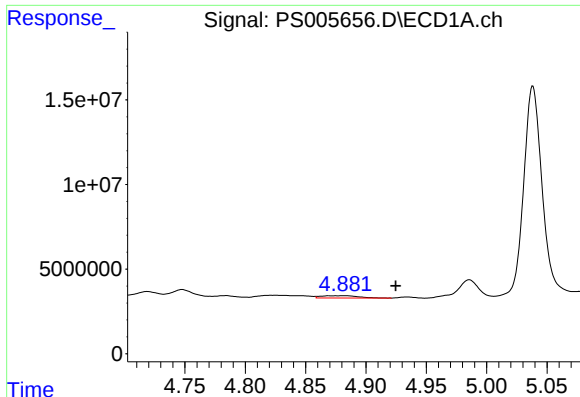

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.881 min
Delta R.T.: -0.044 min
Response: 2807014
Conc: 1.32 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

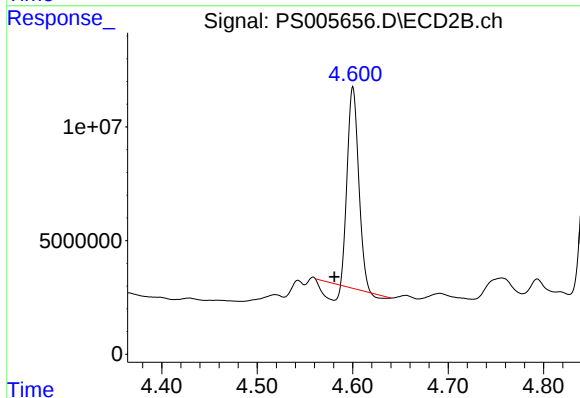


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.600 min
Delta R.T.: 0.019 min
Response: 63640120
Conc: 46.95 ng/ml

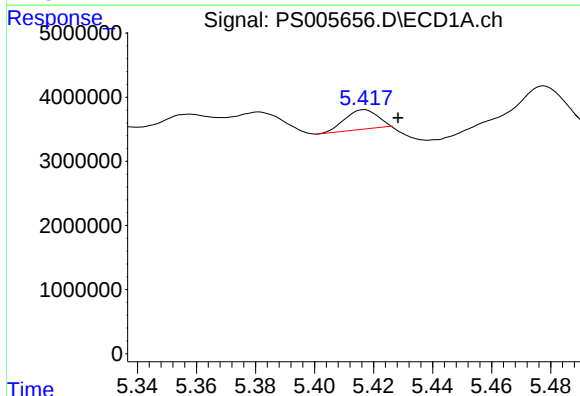


#3 4-Nitrophenol

R.T.: 5.417 min
Delta R.T.: -0.012 min
Response: 2419890
Conc: 3.39 ng/ml

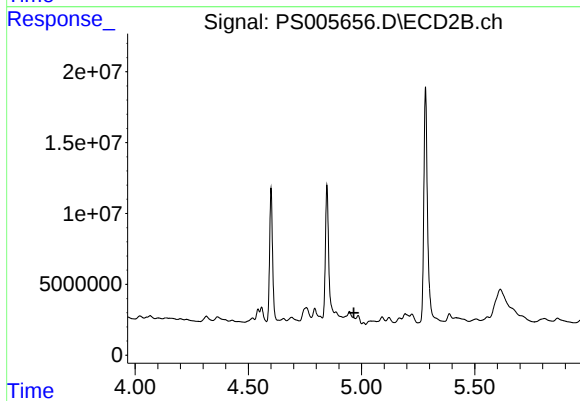

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 4.966 min
Response: 0
Conc: N.D.

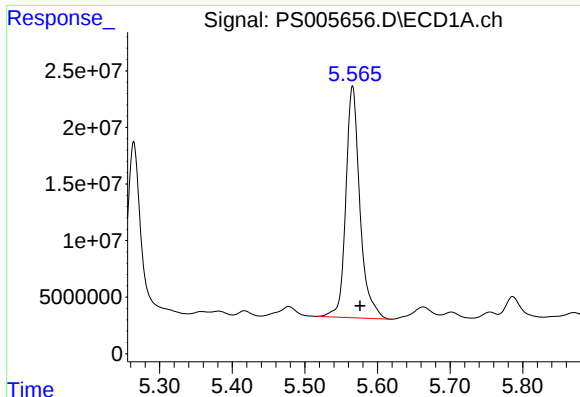

#4 2,4-DCAA


R.T.: 5.566 min
Delta R.T.: -0.010 min
Response: 276159229
Conc: 175.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

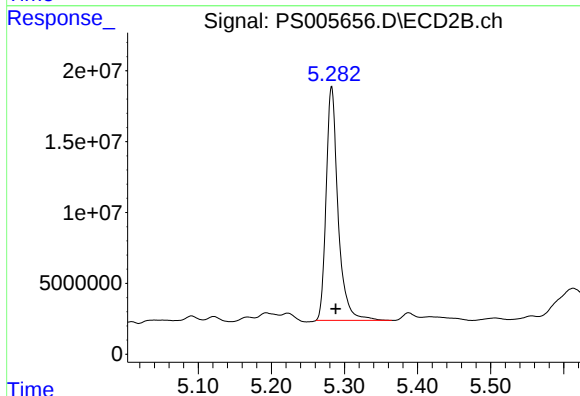


#4 2,4-DCAA

R.T.: 5.283 min
Delta R.T.: -0.005 min
Response: 186882965
Conc: 180.93 ng/ml

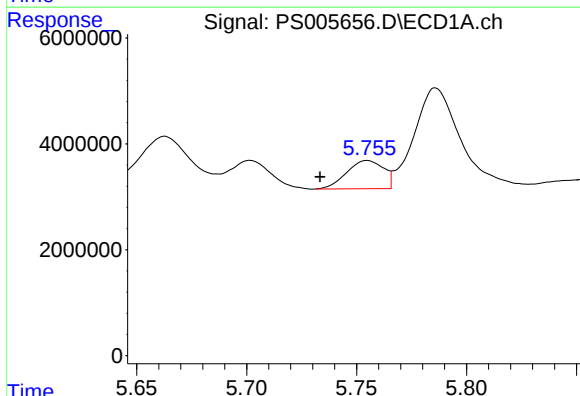


#5 DICAMBA

R.T.: 5.755 min
Delta R.T.: 0.022 min
Response: 6214215
Conc: 1.00 ng/ml

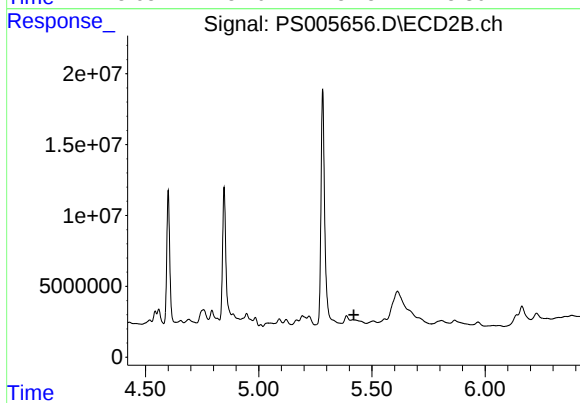

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.420 min
Response: 0
Conc: N.D.

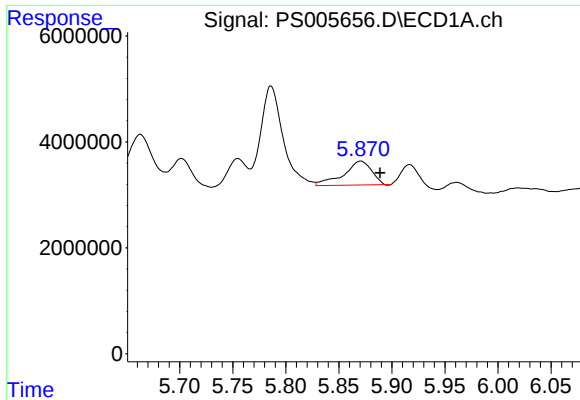

#6 MCP


R.T.: 5.871 min
Delta R.T.: -0.018 min
Response: 8264954
Conc: 1.70 ug/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

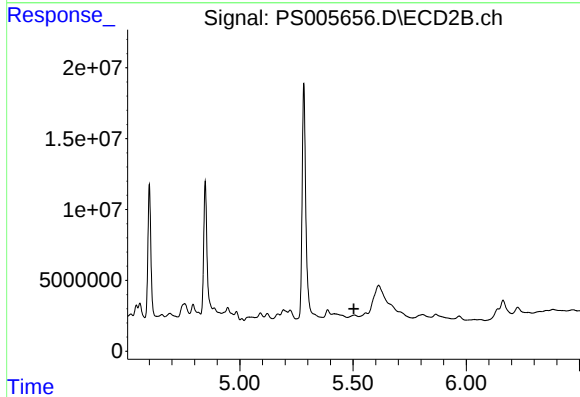


#6 MCP

R.T.: 0.000 min
Exp R.T.: 5.504 min
Response: 0
Conc: N.D.

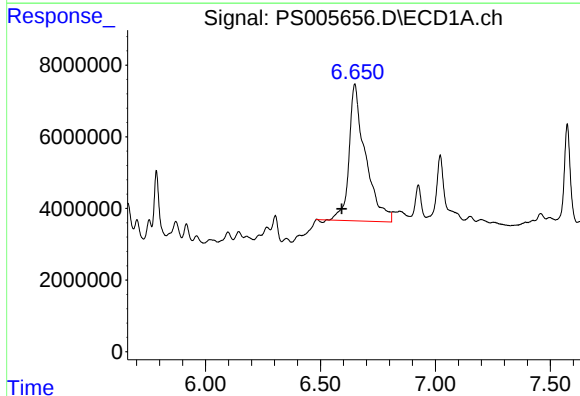


#9 2,4-D

R.T.: 6.649 min
Delta R.T.: 0.056 min
Response: 189075512
Conc: 107.82 ng/ml

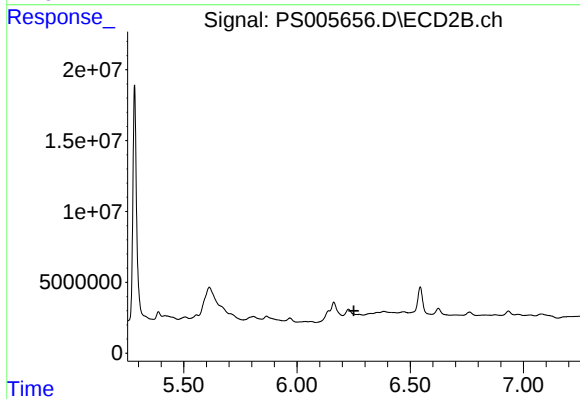

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.251 min
Response: 0
Conc: N.D.

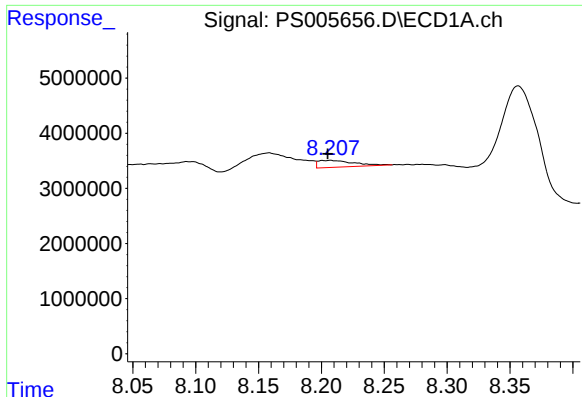

#13 2,4-DB


R.T.: 8.206 min
Delta R.T.: 0.000 min
Response: 2440888
Conc: 1.95 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

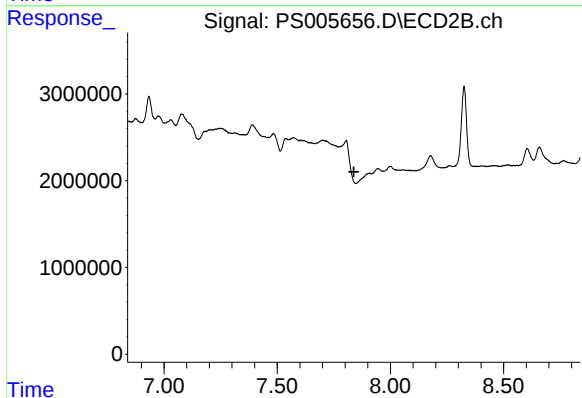


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.

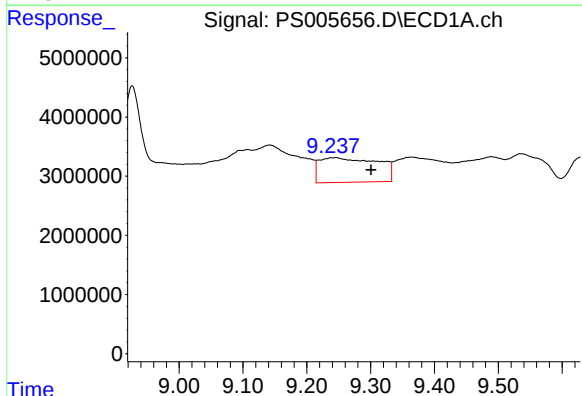


#14 DINOSEB

R.T.: 9.245 min
Delta R.T.: -0.055 min
Response: 26496973
Conc: 3.80 ng/ml

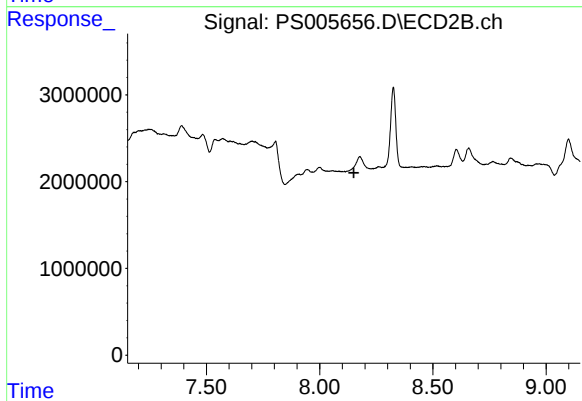

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 8.151 min
Response: 0
Conc: N.D.

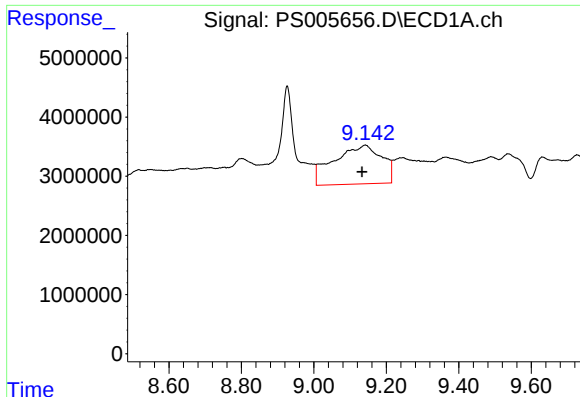

#15 Picloram


R.T.: 9.142 min
Delta R.T.: 0.009 min
Response: 60114548
Conc: 4.83 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

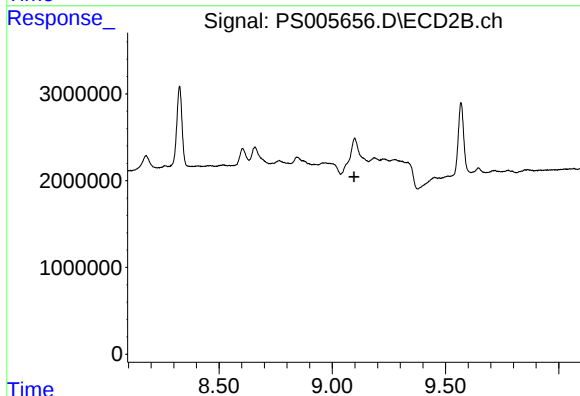


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.096 min
Response: 0
Conc: N.D.

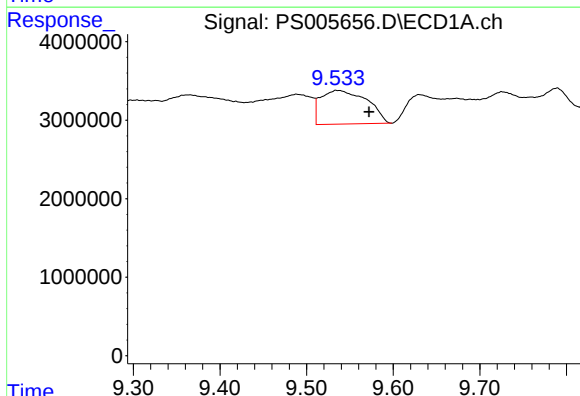

#16 DCPA

R.T.: 9.536 min
Delta R.T.: -0.036 min
Response: 15902410
Conc: 1.46 ng/ml

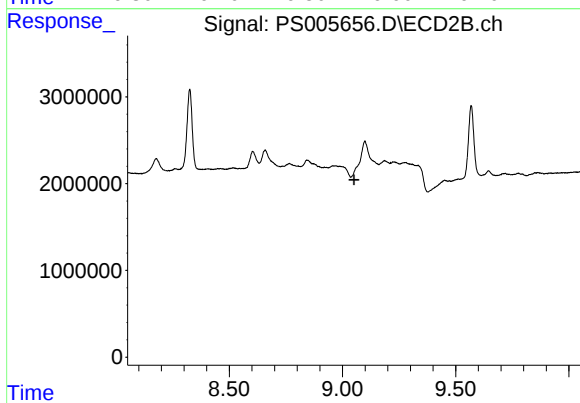

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.051 min
Response: 0
Conc: N.D.