

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072319\
 Data File : PS005664.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2019 21:05
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 00:53:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 19 08:54:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.576	5.293	563.0E6	369.6E6	357.306	357.817
Target Compounds							
2) T	3,5-DICHL...	4.946	0.000	995223	0	<MDL	N.D. #
3) T	4-Nitroph...	5.409	0.000	1180215	0	1.651	N.D. #
6) T	MCP	5.920	0.000	1437580	0	<MDL	N.D. #
7) T	MCPA	0.000	5.626	0	110.3E6	N.D.	25.041
9) T	2,4-D	6.660	0.000	202.8E6	0	115.642	N.D. #
10) T	Pentachlo...	6.863	0.000	10379585	0	<MDL	N.D. #
11) T	2,4,5-TP ...	7.402	0.000	3593508	0	<MDL	N.D. #
12) T	2,4,5-T	7.705	0.000	6689196	0	<MDL	N.D. #
14) T	DINOSEB	9.301	0.000	4225782	0	<MDL	N.D. #
15) T	Picloram	9.189	0.000	17513342	0	1.406	N.D. #
16) T	DCPA	9.573	0.000	3797634	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072319\
Data File : PS005664.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2019 21:05
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 00:53:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
Quant Title : 8080.M
QLast Update : Fri Jul 19 08:54:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

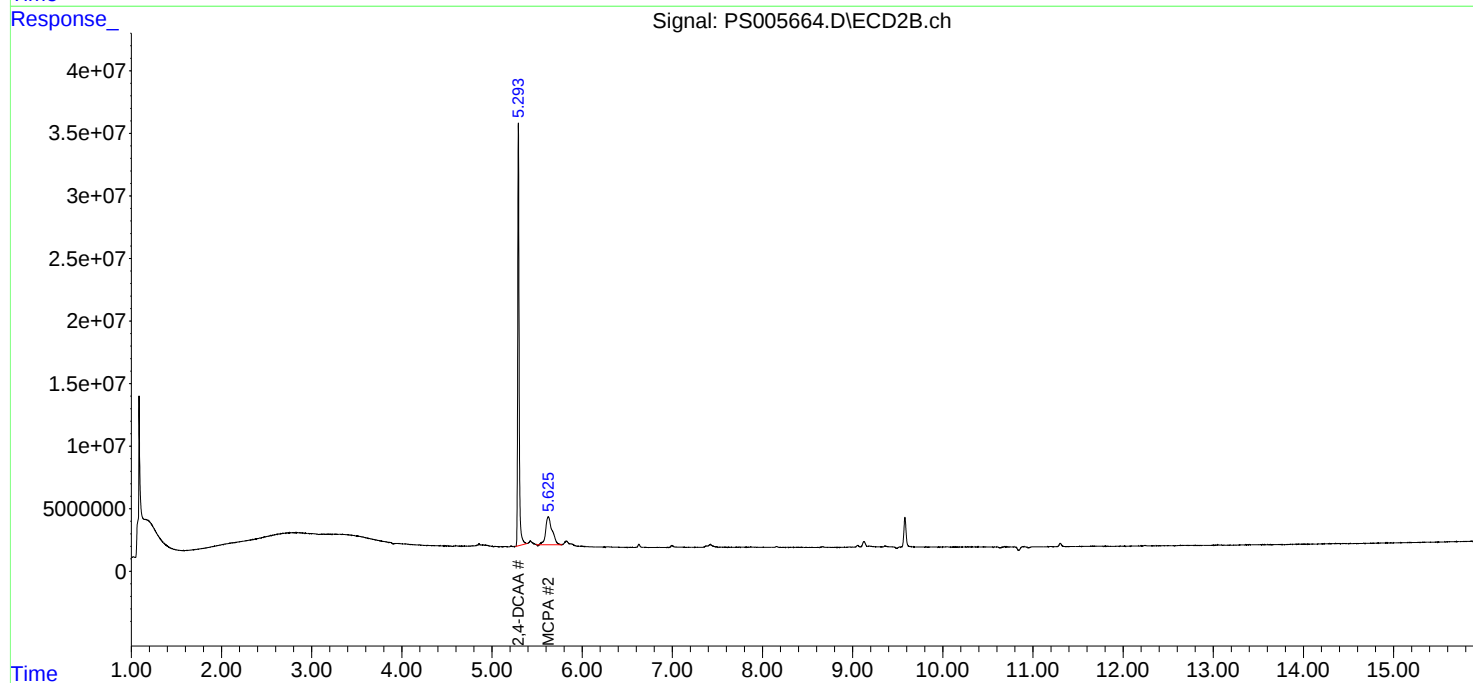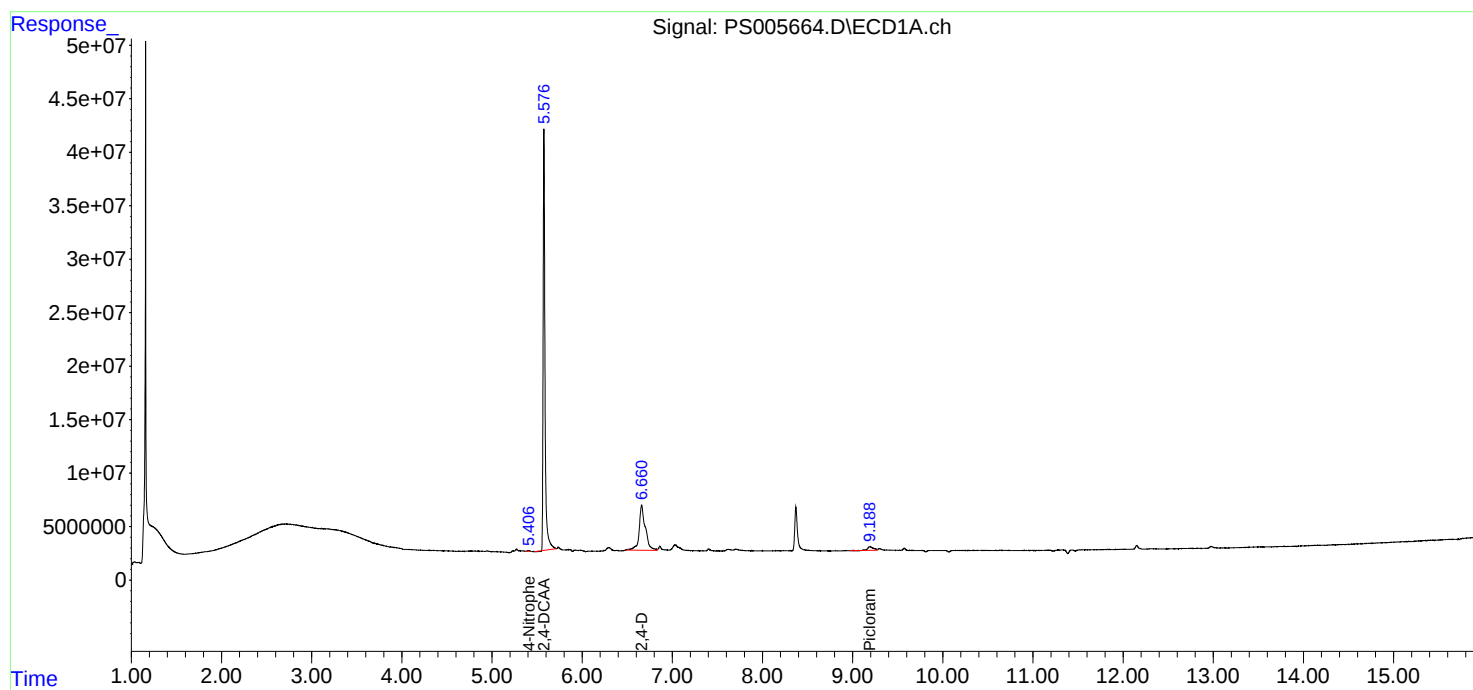


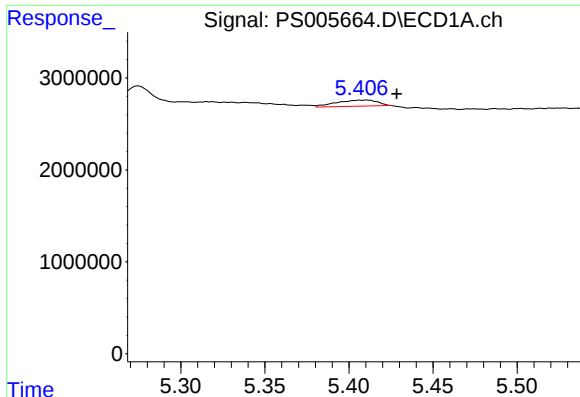

#3 4-Nitrophenol


R.T.: 5.409 min
Delta R.T.: -0.020 min
Response: 1180215
Conc: 1.65 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

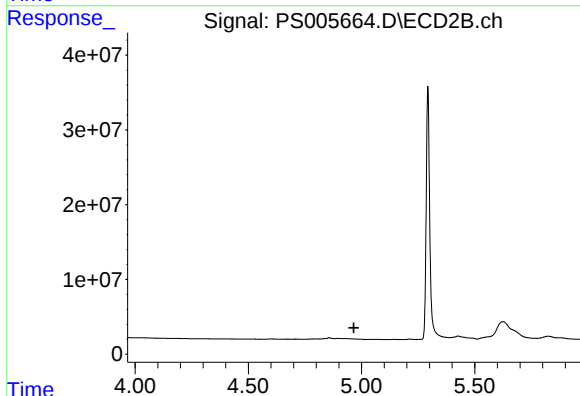


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 4.966 min
Response: 0
Conc: N.D.

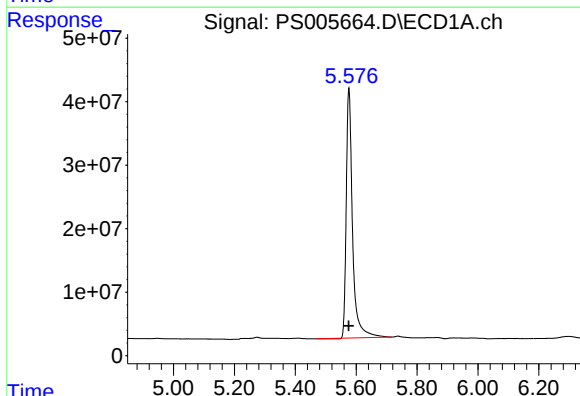


#4 2,4-DCAA

R.T.: 5.576 min
Delta R.T.: 0.000 min
Response: 563026077
Conc: 357.31 ng/ml

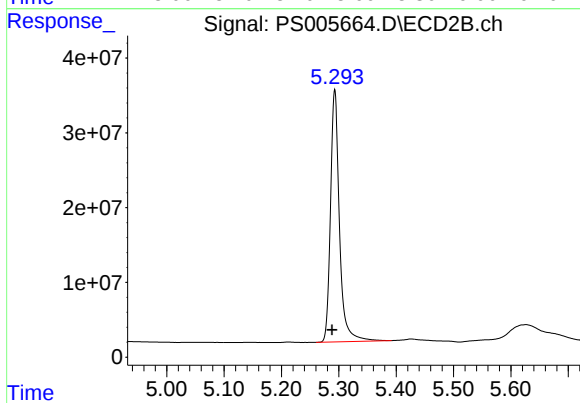

#4 2,4-DCAA


R.T.: 5.293 min
Delta R.T.: 0.005 min
Response: 369589742
Conc: 357.82 ng/ml

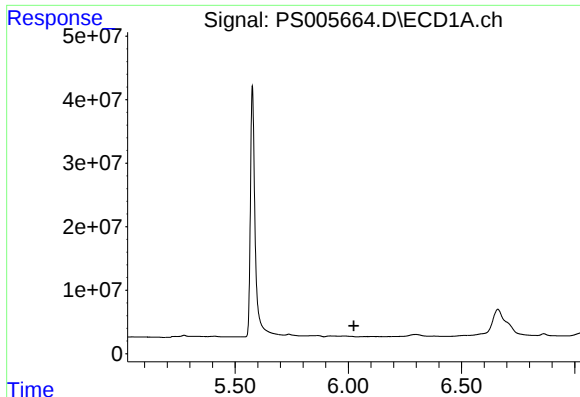

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.024 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

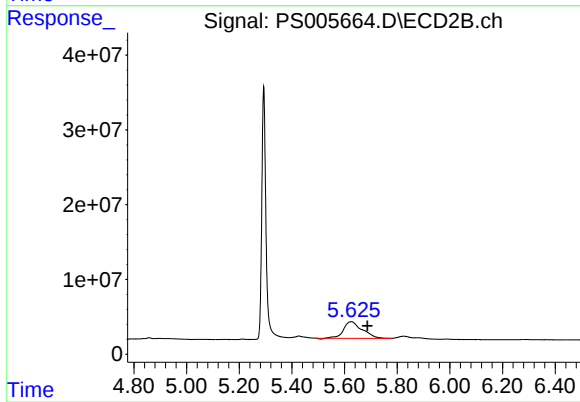


#7 MCPA

R.T.: 5.626 min
Delta R.T.: -0.061 min
Response: 110333804
Conc: 25.04 ug/ml

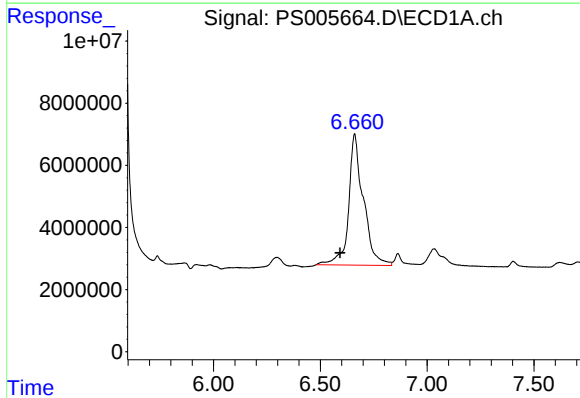


#9 2,4-D

R.T.: 6.660 min
Delta R.T.: 0.067 min
Response: 202799434
Conc: 115.64 ng/ml

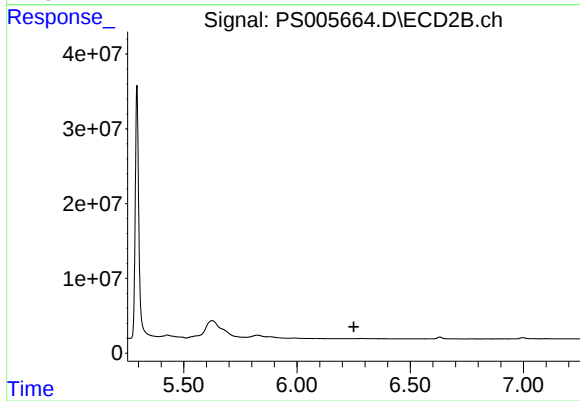

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.251 min
Response: 0
Conc: N.D.

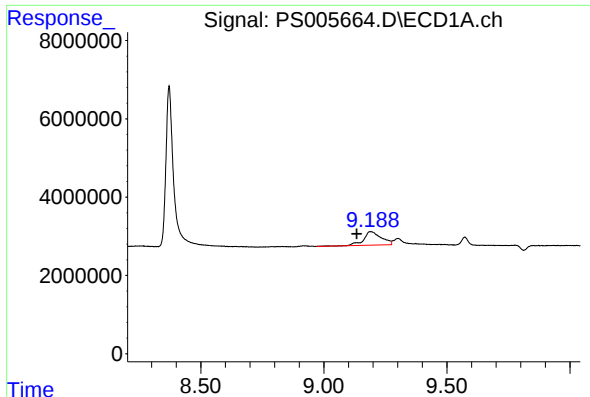

#15 Picloram

R.T.: 9.189 min
Delta R.T.: 0.056 min
Response: 17513342
Conc: 1.41 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

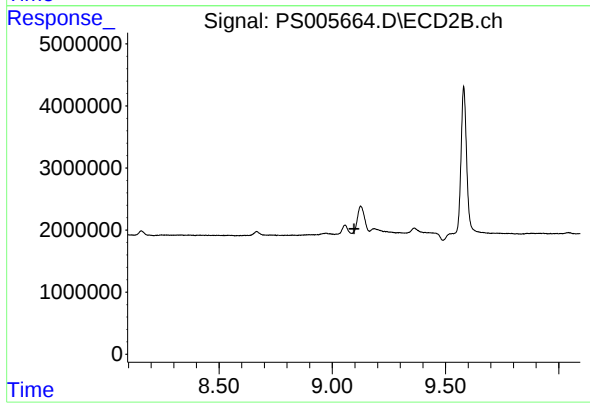

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.096 min
Response: 0
Conc: N.D.