

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072319\
 Data File : PS005667.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2019 22:11
 Operator : SM\AJ
 Sample : K3618-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HD-02-072219

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 00:54:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 19 08:54:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.560	5.277	331.1E6	207.1E6	210.146	200.480
Target Compounds							
2) T	3,5-DICHL...	4.981	4.596	11920093	96002491	5.602	70.826 #
3) T	4-Nitroph...	5.411	0.000	6413157	0	8.971	N.D. #
5) T	DICAMBA	5.696	0.000	8612107	0	1.392	N.D. #
6) T	MCP	5.867	0.000	7639112	0	1.573	N.D. #
8) T	DICHLORPROP	6.346	0.000	1026546	0	<MDL	N.D. #
9) T	2,4-D	6.644	6.222	212.8E6	18958398	121.359	16.236 #
10) T	Pentachlo...	6.840	0.000	18309358	0	<MDL	N.D. #
11) T	2,4,5-TP ...	7.384	0.000	1355345	0	<MDL	N.D. #
12) T	2,4,5-T	7.663	0.000	5623592	0	<MDL	N.D. #
13) T	2,4-DB	8.153	0.000	21042232	0	16.798	N.D. #
14) T	DINOSEB	9.237	0.000	17733919	0	2.542	N.D. #
15) T	Picloram	9.133	0.000	40208216	0	3.227	N.D. #
16) T	DCPA	9.530	0.000	14323803	0	1.315	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072319\
Data File : PS005667.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2019 22:11
Operator : SM\AJ
Sample : K3618-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
HD-02-072219

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 00:54:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
Quant Title : 8080.M
QLast Update : Fri Jul 19 08:54:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

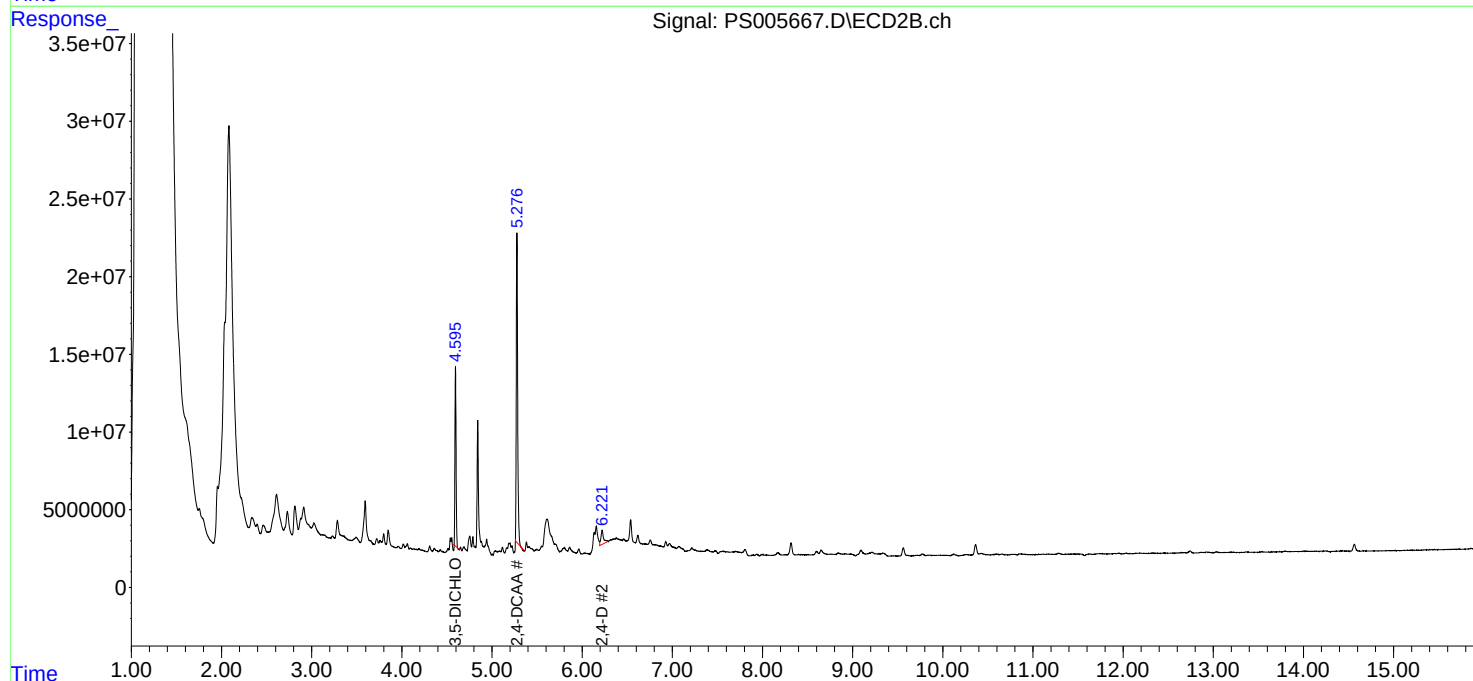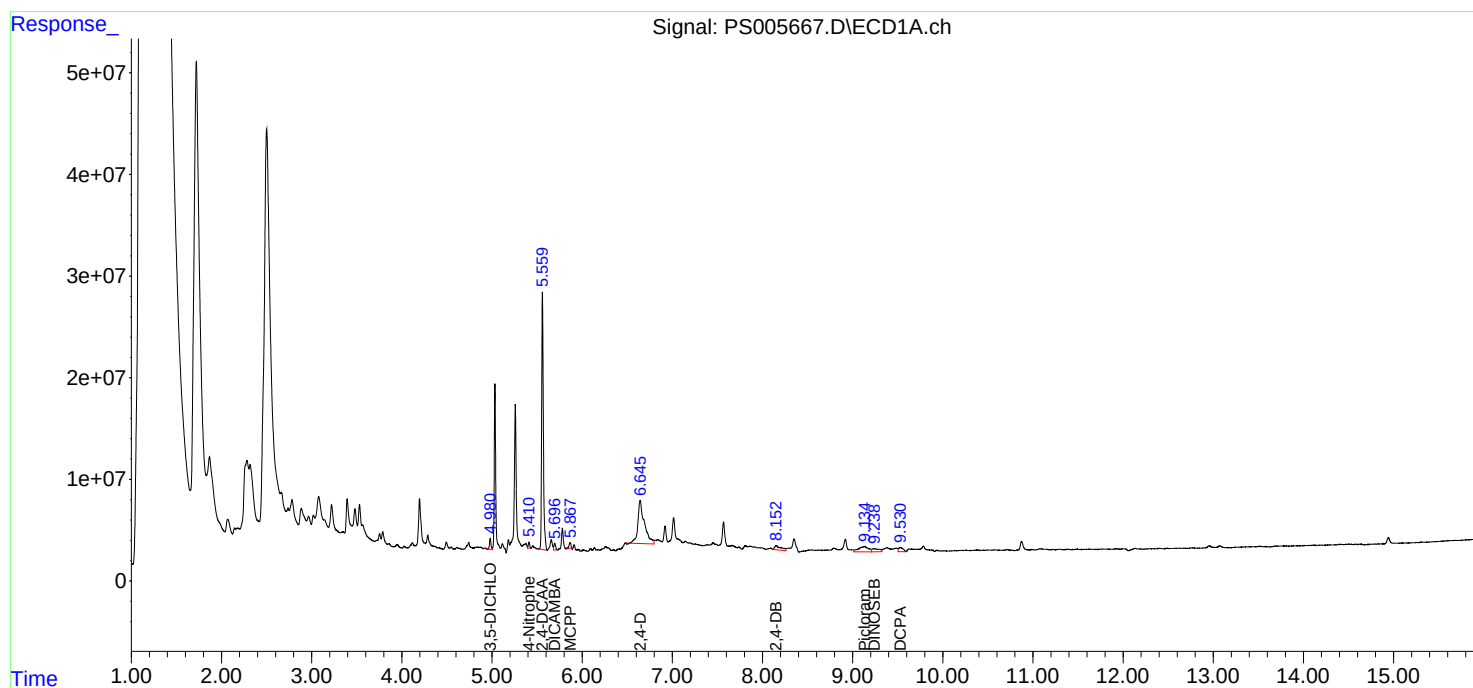


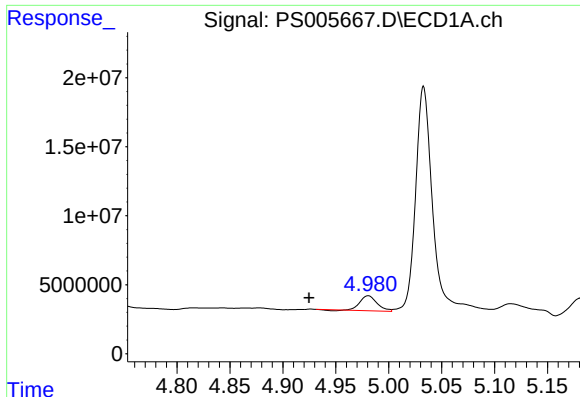

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.981 min
Delta R.T.: 0.056 min
Response: 11920093
Conc: 5.60 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-02-072219

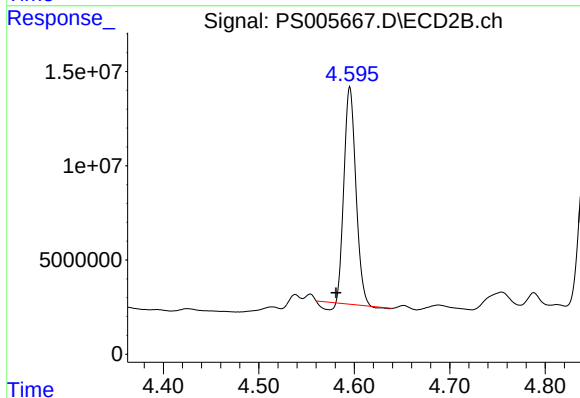


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.596 min
Delta R.T.: 0.015 min
Response: 96002491
Conc: 70.83 ng/ml

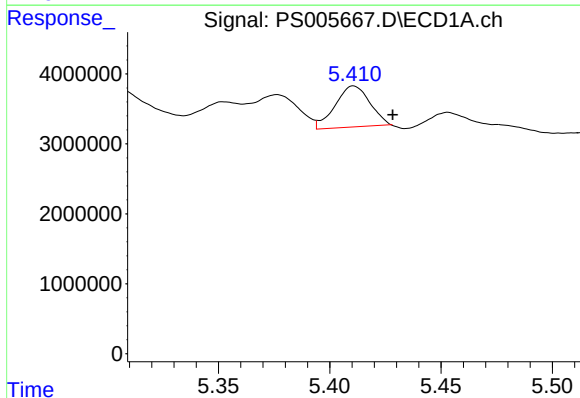


#3 4-Nitrophenol

R.T.: 5.411 min
Delta R.T.: -0.017 min
Response: 6413157
Conc: 8.97 ng/ml

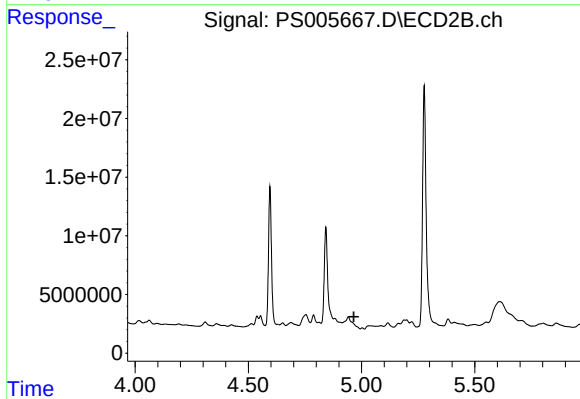

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 4.966 min
Response: 0
Conc: N.D.

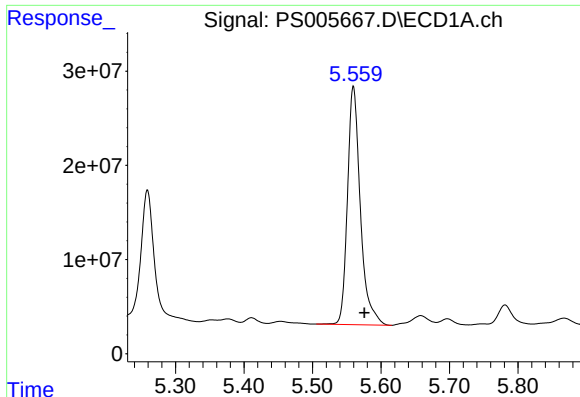

#4 2,4-DCAA


R.T.: 5.560 min
Delta R.T.: -0.016 min
Response: 331138457
Conc: 210.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-02-072219

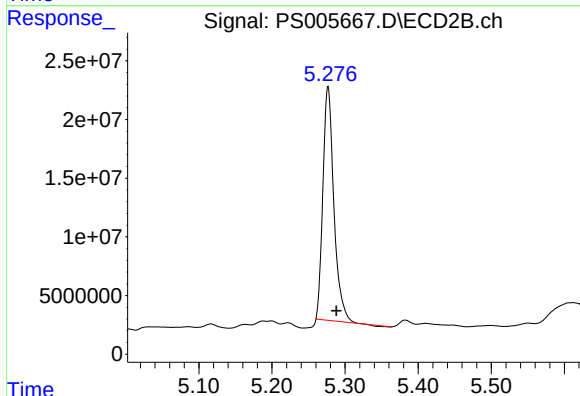


#4 2,4-DCAA

R.T.: 5.277 min
Delta R.T.: -0.011 min
Response: 207076402
Conc: 200.48 ng/ml

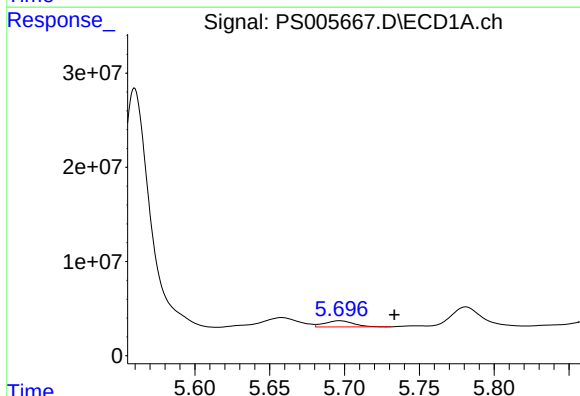


#5 DICAMBA

R.T.: 5.696 min
Delta R.T.: -0.037 min
Response: 8612107
Conc: 1.39 ng/ml

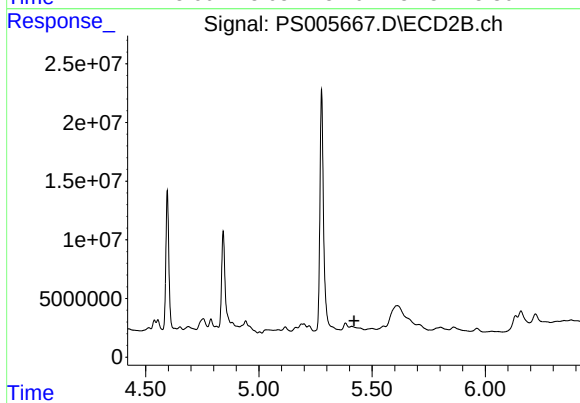

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.420 min
Response: 0
Conc: N.D.

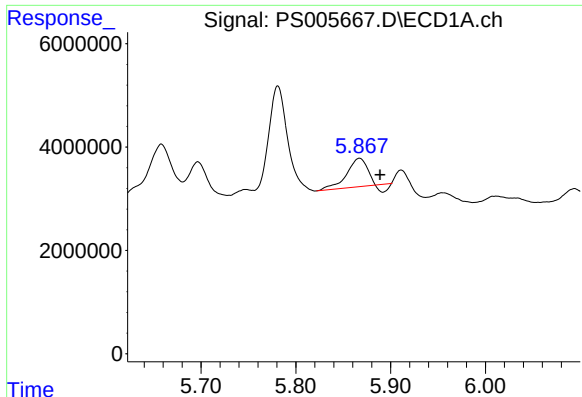

#6 MCP


R.T.: 5.867 min
Delta R.T.: -0.022 min
Response: 7639112
Conc: 1.57 ug/ml

Instrument :
ECD_S
ClientSampleId :
HD-02-072219

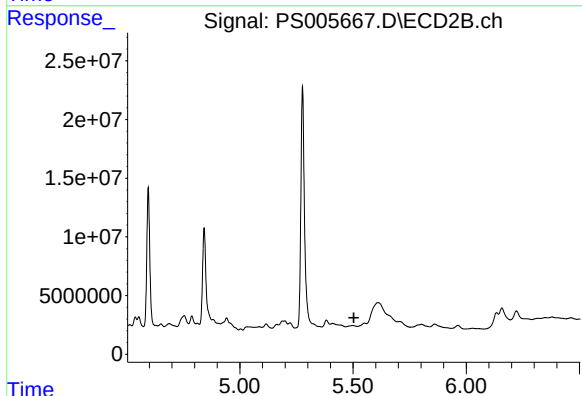


#6 MCP

R.T.: 0.000 min
Exp R.T. : 5.504 min
Response: 0
Conc: N.D.

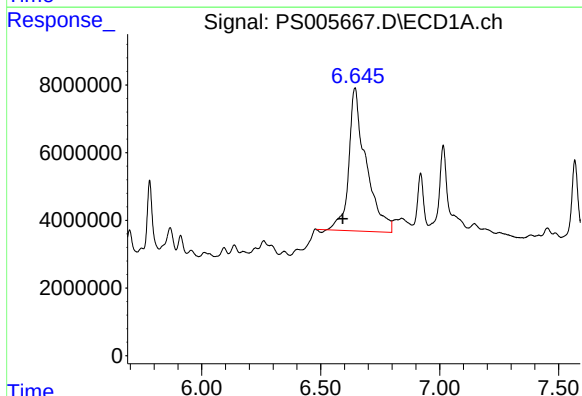


#9 2,4-D

R.T.: 6.644 min
Delta R.T.: 0.051 min
Response: 212825788
Conc: 121.36 ng/ml

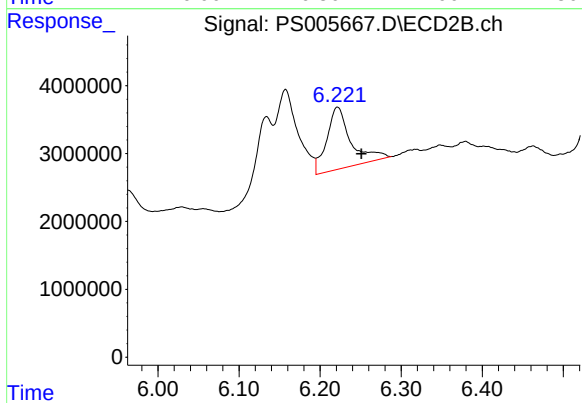

#9 2,4-D


R.T.: 6.222 min
Delta R.T.: -0.029 min
Response: 18958398
Conc: 16.24 ng/ml

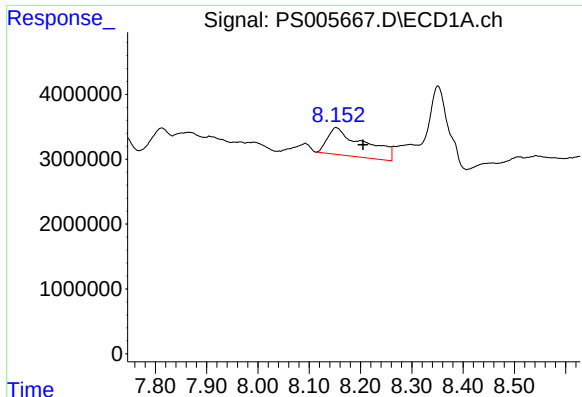

#13 2,4-DB


R.T.: 8.153 min
Delta R.T.: -0.052 min
Response: 21042232
Conc: 16.80 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-02-072219

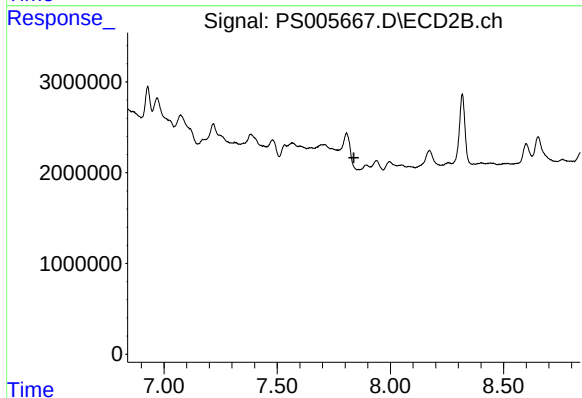


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.

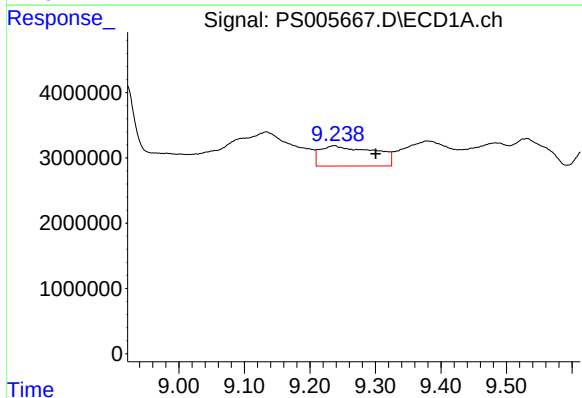


#14 DINOSEB

R.T.: 9.237 min
Delta R.T.: -0.064 min
Response: 17733919
Conc: 2.54 ng/ml

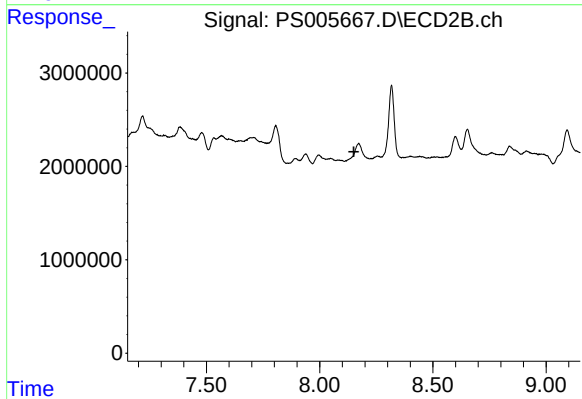

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 8.151 min
Response: 0
Conc: N.D.

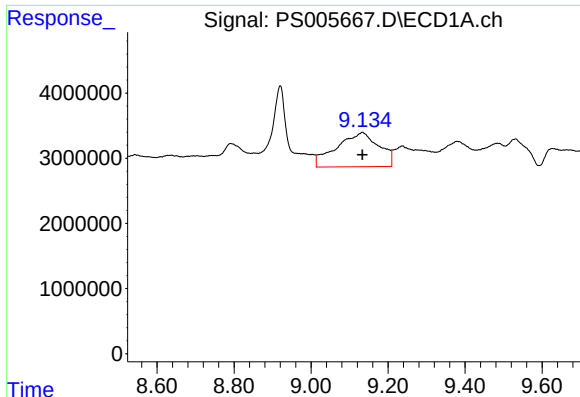

#15 Picloram


R.T.: 9.133 min
Delta R.T.: 0.000 min
Response: 40208216
Conc: 3.23 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-02-072219

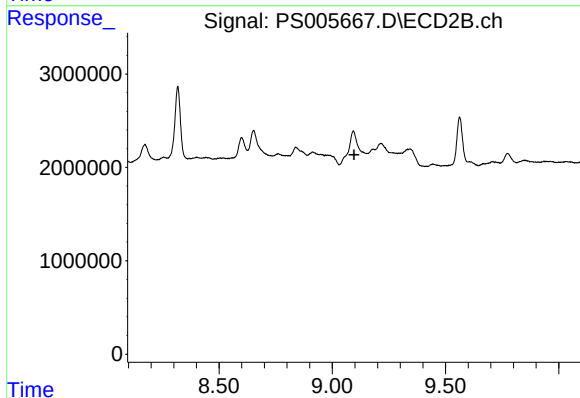


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.096 min
Response: 0
Conc: N.D.

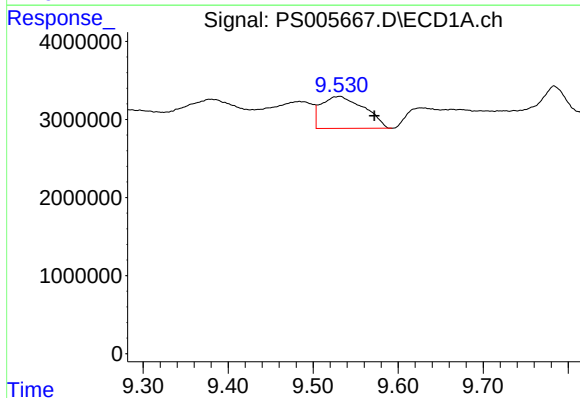

#16 DCPA

R.T.: 9.530 min
Delta R.T.: -0.042 min
Response: 14323803
Conc: 1.32 ng/ml

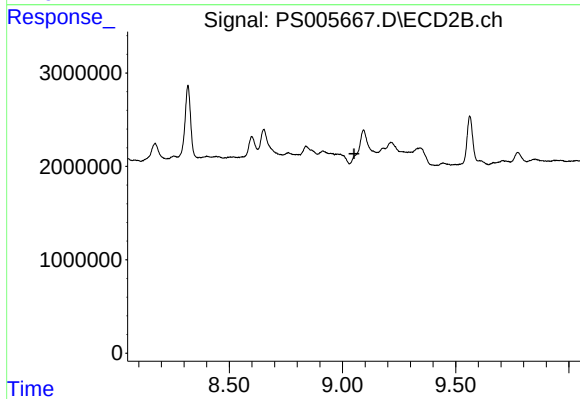

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.051 min
Response: 0
Conc: N.D.