

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072319\
 Data File : PS005671.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2019 23:39
 Operator : SM\AJ
 Sample : K3918-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 S3-02-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 00:56:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 19 08:54:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.551	0.000	239.7E6	0	152.135	N.D. #
Target Compounds							
2) T	3,5-DICHL...	4.919	4.585	-649244	70095427	N.D.	51.713
3) T	4-Nitroph...	5.402	0.000	5585246	0	7.813	N.D. #
5) T	DICAMBA	5.772	0.000	26133053	0	4.225	N.D. #
6) T	MCP	5.858	0.000	9173215	0	1.889	N.D. #
7) T	MCPA	6.001	0.000	174126	0	<MDL	N.D. #
8) T	DICHLORPROP	6.393	0.000	1211252	0	<MDL	N.D. #
9) T	2,4-D	6.634	6.211	210.1E6	11777122	119.807	10.086 #
10) T	Pentachlo...	6.834	0.000	19828830	0	<MDL	N.D. #
11) T	2,4,5-TP ...	7.443	0.000	2267836	0	<MDL	N.D. #
12) T	2,4,5-T	7.732	0.000	2332642	0	<MDL	N.D. #
13) T	2,4-DB	8.143	0.000	23844851	0	19.035	N.D. #
14) T	DINOSEB	9.347	0.000	9316711	0	1.336	N.D. #
15) T	Picloram	9.098	0.000	38394956	0	3.082	N.D. #
16) T	DCPA	9.617	0.000	5601432	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072319\
Data File : PS005671.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2019 23:39
Operator : SM\AJ
Sample : K3918-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
S3-02-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 00:56:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
Quant Title : 8080.M
QLast Update : Fri Jul 19 08:54:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

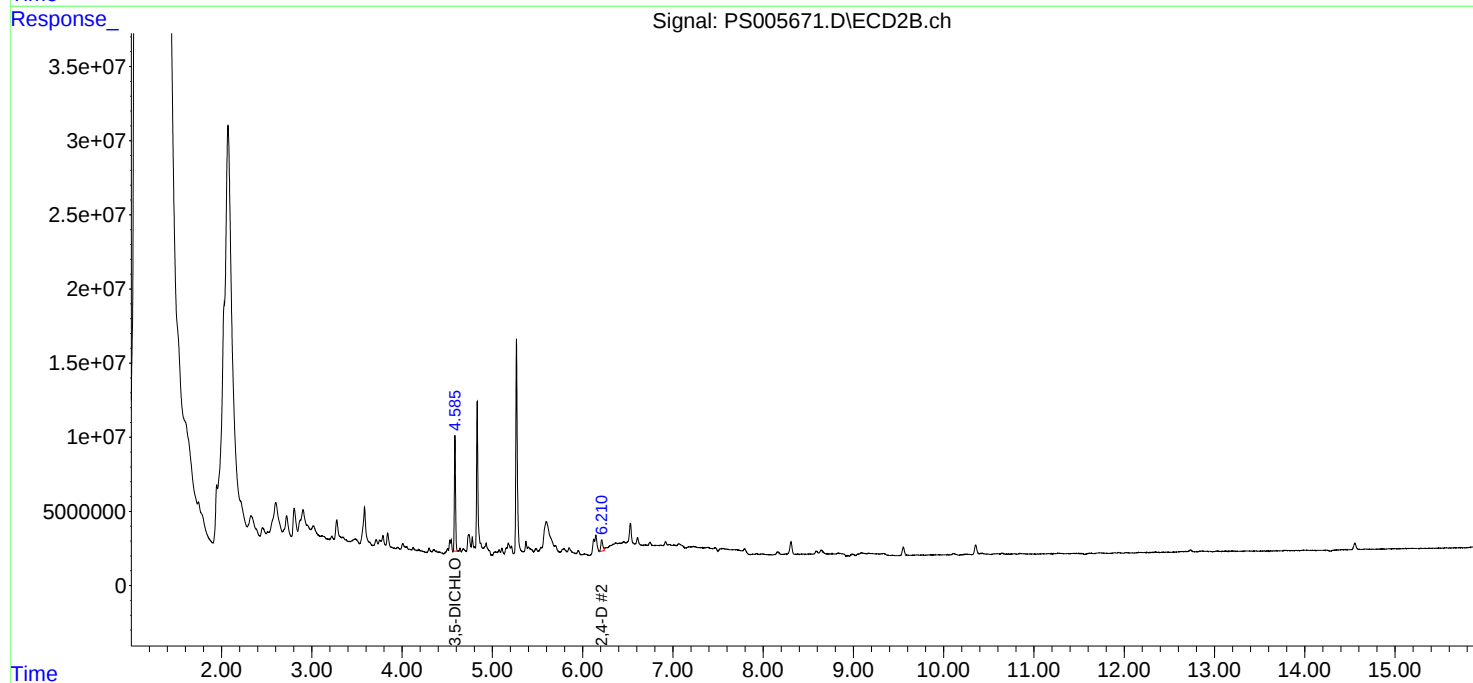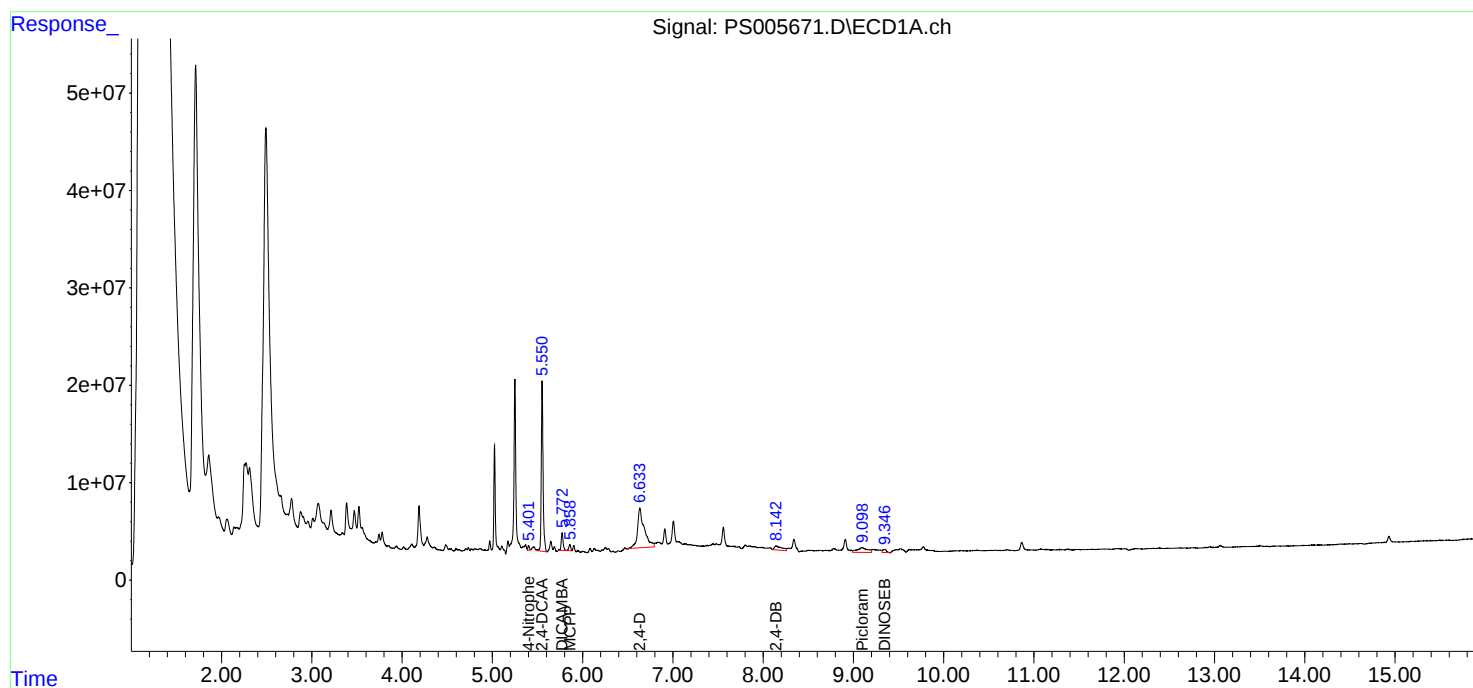


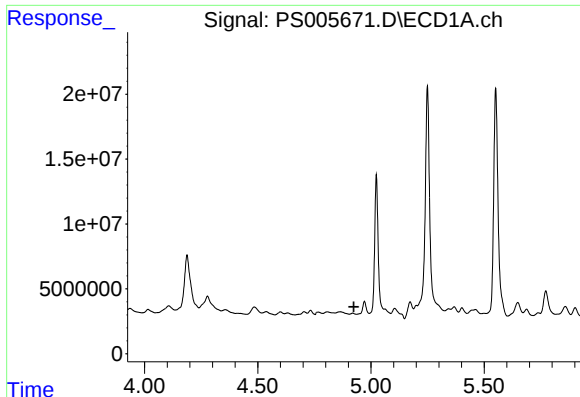

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.919 min
Delta R.T.: -0.005 min
Response: -649244
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
S3-02-B

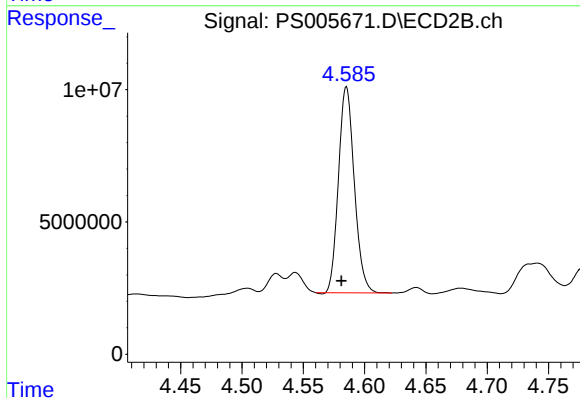


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.585 min
Delta R.T.: 0.004 min
Response: 70095427
Conc: 51.71 ng/ml

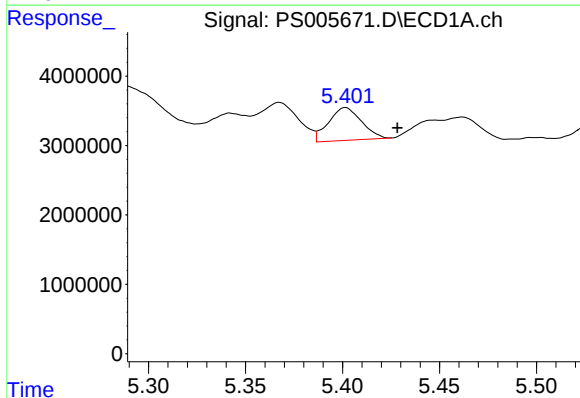


#3 4-Nitrophenol

R.T.: 5.402 min
Delta R.T.: -0.027 min
Response: 5585246
Conc: 7.81 ng/ml

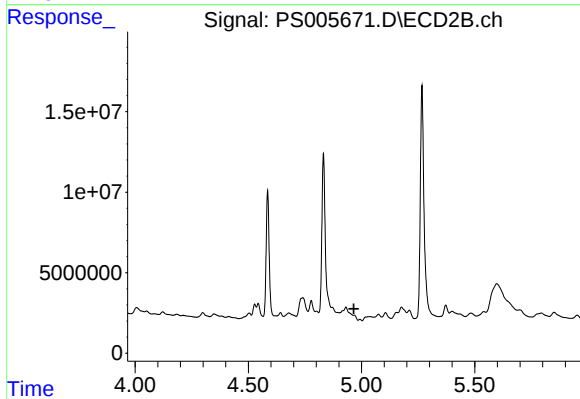

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 4.966 min
Response: 0
Conc: N.D.

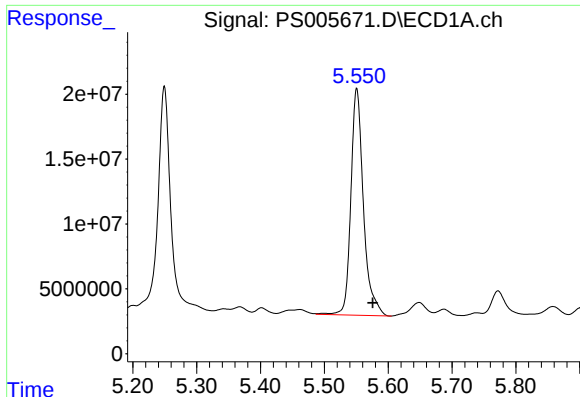

#4 2,4-DCAA


R.T.: 5.551 min
Delta R.T.: -0.025 min
Response: 239727745
Conc: 152.14 ng/ml

Instrument :
ECD_S
ClientSampleId :
S3-02-B

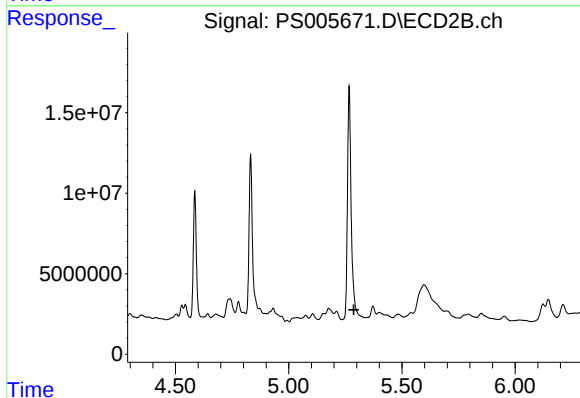


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 5.288 min
Response: 0
Conc: N.D.

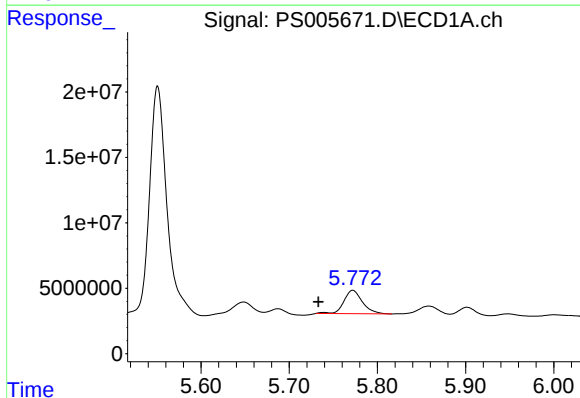


#5 DICAMBA

R.T.: 5.772 min
Delta R.T.: 0.039 min
Response: 26133053
Conc: 4.22 ng/ml

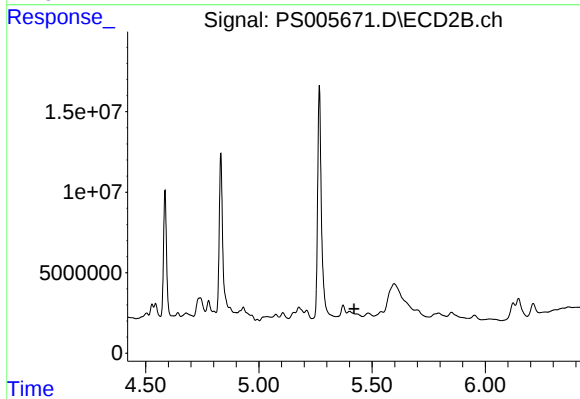

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 5.420 min
Response: 0
Conc: N.D.

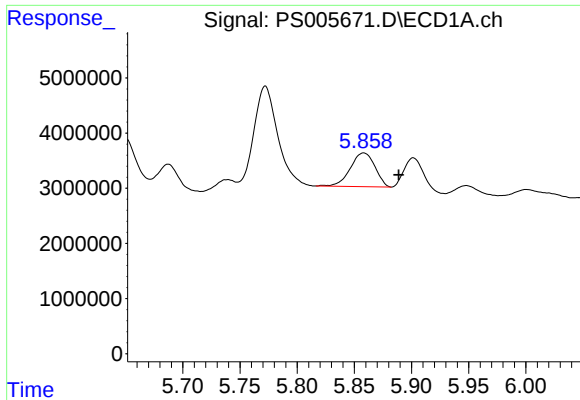

#6 MCP


R.T.: 5.858 min
Delta R.T.: -0.031 min
Response: 9173215
Conc: 1.89 ug/ml

Instrument :
ECD_S
ClientSampleId :
S3-02-B

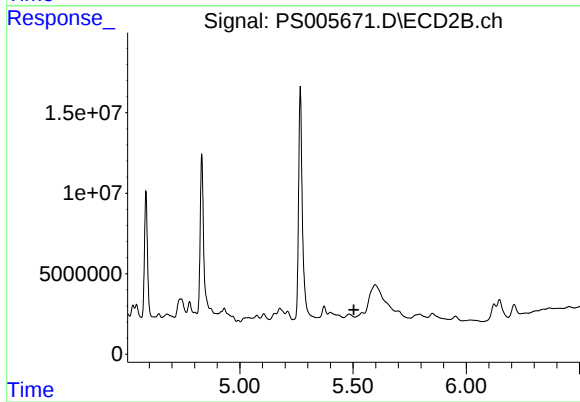


#6 MCP

R.T.: 0.000 min
Exp R.T.: 5.504 min
Response: 0
Conc: N.D.

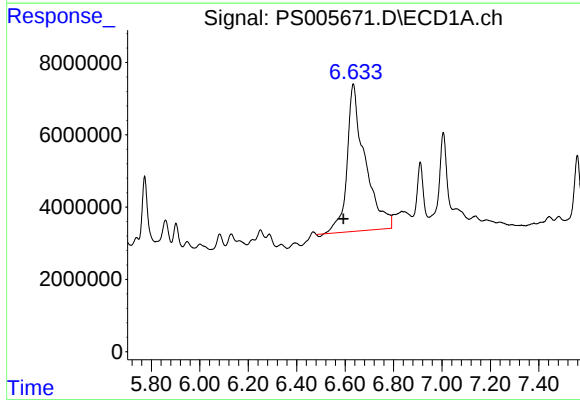


#9 2,4-D

R.T.: 6.634 min
Delta R.T.: 0.041 min
Response: 210103041
Conc: 119.81 ng/ml

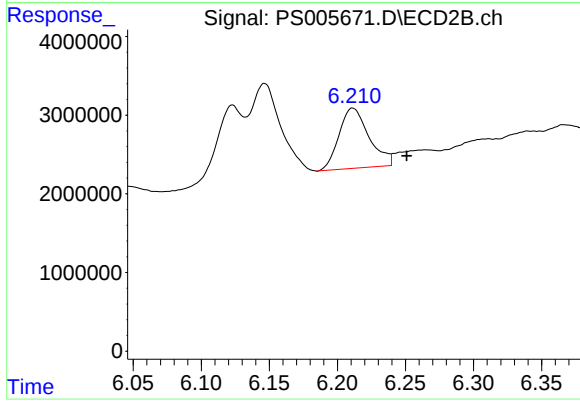

#9 2,4-D


R.T.: 6.211 min
Delta R.T.: -0.039 min
Response: 11777122
Conc: 10.09 ng/ml

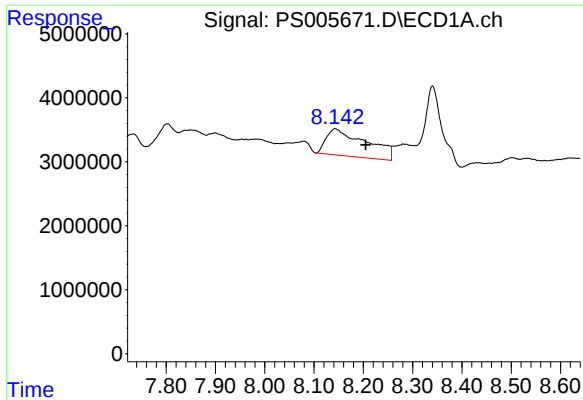

#13 2,4-DB


R.T.: 8.143 min
Delta R.T.: -0.062 min
Response: 23844851
Conc: 19.03 ng/ml

Instrument :
ECD_S
ClientSampleId :
S3-02-B

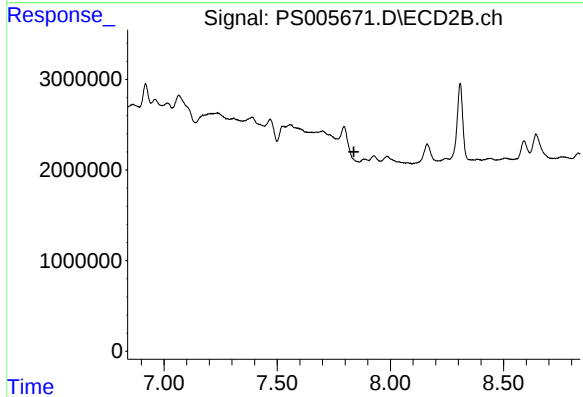


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.

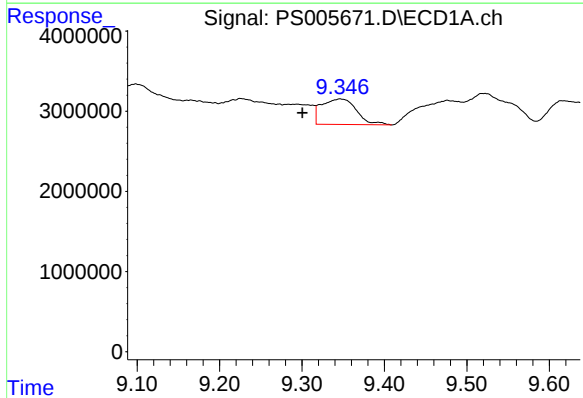


#14 DINOSEB

R.T.: 9.347 min
Delta R.T.: 0.046 min
Response: 9316711
Conc: 1.34 ng/ml

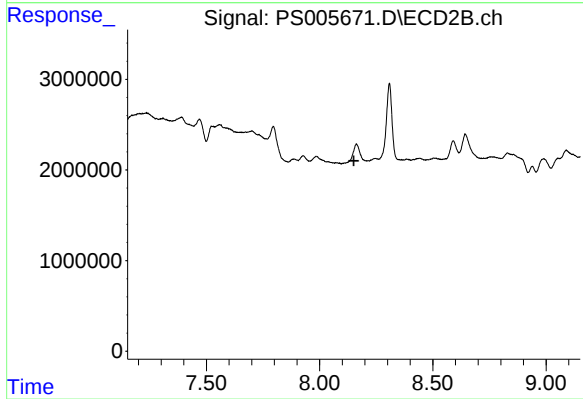

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 8.151 min
Response: 0
Conc: N.D.

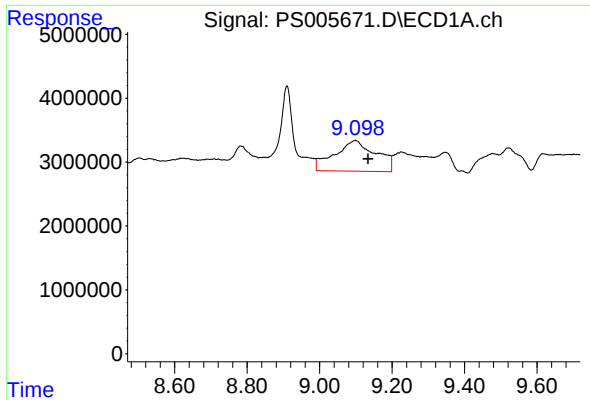

#15 Picloram

R.T.: 9.098 min
Delta R.T.: -0.035 min
Response: 38394956
Conc: 3.08 ng/ml

Instrument :
ECD_S
ClientSampleId :
S3-02-B

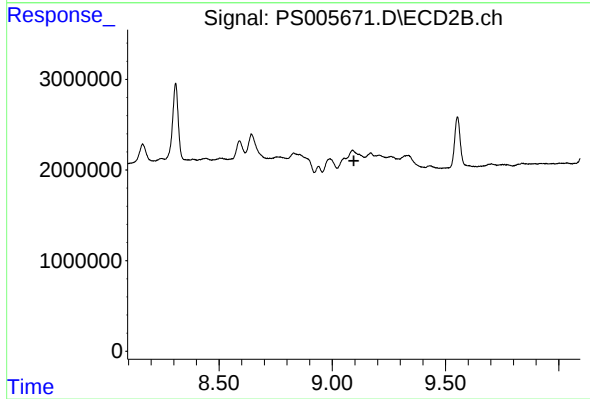

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.096 min
Response: 0
Conc: N.D.