

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072319\
 Data File : PS005679.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2019 02:36
 Operator : SM\AJ
 Sample : K3916-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 GIS-BUILDING-3

Manual Integrations
 APPROVED

Ankita
 7/24/2019 3:46:49 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 06:38:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 19 08:54:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	5.559	5.276	303.0E6	191.3E6	192.292m	185.194m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072319\
Data File : PS005679.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2019 02:36
Operator : SM\AJ
Sample : K3916-03
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
GIS-BUILDING-3


Manual Integrations
APPROVED

Ankita
7/24/2019 3:46:49 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 06:38:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
Quant Title : 8080.M
QLast Update : Fri Jul 19 08:54:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

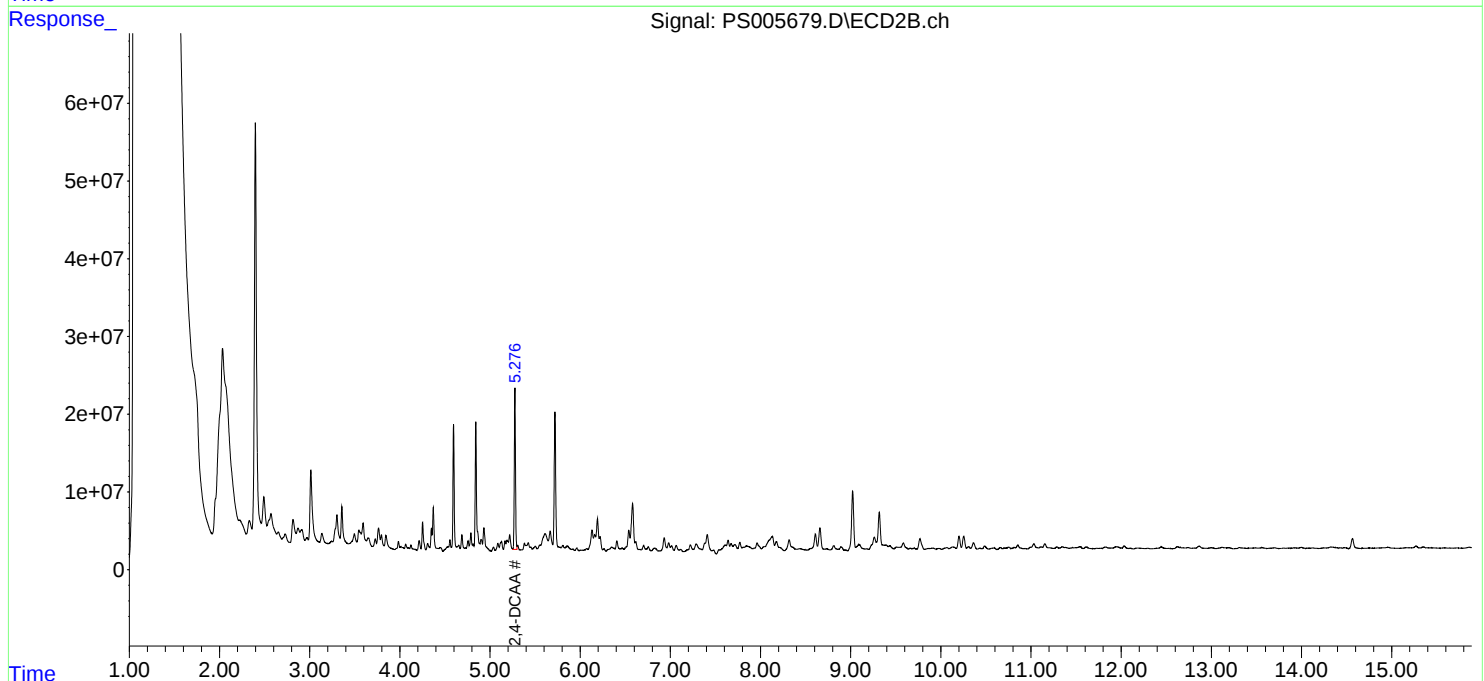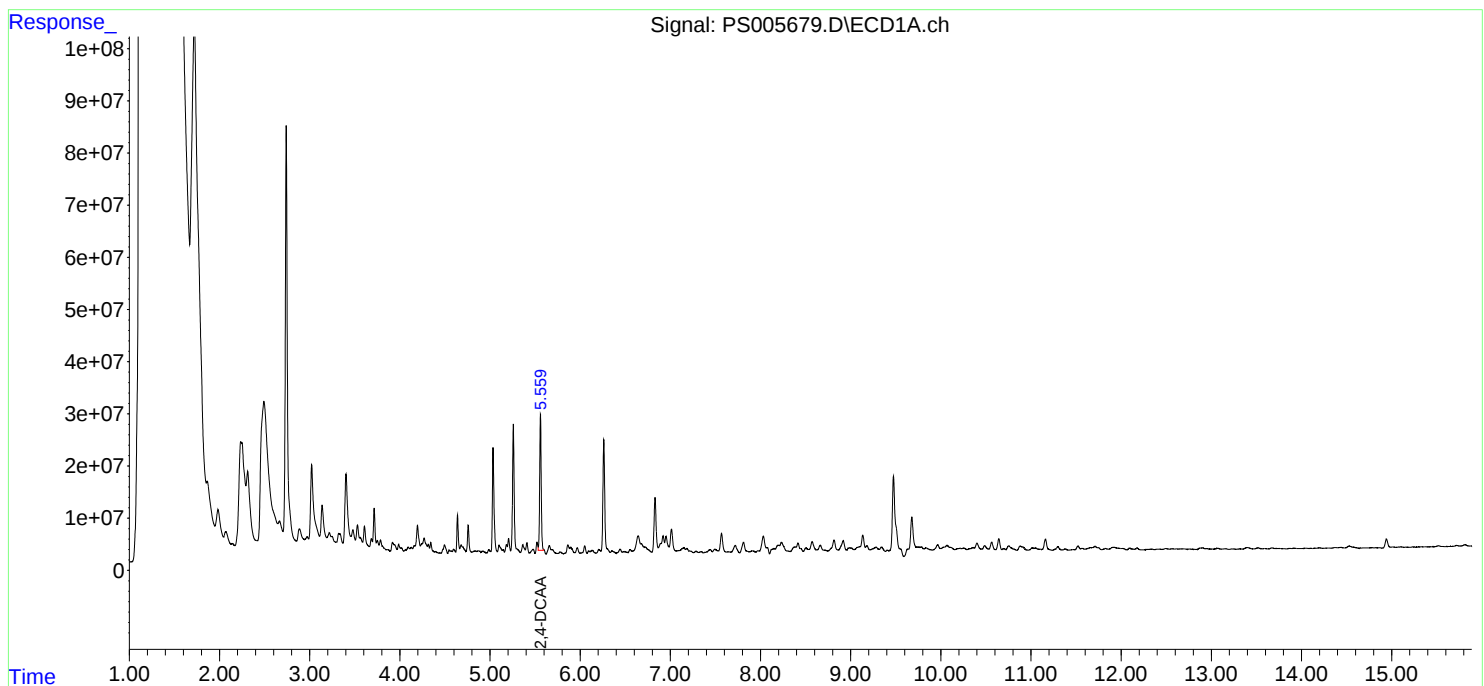

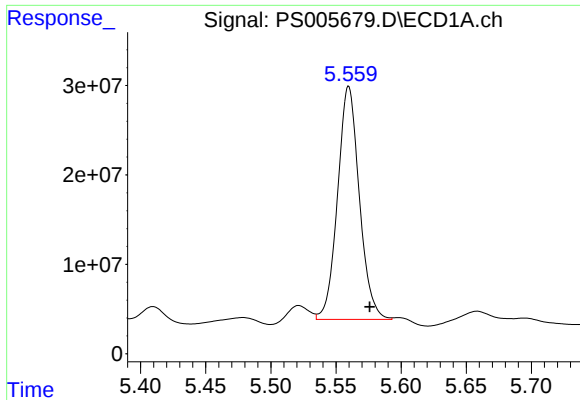


#4 2,4-DCAA

R.T.: 5.559 min
Delta R.T.: -0.017 min
Response: 303004715
Conc: 192.29 ng/ml m

Instrument :
ECD_S
ClientSampleId :
GIS-BUILDING-3

Manual Integrations
APPROVED

Ankita
7/24/2019 3:46:49 PM

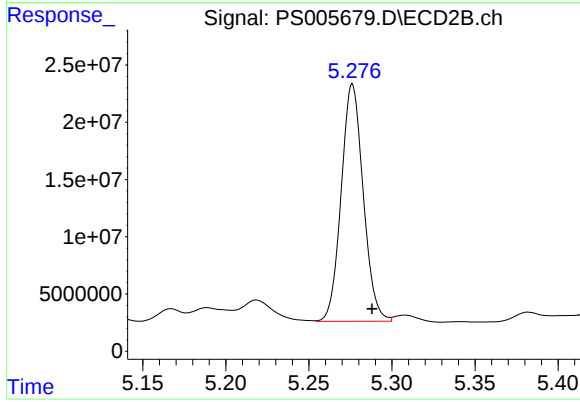

#4 2,4-DCAA

R.T.: 5.276 min
Delta R.T.: -0.012 min
Response: 191286676
Conc: 185.19 ng/ml m