

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072419\
 Data File : PS005685.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2019 07:30
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 12:14:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 19 08:54:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

7) T	MCPA	5.984	0.000	4038609	0	<MDL	N.D.	#
8) T	DICHLORPROP	6.304	0.000	9730038	0	6.401	N.D.	#
9) T	2,4-D	6.554	0.000	36013875	0	20.536	N.D.	#
11) T	2,4,5-TP ...	7.391	0.000	1732912	0	<MDL	N.D.	#
14) T	DINOSEB	9.292	0.000	1689163	0	<MDL	N.D.	#
15) T	Picloram	9.155	0.000	4445434	0	<MDL	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072419\
Data File : PS005685.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2019 07:30
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 12:14:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
Quant Title : 8080.M
QLast Update : Fri Jul 19 08:54:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

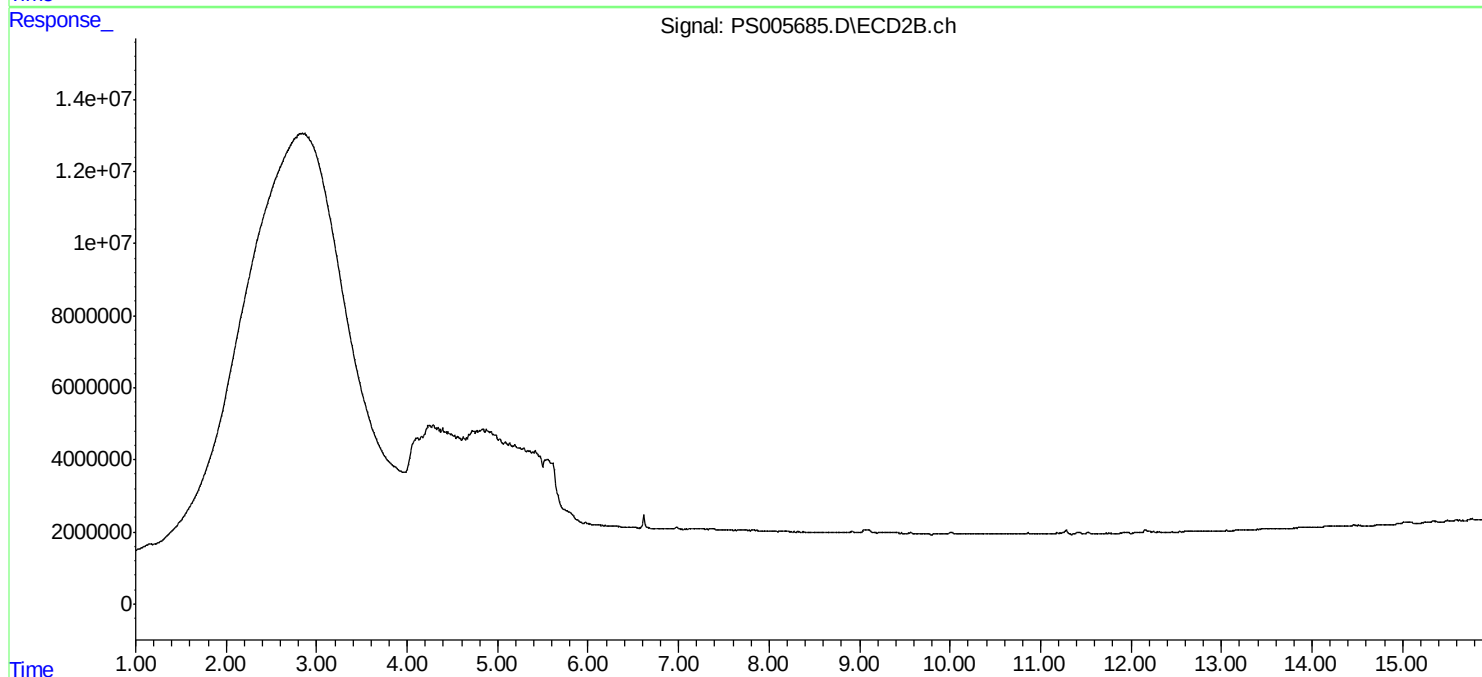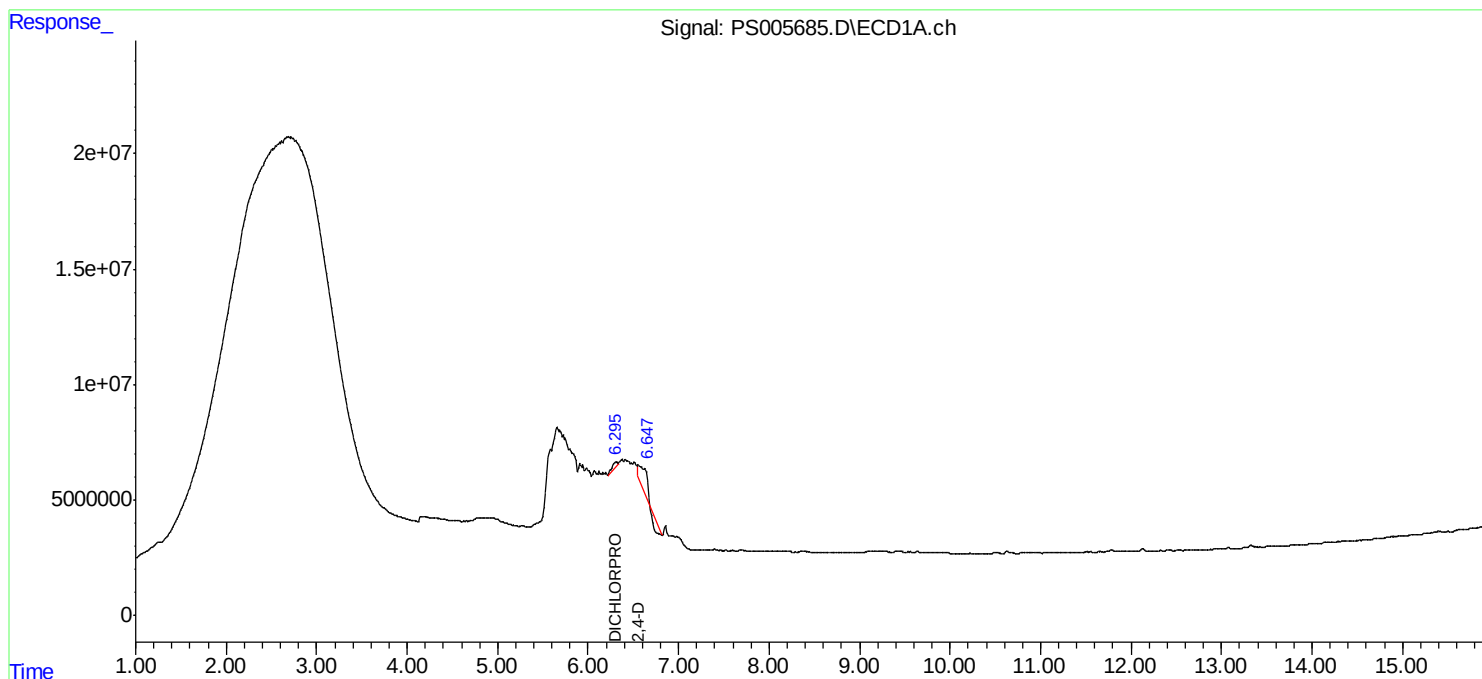


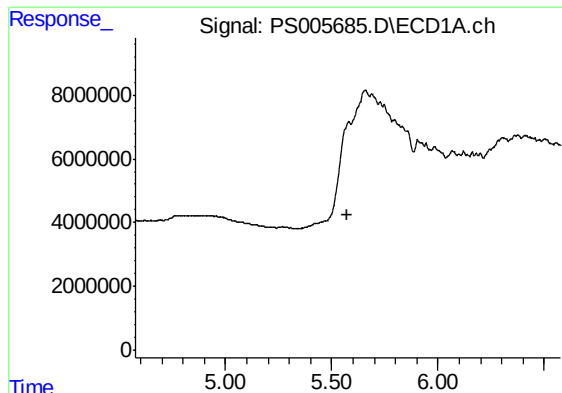

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 5.576 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

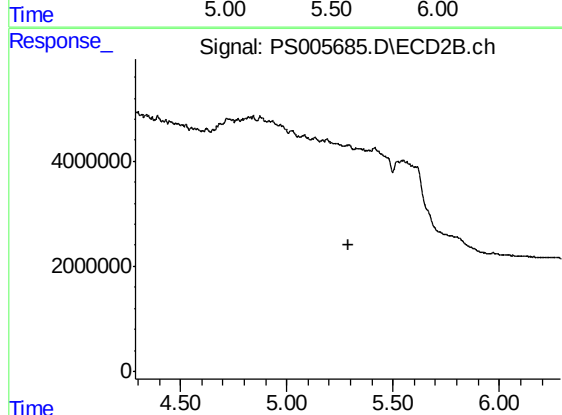


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 5.288 min
Response: 0
Conc: N.D.

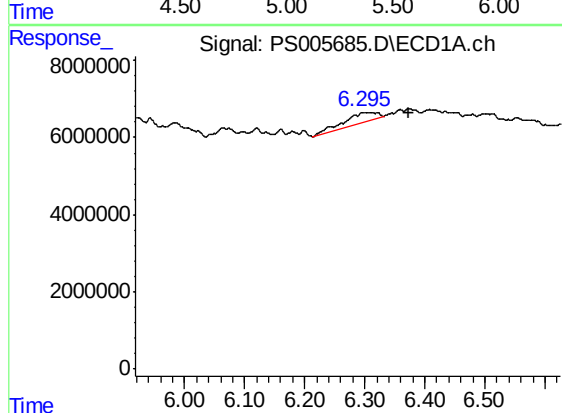


#8 DICHLORPROP

R.T.: 6.304 min
Delta R.T.: -0.069 min
Response: 9730038
Conc: 6.40 ng/ml

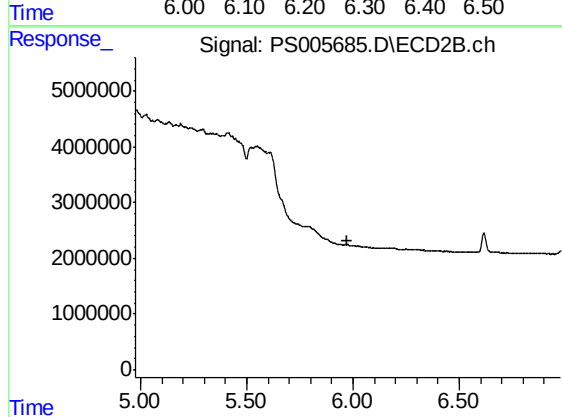

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 5.976 min
Response: 0
Conc: N.D.

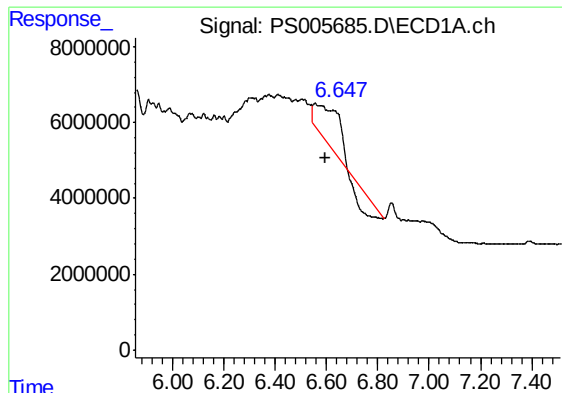

#9 2,4-D

R.T.: 6.554 min
Delta R.T.: -0.039 min
Response: 36013875
Conc: 20.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

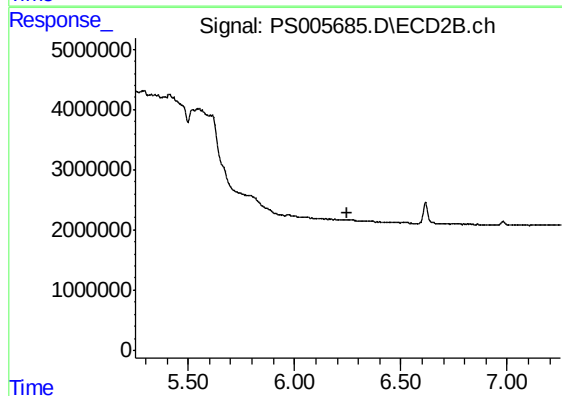

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.251 min
Response: 0
Conc: N.D.