

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072419\
 Data File : PS005690.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2019 11:10
 Operator : SM\AJ
 Sample : K3868-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 12:15:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 19 08:54:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.562	5.279	575.4E6	353.6E6	365.143	342.315
Target Compounds							
2) T	3,5-DICHL...	4.884	4.598	4123939	162.9E6	1.938	120.202 #
3) T	4-Nitroph...	5.413	0.000	4639795	0	6.490	N.D. #
5) T	DICAMBA	5.750	5.432	1849118	15284546	<MDL	3.863 #
6) T	MCP	5.867	0.000	11055592	0	2.276	N.D. #
8) T	DICHLORPROP	6.345	0.000	3241817	0	2.133	N.D. #
9) T	2,4-D	6.646	0.000	156.2E6	0	89.058	N.D. #
10) T	Pentachlo...	6.850	0.000	689896	0	<MDL	N.D. #
11) T	2,4,5-TP ...	7.389	6.928	1853557	125.1E6	<MDL	22.442 #
13) T	2,4-DB	8.204	0.000	29159444	0	23.277	N.D. #
14) T	DINOSEB	9.236	0.000	32509506	0	4.661	N.D. #
15) T	Picloram	9.112	0.000	29811716	0	2.393	N.D. #
16) T	DCPA	9.534	0.000	22151563	0	2.034	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072419\
Data File : PS005690.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2019 11:10
Operator : SM\AJ
Sample : K3868-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
TP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 12:15:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
Quant Title : 8080.M
QLast Update : Fri Jul 19 08:54:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

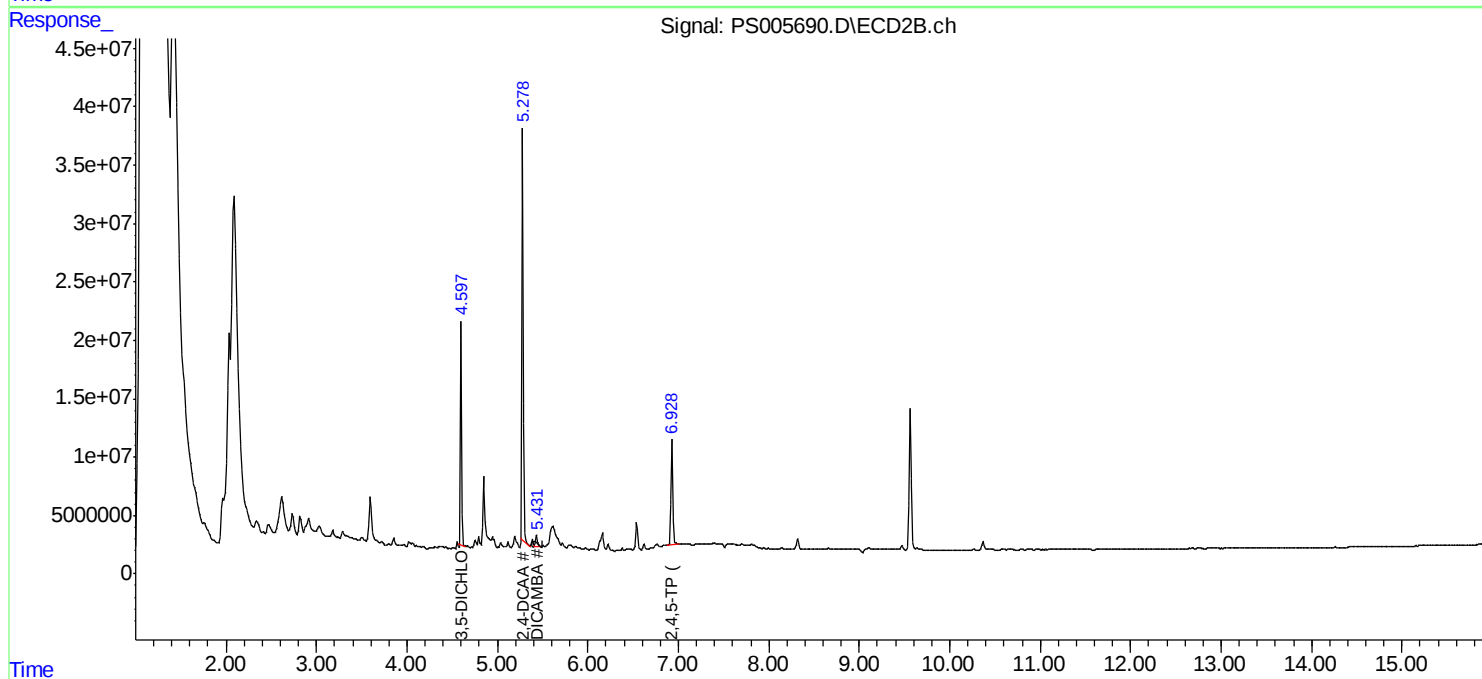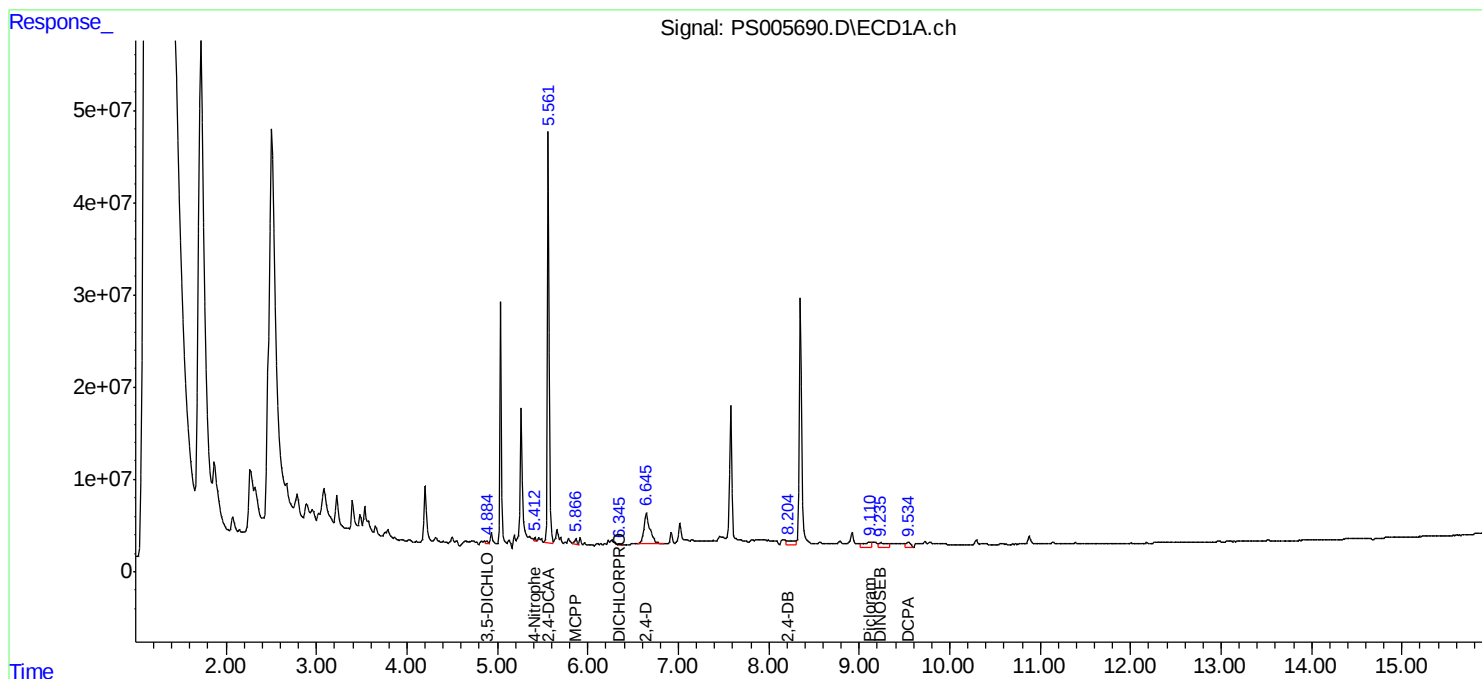


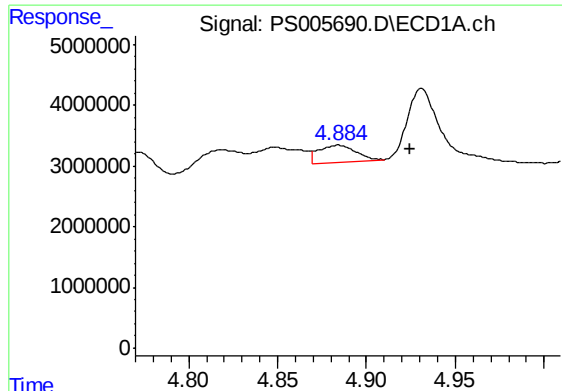

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.884 min
Delta R.T.: -0.041 min
Response: 4123939
Conc: 1.94 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

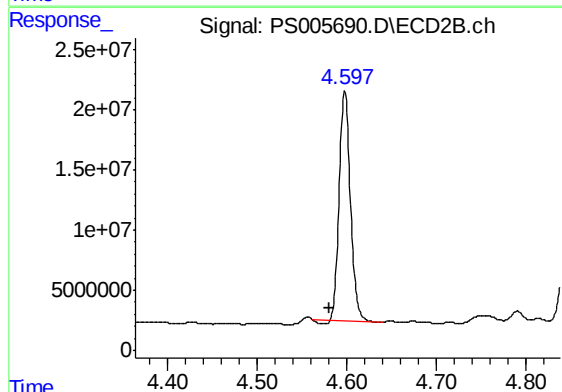


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.598 min
Delta R.T.: 0.017 min
Response: 162930121
Conc: 120.20 ng/ml

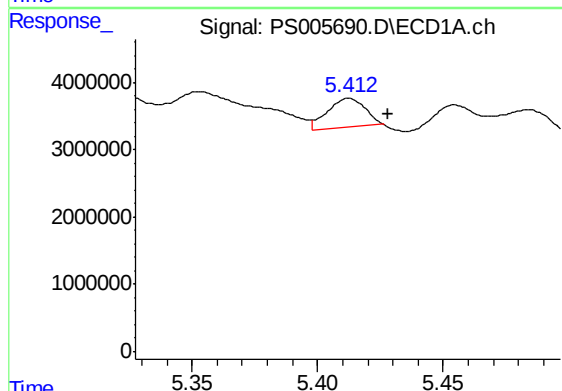


#3 4-Nitrophenol

R.T.: 5.413 min
Delta R.T.: -0.016 min
Response: 4639795
Conc: 6.49 ng/ml

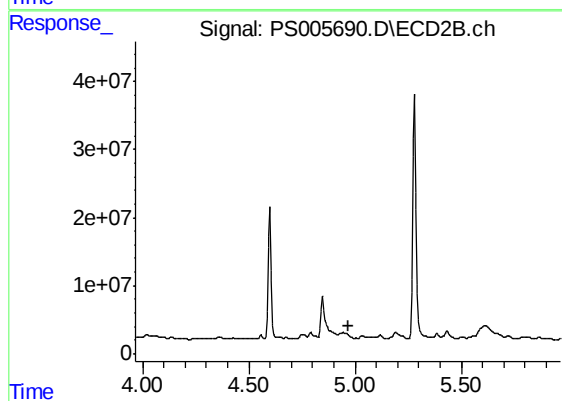

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 4.966 min
Response: 0
Conc: N.D.

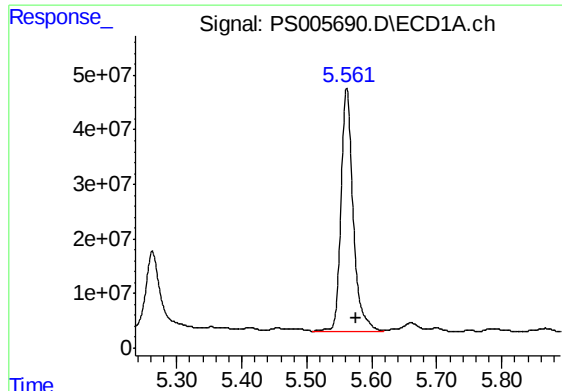

#4 2,4-DCAA


R.T.: 5.562 min
Delta R.T.: -0.014 min
Response: 575374664
Conc: 365.14 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

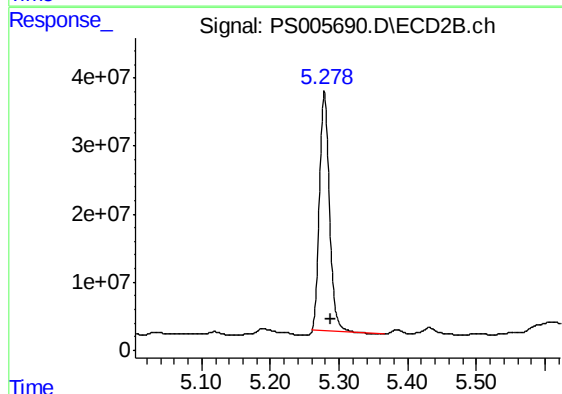


#4 2,4-DCAA

R.T.: 5.279 min
Delta R.T.: -0.009 min
Response: 353576848
Conc: 342.31 ng/ml

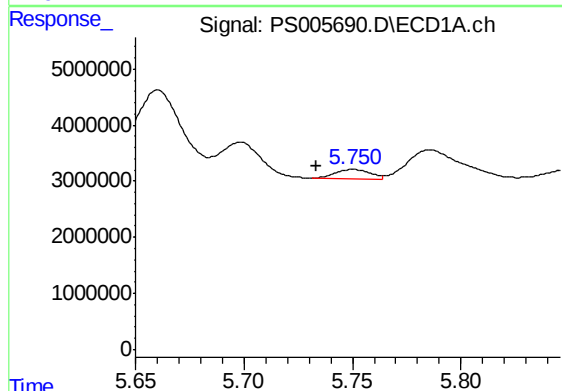


#5 DICAMBA

R.T.: 5.750 min
Delta R.T.: 0.017 min
Response: 1849118
Conc: N.D.

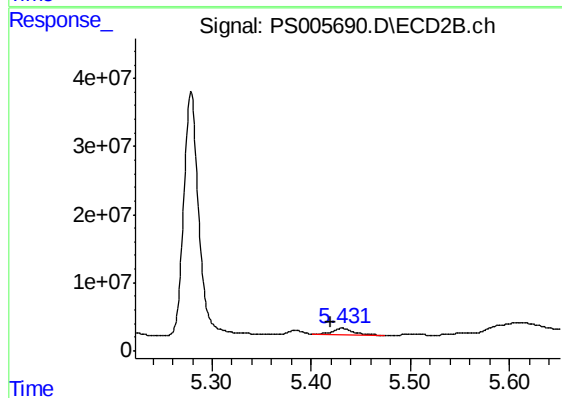

#5 DICAMBA


R.T.: 5.432 min
Delta R.T.: 0.012 min
Response: 15284546
Conc: 3.86 ng/ml

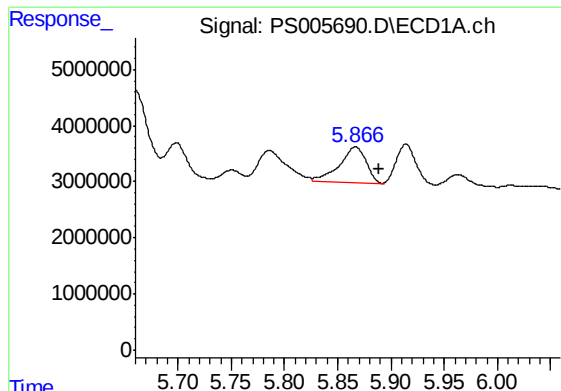

#6 MCP


R.T.: 5.867 min
Delta R.T.: -0.022 min
Response: 11055592
Conc: 2.28 ug/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

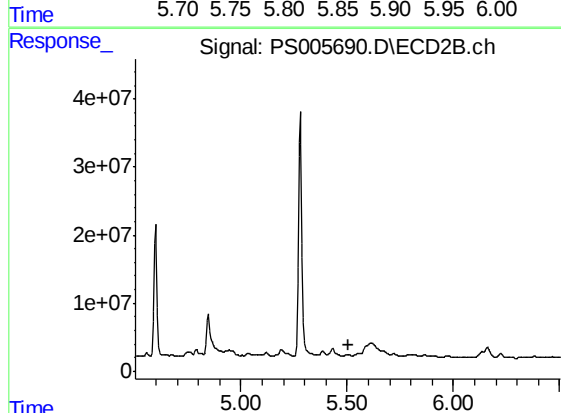


#6 MCP

R.T.: 0.000 min
Exp R.T. : 5.504 min
Response: 0
Conc: N.D.

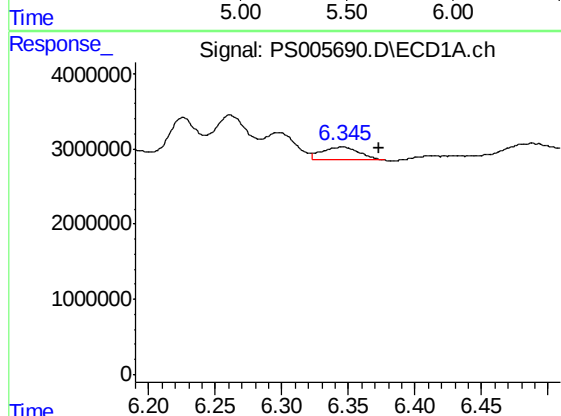


#8 DICHLORPROP

R.T.: 6.345 min
Delta R.T.: -0.028 min
Response: 3241817
Conc: 2.13 ng/ml

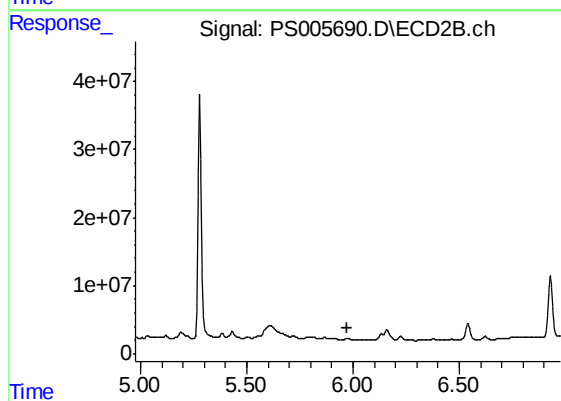

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 5.976 min
Response: 0
Conc: N.D.

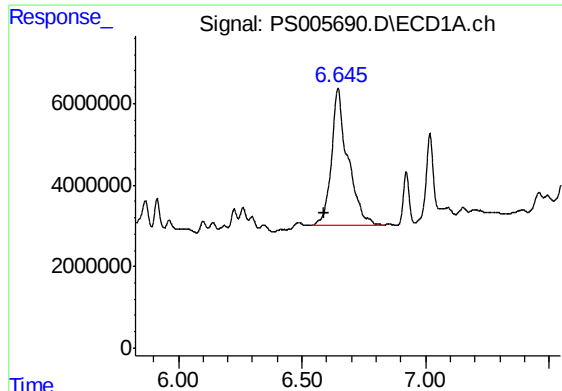

#9 2,4-D


R.T.: 6.646 min
Delta R.T.: 0.053 min
Response: 156180435
Conc: 89.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

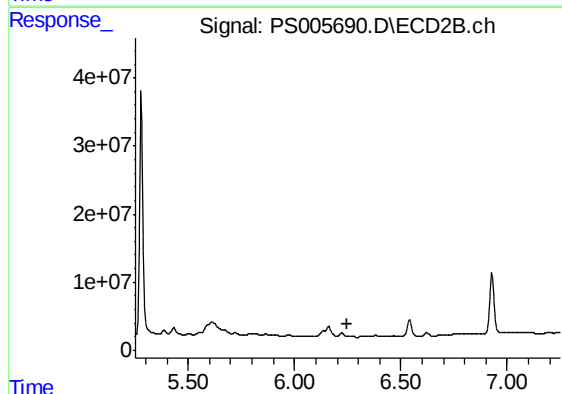


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.251 min
Response: 0
Conc: N.D.

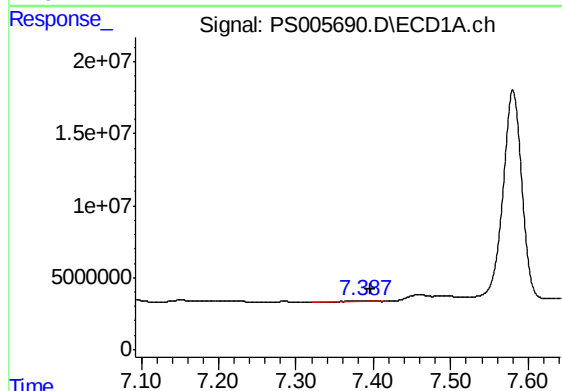


#11 2,4,5-TP (SILVEX)

R.T.: 7.389 min
Delta R.T.: -0.007 min
Response: 1853557
Conc: N.D.

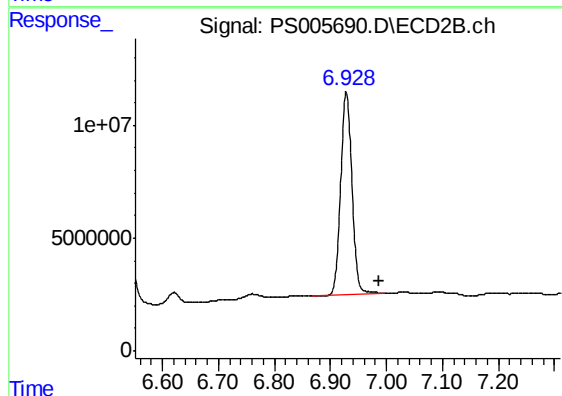

#11 2,4,5-TP (SILVEX)


R.T.: 6.928 min
Delta R.T.: -0.058 min
Response: 125079573
Conc: 22.44 ng/ml

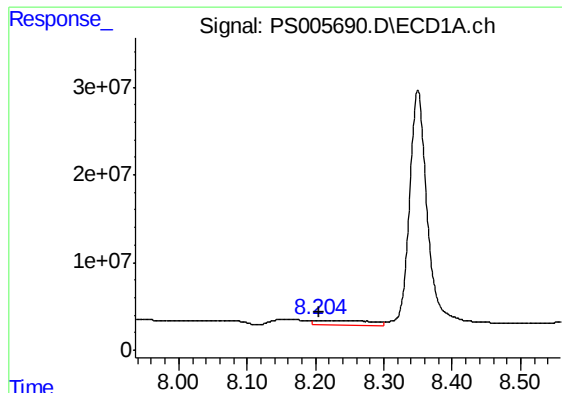

#13 2,4-DB


R.T.: 8.204 min
Delta R.T.: 0.000 min
Response: 29159444
Conc: 23.28 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

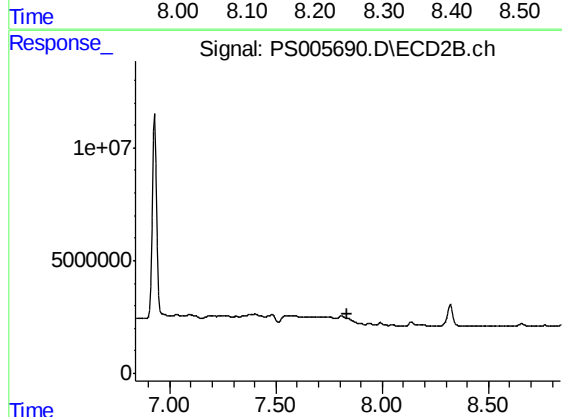


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.

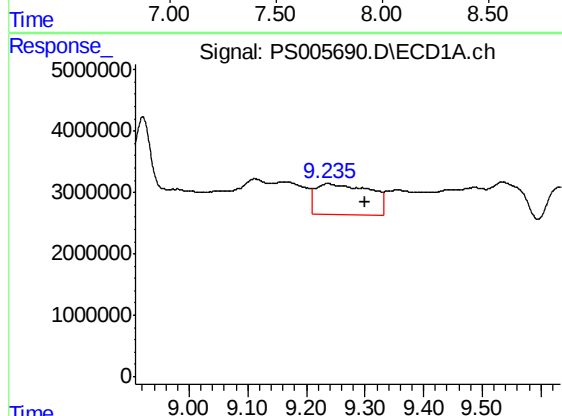


#14 DINOSEB

R.T.: 9.236 min
Delta R.T.: -0.065 min
Response: 32509506
Conc: 4.66 ng/ml

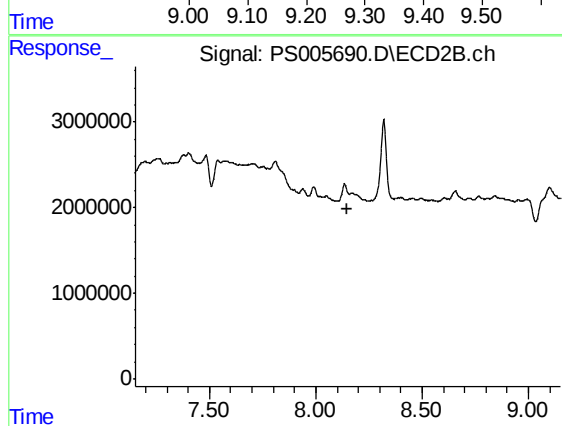

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 8.151 min
Response: 0
Conc: N.D.

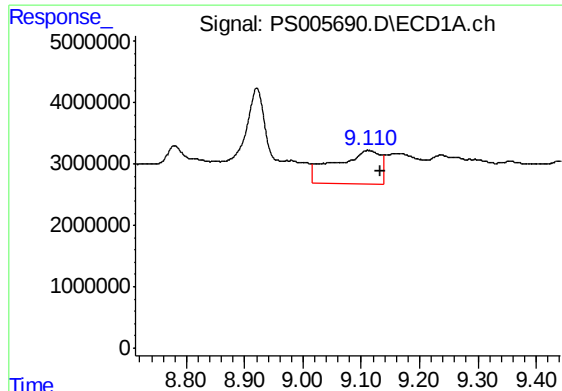

#15 Picloram


R.T.: 9.112 min
Delta R.T.: -0.021 min
Response: 29811716
Conc: 2.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

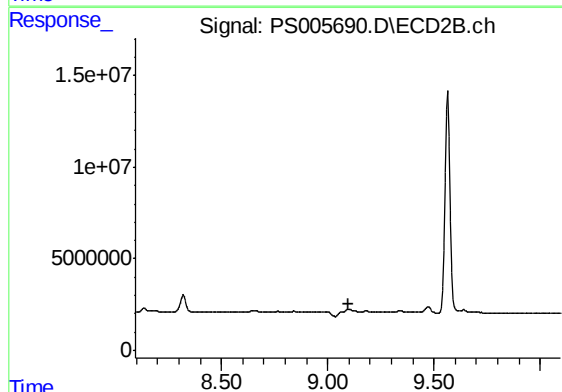


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.096 min
Response: 0
Conc: N.D.

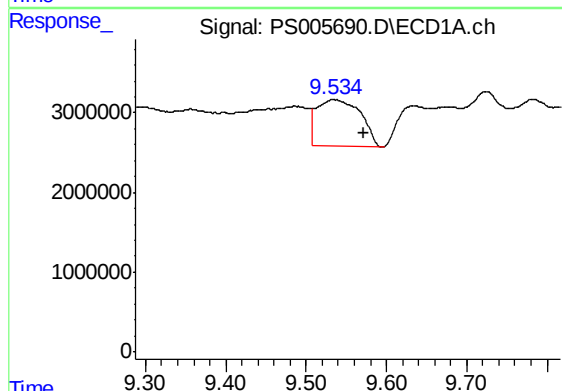

#16 DCPA

R.T.: 9.534 min
Delta R.T.: -0.038 min
Response: 22151563
Conc: 2.03 ng/ml

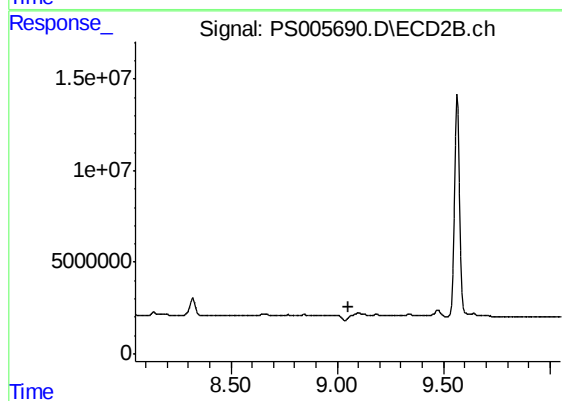

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.051 min
Response: 0
Conc: N.D.