

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072419\
 Data File : PS005693.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2019 12:16
 Operator : SM\AJ
 Sample : K3622-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 OR-02-071919-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 13:44:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 19 08:54:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.542	5.277	629.1E6	394.8E6	399.239	382.264
Target Compounds							
2) T	3,5-DICHL...	4.911	4.596	751654	83879310	<MDL	61.882 #
3) T	4-Nitroph...	5.456	0.000	16054863	0	22.459	N.D. #
5) T	DICAMBA	5.764	0.000	22797607	0	3.686	N.D. #
6) T	MCPD	5.894	0.000	883348	0	<MDL	N.D. #
7) T	MCPA	5.993	0.000	1404474	0	<MDL	N.D. #
8) T	DICHLORPROP	6.395	0.000	1801478	0	1.185	N.D. #
9) T	2,4-D	6.627	0.000	156.3E6	0	89.149	N.D. #
10) T	Pentachlo...	6.826	0.000	1995094	0	<MDL	N.D. #
11) T	2,4,5-TP ...	7.365	6.931	1671703	14816243	<MDL	2.658 #
13) T	2,4-DB	8.185	0.000	2518325	0	2.010	N.D. #
14) T	DINOSEB	9.346	0.000	16155649	0	2.316	N.D. #
15) T	Picloram	9.074	0.000	23379334	0	1.877	N.D. #
16) T	DCPA	9.610	0.000	5161538	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072419\
Data File : PS005693.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2019 12:16
Operator : SM\AJ
Sample : K3622-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
OR-02-071919-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 13:44:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
Quant Title : 8080.M
QLast Update : Fri Jul 19 08:54:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

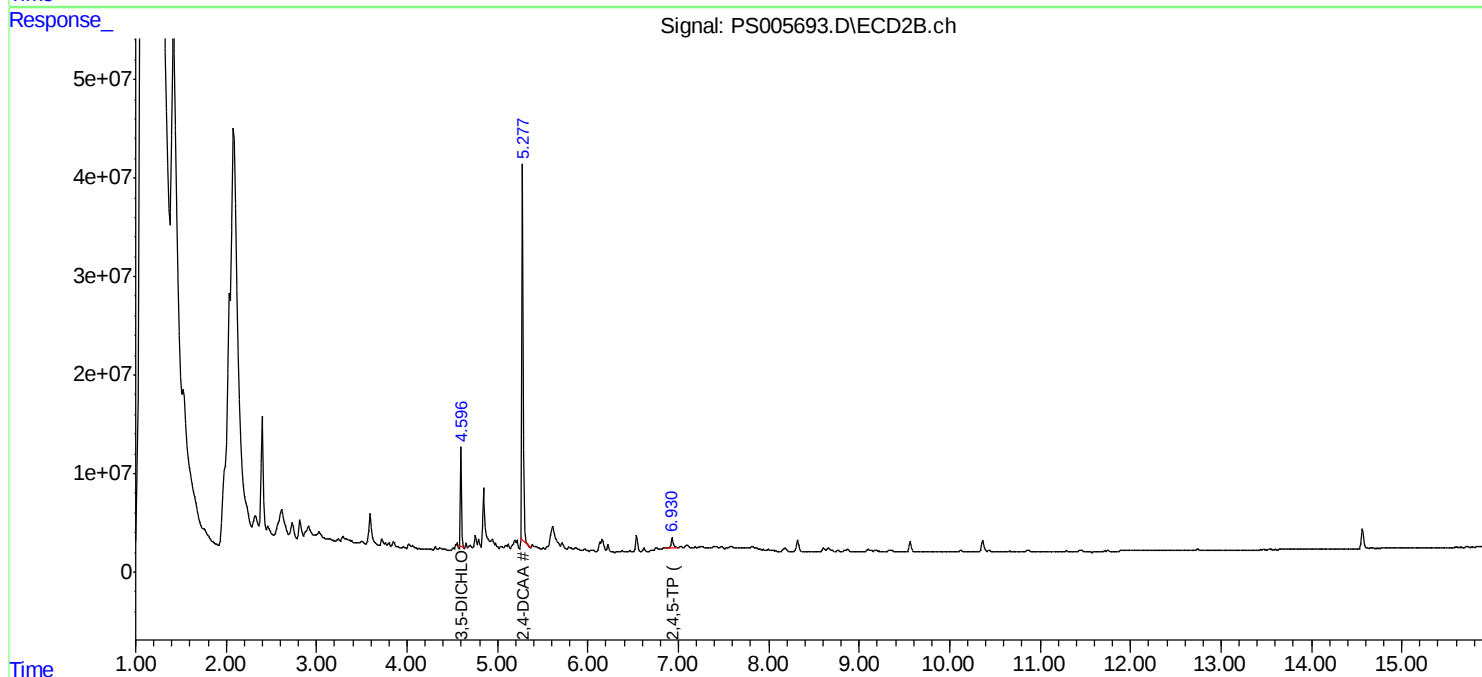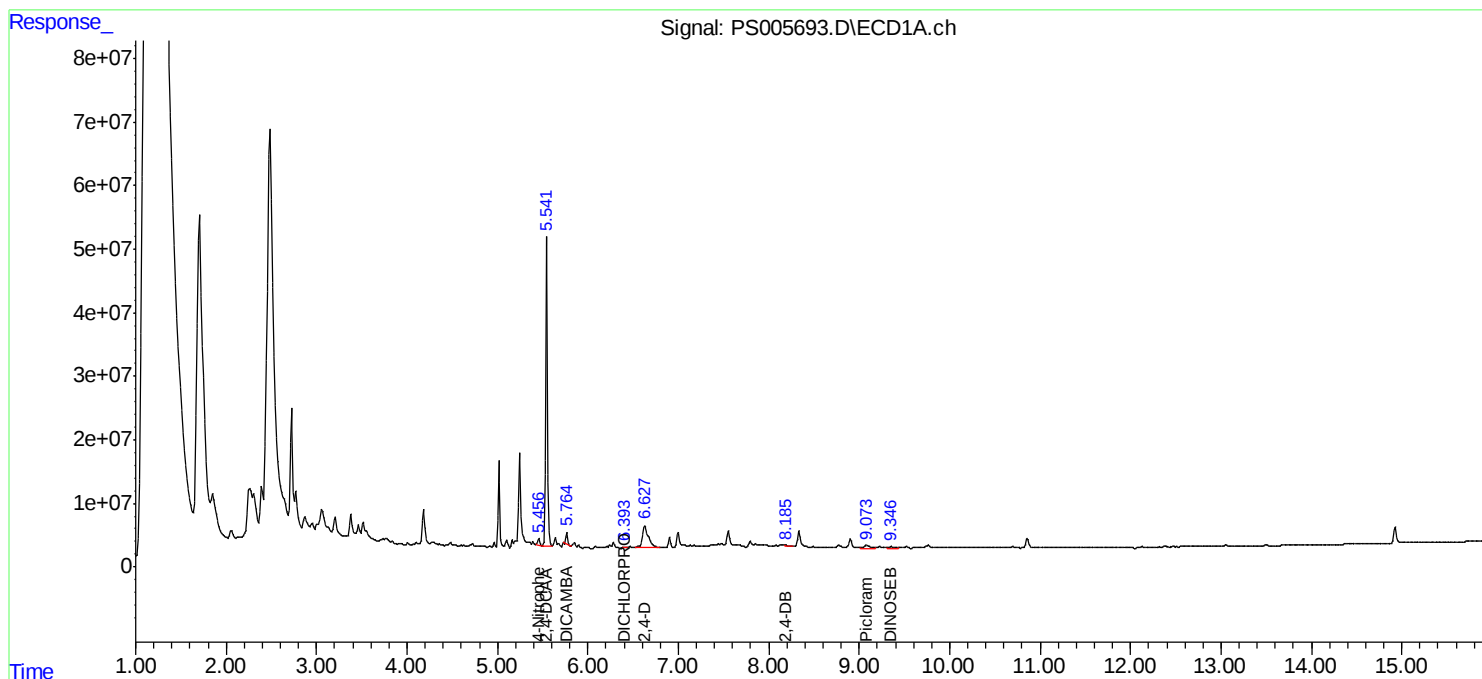


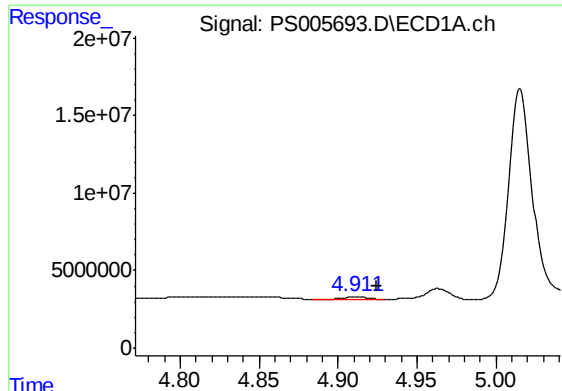

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.911 min
Delta R.T.: -0.013 min
Response: 751654
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OR-02-071919-B

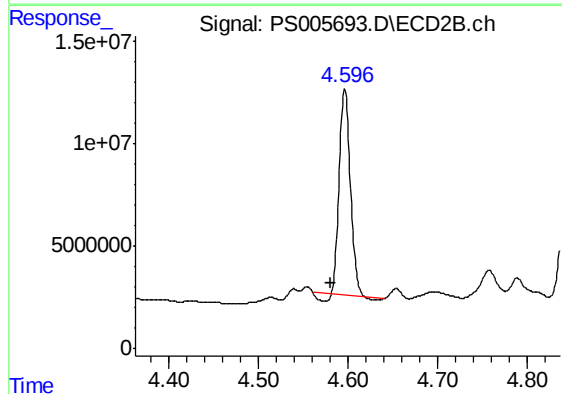


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.596 min
Delta R.T.: 0.015 min
Response: 83879310
Conc: 61.88 ng/ml

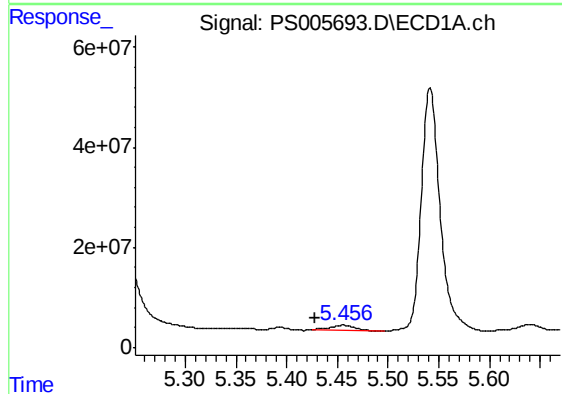


#3 4-Nitrophenol

R.T.: 5.456 min
Delta R.T.: 0.028 min
Response: 16054863
Conc: 22.46 ng/ml

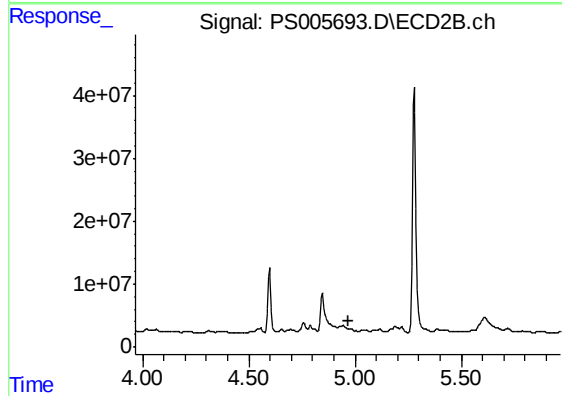

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 4.966 min
Response: 0
Conc: N.D.

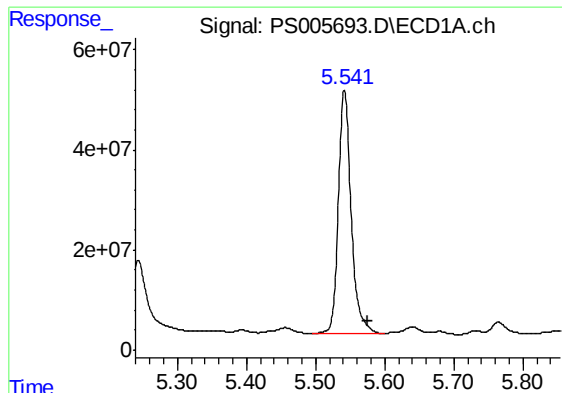

#4 2,4-DCAA


R.T.: 5.542 min
Delta R.T.: -0.034 min
Response: 629102612
Conc: 399.24 ng/ml

Instrument :
ECD_S
ClientSampleId :
OR-02-071919-B

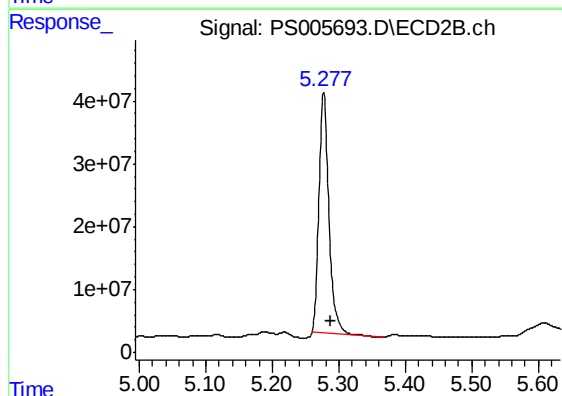


#4 2,4-DCAA

R.T.: 5.277 min
Delta R.T.: -0.011 min
Response: 394840244
Conc: 382.26 ng/ml

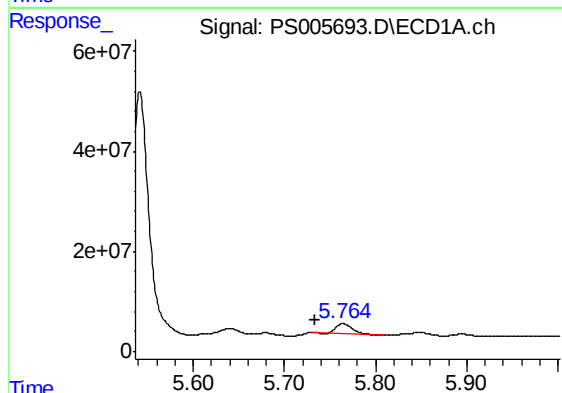


#5 DICAMBA

R.T.: 5.764 min
Delta R.T.: 0.031 min
Response: 22797607
Conc: 3.69 ng/ml

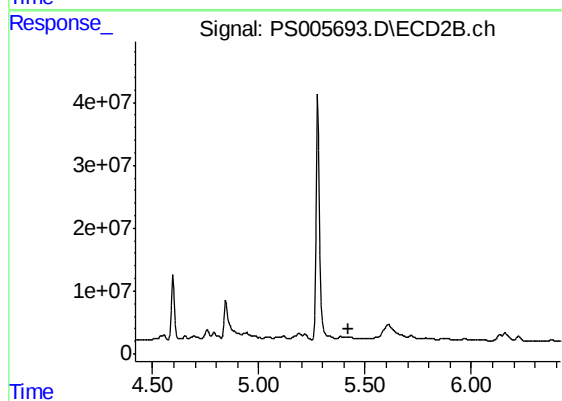

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 5.420 min
Response: 0
Conc: N.D.

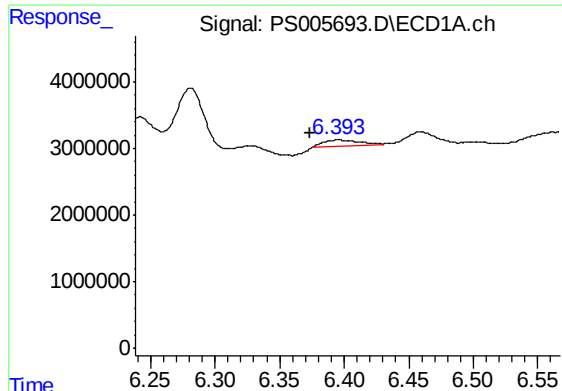

#8 DICHLORPROP


R.T.: 6.395 min
Delta R.T.: 0.022 min
Response: 1801478
Conc: 1.19 ng/ml

Instrument :
ECD_S
ClientSampleId :
OR-02-071919-B

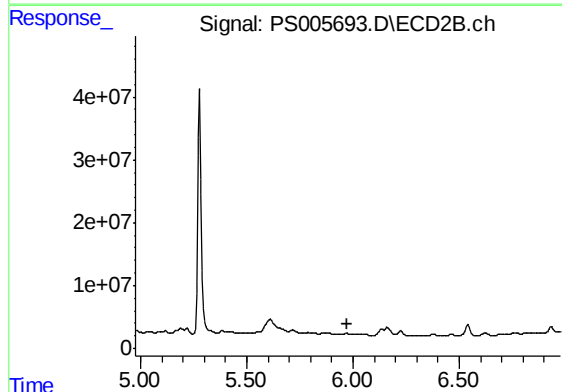


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 5.976 min
Response: 0
Conc: N.D.

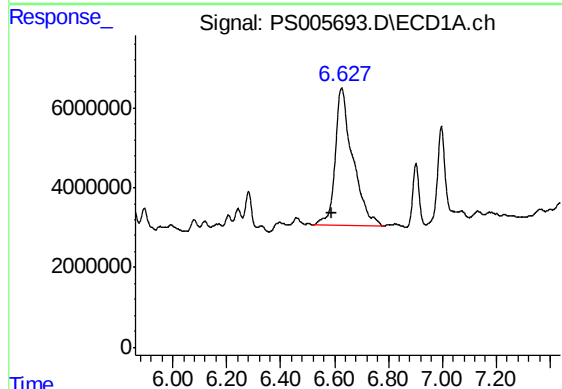


#9 2,4-D

R.T.: 6.627 min
Delta R.T.: 0.034 min
Response: 156339569
Conc: 89.15 ng/ml

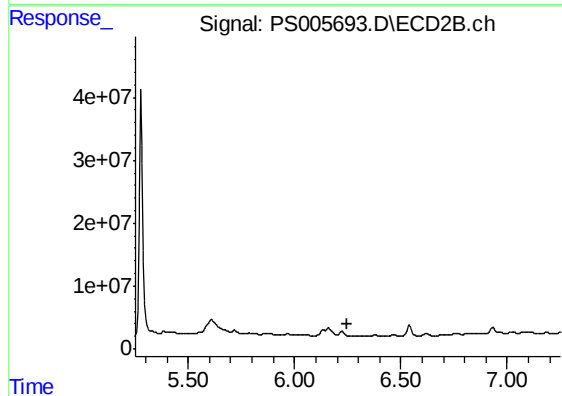

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 6.251 min
Response: 0
Conc: N.D.

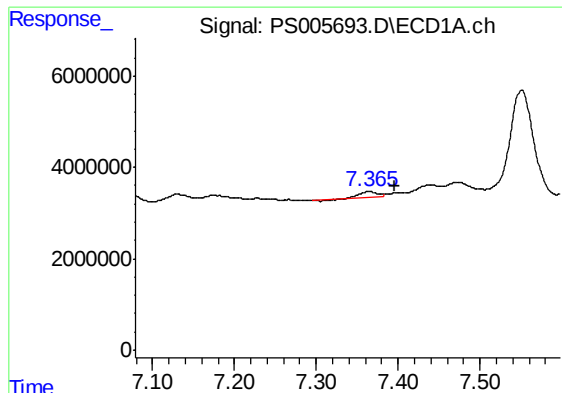

#11 2,4,5-TP (SILVEX)


R.T.: 7.365 min
Delta R.T.: -0.032 min
Response: 1671703
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OR-02-071919-B

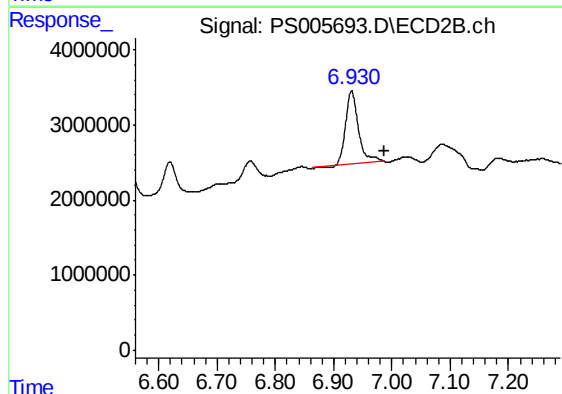


#11 2,4,5-TP (SILVEX)

R.T.: 6.931 min
Delta R.T.: -0.056 min
Response: 14816243
Conc: 2.66 ng/ml

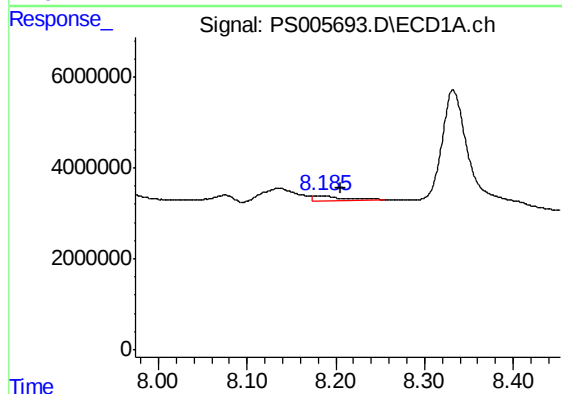


#13 2,4-DB

R.T.: 8.185 min
Delta R.T.: -0.020 min
Response: 2518325
Conc: 2.01 ng/ml

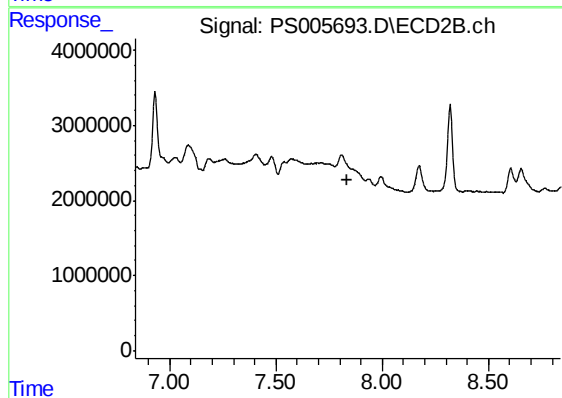

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.

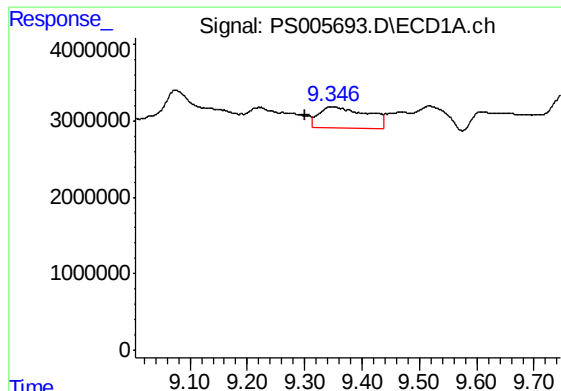

#14 DINOSEB


R.T.: 9.346 min
Delta R.T.: 0.046 min
Response: 16155649
Conc: 2.32 ng/ml

Instrument :
ECD_S
ClientSampleId :
OR-02-071919-B

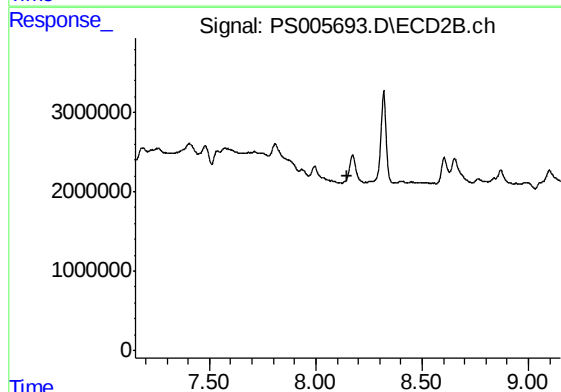


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 8.151 min
Response: 0
Conc: N.D.

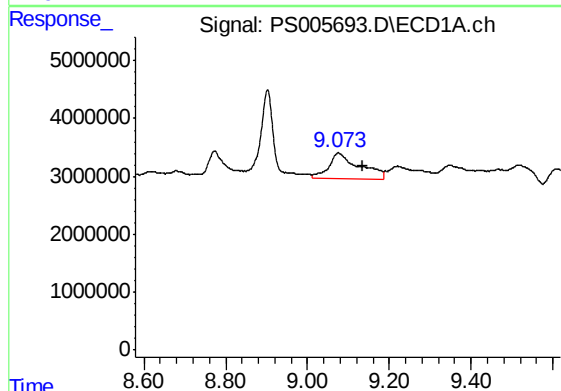

#15 Picloram

R.T.: 9.074 min
Delta R.T.: -0.059 min
Response: 23379334
Conc: 1.88 ng/ml

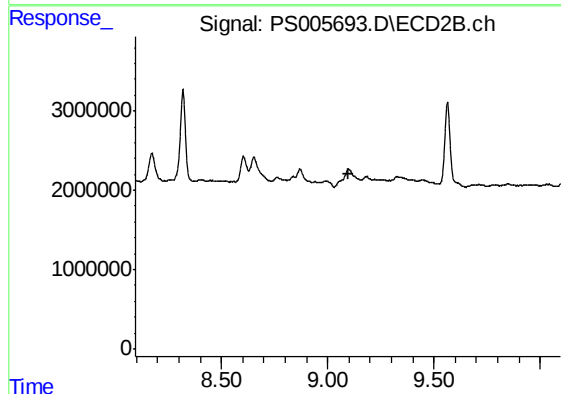

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.096 min
Response: 0
Conc: N.D.