

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072419\
 Data File : PS005700.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2019 15:04
 Operator : SM\AJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 00:43:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 19 08:54:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.560	5.278	1053.2E6	686.7E6	668.406	664.856
Target Compounds							
1) T	Dalapon	2.094	1.793	263.7E6	991.5E6	134.905	687.512 #
2) T	3,5-DICHL...	4.911	0.000	834.4E6	0	392.166	N.D. #
3) T	4-Nitroph...	5.406	4.954	218.1E6	378.3E6	305.133	763.441 #
5) T	DICAMBA	5.719	5.411	2093.4E6	2865.1E6	338.451	724.026 #
6) T	MCPD	5.879	5.501	301.2E6	215.9E6	62.006	74.530
7) T	MCPA	6.017	5.685	376.8E6	318.9E6	55.739	72.383 #
8) T	DICHLORPROP	6.358	5.965	425.2E6	726.1E6	279.708	711.852 #
9) T	2,4-D	6.573	6.237	1105.3E6	822.6E6	630.281	704.493
10) T	Pentachlo...	6.843	6.613	14309.2E6	9470.5E6	660.866	704.096
11) T	2,4,5-TP ...	7.379	6.975	5787.0E6	3986.9E6	653.982	715.348
12) T	2,4,5-T	7.652	7.336	5400.1E6	3732.8E6	637.882	727.425
13) T	2,4-DB	8.184	7.825	797.1E6	452.2E6	636.283	656.326
14) T	DINOSEB	9.283	8.139	5051.9E6	2982.3E6	724.245	736.622
15) T	Picloram	9.112	9.080	7784.5E6	4871.6E6	624.831	621.946
16) T	DCPA	9.554	9.039	7713.0E6	5057.3E6	708.319	715.463



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072419\
Data File : PS005700.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2019 15:04
Operator : SM\AJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 00:43:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071819.M
Quant Title : 8080.M
QLast Update : Fri Jul 19 08:54:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

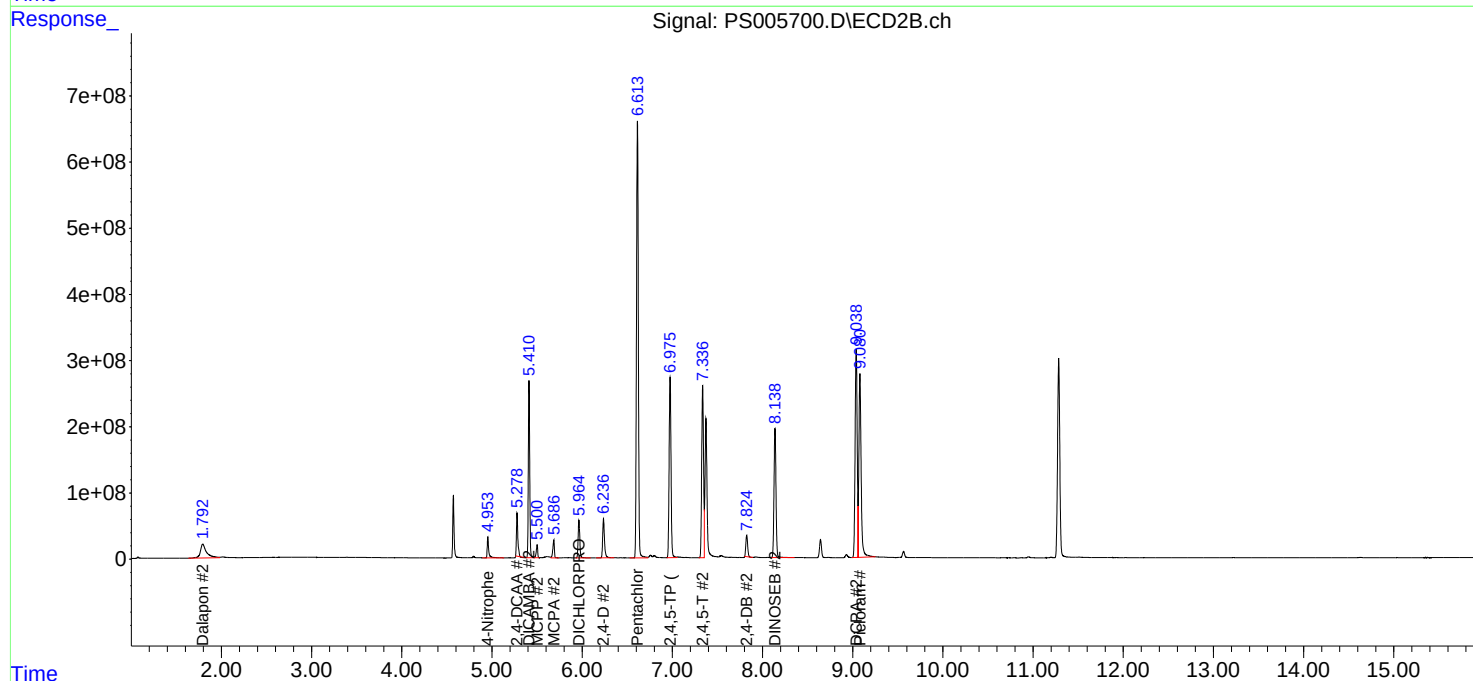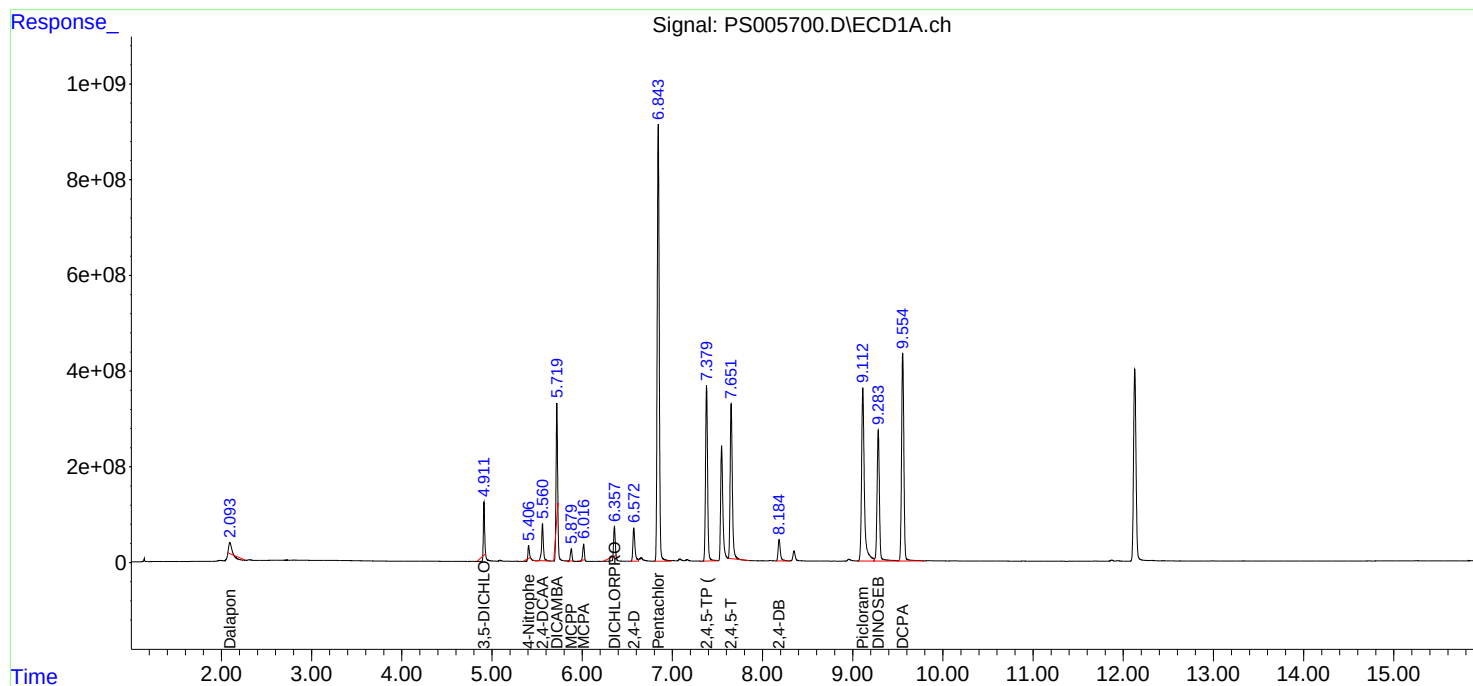


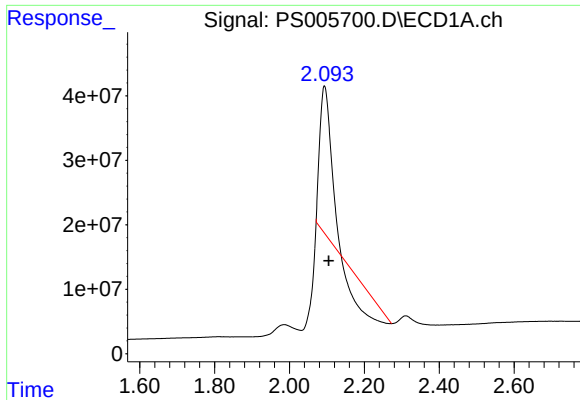

#1 Dalapon


R.T.: 2.094 min
Delta R.T.: -0.011 min
Response: 263678164
Conc: 134.91 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

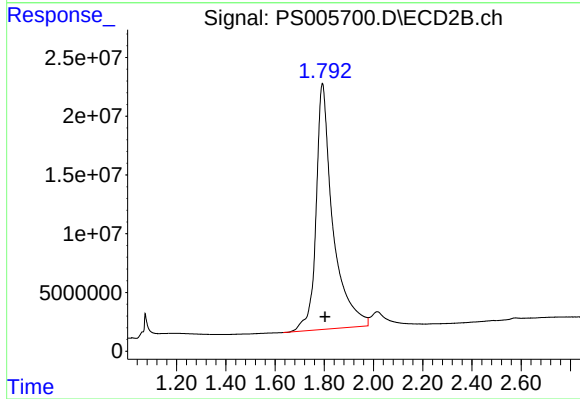


#1 Dalapon

R.T.: 1.793 min
Delta R.T.: -0.010 min
Response: 991520722
Conc: 687.51 ng/ml

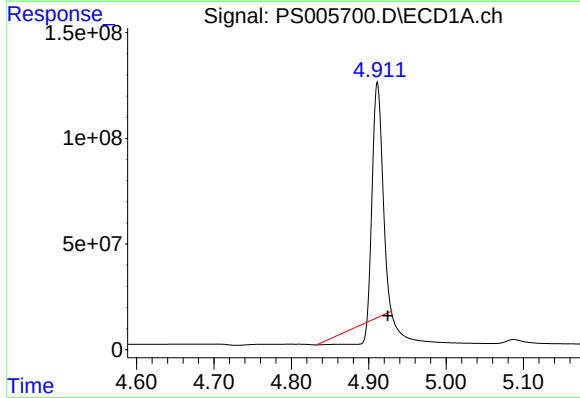


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.911 min
Delta R.T.: -0.013 min
Response: 834398568
Conc: 392.17 ng/ml

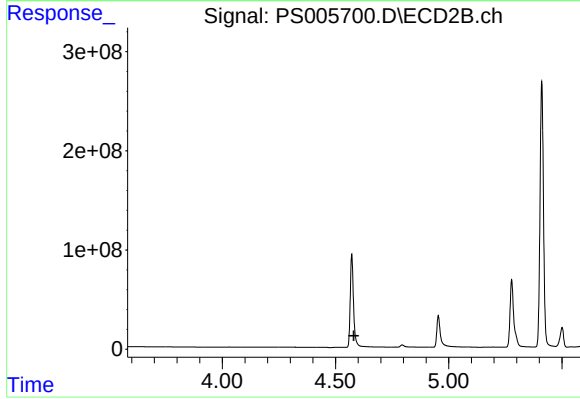

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.581 min
Response: 0
Conc: N.D.

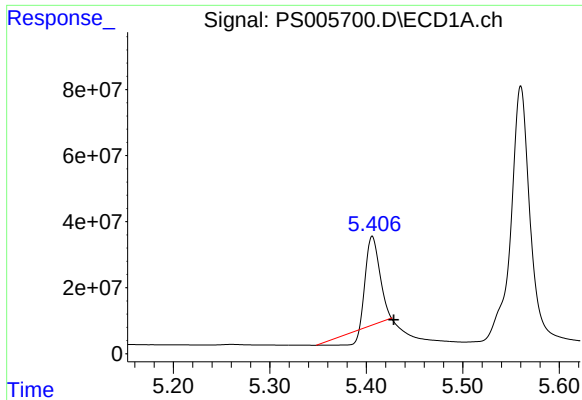

#3 4-Nitrophenol


R.T.: 5.406 min
Delta R.T.: -0.022 min
Response: 218129627
Conc: 305.13 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

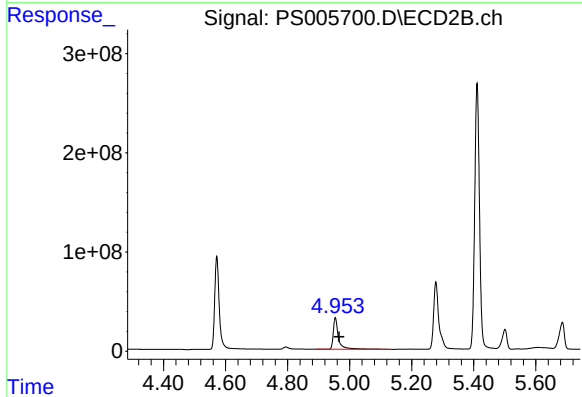


#3 4-Nitrophenol

R.T.: 4.954 min
Delta R.T.: -0.012 min
Response: 378314380
Conc: 763.44 ng/ml

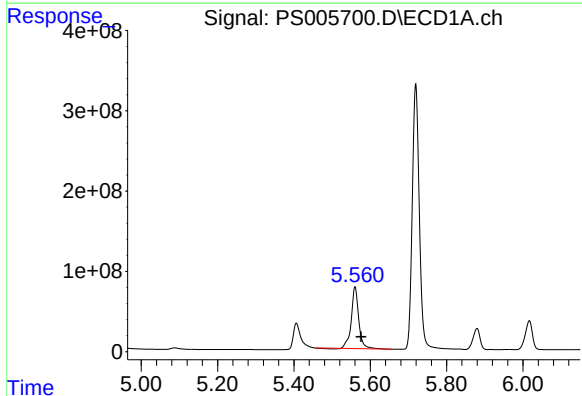


#4 2,4-DCAA

R.T.: 5.560 min
Delta R.T.: -0.016 min
Response: 1053242986
Conc: 668.41 ng/ml

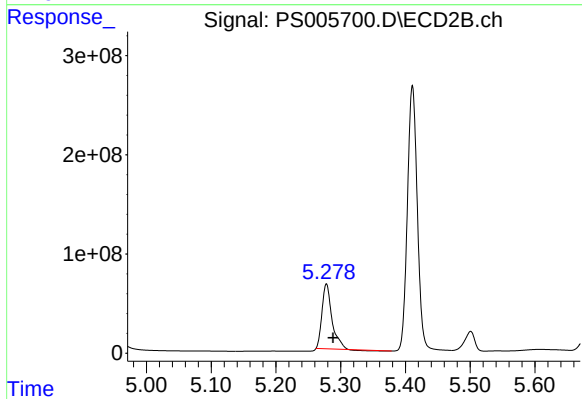

#4 2,4-DCAA


R.T.: 5.278 min
Delta R.T.: -0.010 min
Response: 686730529
Conc: 664.86 ng/ml

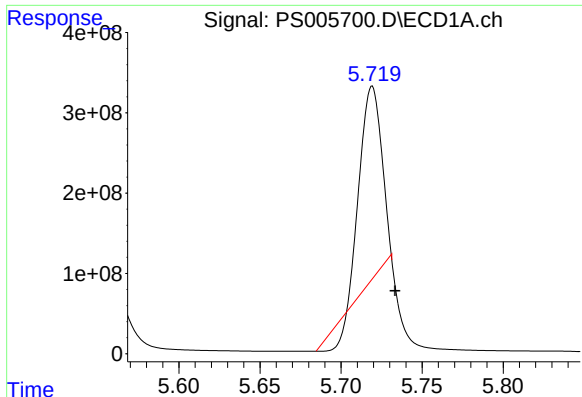

#5 DICAMBA


R.T.: 5.719 min
Delta R.T.: -0.014 min
Response: 2093448111
Conc: 338.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

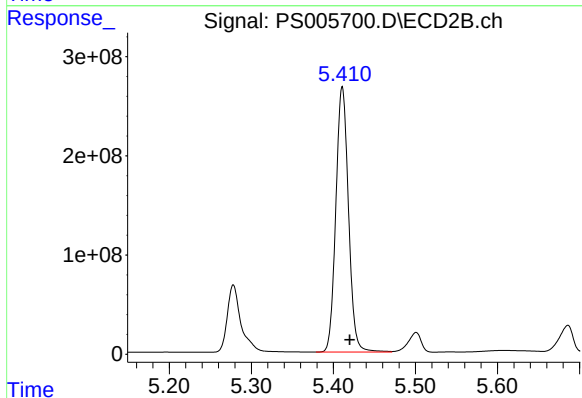


#5 DICAMBA

R.T.: 5.411 min
Delta R.T.: -0.009 min
Response: 2865078451
Conc: 724.03 ng/ml

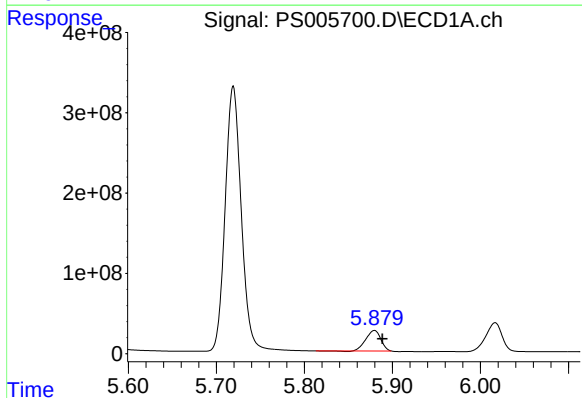


#6 MCP

R.T.: 5.879 min
Delta R.T.: -0.009 min
Response: 301153741
Conc: 62.01 ug/ml

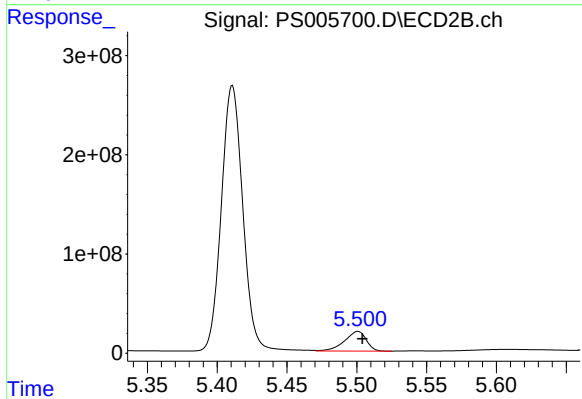

#6 MCP


R.T.: 5.501 min
Delta R.T.: -0.003 min
Response: 215940145
Conc: 74.53 ug/ml

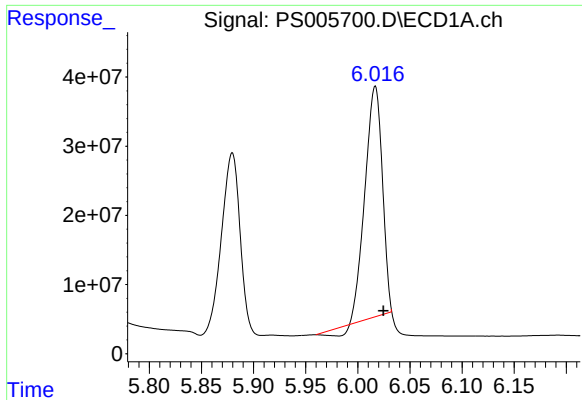

#7 MCPA


R.T.: 6.017 min
Delta R.T.: -0.008 min
Response: 376761012
Conc: 55.74 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

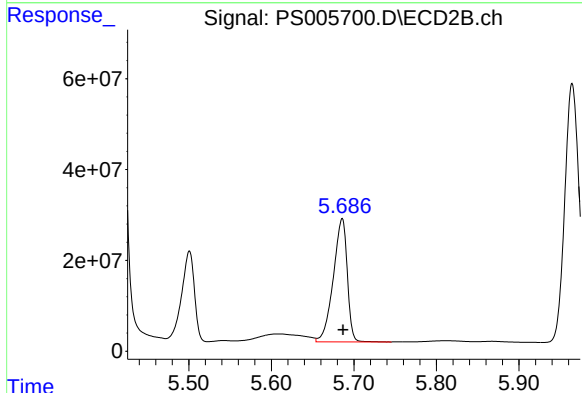


#7 MCPA

R.T.: 5.685 min
Delta R.T.: -0.002 min
Response: 318927148
Conc: 72.38 ug/ml

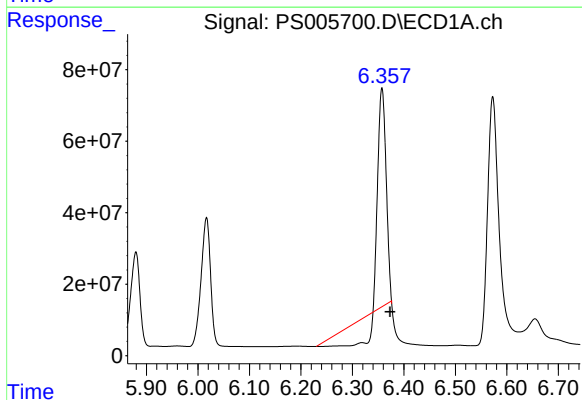


#8 DICHLORPROP

R.T.: 6.358 min
Delta R.T.: -0.016 min
Response: 425161750
Conc: 279.71 ng/ml

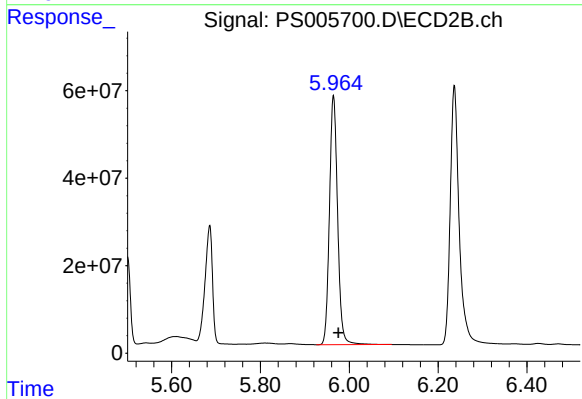

#8 DICHLORPROP


R.T.: 5.965 min
Delta R.T.: -0.011 min
Response: 726138333
Conc: 711.85 ng/ml

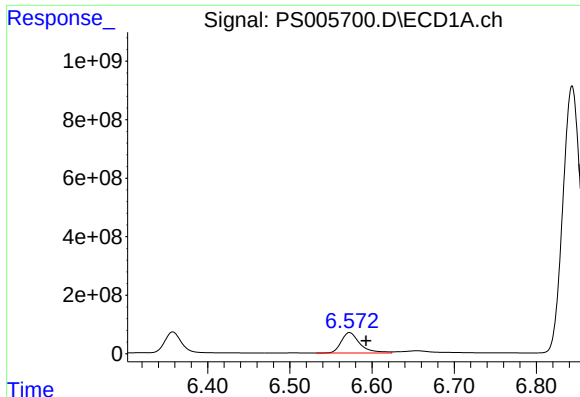

#9 2,4-D


R.T.: 6.573 min
Delta R.T.: -0.020 min
Response: 1105314035
Conc: 630.28 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

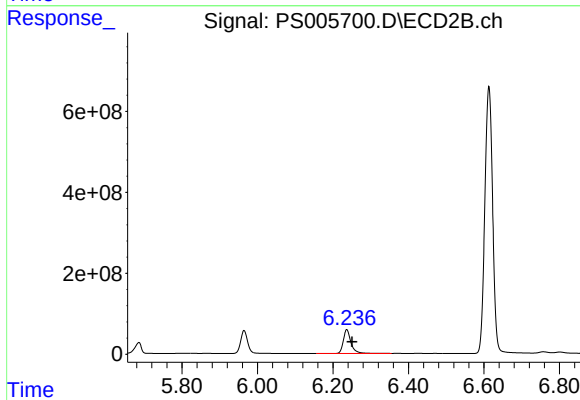


#9 2,4-D

R.T.: 6.237 min
Delta R.T.: -0.014 min
Response: 822624954
Conc: 704.49 ng/ml

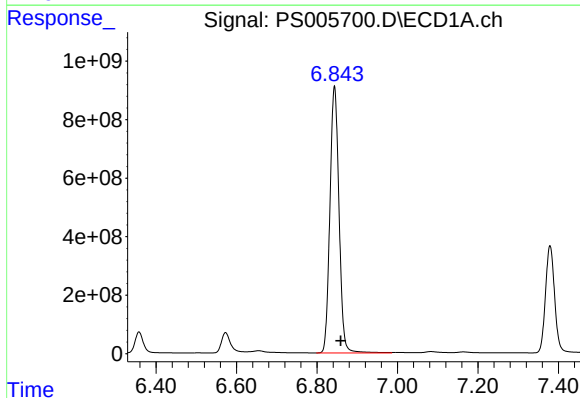


#10 Pentachlorophenol

R.T.: 6.843 min
Delta R.T.: -0.016 min
Response: 14309172646
Conc: 660.87 ng/ml

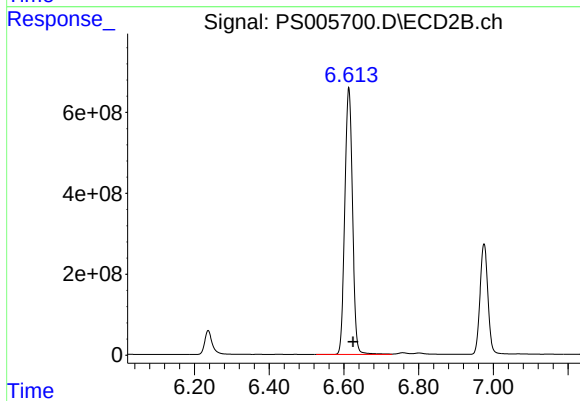

#10 Pentachlorophenol


R.T.: 6.613 min
Delta R.T.: -0.011 min
Response: 9470537413
Conc: 704.10 ng/ml

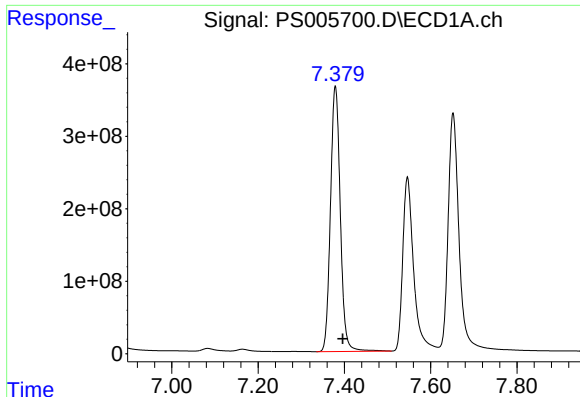

#11 2,4,5-TP (SILVEX)


R.T.: 7.379 min
Delta R.T.: -0.017 min
Response: 5786978622
Conc: 653.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

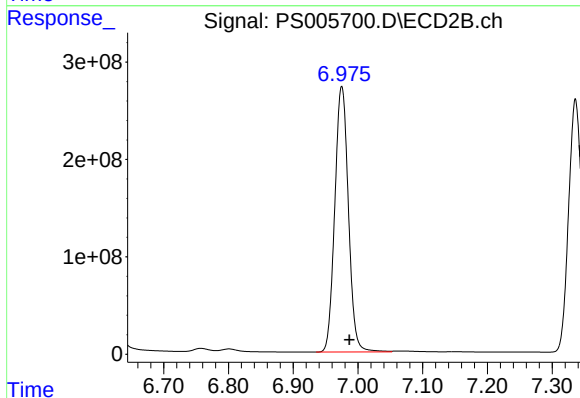


#11 2,4,5-TP (SILVEX)

R.T.: 6.975 min
Delta R.T.: -0.012 min
Response: 3986918008
Conc: 715.35 ng/ml

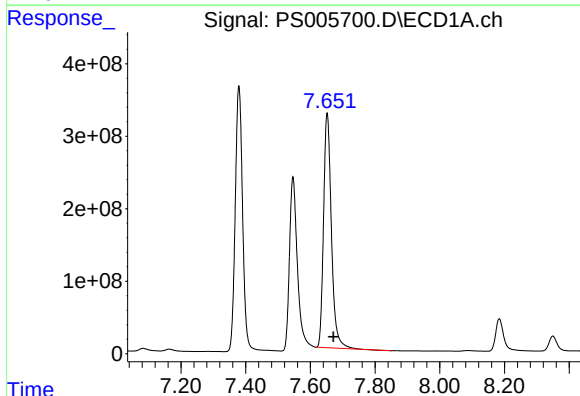


#12 2,4,5-T

R.T.: 7.652 min
Delta R.T.: -0.020 min
Response: 5400124932
Conc: 637.88 ng/ml

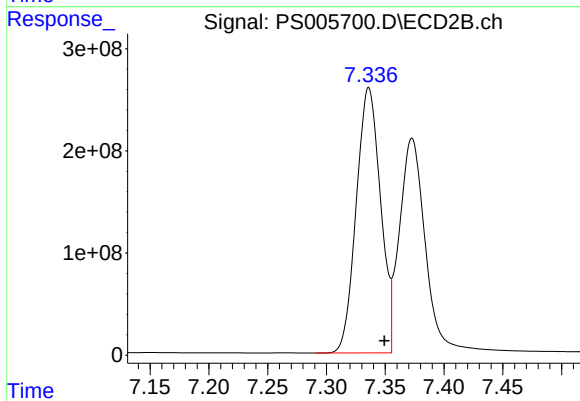

#12 2,4,5-T


R.T.: 7.336 min
Delta R.T.: -0.013 min
Response: 3732753541
Conc: 727.42 ng/ml

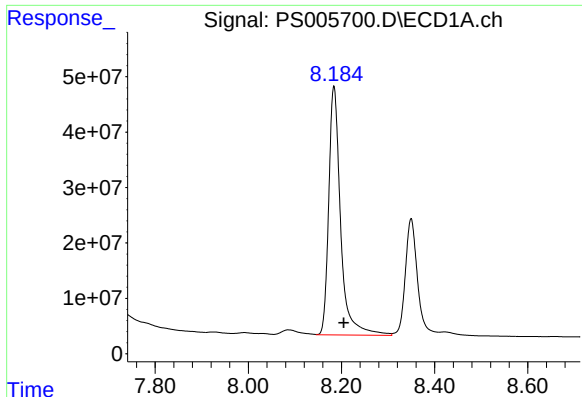

#13 2,4-DB


R.T.: 8.184 min
Delta R.T.: -0.021 min
Response: 797067235
Conc: 636.28 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

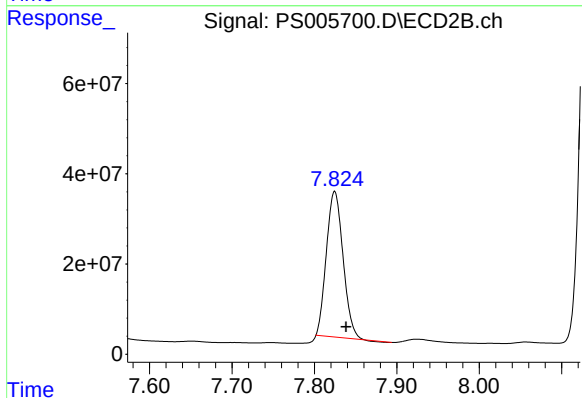


#13 2,4-DB

R.T.: 7.825 min
Delta R.T.: -0.014 min
Response: 452179569
Conc: 656.33 ng/ml

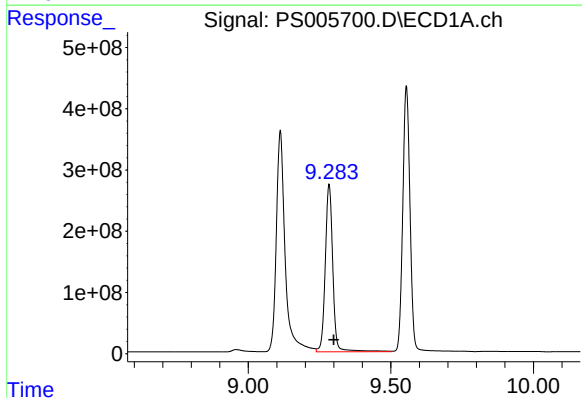


#14 DINOSEB

R.T.: 9.283 min
Delta R.T.: -0.017 min
Response: 5051898082
Conc: 724.24 ng/ml

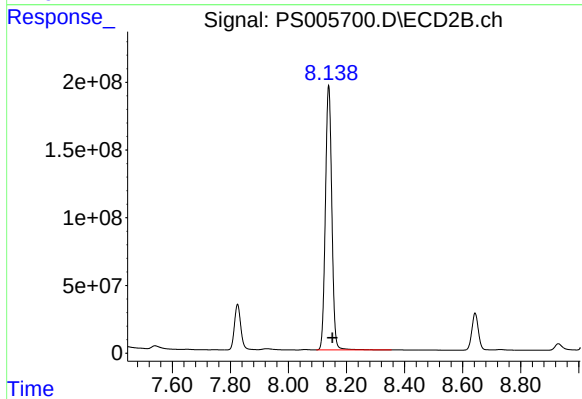

#14 DINOSEB


R.T.: 8.139 min
Delta R.T.: -0.013 min
Response: 2982259560
Conc: 736.62 ng/ml

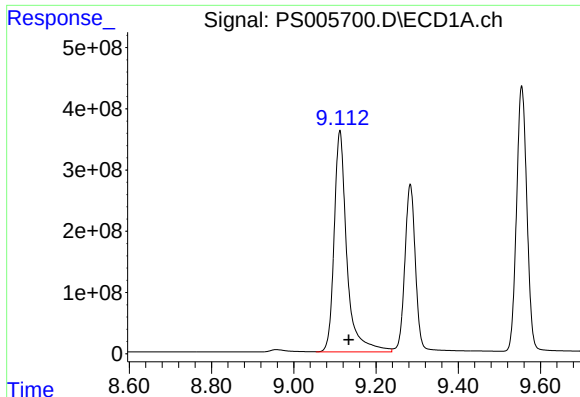

#15 Picloram


R.T.: 9.112 min
Delta R.T.: -0.021 min
Response: 7784509319
Conc: 624.83 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

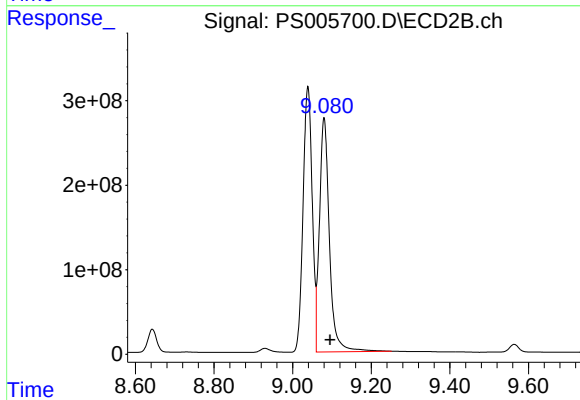


#15 Picloram

R.T.: 9.080 min
Delta R.T.: -0.016 min
Response: 4871630034
Conc: 621.95 ng/ml

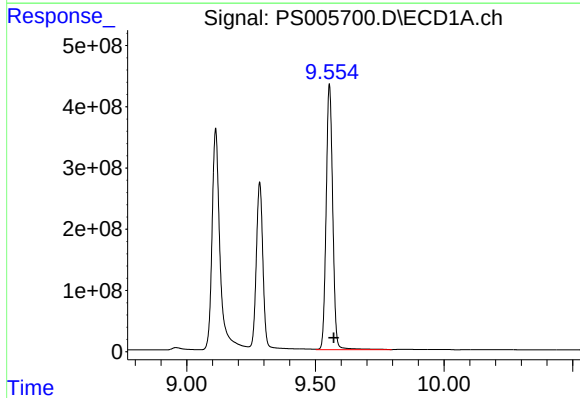

#16 DCPA

R.T.: 9.554 min
Delta R.T.: -0.018 min
Response: 7713043105
Conc: 708.32 ng/ml

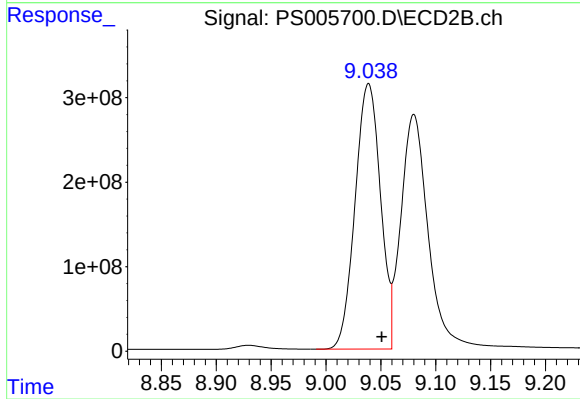

#16 DCPA

R.T.: 9.039 min
Delta R.T.: -0.012 min
Response: 5057269234
Conc: 715.46 ng/ml