

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072919\
 Data File : PS005756.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2019 10:07
 Operator : SM\AJ
 Sample : K3620-12
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 02:04:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.558	5.276	328.6E6	231.8E6	226.499	233.084
Target Compounds							
2) T	3,5-DICHL...	0.000	4.595	0	82621332	N.D.	63.686
5) T	DICAMBA	5.779	5.383	32987327	3841331	5.523	1.029 #
7) T	MCPA	5.954	0.000	52620594	0	8.064	N.D. #
8) T	DICHLORPROP	0.000	5.966	0	35395745	N.D.	38.327
9) T	2,4-D	6.636	0.000	132.0E6	0	88.086	N.D. #
12) T	2,4,5-T	0.000	7.381	0	20211113	N.D.	4.252
15) T	Picloram	9.127	9.083	224.1E6	150.6E6	19.148	20.053
16) T	DCPA	0.000	9.083	0	150.6E6	N.D.	22.845



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072919\
Data File : PS005756.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2019 10:07
Operator : SM\AJ
Sample : K3620-12
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 02:04:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

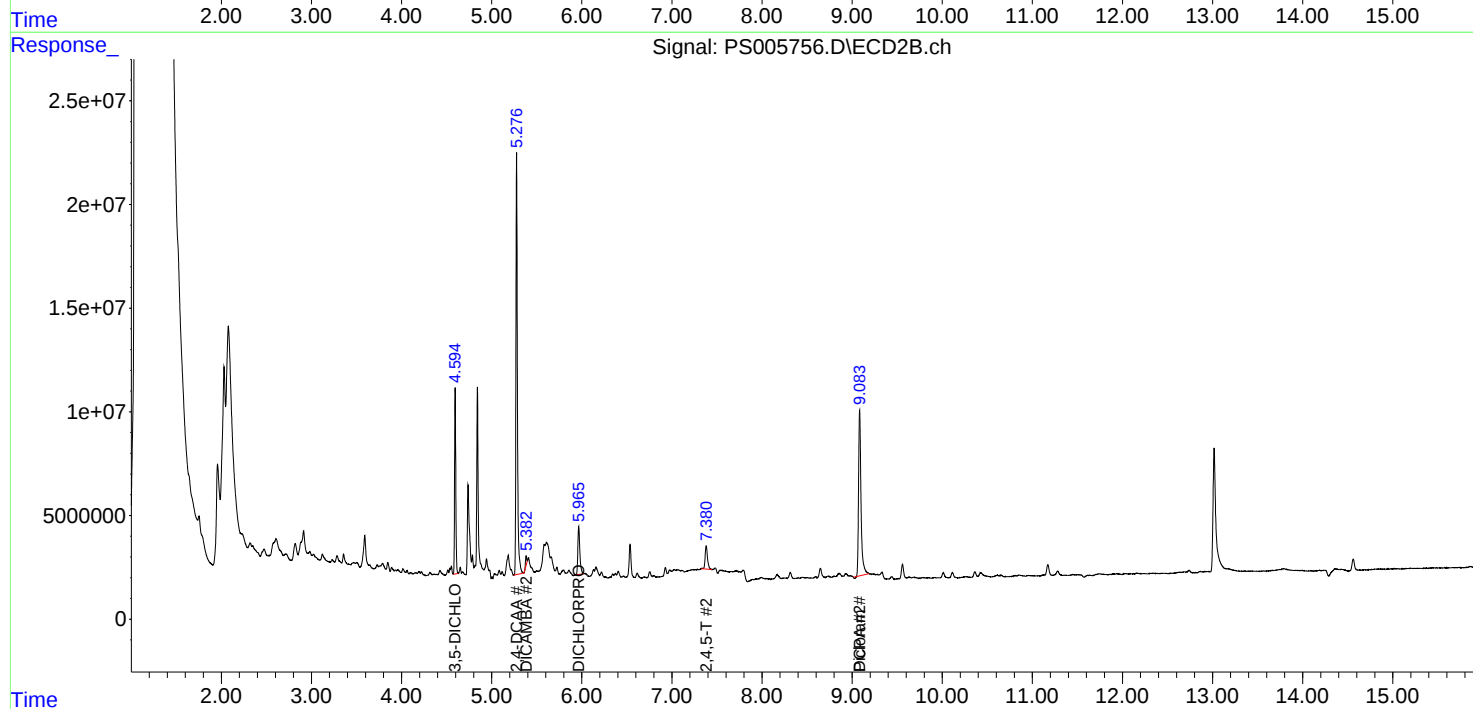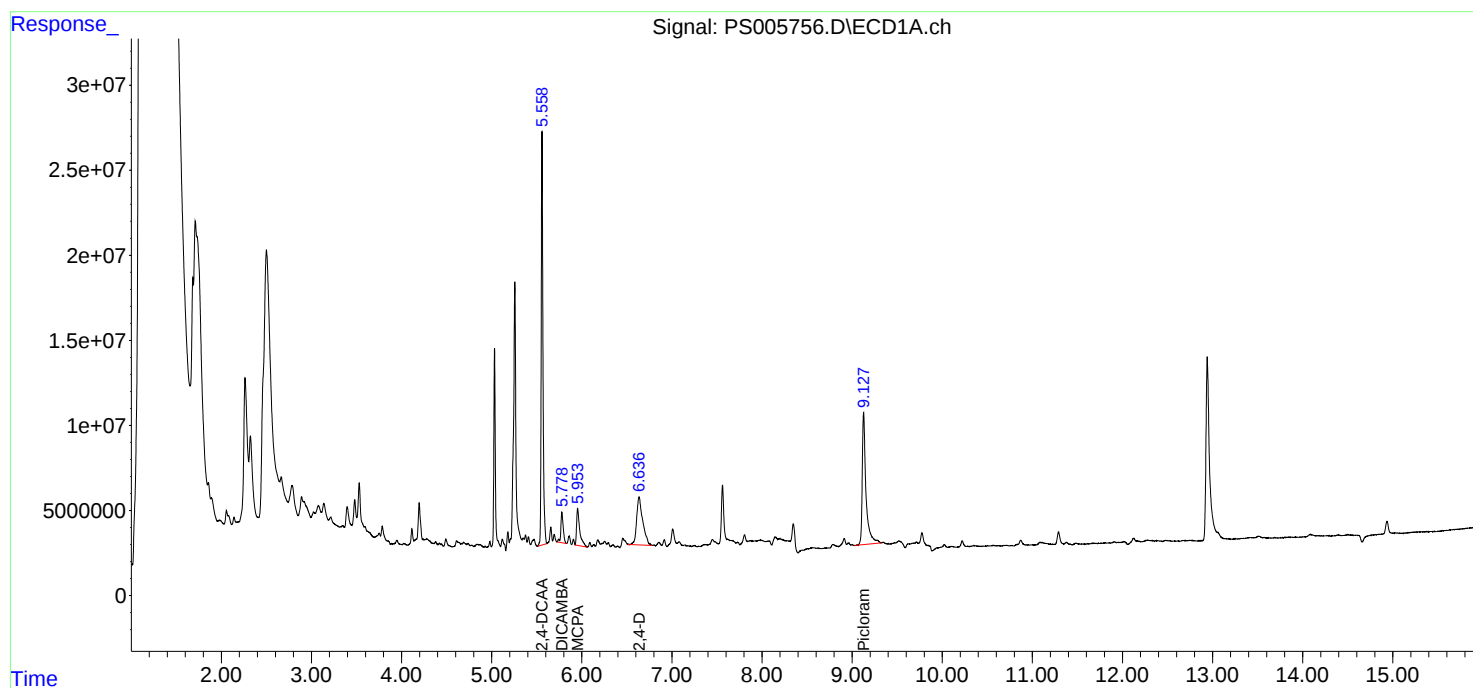


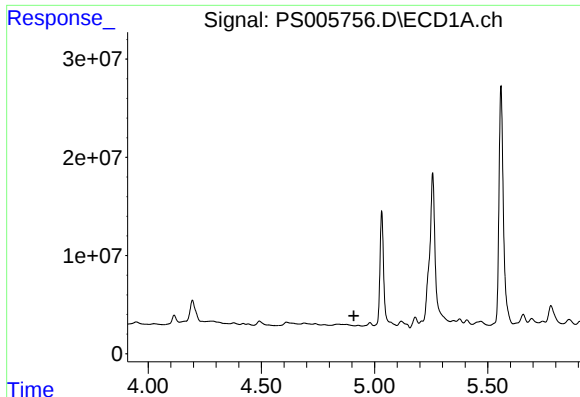

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

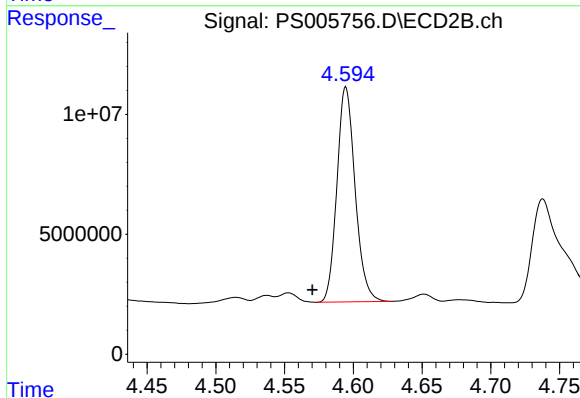


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.595 min
Delta R.T.: 0.025 min
Response: 82621332
Conc: 63.69 ng/ml

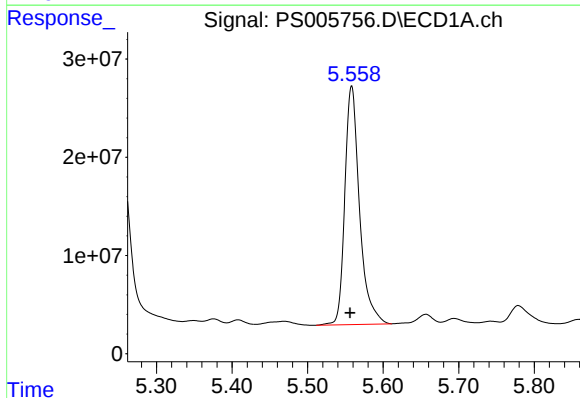


#4 2,4-DCAA

R.T.: 5.558 min
Delta R.T.: 0.002 min
Response: 328608303
Conc: 226.50 ng/ml

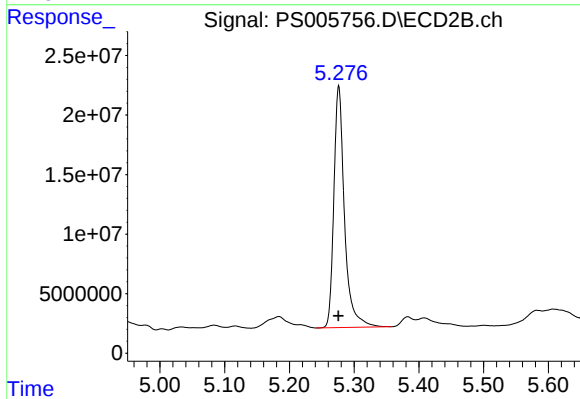

#4 2,4-DCAA


R.T.: 5.276 min
Delta R.T.: 0.000 min
Response: 231843622
Conc: 233.08 ng/ml

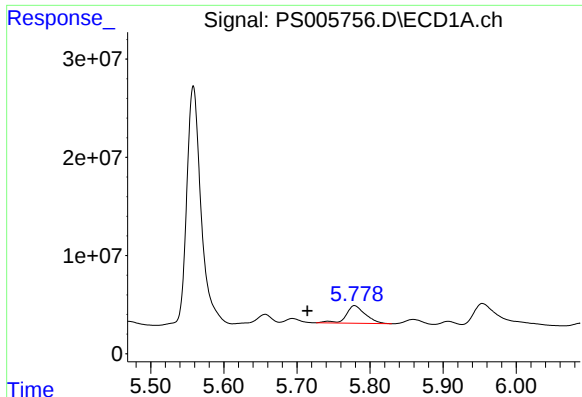

#5 DICAMBA


R.T.: 5.779 min
Delta R.T.: 0.065 min
Response: 32987327
Conc: 5.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

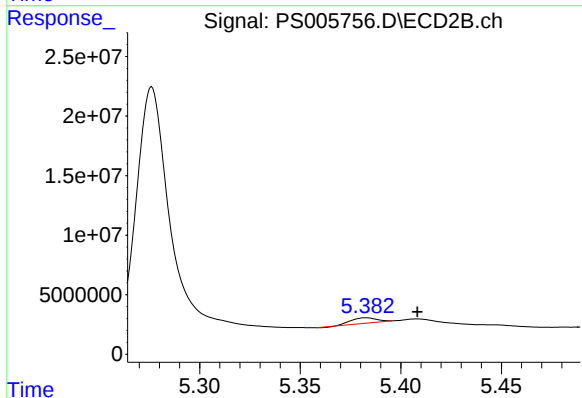


#5 DICAMBA

R.T.: 5.383 min
Delta R.T.: -0.025 min
Response: 3841331
Conc: 1.03 ng/ml

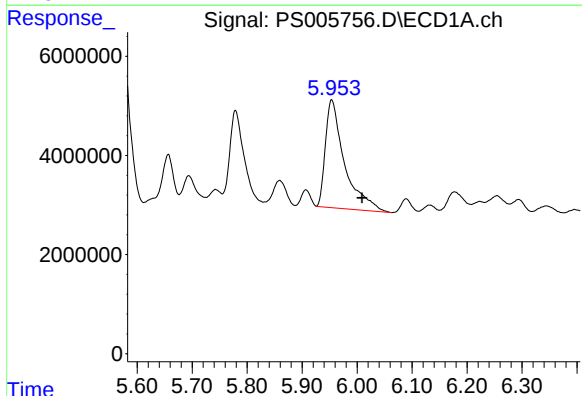


#7 MCPA

R.T.: 5.954 min
Delta R.T.: -0.055 min
Response: 52620594
Conc: 8.06 ug/ml

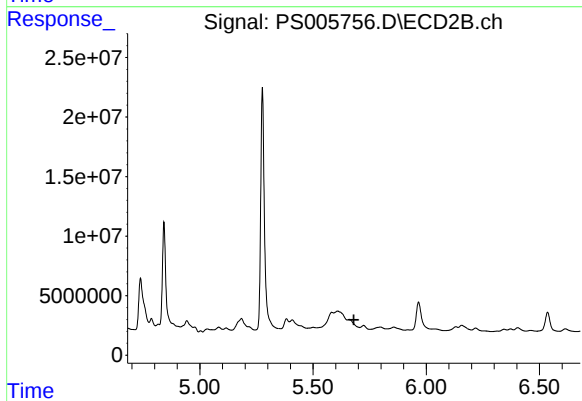

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.681 min
Response: 0
Conc: N.D.

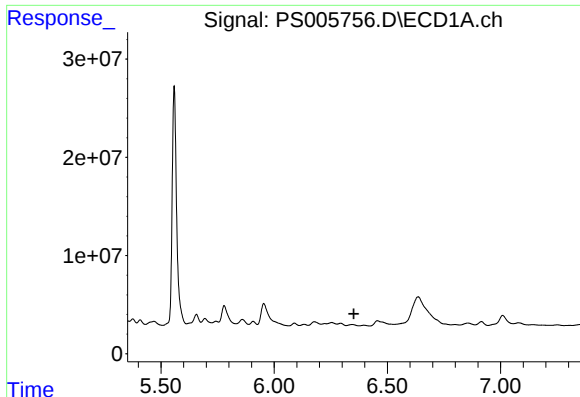

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

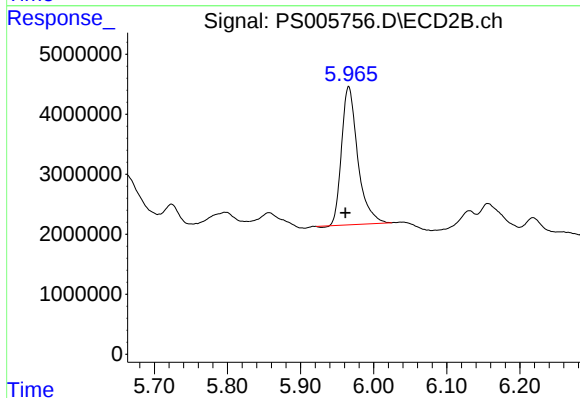


#8 DICHLORPROP

R.T.: 5.966 min
Delta R.T.: 0.005 min
Response: 35395745
Conc: 38.33 ng/ml

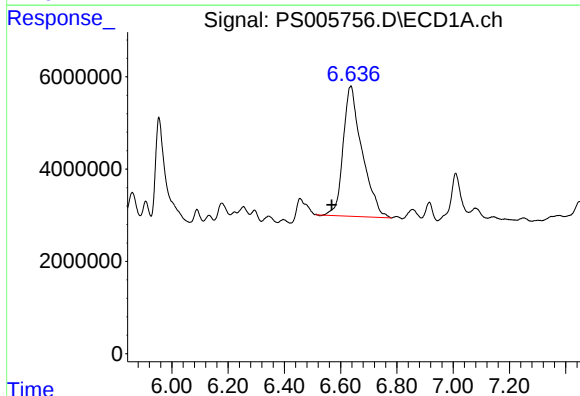


#9 2,4-D

R.T.: 6.636 min
Delta R.T.: 0.067 min
Response: 132011970
Conc: 88.09 ng/ml

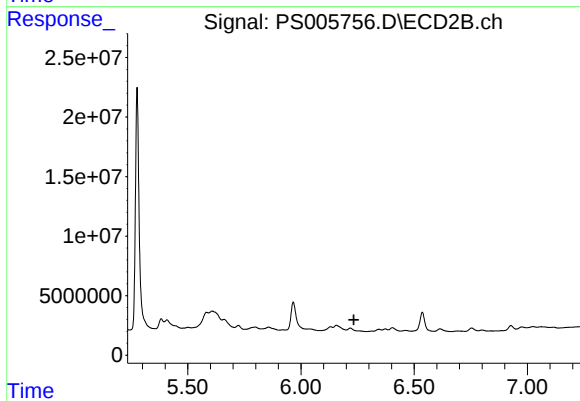

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.234 min
Response: 0
Conc: N.D.

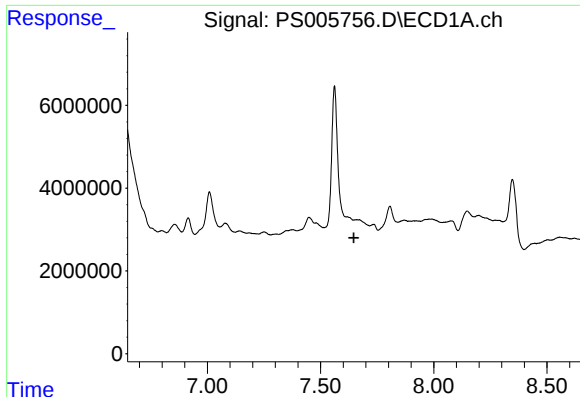

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.647 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

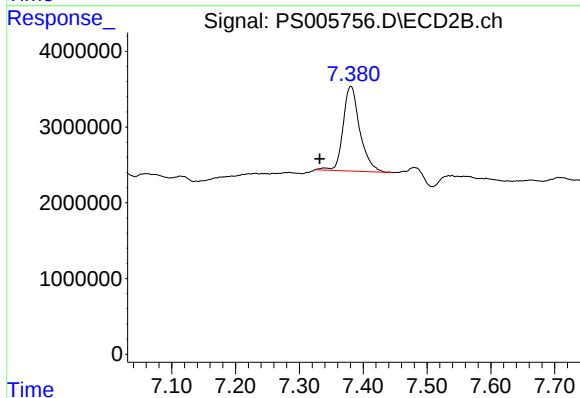


#12 2,4,5-T

R.T.: 7.381 min
Delta R.T.: 0.049 min
Response: 20211113
Conc: 4.25 ng/ml

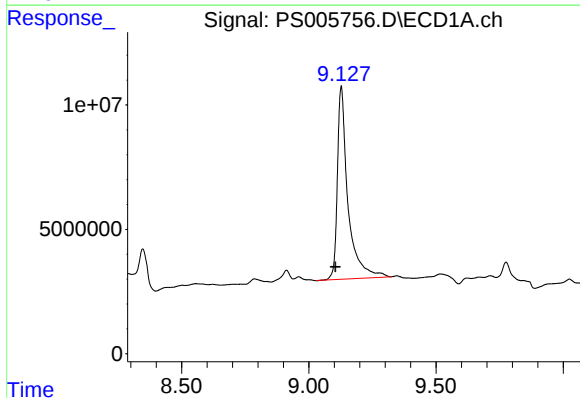


#15 Picloram

R.T.: 9.127 min
Delta R.T.: 0.023 min
Response: 224127265
Conc: 19.15 ng/ml

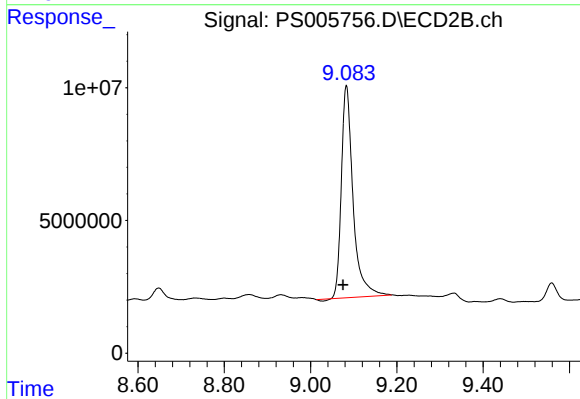

#15 Picloram


R.T.: 9.083 min
Delta R.T.: 0.008 min
Response: 150640357
Conc: 20.05 ng/ml

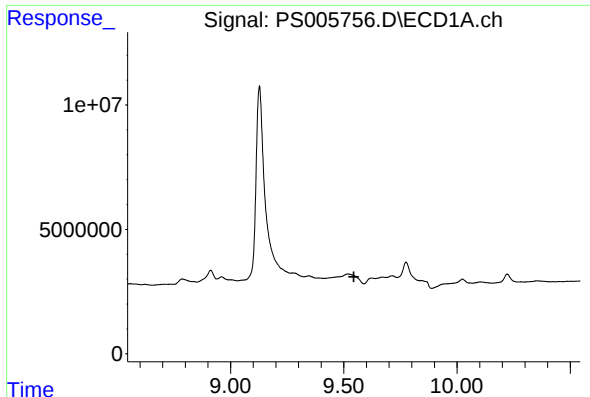

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

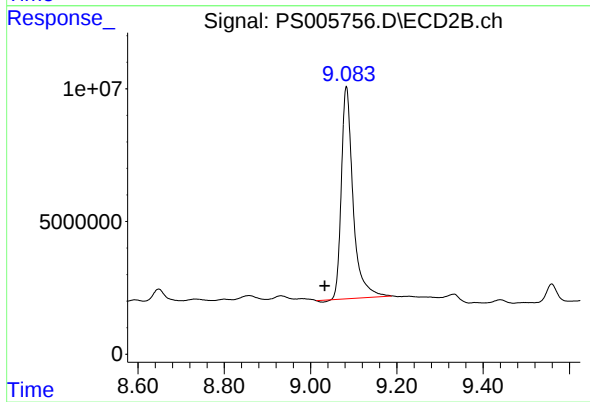

#16 DCPA

R.T.: 9.083 min
Delta R.T.: 0.050 min
Response: 150640357
Conc: 22.84 ng/ml