

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072919\
 Data File : PS005758.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2019 10:51
 Operator : SM\AJ
 Sample : K3620-16
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 02:05:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.588	5.307	300.9E6	214.1E6	207.373	215.279
Target Compounds							
1) T	Dalapon	2.086	0.000	20832055	0	11.240	N.D. #
2) T	3,5-DICHL...	0.000	4.626	0	51387932	N.D.	39.611
6) T	MCP	5.809	0.000	29262730	0	6.316	N.D. #
7) T	MCPA	5.985	5.639	105.7E6	85684770	16.201	20.357 #
8) T	DICHLORPROP	0.000	5.997	0	72680747	N.D.	78.700
10) T	Pentachlo...	0.000	6.566	0	25342685	N.D.	1.952
12) T	2,4,5-T	7.590	0.000	36027938	0	4.316	N.D. #
15) T	Picloram	9.118	0.000	110.1E6	0	9.405	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072919\
Data File : PS005758.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2019 10:51
Operator : SM\AJ
Sample : K3620-16
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 02:05:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

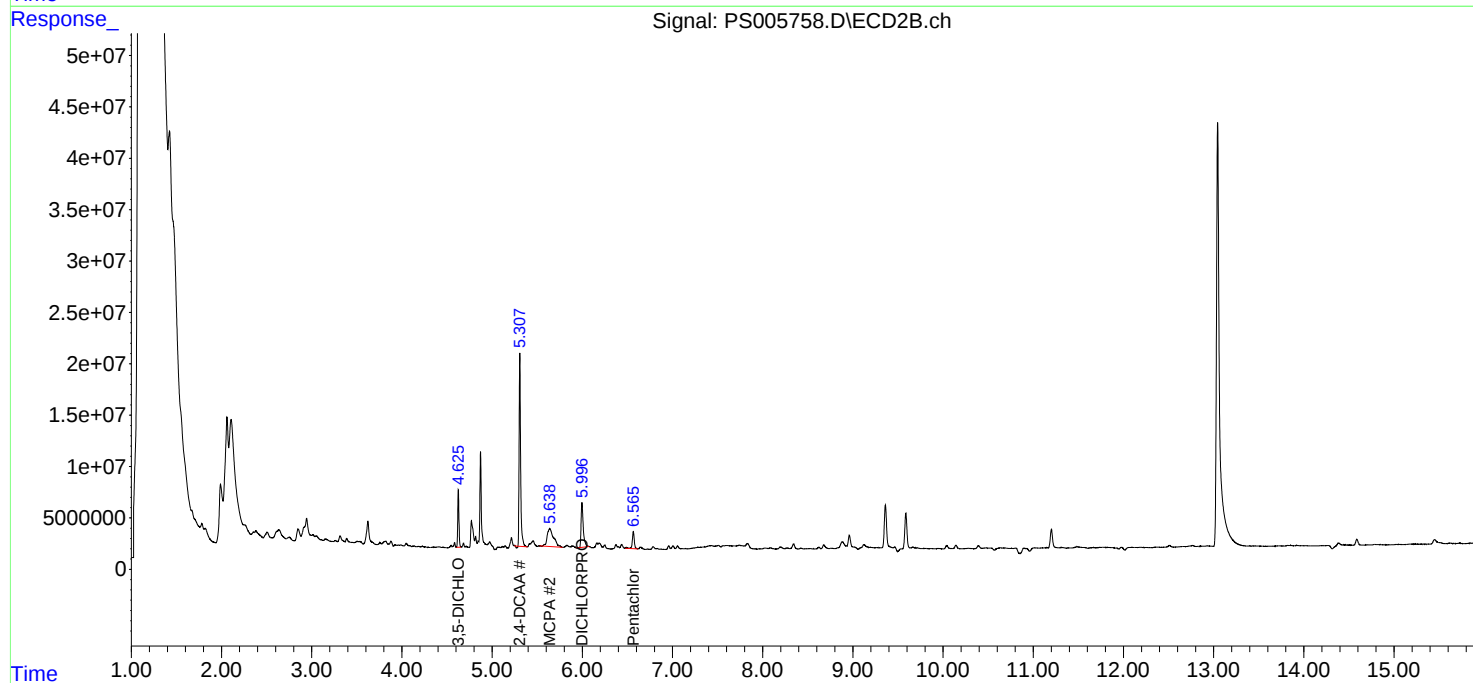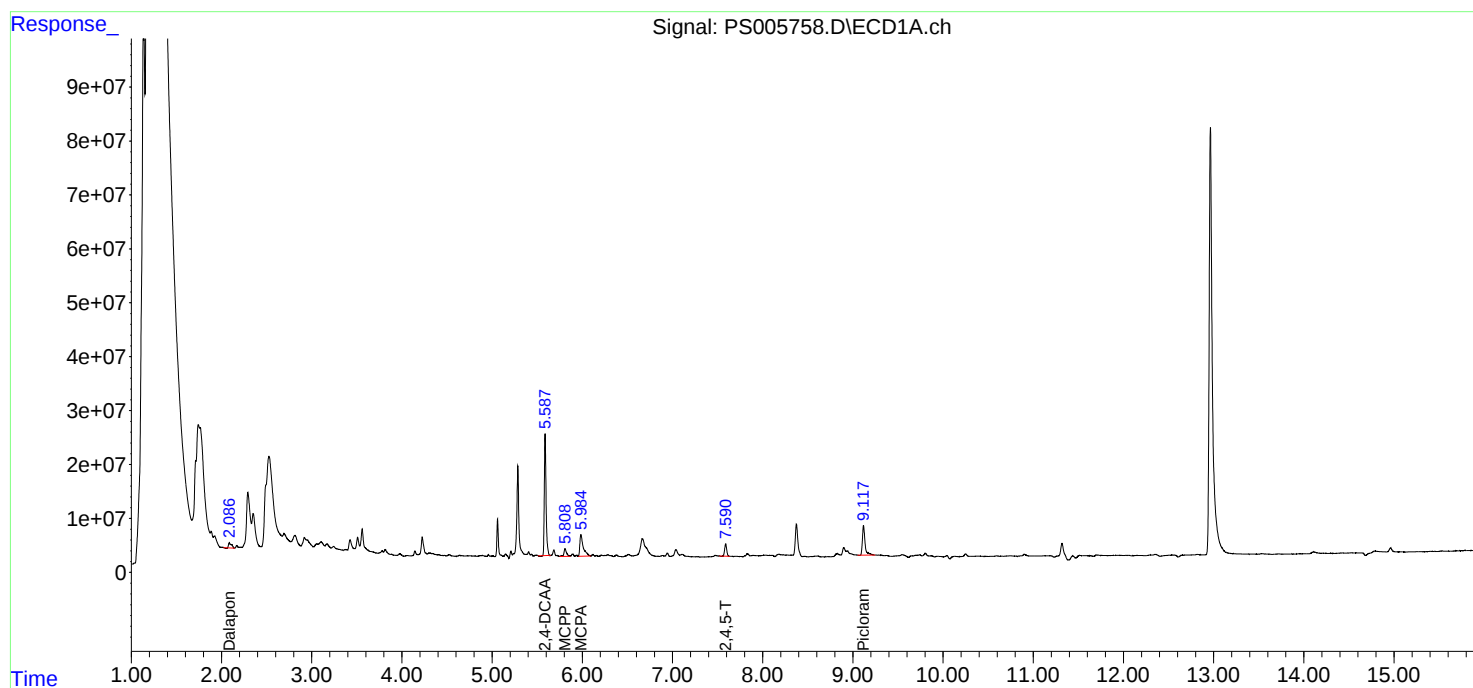


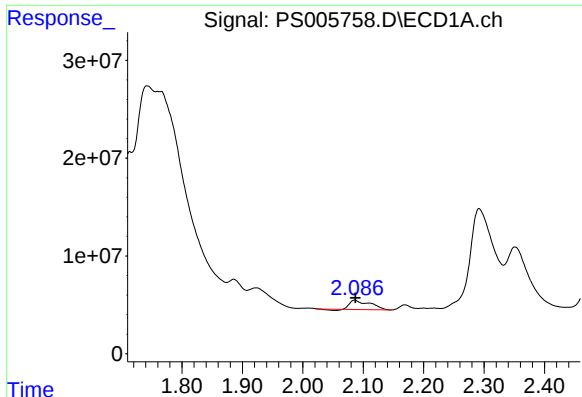

#1 Dalapon


R.T.: 2.086 min
Delta R.T.: 0.000 min
Response: 20832055
Conc: 11.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

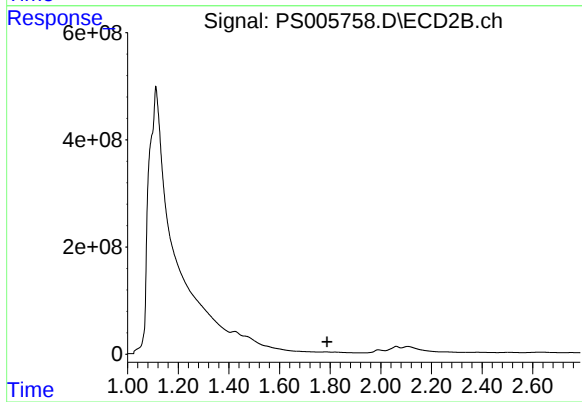


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

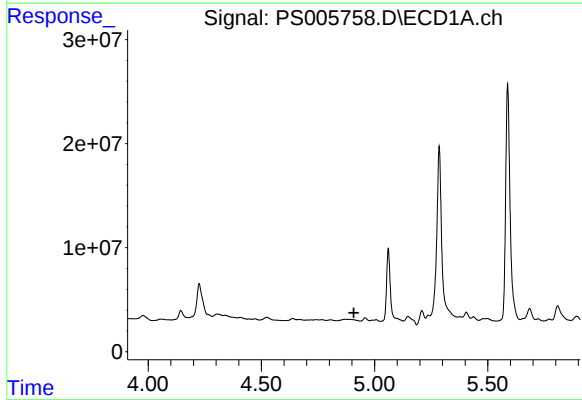


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.909 min
Response: 0
Conc: N.D.

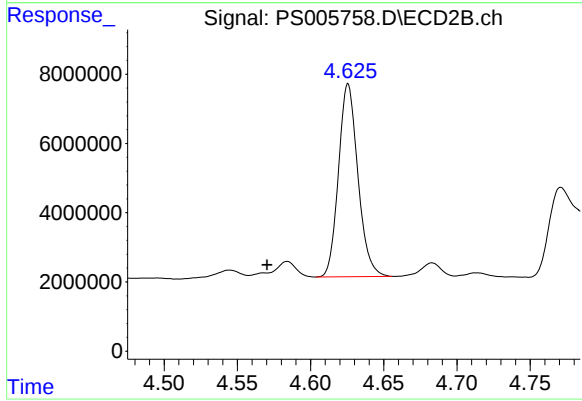

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.626 min
Delta R.T.: 0.056 min
Response: 51387932
Conc: 39.61 ng/ml

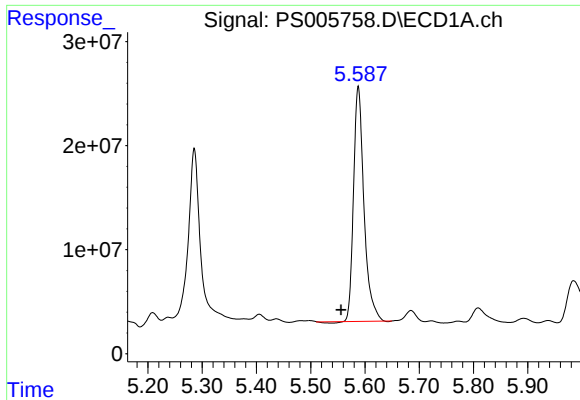

#4 2,4-DCAA


R.T.: 5.588 min
Delta R.T.: 0.032 min
Response: 300861121
Conc: 207.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

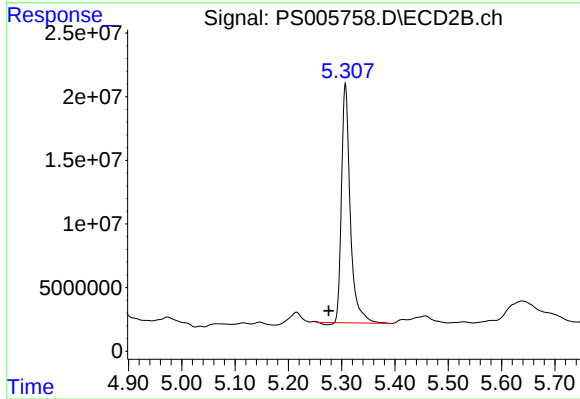


#4 2,4-DCAA

R.T.: 5.307 min
Delta R.T.: 0.031 min
Response: 214133106
Conc: 215.28 ng/ml

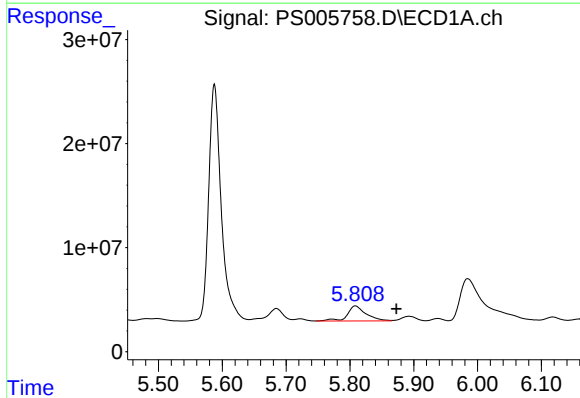


#6 MCP

R.T.: 5.809 min
Delta R.T.: -0.064 min
Response: 29262730
Conc: 6.32 ug/ml

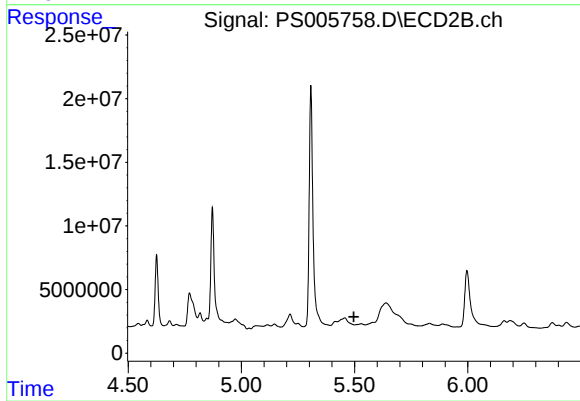

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

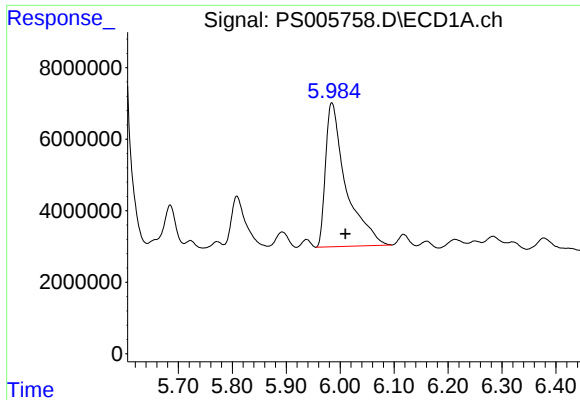

#7 MCPA


R.T.: 5.985 min
Delta R.T.: -0.024 min
Response: 105718545
Conc: 16.20 ug/ml

Instrument :
ECD_S
ClientSampleId :

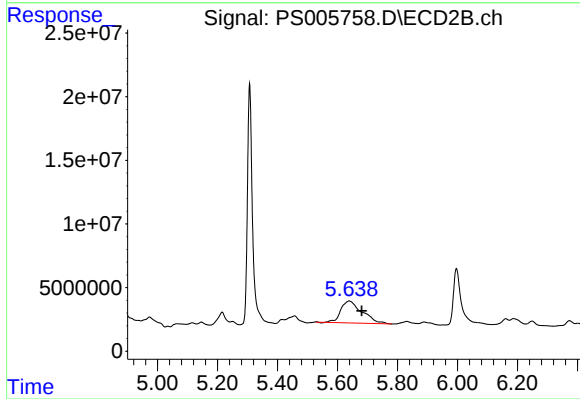


#7 MCPA

R.T.: 5.639 min
Delta R.T.: -0.042 min
Response: 85684770
Conc: 20.36 ug/ml

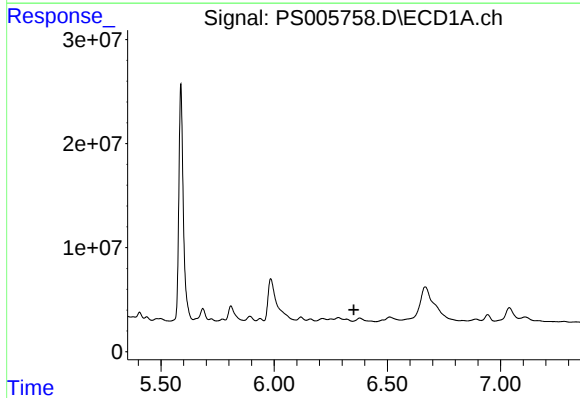


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.352 min
Response: 0
Conc: N.D.

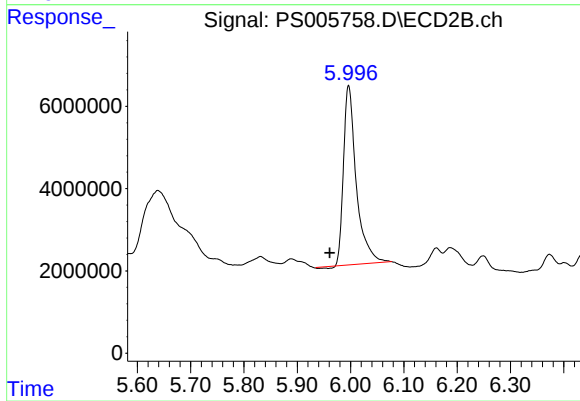

#8 DICHLORPROP


R.T.: 5.997 min
Delta R.T.: 0.035 min
Response: 72680747
Conc: 78.70 ng/ml

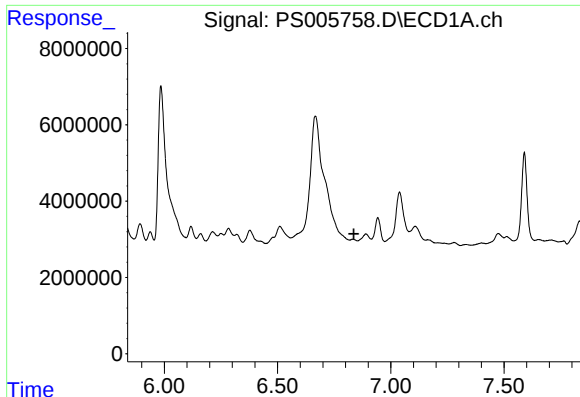

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

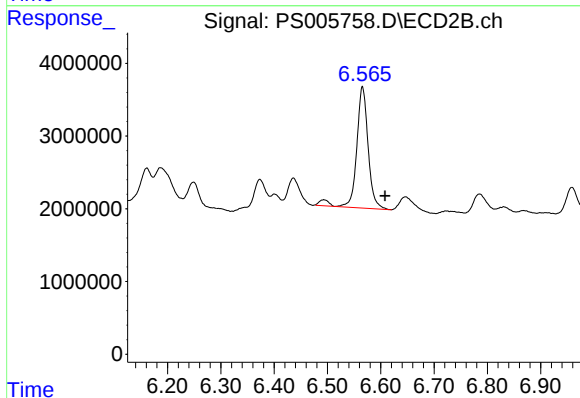


#10 Pentachlorophenol

R.T.: 6.566 min
Delta R.T.: -0.043 min
Response: 25342685
Conc: 1.95 ng/ml

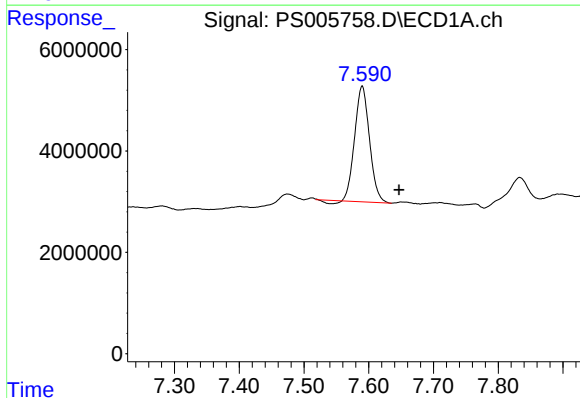


#12 2,4,5-T

R.T.: 7.590 min
Delta R.T.: -0.057 min
Response: 36027938
Conc: 4.32 ng/ml

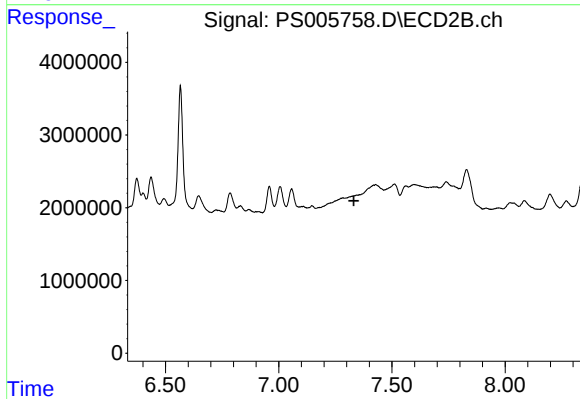

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.332 min
Response: 0
Conc: N.D.

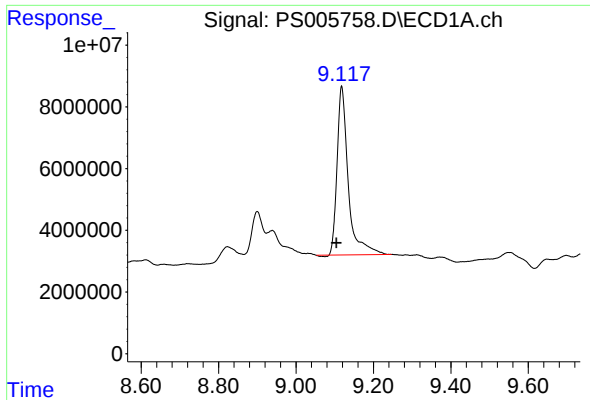

#15 Picloram

R.T.: 9.118 min
Delta R.T.: 0.014 min
Response: 110082847
Conc: 9.40 ng/ml

Instrument :
ECD_S
ClientSampleId :

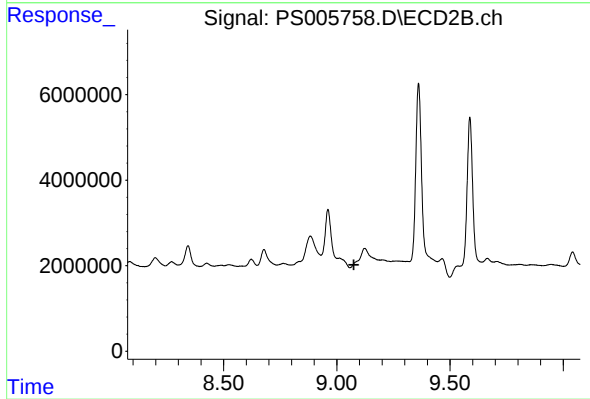

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.075 min
Response: 0
Conc: N.D.