

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072919\
 Data File : PS005759.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2019 11:13
 Operator : SM\AJ
 Sample : K3620-18
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 02:05:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.560	5.279	317.2E6	226.0E6	218.617	227.255
Target Compounds							
1) T	Dalapon	2.058	0.000	23308964	0	12.577	N.D. #
2) T	3,5-DICHL...	4.931	4.597	9361346	55624496	4.513	42.877 #
5) T	DICAMBA	5.781	5.430	27751445	24921767	4.647	6.676 #
6) T	MCP	0.000	5.430	0	24921767	N.D.	8.750
7) T	MCPA	5.948	0.000	346.2E6	0	53.051	N.D. #
8) T	DICHLORPROP	6.348	5.965	27277734	248.0E6	18.968	268.506 #
11) T	2,4,5-TP ...	0.000	6.975	0	16727236	N.D.	3.225
15) T	Picloram	9.086	0.000	376.8E6	0	32.187	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072919\
Data File : PS005759.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2019 11:13
Operator : SM\AJ
Sample : K3620-18
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 02:05:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

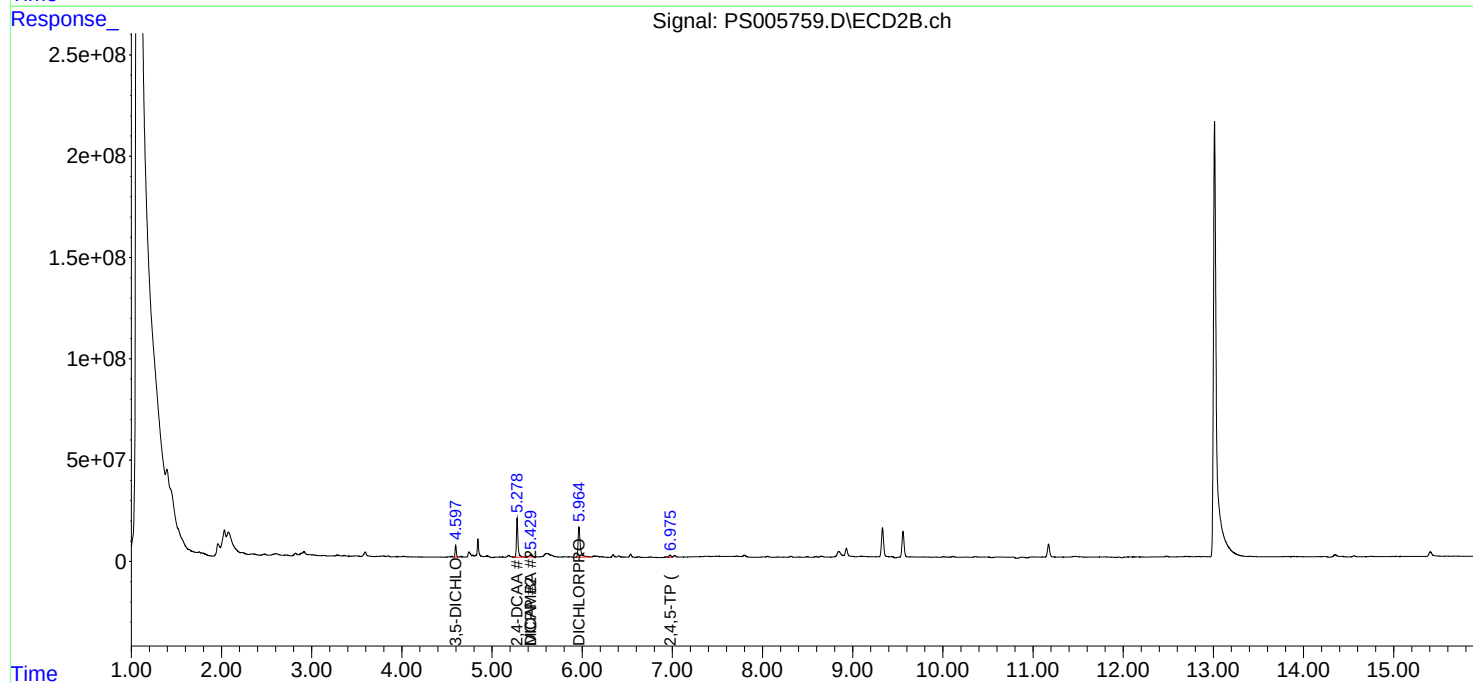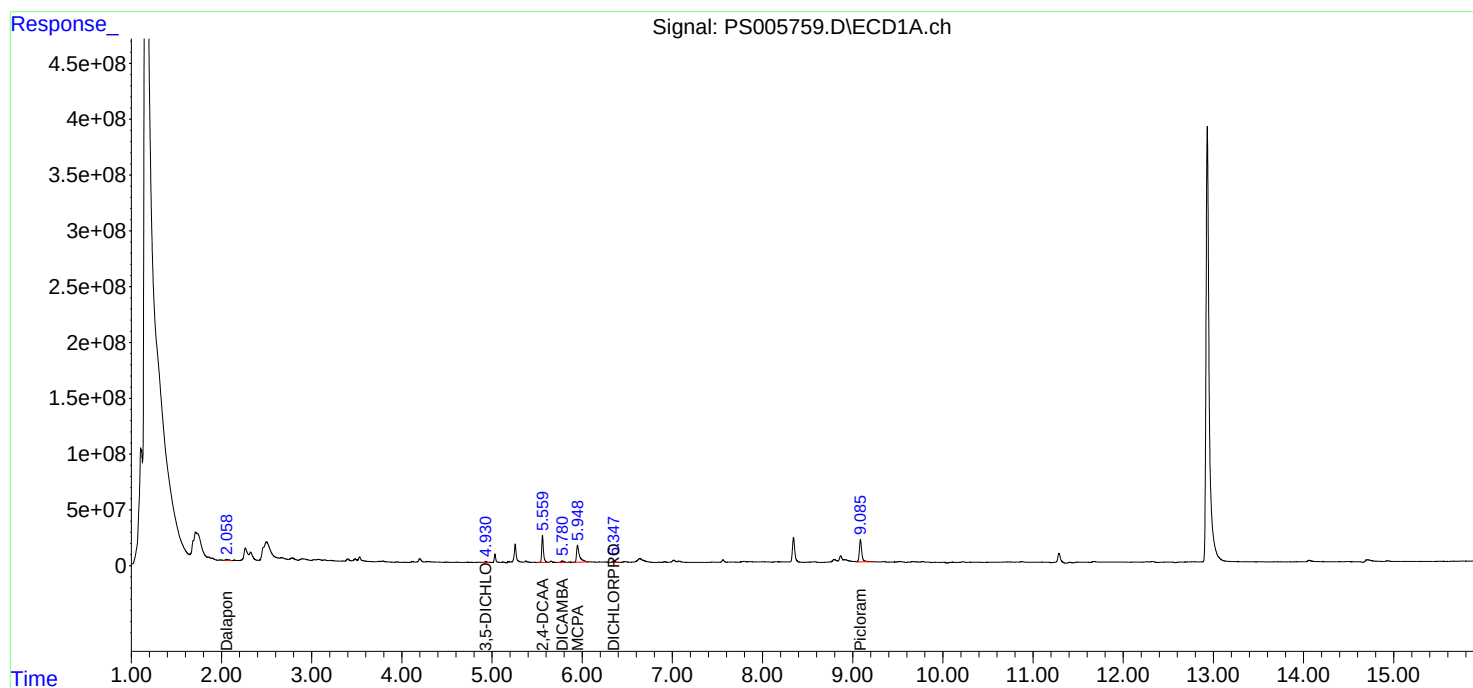


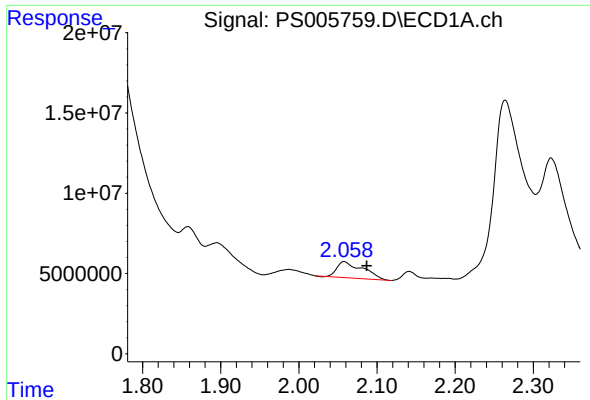

#1 Dalapon


R.T.: 2.058 min
Delta R.T.: -0.029 min
Response: 23308964
Conc: 12.58 ng/ml

Instrument :
ECD_S
ClientSampleId :

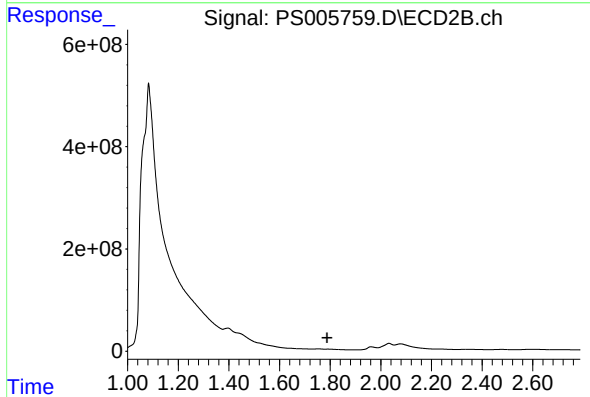


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

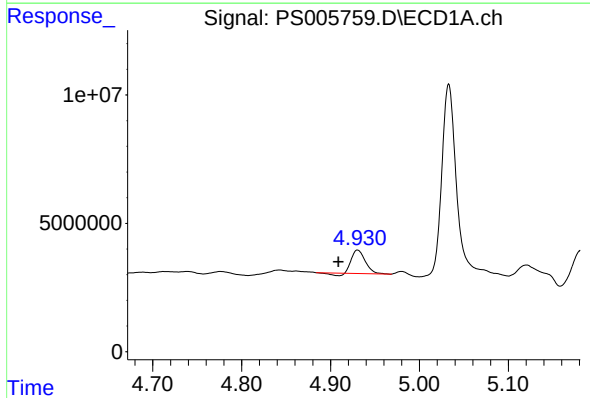


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.931 min
Delta R.T.: 0.022 min
Response: 9361346
Conc: 4.51 ng/ml

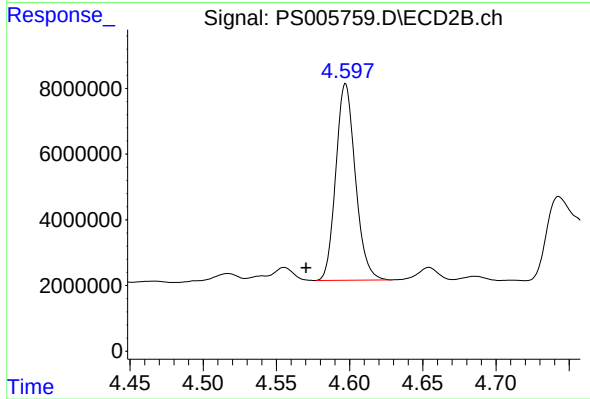

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.597 min
Delta R.T.: 0.027 min
Response: 55624496
Conc: 42.88 ng/ml

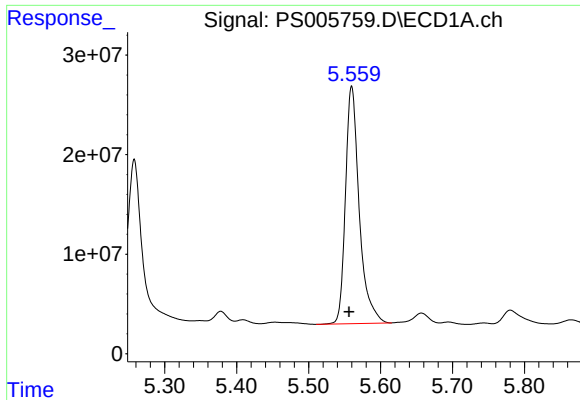

#4 2,4-DCAA


R.T.: 5.560 min
Delta R.T.: 0.004 min
Response: 317174014
Conc: 218.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

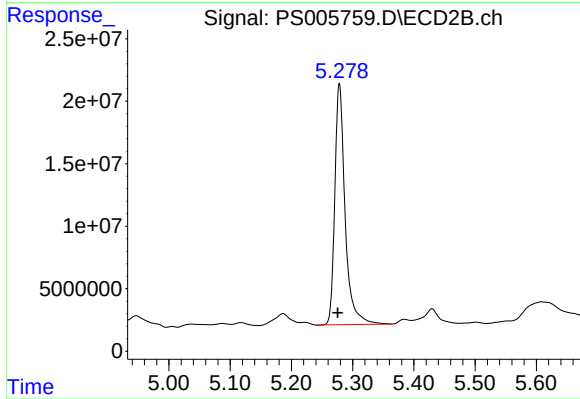


#4 2,4-DCAA

R.T.: 5.279 min
Delta R.T.: 0.003 min
Response: 226045399
Conc: 227.25 ng/ml

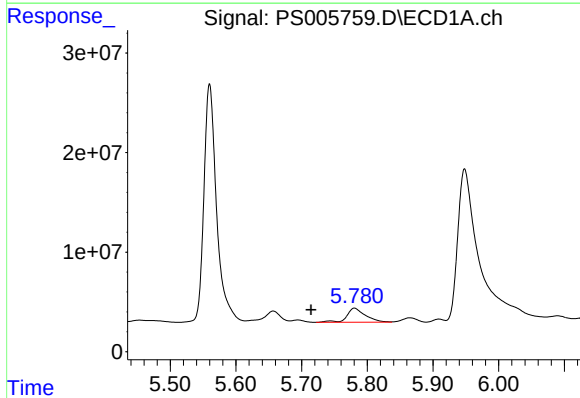


#5 DICAMBA

R.T.: 5.781 min
Delta R.T.: 0.066 min
Response: 27751445
Conc: 4.65 ng/ml

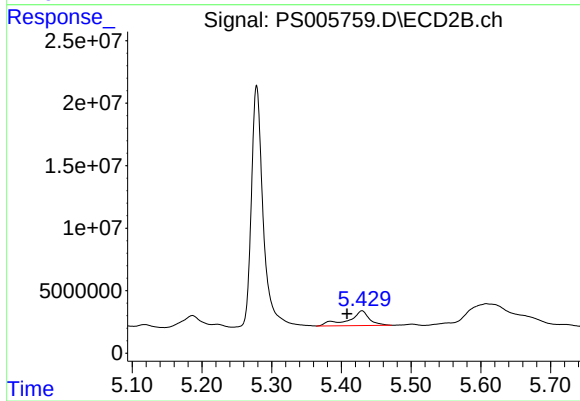

#5 DICAMBA


R.T.: 5.430 min
Delta R.T.: 0.021 min
Response: 24921767
Conc: 6.68 ng/ml

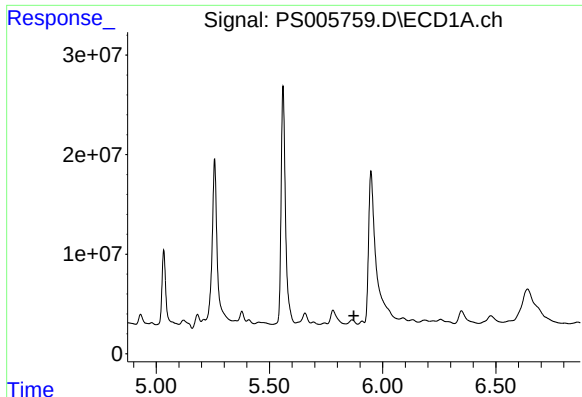

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 5.873 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

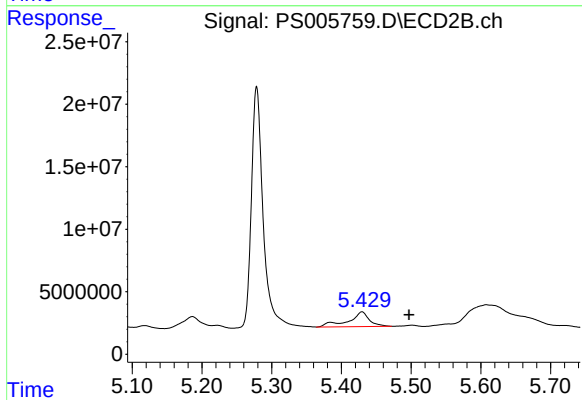


#6 MCPP

R.T.: 5.430 min
Delta R.T.: -0.067 min
Response: 24921767
Conc: 8.75 ug/ml

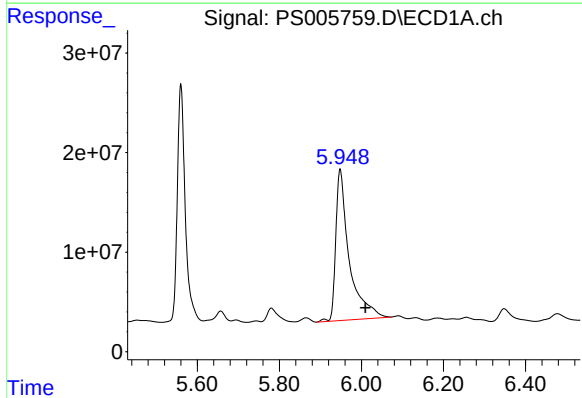


#7 MCPA

R.T.: 5.948 min
Delta R.T.: -0.061 min
Response: 346189468
Conc: 53.05 ug/ml

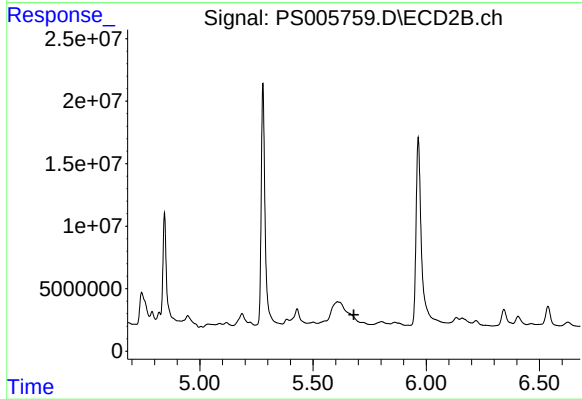

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.681 min
Response: 0
Conc: N.D.

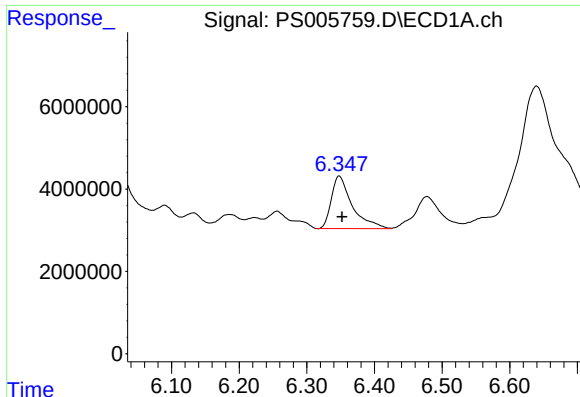

#8 DICHLORPROP


R.T.: 6.348 min
Delta R.T.: -0.004 min
Response: 27277734
Conc: 18.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

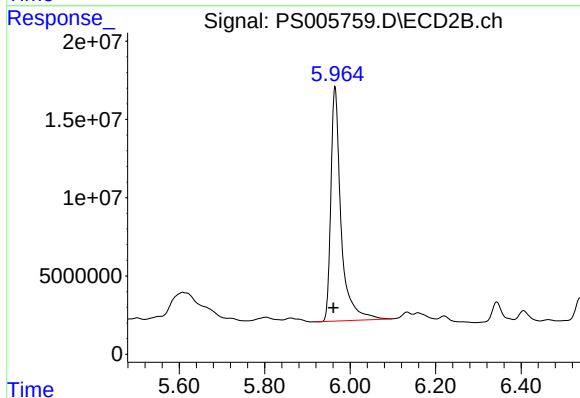


#8 DICHLORPROP

R.T.: 5.965 min
Delta R.T.: 0.003 min
Response: 247971088
Conc: 268.51 ng/ml

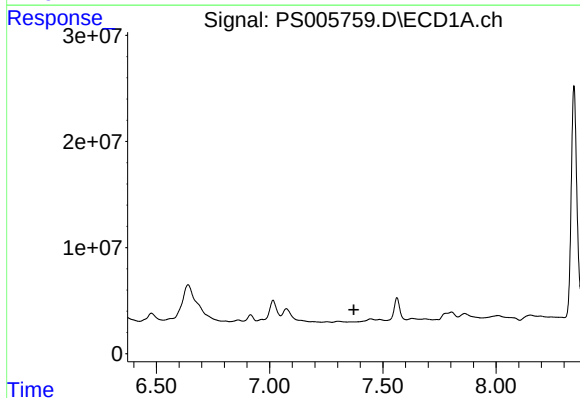


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.372 min
Response: 0
Conc: N.D.

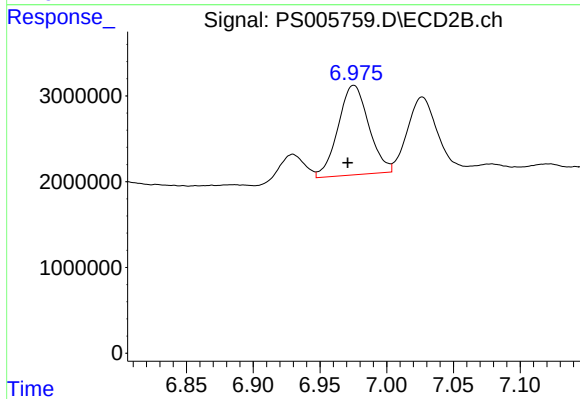

#11 2,4,5-TP (SILVEX)


R.T.: 6.975 min
Delta R.T.: 0.005 min
Response: 16727236
Conc: 3.22 ng/ml

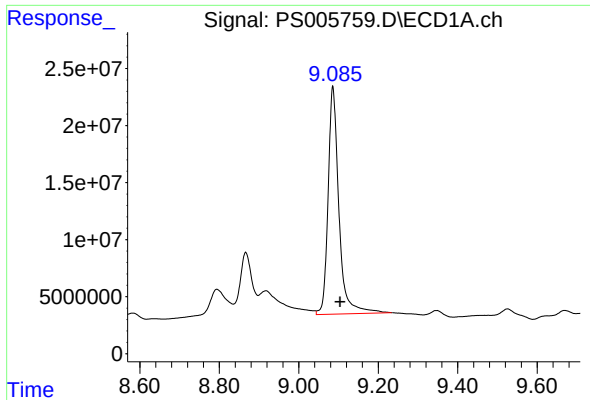

#15 Picloram

R.T.: 9.086 min
Delta R.T.: -0.018 min
Response: 376754461
Conc: 32.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

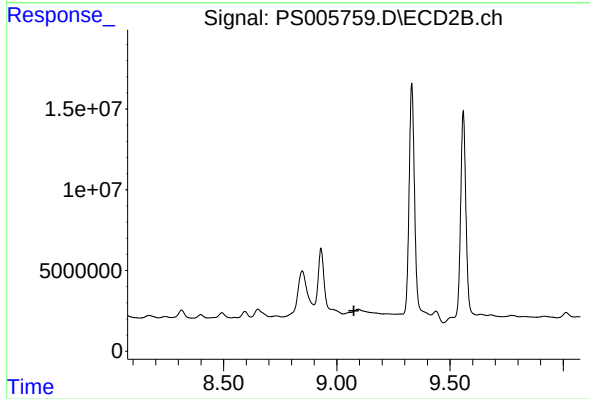

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.075 min
Response: 0
Conc: N.D.