

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072919\
 Data File : PS005760.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2019 11:35
 Operator : SM\AJ
 Sample : K3620-16RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 02:06:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.563	5.282	309.8E6	220.5E6	213.504	221.649
Target Compounds							
1) T	Dalapon	2.061	0.000	25976611	0	14.016	N.D. #
2) T	3,5-DICHL...	0.000	4.601	0	52011263	N.D.	40.091
5) T	DICAMBA	5.783	0.000	27615823	0	4.624	N.D. #
7) T	MCPA	5.955	5.614	180.5E6	91230808	27.661	21.675
8) T	DICHLORPROP	0.000	5.970	0	134.5E6	N.D.	145.613
10) T	Pentachlo...	0.000	6.541	0	20971017	N.D.	1.615
11) T	2,4,5-TP ...	0.000	6.979	0	9709845	N.D.	1.872
15) T	Picloram	9.092	0.000	108.5E6	0	9.269	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072919\
Data File : PS005760.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2019 11:35
Operator : SM\AJ
Sample : K3620-16RE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 02:06:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

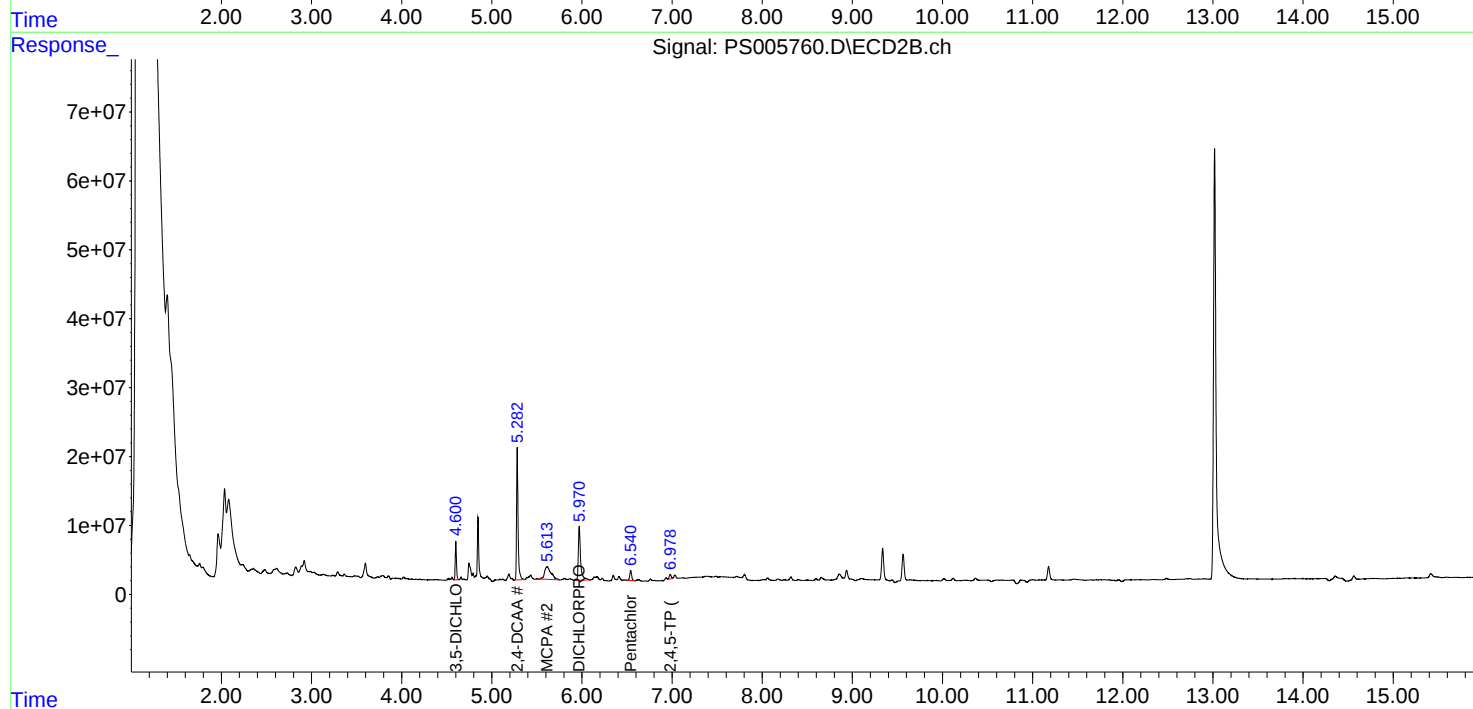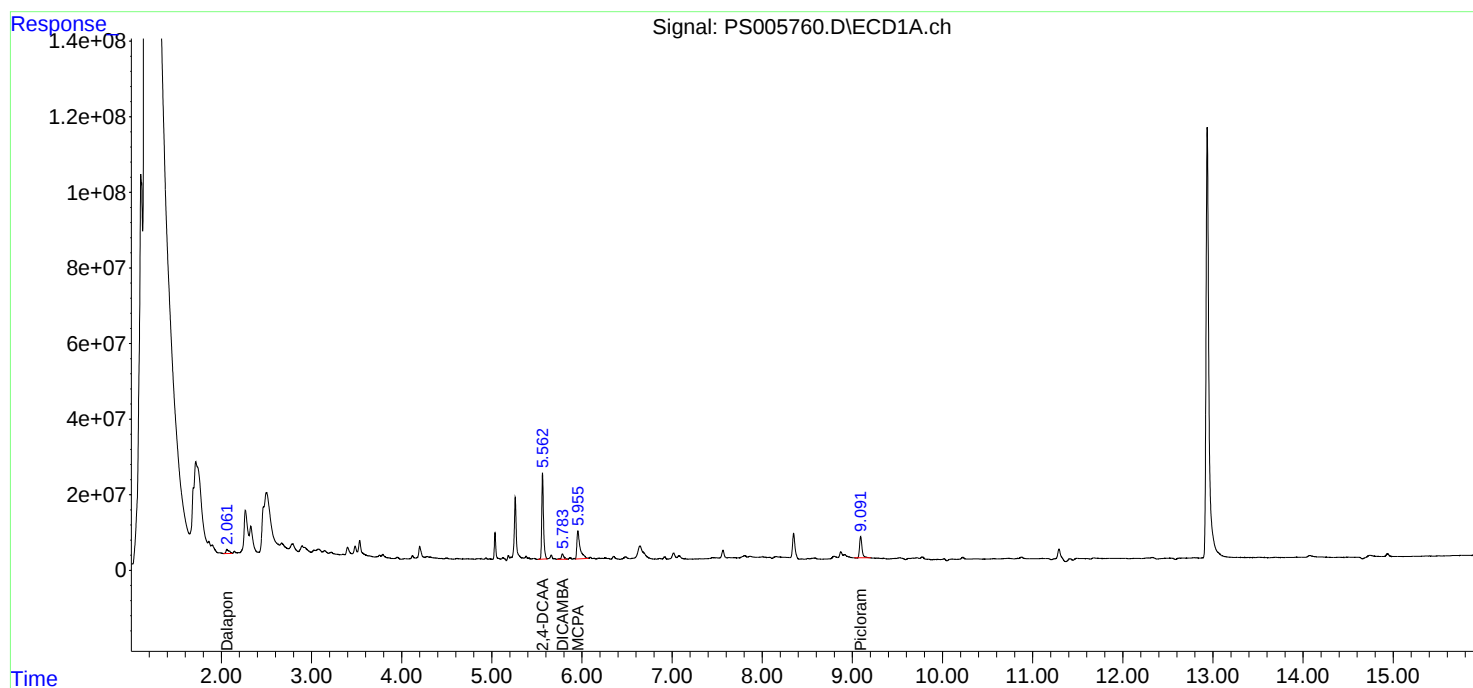


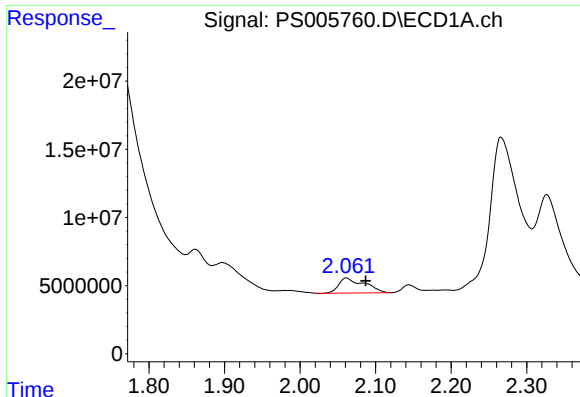

#1 Dalapon


R.T.: 2.061 min
Delta R.T.: -0.026 min
Response: 25976611
Conc: 14.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

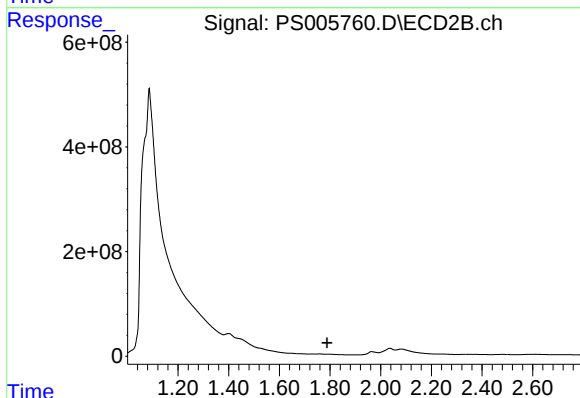


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

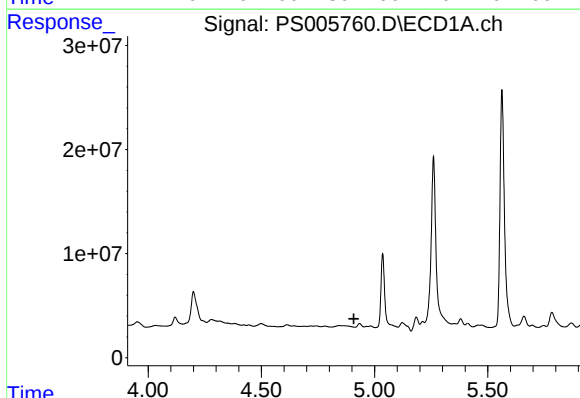


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.909 min
Response: 0
Conc: N.D.

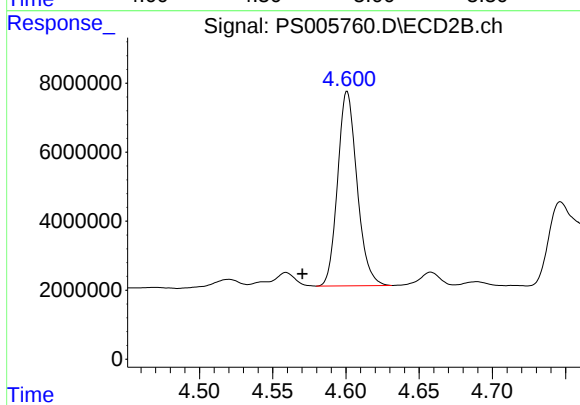

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.601 min
Delta R.T.: 0.031 min
Response: 52011263
Conc: 40.09 ng/ml

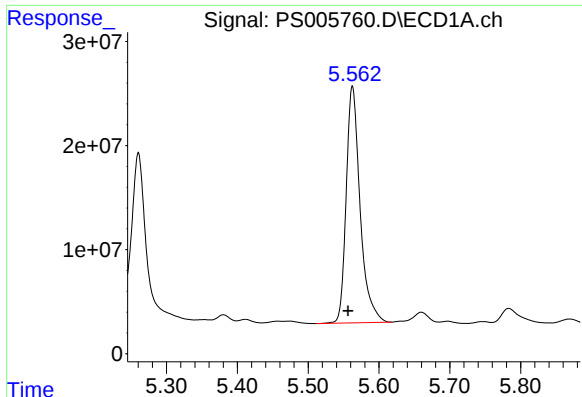

#4 2,4-DCAA


R.T.: 5.563 min
Delta R.T.: 0.007 min
Response: 309755674
Conc: 213.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

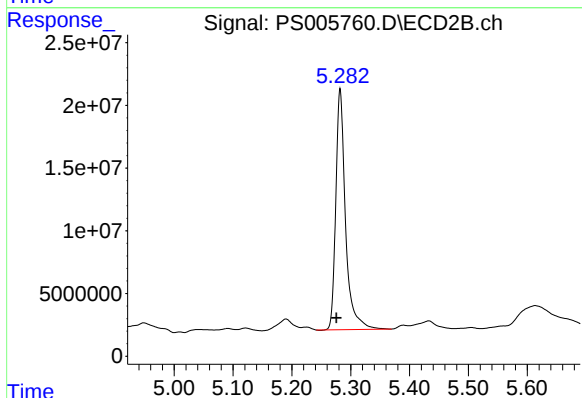


#4 2,4-DCAA

R.T.: 5.282 min
Delta R.T.: 0.006 min
Response: 220469784
Conc: 221.65 ng/ml

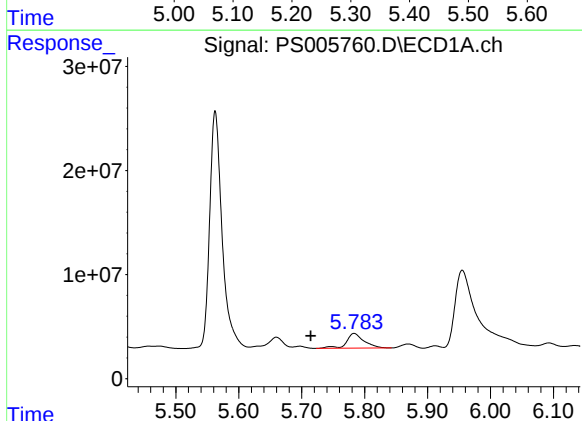


#5 DICAMBA

R.T.: 5.783 min
Delta R.T.: 0.069 min
Response: 27615823
Conc: 4.62 ng/ml

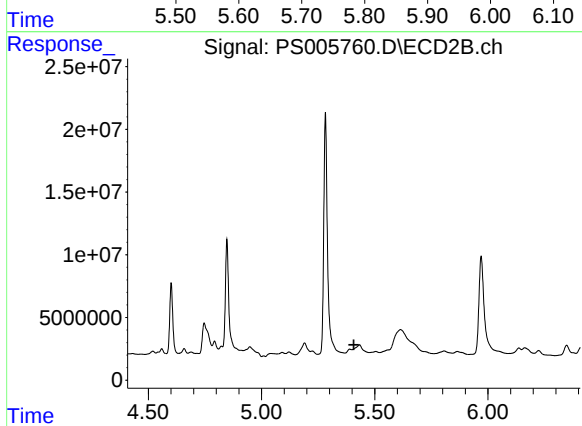

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.408 min
Response: 0
Conc: N.D.

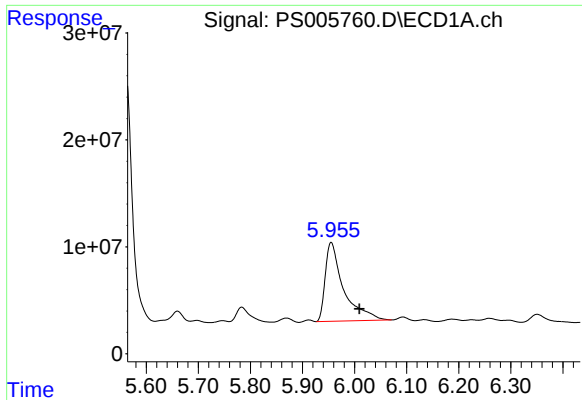

#7 MCPA


R.T.: 5.955 min
Delta R.T.: -0.054 min
Response: 180506066
Conc: 27.66 ug/ml

Instrument :
ECD_S
ClientSampleId :

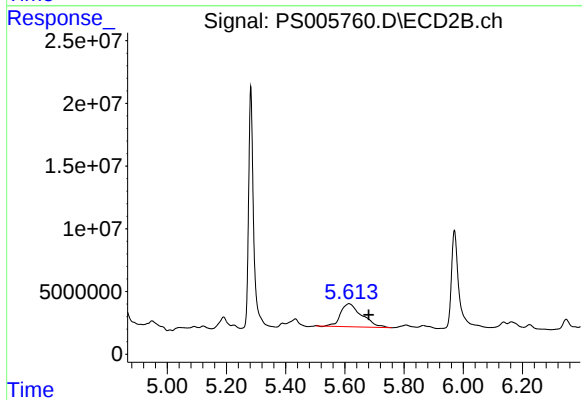


#7 MCPA

R.T.: 5.614 min
Delta R.T.: -0.067 min
Response: 91230808
Conc: 21.68 ug/ml

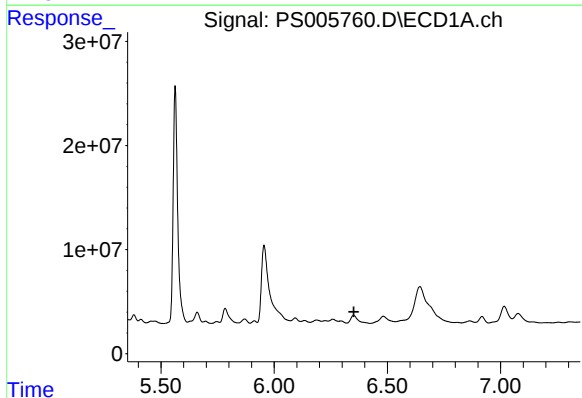


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.352 min
Response: 0
Conc: N.D.

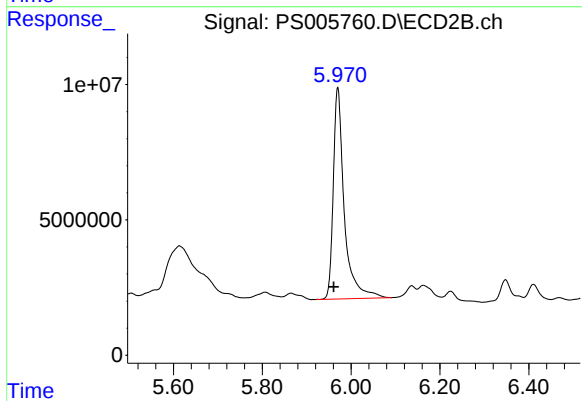

#8 DICHLORPROP


R.T.: 5.970 min
Delta R.T.: 0.009 min
Response: 134476308
Conc: 145.61 ng/ml

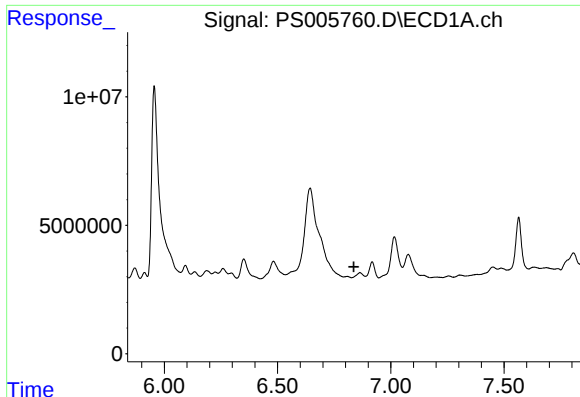

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

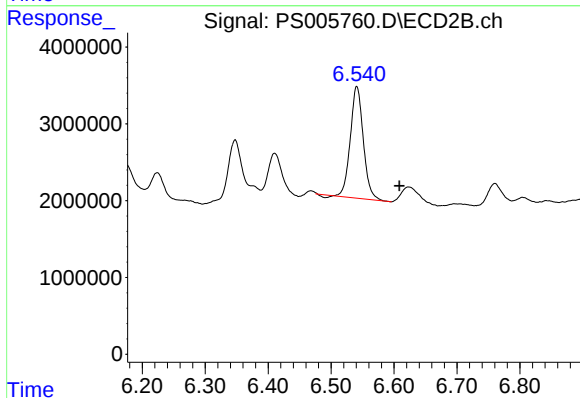


#10 Pentachlorophenol

R.T.: 6.541 min
Delta R.T.: -0.067 min
Response: 20971017
Conc: 1.62 ng/ml

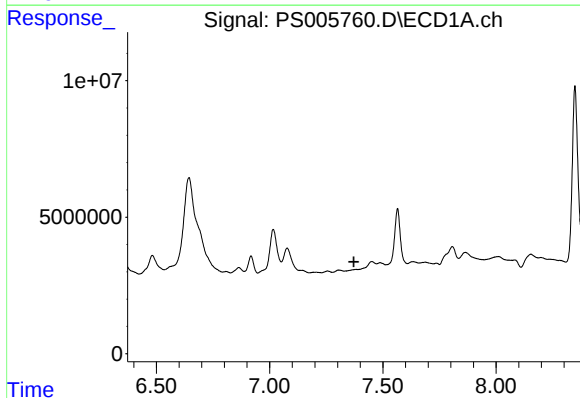


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

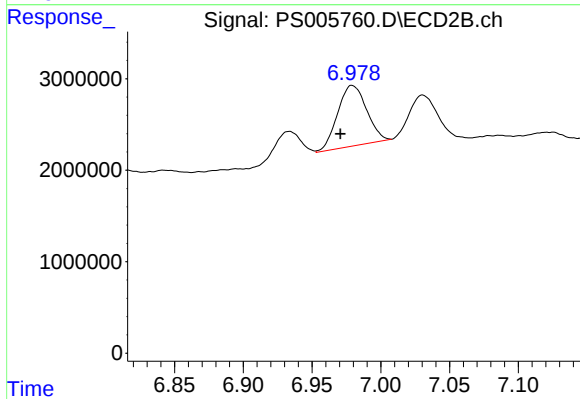

#11 2,4,5-TP (SILVEX)


R.T.: 6.979 min
Delta R.T.: 0.009 min
Response: 9709845
Conc: 1.87 ng/ml

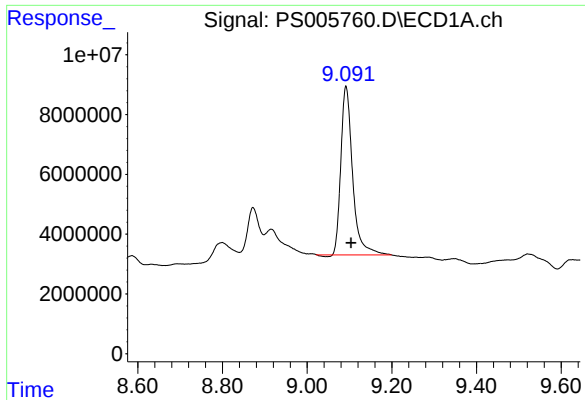

#15 Picloram

R.T.: 9.092 min
Delta R.T.: -0.012 min
Response: 108498532
Conc: 9.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

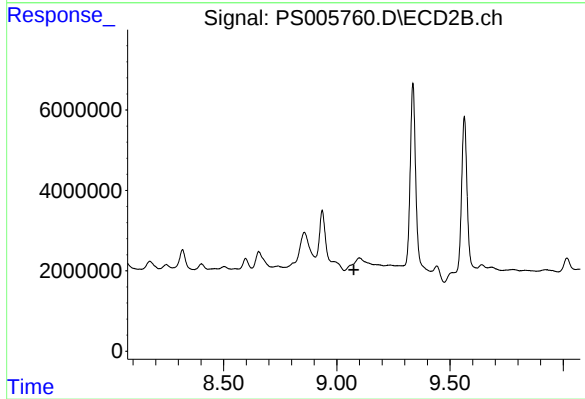

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.075 min
Response: 0
Conc: N.D.