

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072919\
 Data File : PS005762.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2019 12:19
 Operator : SM\AJ
 Sample : K3626-10
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 02:07:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.581	5.300	311.1E6	215.9E6	214.456	217.036
Target Compounds							
1) T	Dalapon	2.079	0.000	22128632	0	11.940	N.D. #
2) T	3,5-DICHL...	0.000	4.618	0	59856932	N.D.	46.139
7) T	MCPA	5.973	5.630	91153776	101.2E6	13.969	24.036 #
8) T	DICHLORPROP	0.000	5.989	0	59181182	N.D.	64.082
10) T	Pentachlo...	0.000	6.559	0	25723595	N.D.	1.981
12) T	2,4,5-T	7.583	0.000	39036968	0	4.677	N.D. #
15) T	Picloram	9.113	0.000	48688470	0	4.160	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072919\
Data File : PS005762.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2019 12:19
Operator : SM\AJ
Sample : K3626-10
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 02:07:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

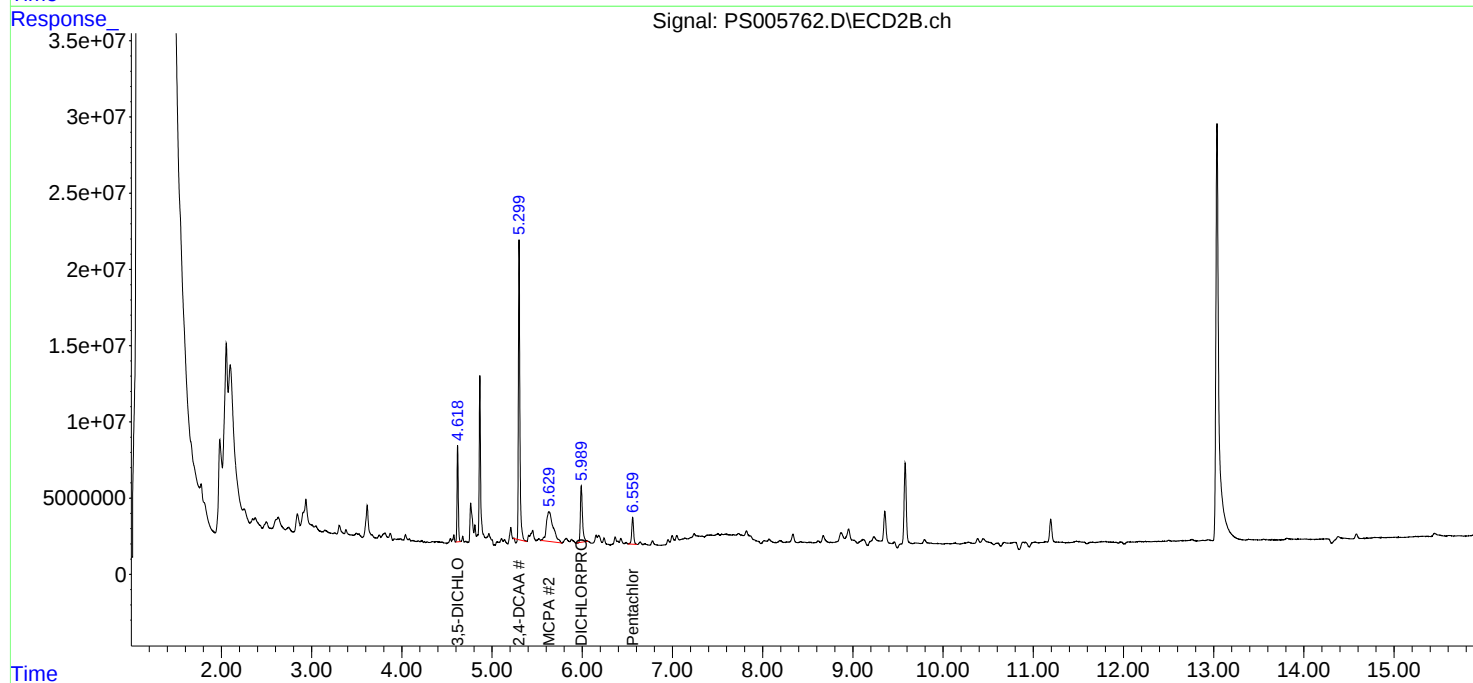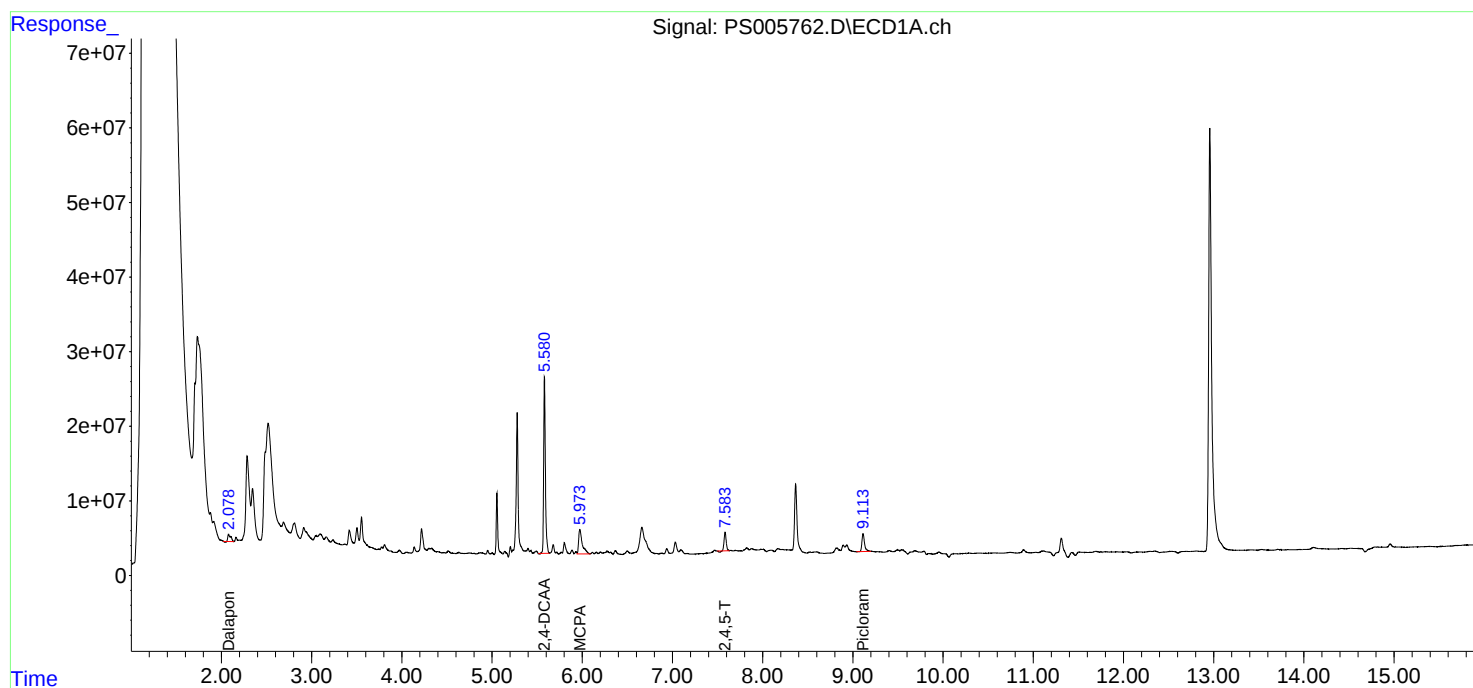


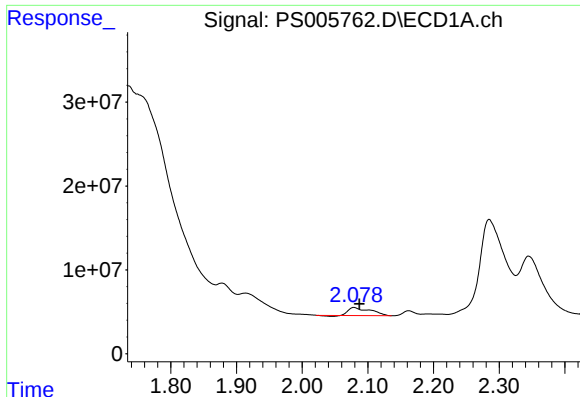

#1 Dalapon


R.T.: 2.079 min
Delta R.T.: -0.008 min
Response: 22128632
Conc: 11.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

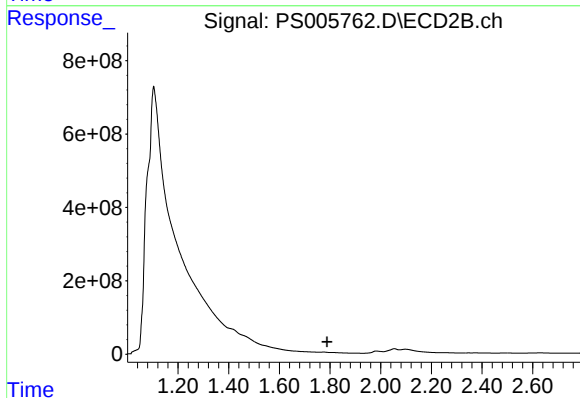


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

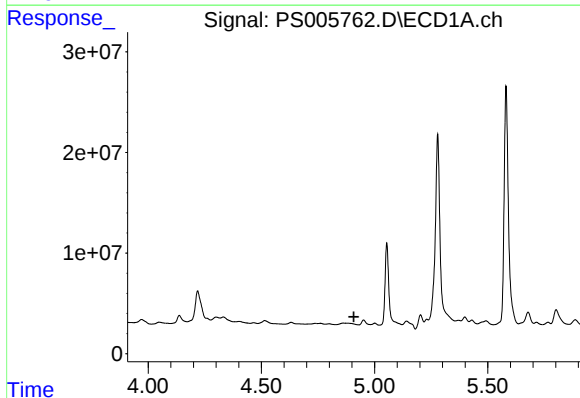


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.909 min
Response: 0
Conc: N.D.

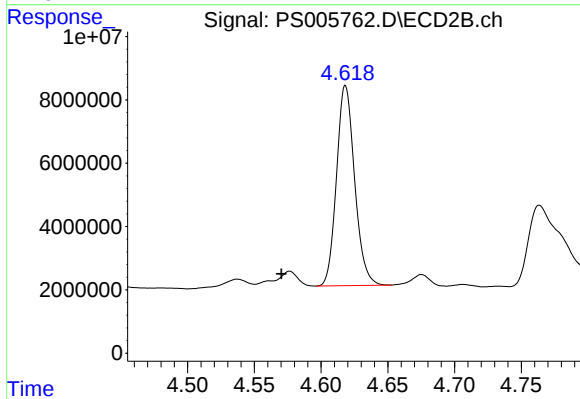

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.618 min
Delta R.T.: 0.048 min
Response: 59856932
Conc: 46.14 ng/ml

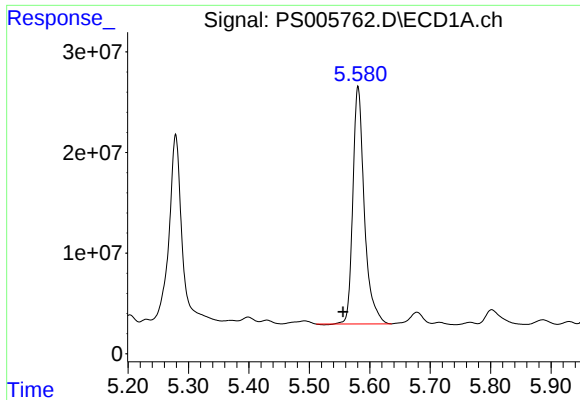

#4 2,4-DCAA


R.T.: 5.581 min
Delta R.T.: 0.025 min
Response: 311136486
Conc: 214.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

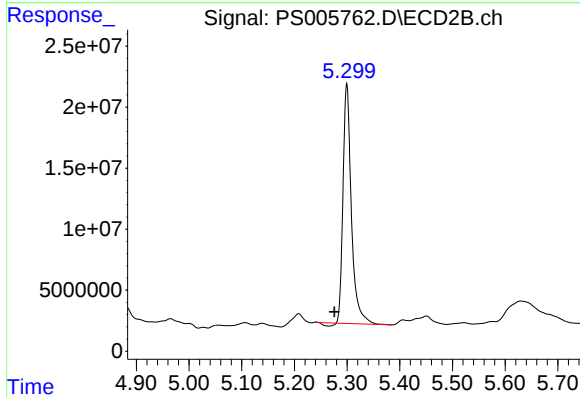


#4 2,4-DCAA

R.T.: 5.300 min
Delta R.T.: 0.024 min
Response: 215881386
Conc: 217.04 ng/ml

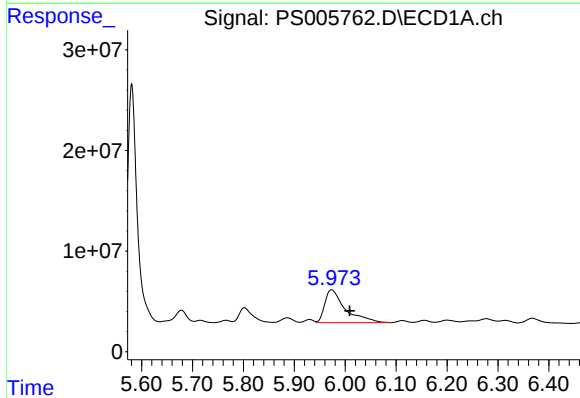


#7 MCPA

R.T.: 5.973 min
Delta R.T.: -0.036 min
Response: 91153776
Conc: 13.97 ug/ml

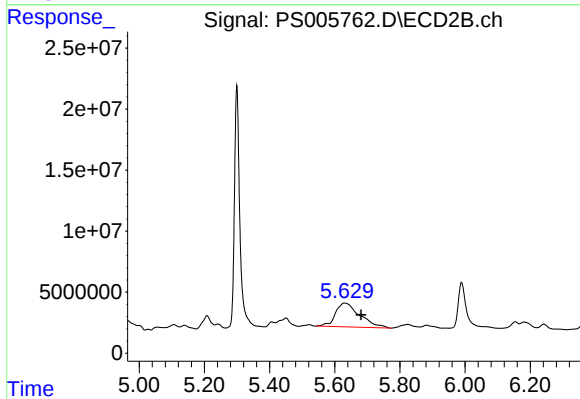

#7 MCPA


R.T.: 5.630 min
Delta R.T.: -0.050 min
Response: 101169147
Conc: 24.04 ug/ml

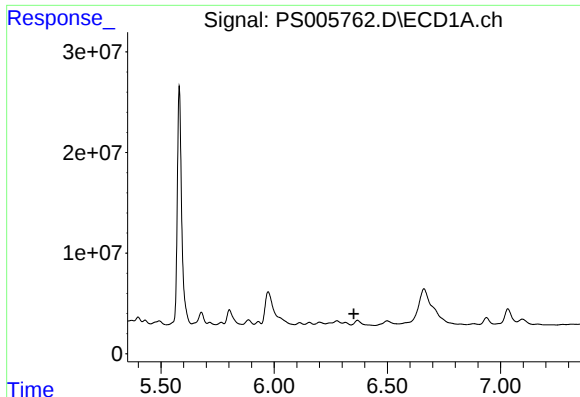

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

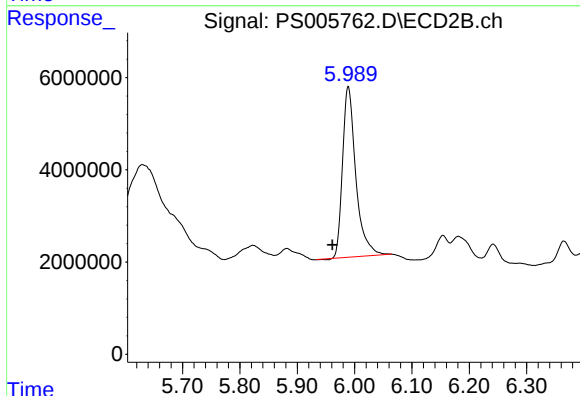


#8 DICHLORPROP

R.T.: 5.989 min
Delta R.T.: 0.028 min
Response: 59181182
Conc: 64.08 ng/ml

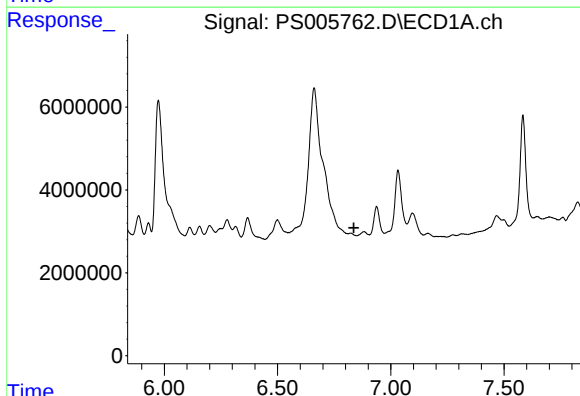


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

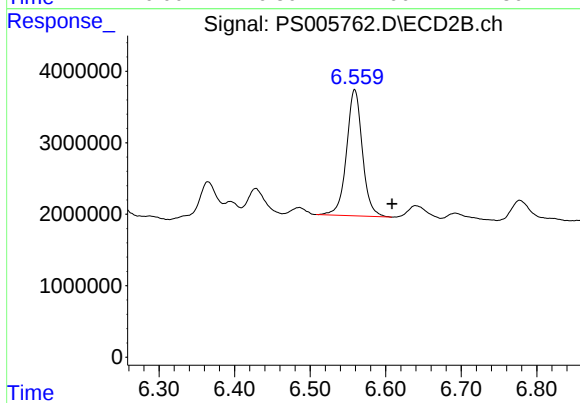

#10 Pentachlorophenol


R.T.: 6.559 min
Delta R.T.: -0.049 min
Response: 25723595
Conc: 1.98 ng/ml

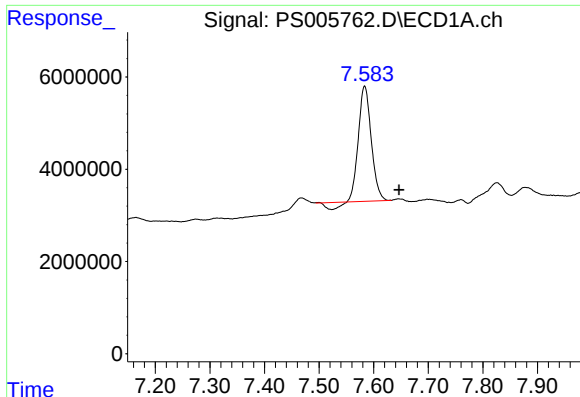

#12 2,4,5-T


R.T.: 7.583 min
Delta R.T.: -0.063 min
Response: 39036968
Conc: 4.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

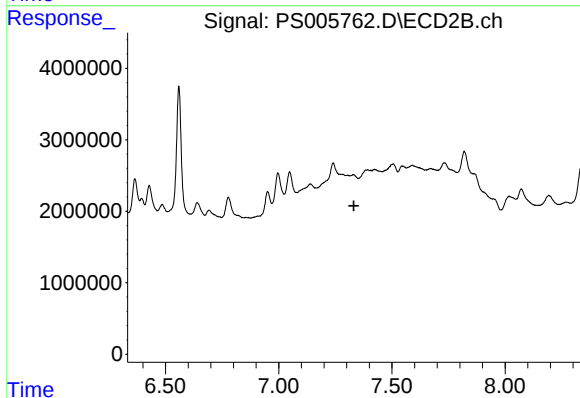


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.332 min
Response: 0
Conc: N.D.

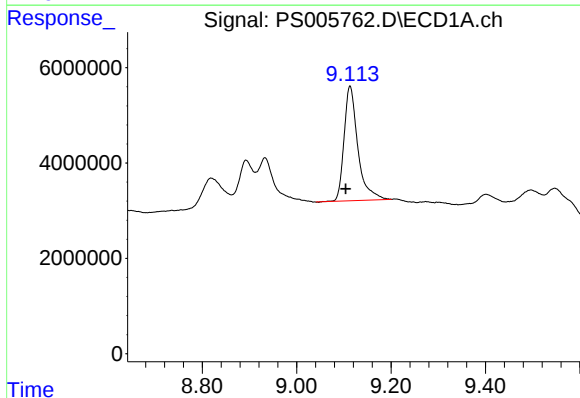

#15 Picloram

R.T.: 9.113 min
Delta R.T.: 0.009 min
Response: 48688470
Conc: 4.16 ng/ml

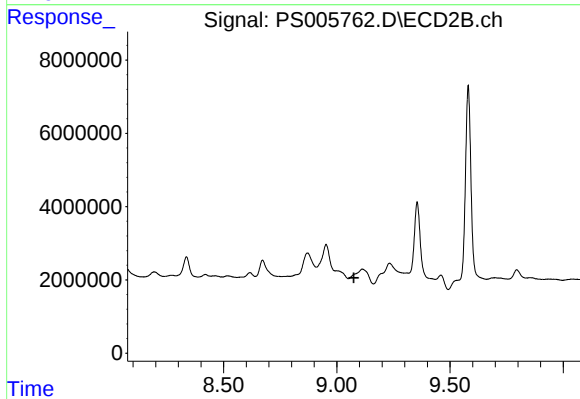

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.075 min
Response: 0
Conc: N.D.