

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072919\
 Data File : PS005763.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2019 12:41
 Operator : SM\AJ
 Sample : K3626-12
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 02:07:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.561	5.280	327.5E6	232.6E6	225.768	233.850
Target Compounds							
1) T	Dalapon	2.059	0.000	25462082	0	13.739	N.D. #
2) T	3,5-DICHL...	0.000	4.599	0	61888348	N.D.	47.705
5) T	DICAMBA	5.782	0.000	31158664	0	5.217	N.D. #
7) T	MCPA	5.953	0.000	105.5E6	0	16.161	N.D. #
8) T	DICHLORPROP	0.000	5.968	0	68253021	N.D.	73.905
10) T	Pentachlo...	0.000	6.539	0	29893053	N.D.	2.302
15) T	Picloram	9.094	0.000	38003365	0	3.247	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072919\
Data File : PS005763.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2019 12:41
Operator : SM\AJ
Sample : K3626-12
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 02:07:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

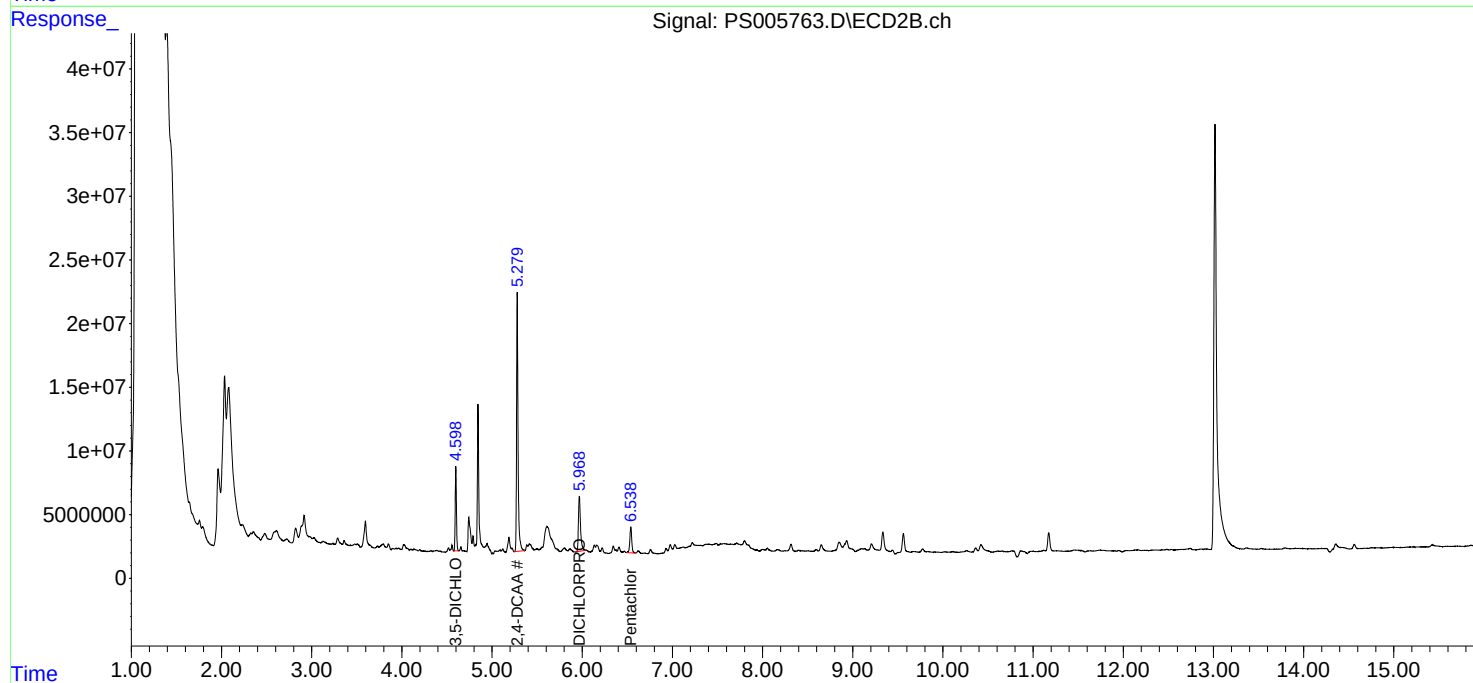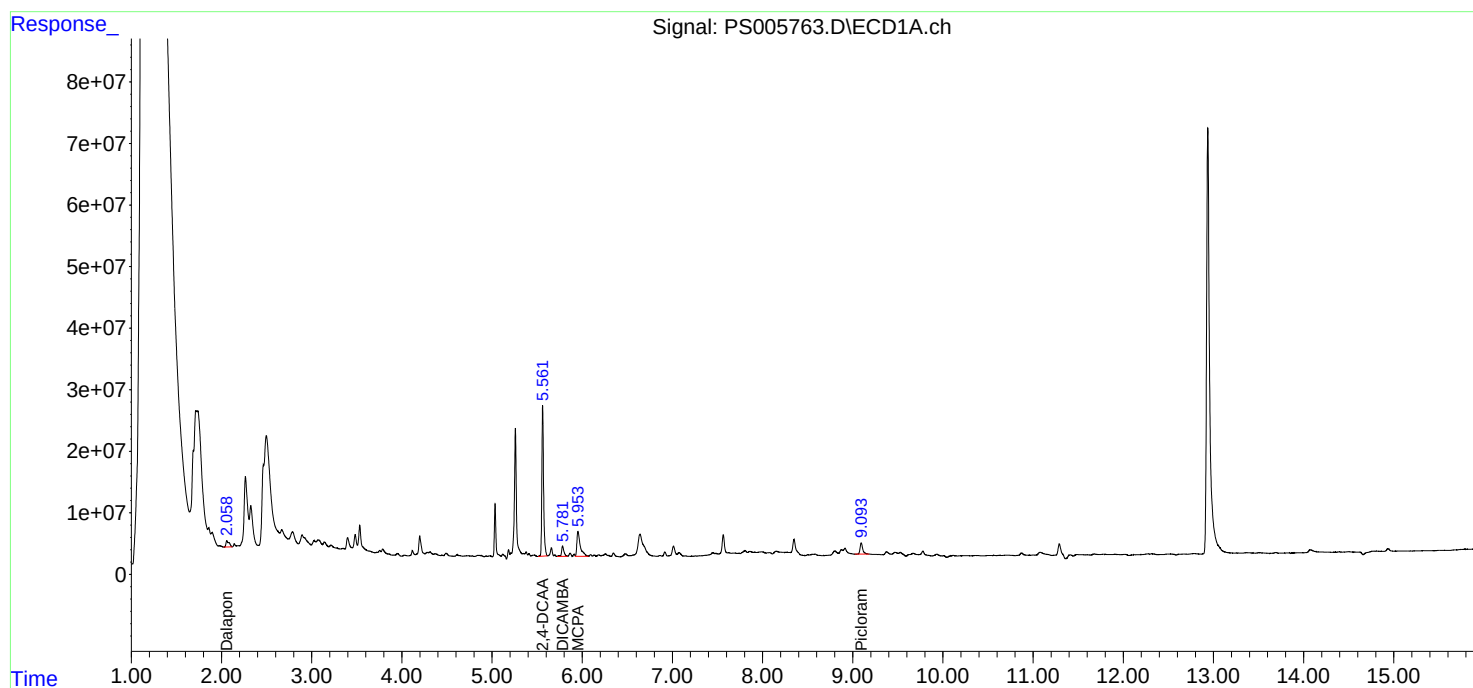


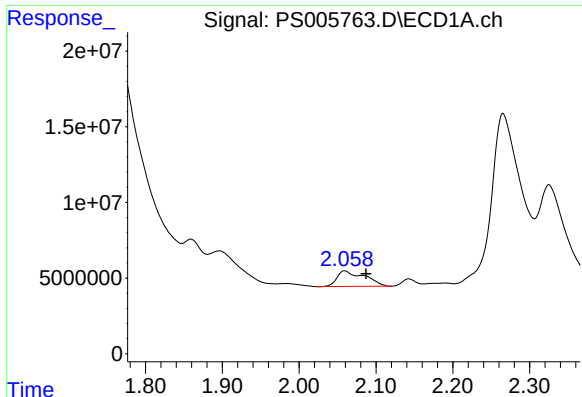

#1 Dalapon


R.T.: 2.059 min
Delta R.T.: -0.028 min
Response: 25462082
Conc: 13.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

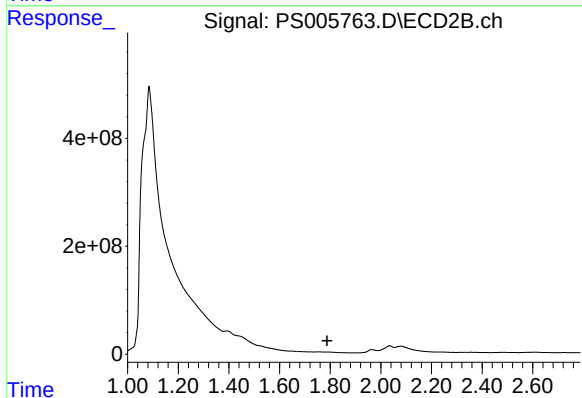


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

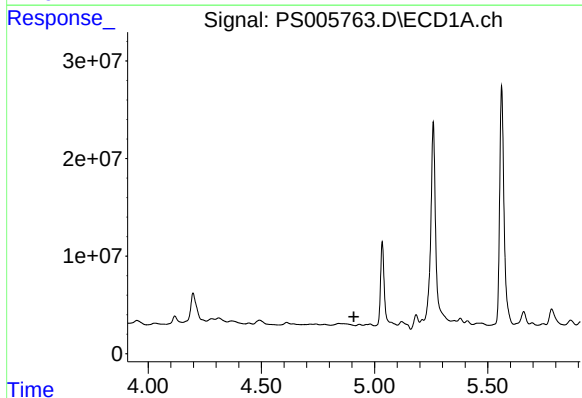


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.909 min
Response: 0
Conc: N.D.

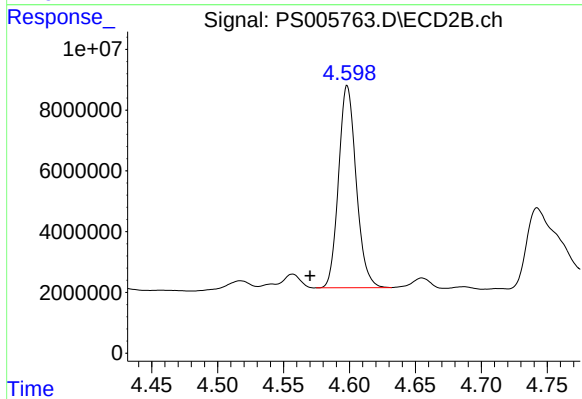

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.599 min
Delta R.T.: 0.028 min
Response: 61888348
Conc: 47.70 ng/ml

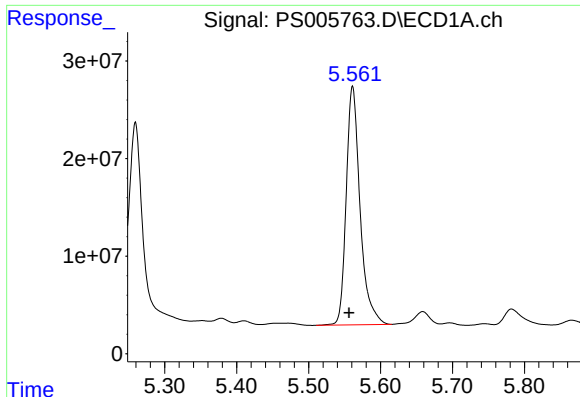

#4 2,4-DCAA


R.T.: 5.561 min
Delta R.T.: 0.005 min
Response: 327548476
Conc: 225.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

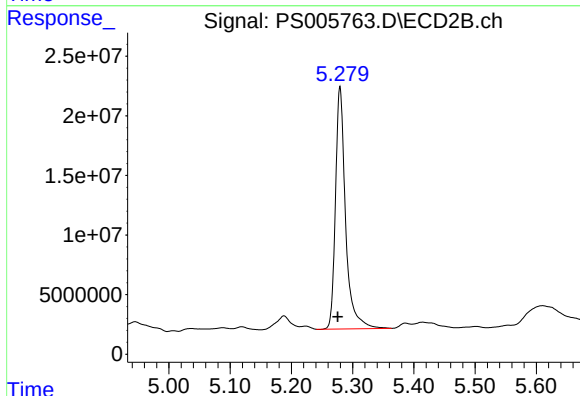


#4 2,4-DCAA

R.T.: 5.280 min
Delta R.T.: 0.004 min
Response: 232605621
Conc: 233.85 ng/ml

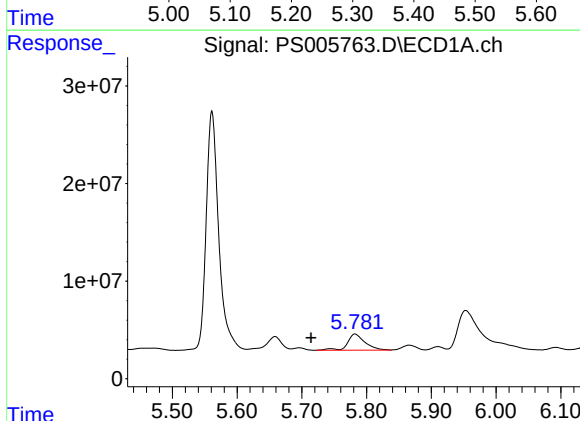


#5 DICAMBA

R.T.: 5.782 min
Delta R.T.: 0.068 min
Response: 31158664
Conc: 5.22 ng/ml

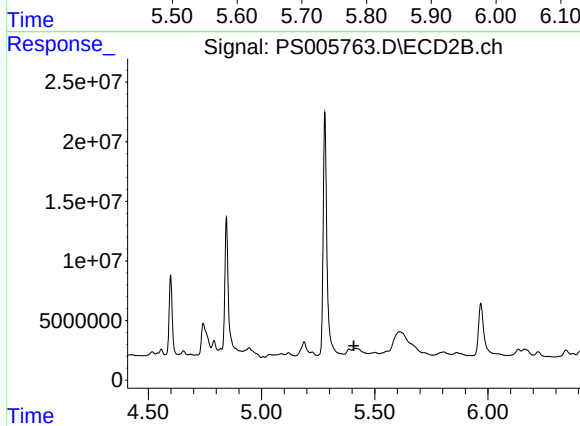

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 5.408 min
Response: 0
Conc: N.D.

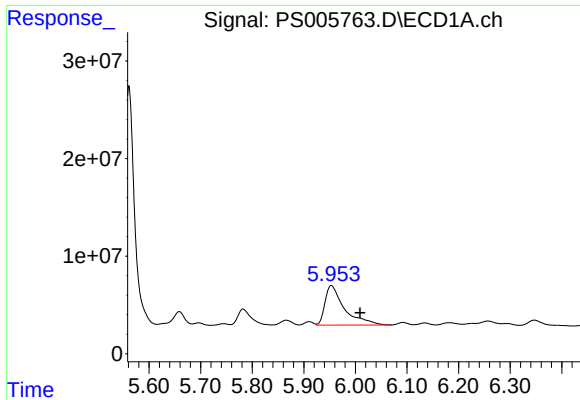

#7 MCPA


R.T.: 5.953 min
Delta R.T.: -0.056 min
Response: 105461809
Conc: 16.16 ug/ml

Instrument :
ECD_S
ClientSampleId :

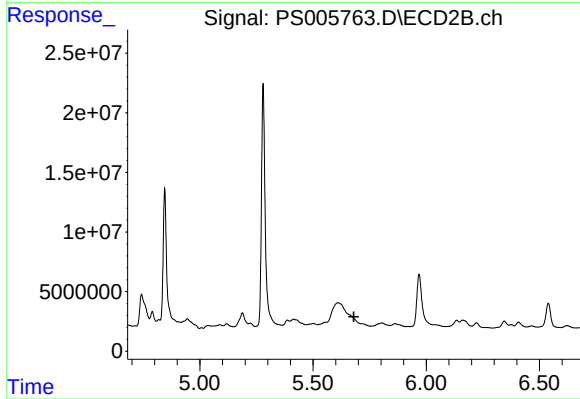


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.681 min
Response: 0
Conc: N.D.

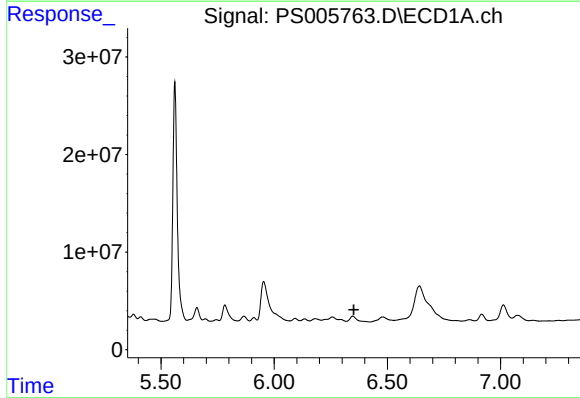


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.352 min
Response: 0
Conc: N.D.

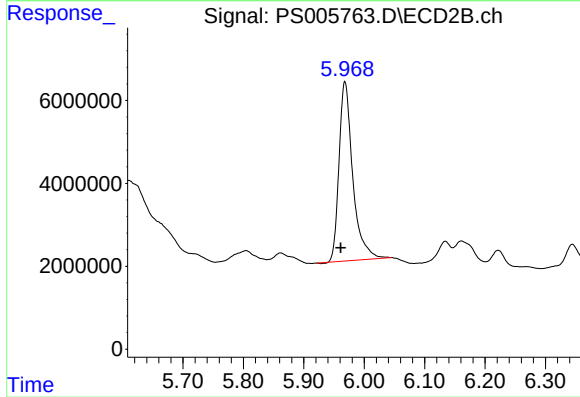

#8 DICHLORPROP


R.T.: 5.968 min
Delta R.T.: 0.007 min
Response: 68253021
Conc: 73.91 ng/ml

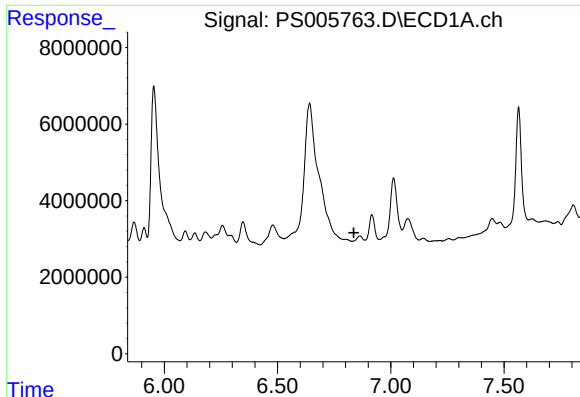

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

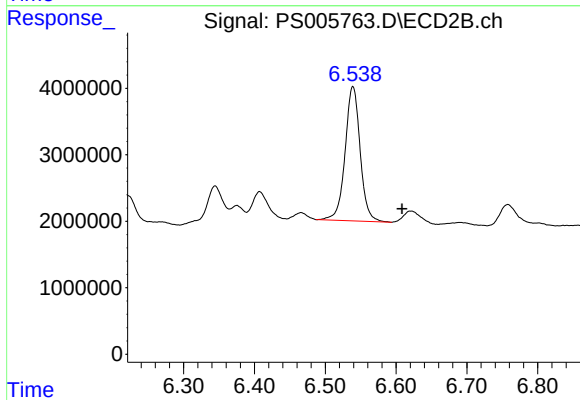


#10 Pentachlorophenol

R.T.: 6.539 min
Delta R.T.: -0.069 min
Response: 29893053
Conc: 2.30 ng/ml

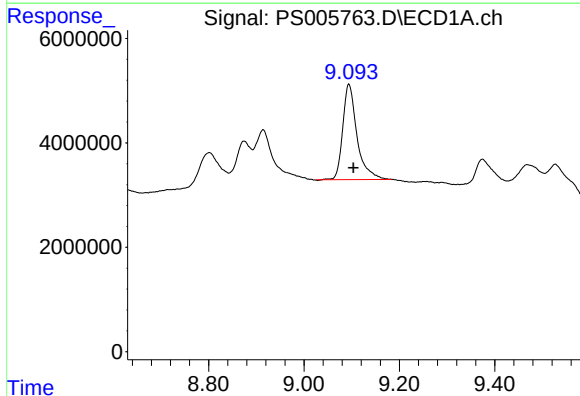

#15 Picloram

R.T.: 9.094 min
Delta R.T.: -0.010 min
Response: 38003365
Conc: 3.25 ng/ml

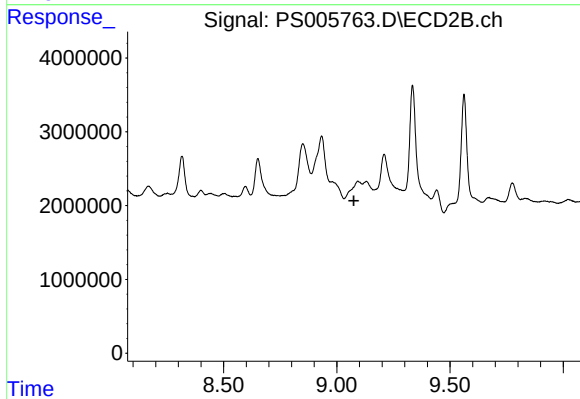

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 9.075 min
Response: 0
Conc: N.D.