

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072919\
 Data File : PS005764.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2019 13:03
 Operator : SM\AJ
 Sample : K3626-10RE
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 02:07:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.562	5.282	317.5E6	227.3E6	218.846	228.542
Target Compounds							
1) T	Dalapon	2.061	0.000	25743503	0	13.891	N.D. #
2) T	3,5-DICHL...	0.000	4.601	0	59982728	N.D.	46.236
5) T	DICAMBA	5.784	5.433	26481454	27012136	4.434	7.236 #
6) T	MCP	0.000	5.433	0	27012136	N.D.	9.484
7) T	MCPA	5.953	5.615	116.9E6	119.2E6	17.920	28.328 #
8) T	DICHLORPROP	0.000	5.971	0	76364858	N.D.	82.689
10) T	Pentachlo...	0.000	6.541	0	23057916	N.D.	1.776
15) T	Picloram	9.094	0.000	57581243	0	4.919	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072919\
Data File : PS005764.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2019 13:03
Operator : SM\AJ
Sample : K3626-10RE
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 02:07:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

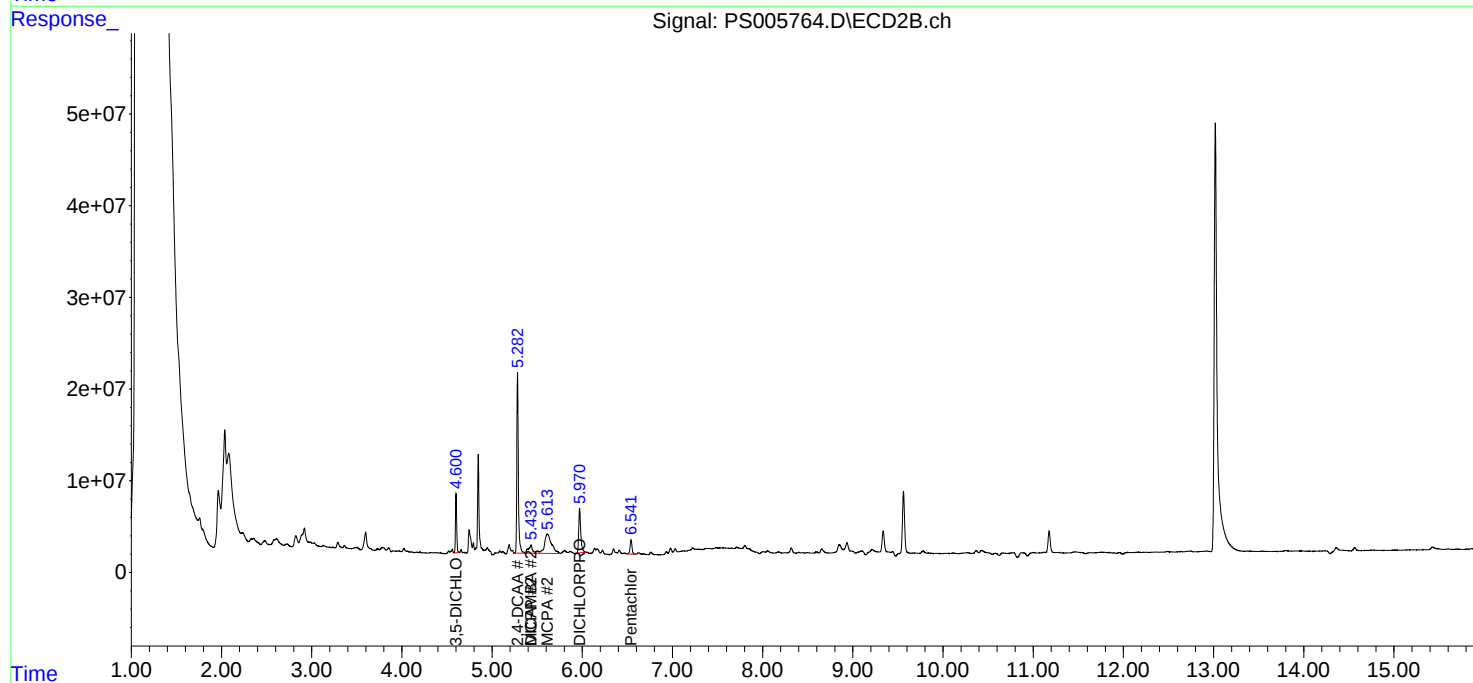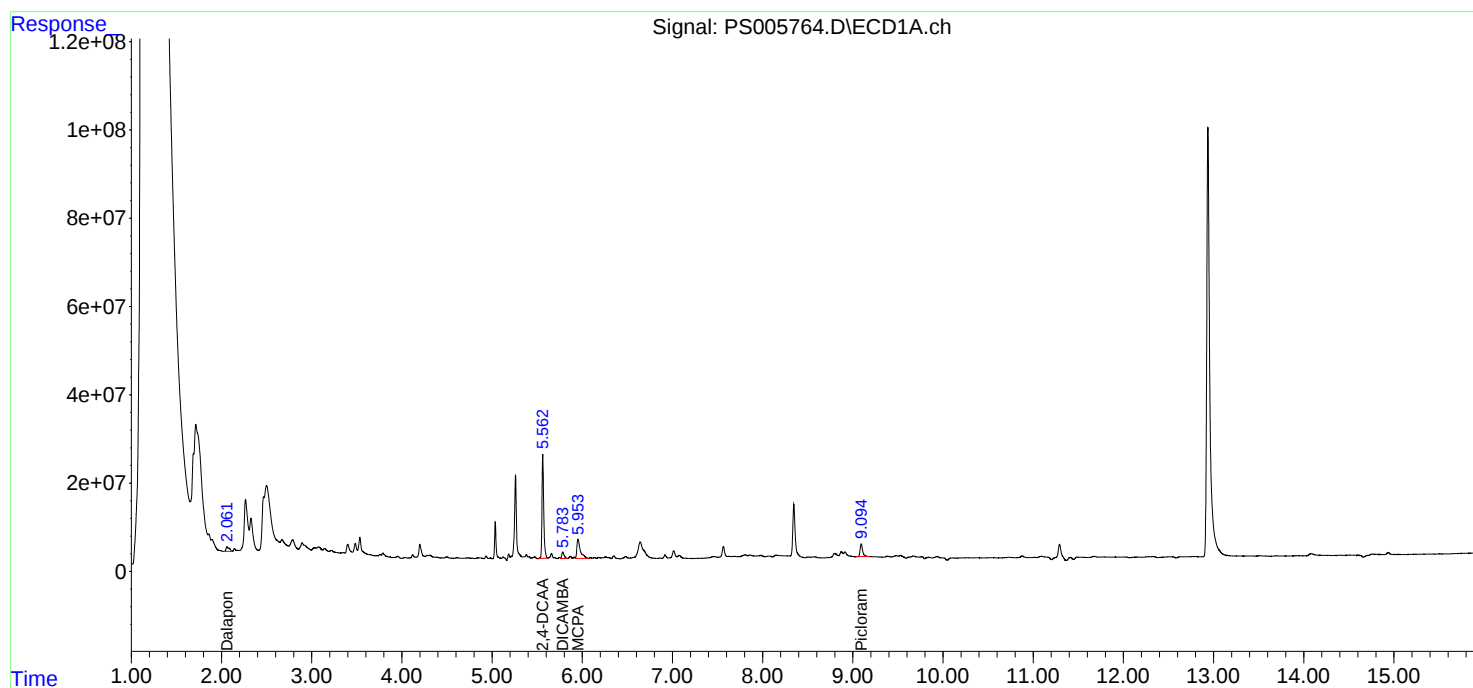


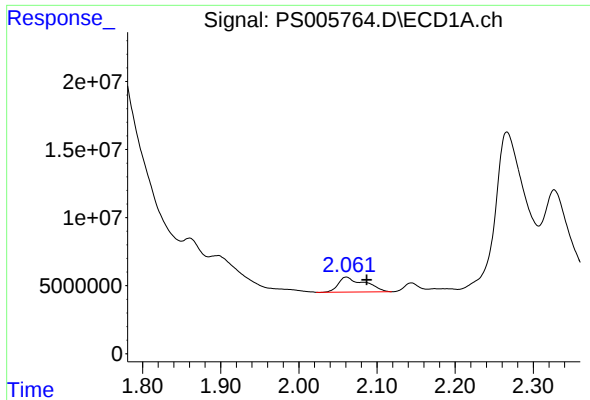

#1 Dalapon


R.T.: 2.061 min
Delta R.T.: -0.026 min
Response: 25743503
Conc: 13.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

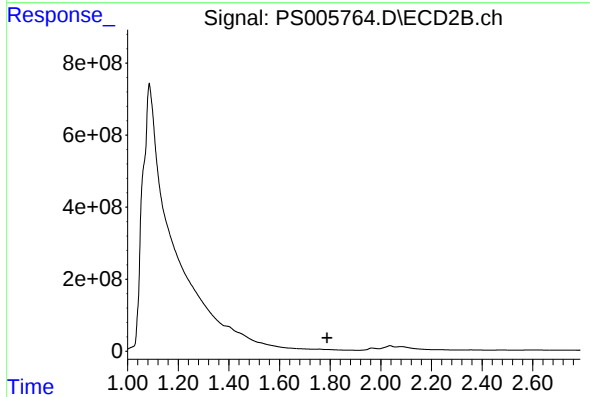


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

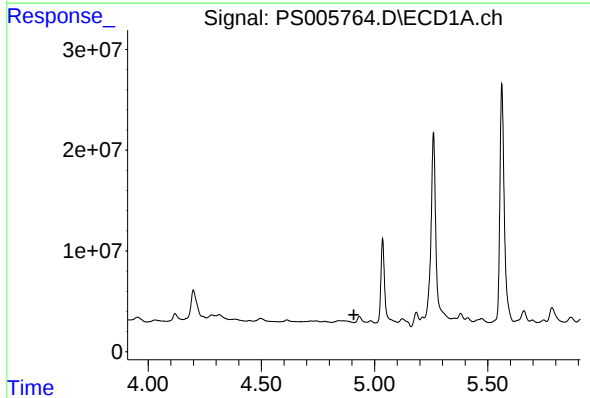


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.909 min
Response: 0
Conc: N.D.

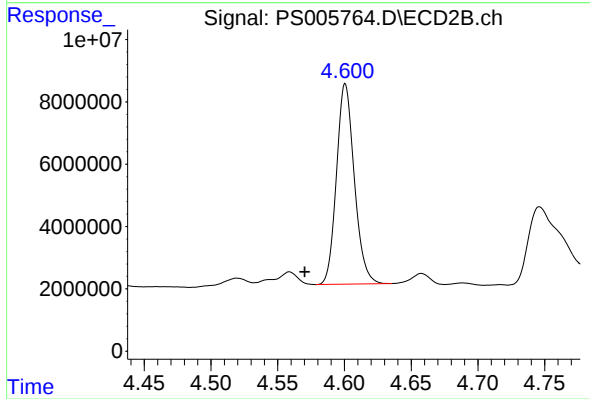

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.601 min
Delta R.T.: 0.031 min
Response: 59982728
Conc: 46.24 ng/ml

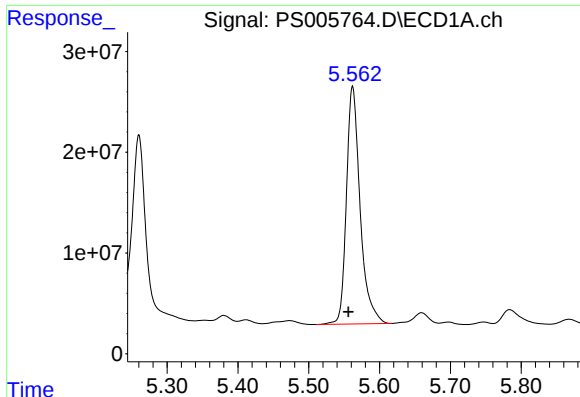

#4 2,4-DCAA


R.T.: 5.562 min
Delta R.T.: 0.006 min
Response: 317506360
Conc: 218.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

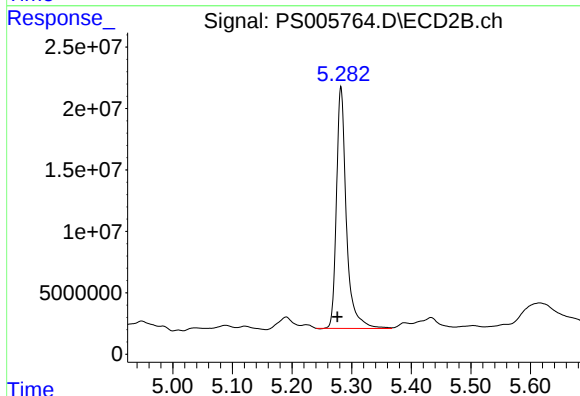


#4 2,4-DCAA

R.T.: 5.282 min
Delta R.T.: 0.006 min
Response: 227325791
Conc: 228.54 ng/ml

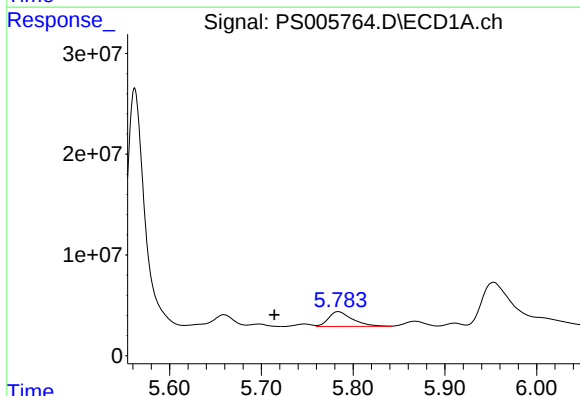


#5 DICAMBA

R.T.: 5.784 min
Delta R.T.: 0.070 min
Response: 26481454
Conc: 4.43 ng/ml

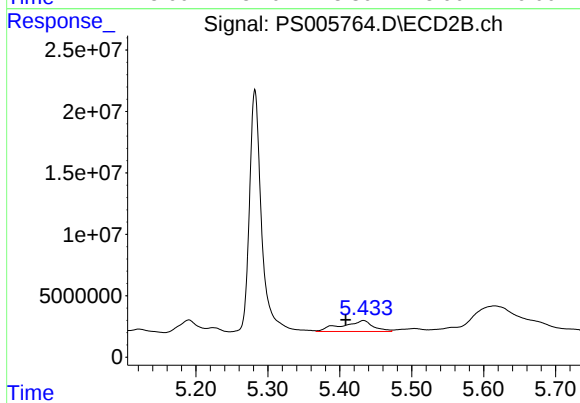

#5 DICAMBA


R.T.: 5.433 min
Delta R.T.: 0.025 min
Response: 27012136
Conc: 7.24 ng/ml

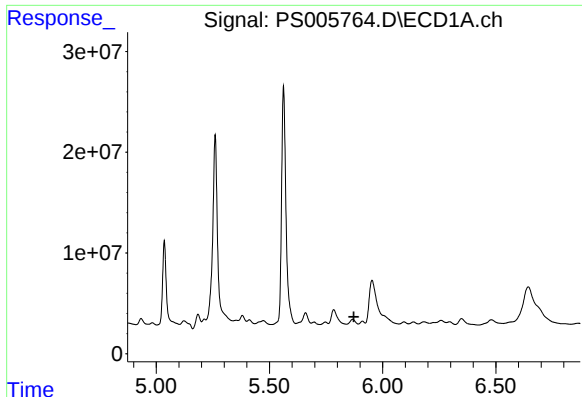

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 5.873 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

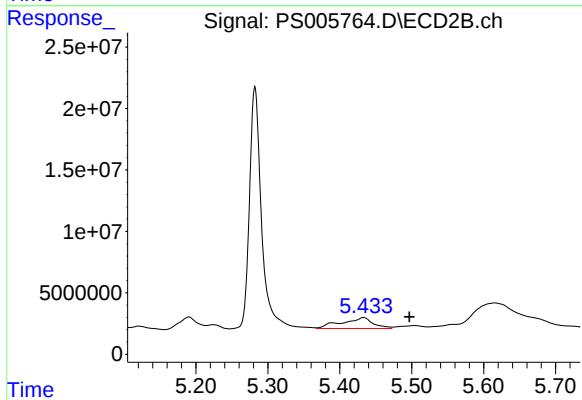


#6 MCPP

R.T.: 5.433 min
Delta R.T.: -0.064 min
Response: 27012136
Conc: 9.48 ug/ml

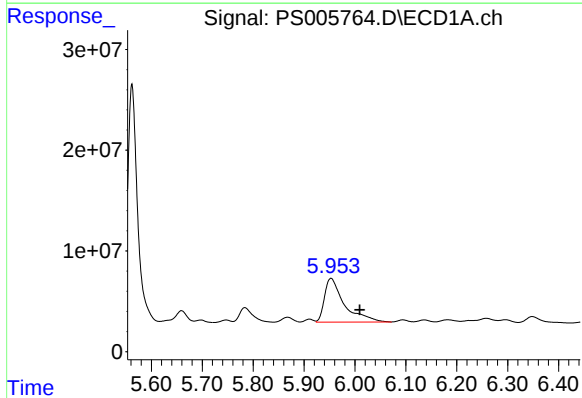


#7 MCPA

R.T.: 5.953 min
Delta R.T.: -0.056 min
Response: 116936626
Conc: 17.92 ug/ml

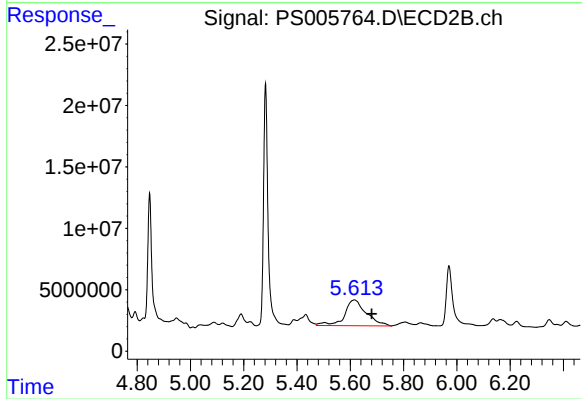

#7 MCPA


R.T.: 5.615 min
Delta R.T.: -0.066 min
Response: 119232724
Conc: 28.33 ug/ml

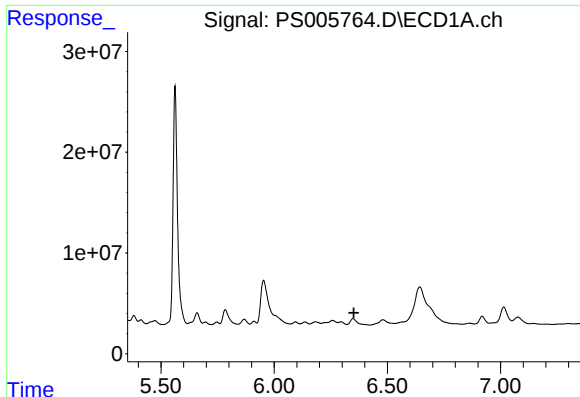

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

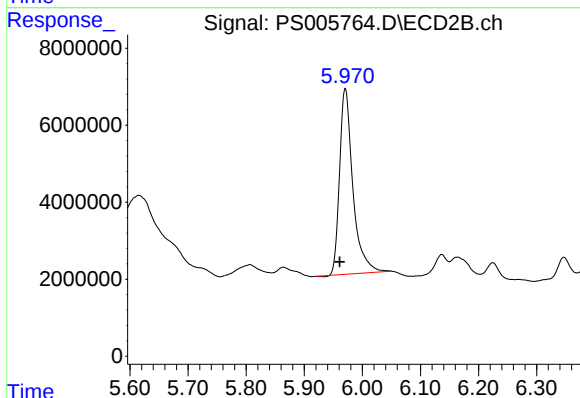


#8 DICHLORPROP

R.T.: 5.971 min
Delta R.T.: 0.009 min
Response: 76364858
Conc: 82.69 ng/ml

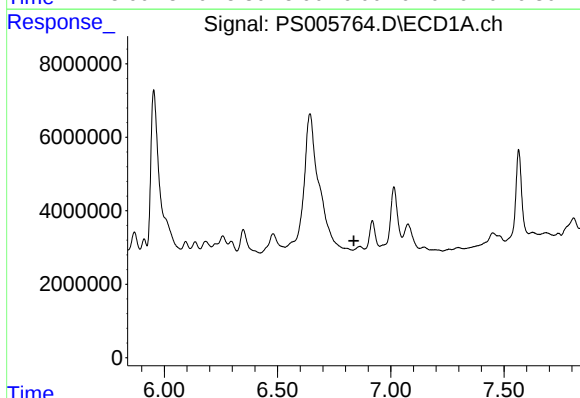


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

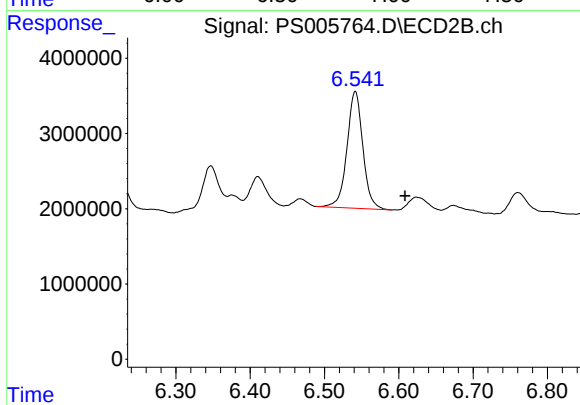

#10 Pentachlorophenol


R.T.: 6.541 min
Delta R.T.: -0.067 min
Response: 23057916
Conc: 1.78 ng/ml

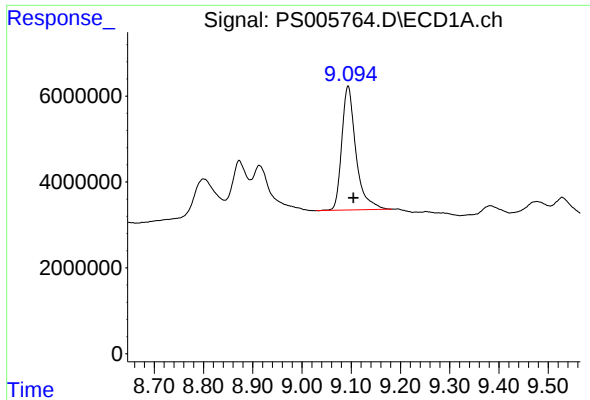

#15 Picloram

R.T.: 9.094 min
Delta R.T.: -0.010 min
Response: 57581243
Conc: 4.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

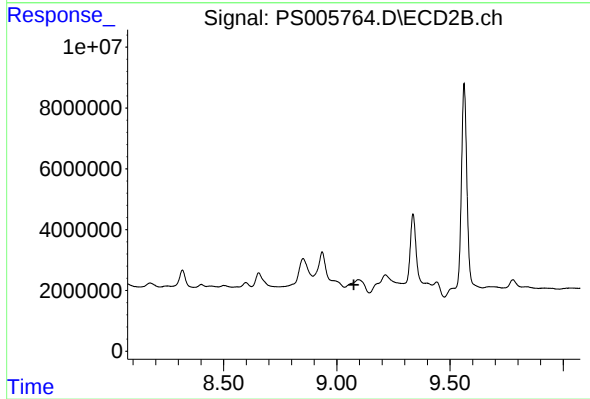

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.075 min
Response: 0
Conc: N.D.