

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072919\
 Data File : PS005769.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2019 15:38
 Operator : SM\AJ
 Sample : K3961-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 02:09:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.560	5.280	330.3E6	233.7E6	227.684	234.932
Target Compounds							
1) T	Dalapon	2.059	0.000	26661972	0	14.386	N.D. #
2) T	3,5-DICHL...	4.931	4.599	8972803	58553402	4.326	45.134 #
5) T	DICAMBA	5.783	5.431	24549719	28605330	4.110	7.663 #
6) T	MCP	0.000	5.431	0	28605330	N.D.	10.043
7) T	MCPA	5.947	5.664	191.3E6	35297178	29.308	8.386 #
8) T	DICHLORPROP	6.344	5.967	14272630	132.6E6	9.925	143.586 #
10) T	Pentachlo...	0.000	6.540	0	22029071	N.D.	1.697
11) T	2,4,5-TP ...	0.000	6.976	0	9995040	N.D.	1.927
12) T	2,4,5-T	0.000	7.384	0	16579528	N.D.	3.488
15) T	Picloram	9.089	9.088	159.6E6	103.2E6	13.635	13.741
16) T	DCPA	0.000	9.088	0	103.2E6	N.D.	15.654



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072919\
Data File : PS005769.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2019 15:38
Operator : SM\AJ
Sample : K3961-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 02:09:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

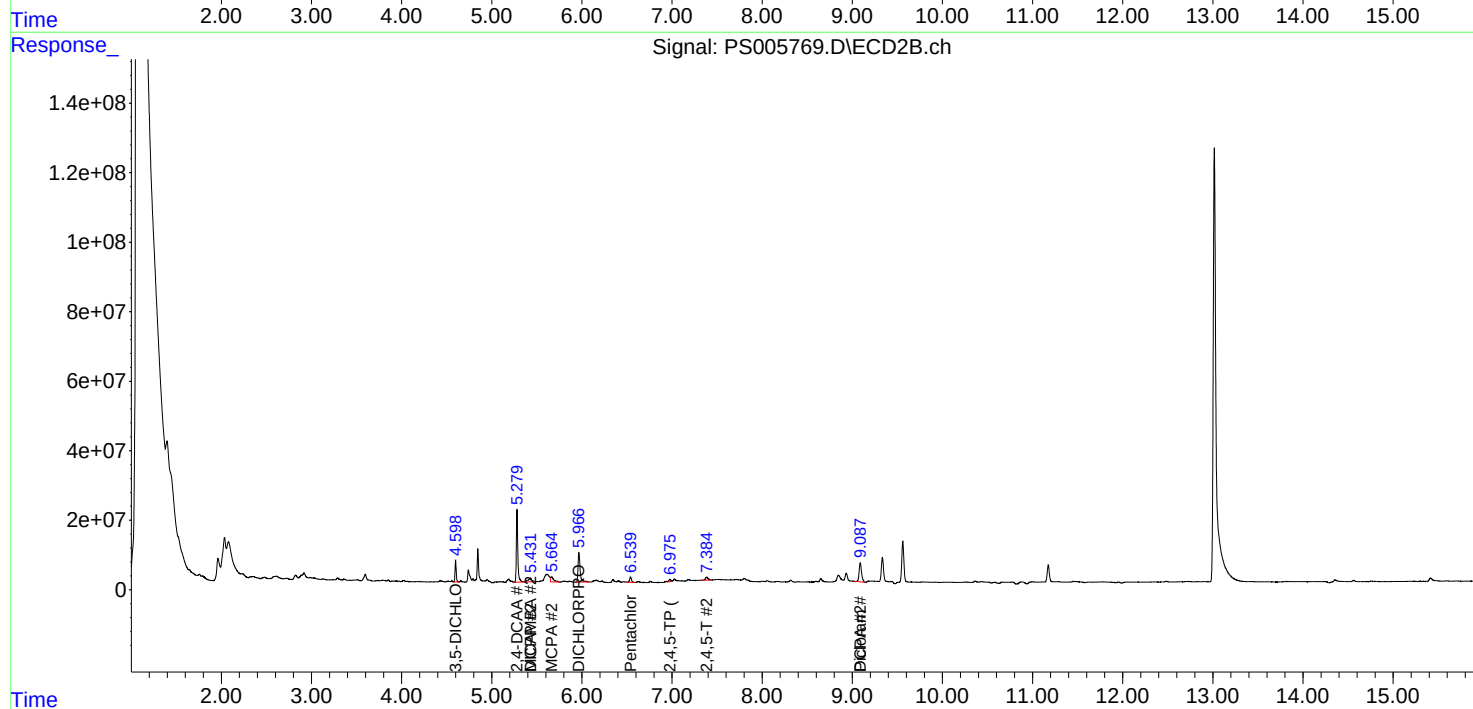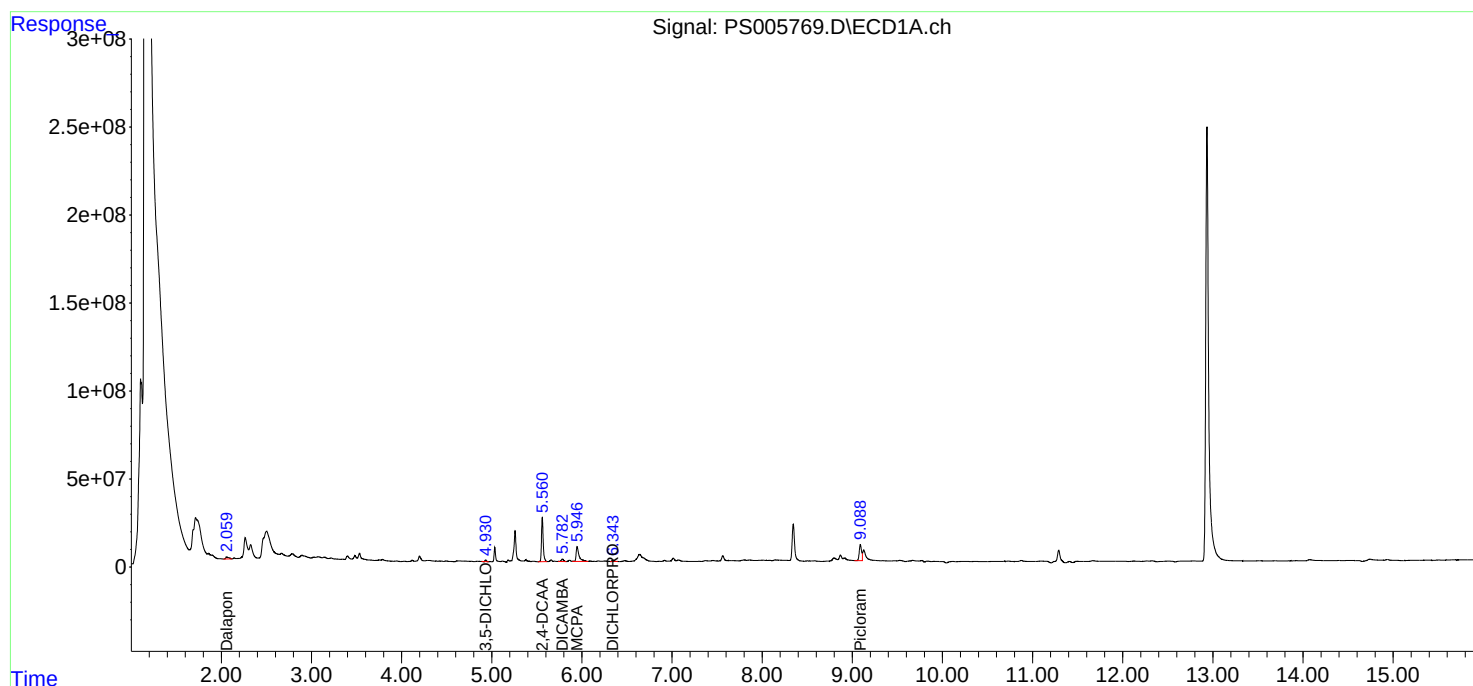


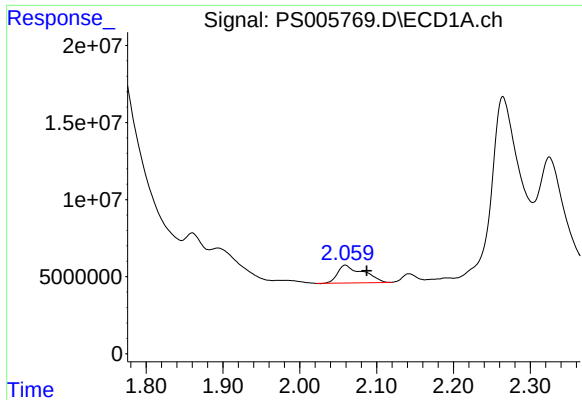

#1 Dalapon


R.T.: 2.059 min
Delta R.T.: -0.028 min
Response: 26661972
Conc: 14.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

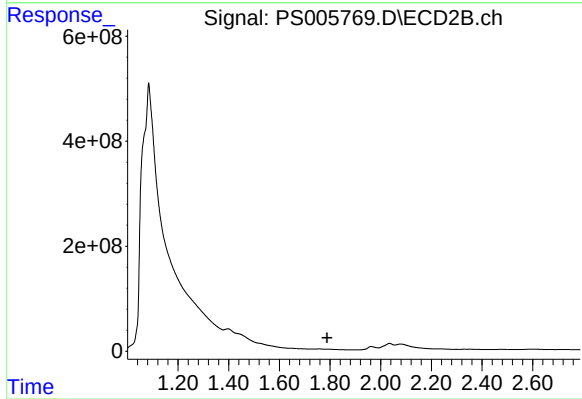


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

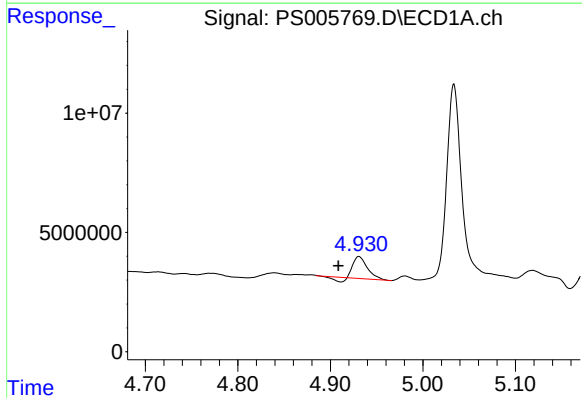


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.931 min
Delta R.T.: 0.022 min
Response: 8972803
Conc: 4.33 ng/ml

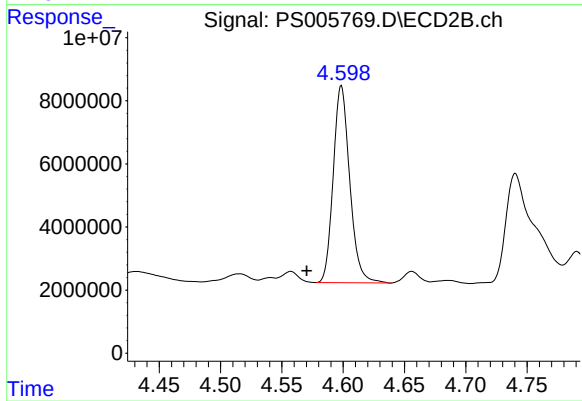

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.599 min
Delta R.T.: 0.028 min
Response: 58553402
Conc: 45.13 ng/ml

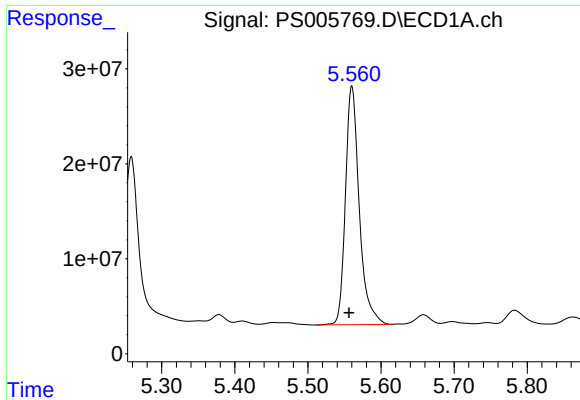

#4 2,4-DCAA


R.T.: 5.560 min
Delta R.T.: 0.004 min
Response: 330328203
Conc: 227.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

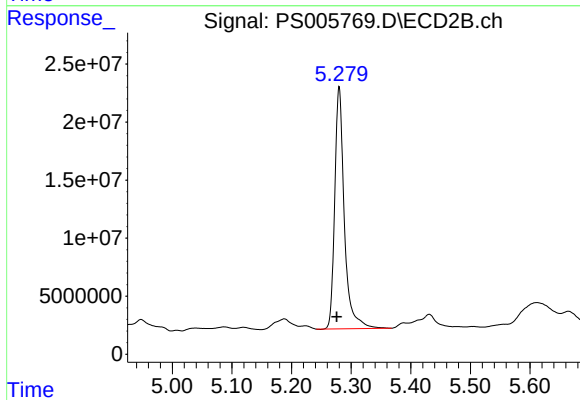


#4 2,4-DCAA

R.T.: 5.280 min
Delta R.T.: 0.004 min
Response: 233681988
Conc: 234.93 ng/ml

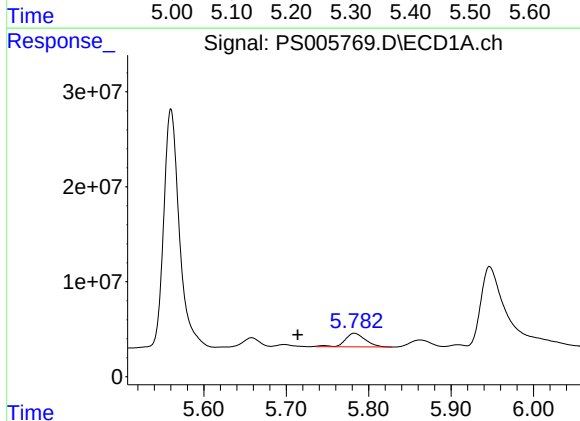


#5 DICAMBA

R.T.: 5.783 min
Delta R.T.: 0.069 min
Response: 24549719
Conc: 4.11 ng/ml

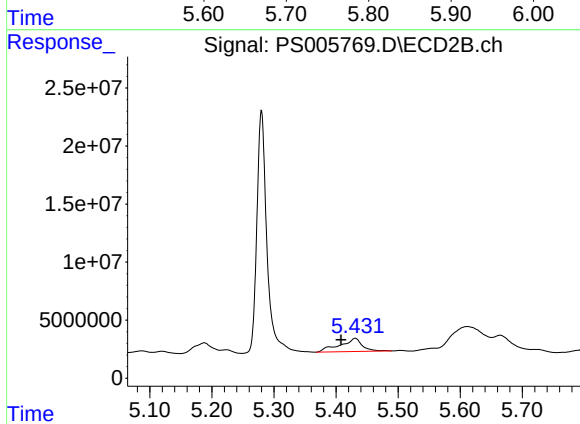

#5 DICAMBA


R.T.: 5.431 min
Delta R.T.: 0.023 min
Response: 28605330
Conc: 7.66 ng/ml

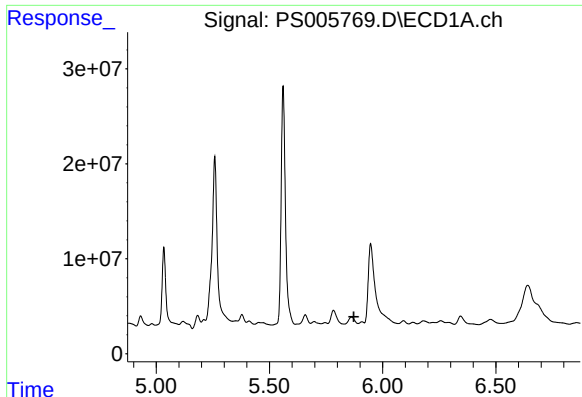

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 5.873 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

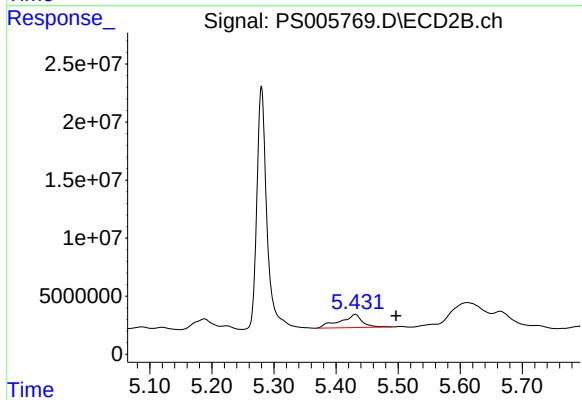


#6 MCPP

R.T.: 5.431 min
Delta R.T.: -0.066 min
Response: 28605330
Conc: 10.04 ug/ml

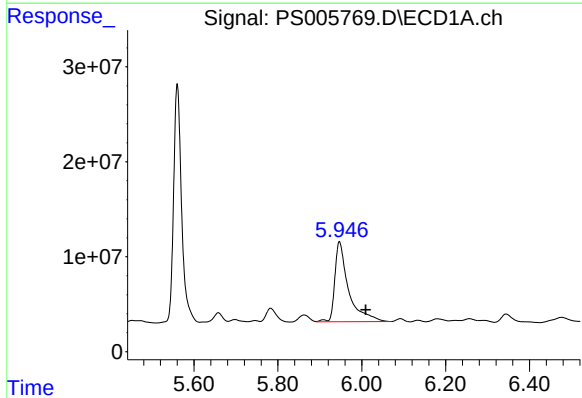


#7 MCPA

R.T.: 5.947 min
Delta R.T.: -0.062 min
Response: 191251123
Conc: 29.31 ug/ml

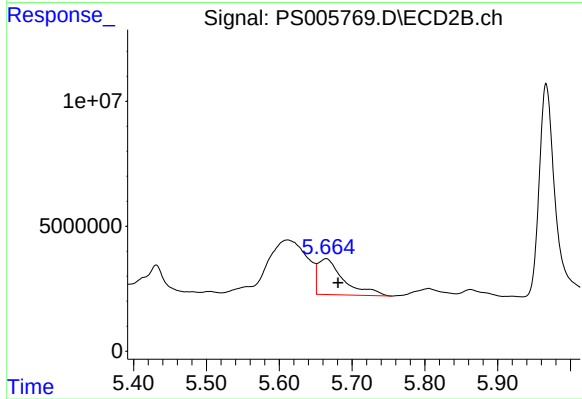

#7 MCPA


R.T.: 5.664 min
Delta R.T.: -0.017 min
Response: 35297178
Conc: 8.39 ug/ml

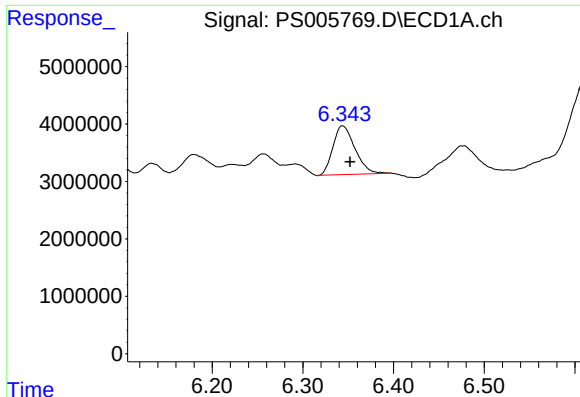

#8 DICHLORPROP


R.T.: 6.344 min
Delta R.T.: -0.008 min
Response: 14272630
Conc: 9.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

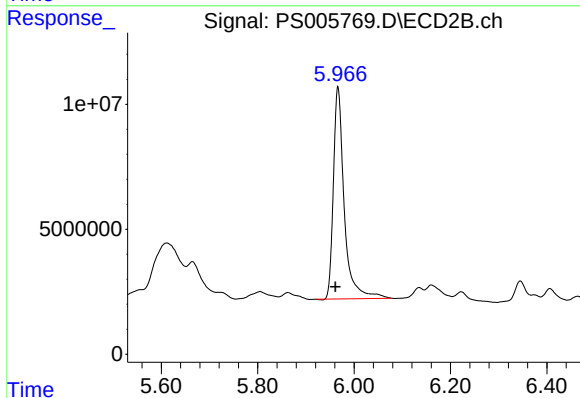


#8 DICHLORPROP

R.T.: 5.967 min
Delta R.T.: 0.005 min
Response: 132604386
Conc: 143.59 ng/ml

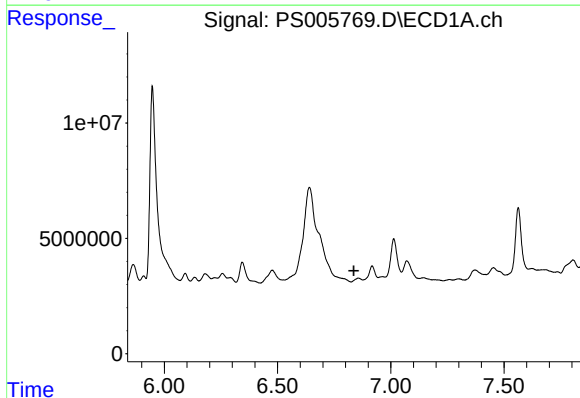


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.837 min
Response: 0
Conc: N.D.

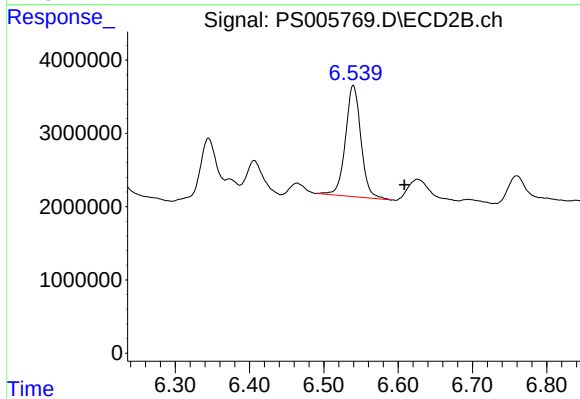

#10 Pentachlorophenol


R.T.: 6.540 min
Delta R.T.: -0.069 min
Response: 22029071
Conc: 1.70 ng/ml

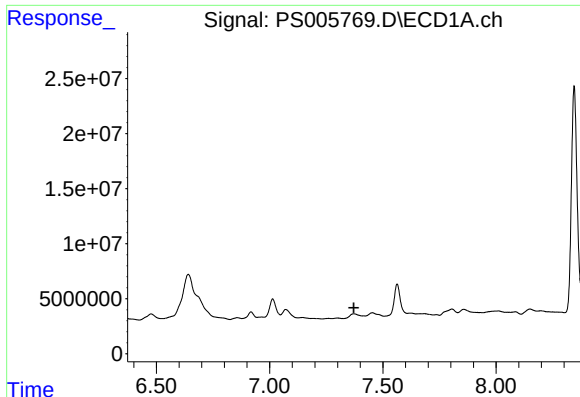

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

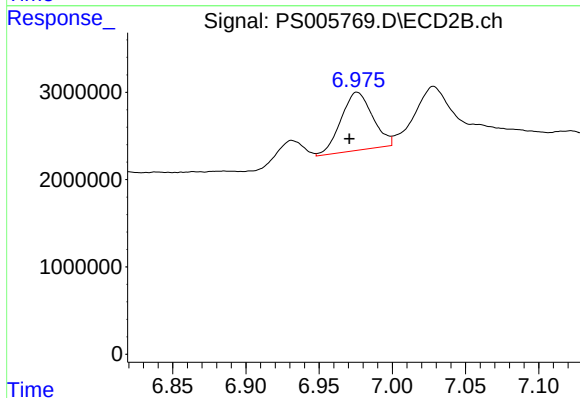


#11 2,4,5-TP (SILVEX)

R.T.: 6.976 min
Delta R.T.: 0.005 min
Response: 9995040
Conc: 1.93 ng/ml

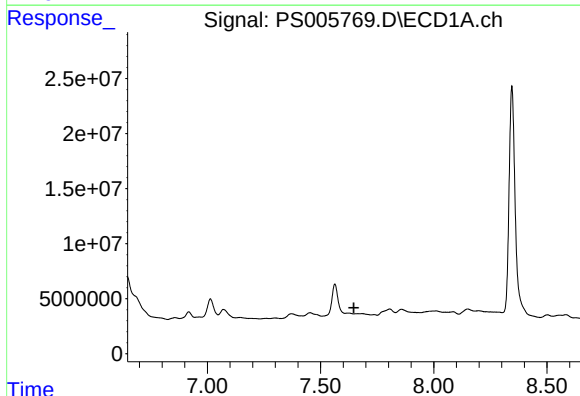


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.647 min
Response: 0
Conc: N.D.

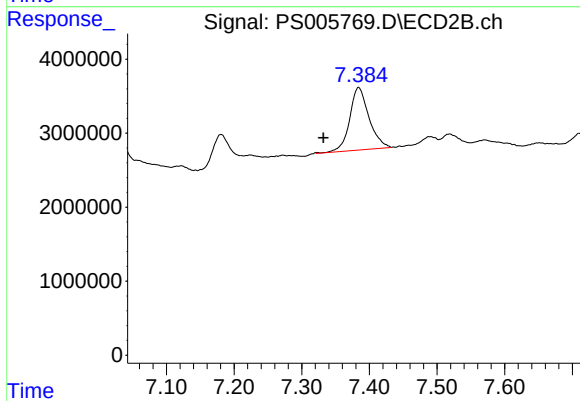

#12 2,4,5-T


R.T.: 7.384 min
Delta R.T.: 0.052 min
Response: 16579528
Conc: 3.49 ng/ml

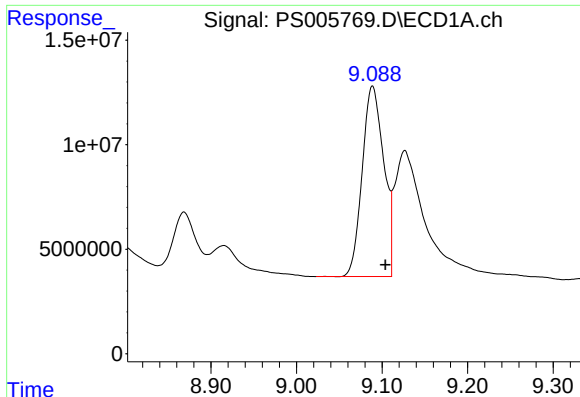

#15 Picloram


R.T.: 9.089 min
Delta R.T.: -0.015 min
Response: 159602014
Conc: 13.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

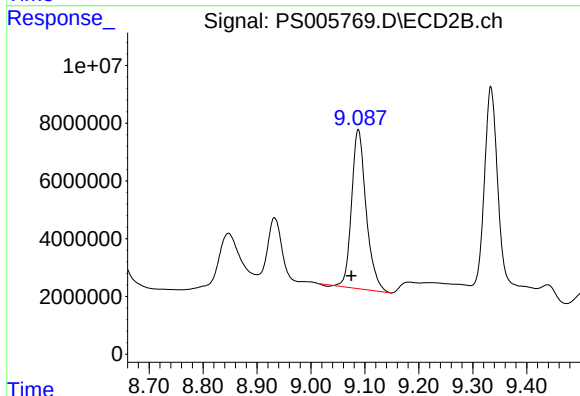


#15 Picloram

R.T.: 9.088 min
Delta R.T.: 0.013 min
Response: 103222444
Conc: 13.74 ng/ml

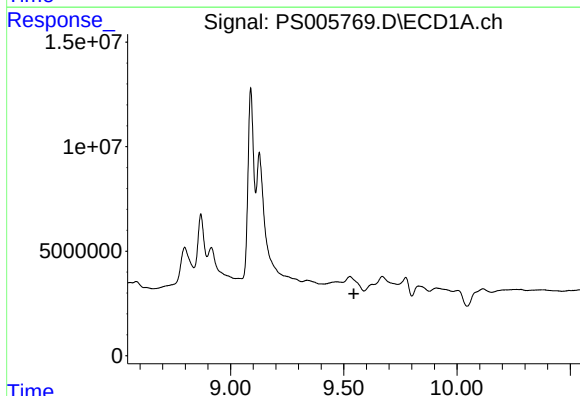

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.545 min
Response: 0
Conc: N.D.

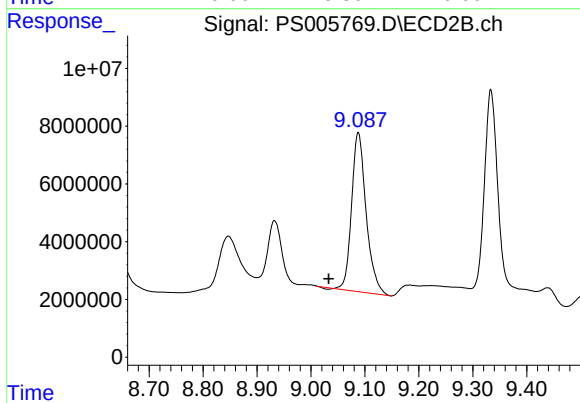

#16 DCPA

R.T.: 9.088 min
Delta R.T.: 0.055 min
Response: 103222444
Conc: 15.65 ng/ml