

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072919\
 Data File : PS005772.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2019 16:44
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 02:10:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.564	5.283	637.8E6	441.0E6	439.588	443.334
Target Compounds							
2) T	3,5-DICHL...	4.939	0.000	21909685	0	10.563	N.D. #
5) T	DICAMBA	0.000	5.438	0	12778632	N.D.	3.423
6) T	MCP	0.000	5.438	0	12778632	N.D.	4.487
7) T	MCPA	0.000	5.613	0	117.6E6	N.D.	27.950
15) T	Picloram	9.099	0.000	170.2E6	0	14.537	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS072919\
Data File : PS005772.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2019 16:44
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 02:10:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

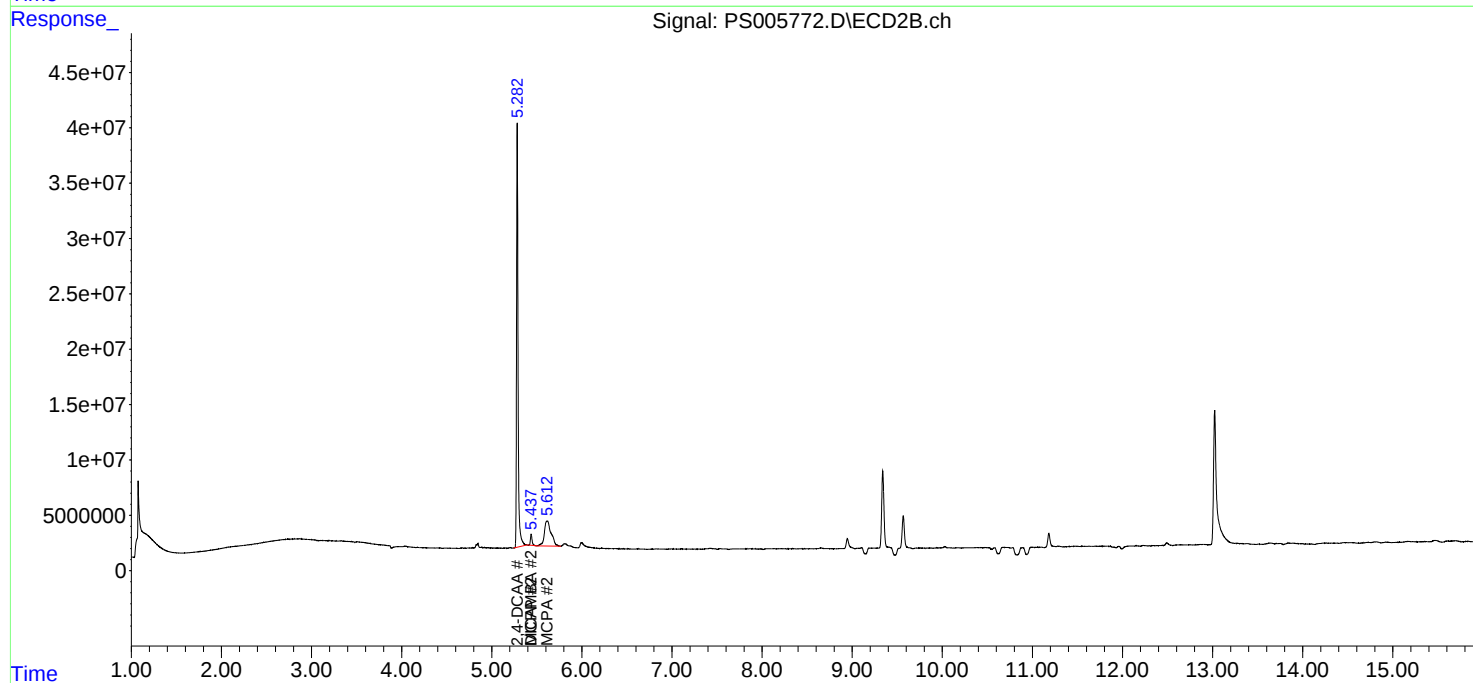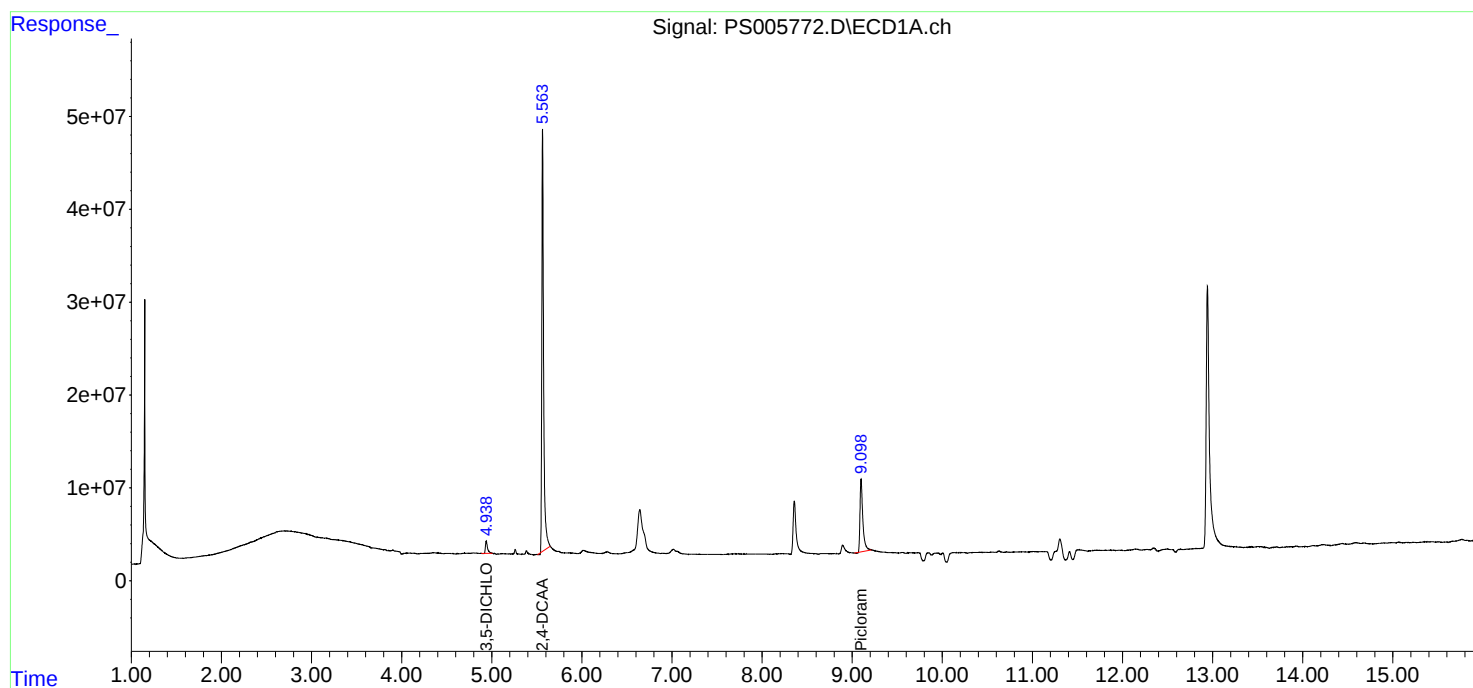


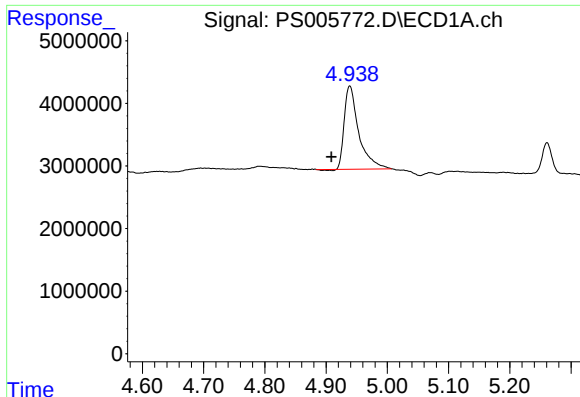

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.939 min
Delta R.T.: 0.030 min
Response: 21909685
Conc: 10.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

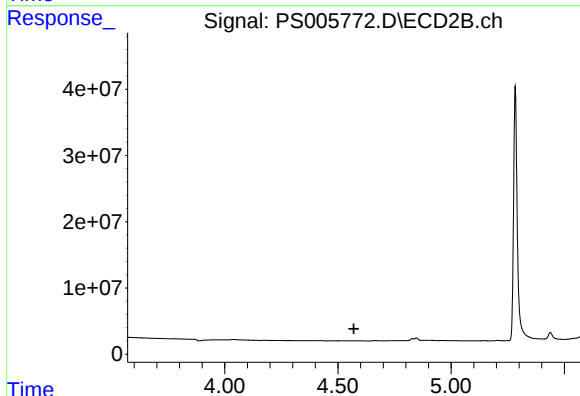


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.570 min
Response: 0
Conc: N.D.

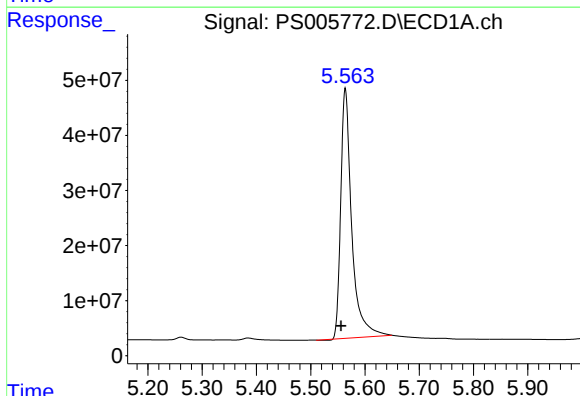


#4 2,4-DCAA

R.T.: 5.564 min
Delta R.T.: 0.008 min
Response: 637761859
Conc: 439.59 ng/ml

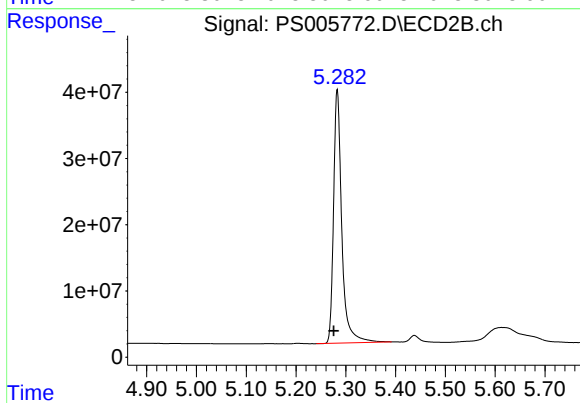

#4 2,4-DCAA


R.T.: 5.283 min
Delta R.T.: 0.007 min
Response: 440974306
Conc: 443.33 ng/ml

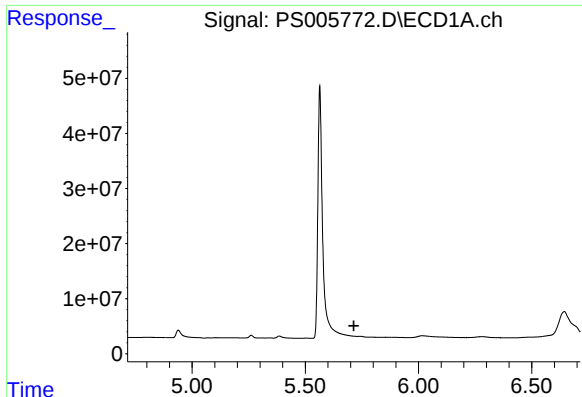

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.714 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

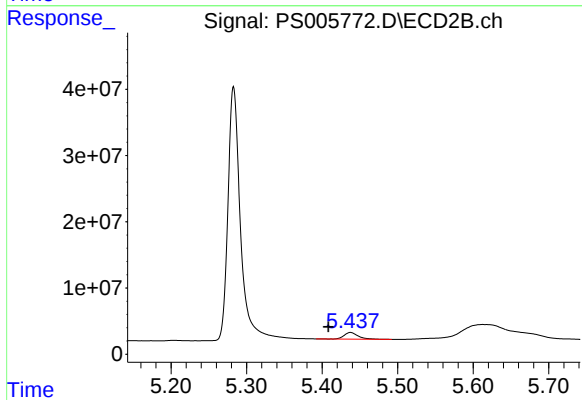


#5 DICAMBA

R.T.: 5.438 min
Delta R.T.: 0.030 min
Response: 12778632
Conc: 3.42 ng/ml

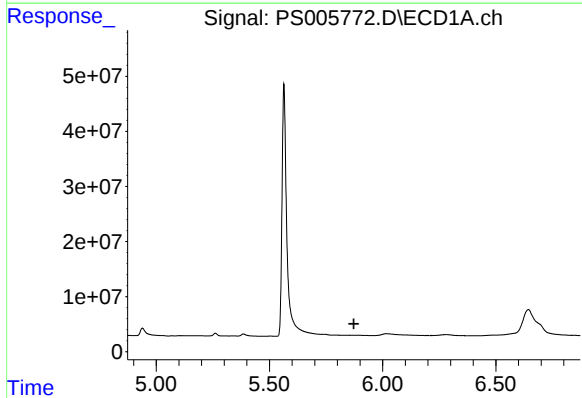


#6 MCP

R.T.: 0.000 min
Exp R.T.: 5.873 min
Response: 0
Conc: N.D.

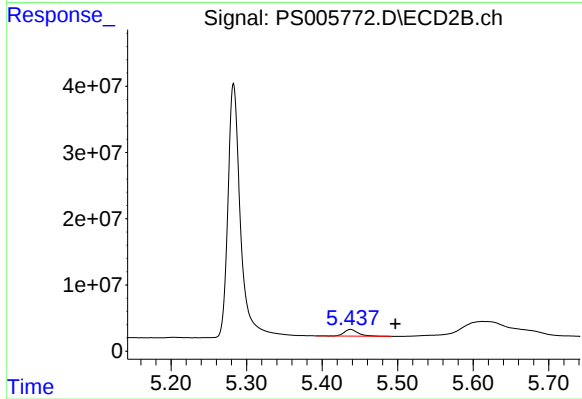

#6 MCP


R.T.: 5.438 min
Delta R.T.: -0.059 min
Response: 12778632
Conc: 4.49 ug/ml

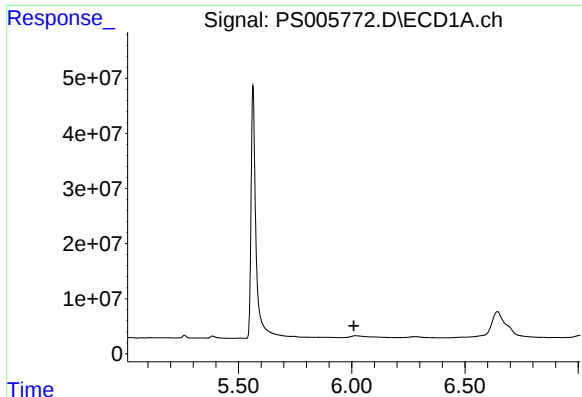

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.009 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

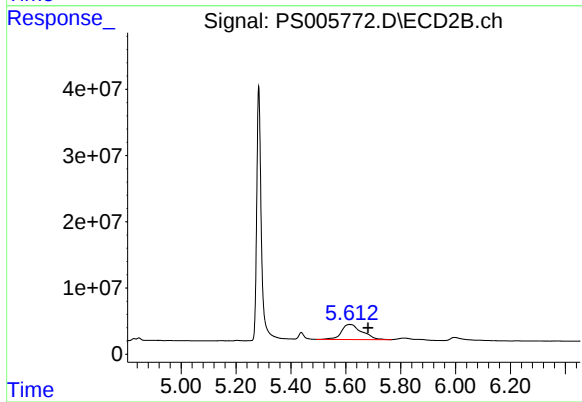


#7 MCPA

R.T.: 5.613 min
Delta R.T.: -0.067 min
Response: 117643712
Conc: 27.95 ug/ml

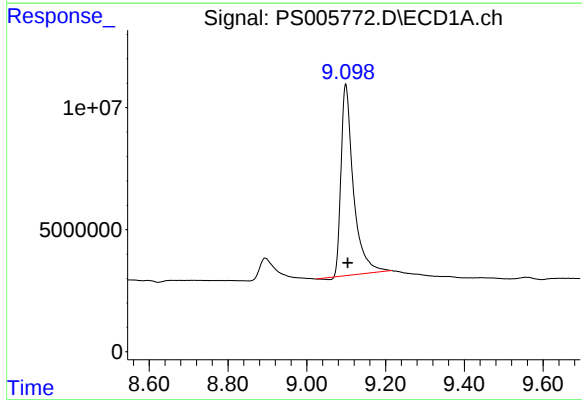

#15 Picloram

R.T.: 9.099 min
Delta R.T.: -0.005 min
Response: 170151153
Conc: 14.54 ng/ml

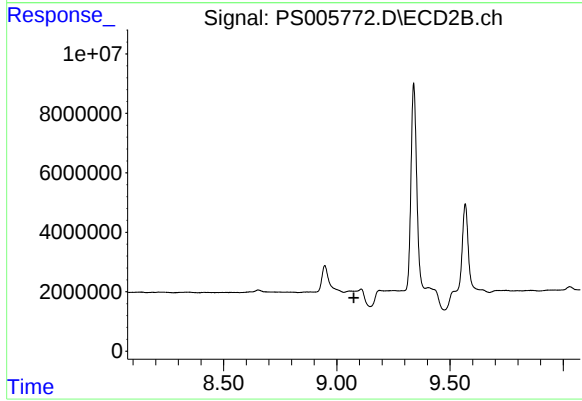

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 9.075 min
Response: 0
Conc: N.D.