

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082019\
 Data File : PS006225.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2019 09:15
 Operator : SM\AJ
 Sample : PB122363BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB122363BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 12:47:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.499	5.226	333.3E6	213.3E6	386.131	433.648
Target Compounds							
1) T	Dalapon	2.037	1.752	62093573	129.8E6	56.986	206.783 #
2) T	3,5-DICHL...	4.877	0.000	228.8E6	0	212.234	N.D. #
5) T	DICAMBA	0.000	5.368	0	154.4E6	N.D.	83.700
7) T	MCPA	5.899	0.000	181.0E6	0	57.326	N.D. #
8) T	DICHLORPROP	0.000	5.899	0	125.0E6	N.D.	281.097
9) T	2,4-D	6.518	0.000	428.5E6	0	525.869	N.D. #
12) T	2,4,5-T	0.000	7.316	0	21632640	N.D.	8.702
15) T	Picloram	9.005	9.006	97174585	70961181	13.060	15.731
16) T	DCPA	0.000	9.006	0	70961181	N.D.	20.349



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082019\
Data File : PS006225.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2019 09:15
Operator : SM\AJ
Sample : PB122363BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
PB122363BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 12:47:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

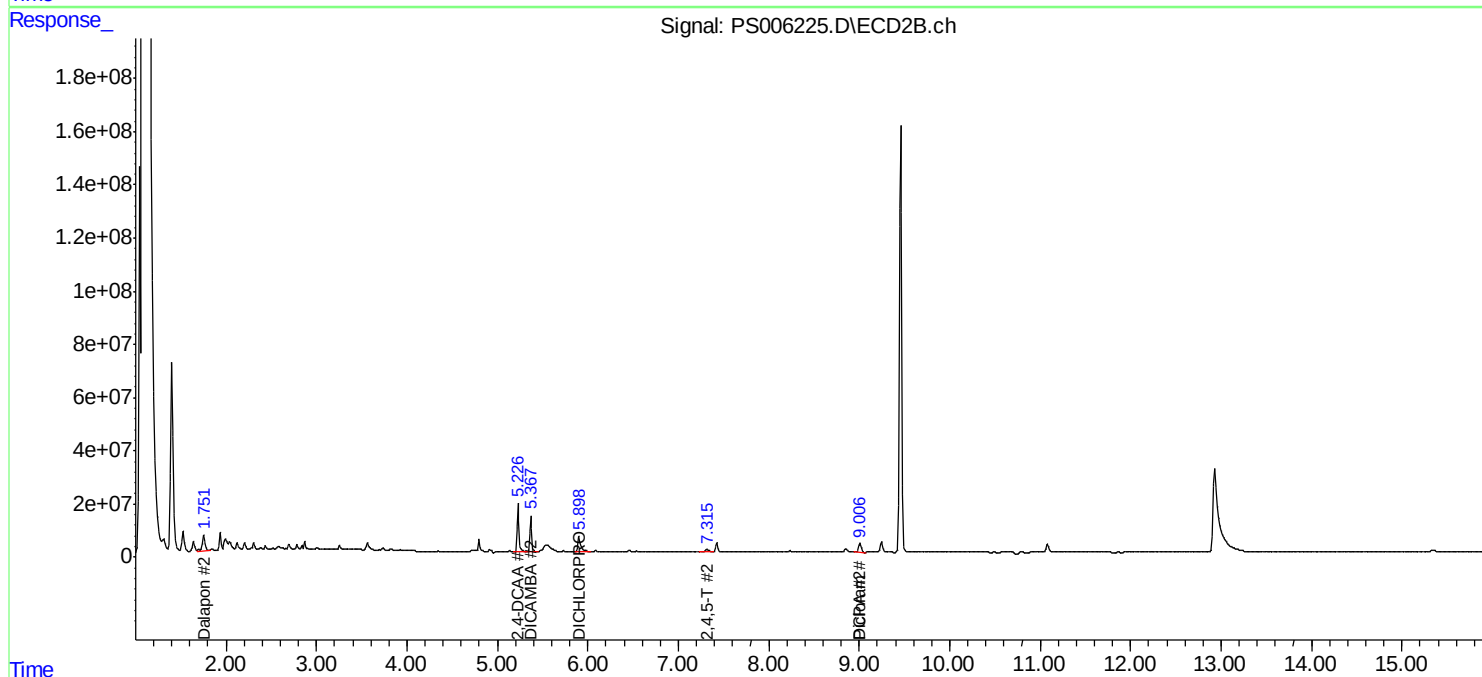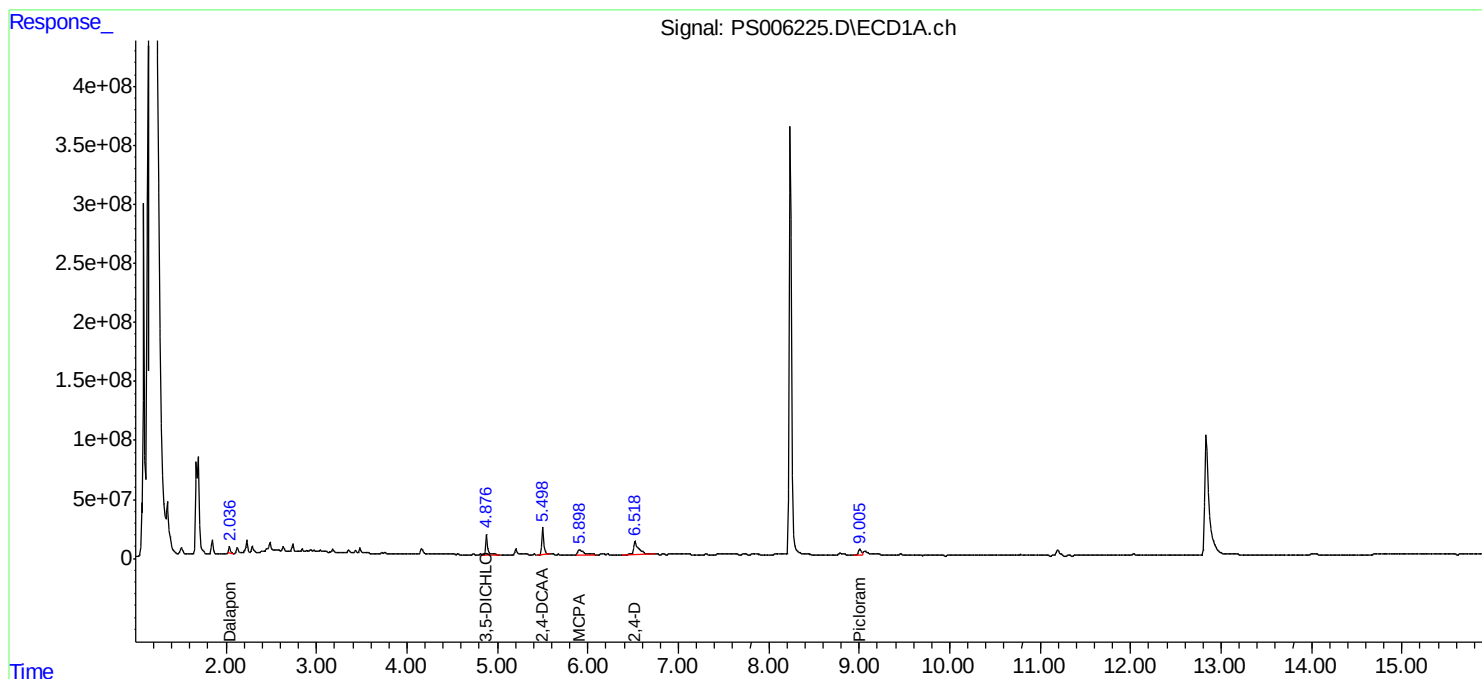


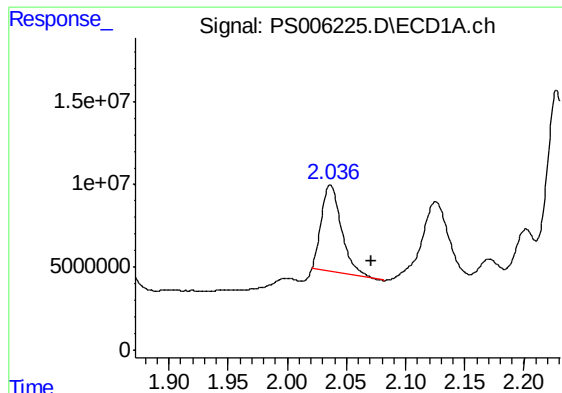

#1 Dalapon


R.T.: 2.037 min
Delta R.T.: -0.034 min
Response: 62093573
Conc: 56.99 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB122363BL

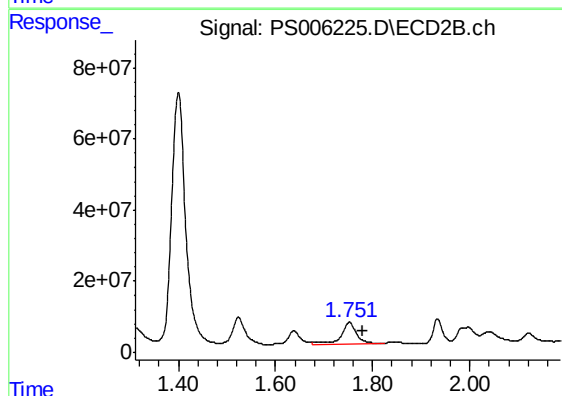


#1 Dalapon

R.T.: 1.752 min
Delta R.T.: -0.027 min
Response: 129754633
Conc: 206.78 ng/ml

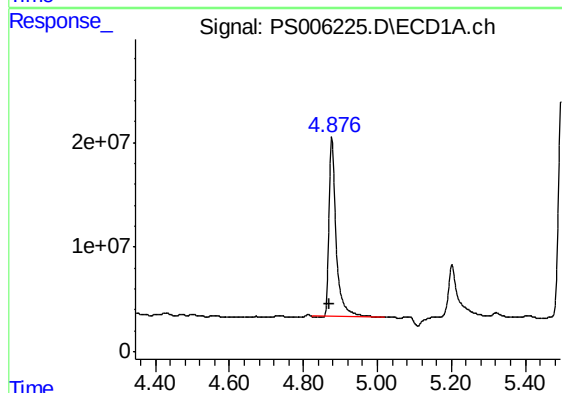


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.877 min
Delta R.T.: 0.005 min
Response: 228816815
Conc: 212.23 ng/ml

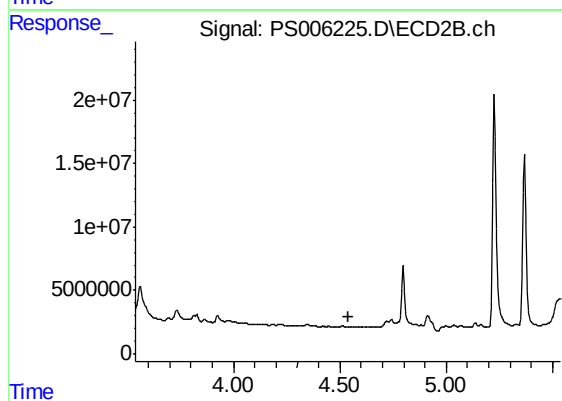

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T. : 4.538 min
Response: 0
Conc: N.D.

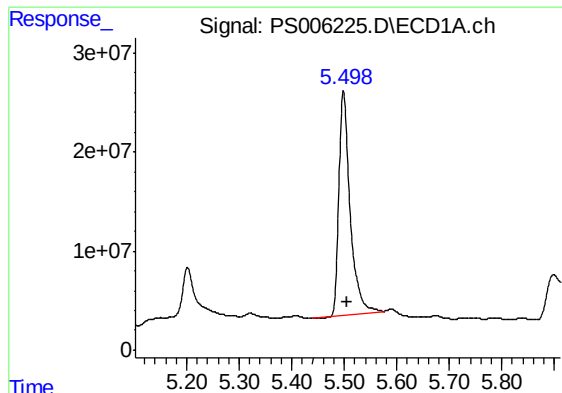

#4 2,4-DCAA


R.T.: 5.499 min
Delta R.T.: -0.007 min
Response: 333308840
Conc: 386.13 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB122363BL

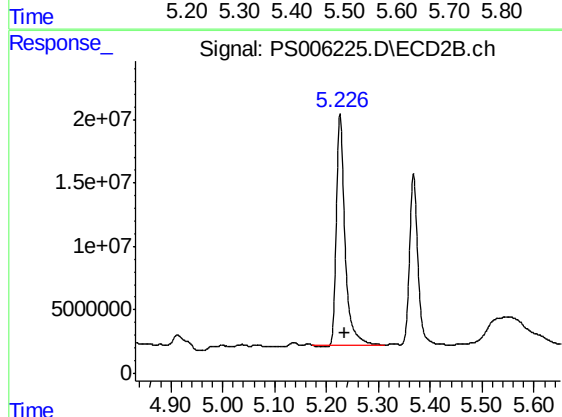


#4 2,4-DCAA

R.T.: 5.226 min
Delta R.T.: -0.010 min
Response: 213290748
Conc: 433.65 ng/ml

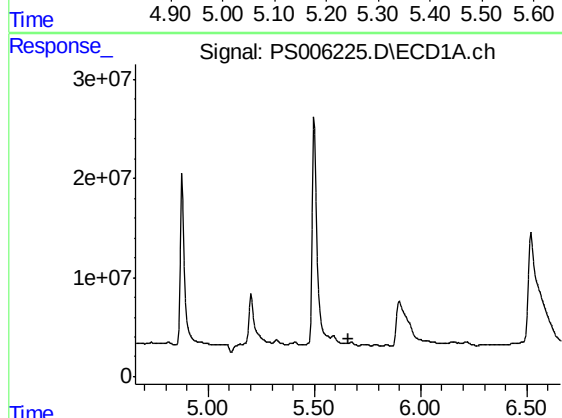


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.658 min
Response: 0
Conc: N.D.

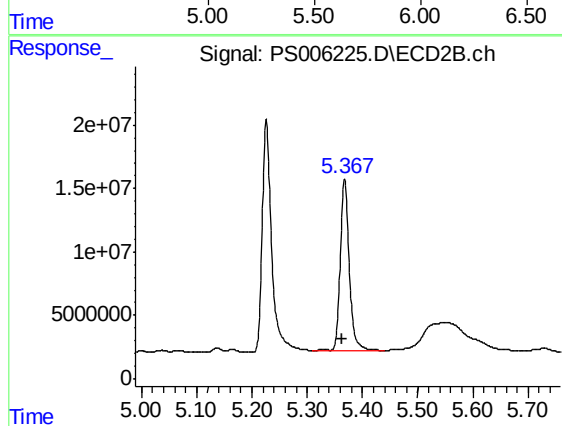

#5 DICAMBA


R.T.: 5.368 min
Delta R.T.: 0.004 min
Response: 154385488
Conc: 83.70 ng/ml

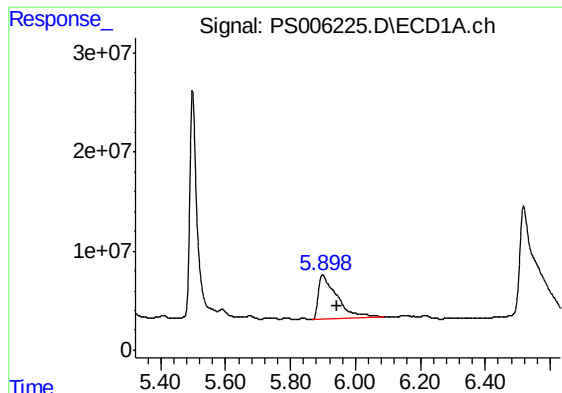

#7 MCPA


R.T.: 5.899 min
Delta R.T.: -0.044 min
Response: 180981990
Conc: 57.33 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB122363BL

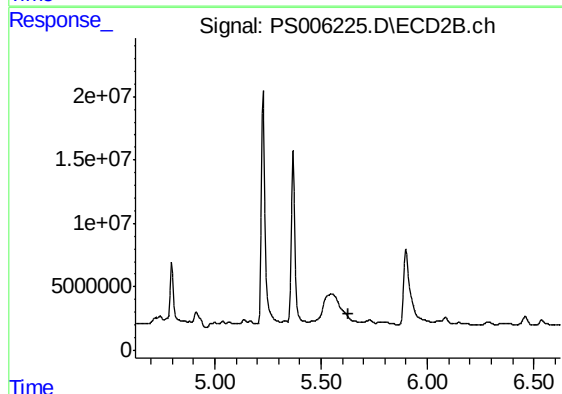


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.626 min
Response: 0
Conc: N.D.

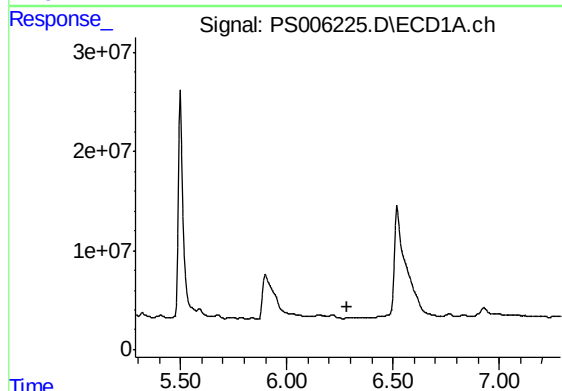


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.288 min
Response: 0
Conc: N.D.

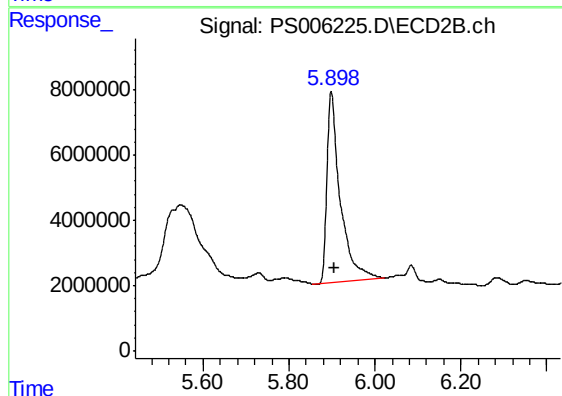

#8 DICHLORPROP


R.T.: 5.899 min
Delta R.T.: -0.006 min
Response: 124976976
Conc: 281.10 ng/ml

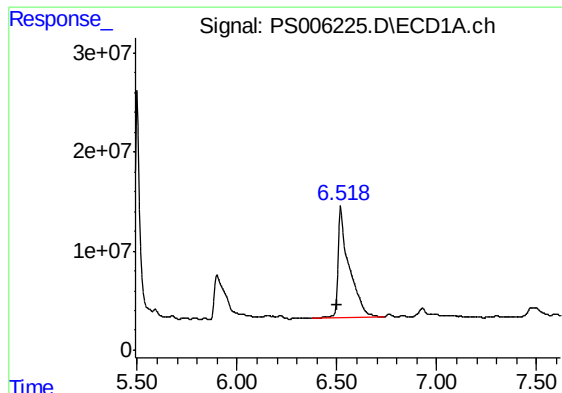

#9 2,4-D


R.T.: 6.518 min
Delta R.T.: 0.016 min
Response: 428470201
Conc: 525.87 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB122363BL

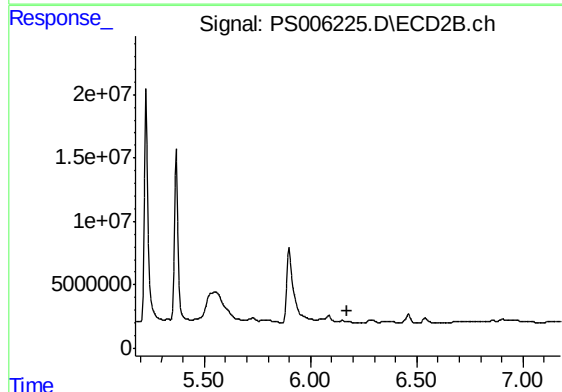


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.176 min
Response: 0
Conc: N.D.

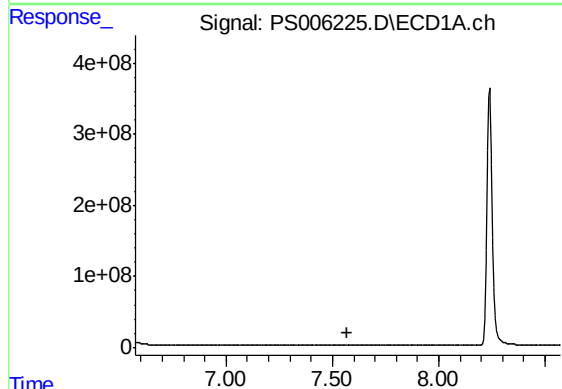


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.573 min
Response: 0
Conc: N.D.

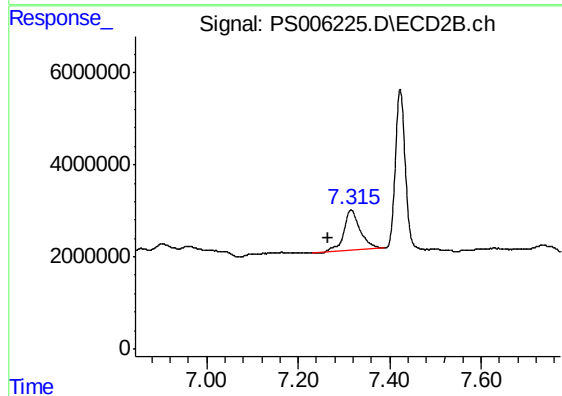

#12 2,4,5-T


R.T.: 7.316 min
Delta R.T.: 0.050 min
Response: 21632640
Conc: 8.70 ng/ml

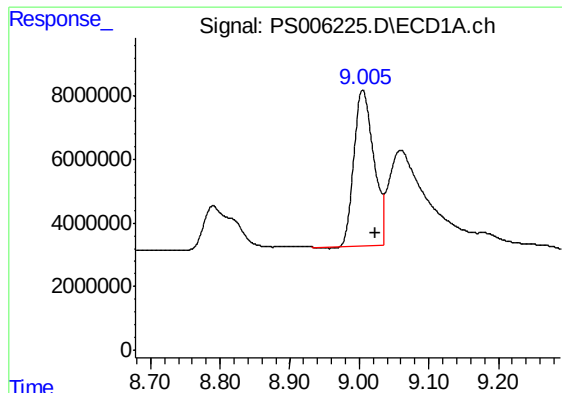

#15 Picloram


R.T.: 9.005 min
Delta R.T.: -0.018 min
Response: 97174585
Conc: 13.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB122363BL

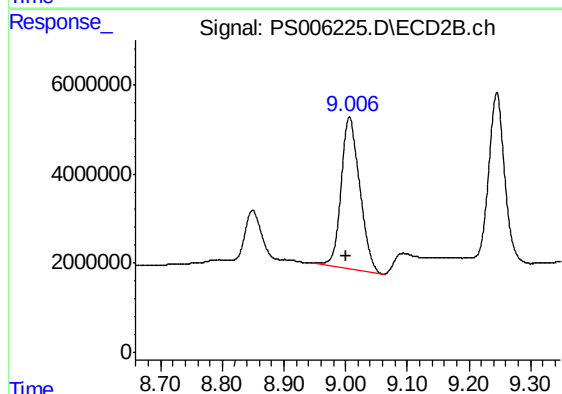


#15 Picloram

R.T.: 9.006 min
Delta R.T.: 0.006 min
Response: 70961181
Conc: 15.73 ng/ml

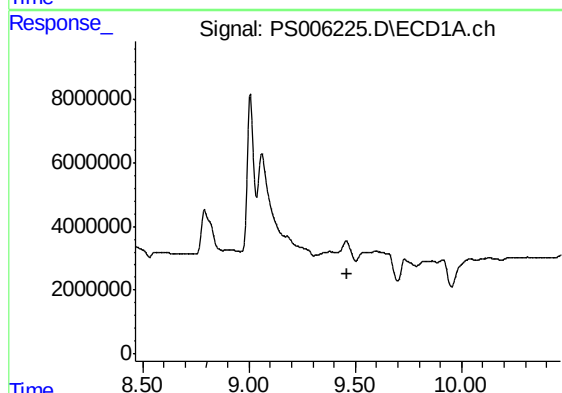

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.465 min
Response: 0
Conc: N.D.

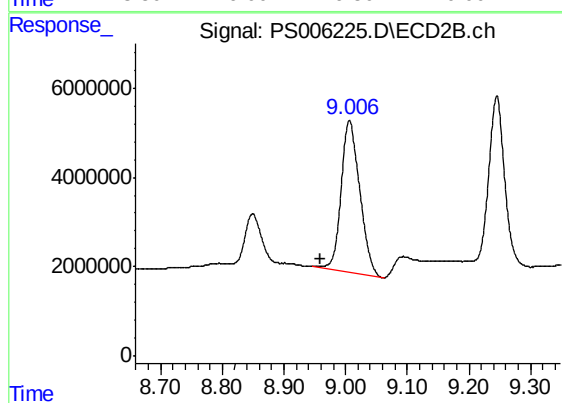

#16 DCPA

R.T.: 9.006 min
Delta R.T.: 0.047 min
Response: 70961181
Conc: 20.35 ng/ml