

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082019\
 Data File : PS006228.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2019 10:21
 Operator : SM\AJ
 Sample : K4250-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SS-18_081519

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 12:48:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.490	5.203	413.5E6	263.9E6	479.005	536.500
Target Compounds							
1) T	Dalapon	2.098	1.730	7452978	116.5E6	6.840	185.593 #
2) T	3,5-DICHL...	4.872	0.000	101.1E6	0	93.777	N.D. #
5) T	DICAMBA	0.000	5.347	0	74486990	N.D.	40.383
7) T	MCPA	5.894	0.000	162.3E6	0	51.410	N.D. #
8) T	DICHLORPROP	0.000	5.878	0	107.6E6	N.D.	241.955
9) T	2,4-D	6.550	0.000	267.6E6	0	328.425	N.D. #
15) T	Picloram	9.002	8.986	39886437	45332042	5.361	10.050 #
16) T	DCPA	0.000	8.986	0	45332042	N.D.	13.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082019\
Data File : PS006228.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2019 10:21
Operator : SM\AJ
Sample : K4250-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
SS-18_081519

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 12:48:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

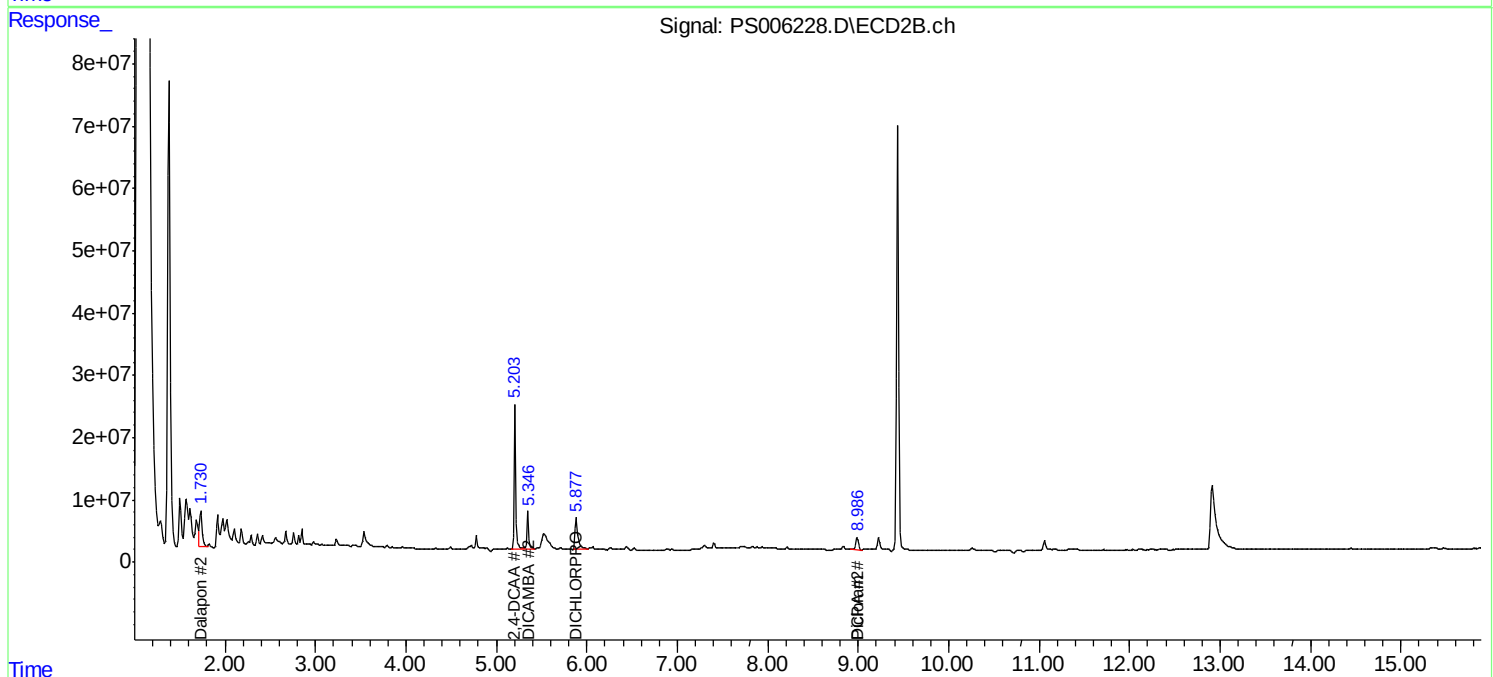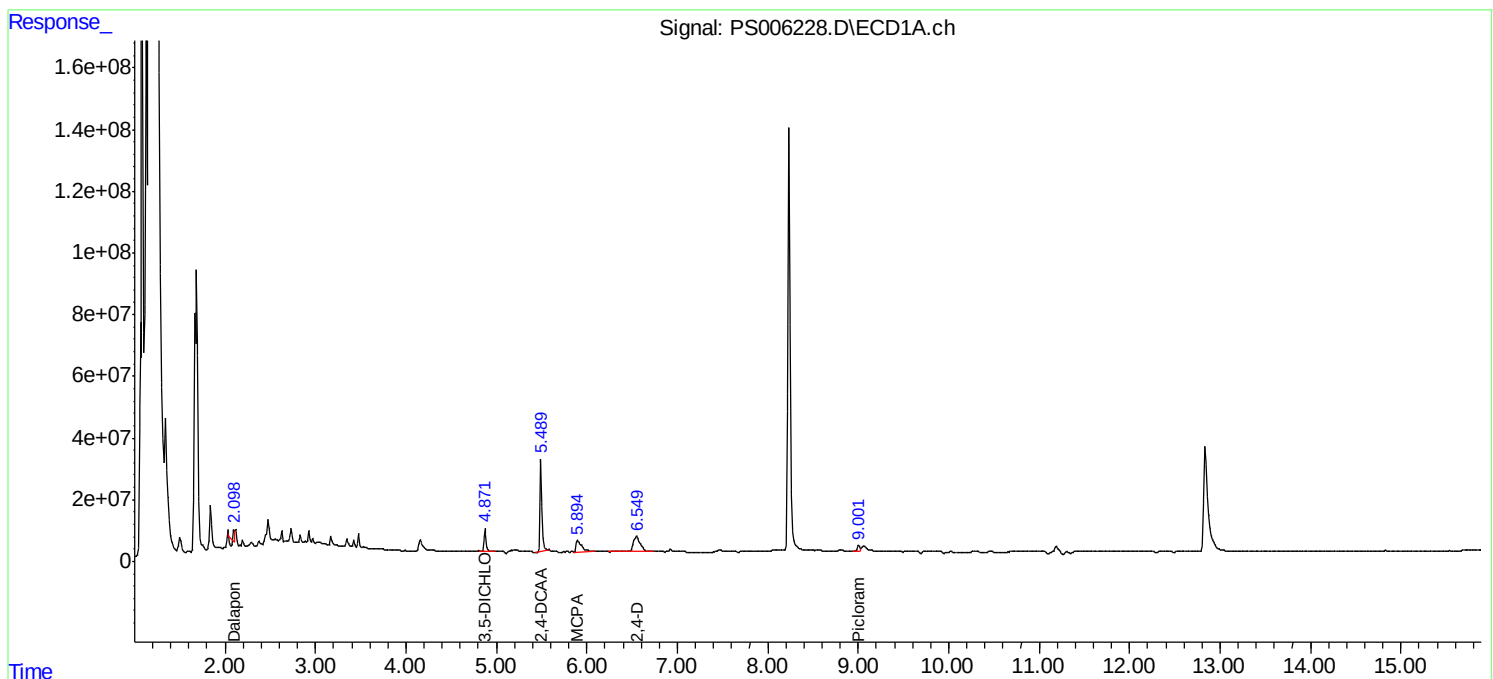


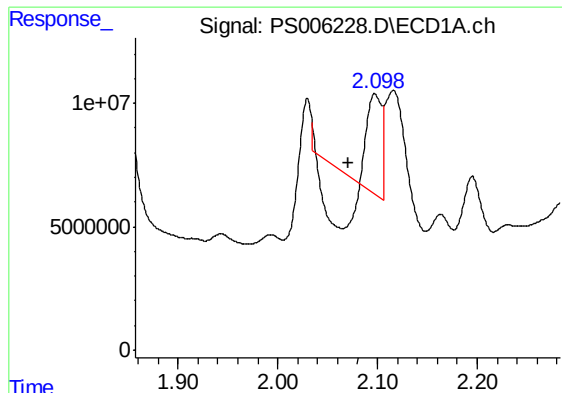

#1 Dalapon


R.T.: 2.098 min
Delta R.T.: 0.027 min
Response: 7452978
Conc: 6.84 ng/ml

Instrument :
ECD_S
ClientSampleId :
SS-18_081519

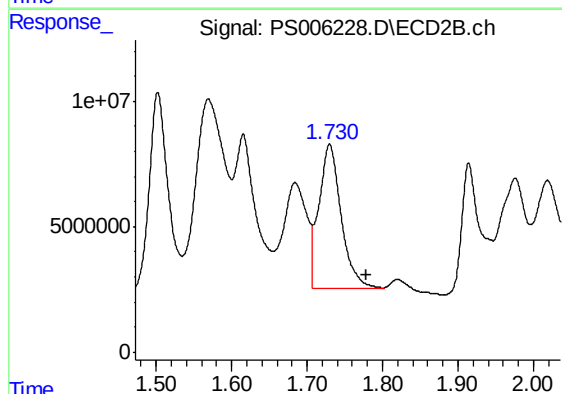


#1 Dalapon

R.T.: 1.730 min
Delta R.T.: -0.049 min
Response: 116458365
Conc: 185.59 ng/ml

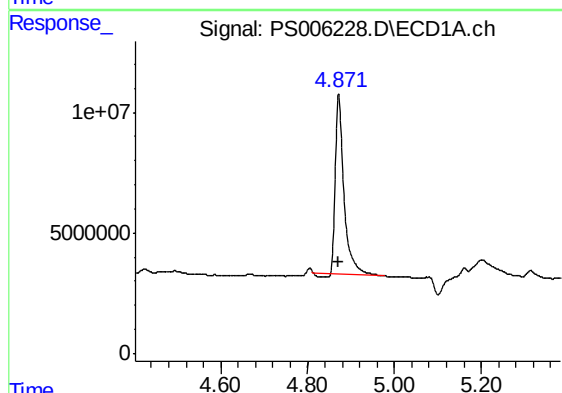


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.872 min
Delta R.T.: 0.000 min
Response: 101104018
Conc: 93.78 ng/ml

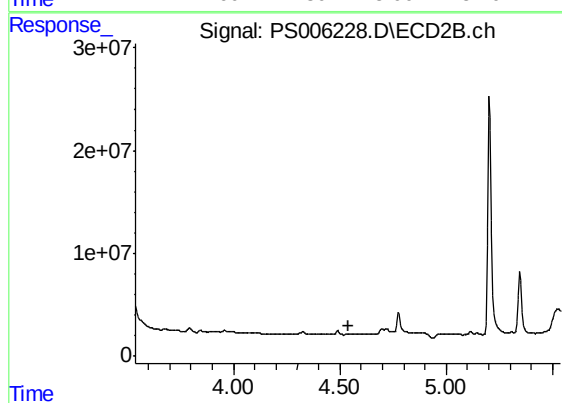

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.538 min
Response: 0
Conc: N.D.

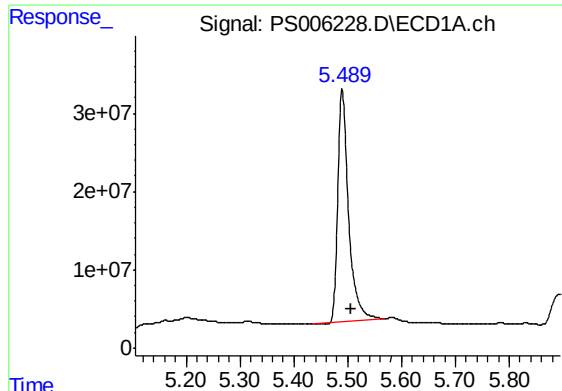

#4 2,4-DCAA


R.T.: 5.490 min
Delta R.T.: -0.015 min
Response: 413477665
Conc: 479.01 ng/ml

Instrument :
ECD_S
ClientSampleId :
SS-18_081519

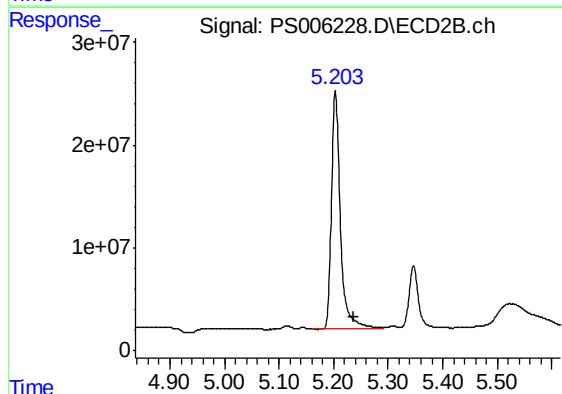


#4 2,4-DCAA

R.T.: 5.203 min
Delta R.T.: -0.032 min
Response: 263878448
Conc: 536.50 ng/ml

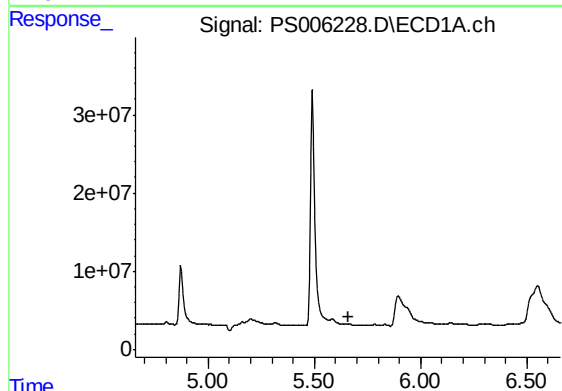


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.658 min
Response: 0
Conc: N.D.

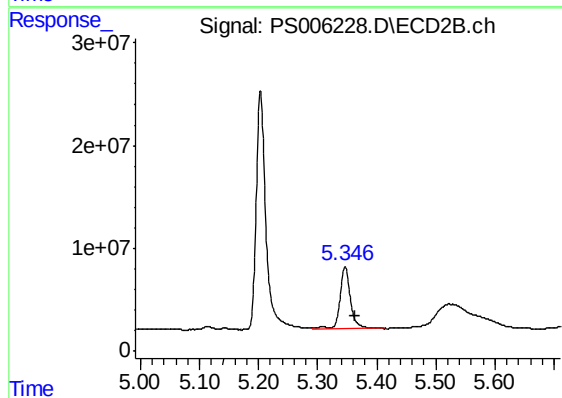

#5 DICAMBA


R.T.: 5.347 min
Delta R.T.: -0.018 min
Response: 74486990
Conc: 40.38 ng/ml

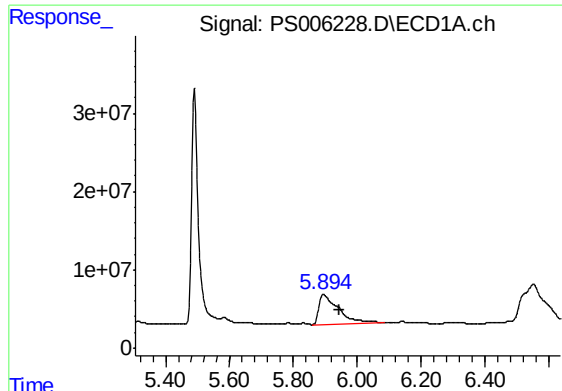

#7 MCPA


R.T.: 5.894 min
Delta R.T.: -0.049 min
Response: 162305271
Conc: 51.41 ug/ml

Instrument :
ECD_S
ClientSampleId :
SS-18_081519

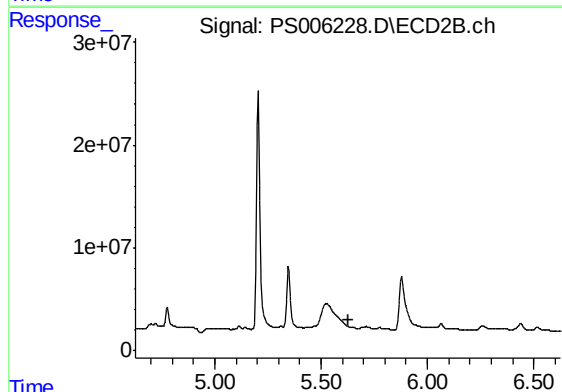


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.626 min
Response: 0
Conc: N.D.

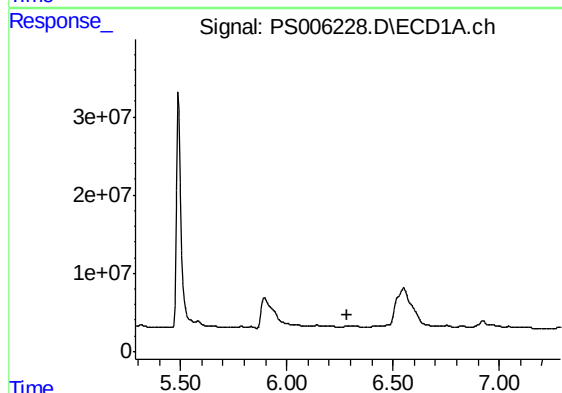


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.288 min
Response: 0
Conc: N.D.

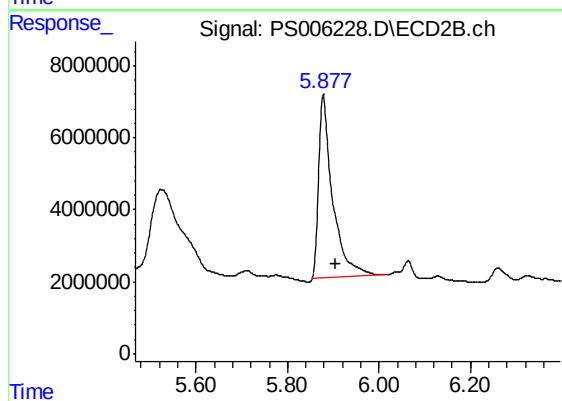

#8 DICHLORPROP


R.T.: 5.878 min
Delta R.T.: -0.027 min
Response: 107574148
Conc: 241.95 ng/ml

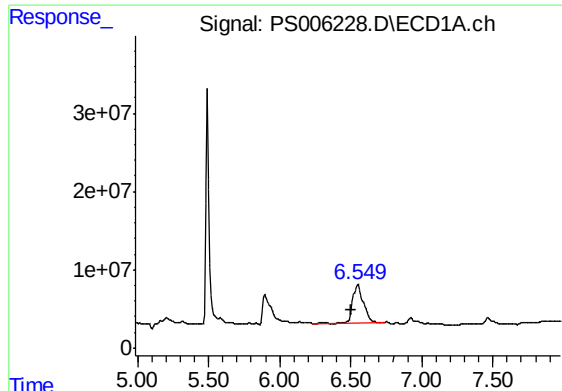

#9 2,4-D


R.T.: 6.550 min
Delta R.T.: 0.047 min
Response: 267595228
Conc: 328.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
SS-18_081519

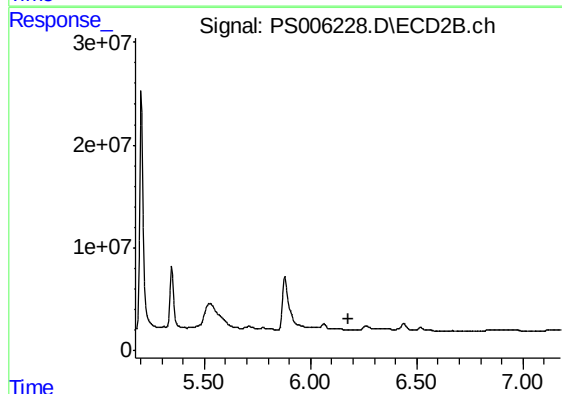


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.176 min
Response: 0
Conc: N.D.

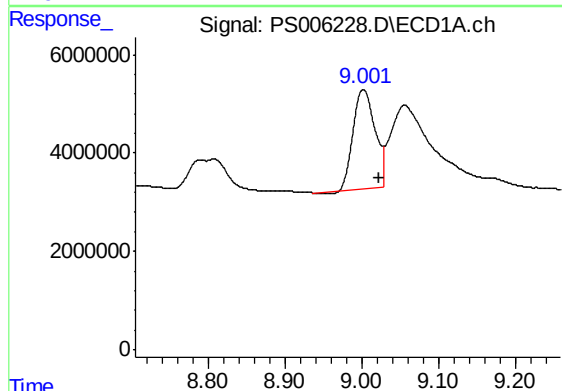


#15 Picloram

R.T.: 9.002 min
Delta R.T.: -0.021 min
Response: 39886437
Conc: 5.36 ng/ml

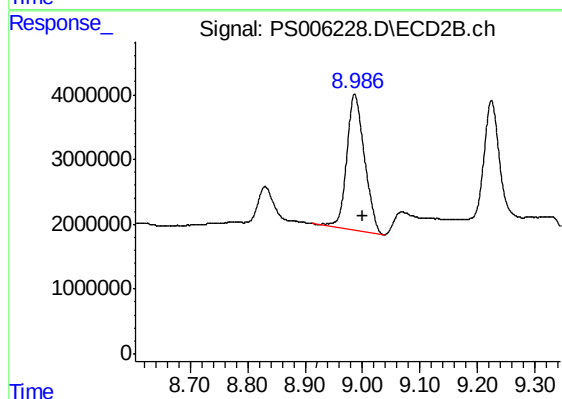

#15 Picloram


R.T.: 8.986 min
Delta R.T.: -0.014 min
Response: 45332042
Conc: 10.05 ng/ml

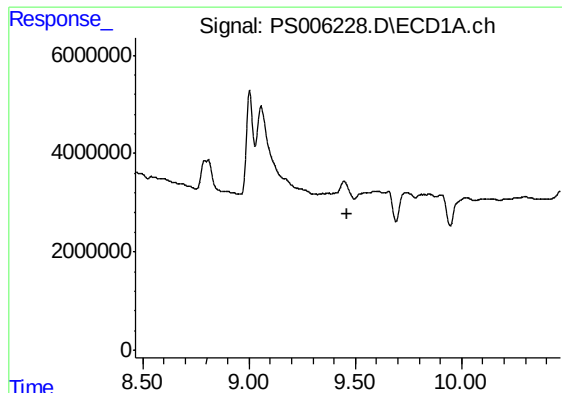

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.465 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SS-18_081519

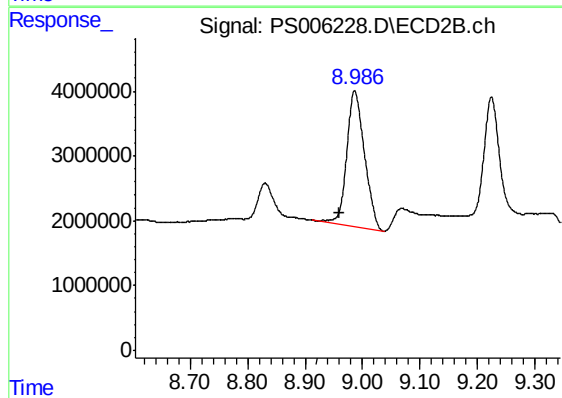

#16 DCPA

R.T.: 8.986 min
Delta R.T.: 0.027 min
Response: 45332042
Conc: 13.00 ng/ml