

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082019\
 Data File : PS006231.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2019 11:27
 Operator : SM\AJ
 Sample : K4385-21
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 T8-A1-A4-(0-2)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 12:49:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.485	5.215	389.9E6	244.4E6	451.685	496.894
Target Compounds							
1) T	Dalapon	2.112	1.741	65757271	127.5E6	60.349	203.225 #
2) T	3,5-DICHL...	4.868	0.000	57355454	0	53.199	N.D. #
5) T	DICAMBA	0.000	5.358	0	44581493	N.D.	24.170
7) T	MCPA	5.886	0.000	139.7E6	0	44.237	N.D. #
8) T	DICHLORPROP	0.000	5.889	0	106.1E6	N.D.	238.546
9) T	2,4-D	6.546	0.000	236.4E6	0	290.114	N.D. #
15) T	Picloram	8.995	0.000	39252383	0	5.275	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082019\
Data File : PS006231.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2019 11:27
Operator : SM\AJ
Sample : K4385-21
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
T8-A1-A4-(0-2)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 12:49:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

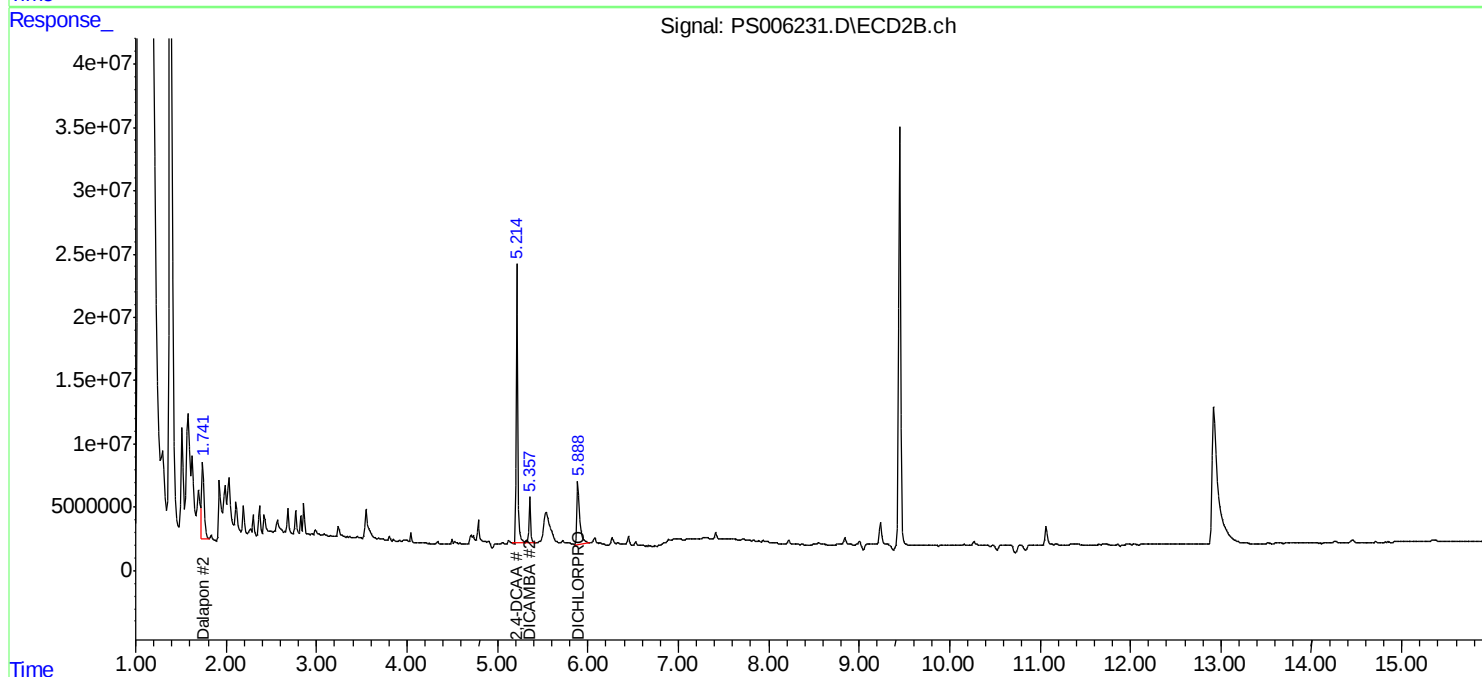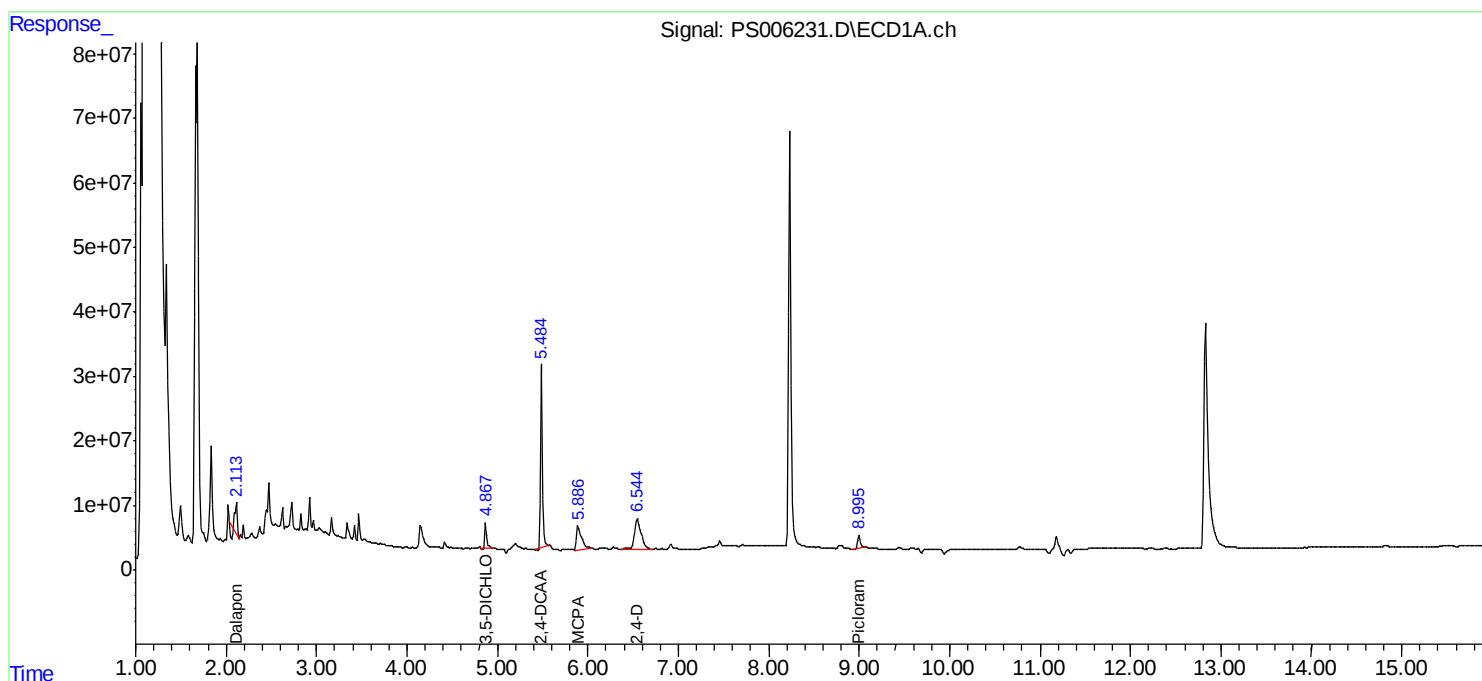


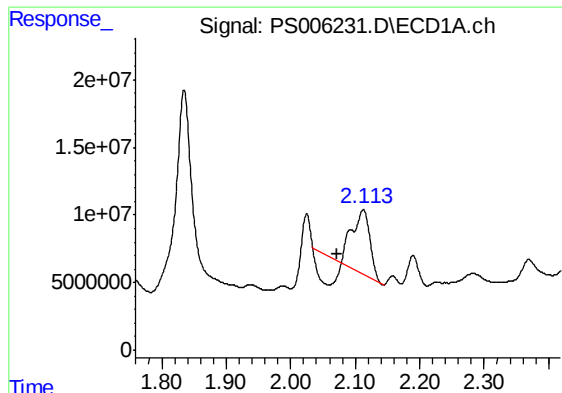

#1 Dalapon


R.T.: 2.112 min
Delta R.T.: 0.041 min
Response: 65757271
Conc: 60.35 ng/ml

Instrument :
ECD_S
ClientSampleId :
T8-A1-A4-(0-2)

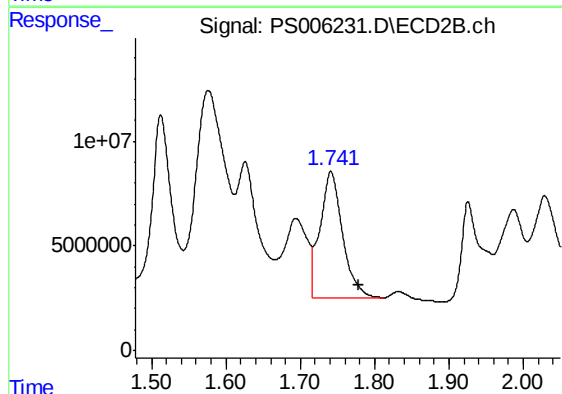


#1 Dalapon

R.T.: 1.741 min
Delta R.T.: -0.038 min
Response: 127522056
Conc: 203.22 ng/ml

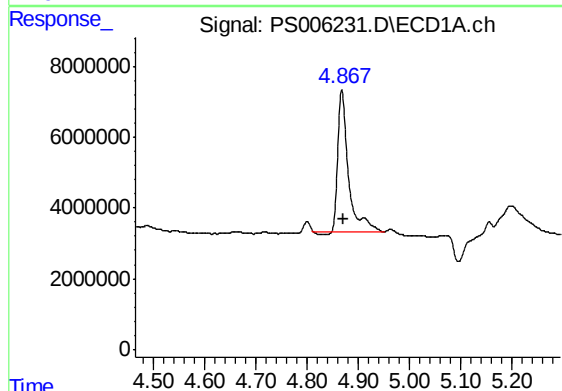


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.868 min
Delta R.T.: -0.004 min
Response: 57355454
Conc: 53.20 ng/ml

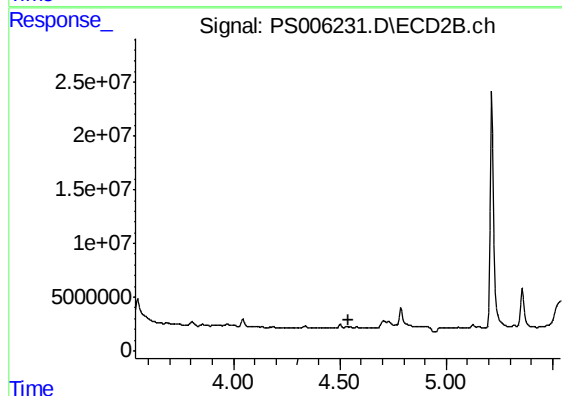

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T. : 4.538 min
Response: 0
Conc: N.D.

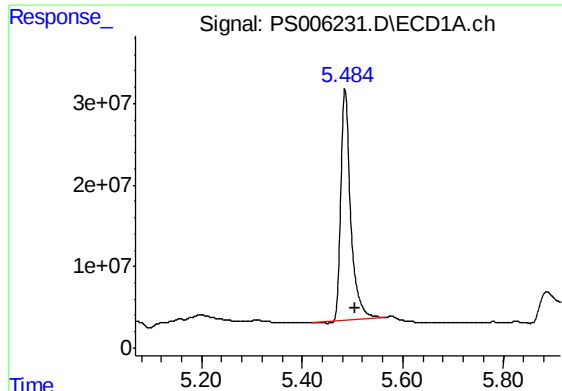

#4 2,4-DCAA


R.T.: 5.485 min
Delta R.T.: -0.020 min
Response: 389894537
Conc: 451.68 ng/ml

Instrument :
ECD_S
ClientSampleId :
T8-A1-A4-(0-2)

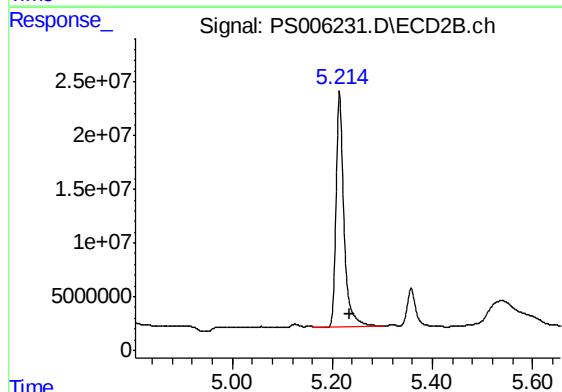


#4 2,4-DCAA

R.T.: 5.215 min
Delta R.T.: -0.021 min
Response: 244398033
Conc: 496.89 ng/ml

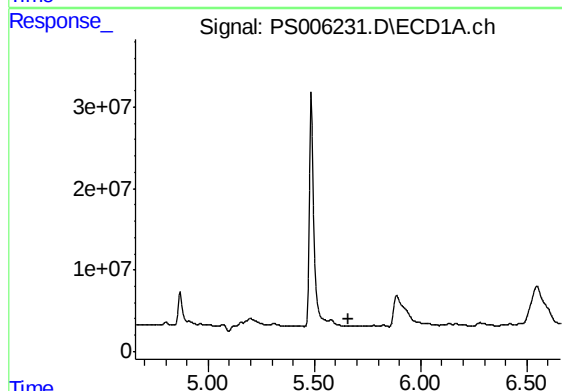


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.658 min
Response: 0
Conc: N.D.

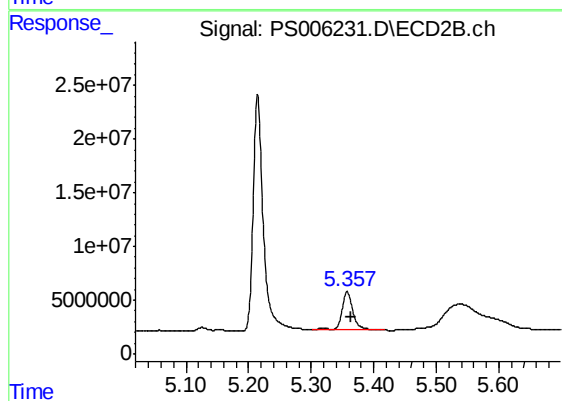

#5 DICAMBA


R.T.: 5.358 min
Delta R.T.: -0.006 min
Response: 44581493
Conc: 24.17 ng/ml

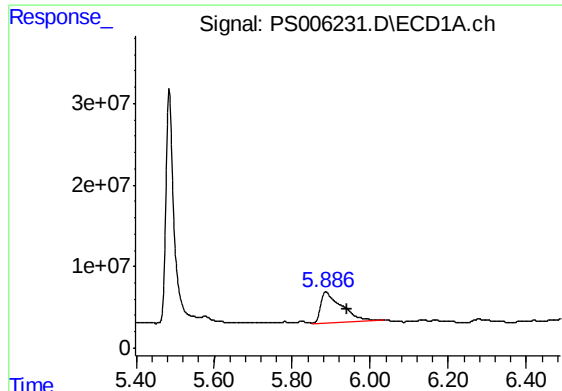

#7 MCPA


R.T.: 5.886 min
Delta R.T.: -0.056 min
Response: 139660701
Conc: 44.24 ug/ml

Instrument :
ECD_S
ClientSampleId :
T8-A1-A4-(0-2)

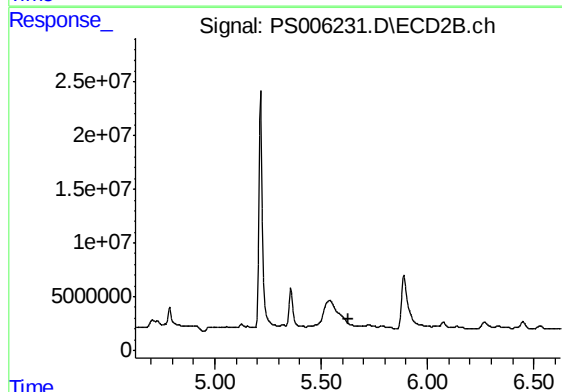


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.626 min
Response: 0
Conc: N.D.

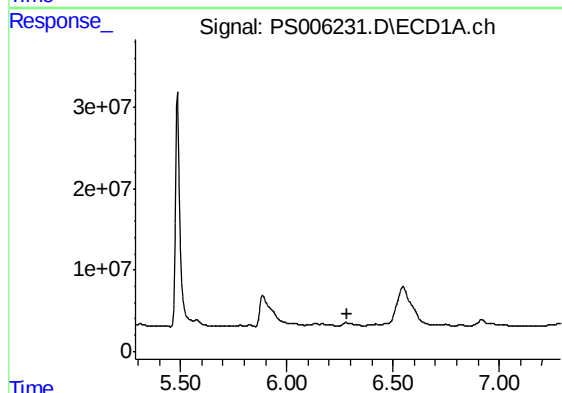


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.288 min
Response: 0
Conc: N.D.

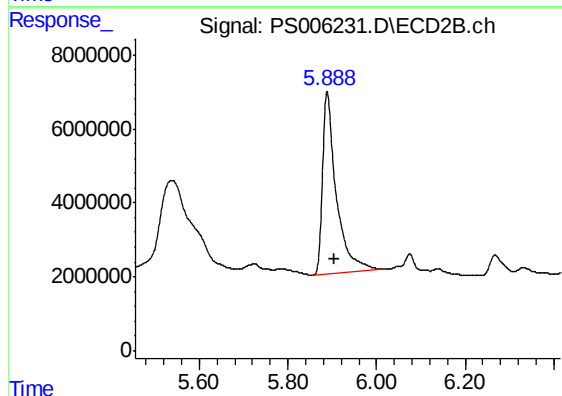

#8 DICHLORPROP


R.T.: 5.889 min
Delta R.T.: -0.016 min
Response: 106058855
Conc: 238.55 ng/ml

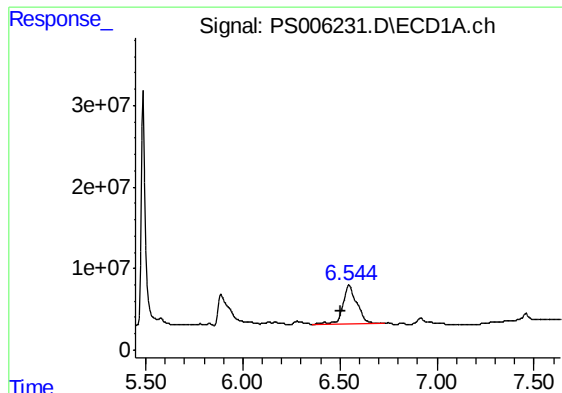

#9 2,4-D


R.T.: 6.546 min
Delta R.T.: 0.043 min
Response: 236380374
Conc: 290.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
T8-A1-A4-(0-2)

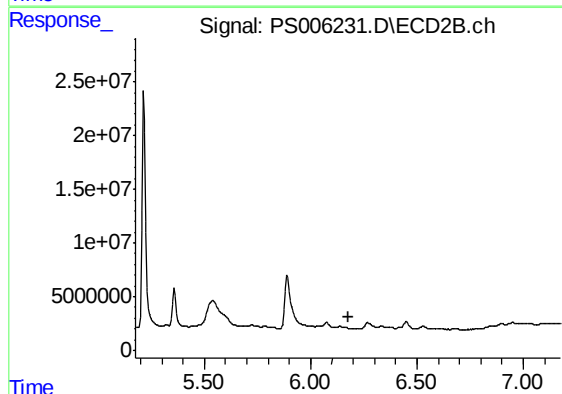


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.176 min
Response: 0
Conc: N.D.

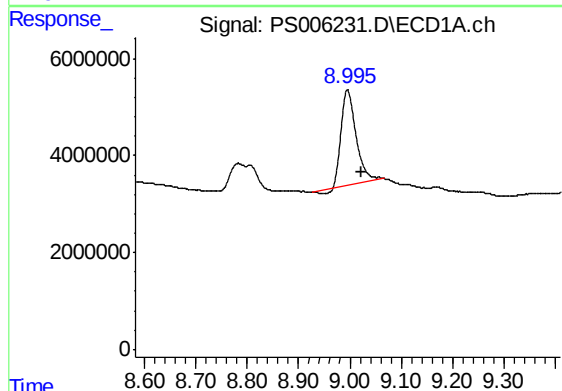

#15 Picloram

R.T.: 8.995 min
Delta R.T.: -0.028 min
Response: 39252383
Conc: 5.28 ng/ml

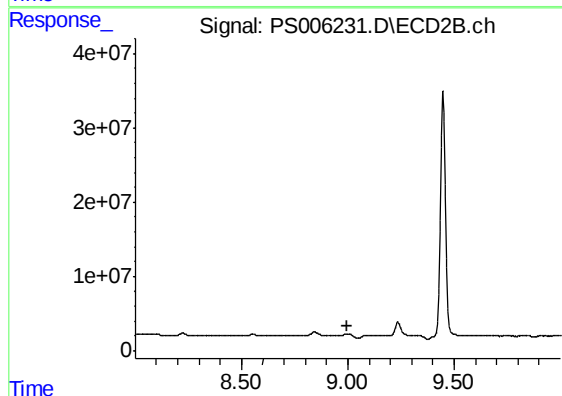

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.000 min
Response: 0
Conc: N.D.