

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082019\
 Data File : PS006234.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2019 12:34
 Operator : SM\AJ
 Sample : K4385-36
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 T8-D-(0-2)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 16:27:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.488	5.218	354.6E6	220.5E6	410.775	448.395
Target Compounds							
1) T	Dalapon	2.115	1.744	54527190	119.5E6	50.042	190.437 #
2) T	3,5-DICHL...	4.872	0.000	26730623	0	24.793	N.D. #
5) T	DICAMBA	0.000	5.361	0	21896401	N.D.	11.871
7) T	MCPA	5.895	0.000	95482130	0	30.244	N.D. #
8) T	DICHLORPROP	0.000	5.893	0	79752588	N.D.	179.379
9) T	2,4-D	6.550	0.000	223.4E6	0	274.170	N.D. #
15) T	Picloram	8.999	0.000	30762723	0	4.134	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082019\
Data File : PS006234.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2019 12:34
Operator : SM\AJ
Sample : K4385-36
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
T8-D-(0-2)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 16:27:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

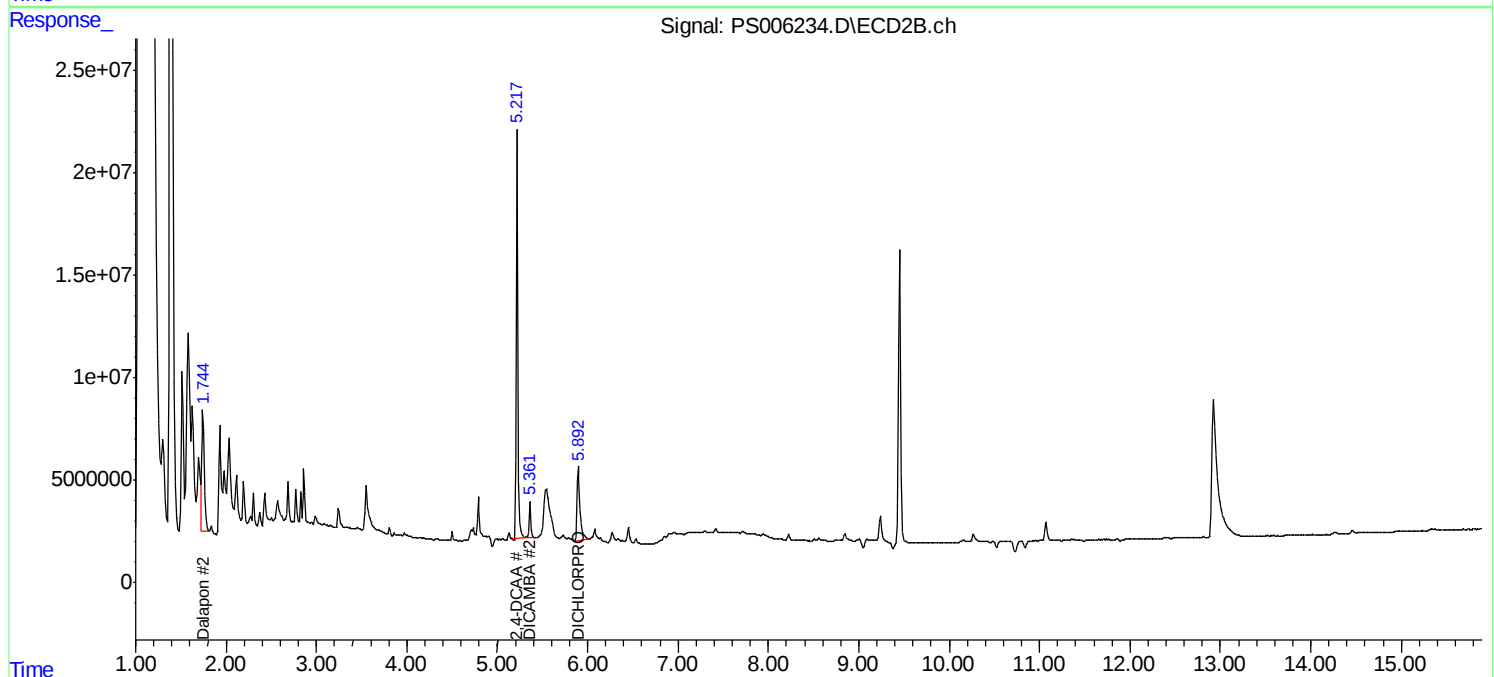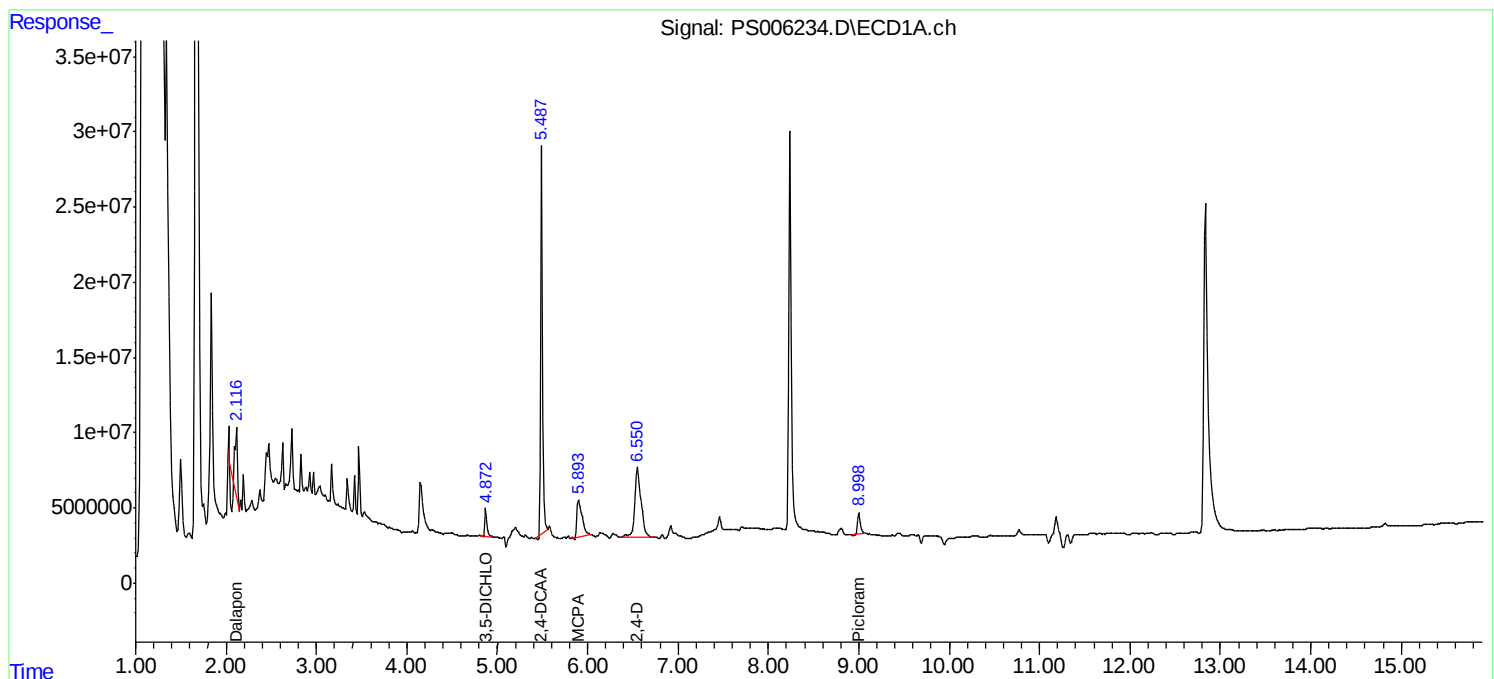


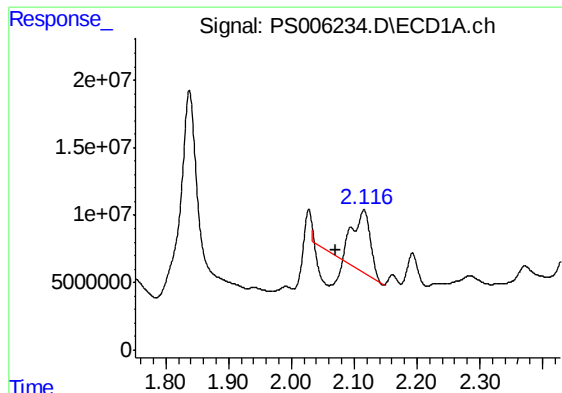

#1 Dalapon


R.T.: 2.115 min
Delta R.T.: 0.044 min
Response: 54527190
Conc: 50.04 ng/ml

Instrument :
ECD_S
ClientSampleId :
T8-D-(0-2)

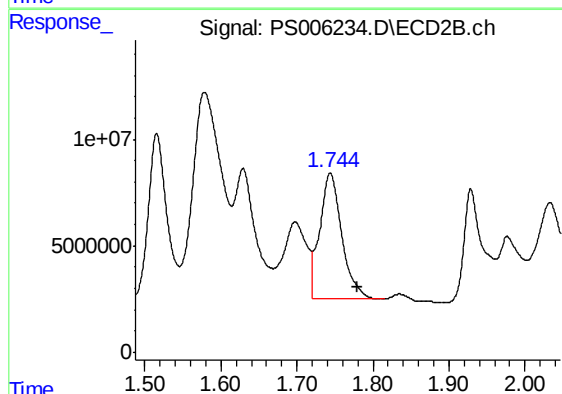


#1 Dalapon

R.T.: 1.744 min
Delta R.T.: -0.035 min
Response: 119497850
Conc: 190.44 ng/ml

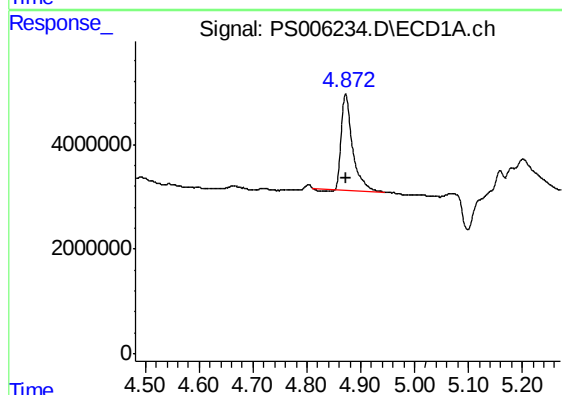


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.872 min
Delta R.T.: 0.000 min
Response: 26730623
Conc: 24.79 ng/ml

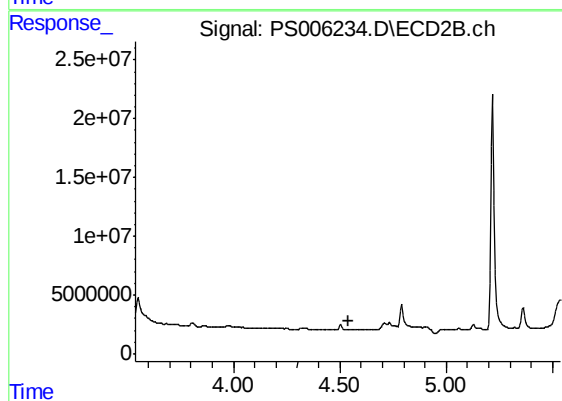

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T. : 4.538 min
Response: 0
Conc: N.D.

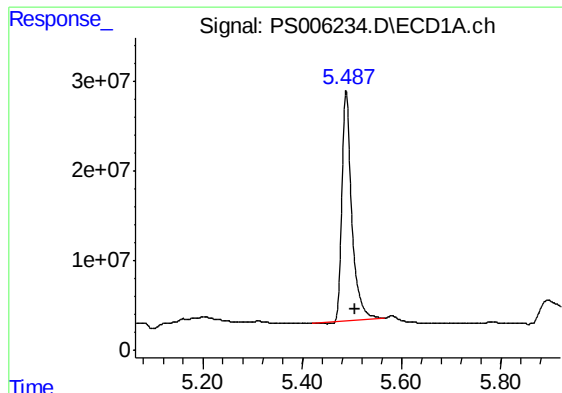

#4 2,4-DCAA


R.T.: 5.488 min
Delta R.T.: -0.017 min
Response: 354580981
Conc: 410.77 ng/ml

Instrument :
ECD_S
ClientSampleId :
T8-D-(0-2)

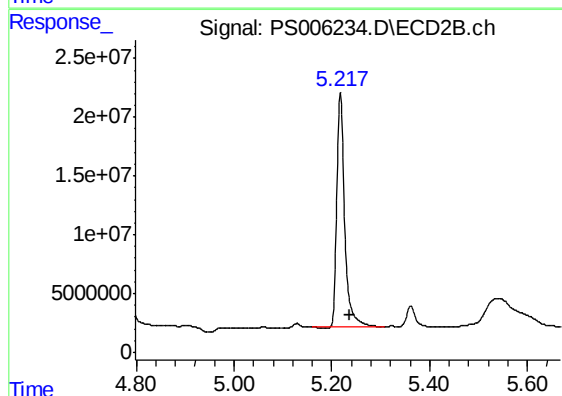


#4 2,4-DCAA

R.T.: 5.218 min
Delta R.T.: -0.018 min
Response: 220544054
Conc: 448.40 ng/ml

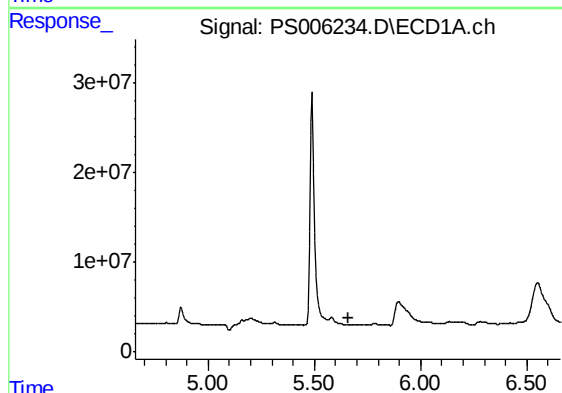


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.658 min
Response: 0
Conc: N.D.

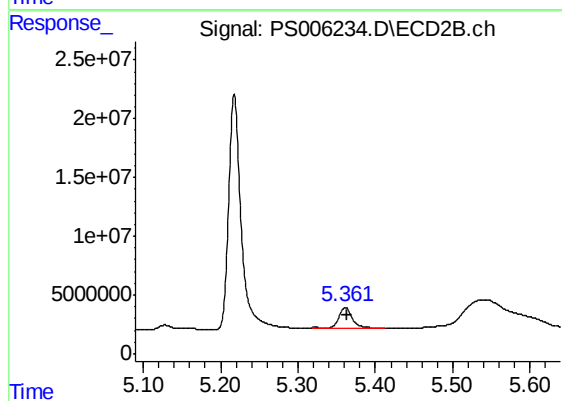

#5 DICAMBA


R.T.: 5.361 min
Delta R.T.: -0.003 min
Response: 21896401
Conc: 11.87 ng/ml

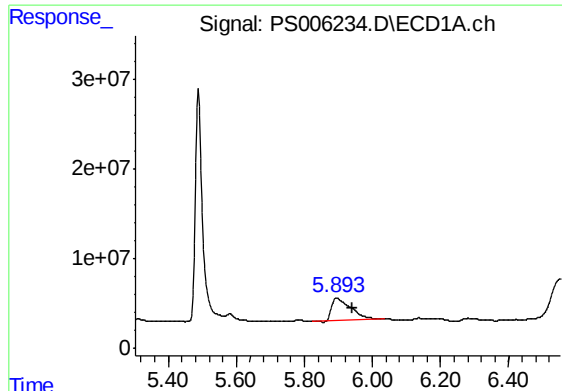

#7 MCPA


R.T.: 5.895 min
Delta R.T.: -0.047 min
Response: 95482130
Conc: 30.24 ug/ml

Instrument :
ECD_S
ClientSampleId :
T8-D-(0-2)

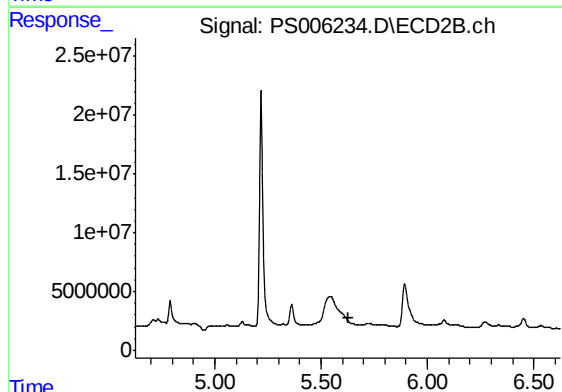


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.626 min
Response: 0
Conc: N.D.

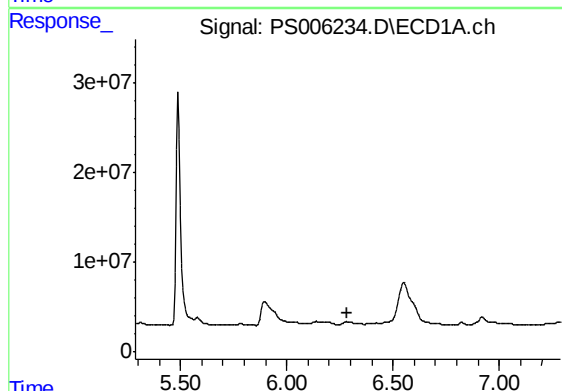


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.288 min
Response: 0
Conc: N.D.

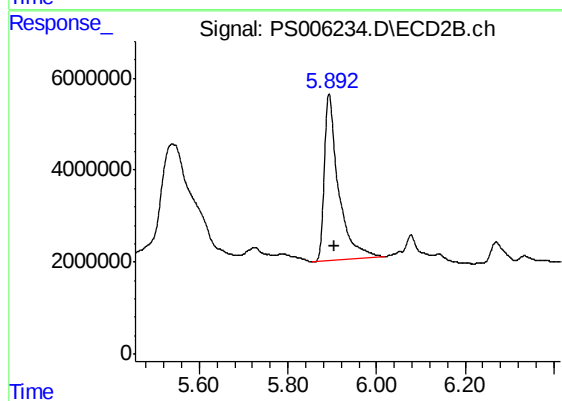

#8 DICHLORPROP


R.T.: 5.893 min
Delta R.T.: -0.012 min
Response: 79752588
Conc: 179.38 ng/ml

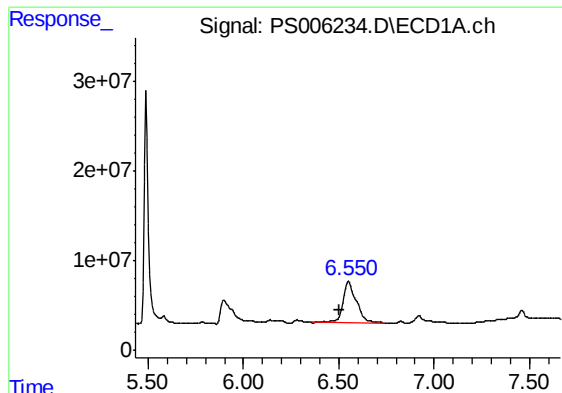

#9 2,4-D


R.T.: 6.550 min
Delta R.T.: 0.047 min
Response: 223389752
Conc: 274.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
T8-D-(0-2)

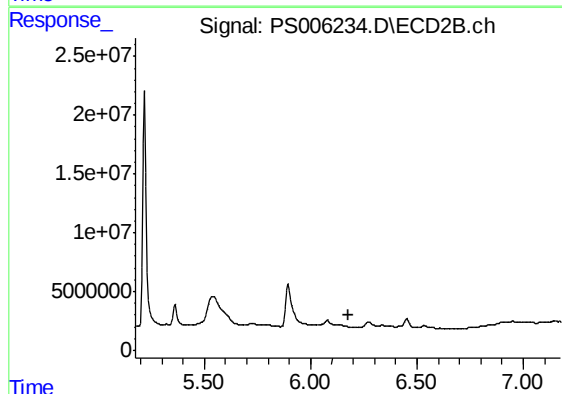


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.176 min
Response: 0
Conc: N.D.

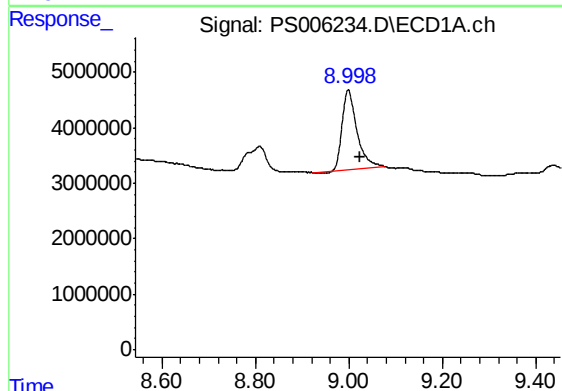

#15 Picloram

R.T.: 8.999 min
Delta R.T.: -0.025 min
Response: 30762723
Conc: 4.13 ng/ml

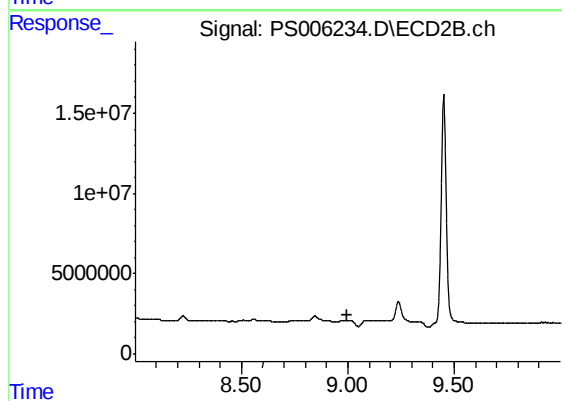

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.000 min
Response: 0
Conc: N.D.