

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082019\
 Data File : PS006237.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2019 13:40
 Operator : SM\AJ
 Sample : K4385-39
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 T8-E1-E4-(0-2)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 16:28:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.503	5.232	355.5E6	225.4E6	411.835	458.316
Target Compounds							
1) T	Dalapon	2.043	1.759	70164563	117.9E6	64.393	187.923 #
2) T	3,5-DICHL...	4.888	0.000	21027036	0	19.503	N.D. #
5) T	DICAMBA	0.000	5.376	0	18799635	N.D.	10.192
7) T	MCPA	5.916	0.000	73697499	0	23.343	N.D. #
8) T	DICHLORPROP	0.000	5.910	0	59557100	N.D.	133.955
9) T	2,4-D	6.564	0.000	193.0E6	0	236.893	N.D. #
15) T	Picloram	9.073	9.017	58441462	30586838	7.854	6.781
16) T	DCPA	0.000	9.017	0	30586838	N.D.	8.771



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082019\
Data File : PS006237.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2019 13:40
Operator : SM\AJ
Sample : K4385-39
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
T8-E1-E4-(0-2)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 16:28:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

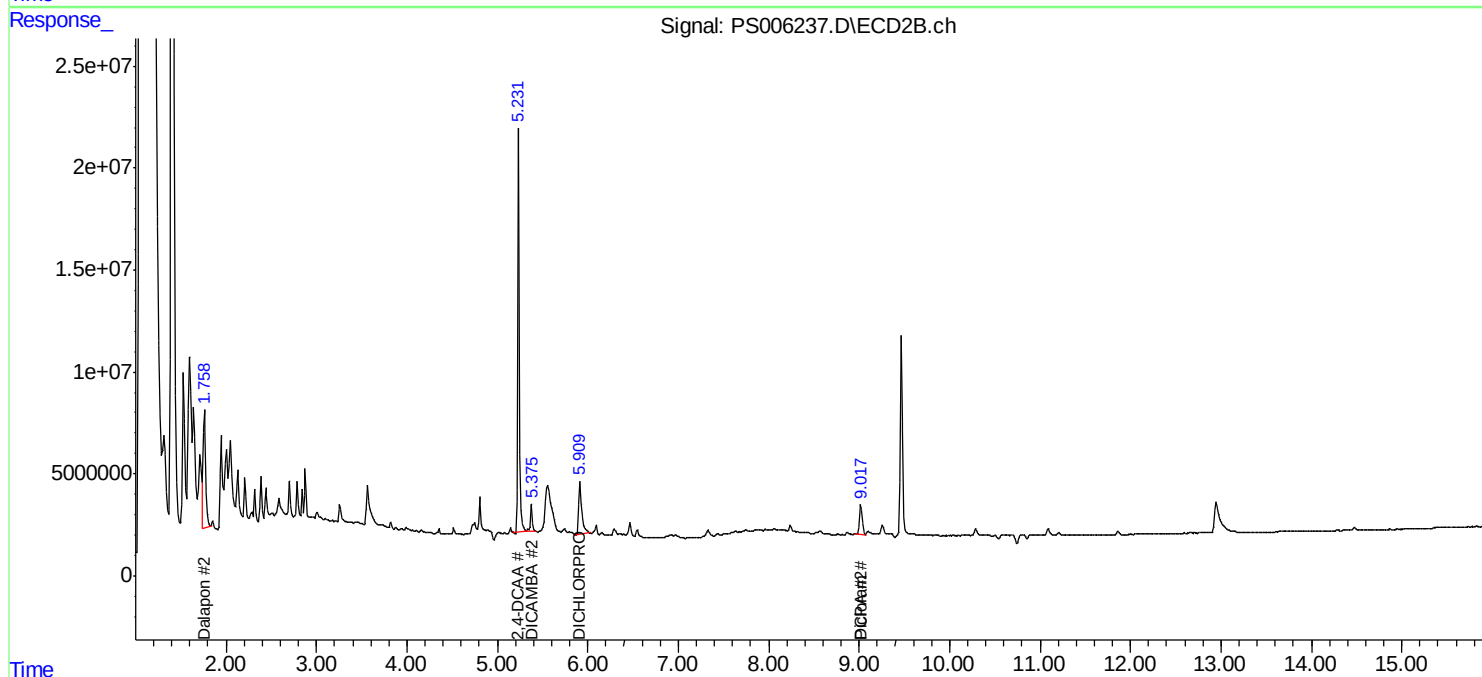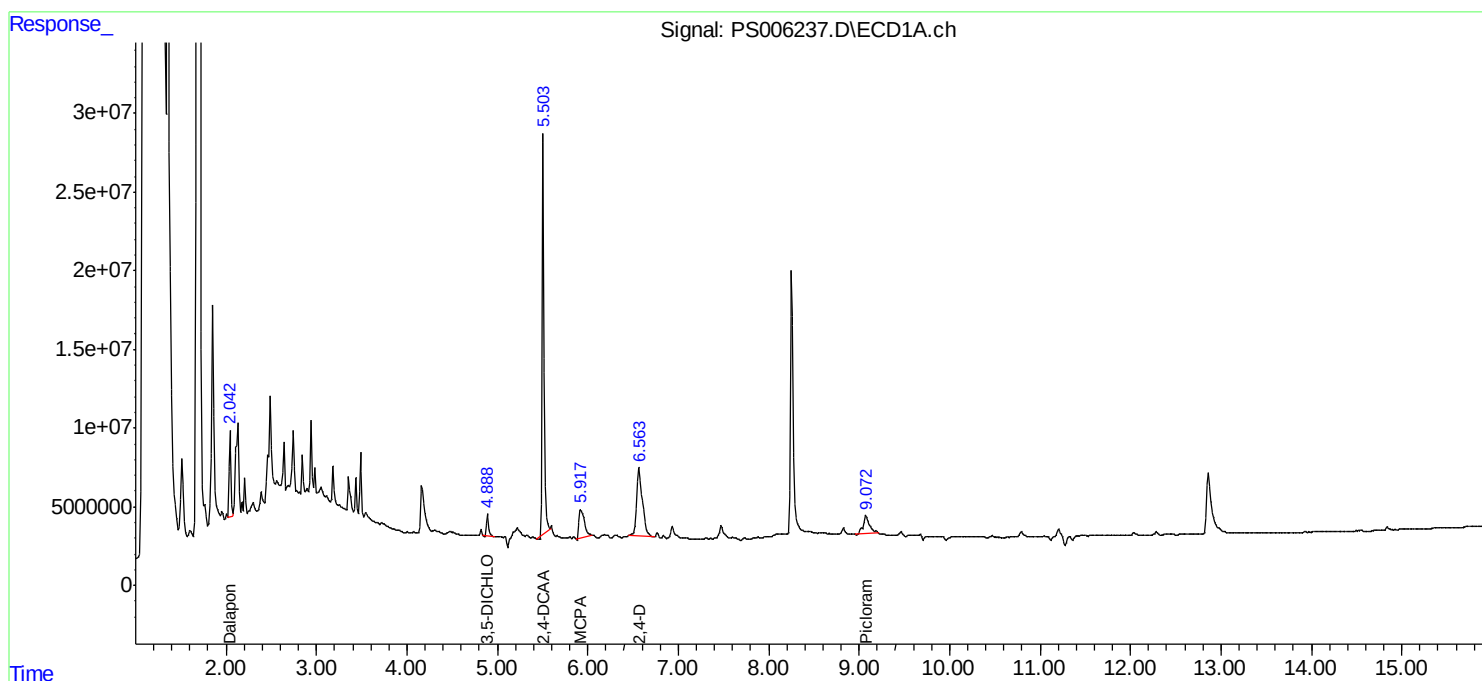


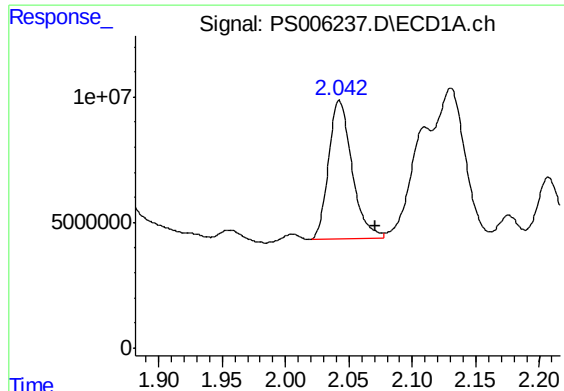

#1 Dalapon


R.T.: 2.043 min
Delta R.T.: -0.028 min
Response: 70164563
Conc: 64.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
T8-E1-E4-(0-2)

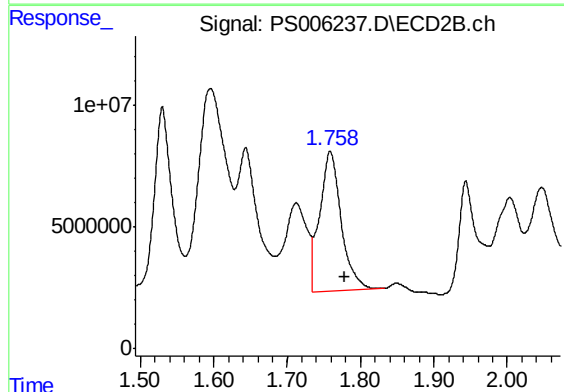


#1 Dalapon

R.T.: 1.759 min
Delta R.T.: -0.020 min
Response: 117920278
Conc: 187.92 ng/ml

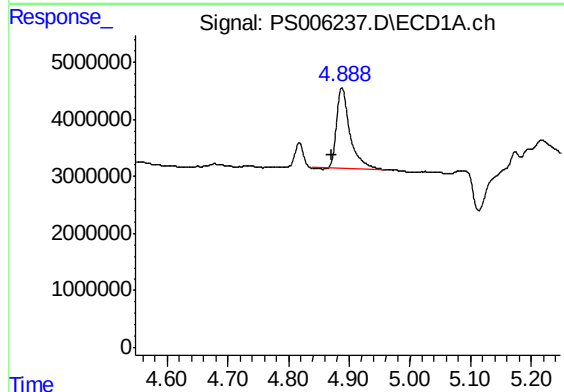


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.888 min
Delta R.T.: 0.016 min
Response: 21027036
Conc: 19.50 ng/ml

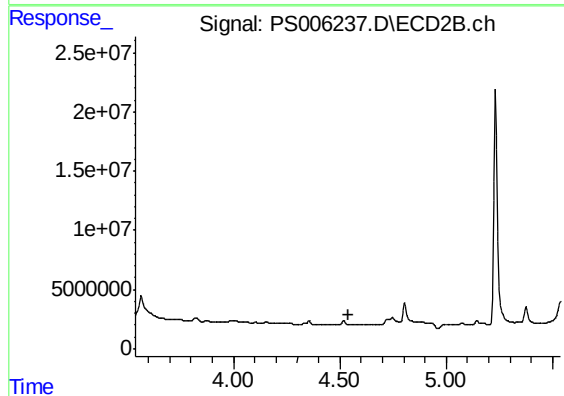

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T. : 4.538 min
Response: 0
Conc: N.D.

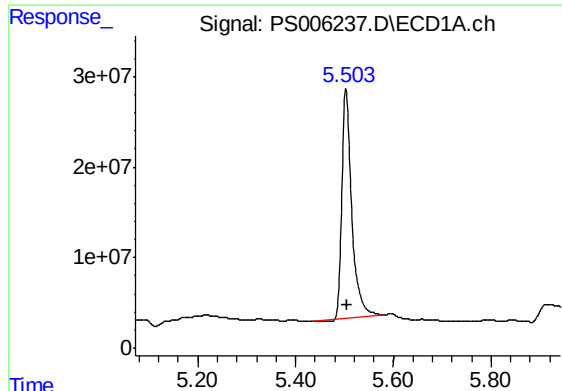

#4 2,4-DCAA


R.T.: 5.503 min
Delta R.T.: -0.002 min
Response: 355495964
Conc: 411.83 ng/ml

Instrument :
ECD_S
ClientSampleId :
T8-E1-E4-(0-2)

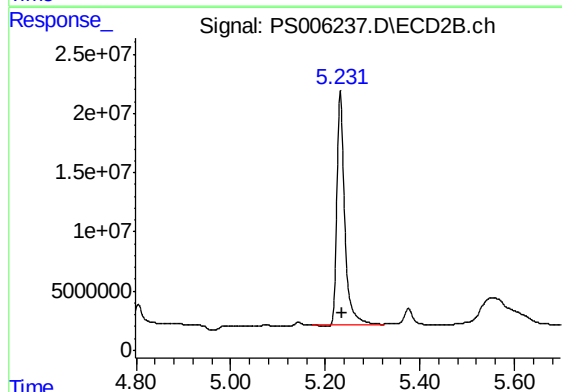


#4 2,4-DCAA

R.T.: 5.232 min
Delta R.T.: -0.004 min
Response: 225423535
Conc: 458.32 ng/ml

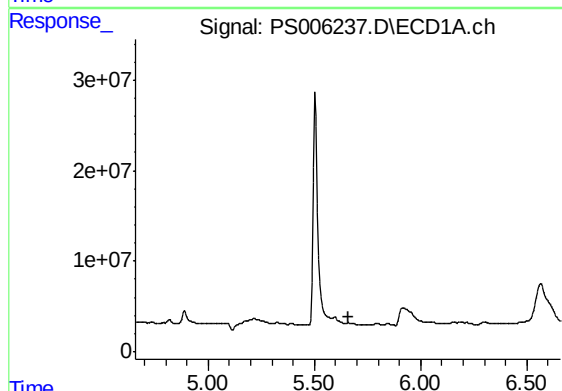


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.658 min
Response: 0
Conc: N.D.

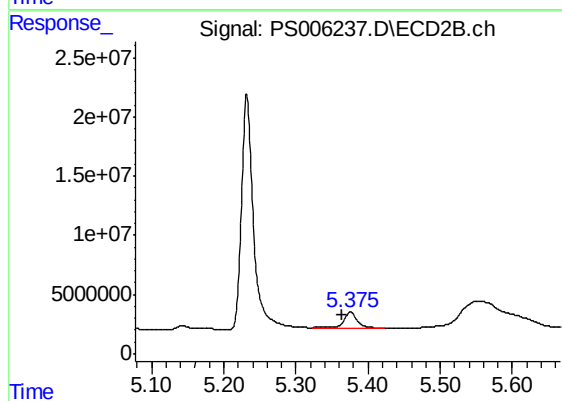

#5 DICAMBA


R.T.: 5.376 min
Delta R.T.: 0.012 min
Response: 18799635
Conc: 10.19 ng/ml

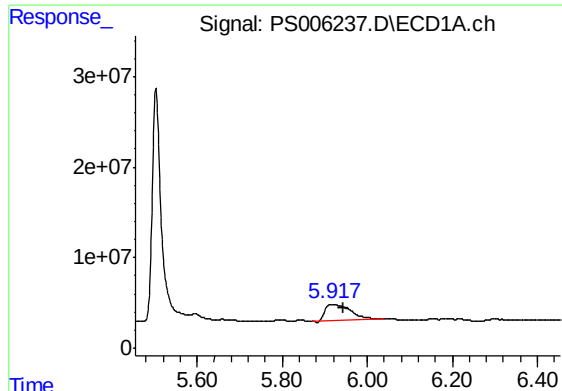

#7 MCPA


R.T.: 5.916 min
Delta R.T.: -0.026 min
Response: 73697499
Conc: 23.34 ug/ml

Instrument :
ECD_S
ClientSampleId :
T8-E1-E4-(0-2)

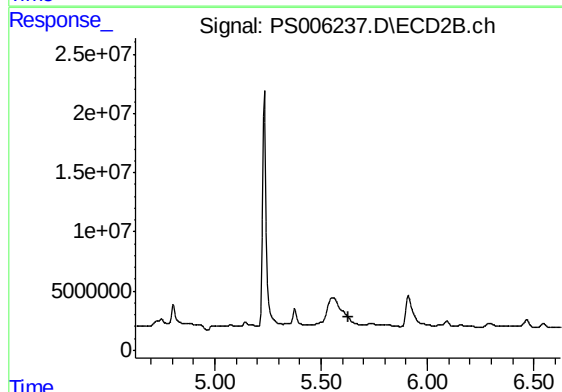


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.626 min
Response: 0
Conc: N.D.

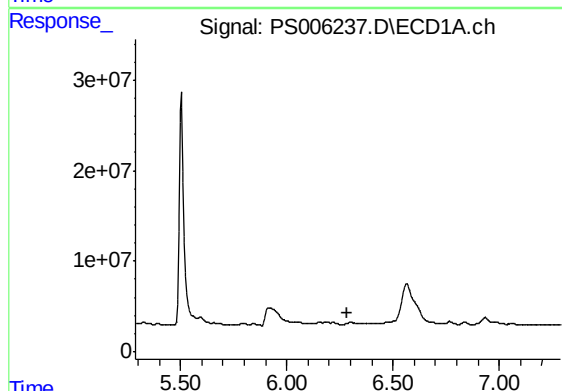


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.288 min
Response: 0
Conc: N.D.

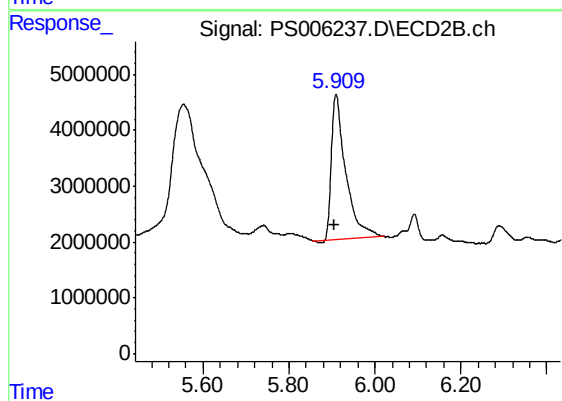

#8 DICHLORPROP


R.T.: 5.910 min
Delta R.T.: 0.005 min
Response: 59557100
Conc: 133.96 ng/ml

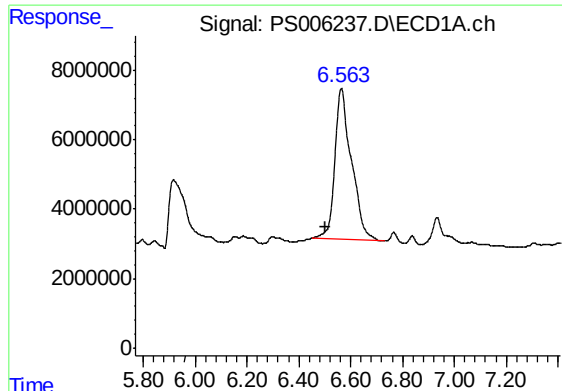

#9 2,4-D


R.T.: 6.564 min
Delta R.T.: 0.061 min
Response: 193016709
Conc: 236.89 ng/ml

Instrument :
ECD_S
ClientSampleId :
T8-E1-E4-(0-2)

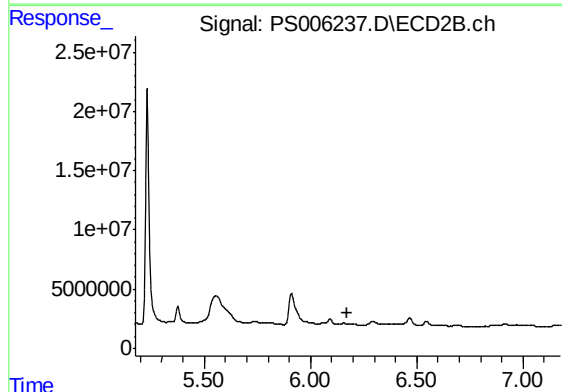


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.176 min
Response: 0
Conc: N.D.

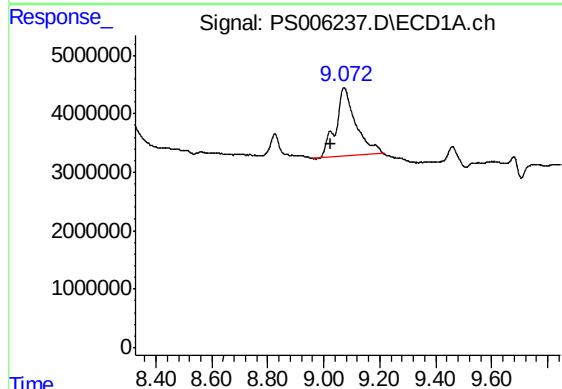


#15 Picloram

R.T.: 9.073 min
Delta R.T.: 0.049 min
Response: 58441462
Conc: 7.85 ng/ml

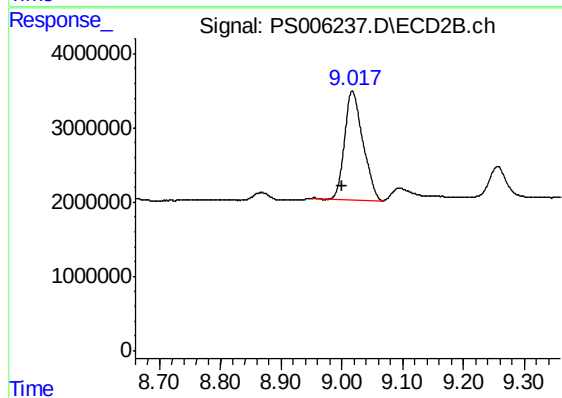

#15 Picloram


R.T.: 9.017 min
Delta R.T.: 0.017 min
Response: 30586838
Conc: 6.78 ng/ml

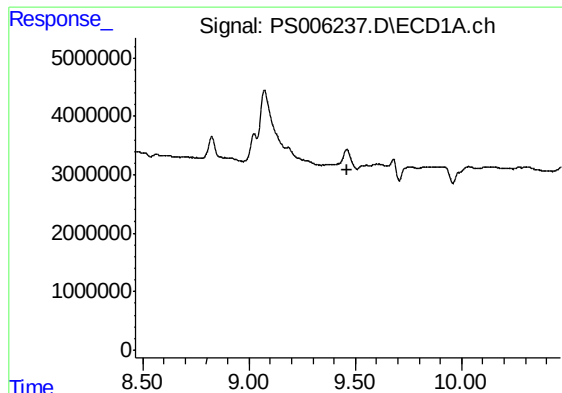

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.465 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
T8-E1-E4-(0-2)

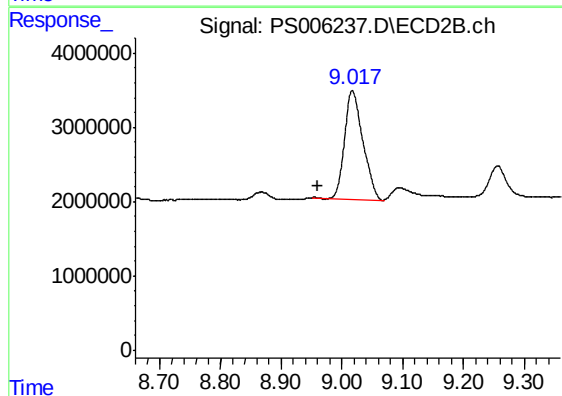

#16 DCPA

R.T.: 9.017 min
Delta R.T.: 0.058 min
Response: 30586838
Conc: 8.77 ng/ml