

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082019\
 Data File : PS006238.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2019 14:02
 Operator : SM\AJ
 Sample : K4386-28
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 T8-F-(0-2)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 16:28:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.490	5.219	383.3E6	236.8E6	444.027	481.346
Target Compounds							
1) T	Dalapon	2.119	1.747	-963254	118.5E6	N.D.	188.810
2) T	3,5-DICHL...	4.871	0.000	82099867	0	76.150	N.D. #
5) T	DICAMBA	0.000	5.362	0	59847887	N.D.	32.447
7) T	MCPA	5.893	0.000	144.1E6	0	45.647	N.D. #
8) T	DICHLORPROP	0.000	5.894	0	107.3E6	N.D.	241.243
9) T	2,4-D	6.550	0.000	258.0E6	0	316.620	N.D. #
15) T	Picloram	9.001	0.000	35024043	0	4.707	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082019\
Data File : PS006238.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2019 14:02
Operator : SM\AJ
Sample : K4386-28
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
T8-F-(0-2)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 16:28:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

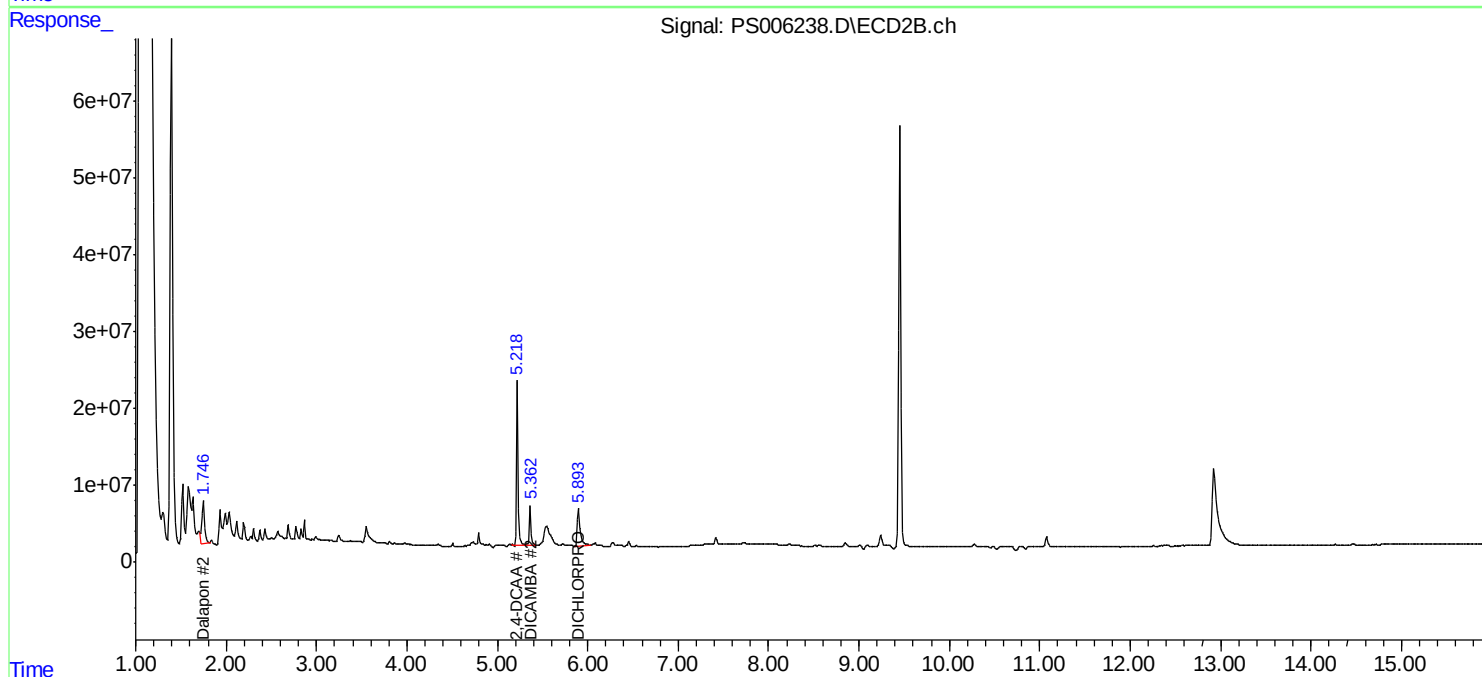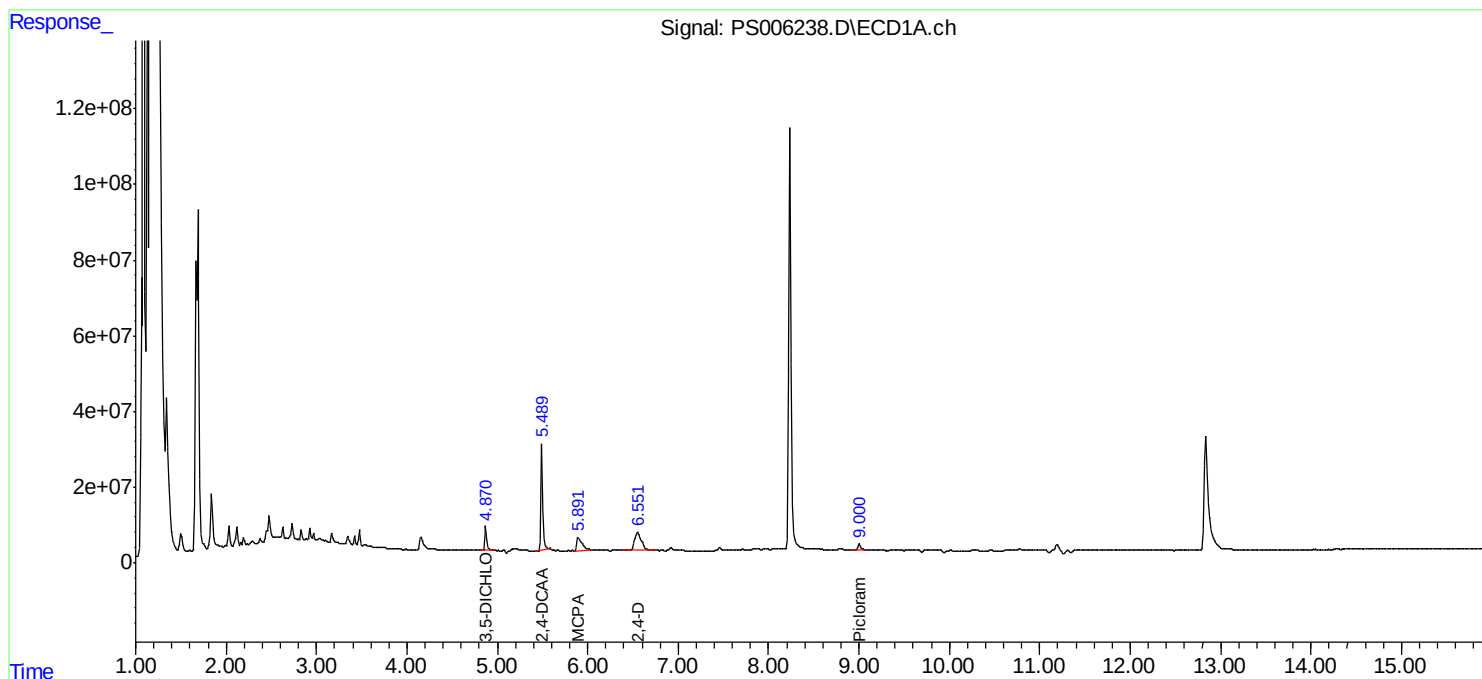


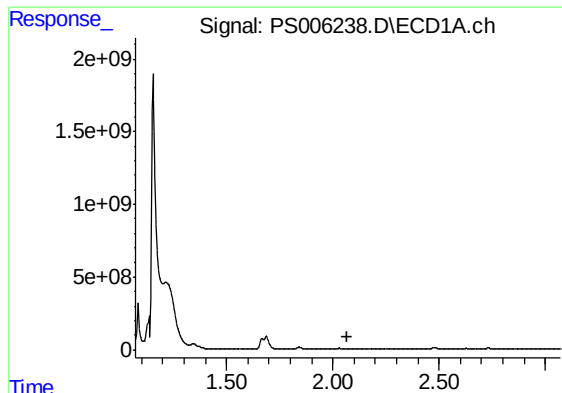

#1 Dalapon


R.T.: 2.119 min
Delta R.T.: 0.048 min
Response: -963254
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
T8-F-(0-2)

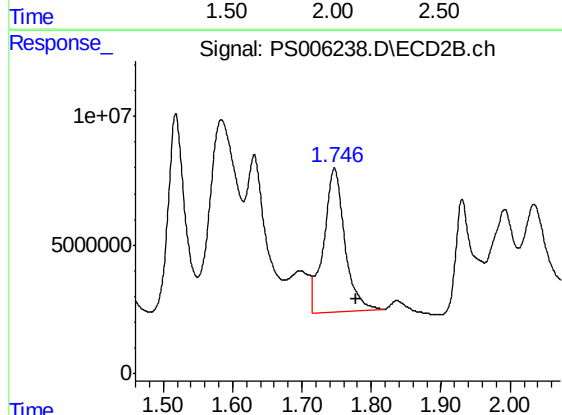


#1 Dalapon

R.T.: 1.747 min
Delta R.T.: -0.032 min
Response: 118477006
Conc: 188.81 ng/ml

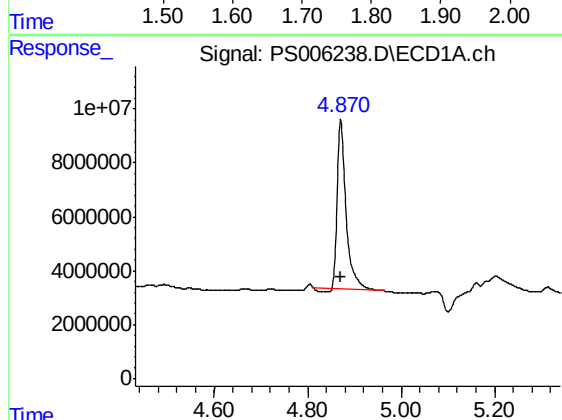


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.871 min
Delta R.T.: 0.000 min
Response: 82099867
Conc: 76.15 ng/ml

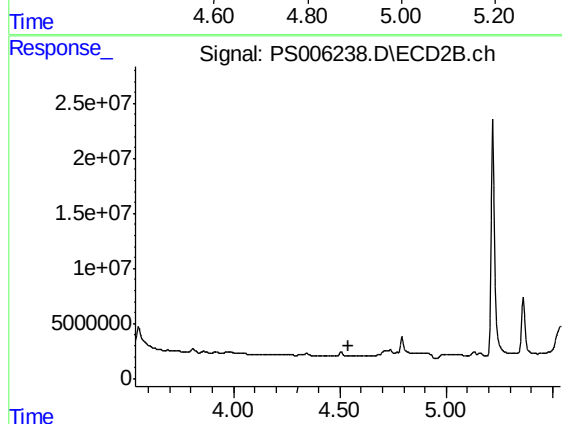

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T. : 4.538 min
Response: 0
Conc: N.D.

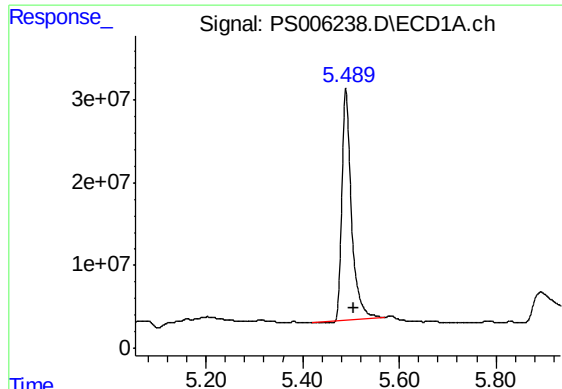

#4 2,4-DCAA


R.T.: 5.490 min
Delta R.T.: -0.016 min
Response: 383284690
Conc: 444.03 ng/ml

Instrument :
ECD_S
ClientSampleId :
T8-F-(0-2)

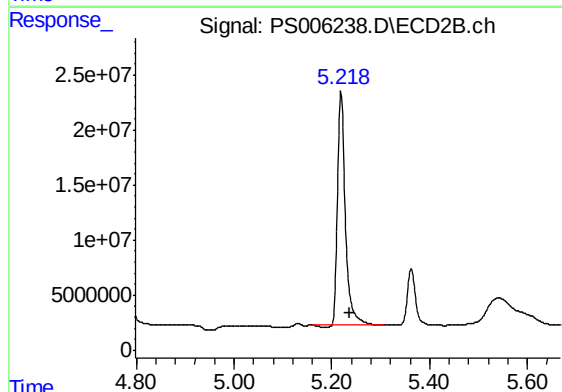


#4 2,4-DCAA

R.T.: 5.219 min
Delta R.T.: -0.017 min
Response: 236751167
Conc: 481.35 ng/ml

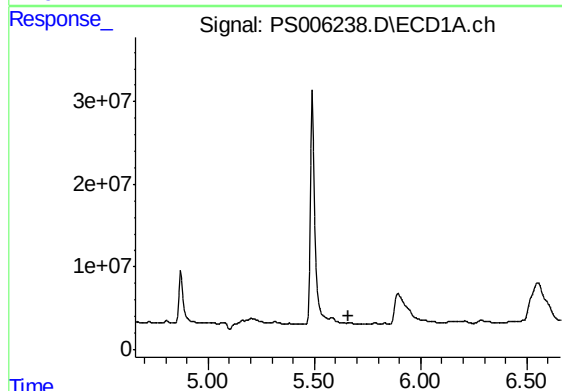


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.658 min
Response: 0
Conc: N.D.

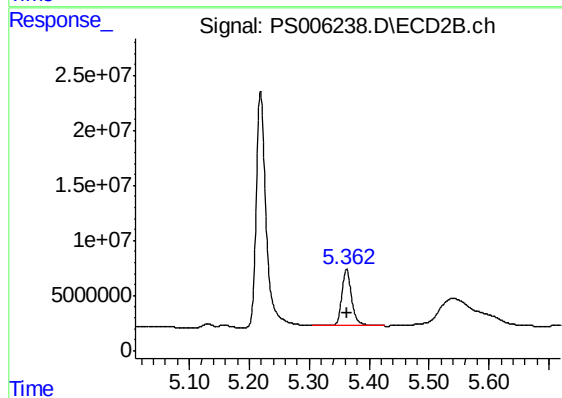

#5 DICAMBA


R.T.: 5.362 min
Delta R.T.: -0.002 min
Response: 59847887
Conc: 32.45 ng/ml

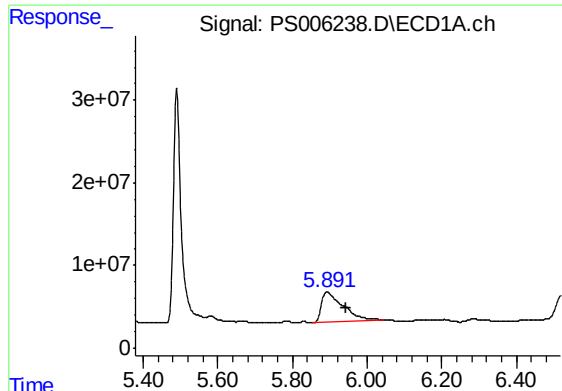

#7 MCPA


R.T.: 5.893 min
Delta R.T.: -0.050 min
Response: 144111473
Conc: 45.65 ug/ml

Instrument :
ECD_S
ClientSampleId :
T8-F-(0-2)

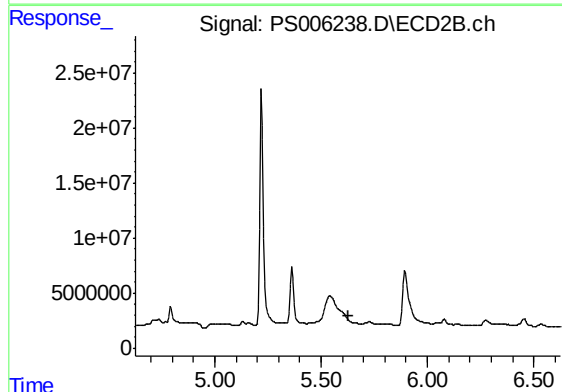


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.626 min
Response: 0
Conc: N.D.

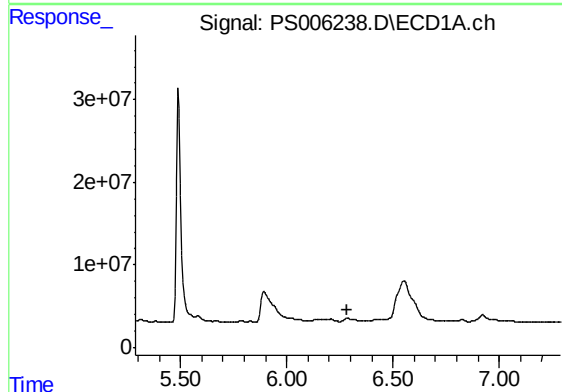


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.288 min
Response: 0
Conc: N.D.

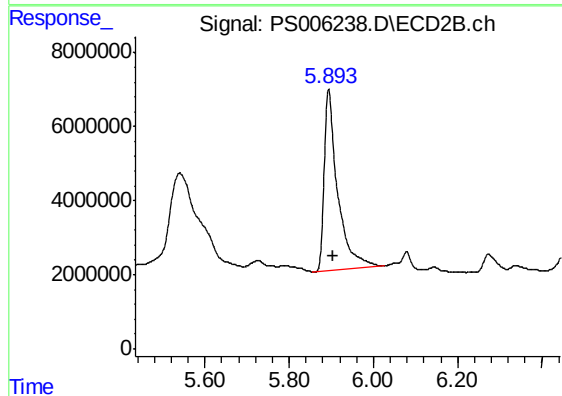

#8 DICHLORPROP


R.T.: 5.894 min
Delta R.T.: -0.011 min
Response: 107257635
Conc: 241.24 ng/ml

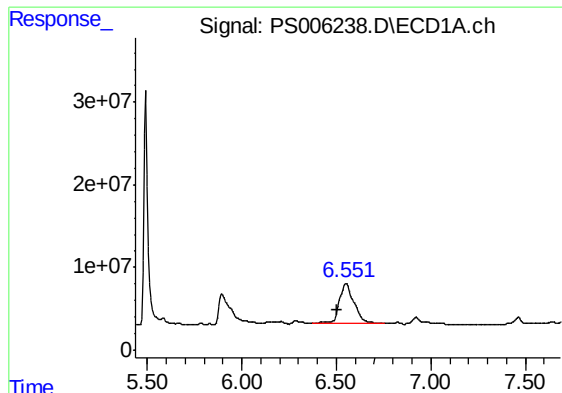

#9 2,4-D


R.T.: 6.550 min
Delta R.T.: 0.047 min
Response: 257977240
Conc: 316.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
T8-F-(0-2)

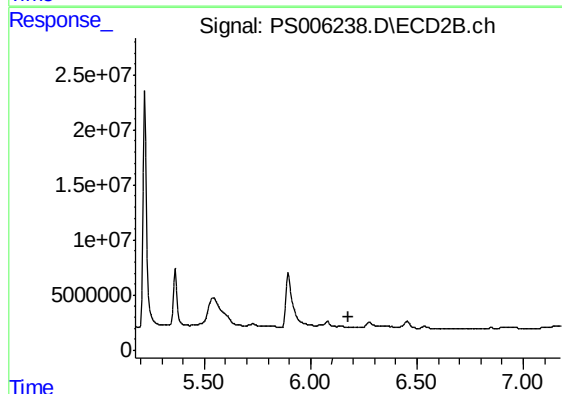


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.176 min
Response: 0
Conc: N.D.

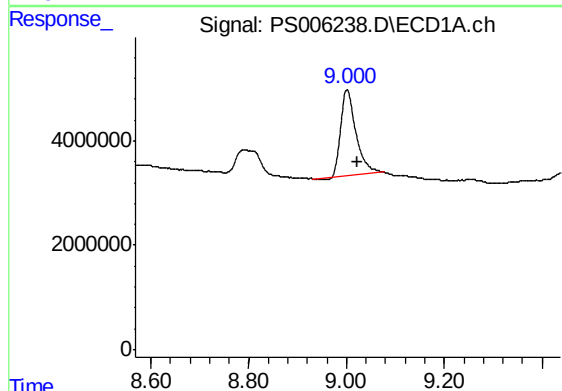

#15 Picloram

R.T.: 9.001 min
Delta R.T.: -0.023 min
Response: 35024043
Conc: 4.71 ng/ml

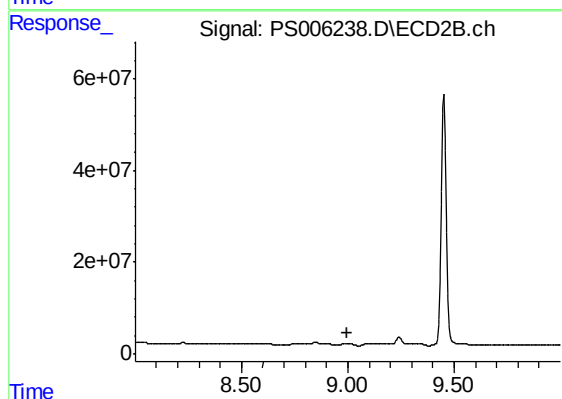

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.000 min
Response: 0
Conc: N.D.