

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082019\
 Data File : PS006239.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2019 14:24
 Operator : SM\AJ
 Sample : K4386-31
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 T6-A1-A4-(0-2)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 16:28:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.507	5.236	341.7E6	221.3E6	395.881	449.976
Target Compounds							
1) T	Dalapon	2.046	1.763	78091596	136.7E6	71.668	217.779 #
2) T	3,5-DICHL...	4.888	0.000	27989399	0	25.961	N.D. #
5) T	DICAMBA	0.000	5.380	0	31825961	N.D.	17.254
6) T	MCPD	0.000	5.380	0	31825961	N.D.	25.726
7) T	MCPA	5.901	0.000	238.2E6	0	75.465	N.D. #
8) T	DICHLORPROP	0.000	5.909	0	150.7E6	N.D.	338.922
9) T	2,4-D	6.568	0.000	236.1E6	0	289.747	N.D. #
15) T	Picloram	9.017	0.000	40472686	0	5.439	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082019\
Data File : PS006239.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2019 14:24
Operator : SM\AJ
Sample : K4386-31
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
T6-A1-A4-(0-2)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 16:28:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

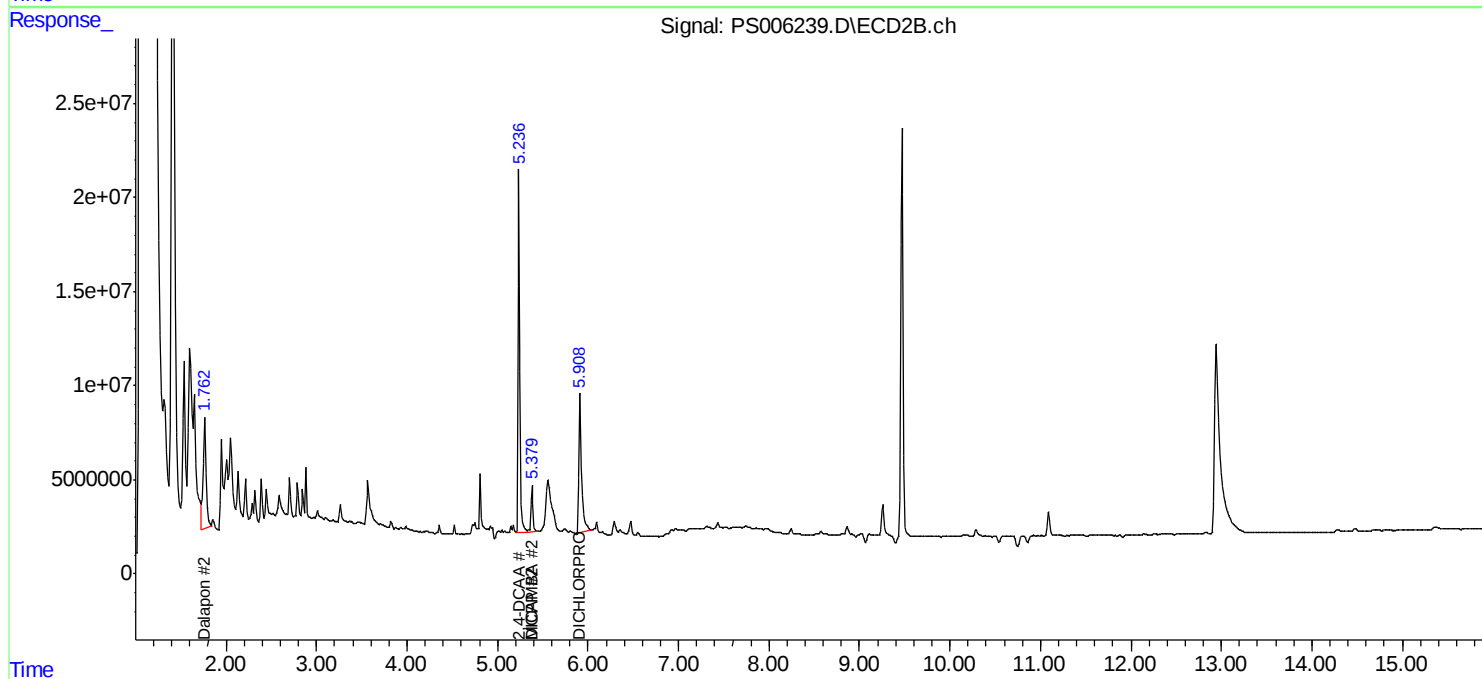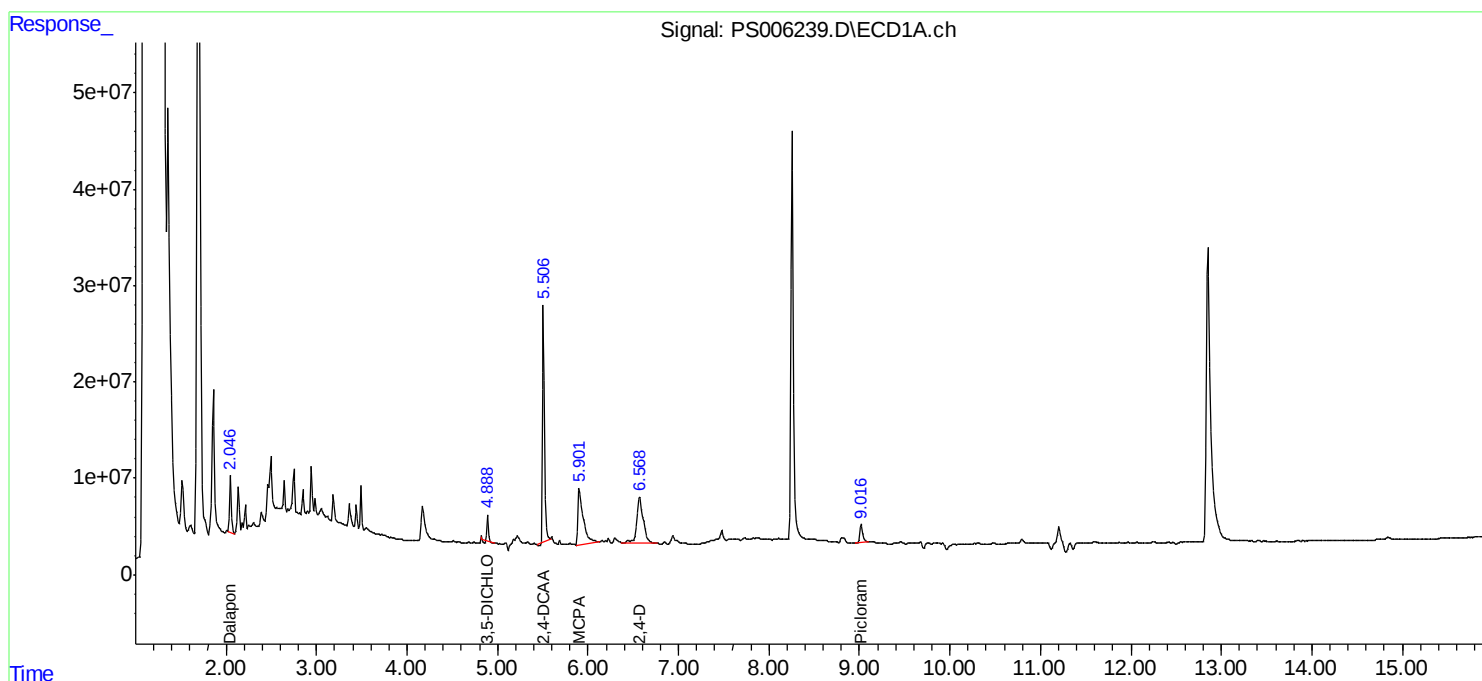


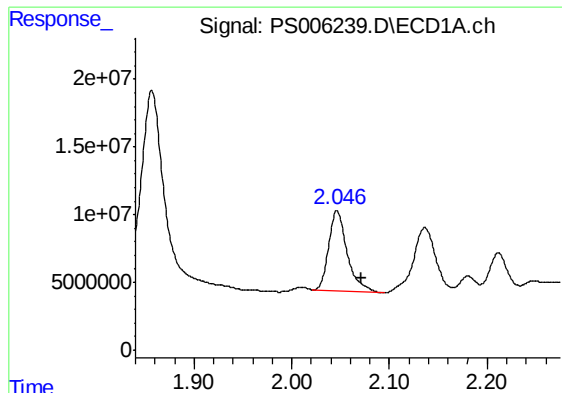

#1 Dalapon


R.T.: 2.046 min
Delta R.T.: -0.025 min
Response: 78091596
Conc: 71.67 ng/ml

Instrument :
ECD_S
ClientSampleId :
T6-A1-A4-(0-2)

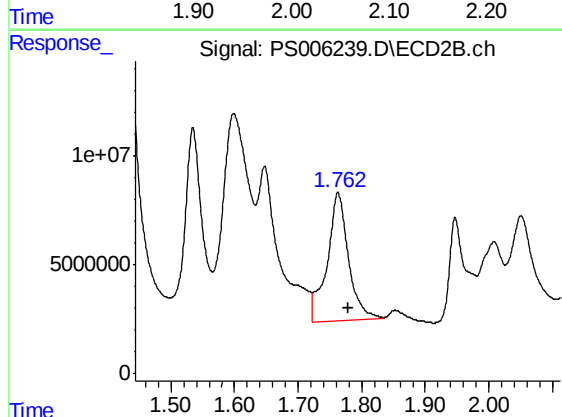


#1 Dalapon

R.T.: 1.763 min
Delta R.T.: -0.016 min
Response: 136654815
Conc: 217.78 ng/ml

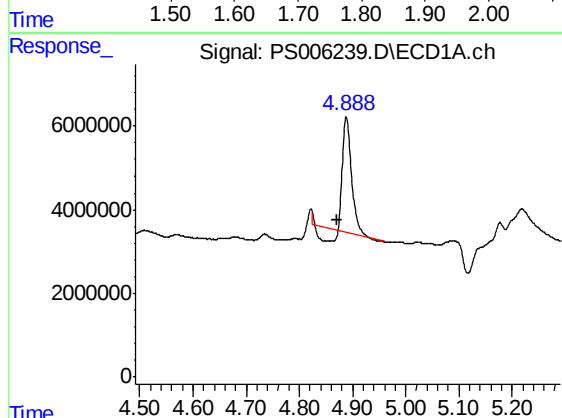


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.888 min
Delta R.T.: 0.017 min
Response: 27989399
Conc: 25.96 ng/ml

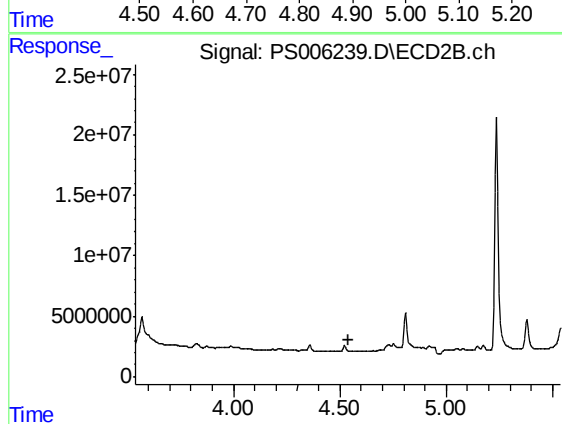

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T. : 4.538 min
Response: 0
Conc: N.D.

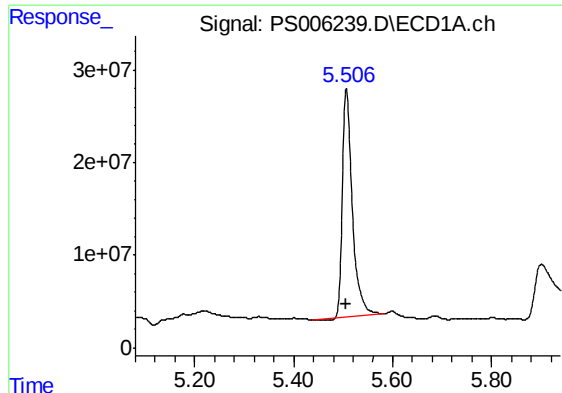

#4 2,4-DCAA


R.T.: 5.507 min
Delta R.T.: 0.002 min
Response: 341724715
Conc: 395.88 ng/ml

Instrument :
ECD_S
ClientSampleId :
T6-A1-A4-(0-2)

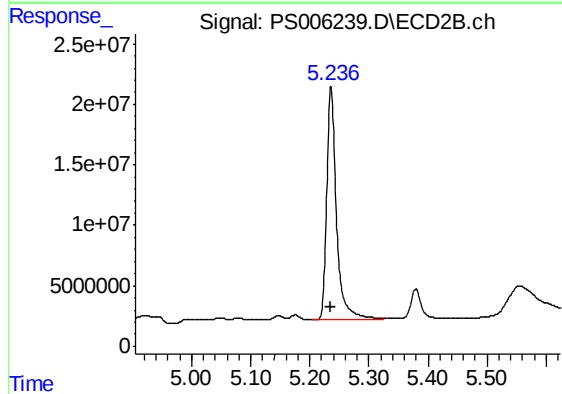


#4 2,4-DCAA

R.T.: 5.236 min
Delta R.T.: 0.000 min
Response: 221321522
Conc: 449.98 ng/ml

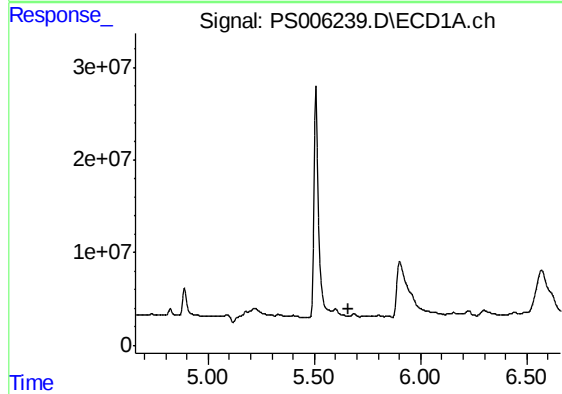


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.658 min
Response: 0
Conc: N.D.

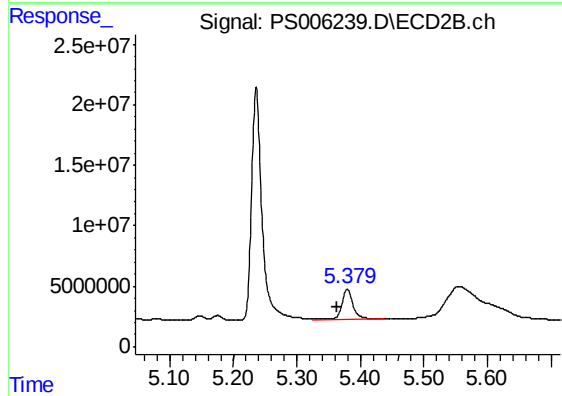

#5 DICAMBA


R.T.: 5.380 min
Delta R.T.: 0.015 min
Response: 31825961
Conc: 17.25 ng/ml

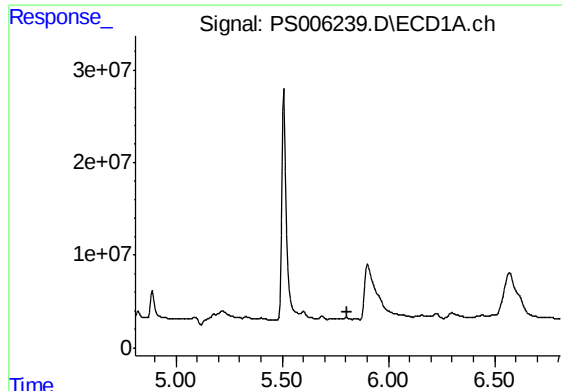

#6 MCPP


R.T.: 0.000 min
Exp R.T. : 5.810 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
T6-A1-A4-(0-2)

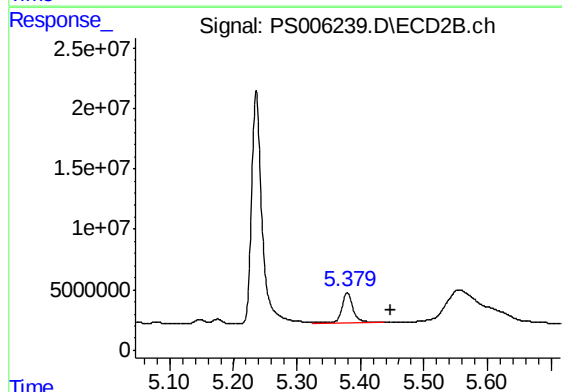


#6 MCPP

R.T.: 5.380 min
Delta R.T.: -0.068 min
Response: 31825961
Conc: 25.73 ug/ml

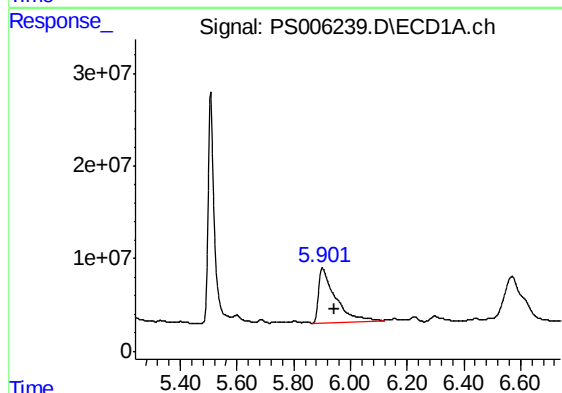


#7 MCPA

R.T.: 5.901 min
Delta R.T.: -0.041 min
Response: 238248293
Conc: 75.46 ug/ml

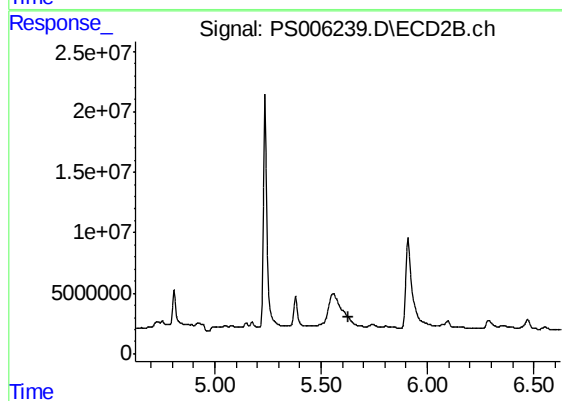

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 5.626 min
Response: 0
Conc: N.D.

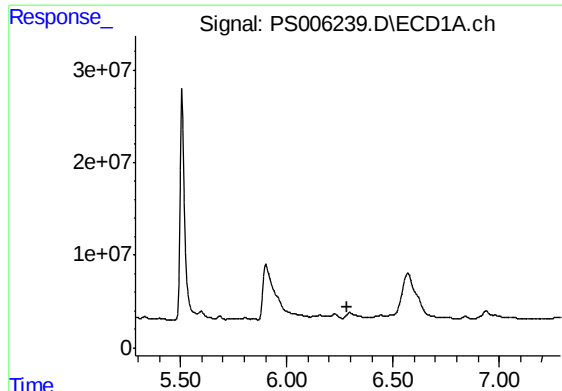

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 6.288 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
T6-A1-A4-(0-2)

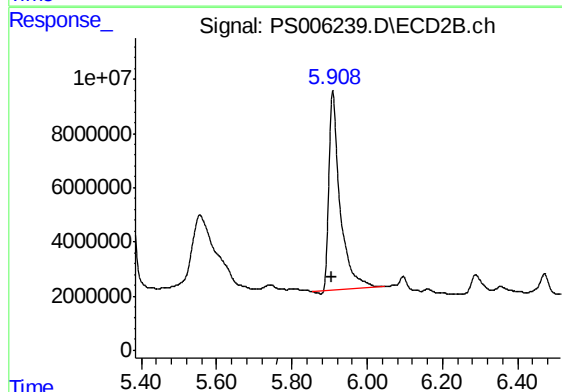


#8 DICHLORPROP

R.T.: 5.909 min
Delta R.T.: 0.004 min
Response: 150686280
Conc: 338.92 ng/ml

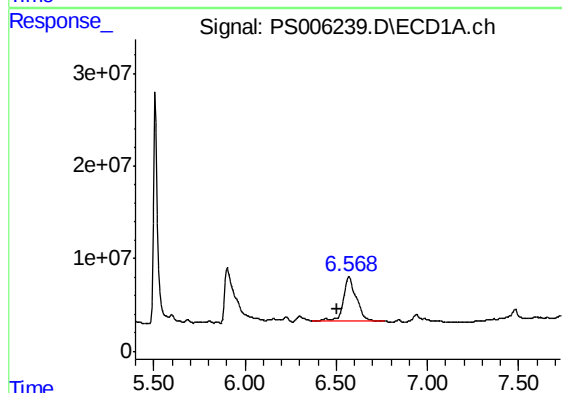


#9 2,4-D

R.T.: 6.568 min
Delta R.T.: 0.065 min
Response: 236081188
Conc: 289.75 ng/ml

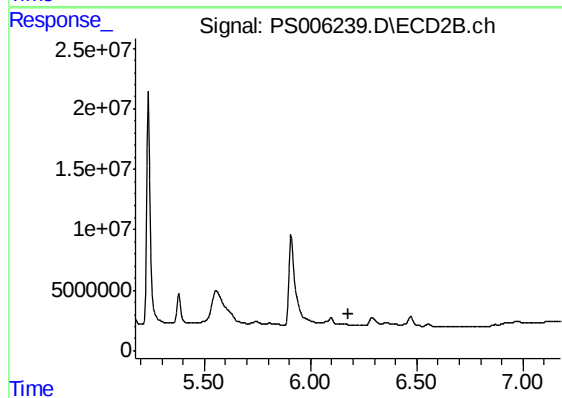

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 6.176 min
Response: 0
Conc: N.D.

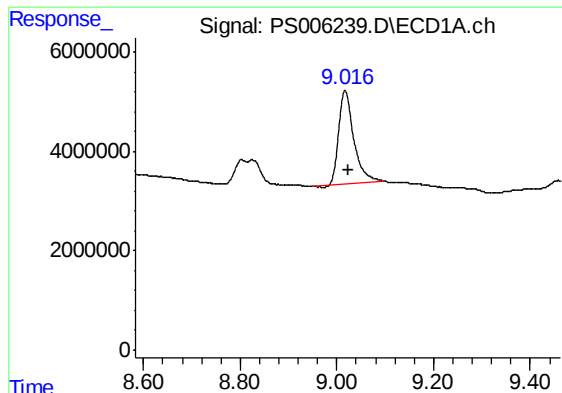

#15 Picloram

R.T.: 9.017 min
Delta R.T.: -0.007 min
Response: 40472686
Conc: 5.44 ng/ml

Instrument :
ECD_S
ClientSampleId :
T6-A1-A4-(0-2)

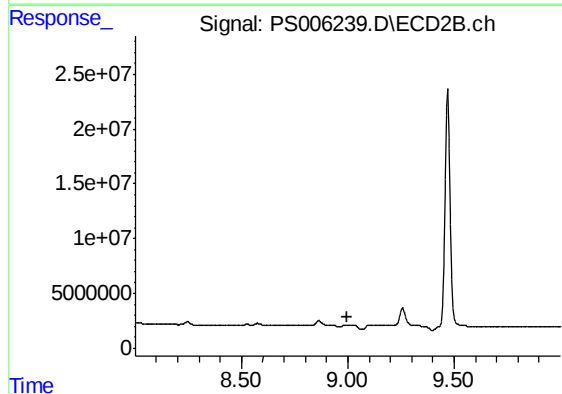

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.000 min
Response: 0
Conc: N.D.