

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082019\
 Data File : PS006240.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2019 14:46
 Operator : SM\AJ
 Sample : K4386-40
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 T6-B-(0-2)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 16:28:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.490	5.220	354.2E6	215.6E6	410.386	438.330
Target Compounds							
1) T	Dalapon	2.119	1.746	42073387	112.7E6	38.613	179.546 #
2) T	3,5-DICHL...	4.872	0.000	44330671	0	41.118	N.D. #
5) T	DICAMBA	0.000	5.363	0	37887812	N.D.	20.541
7) T	MCPA	5.895	0.000	177.9E6	0	56.361	N.D. #
8) T	DICHLORPROP	0.000	5.897	0	114.0E6	N.D.	256.427
9) T	2,4-D	6.552	0.000	240.1E6	0	294.683	N.D. #
15) T	Picloram	8.998	0.000	55061060	0	7.400	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082019\
Data File : PS006240.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2019 14:46
Operator : SM\AJ
Sample : K4386-40
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
T6-B-(0-2)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 16:28:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

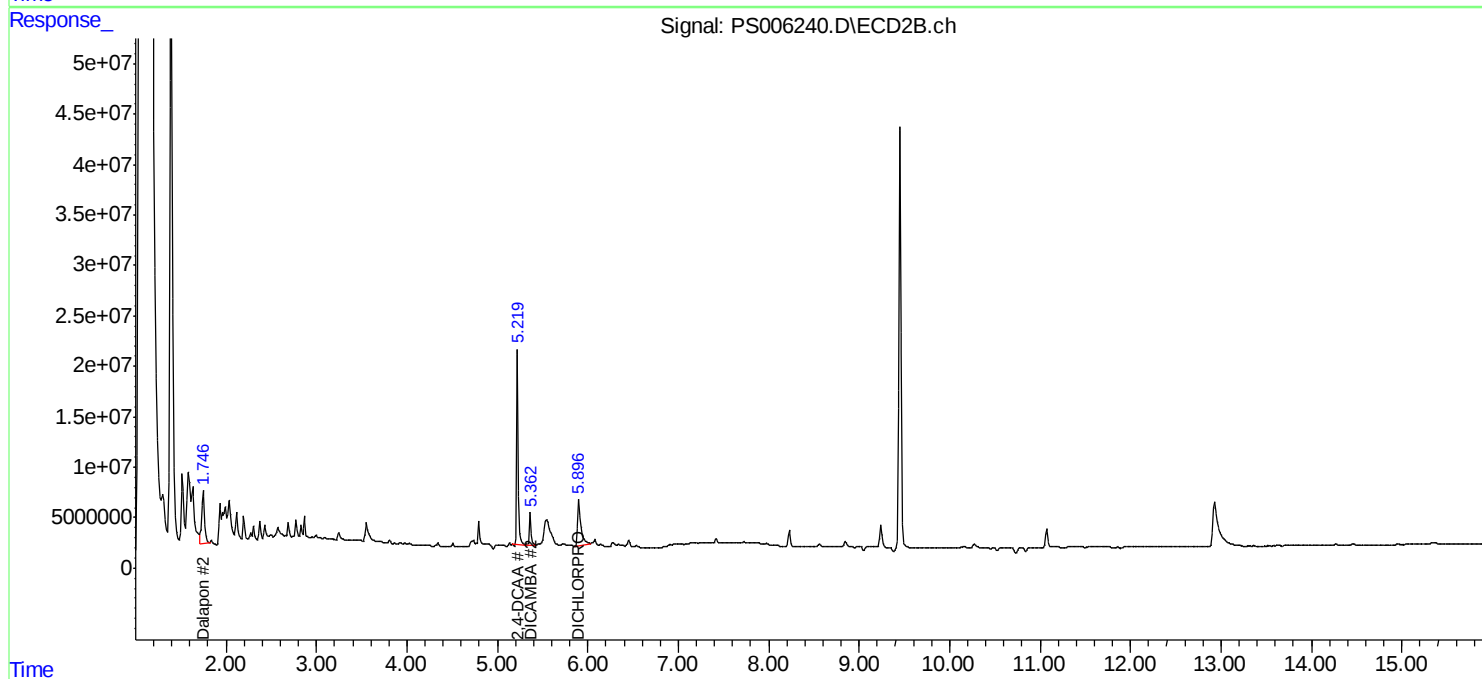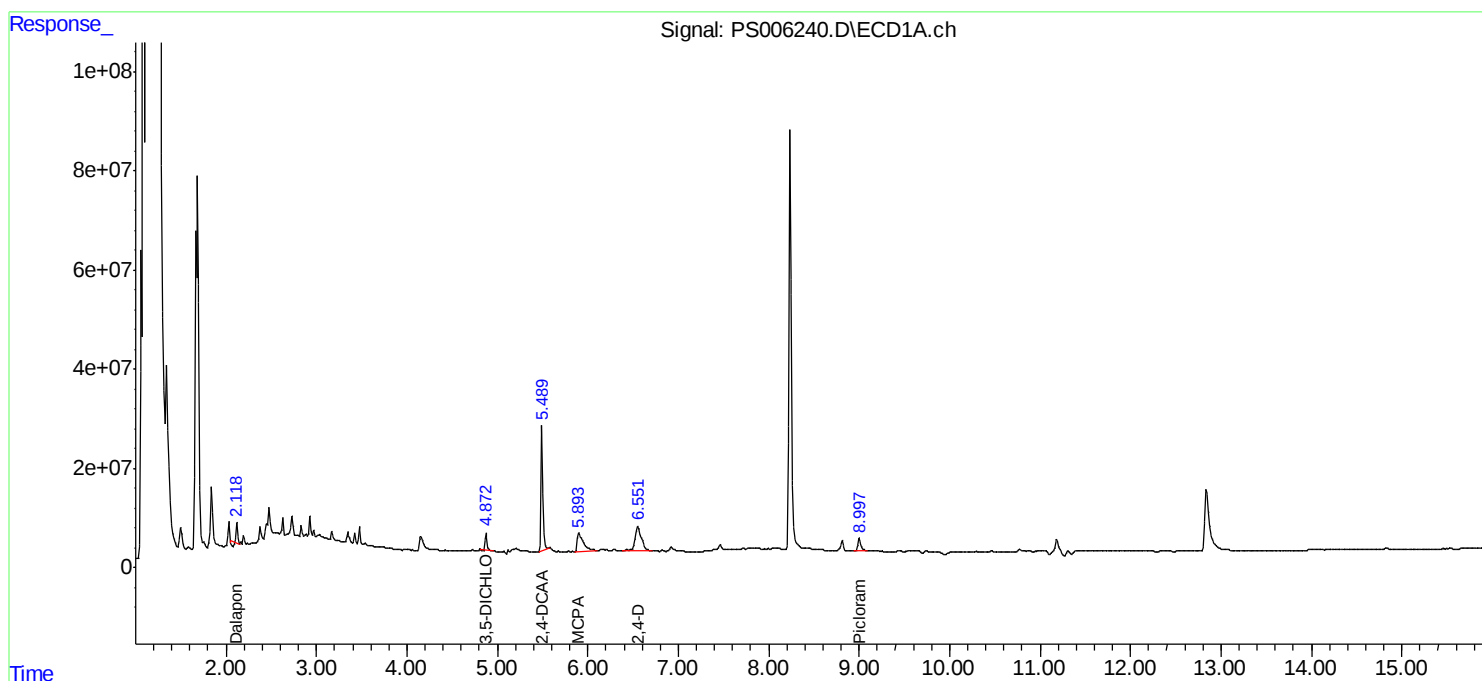


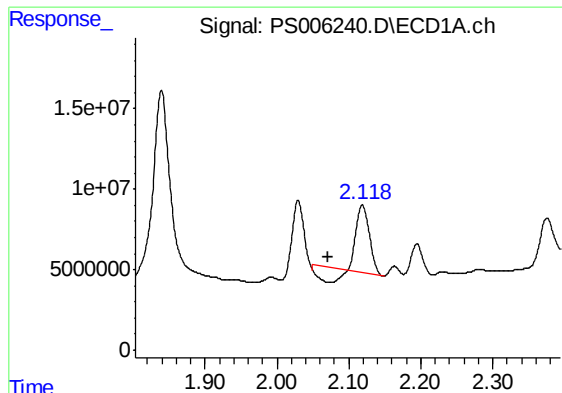

#1 Dalapon


R.T.: 2.119 min
Delta R.T.: 0.048 min
Response: 42073387
Conc: 38.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
T6-B-(0-2)

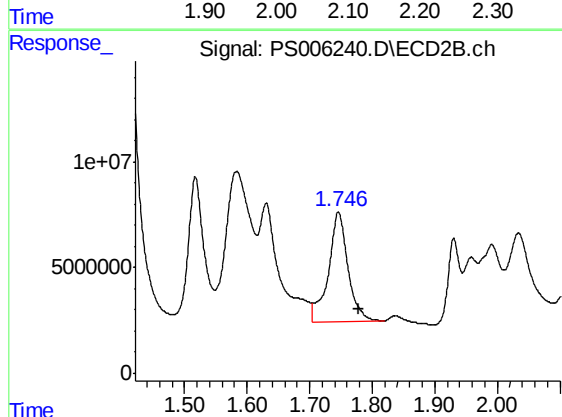


#1 Dalapon

R.T.: 1.746 min
Delta R.T.: -0.033 min
Response: 112663654
Conc: 179.55 ng/ml

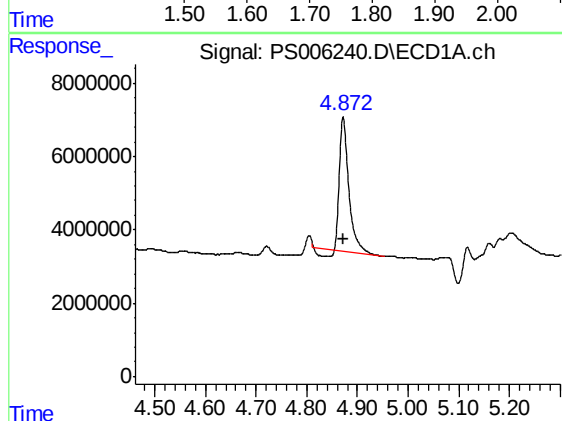


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.872 min
Delta R.T.: 0.000 min
Response: 44330671
Conc: 41.12 ng/ml

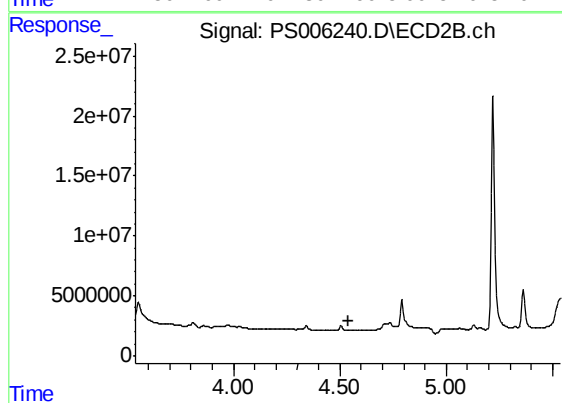

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T. : 4.538 min
Response: 0
Conc: N.D.

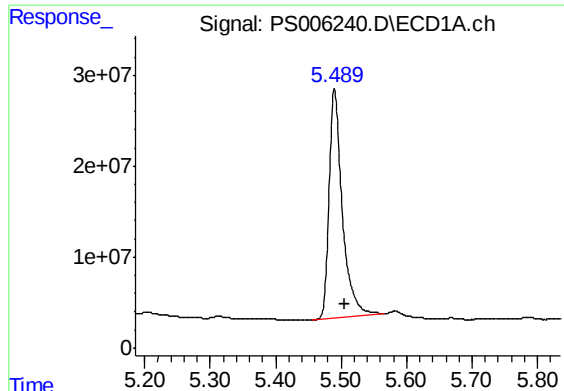

#4 2,4-DCAA


R.T.: 5.490 min
Delta R.T.: -0.015 min
Response: 354245375
Conc: 410.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
T6-B-(0-2)

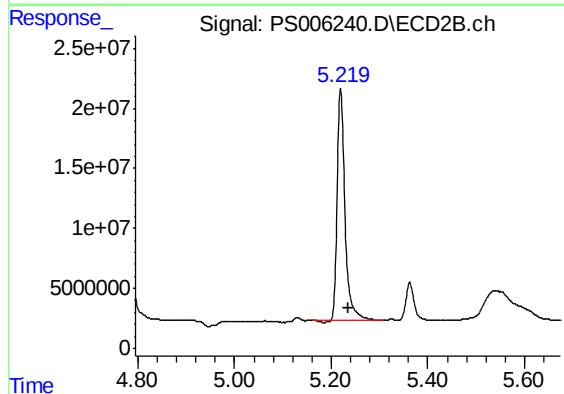


#4 2,4-DCAA

R.T.: 5.220 min
Delta R.T.: -0.016 min
Response: 215593669
Conc: 438.33 ng/ml

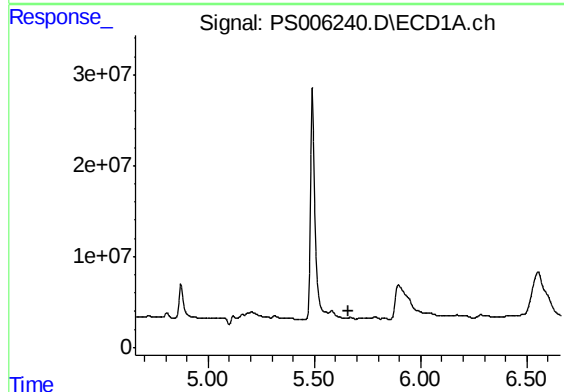


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.658 min
Response: 0
Conc: N.D.

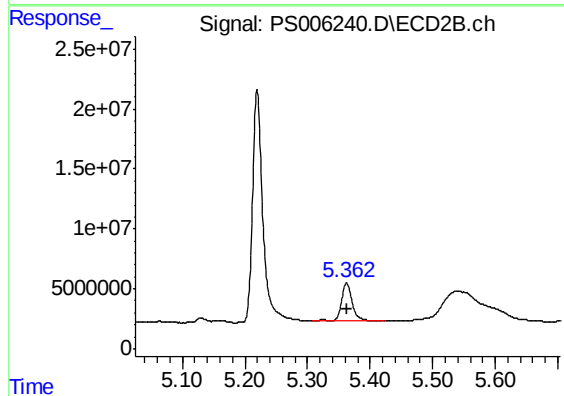

#5 DICAMBA


R.T.: 5.363 min
Delta R.T.: -0.002 min
Response: 37887812
Conc: 20.54 ng/ml

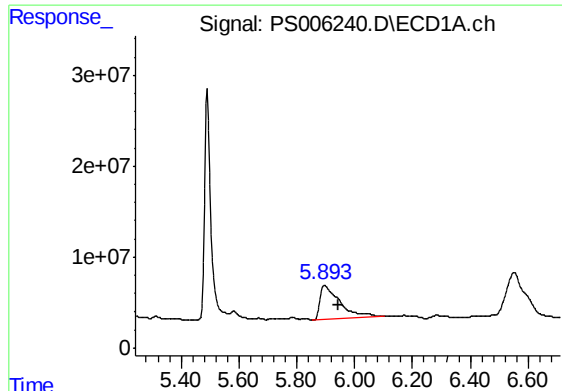

#7 MCPA


R.T.: 5.895 min
Delta R.T.: -0.048 min
Response: 177935572
Conc: 56.36 ug/ml

Instrument :
ECD_S
ClientSampleId :
T6-B-(0-2)

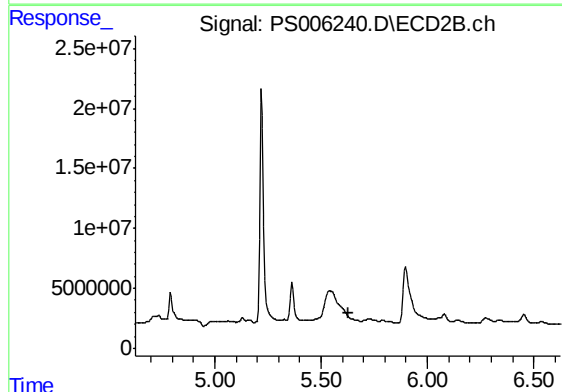


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.626 min
Response: 0
Conc: N.D.

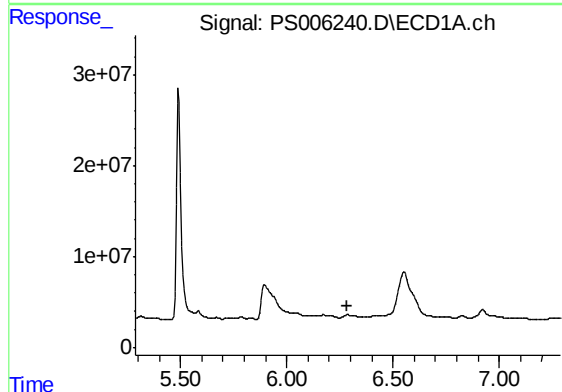


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.288 min
Response: 0
Conc: N.D.

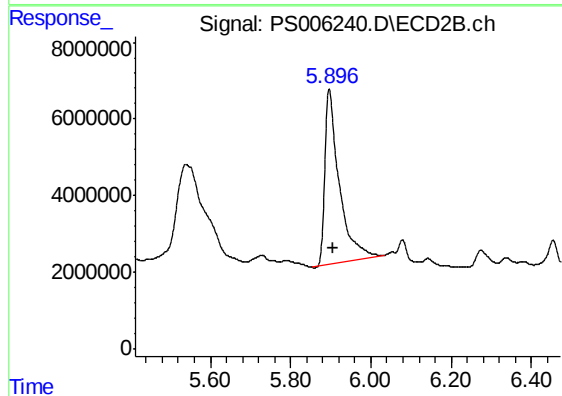

#8 DICHLORPROP


R.T.: 5.897 min
Delta R.T.: -0.008 min
Response: 114008457
Conc: 256.43 ng/ml

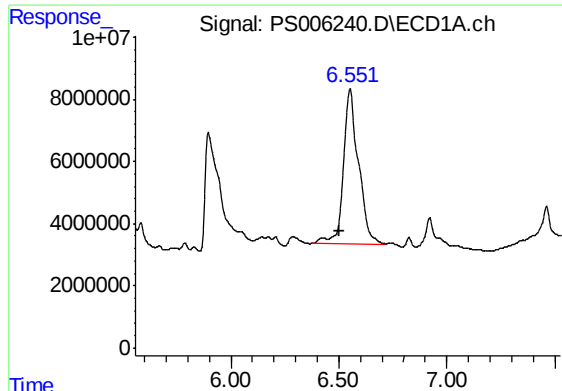

#9 2,4-D


R.T.: 6.552 min
Delta R.T.: 0.049 min
Response: 240103339
Conc: 294.68 ng/ml

Instrument :
ECD_S
ClientSampleId :
T6-B-(0-2)

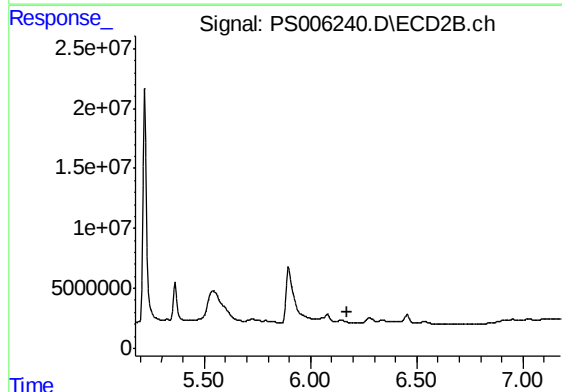


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.176 min
Response: 0
Conc: N.D.

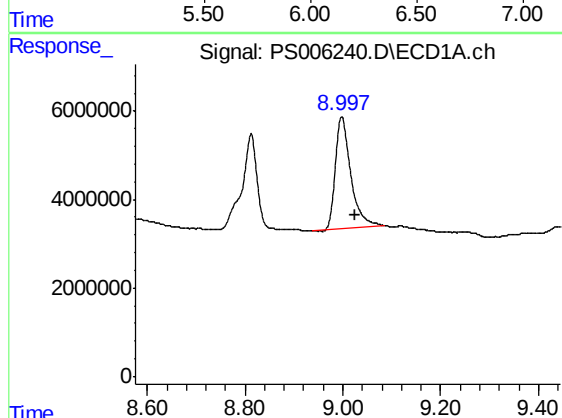

#15 Picloram

R.T.: 8.998 min
Delta R.T.: -0.026 min
Response: 55061060
Conc: 7.40 ng/ml

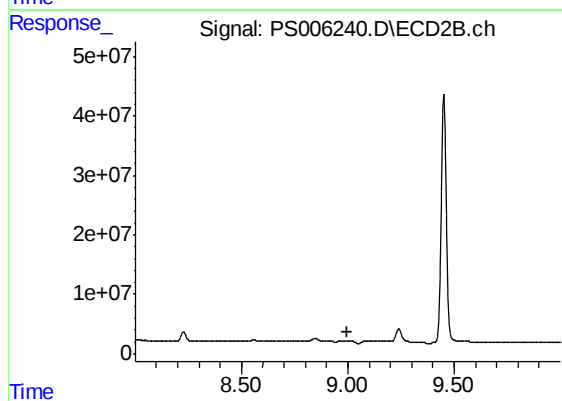

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.000 min
Response: 0
Conc: N.D.