

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082019\
 Data File : PS006244.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2019 17:32
 Operator : SM\AJ
 Sample : PB122403BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 03:25:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.488	5.213	403.6E6	246.5E6	467.574	501.255
Target Compounds							
1) T	Dalapon	2.115	1.738	-28144922	81074124	N.D.	129.203
3) T	4-Nitroph...	0.000	4.893	0	74492617	N.D.	300.707
7) T	MCPA	5.909	0.000	17482106	0	5.537	N.D. #
8) T	DICHLORPROP	6.315	0.000	30076589	0	39.659	N.D. #
15) T	Picloram	0.000	9.003	0	30898163	N.D.	6.850
16) T	DCPA	0.000	9.003	0	30898163	N.D.	8.861



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082019\
Data File : PS006244.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2019 17:32
Operator : SM\AJ
Sample : PB122403BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 03:25:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

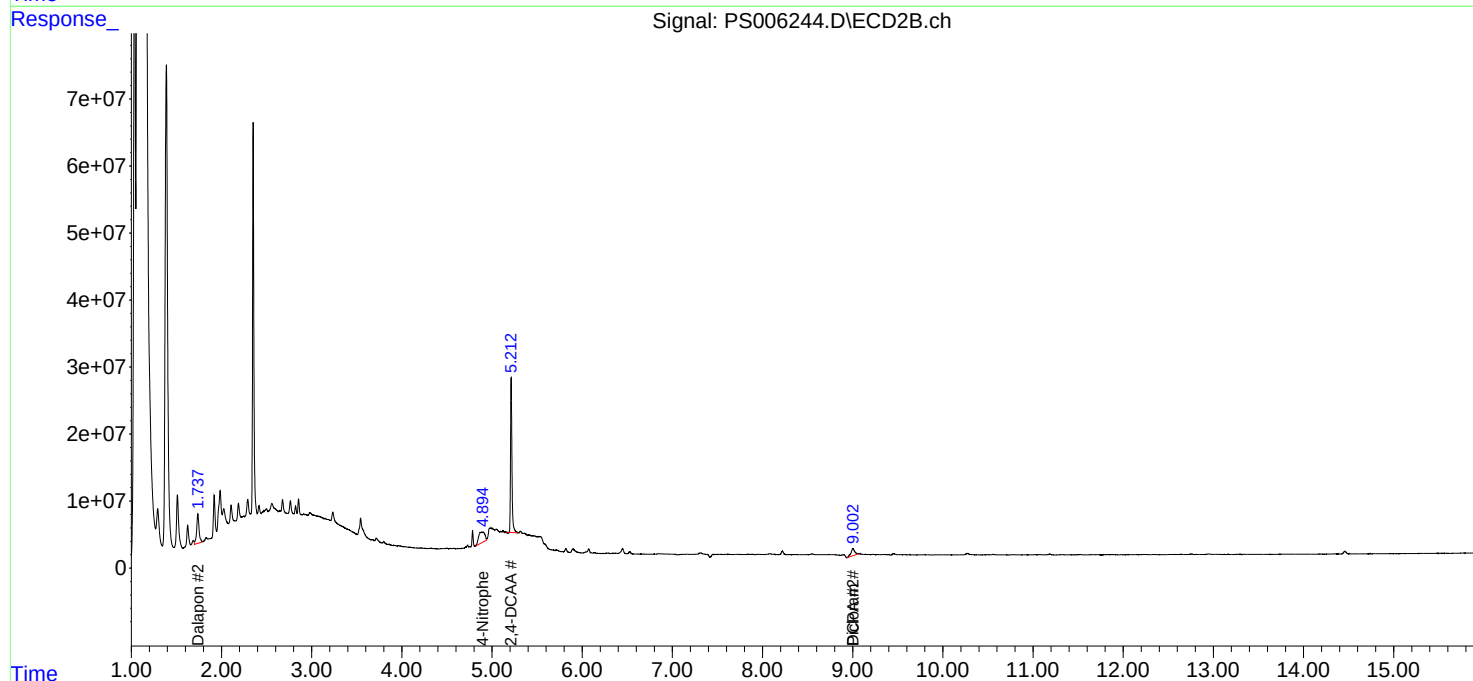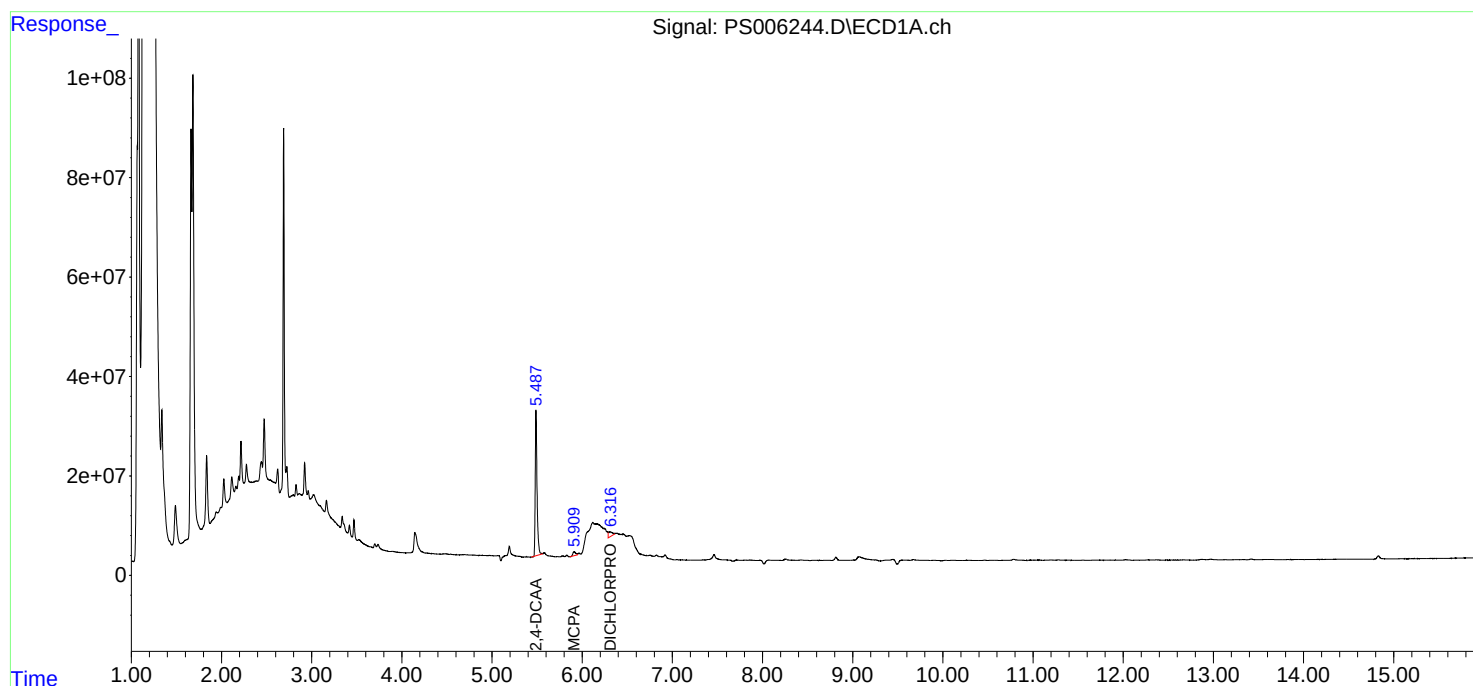


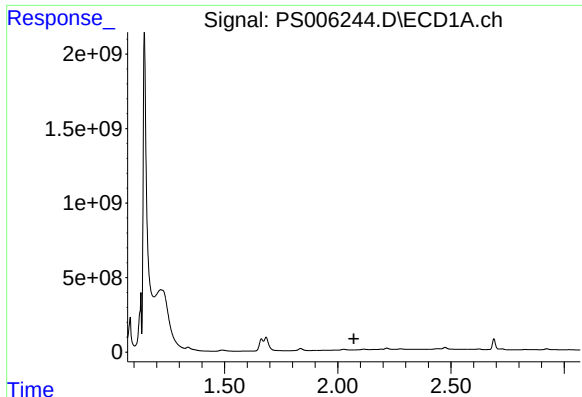

#1 Dalapon


R.T.: 2.115 min
Delta R.T.: 0.044 min
Response: -28144922
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

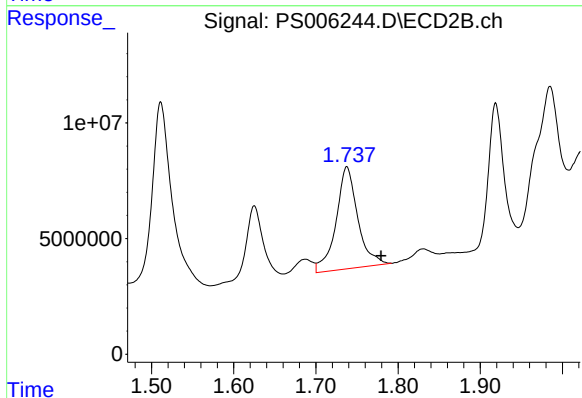


#1 Dalapon

R.T.: 1.738 min
Delta R.T.: -0.041 min
Response: 81074124
Conc: 129.20 ng/ml

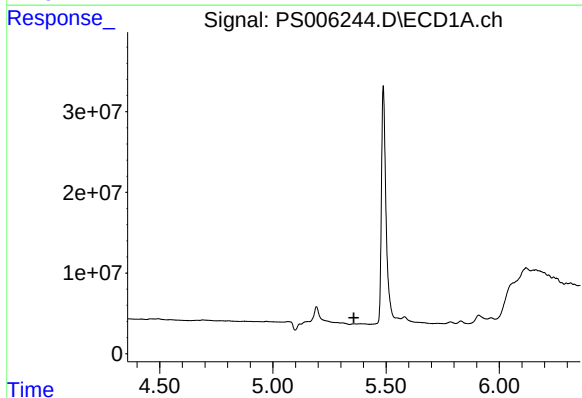


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 5.358 min
Response: 0
Conc: N.D.

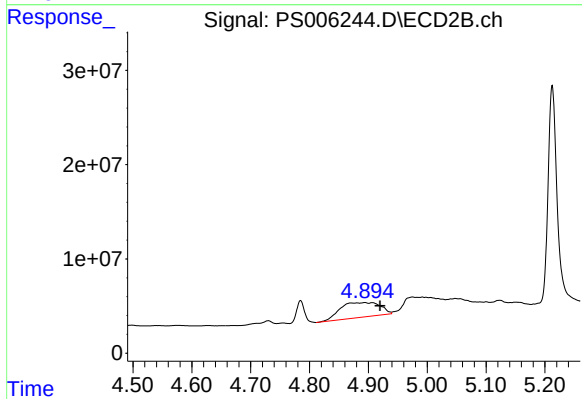

#3 4-Nitrophenol


R.T.: 4.893 min
Delta R.T.: -0.027 min
Response: 74492617
Conc: 300.71 ng/ml

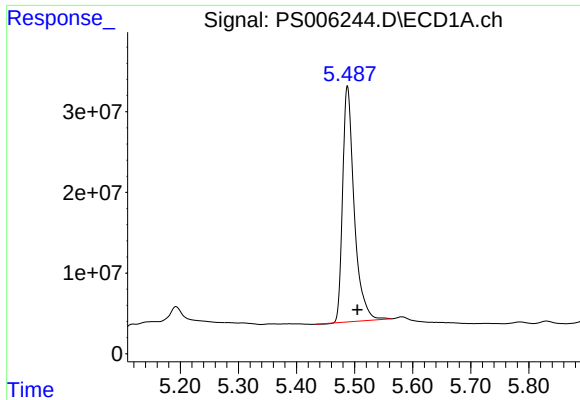

#4 2,4-DCAA


R.T.: 5.488 min
Delta R.T.: -0.017 min
Response: 403610176
Conc: 467.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

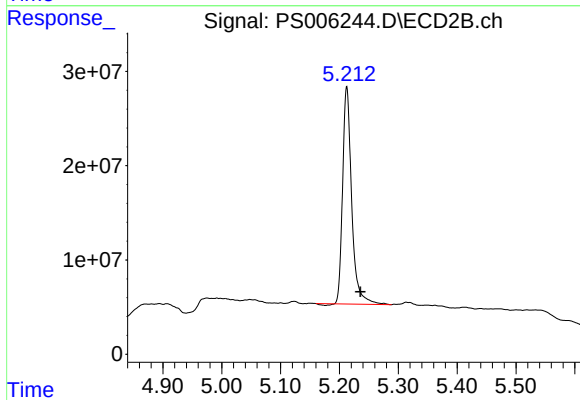


#4 2,4-DCAA

R.T.: 5.213 min
Delta R.T.: -0.023 min
Response: 246543464
Conc: 501.26 ng/ml

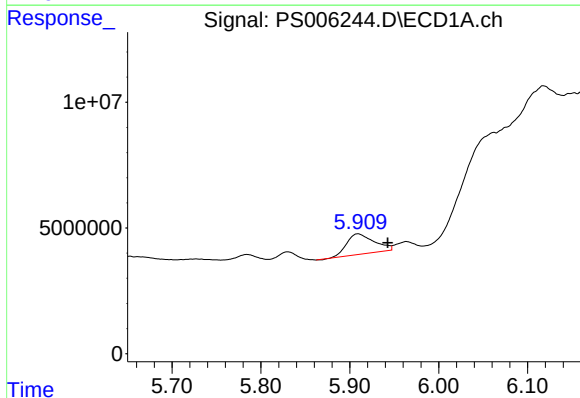


#7 MCPA

R.T.: 5.909 min
Delta R.T.: -0.033 min
Response: 17482106
Conc: 5.54 ug/ml

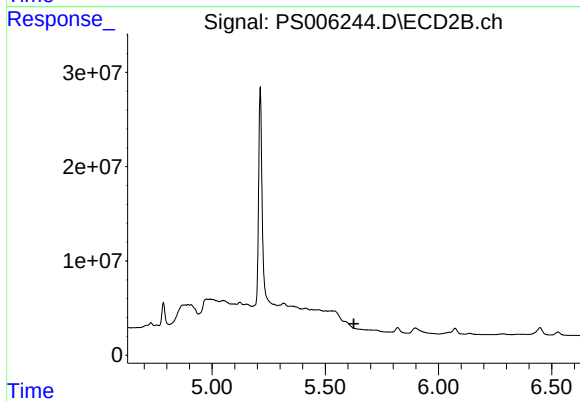

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.626 min
Response: 0
Conc: N.D.

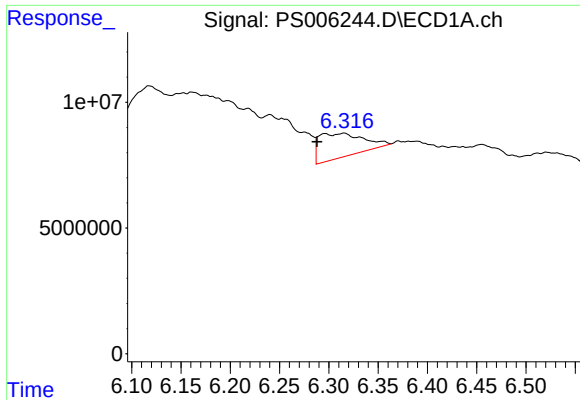

#8 DICHLORPROP


R.T.: 6.315 min
Delta R.T.: 0.027 min
Response: 30076589
Conc: 39.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

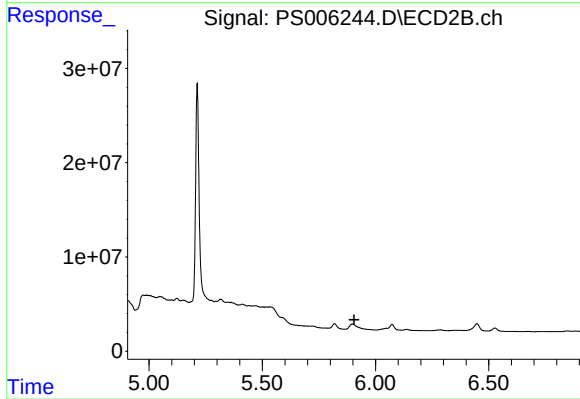


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 5.905 min
Response: 0
Conc: N.D.

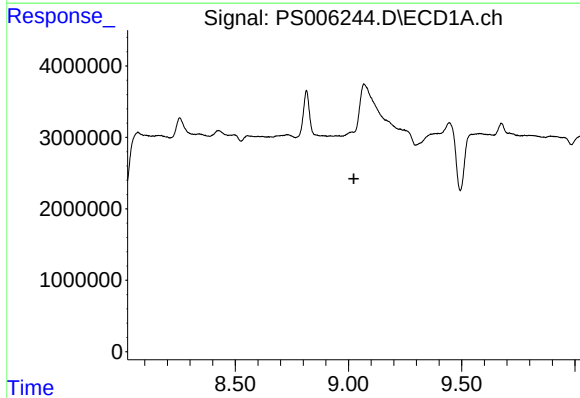


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.024 min
Response: 0
Conc: N.D.

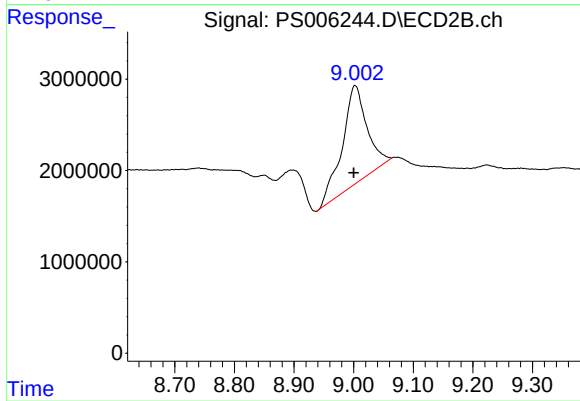

#15 Picloram


R.T.: 9.003 min
Delta R.T.: 0.002 min
Response: 30898163
Conc: 6.85 ng/ml

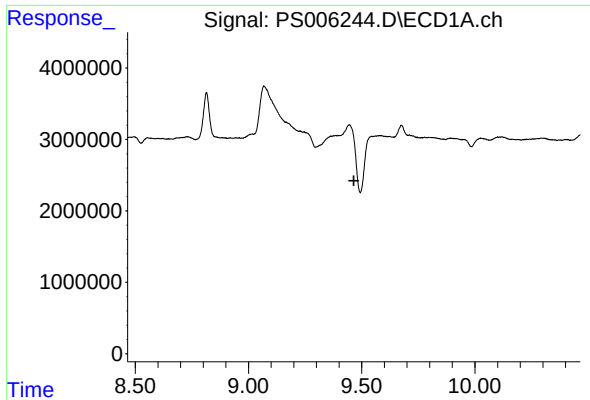

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.465 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

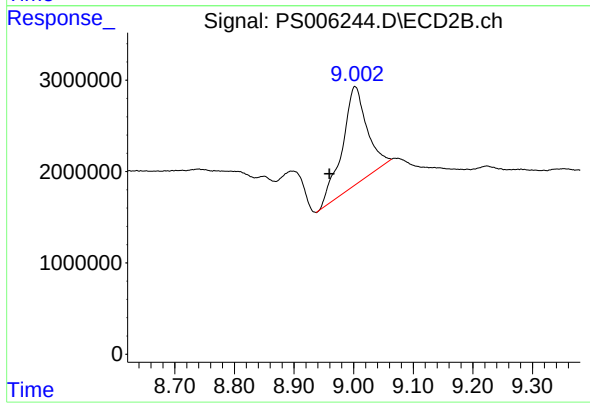

#16 DCPA

R.T.: 9.003 min
Delta R.T.: 0.043 min
Response: 30898163
Conc: 8.86 ng/ml