

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082119\
 Data File : PS006267.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2019 11:45
 Operator : SM\AJ
 Sample : K4403-29
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 22 01:47:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.494	5.223	395.2E6	253.7E6	457.861	515.723
Target Compounds							
1) T	Dalapon	2.034	1.749	45579518	88817058	41.830	141.543 #
2) T	3,5-DICHL...	4.880	0.000	28105203	0	26.068	N.D. #
5) T	DICAMBA	0.000	5.367	0	21943117	N.D.	11.896
7) T	MCPA	5.910	0.000	86848614	0	27.509	N.D. #
8) T	DICHLORPROP	0.000	5.903	0	55592410	N.D.	125.038
9) T	2,4-D	6.554	0.000	239.6E6	0	294.022	N.D. #
15) T	Picloram	9.010	0.000	23109351	0	3.106	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS082119\
Data File : PS006267.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2019 11:45
Operator : SM\AJ
Sample : K4403-29
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 22 01:47:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

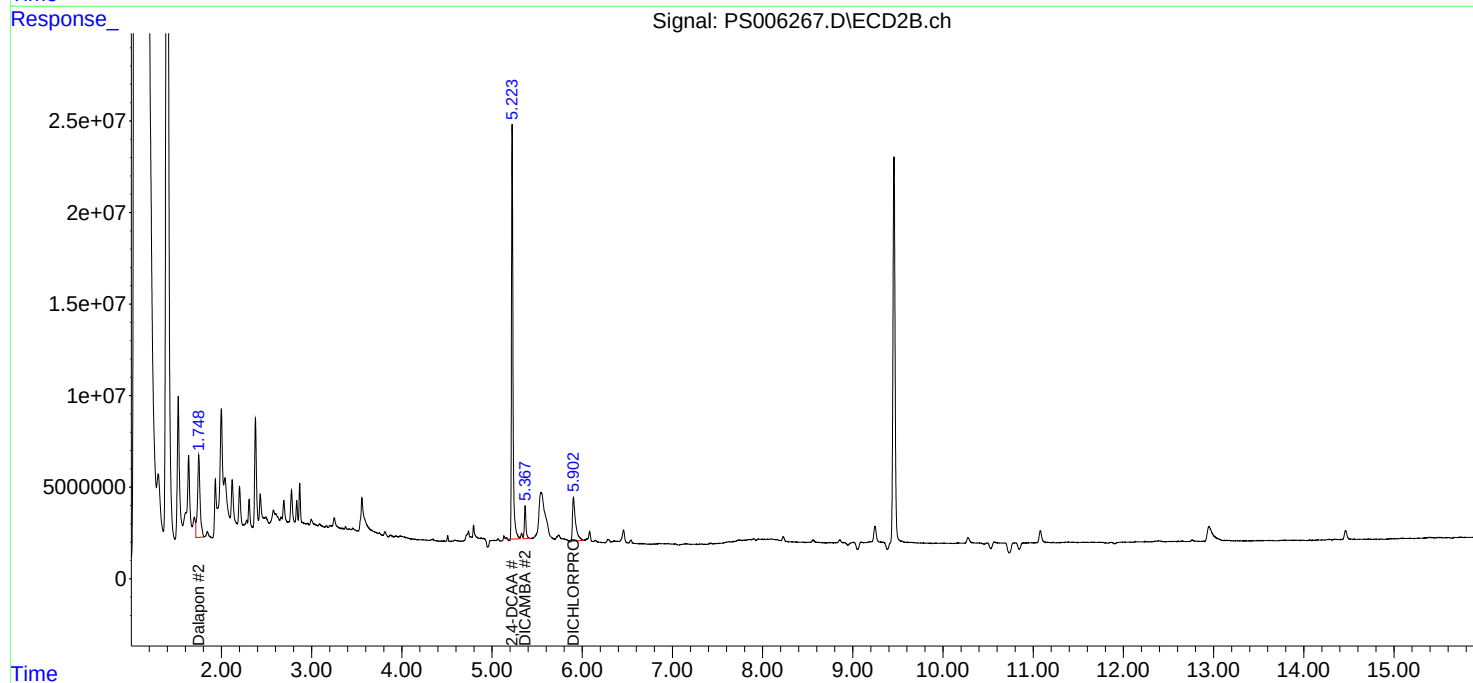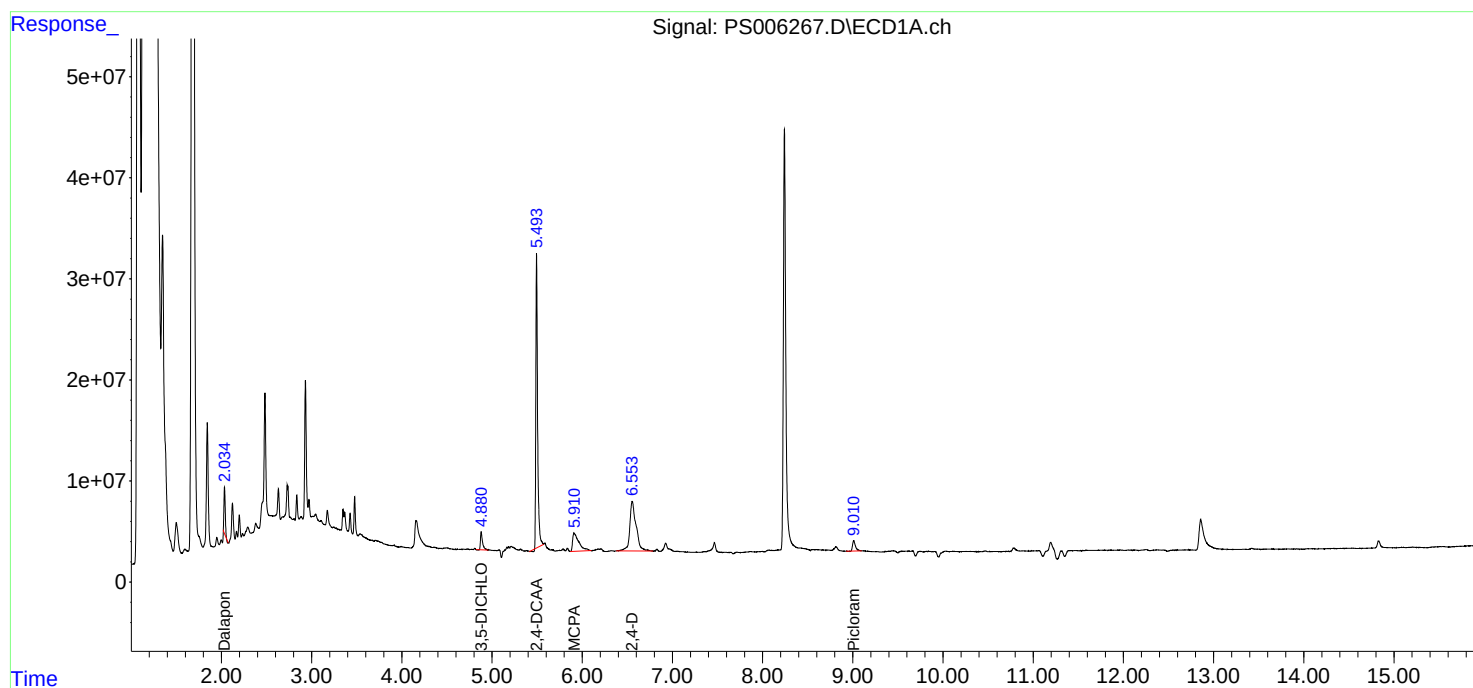


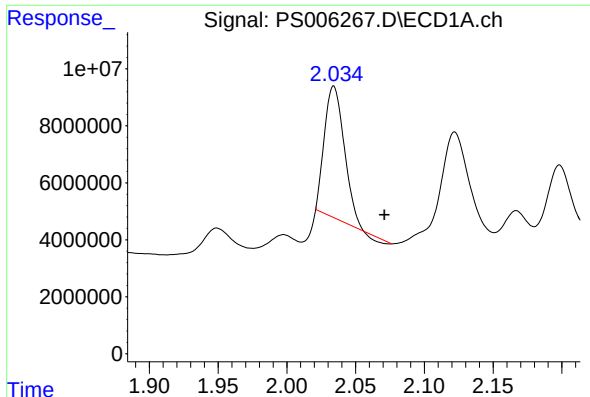

#1 Dalapon


R.T.: 2.034 min
Delta R.T.: -0.037 min
Response: 45579518
Conc: 41.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

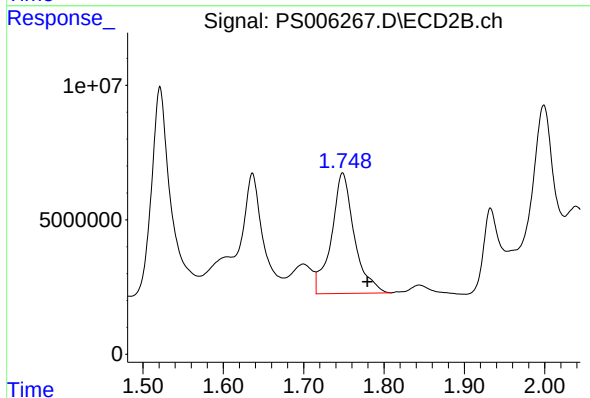


#1 Dalapon

R.T.: 1.749 min
Delta R.T.: -0.031 min
Response: 88817058
Conc: 141.54 ng/ml

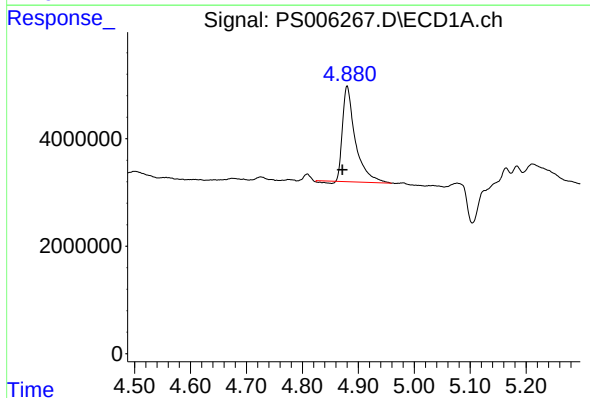


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.880 min
Delta R.T.: 0.009 min
Response: 28105203
Conc: 26.07 ng/ml

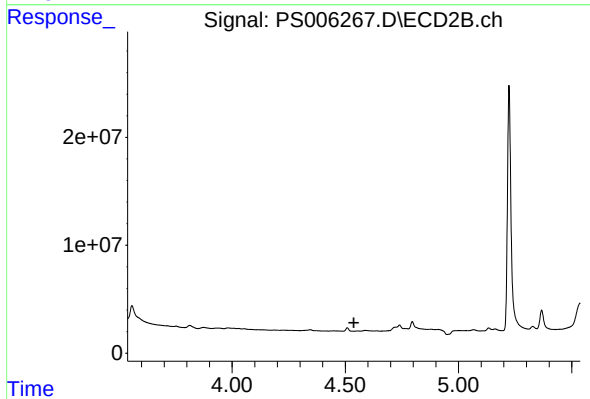

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.538 min
Response: 0
Conc: N.D.

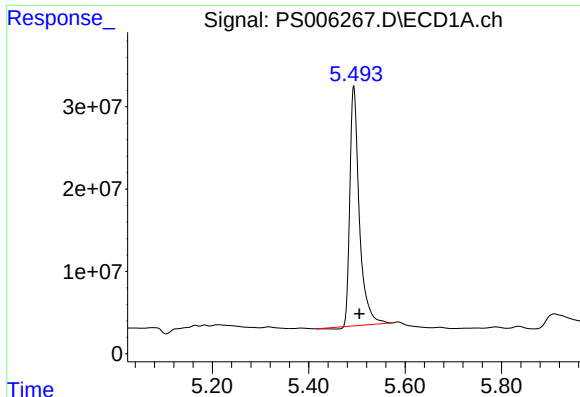

#4 2,4-DCAA


R.T.: 5.494 min
Delta R.T.: -0.012 min
Response: 395226176
Conc: 457.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

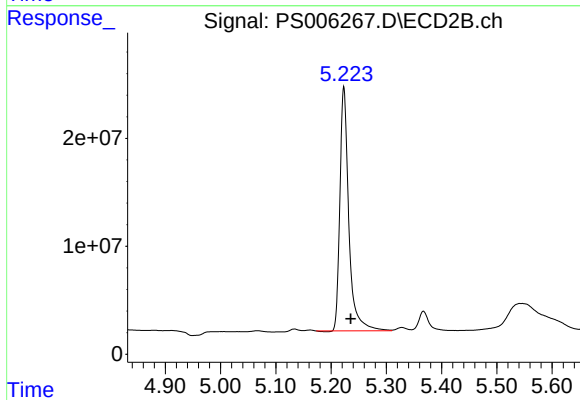


#4 2,4-DCAA

R.T.: 5.223 min
Delta R.T.: -0.012 min
Response: 253659470
Conc: 515.72 ng/ml

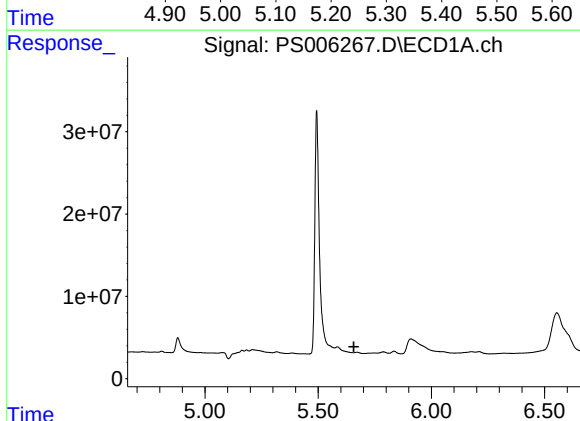


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.658 min
Response: 0
Conc: N.D.

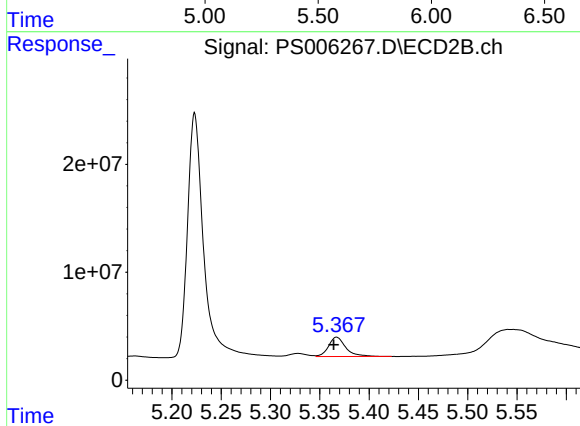

#5 DICAMBA


R.T.: 5.367 min
Delta R.T.: 0.003 min
Response: 21943117
Conc: 11.90 ng/ml

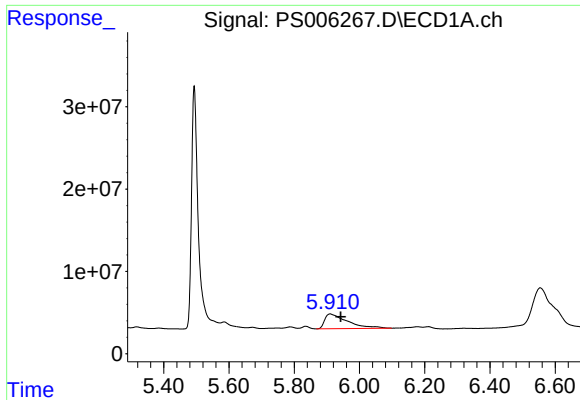

#7 MCPA


R.T.: 5.910 min
Delta R.T.: -0.032 min
Response: 86848614
Conc: 27.51 ug/ml

Instrument :
ECD_S
ClientSampleId :

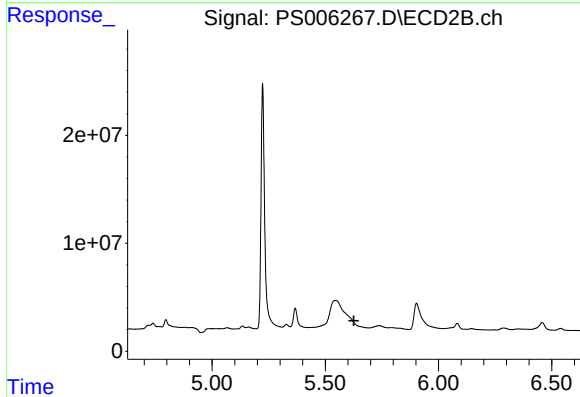


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.626 min
Response: 0
Conc: N.D.

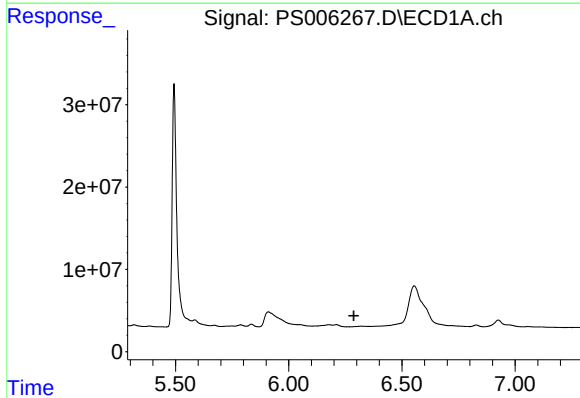


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.288 min
Response: 0
Conc: N.D.

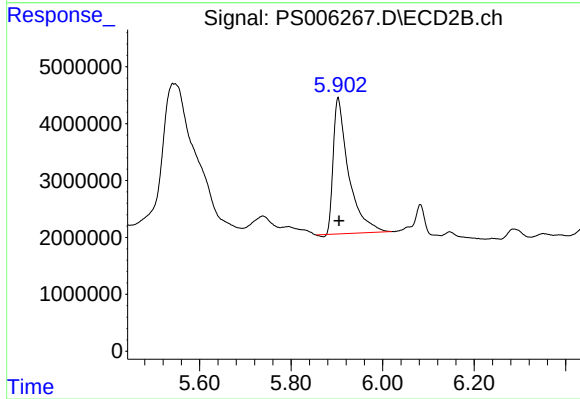

#8 DICHLORPROP


R.T.: 5.903 min
Delta R.T.: -0.002 min
Response: 55592410
Conc: 125.04 ng/ml

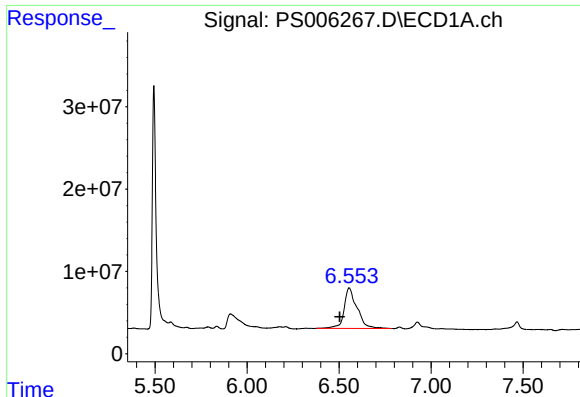

#9 2,4-D


R.T.: 6.554 min
Delta R.T.: 0.051 min
Response: 239564522
Conc: 294.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

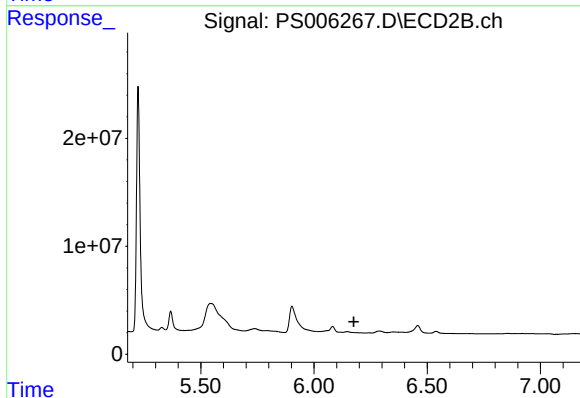


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.176 min
Response: 0
Conc: N.D.

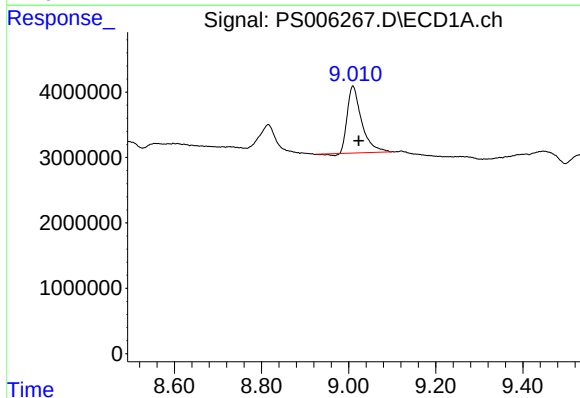

#15 Picloram

R.T.: 9.010 min
Delta R.T.: -0.014 min
Response: 23109351
Conc: 3.11 ng/ml

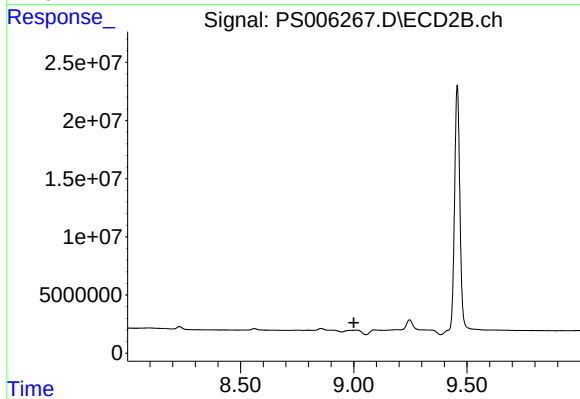

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.000 min
Response: 0
Conc: N.D.