

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083118\
 Data File : PS001667.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2018 23:07
 Operator : EI\SJ
 Sample : J4726-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 00:25:04 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 23 02:55:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.466	10.966	97332655	95530868	527.261	471.688
Target Compounds							
2) T	3,5-DICHL...	0.000	9.206	0 43223409		N.D.	169.136 #
5) T	DICAMBA	0.000	11.209	0 3221258		N.D.	4.593 #
6) T	MCP	12.154	0.000	12474160	0	24.792	N.D. #
15) T	Picloram	0.000	16.900	0 6484372		N.D.	4.973 #
16) T	DCPA	0.000	16.900	0 6484372		N.D.	4.542 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS083118\
Data File : PS001667.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2018 23:07
Operator : EI\SJ
Sample : J4726-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 00:25:04 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS082218.M
Quant Title : 8080.M
QLast Update : Thu Aug 23 02:55:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

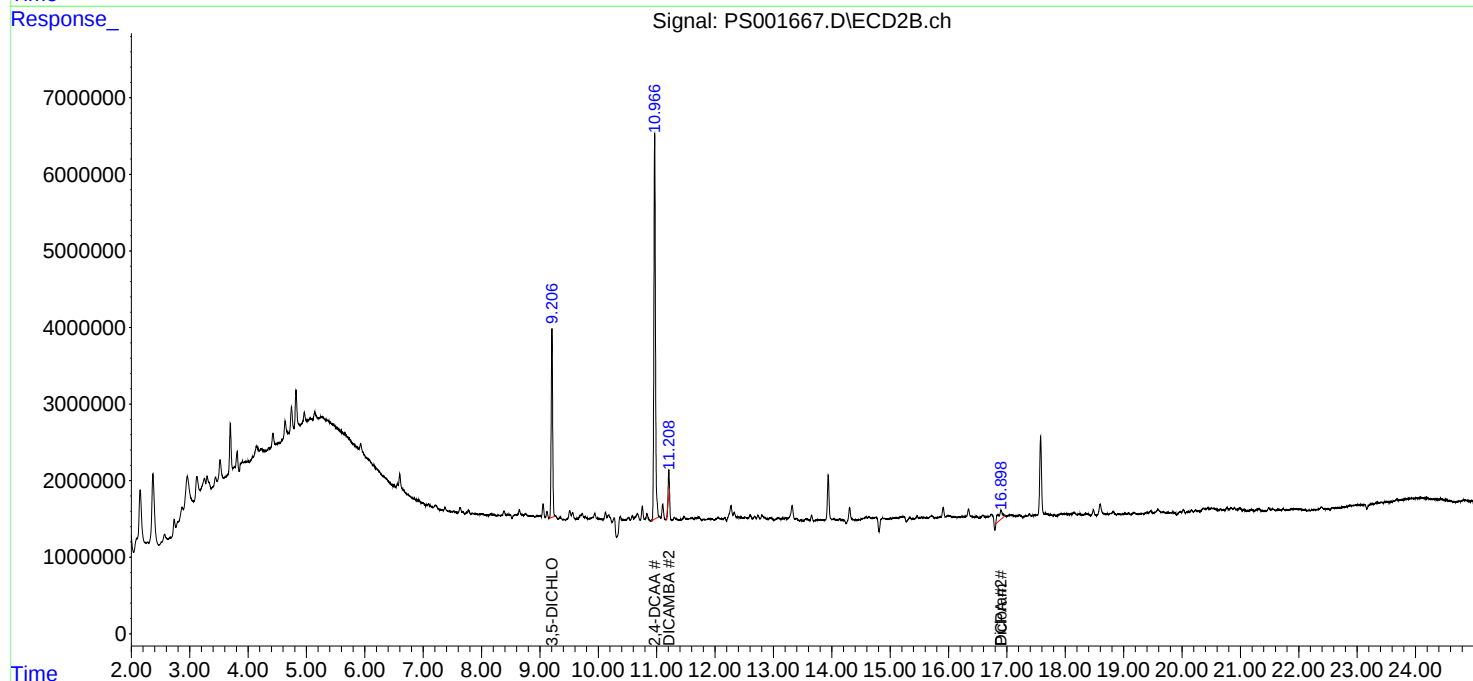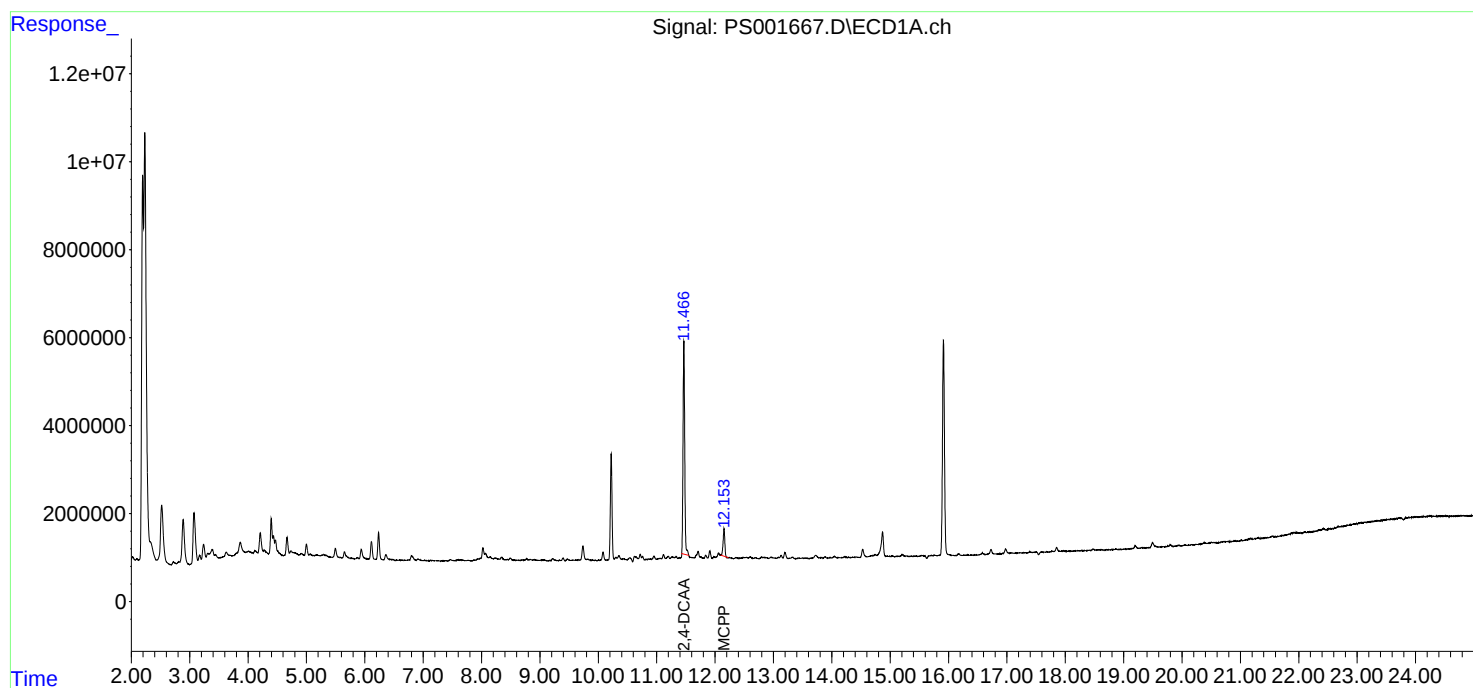


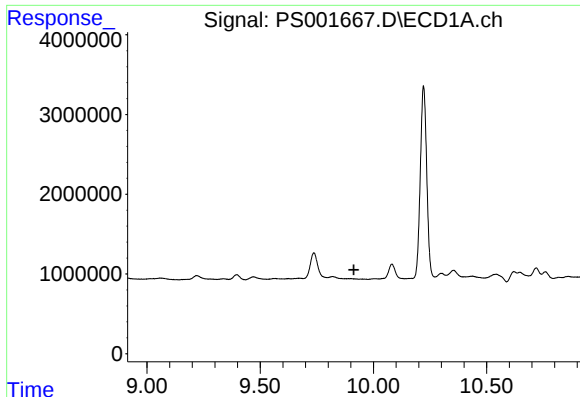

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

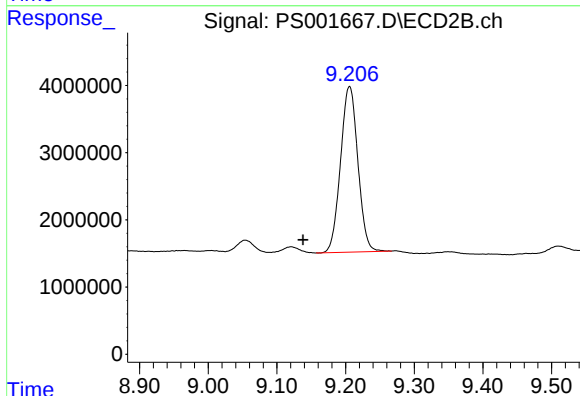


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.206 min
Delta R.T.: 0.068 min
Response: 43223409
Conc: 169.14 ng/ml

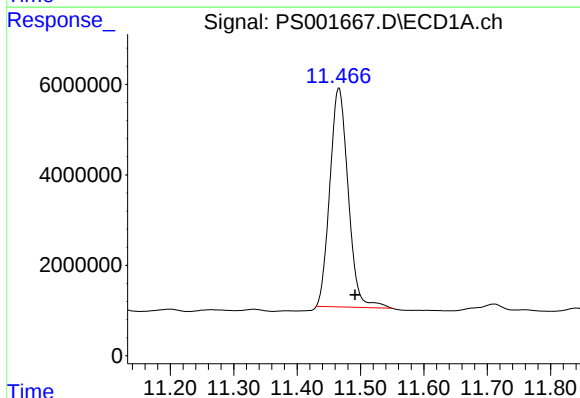


#4 2,4-DCAA

R.T.: 11.466 min
Delta R.T.: -0.026 min
Response: 97332655
Conc: 527.26 ng/ml

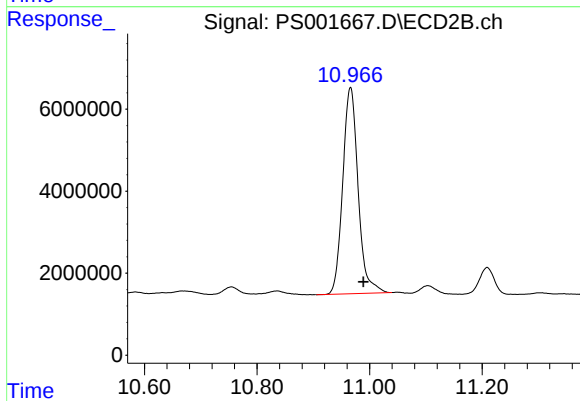

#4 2,4-DCAA


R.T.: 10.966 min
Delta R.T.: -0.023 min
Response: 95530868
Conc: 471.69 ng/ml

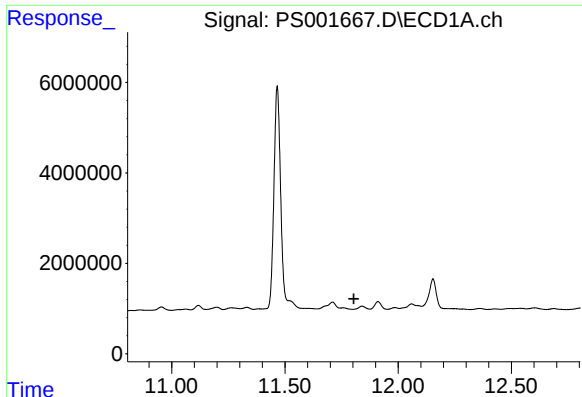

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.805 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

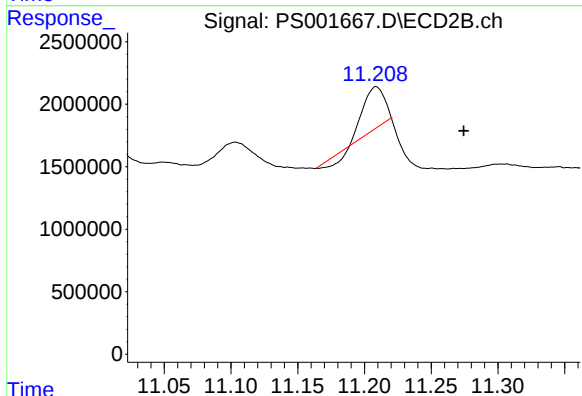


#5 DICAMBA

R.T.: 11.209 min
Delta R.T.: -0.066 min
Response: 3221258
Conc: 4.59 ng/ml

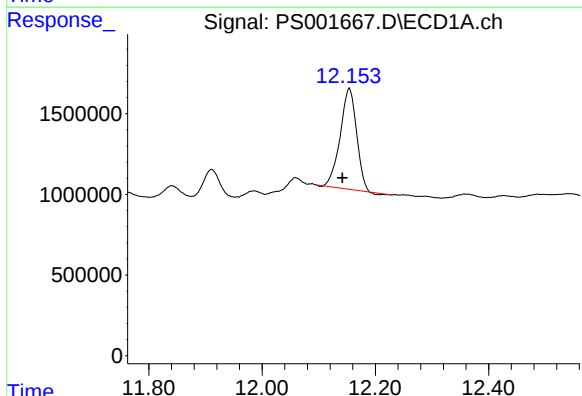


#6 MCP

R.T.: 12.154 min
Delta R.T.: 0.012 min
Response: 12474160
Conc: 24.79 ug/ml

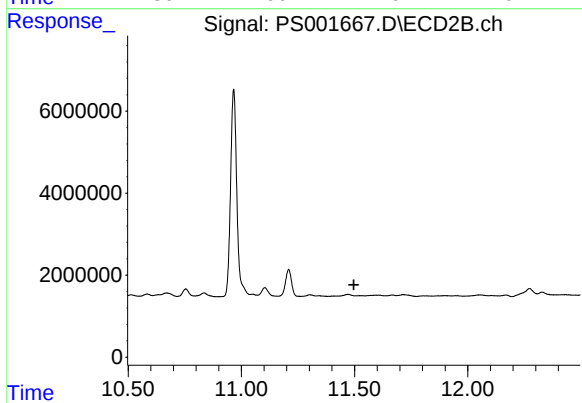

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.497 min
Response: 0
Conc: N.D.

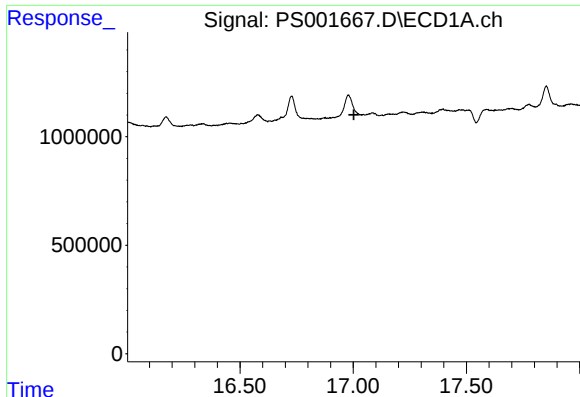

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 17.003 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

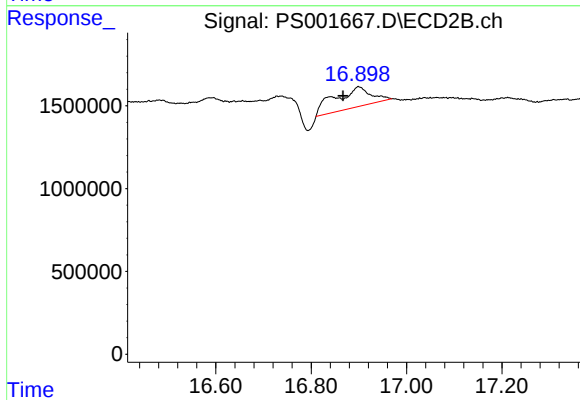


#15 Picloram

R.T.: 16.900 min
Delta R.T.: 0.032 min
Response: 6484372
Conc: 4.97 ng/ml

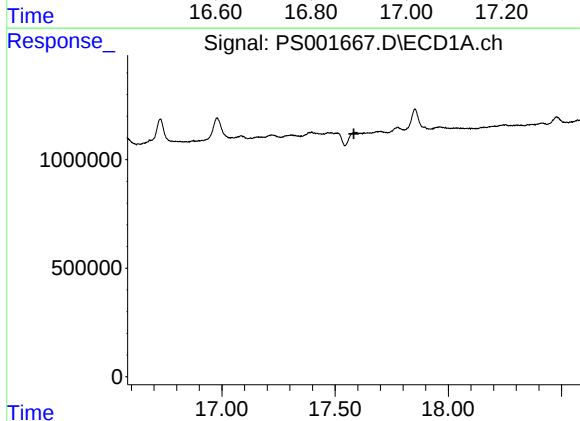

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.583 min
Response: 0
Conc: N.D.

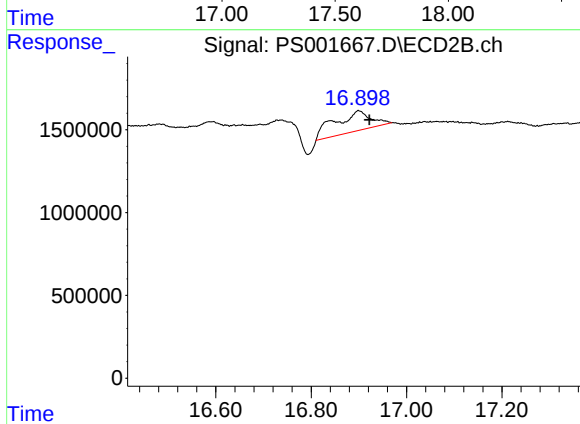

#16 DCPA

R.T.: 16.900 min
Delta R.T.: -0.023 min
Response: 6484372
Conc: 4.54 ng/ml