

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091419\
 Data File : PS006718.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2019 08:52
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 00:44:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 10 06:14:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	4.862	0.000	2780570	0	2.809	N.D. #
7) T	MCPA	5.974	0.000	13678778	0	4.840	N.D. #
9) T	2,4-D	6.499	0.000	42008498	0	54.371	N.D. #
12) T	2,4,5-T	0.000	7.275	0	15265023	N.D.	7.080
15) T	Picloram	9.007	8.971	139.7E6	79042517	20.712	21.359
16) T	DCPA	0.000	8.971	0	79042517	N.D.	25.091



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091419\
Data File : PS006718.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2019 08:52
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 00:44:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
Quant Title : 8080.M
QLast Update : Tue Sep 10 06:14:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

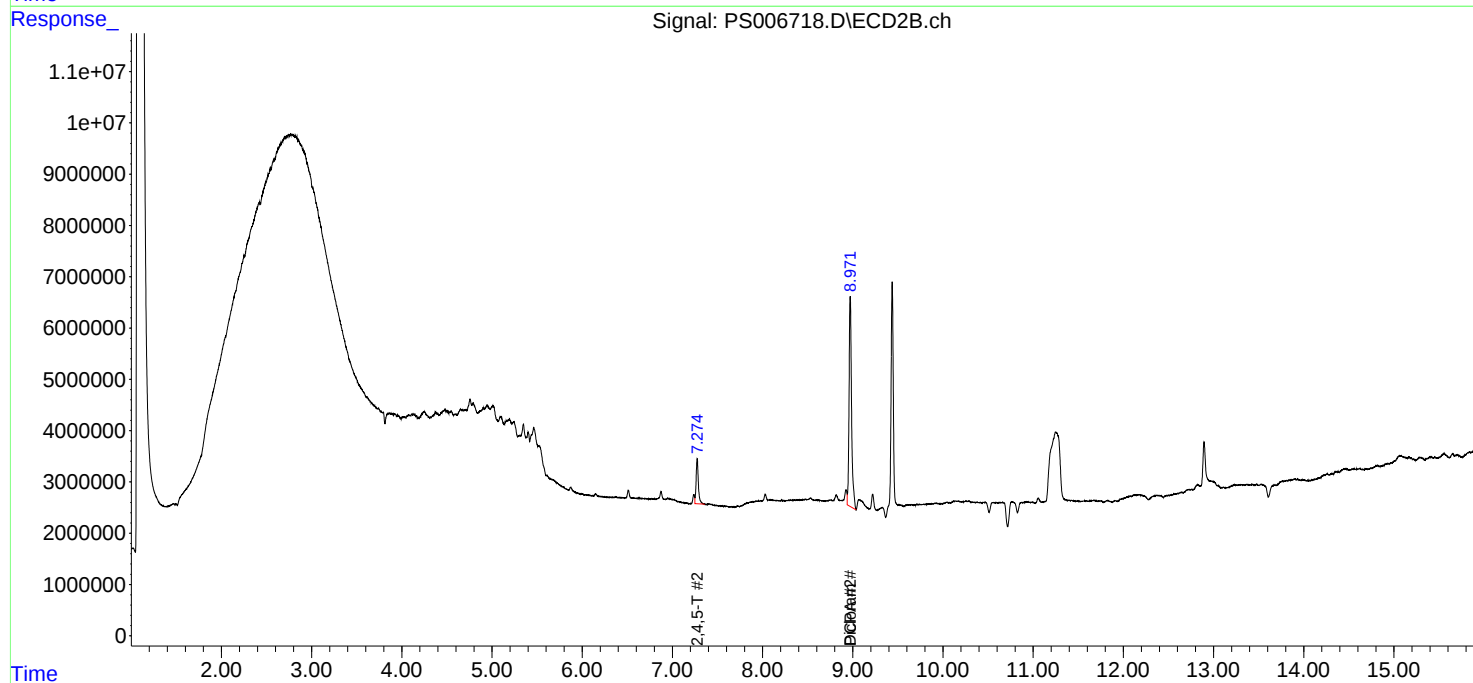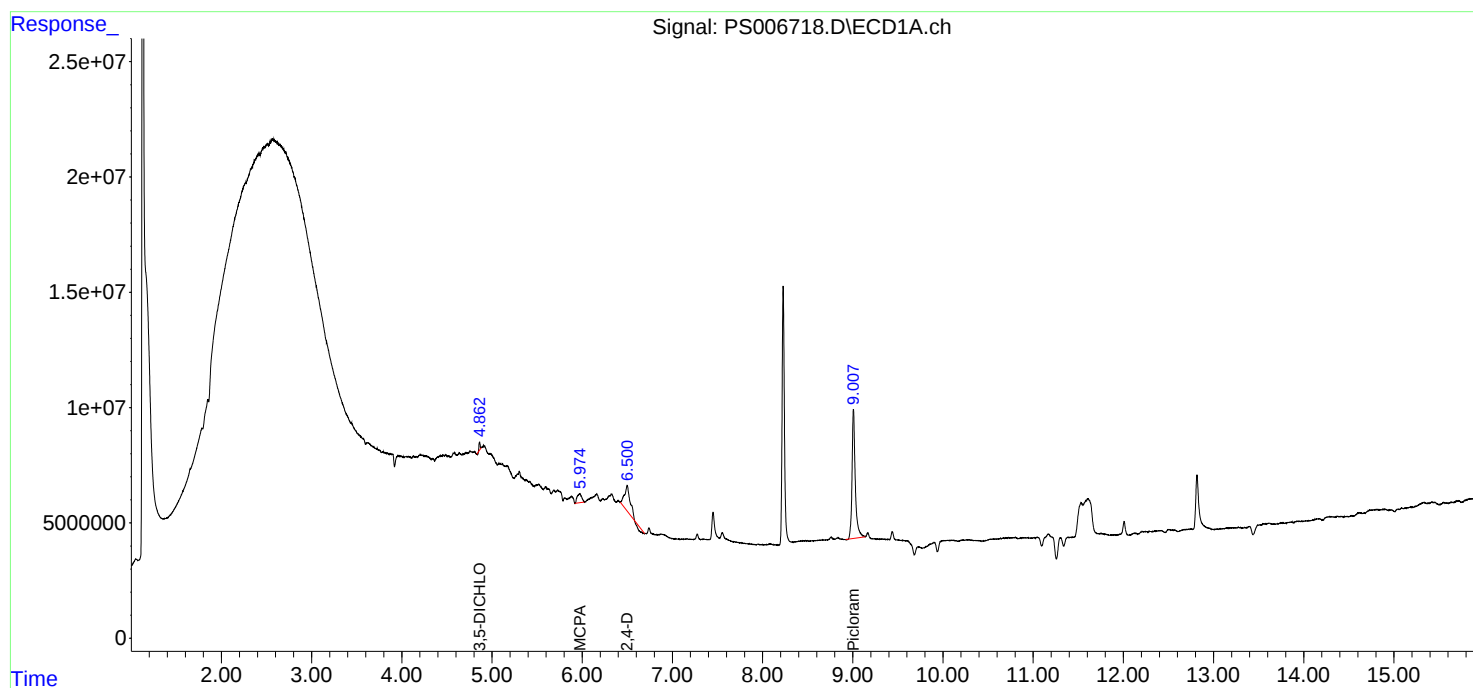


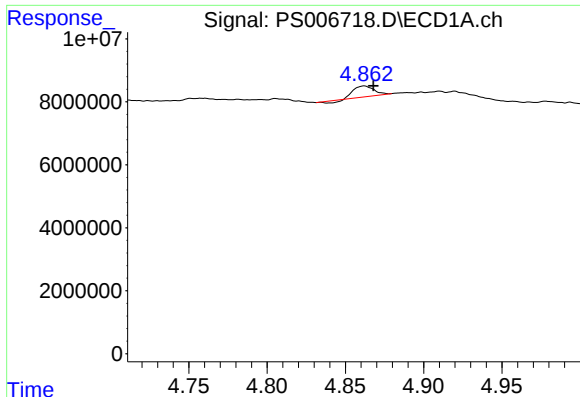

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.862 min
Delta R.T.: -0.006 min
Response: 2780570
Conc: 2.81 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

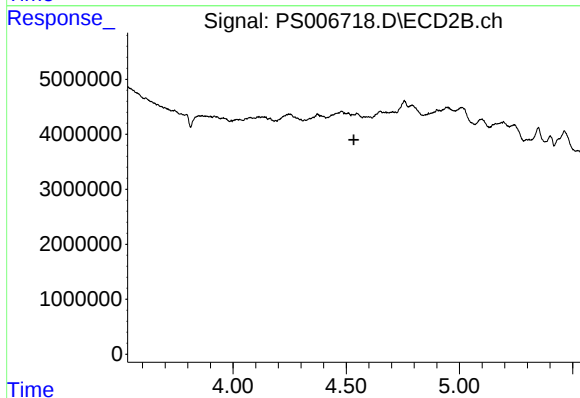


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.533 min
Response: 0
Conc: N.D.

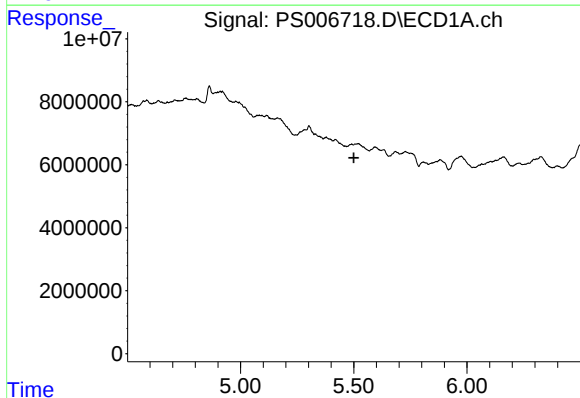


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

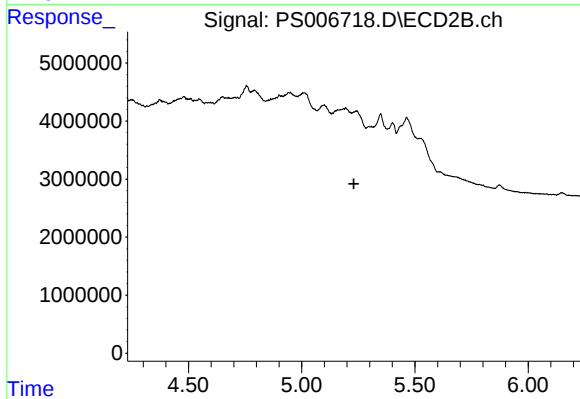

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 5.230 min
Response: 0
Conc: N.D.

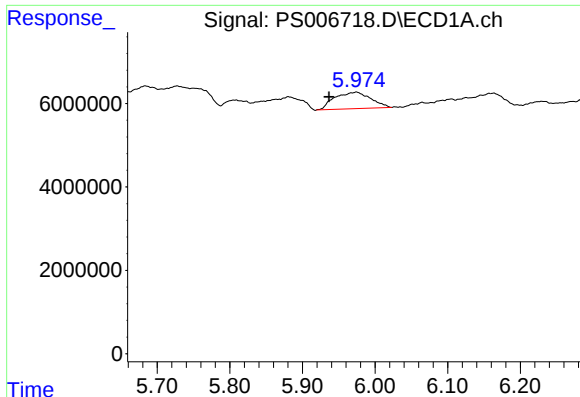

#7 MCPA


R.T.: 5.974 min
Delta R.T.: 0.037 min
Response: 13678778
Conc: 4.84 ug/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

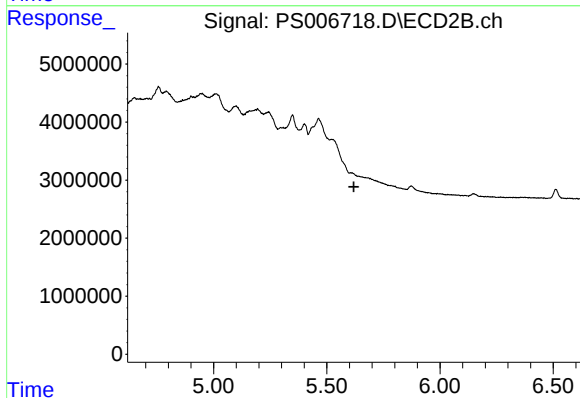


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.619 min
Response: 0
Conc: N.D.

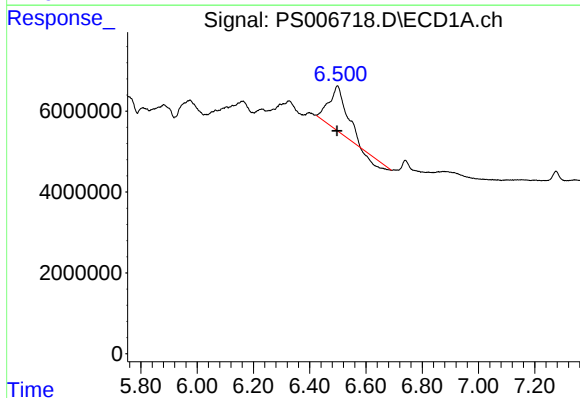


#9 2,4-D

R.T.: 6.499 min
Delta R.T.: 0.002 min
Response: 42008498
Conc: 54.37 ng/ml

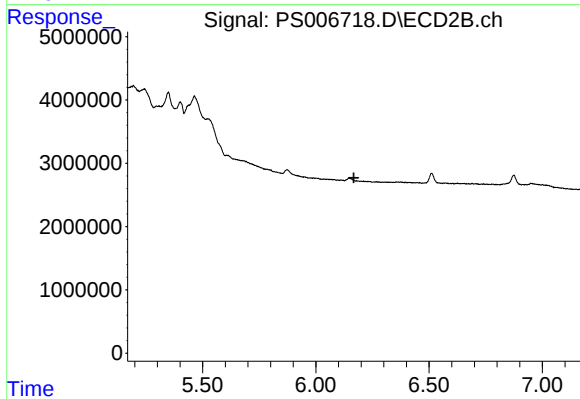

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 6.168 min
Response: 0
Conc: N.D.

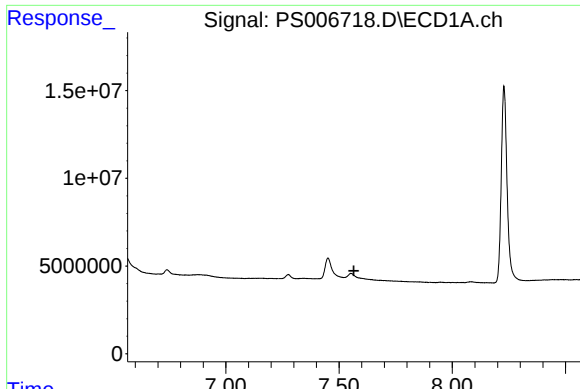

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.565 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

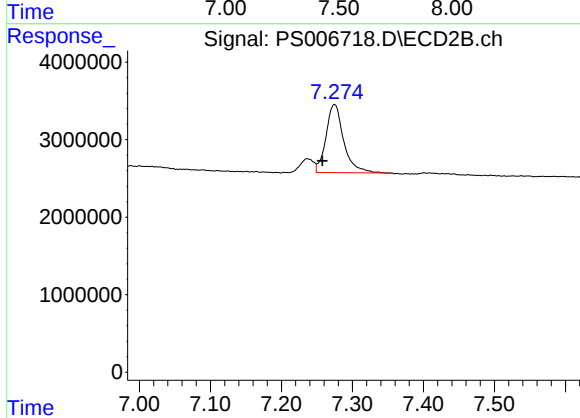


#12 2,4,5-T

R.T.: 7.275 min
Delta R.T.: 0.017 min
Response: 15265023
Conc: 7.08 ng/ml

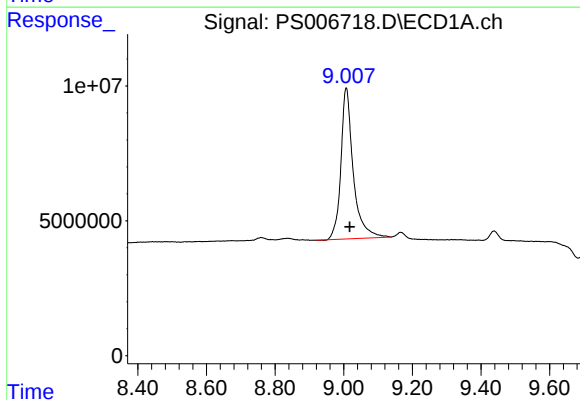


#15 Picloram

R.T.: 9.007 min
Delta R.T.: -0.010 min
Response: 139719618
Conc: 20.71 ng/ml

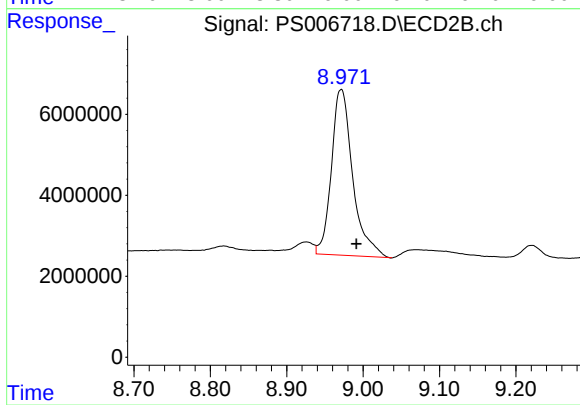

#15 Picloram


R.T.: 8.971 min
Delta R.T.: -0.020 min
Response: 79042517
Conc: 21.36 ng/ml

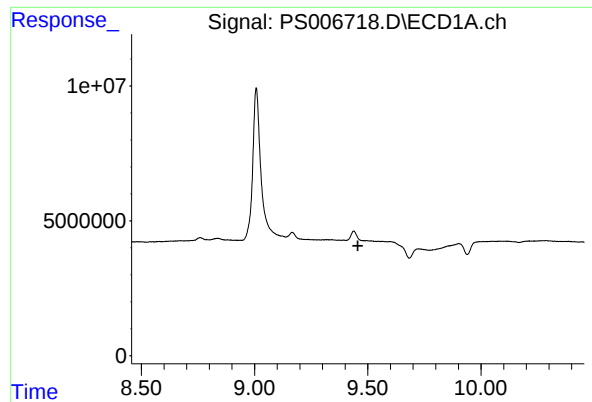

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.456 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

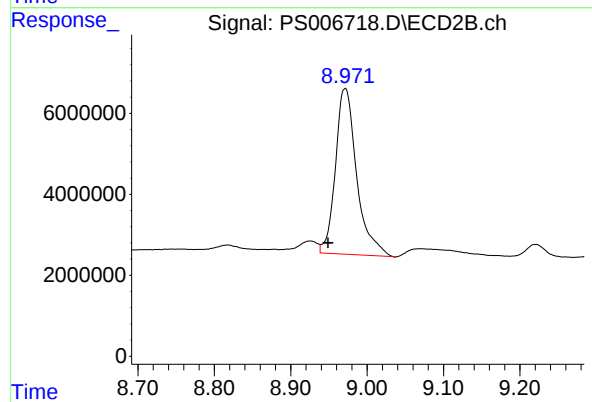

#16 DCPA

R.T.: 8.971 min
Delta R.T.: 0.023 min
Response: 79042517
Conc: 25.09 ng/ml