

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091419\
 Data File : PS006723.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2019 10:42
 Operator : SM\AJ
 Sample : K4852-13RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 BUS-1(0-5)RE

Manual Integrations
 APPROVED

Ankita
 9/16/2019 5:58:13 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 00:46:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 10 06:14:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.491	5.200	134.4E6	18730057	173.058	43.864m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS091419\
Data File : PS006723.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2019 10:42
Operator : SM\AJ
Sample : K4852-13RE
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
BUS-1(0-5)RE


Manual Integrations
APPROVED

Ankita
9/16/2019 5:58:13 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 00:46:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS090919.M
Quant Title : 8080.M
QLast Update : Tue Sep 10 06:14:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

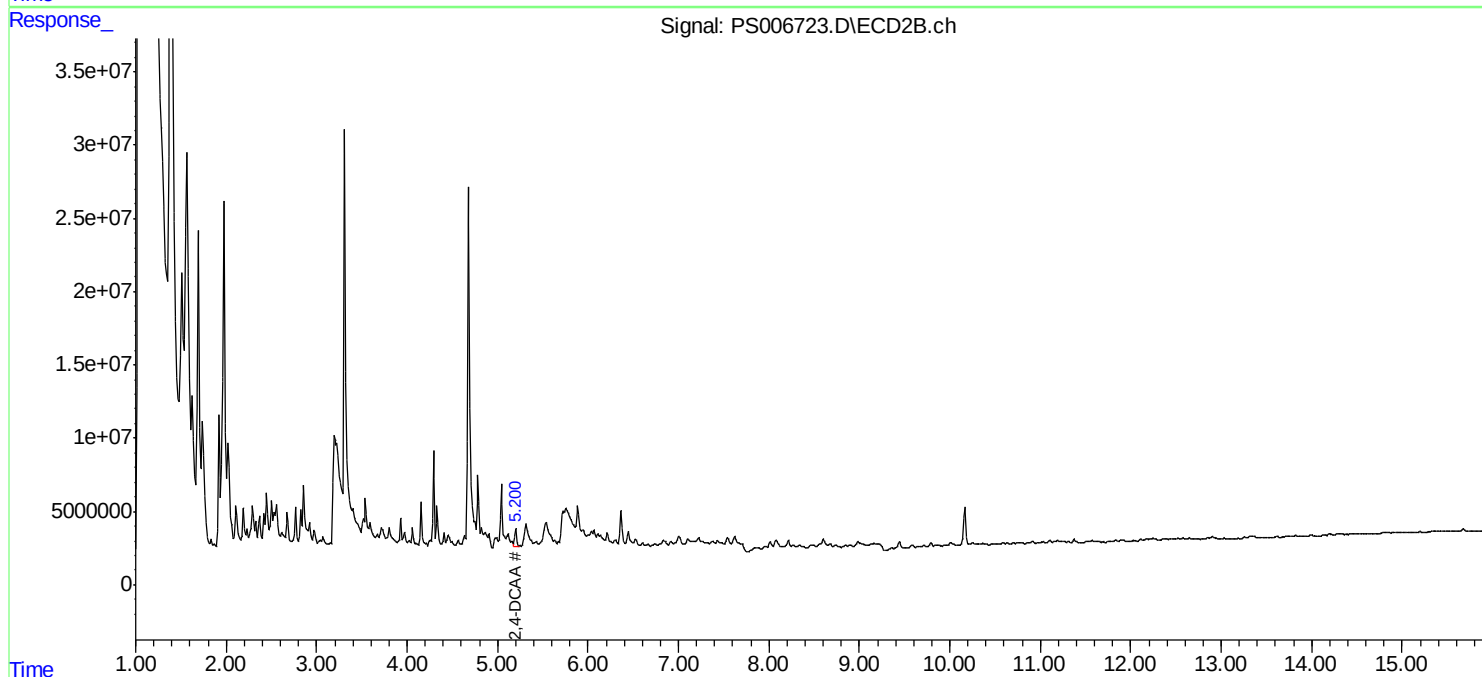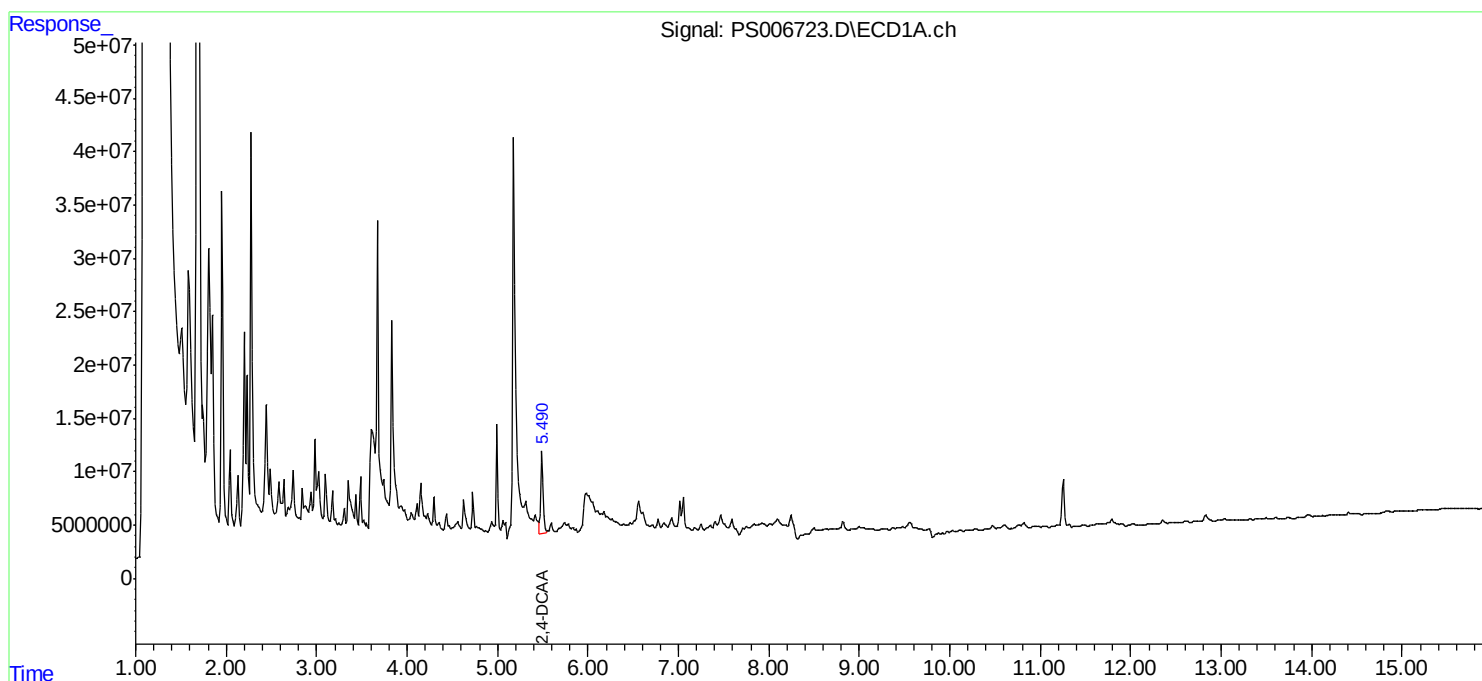

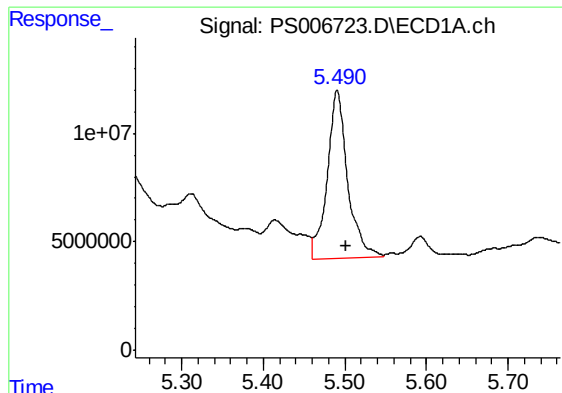


#4 2,4-DCAA

R.T.: 5.491 min
Delta R.T.: -0.010 min
Response: 134446365
Conc: 173.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
BUS-1(0-5)RE

Manual Integrations
APPROVED

Ankita
9/16/2019 5:58:13 PM

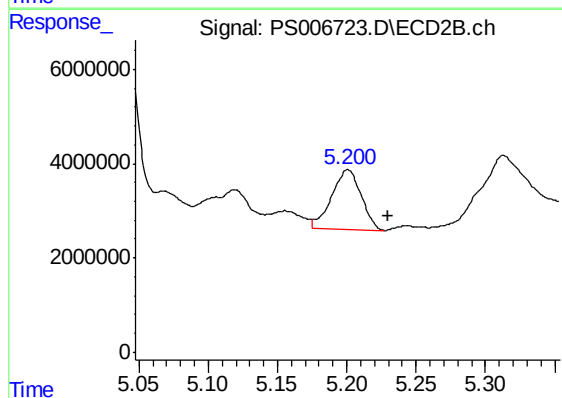

#4 2,4-DCAA

R.T.: 5.200 min
Delta R.T.: -0.030 min
Response: 18730057
Conc: 43.86 ng/ml m