

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092322\
 Data File : PS020635.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2022 09:10
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 00:26:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 14 02:51:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.181	6.761	1786.3E6	490.0E6	519.048	575.321
Target Compounds							
1) T	Dalapon	3.029	0.000	646615	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.457f	0.000	25702314	0	5.154	N.D. #
6) T	MCP	0.000	6.989	0	2022102	N.D.	<MDL
7) T	MCPA	7.649	0.000	493394	0	<MDL	N.D. #
9) T	2,4-D	8.358f	0.000	47308273	0	10.178	N.D. #
10) T	Pentachlo...	8.537f	0.000	1888352	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.166	0.000	2747957	0	<MDL	N.D. #
12) T	2,4,5-T	9.498f	0.000	9618551	0	<MDL	N.D. #
13) T	2,4-DB	9.917f	0.000	2741317	0	<MDL	N.D. #
14) T	DINOSEB	11.085f	0.000	81293995	0	4.426	N.D. #
15) T	Picloram	10.962	0.000	123.3E6	0	4.096	N.D. #
16) T	DCPA	11.401	0.000	6896347	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092322\
Data File : PS020635.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2022 09:10
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 00:26:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
Quant Title : 8080.M
QLast Update : Wed Sep 14 02:51:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

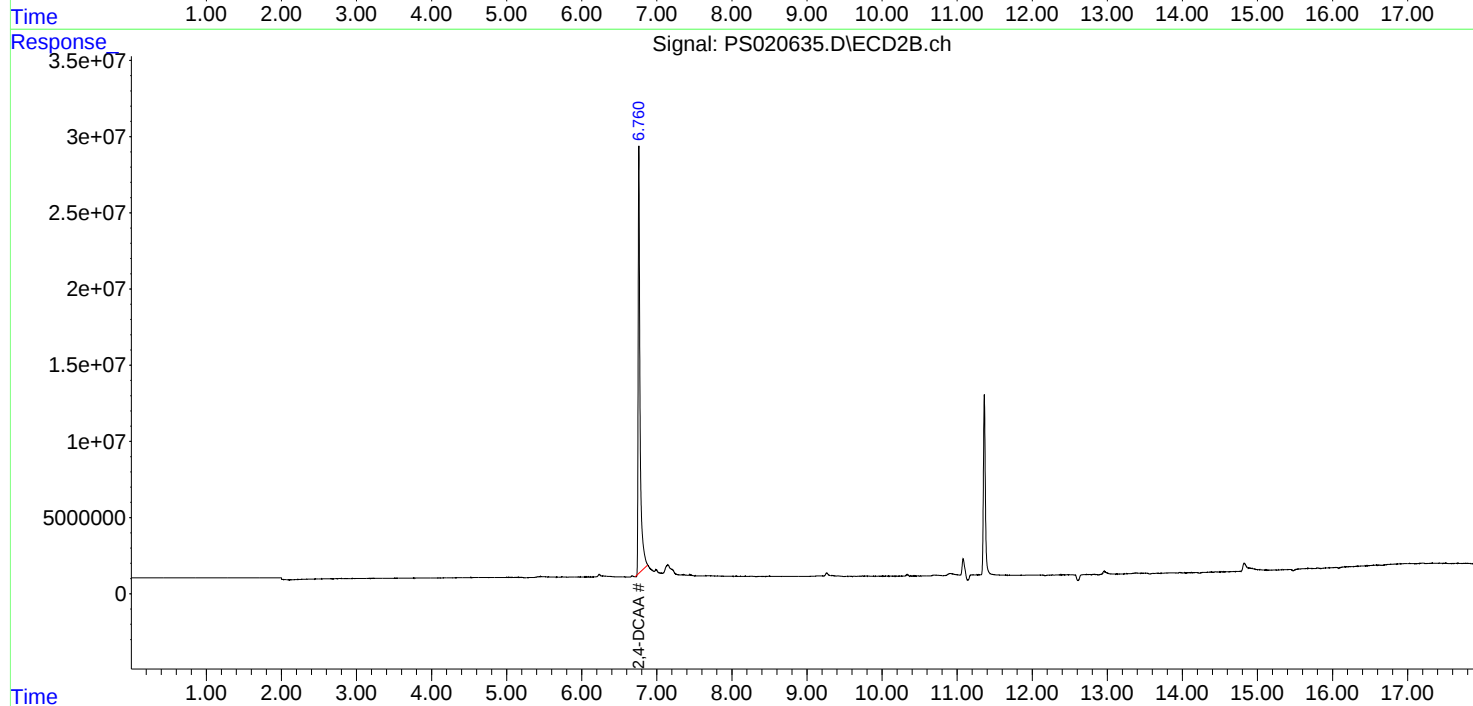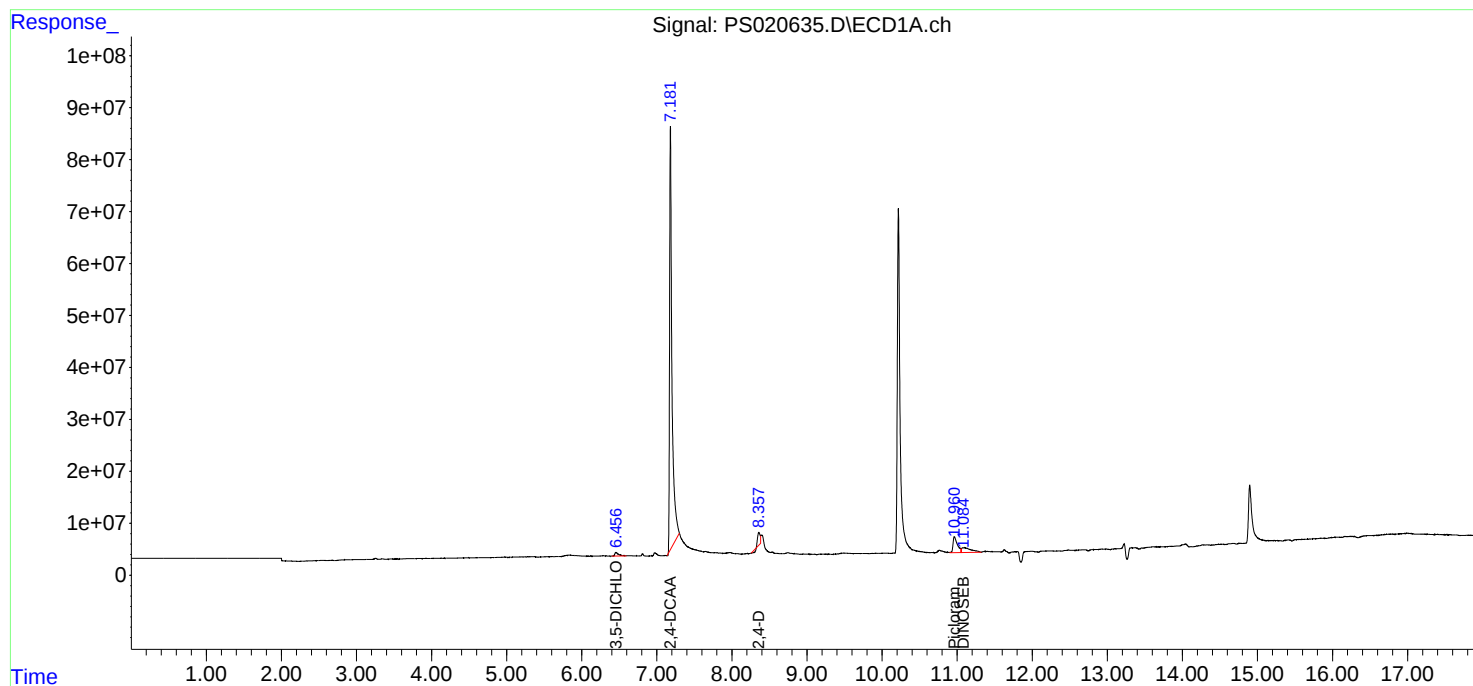


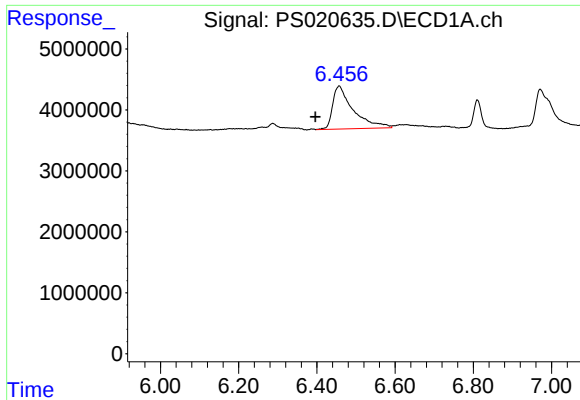

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.457 min
Delta R.T.: 0.061 min
Response: 25702314
Conc: 5.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

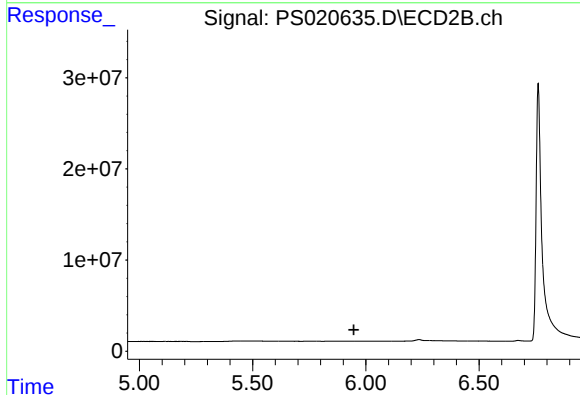


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.947 min
Response: 0
Conc: N.D.

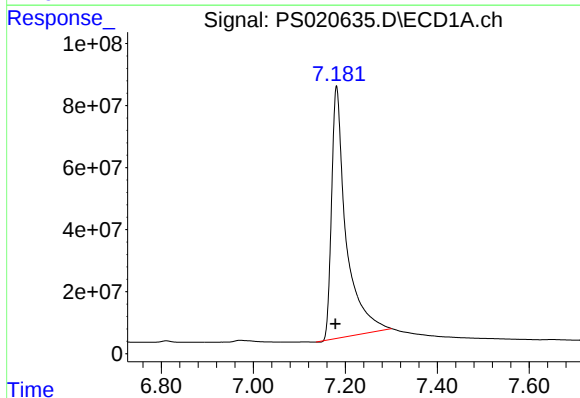


#4 2,4-DCAA

R.T.: 7.181 min
Delta R.T.: 0.002 min
Response: 1786297114
Conc: 519.05 ng/ml

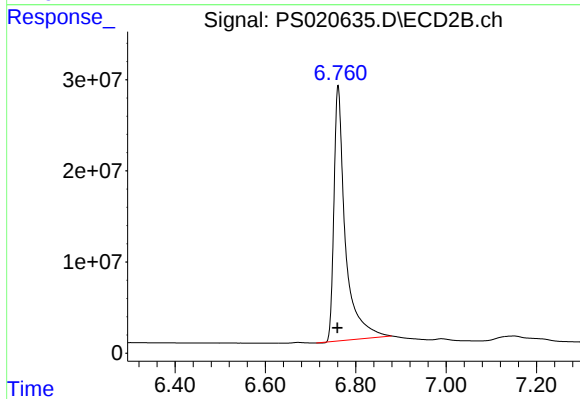

#4 2,4-DCAA


R.T.: 6.761 min
Delta R.T.: 0.001 min
Response: 489998393
Conc: 575.32 ng/ml

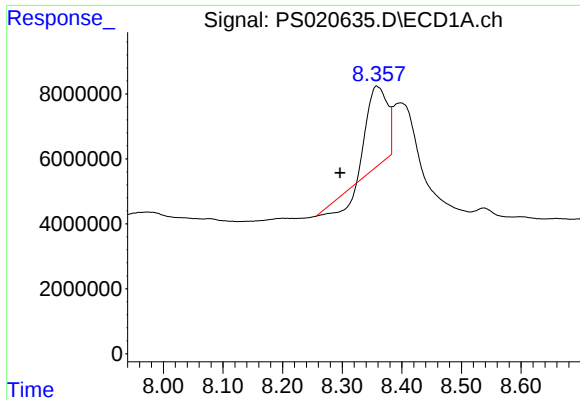

#9 2,4-D


R.T.: 8.358 min
Delta R.T.: 0.062 min
Response: 47308273
Conc: 10.18 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

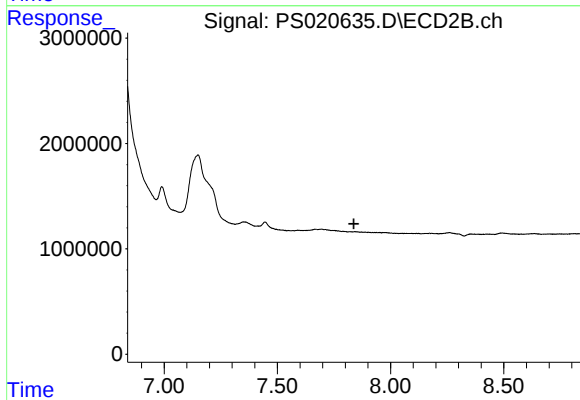


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.

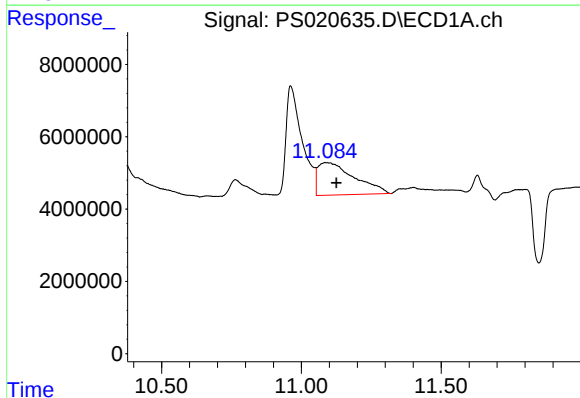


#14 DINOSEB

R.T.: 11.085 min
Delta R.T.: -0.040 min
Response: 81293995
Conc: 4.43 ng/ml

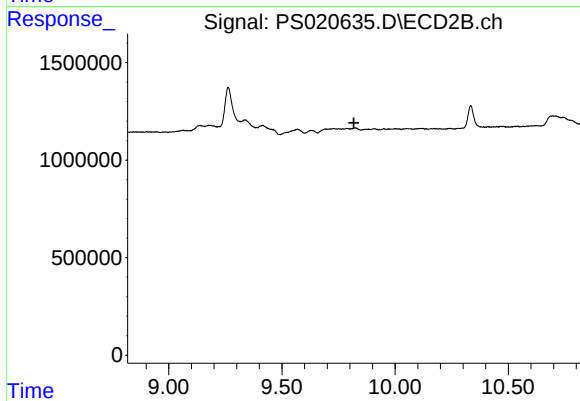

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.818 min
Response: 0
Conc: N.D.

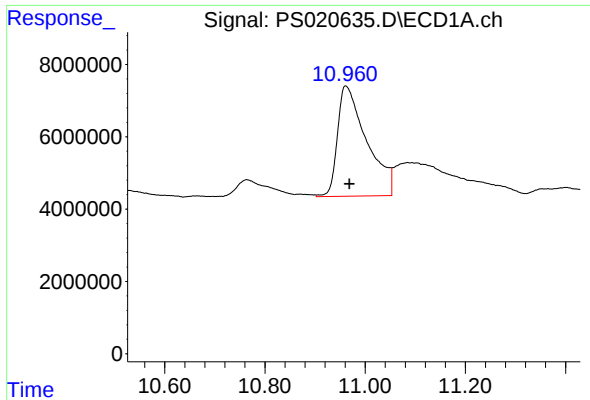

#15 Picloram

R.T.: 10.962 min
Delta R.T.: -0.007 min
Response: 123252514
Conc: 4.10 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

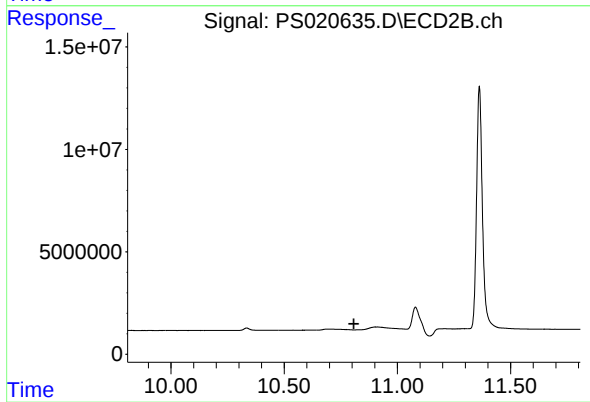

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.808 min
Response: 0
Conc: N.D.