

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092322\
 Data File : PS020643.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2022 20:24
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 00:33:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 14 02:51:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.179	6.760	1838.9E6	509.8E6	534.337	598.561
Target Compounds							
1) T	Dalapon	3.041	0.000	1056685	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.451f	0.000	18048564	0	3.619	N.D. #
3) T	4-Nitroph...	6.967f	0.000	-8901733	0	122.474	N.D. #
5) T	DICAMBA	0.000	6.988f	0	2600028	N.D.	<MDL
6) T	MCP	0.000	6.988	0	2600028	N.D.	<MDL
7) T	MCPA	7.644	0.000	1718980	0	<MDL	N.D. #
8) T	DICHLORPROP	8.038	0.000	3264787	0	<MDL	N.D. #
9) T	2,4-D	8.360f	0.000	192.3E6	0	41.369	N.D. #
10) T	Pentachlo...	8.591	0.000	757020	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.164	0.000	5756489	0	<MDL	N.D. #
12) T	2,4,5-T	9.431	0.000	7474040	0	<MDL	N.D. #
13) T	2,4-DB	10.006	0.000	3986158	0	1.098	N.D. #
14) T	DINOSEB	11.103	0.000	30890897	0	1.682	N.D. #
15) T	Picloram	10.949	10.745f	142.7E6	824789	4.743	<MDL #
16) T	DCPA	11.399	10.745	8936657	824789	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS092322\
Data File : PS020643.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2022 20:24
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 00:33:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS091322.M
Quant Title : 8080.M
QLast Update : Wed Sep 14 02:51:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

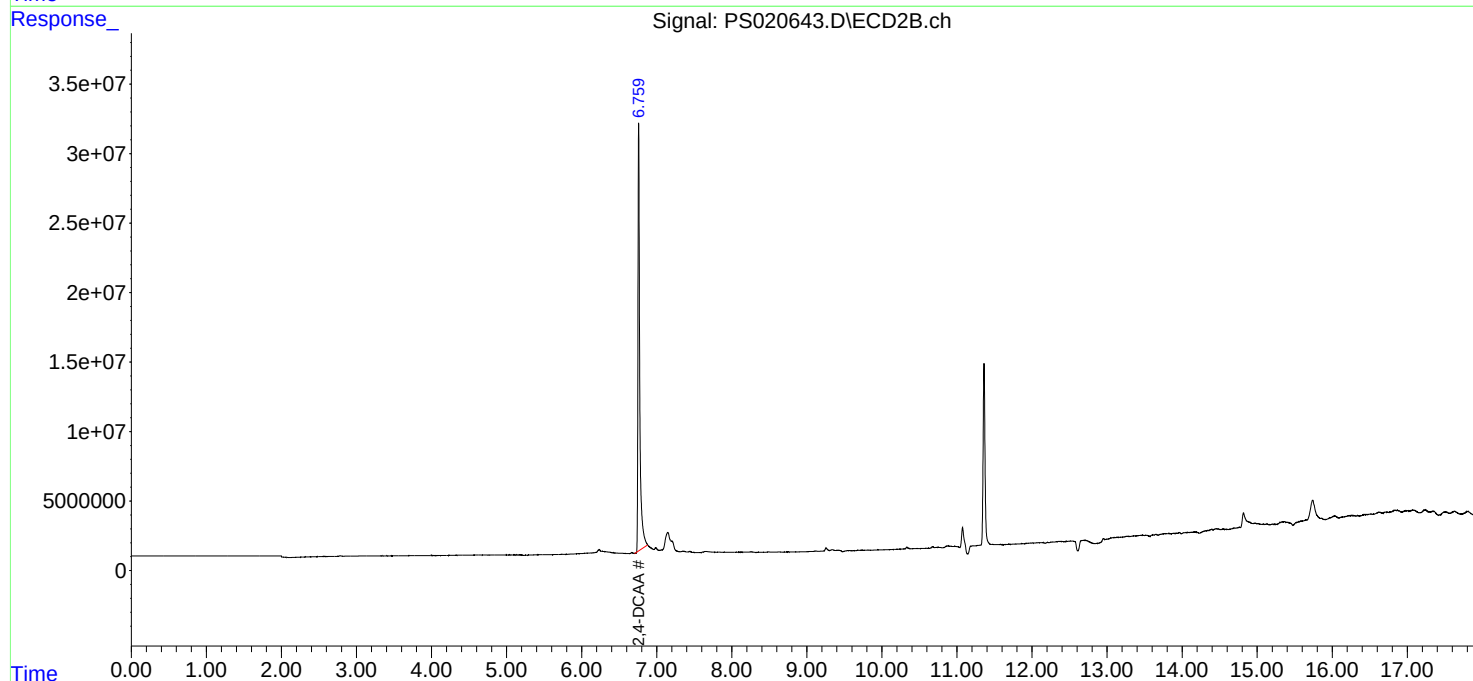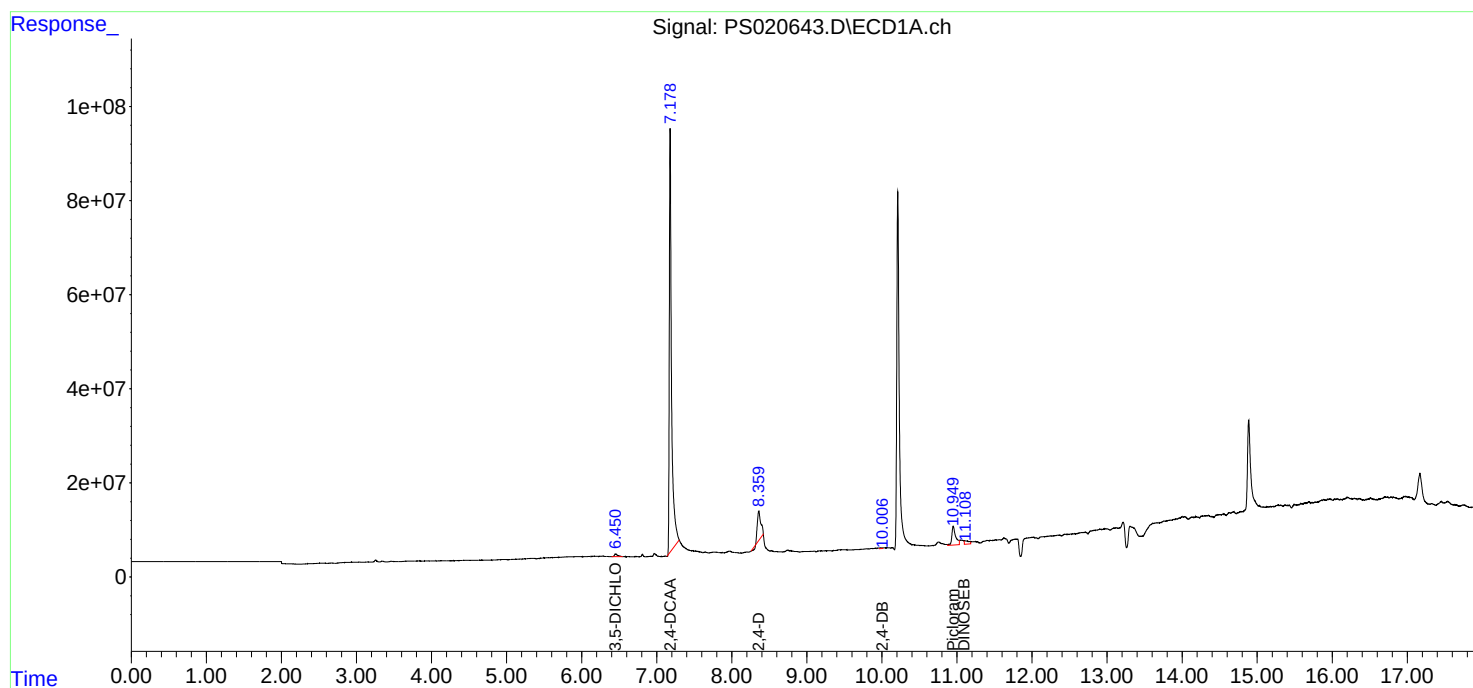


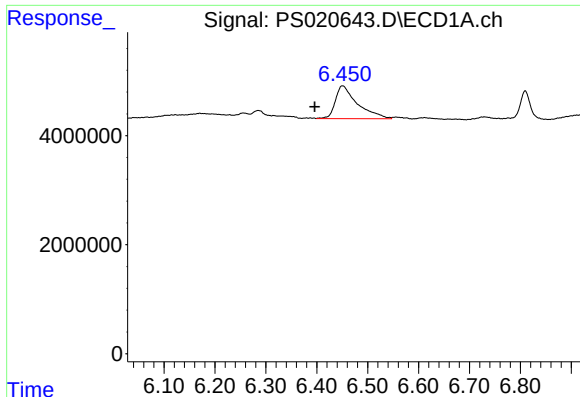

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.451 min
Delta R.T.: 0.054 min
Response: 18048564
Conc: 3.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

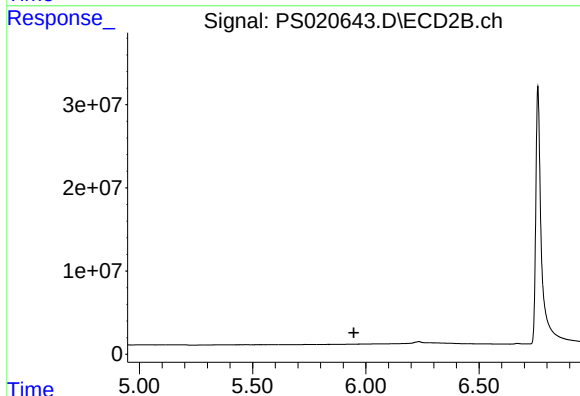


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.947 min
Response: 0
Conc: N.D.

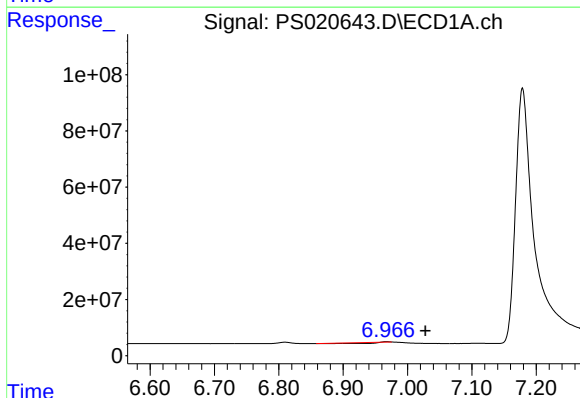


#3 4-Nitrophenol

R.T.: 6.967 min
Delta R.T.: -0.061 min
Response: -8901733
Conc: 122.47 ng/ml

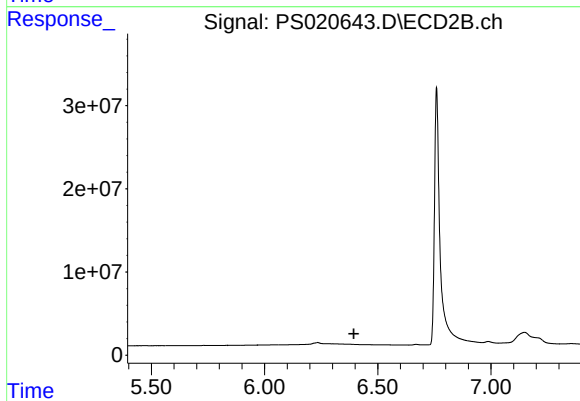

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.394 min
Response: 0
Conc: N.D.

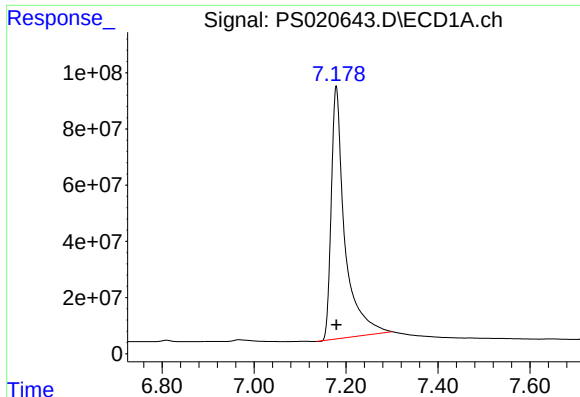

#4 2,4-DCAA


R.T.: 7.179 min
Delta R.T.: 0.000 min
Response: 1838911875
Conc: 534.34 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

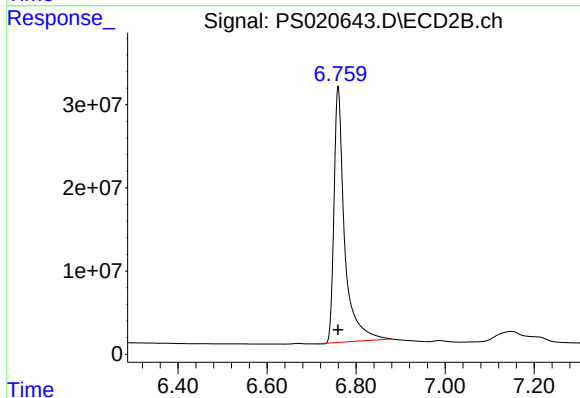


#4 2,4-DCAA

R.T.: 6.760 min
Delta R.T.: 0.000 min
Response: 509791197
Conc: 598.56 ng/ml

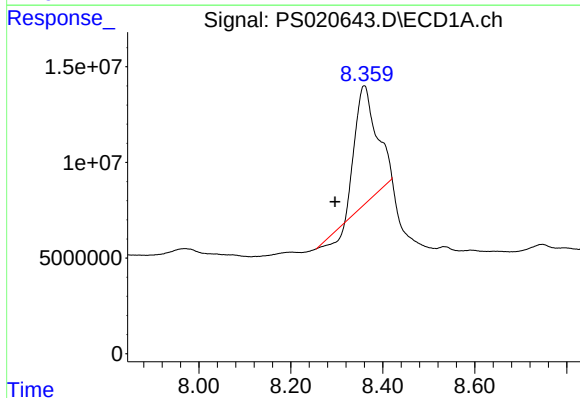


#9 2,4-D

R.T.: 8.360 min
Delta R.T.: 0.063 min
Response: 192287428
Conc: 41.37 ng/ml

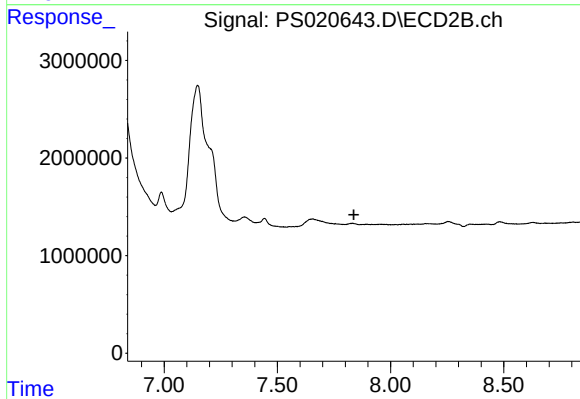

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.838 min
Response: 0
Conc: N.D.

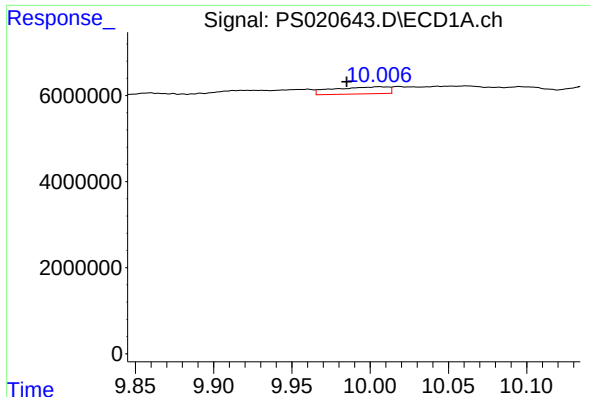

#13 2,4-DB


R.T.: 10.006 min
Delta R.T.: 0.021 min
Response: 3986158
Conc: 1.10 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

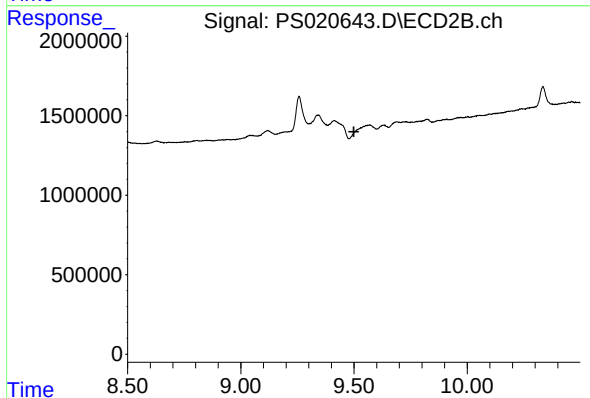


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.499 min
Response: 0
Conc: N.D.

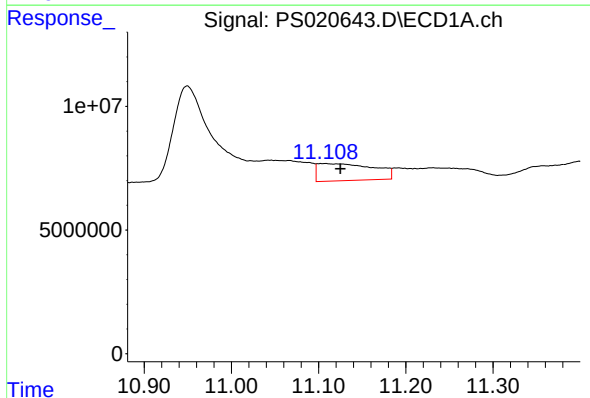


#14 DINOSEB

R.T.: 11.103 min
Delta R.T.: -0.022 min
Response: 30890897
Conc: 1.68 ng/ml

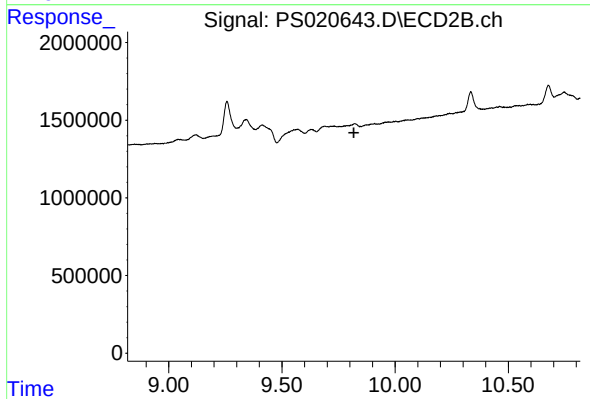

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.818 min
Response: 0
Conc: N.D.

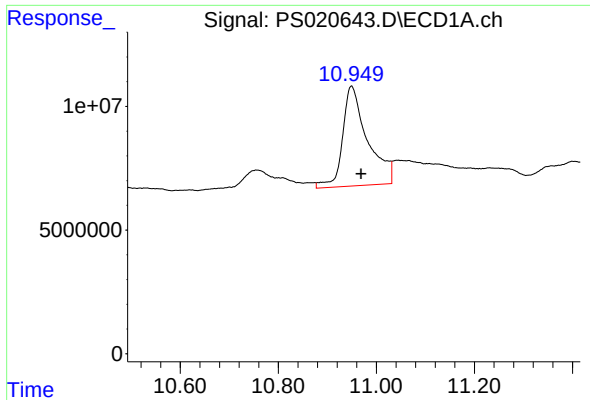

#15 Picloram

R.T.: 10.949 min
Delta R.T.: -0.019 min
Response: 142734763
Conc: 4.74 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

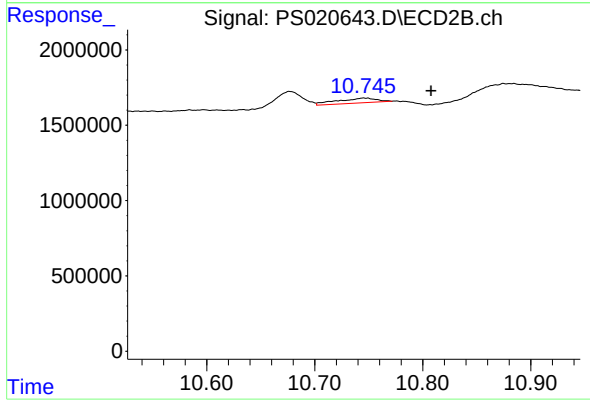

#15 Picloram

R.T.: 10.745 min
Delta R.T.: -0.063 min
Response: 824789
Conc: N.D.